

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062122\
 Data File : BN020312.D
 Acq On : 21 Jun 2022 17:51
 Operator : CG/JU
 Sample : N3313-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YB7L6

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :mohammad ahmed 06/28/2022

Quant Time: Jun 22 00:08:37 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:13:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.796	152	589	0.400	ng/ul	0.00
4) Naphthalene-d8	10.579	136	2086	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.419	164	1514	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.159	188	3958	0.400	ng/ul	0.00
17) Chrysene-d12	21.351	240	6288	0.400	ng/ul	0.00
23) Perylene-d12	23.657	264	9948	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.256	96	3017m	4.486	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.179	152	1048	0.304	ng/ul	0.00
18) Fluoranthene-d10	19.193	212	5207	0.401	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.290	88	578	0.893	ng/ul#	62

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062122\
Data File : BN020312.D
Acq On : 21 Jun 2022 17:51
Operator : CG/JU
Sample : N3313-08
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
YB7L6

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 06/22/2022
Supervised By :mohammad ahmed 06/28/2022


Quant Time: Jun 22 00:08:37 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:13:51 2022
Response via : Initial Calibration

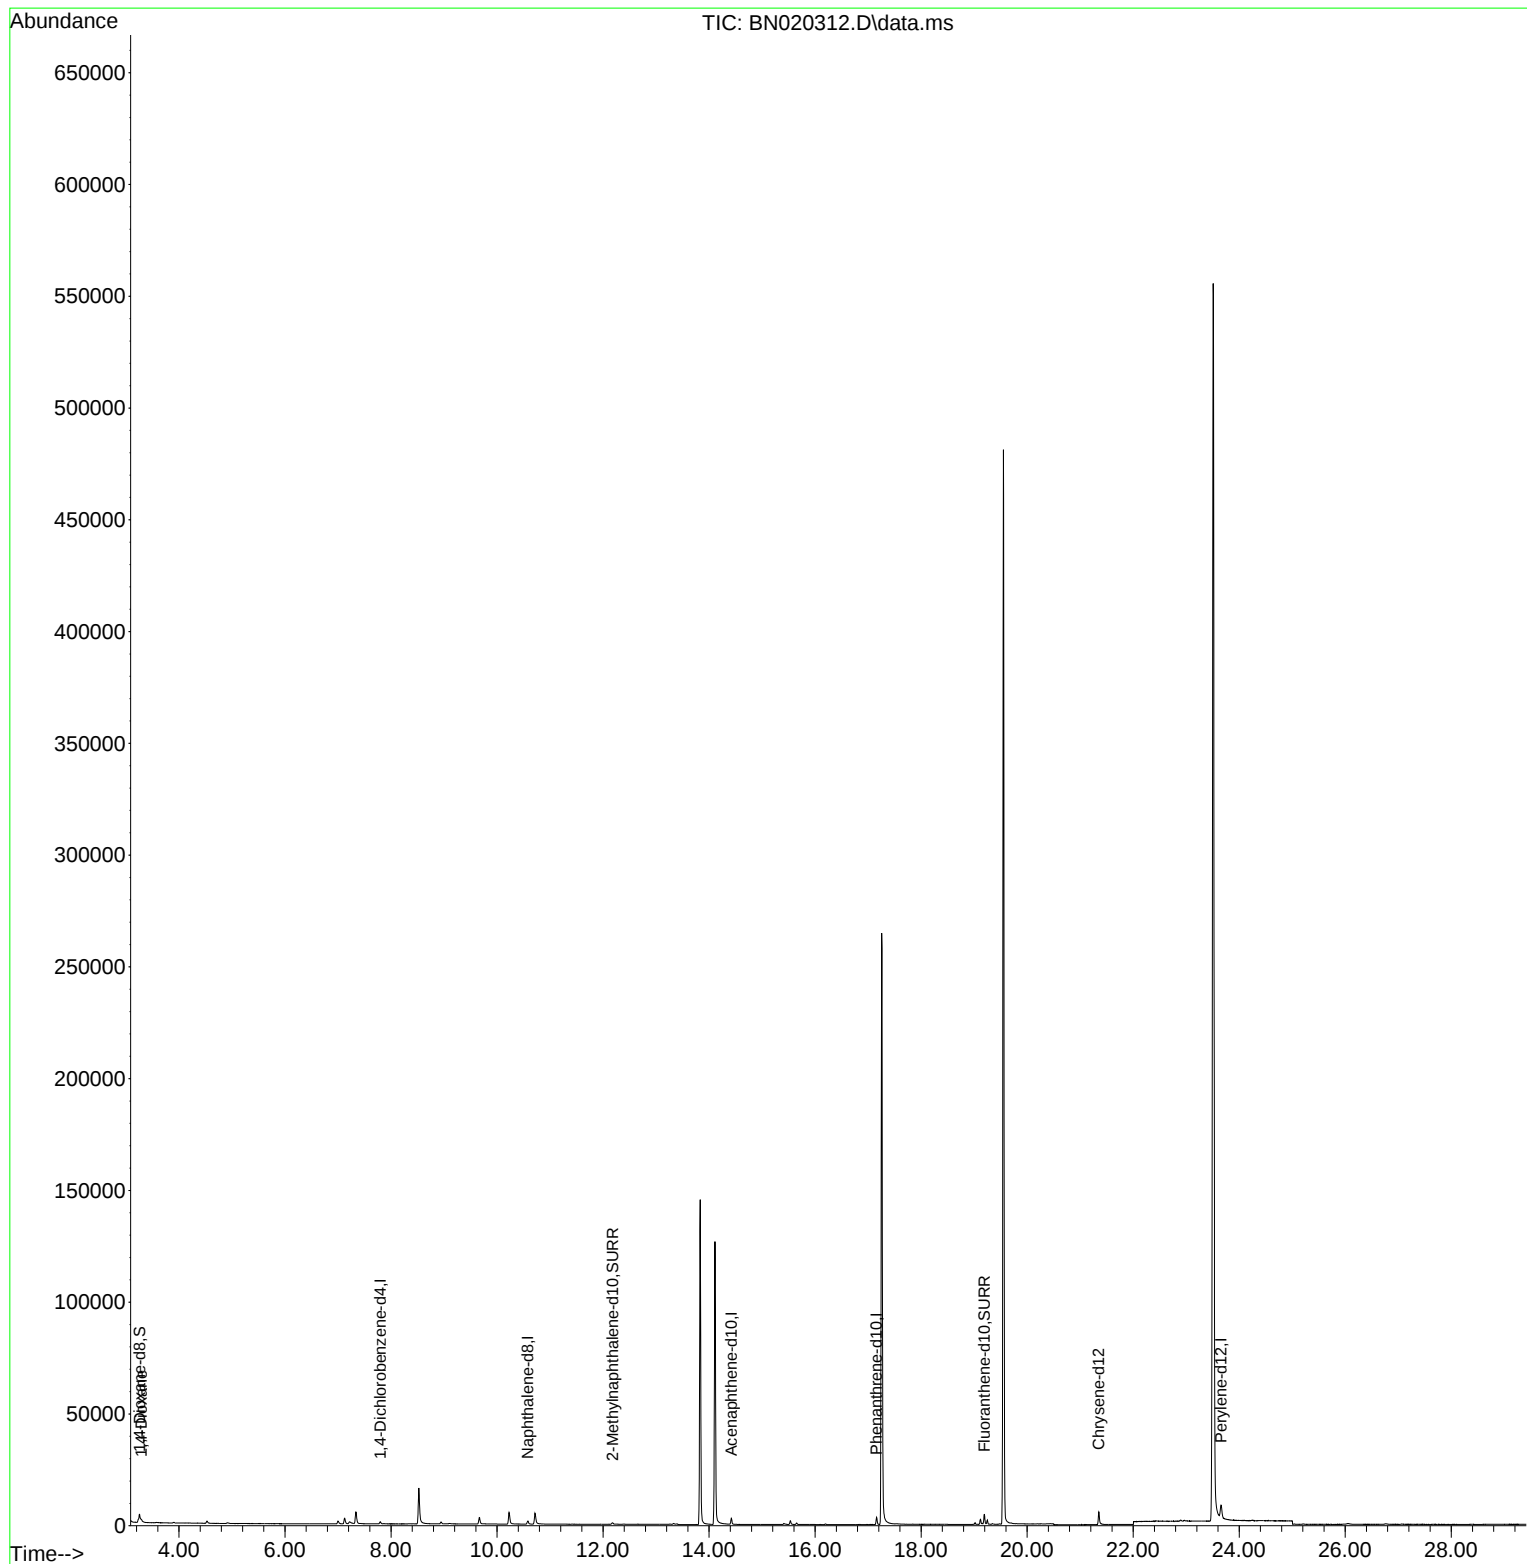

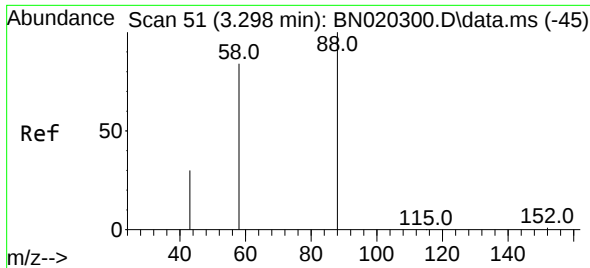

#2
 1,4-Dioxane
 Concen: 0.893 ng/ul
 RT: 3.290 min Scan# 49
 Delta R.T. -0.004 min
 Lab File: BN020312.D
 Acq: 21 Jun 2022 17:51

Instrument :
 BNA_N
 ClientSampleId :
 YB7L6

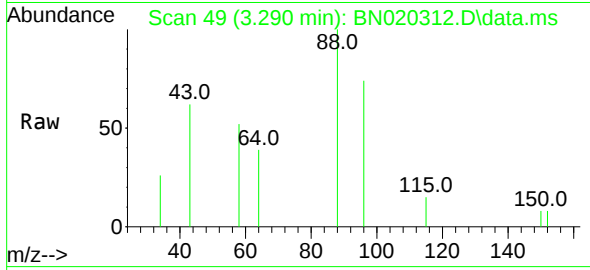

Tgt Ion: 88 Resp: 578

Ion	Ratio	Lower	Upper
88	100		
43	61.7	31.6	47.4
58	51.7	23.8	35.6

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :mohammad ahmed 06/28/2022

