
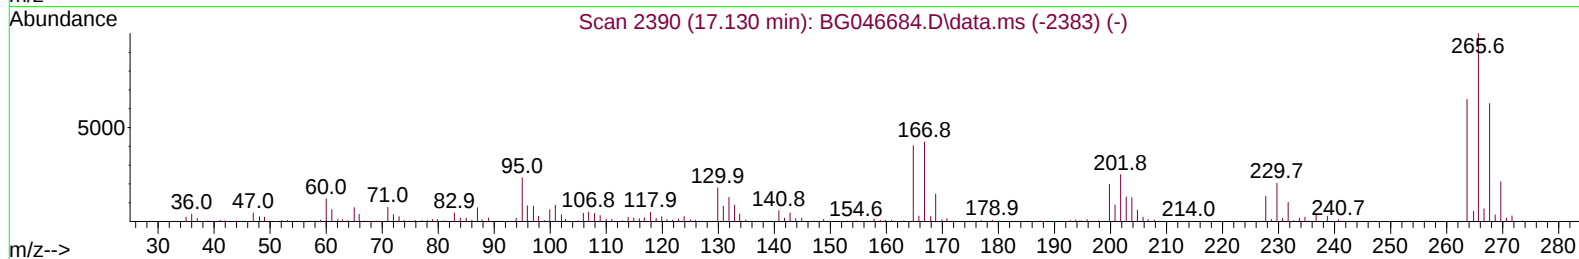
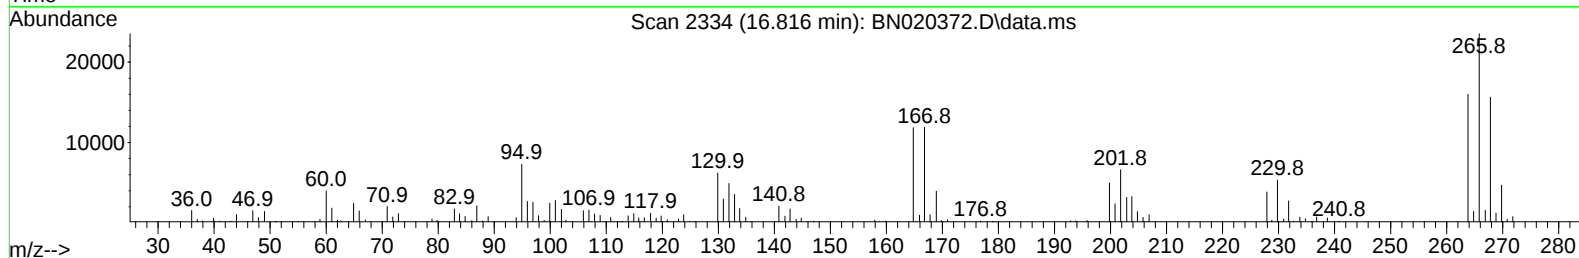


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062322\
Data File : BN020372.D
Acq On : 23 Jun 2022 14:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 16:21:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 23 16:21:20 2022
Response via : Initial Calibration

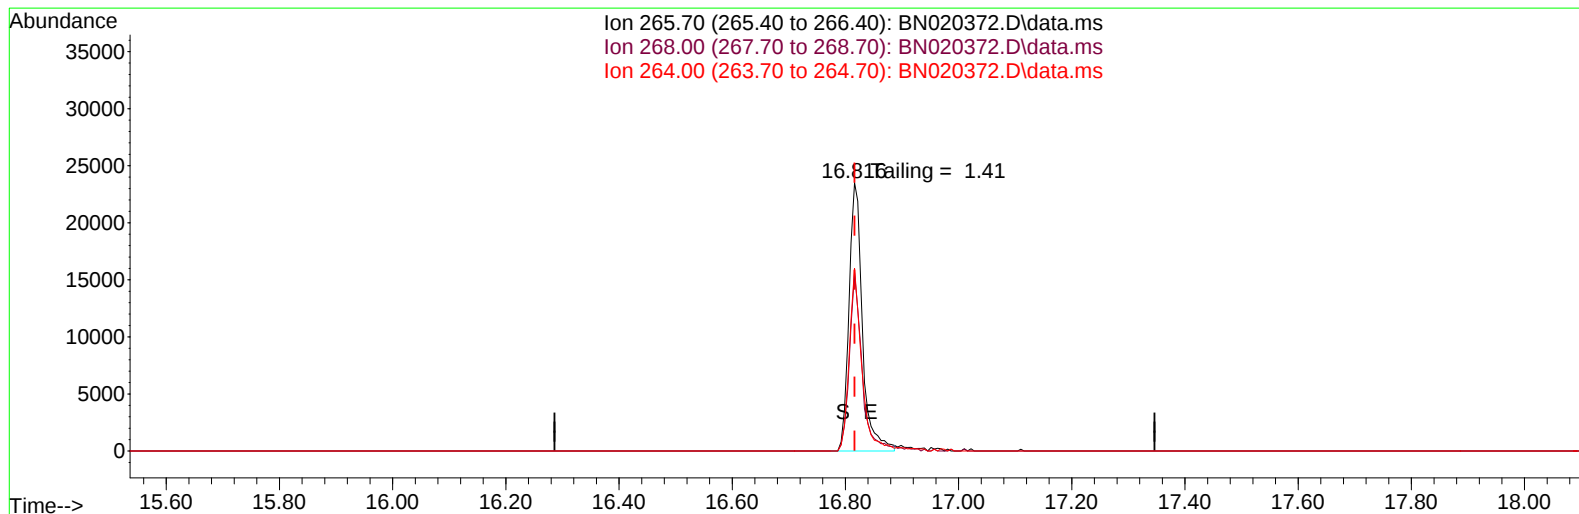

TIC: BN020372.D\data.ms

(70) Pentachlorophenol (C)




16.816min (0.000) 0.00 ng

response 39668

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.45
264.00	61.60	68.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062322\
Data File : BN020372.D
Acq On : 23 Jun 2022 14:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 16:21:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 23 16:21:20 2022
Response via : Initial Calibration

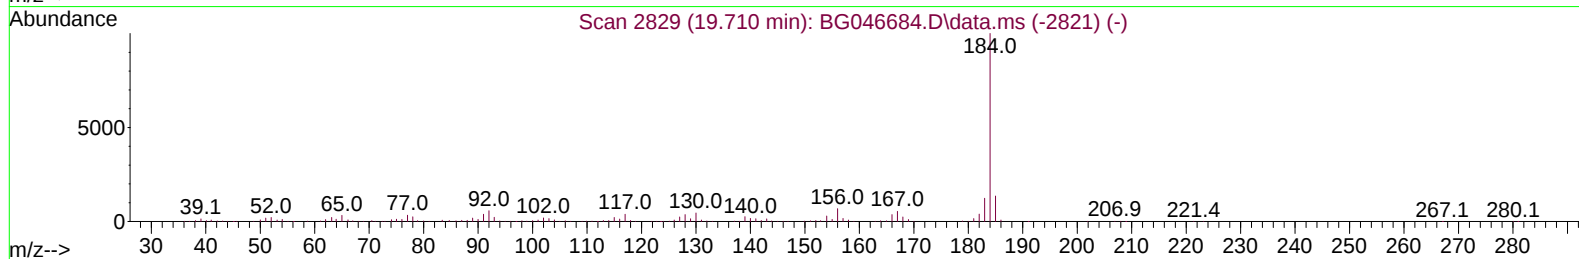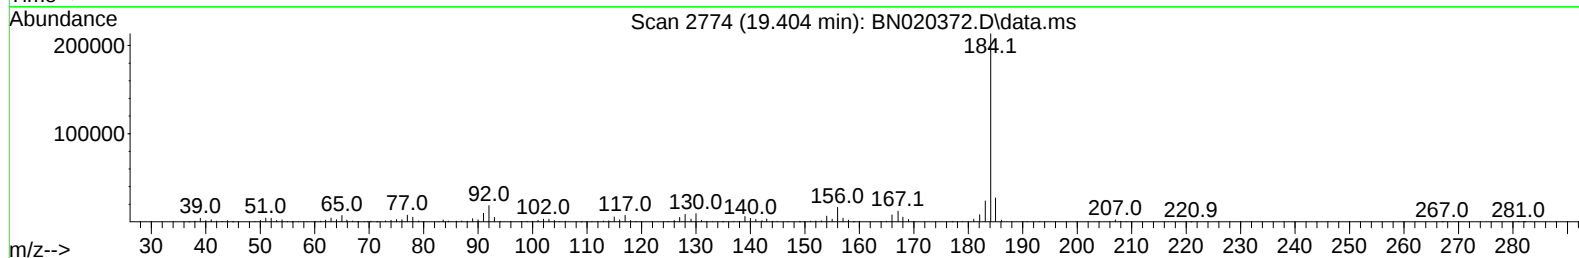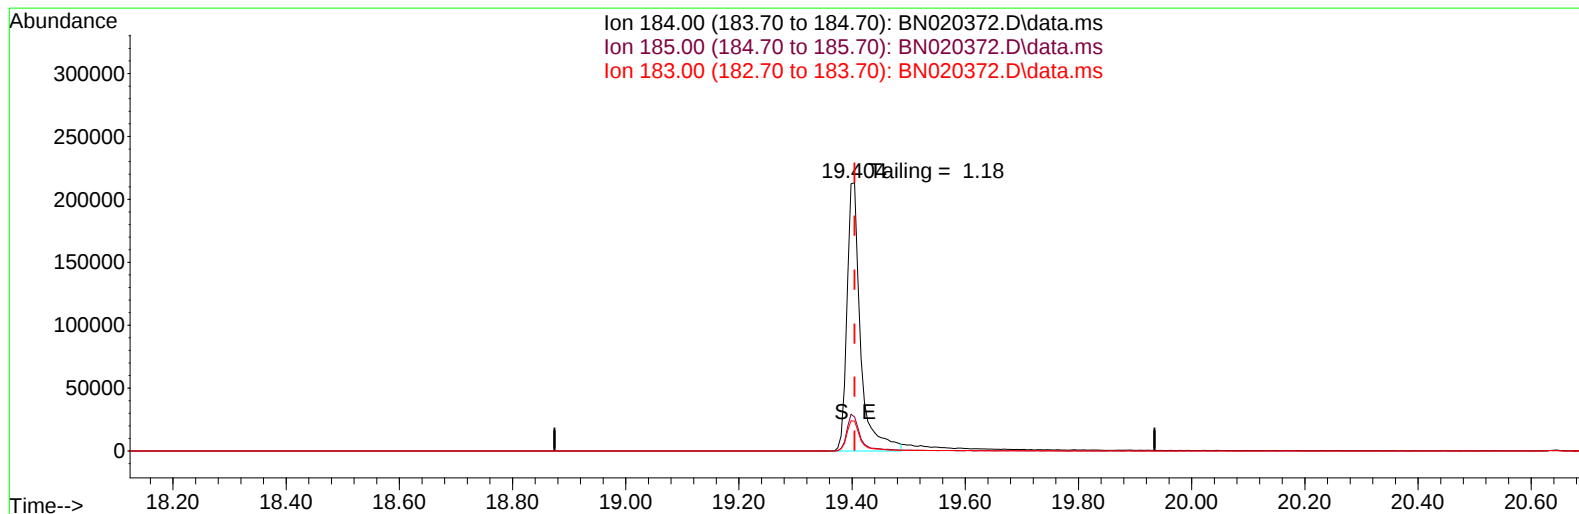

TIC: BN020372.D\data.ms

(77) Benzidine

19.404min (0.000) 0.00 ng

response 375548

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	12.73
183.00	13.20	11.16
0.00	0.00	0.00