
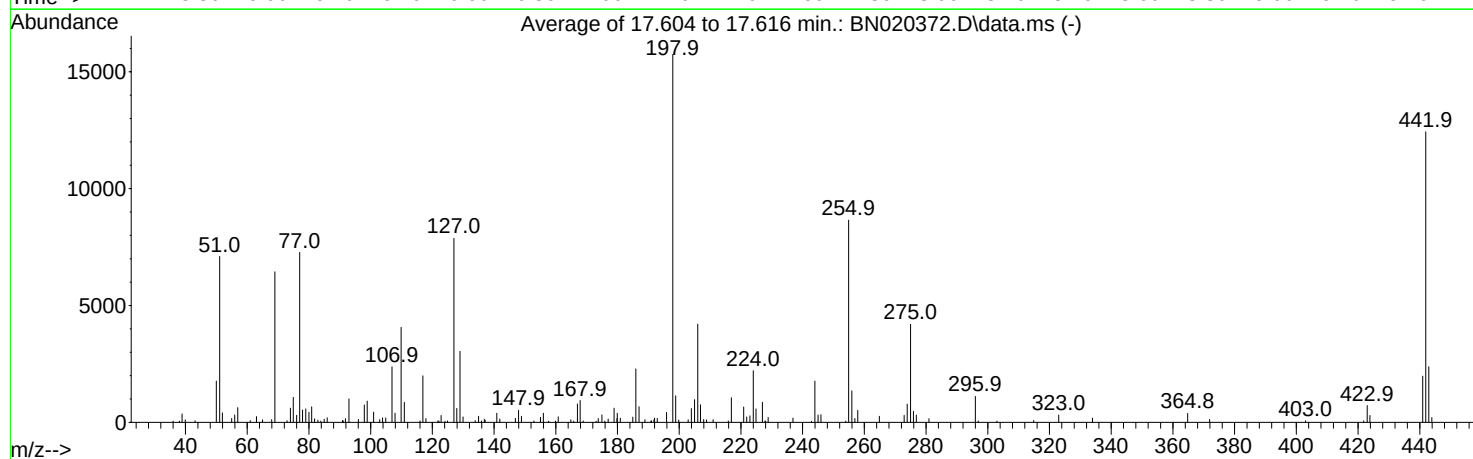


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062322\  
 Data File : BN020372.D  
 Acq On : 23 Jun 2022 14:06  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\8270-SIM-BN062222.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Jun 22 15:57:15 2022

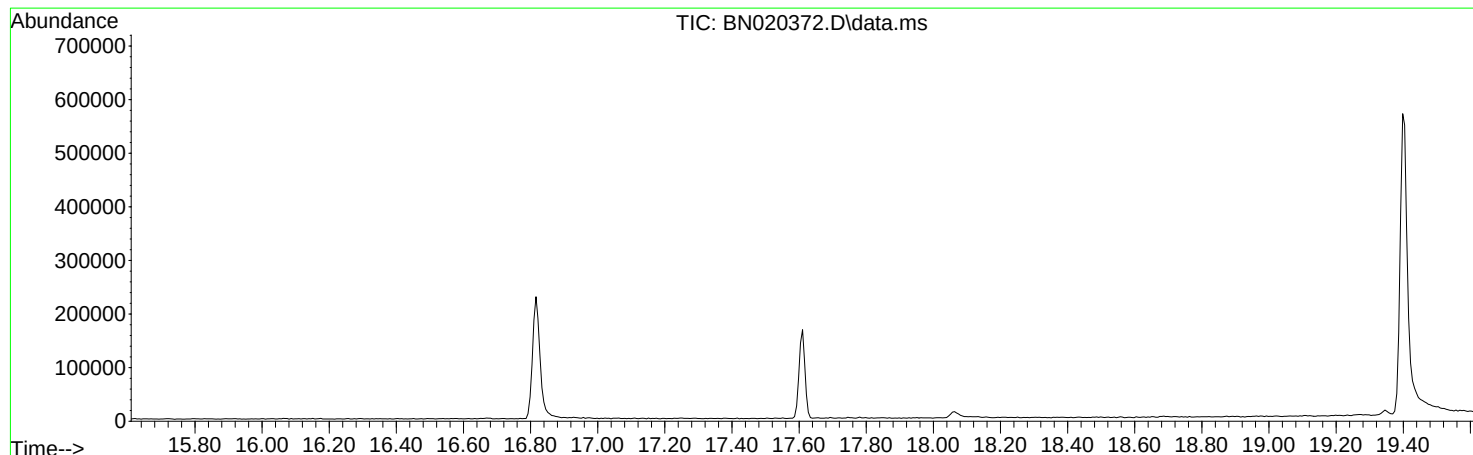




AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2462

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 45.1         | 7098       | PASS                |
| 68             | 69              | 0.00            | 2               | 1.8          | 117        | PASS                |
| 69             | 198             | 0.00            | 100             | 40.9         | 6442       | PASS                |
| 70             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 127            | 198             | 10              | 80              | 50.0         | 7875       | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 15739      | PASS                |
| 199            | 198             | 5               | 9               | 7.2          | 1138       | PASS                |
| 275            | 198             | 10              | 60              | 26.6         | 4194       | PASS                |
| 365            | 198             | 1               | 100             | 2.5          | 386        | PASS                |
| 441            | 198             | 0.01            | 100             | 12.6         | 1982       | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 12434      | PASS                |
| 443            | 442             | 15              | 24              | 19.2         | 2384       | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062322\  
Data File : BN020372.D  
Acq On : 23 Jun 2022 14:06  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: Jun 23 16:21:34 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jun 23 16:21:20 2022  
Response via : Initial Calibration

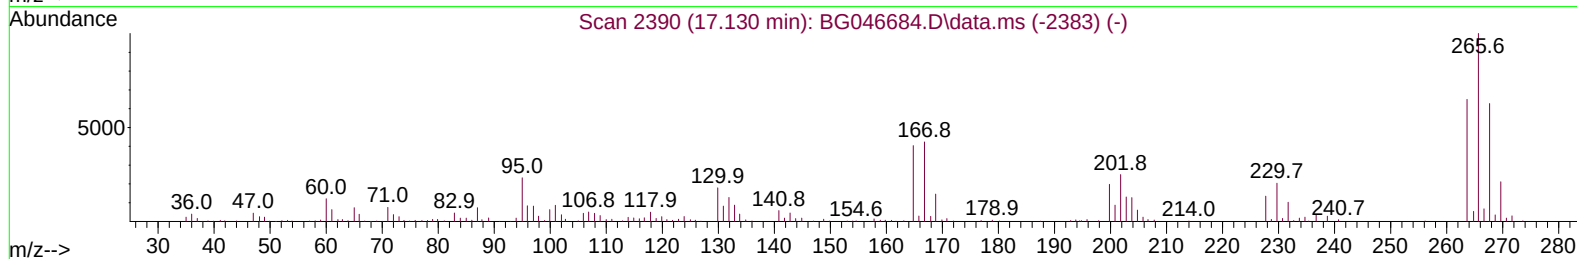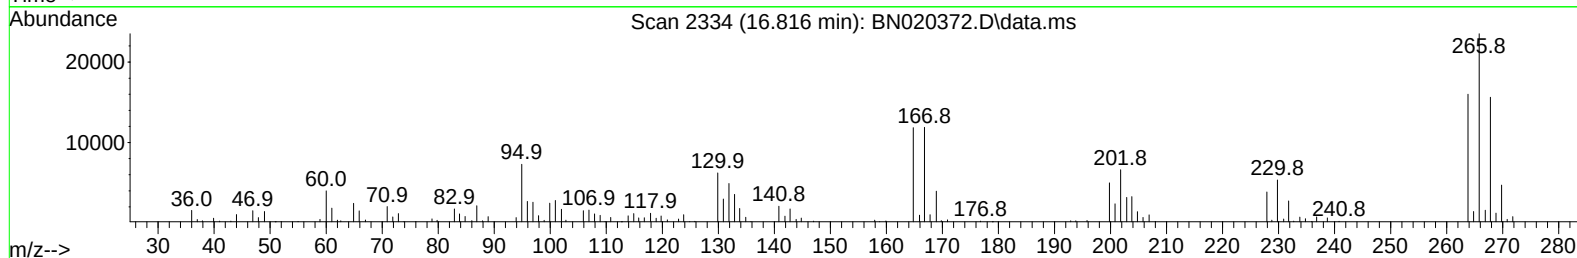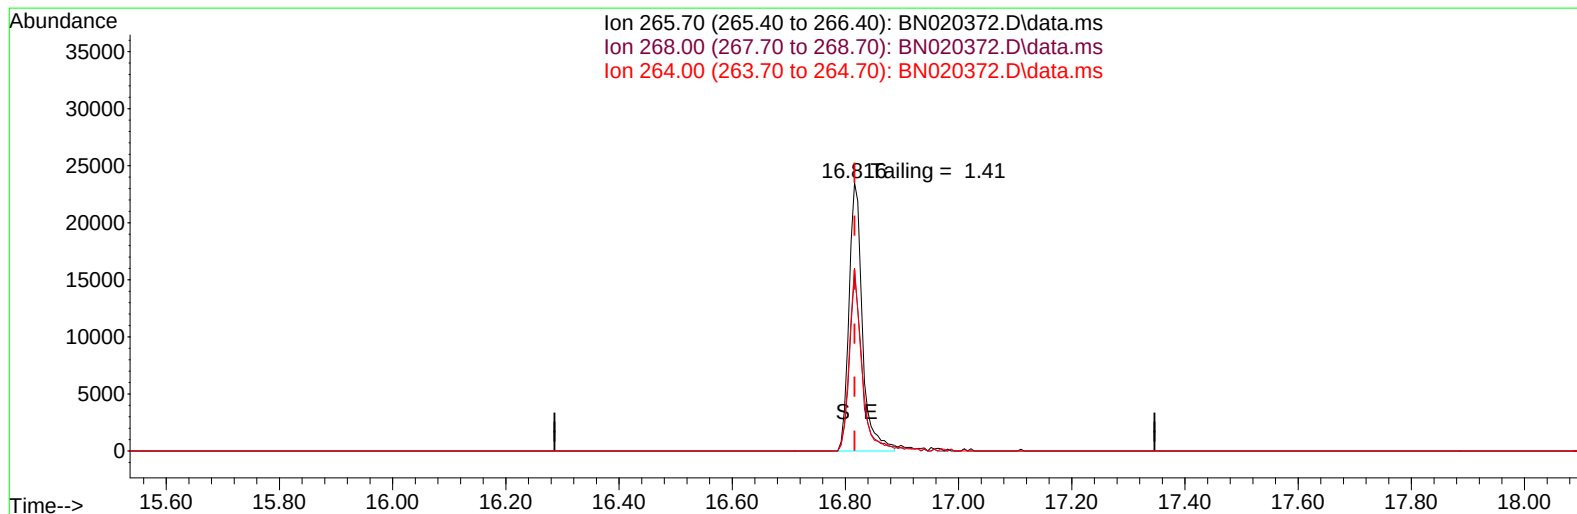

TIC: BN020372.D\data.ms

**(70) Pentachlorophenol (C)**

16.816min ( 0.000) 0.00 ng




response 39668

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 66.45  |
| 264.00 | 61.60  | 68.01  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062322\  
Data File : BN020372.D  
Acq On : 23 Jun 2022 14:06  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: Jun 23 16:21:34 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jun 23 16:21:20 2022  
Response via : Initial Calibration

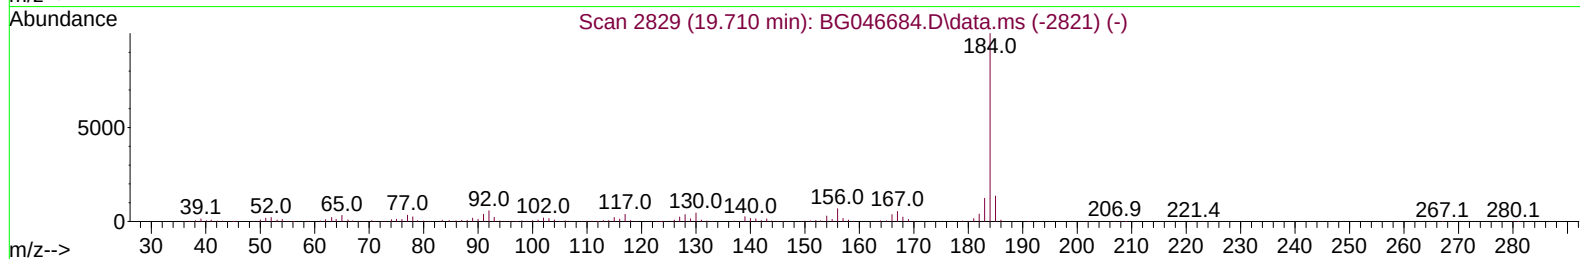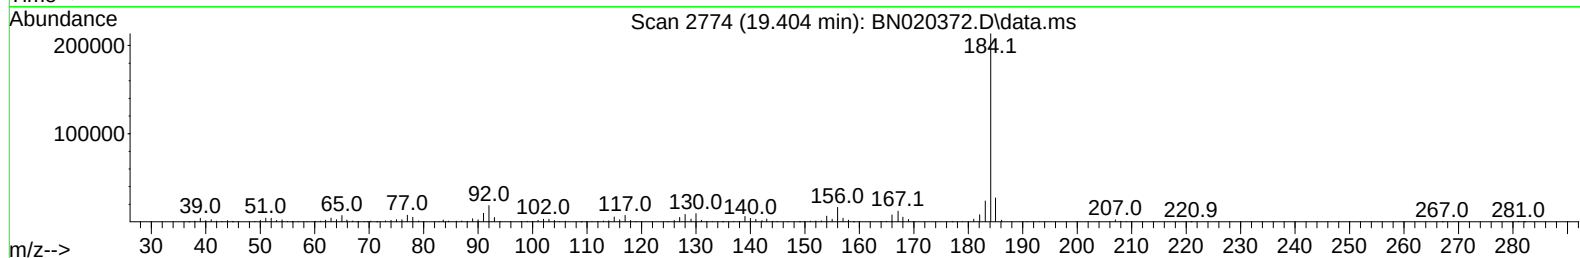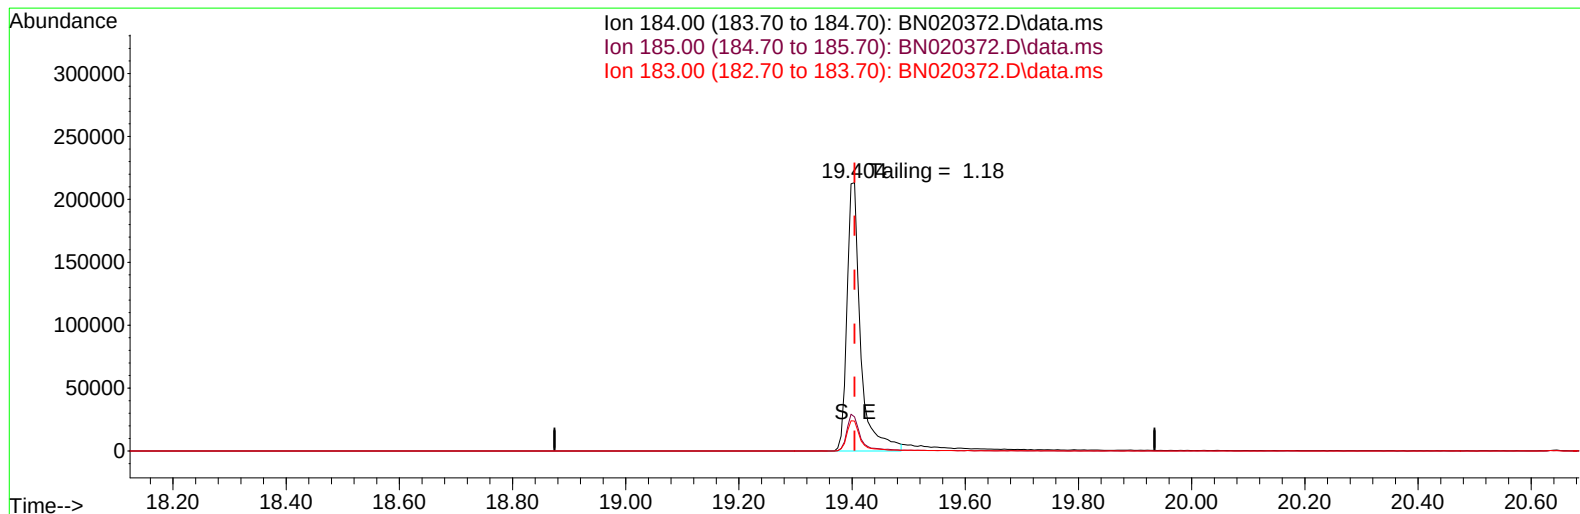

TIC: BN020372.D\data.ms

**(77) Benzidine**

19.404min ( 0.000) 0.00 ng

response 375548

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 12.73  |
| 183.00 | 13.20  | 11.16  |
| 0.00   | 0.00   | 0.00   |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 6/23/2022     | BNA_N            | <u>BN020372.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 135484           | 20.63              |
| DDD           | 6384             | 20.2               |
| DDE           | 537              | 19.69              |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 6921          | 142405           | 4.86               |

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP