
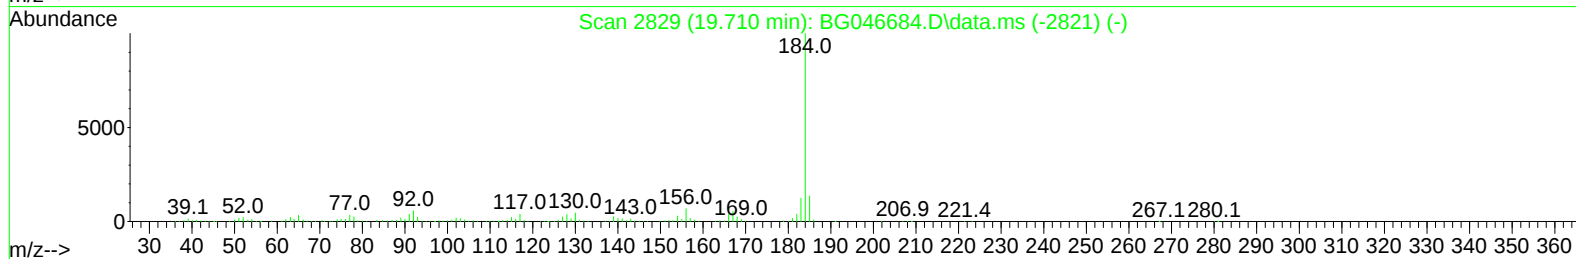
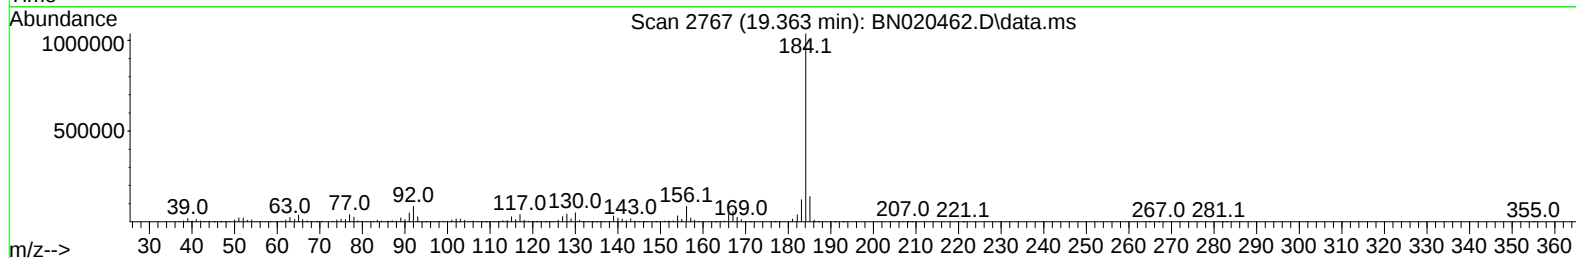


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062622\  
Data File : BN020462.D  
Acq On : 26 Jun 2022 12:29  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 27 02:09:20 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Jun 27 02:09:13 2022  
Response via : Initial Calibration

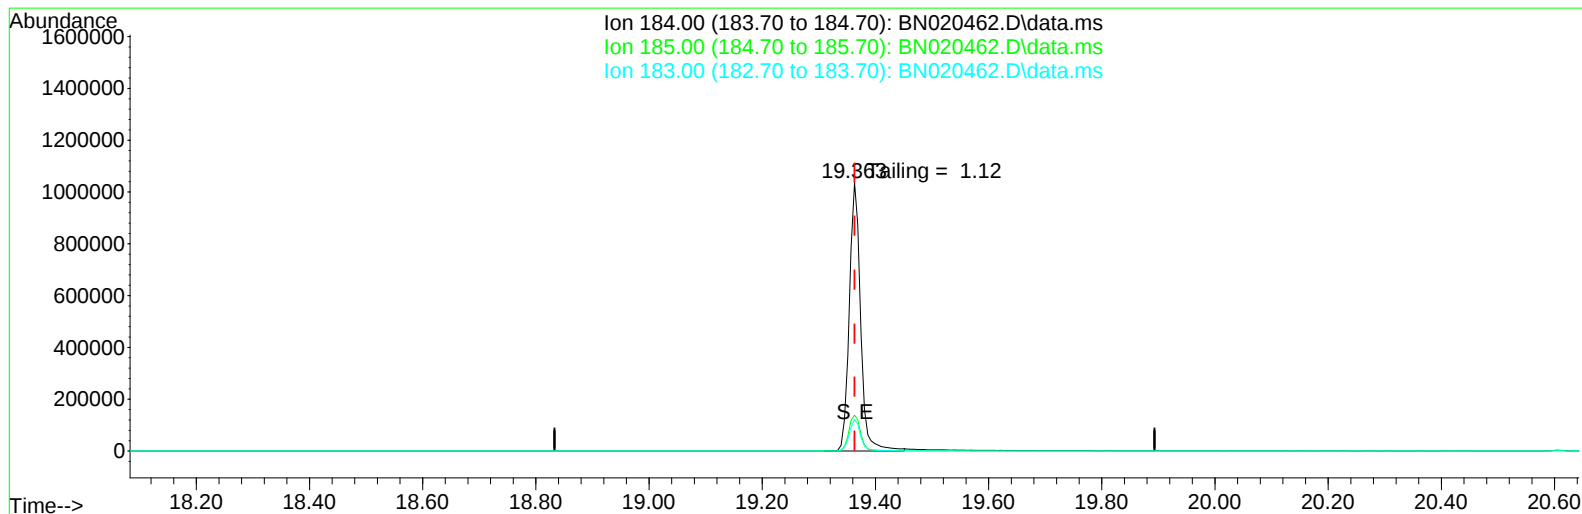

TIC: BN020462.D\data.ms

**(77) Benzdine**

19.363min ( 0.000) 0.00 ng

response 1473691

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 13.36  |
| 183.00 | 13.20  | 11.72  |
| 0.00   | 0.00   | 0.00   |