

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062622\
 Data File : BN020463.D
 Acq On : 26 Jun 2022 13:05
 Operator : CG/JU
 Sample : SSTDICC0.1
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1

Quant Time: Jun 27 01:37:18 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 27 01:36:24 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.739	152	2596	0.400	ng	0.00
7) Naphthalene-d8	10.530	136	7929	0.400	ng	0.01
13) Acenaphthene-d10	14.367	164	4702	0.400	ng	0.00
19) Phenanthrene-d10	17.113	188	9869	0.400	ng	# 0.00
29) Chrysene-d12	21.306	240	8823	0.400	ng	0.00
35) Perylene-d12	23.597	264	8556	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.348	112	845	0.111	ng	0.00
5) Phenol-d6	6.952	99	907	0.093	ng	0.00
8) Nitrobenzene-d5	8.897	82	615	0.111	ng	0.00
11) 2-Methylnaphthalene-d10	12.121	152	1374	0.093	ng	0.00
14) 2,4,6-Tribromophenol	15.872	330	188	0.084	ng	0.01
15) 2-Fluorobiphenyl	12.998	172	1988	0.118	ng	0.00
27) Fluoranthene-d10	19.152	212	3043	0.088	ng	0.00
31) Terphenyl-d14	19.750	244	2251	0.128	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.232	88	398	0.134	ng	97
3) n-Nitrosodimethylamine	3.572	42	289	0.107	ng	# 79
6) bis(2-Chloroethyl)ether	7.175	93	738	0.097	ng	99
9) Naphthalene	10.573	128	2411	0.102	ng	# 90
10) Hexachlorobutadiene	10.872	225	461	0.116	ng	# 98
12) 2-Methylnaphthalene	12.197	142	1589	0.092	ng	97
16) Acenaphthylene	14.089	152	2153	0.098	ng	100
17) Acenaphthene	14.431	154	1572	0.102	ng	96
18) Fluorene	15.425	166	2104	0.095	ng	100
20) 4,6-Dinitro-2-methylph...	15.532	198	84	0.054	ng	# 1
21) 4-Bromophenyl-phenylether	16.313	248	587	0.108	ng	94
22) Hexachlorobenzene	16.425	284	671	0.109	ng	96
23) Atrazine	16.579	200	471	0.116	ng	# 85
24) Pentachlorophenol	16.784	266	135	0.050	ng	97
25) Phenanthrene	17.154	178	3518	0.104	ng	98
26) Anthracene	17.246	178	2806	0.096	ng	99
28) Fluoranthene	19.181	202	3709	0.083	ng	98
30) Pyrene	19.544	202	4001	0.123	ng	99
32) Benzo(a)anthracene	21.297	228	3216	0.102	ng	96
33) Chrysene	21.351	228	3617	0.100	ng	94
34) Bis(2-ethylhexyl)phtha...	21.234	149	2296	0.158	ng	# 98
36) Indeno(1,2,3-cd)pyrene	25.939	276	3648	0.087	ng	95
37) Benzo(b)fluoranthene	22.910	252	3209	0.095	ng	# 68
38) Benzo(k)fluoranthene	22.951	252	3368	0.097	ng	# 70
39) Benzo(a)pyrene	23.495	252	2789	0.095	ng	# 55
40) Dibenzo(a,h)anthracene	25.951	278	2864	0.086	ng	# 80
41) Benzo(g,h,i)perylene	26.656	276	3264	0.088	ng	# 90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062622\
Data File : BN020463.D
Acq On : 26 Jun 2022 13:05
Operator : CG/JU
Sample : SSTDICC0.1
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Quant Time: Jun 27 01:37:18 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 01:36:24 2022
Response via : Initial Calibration

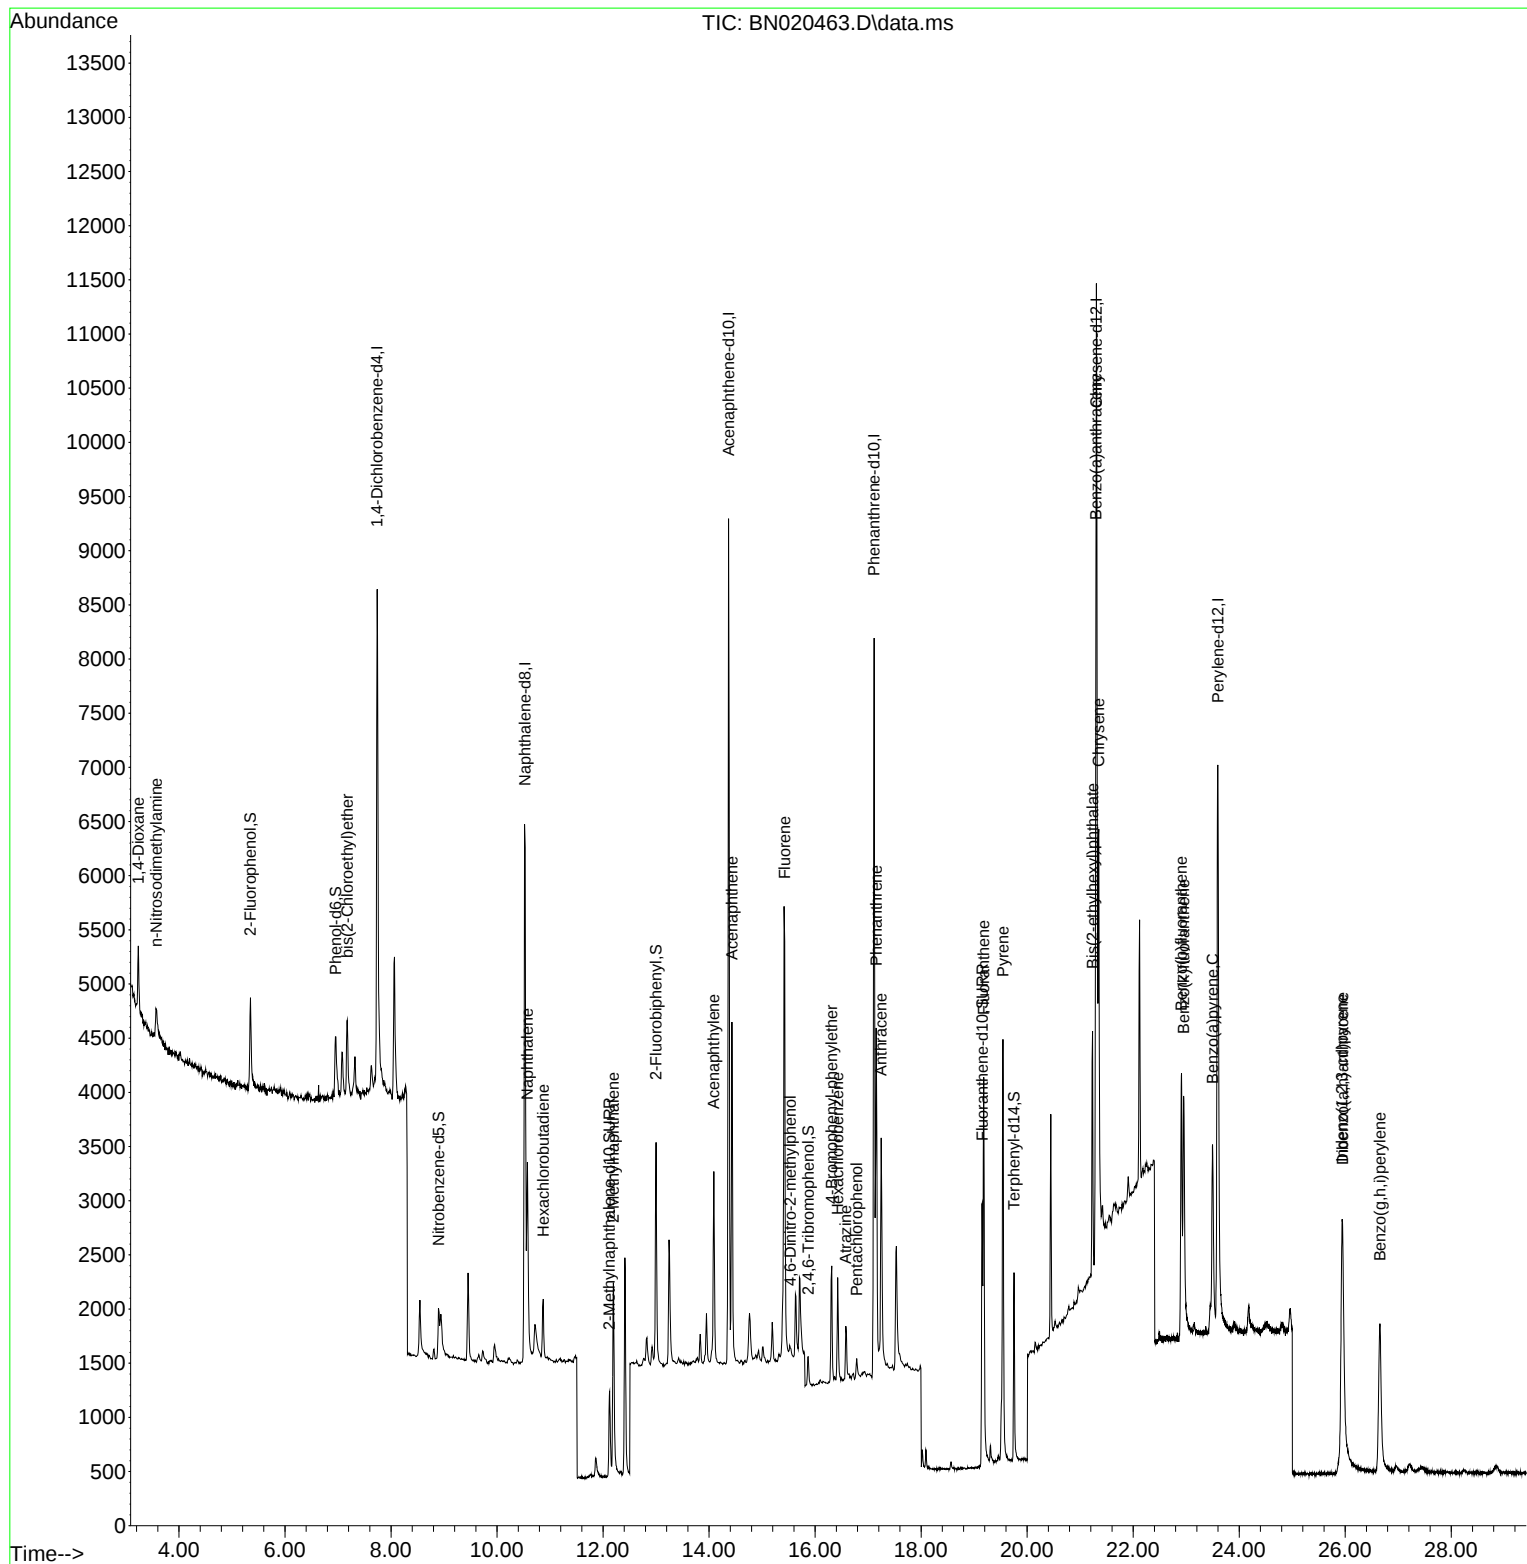





#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.739 min Scan# 64
 Delta R.T. -0.000 min
 Lab File: BN020463.D
 Acq: 26 Jun 2022 13:05


Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1

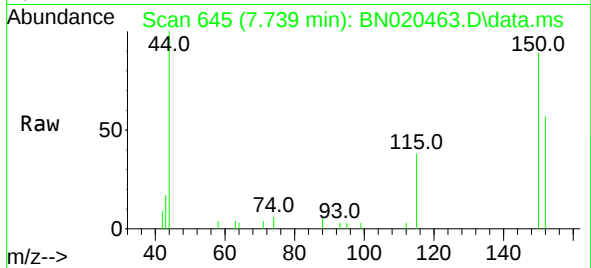



Tgt Ion:152 Resp: 2596
 Ion Ratio Lower Upper
 152 100
 150 155.6 127.9 191.9
 115 67.0 51.4 77.2

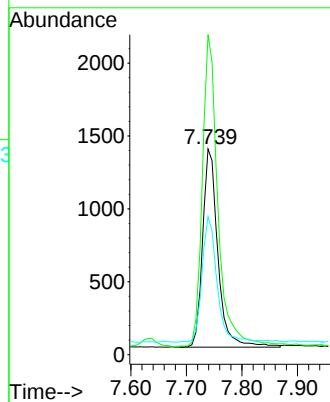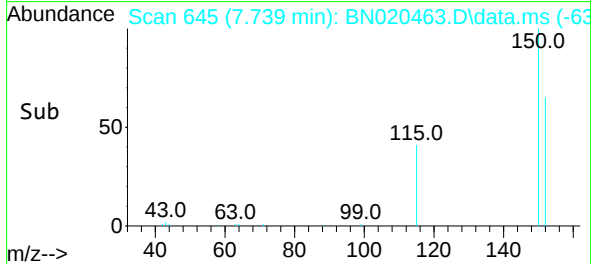


#2
 1,4-Dioxane
 Concen: 0.134 ng
 RT: 3.232 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BN020463.D
 Acq: 26 Jun 2022 13:05

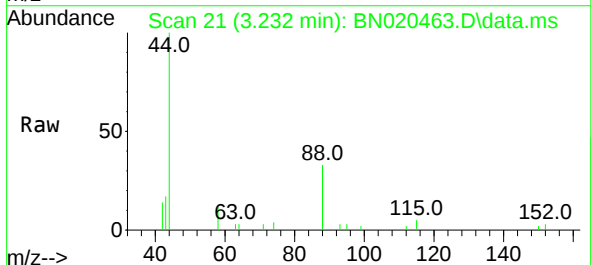

Tgt Ion: 88 Resp: 398
 Ion Ratio Lower Upper
 88 100
 43 39.2 30.2 45.2
 58 88.2 73.0 109.6

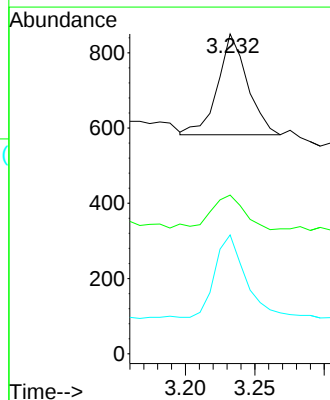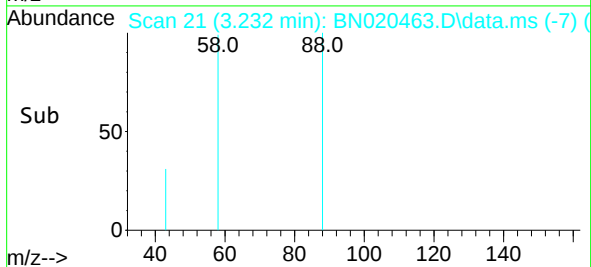



#3

n-Nitrosodimethylamine

Concen: 0.107 ng

RT: 3.572 min Scan# 61

Delta R.T. 0.014 min

Lab File: BN020463.D

Acq: 26 Jun 2022 13:05

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion: 42 Resp: 289

Ion Ratio Lower Upper

42 100

74 124.9 84.0 126.0

44 0.0 9.8 14.8#

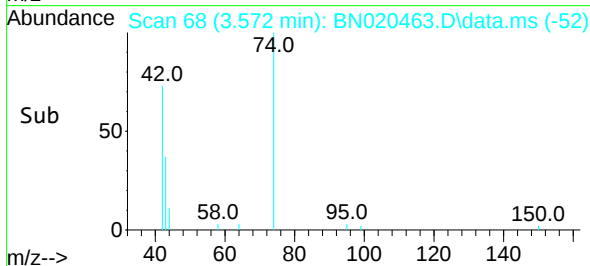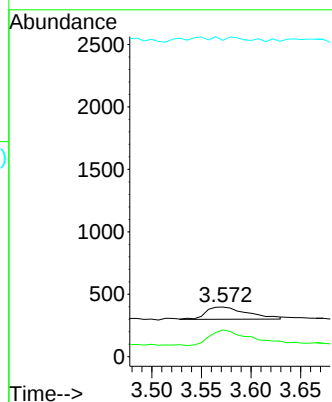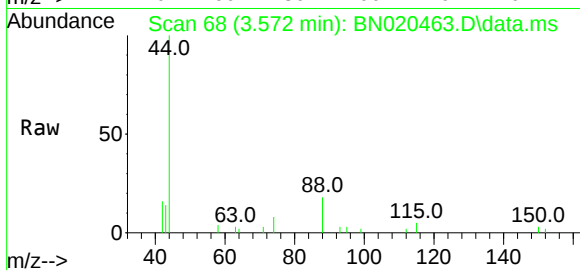

#4

2-Fluorophenol

Concen: 0.111 ng

RT: 5.348 min Scan# 314

Delta R.T. -0.000 min

Lab File: BN020463.D

Acq: 26 Jun 2022 13:05




Tgt Ion: 112 Resp: 845

Ion Ratio Lower Upper

112 100

64 61.2 49.1 73.7

63 33.3 26.3 39.5

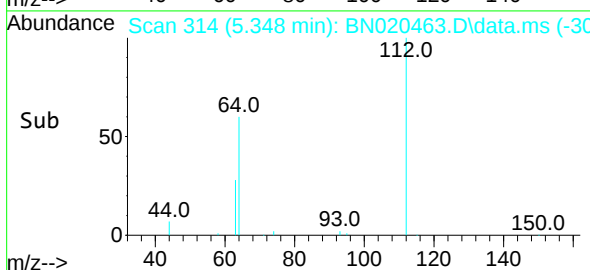

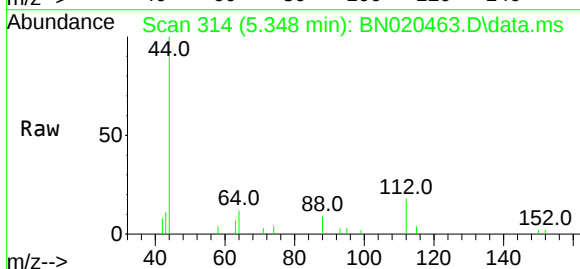




#5
Phenol-d6
Concen: 0.093 ng
RT: 6.952 min Scan# 51
Delta R.T. 0.007 min
Lab File: BN020463.D
Acq: 26 Jun 2022 13:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1

Tgt Ion: 99 Resp: 907
Ion Ratio Lower Upper
99 100
42 23.6 19.3 28.9
71 34.2 27.5 41.3

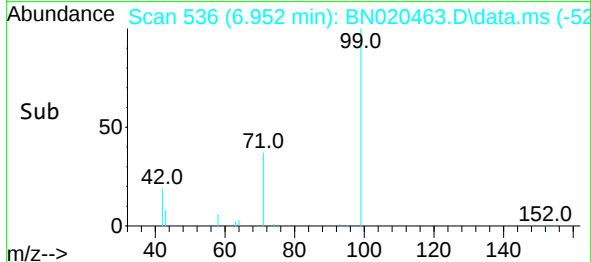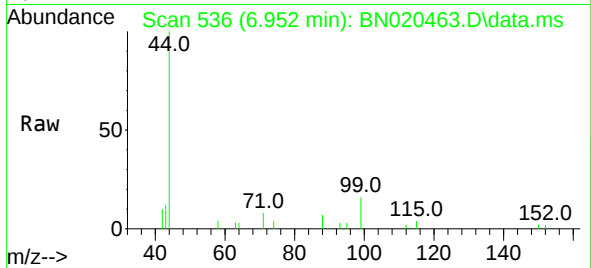

#6
bis(2-Chloroethyl)ether
Concen: 0.097 ng
RT: 7.175 min Scan# 567
Delta R.T. 0.007 min
Lab File: BN020463.D
Acq: 26 Jun 2022 13:05

Tgt Ion: 93 Resp: 738
Ion Ratio Lower Upper
93 100
63 84.6 67.4 101.0
95 35.2 26.5 39.7

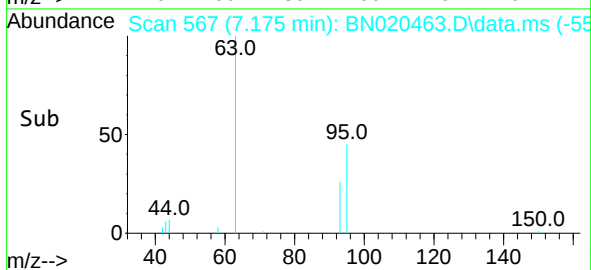

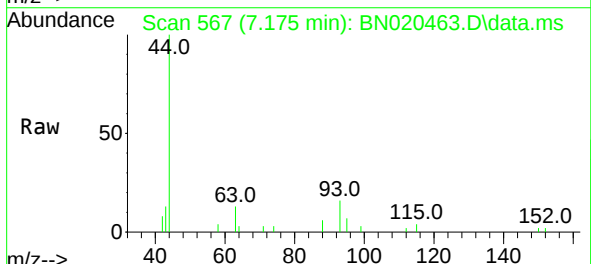




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.530 min Scan# 91
Delta R.T. 0.011 min
Lab File: BN020463.D
Acq: 26 Jun 2022 13:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1

Tgt Ion:	136	Resp:	7929
Ion Ratio	Lower	Upper	
136	100		
137	12.0	9.0	13.6
54	8.6	6.2	9.2
68	5.9	4.4	6.6

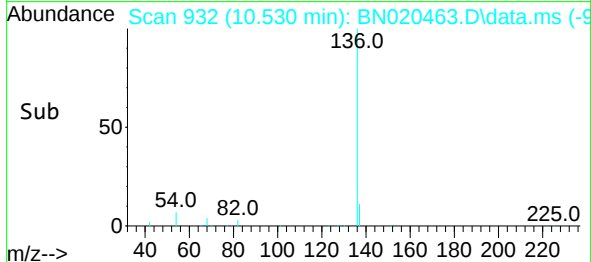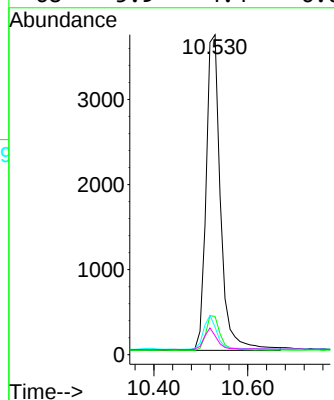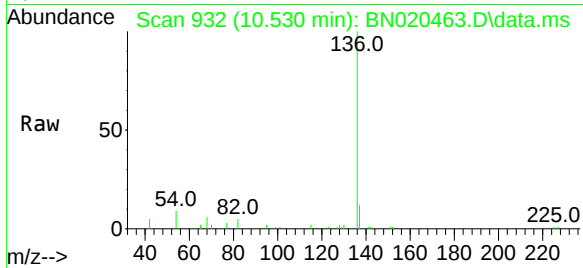

#8
Nitrobenzene-d5
Concen: 0.111 ng
RT: 8.897 min Scan# 779
Delta R.T. -0.000 min
Lab File: BN020463.D
Acq: 26 Jun 2022 13:05

Tgt Ion:	82	Resp:	615
Ion Ratio	Lower	Upper	
82	100		
128	48.2	35.0	52.6
54	70.1	46.2	69.4


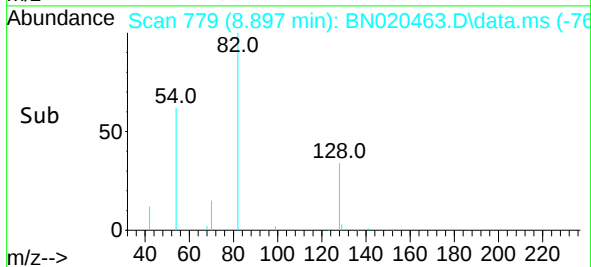
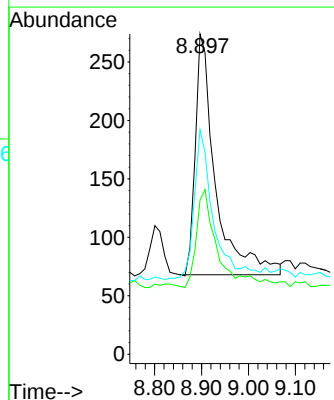
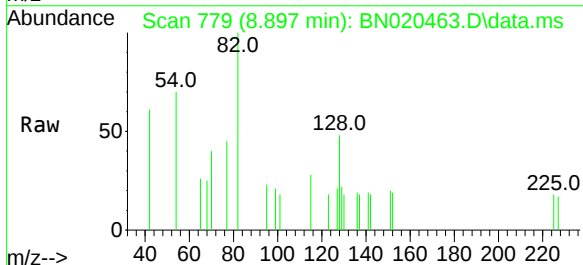




#9
Naphthalene
Concen: 0.102 ng
RT: 10.573 min Scan# 91
Delta R.T. -0.000 min
Lab File: BN020463.D
Acq: 26 Jun 2022 13:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1

Tgt Ion:128 Resp: 2411
Ion Ratio Lower Upper
128 100
129 15.1 8.9 13.3#
127 17.3 10.8 16.2#

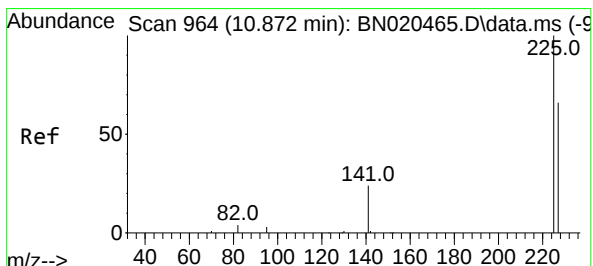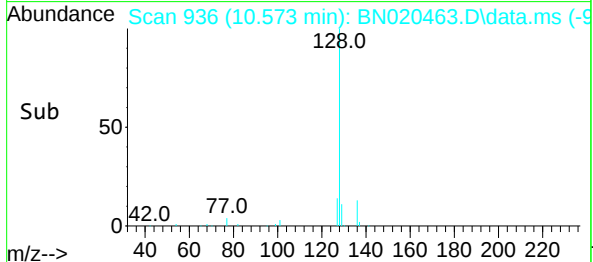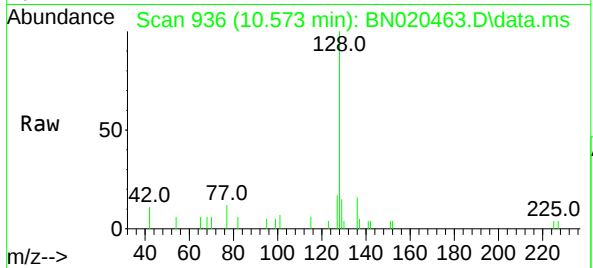

#10
Hexachlorobutadiene
Concen: 0.116 ng
RT: 10.872 min Scan# 964
Delta R.T. -0.000 min
Lab File: BN020463.D
Acq: 26 Jun 2022 13:05

Tgt Ion:225 Resp: 461
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 65.5 50.9 76.3


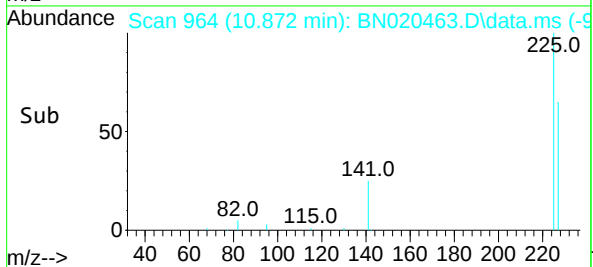

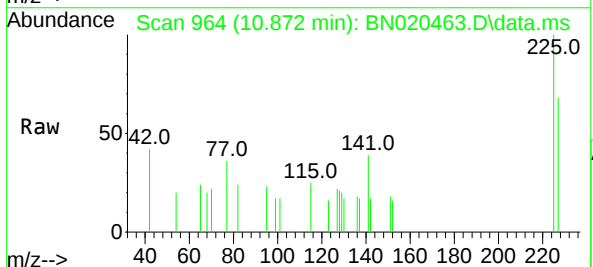




#11
2-Methylnaphthalene-d10
Concen: 0.093 ng
RT: 12.121 min Scan# 1185
Delta R.T. -0.000 min
Lab File: BN020463.D
Acq: 26 Jun 2022 13:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1

Tgt Ion:152 Resp: 1374
Ion Ratio Lower Upper
152 100
151 19.1 16.2 24.4

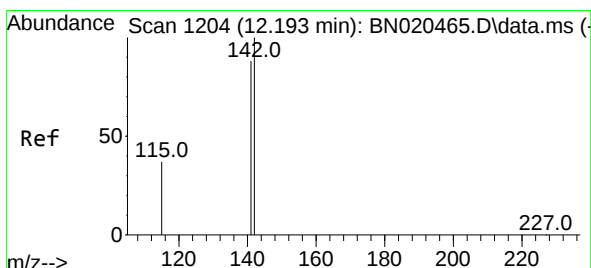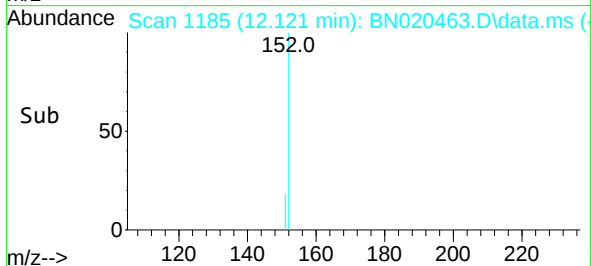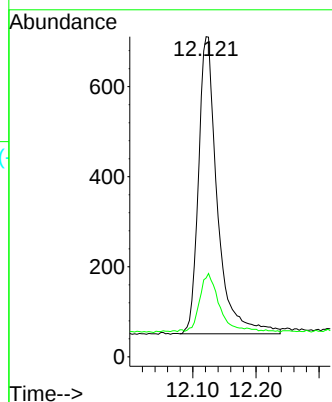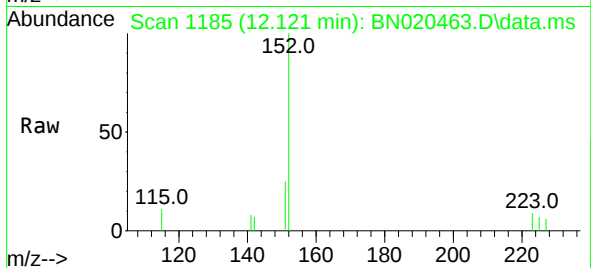

#12
2-Methylnaphthalene
Concen: 0.092 ng
RT: 12.197 min Scan# 1205
Delta R.T. 0.004 min
Lab File: BN020463.D
Acq: 26 Jun 2022 13:05

Tgt Ion:142 Resp: 1589
Ion Ratio Lower Upper
142 100
141 88.9 71.6 107.4
115 43.3 29.8 44.8

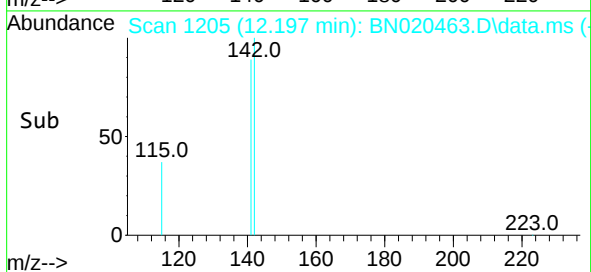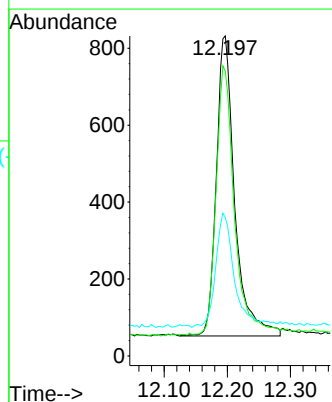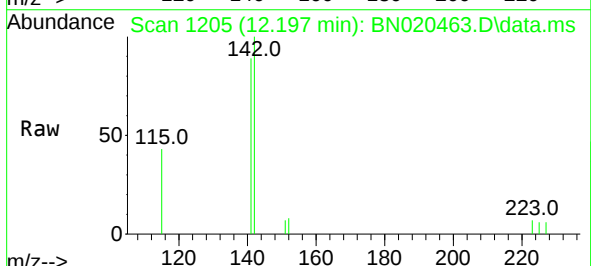



#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.367 min Scan# 14

Delta R.T. -0.000 min

Lab File: BN020463.D

Acq: 26 Jun 2022 13:05

Instrument :

BNA_N

ClientSampleId :

SSTDIC0.1





Tgt Ion:164 Resp: 4702

Ion Ratio Lower Upper

164 100

162 103.4 82.1 123.1

160 48.4 38.6 58.0

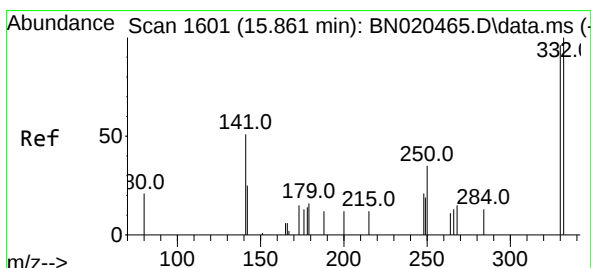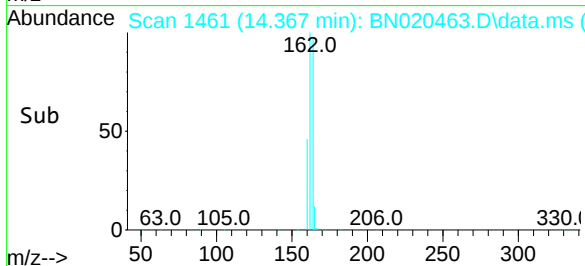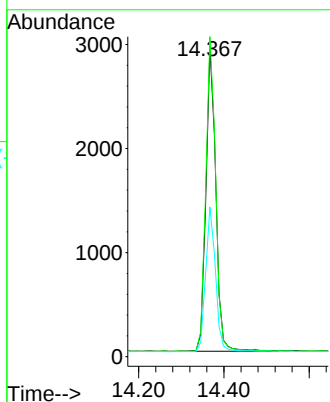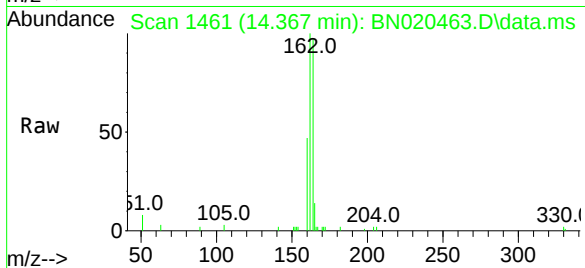

#14

2,4,6-Tribromophenol

Concen: 0.084 ng

RT: 15.872 min Scan# 1602

Delta R.T. 0.010 min

Lab File: BN020463.D

Acq: 26 Jun 2022 13:05




Tgt Ion:330 Resp: 188

Ion Ratio Lower Upper

330 100

332 322.9 77.6 116.4#

141 50.5 41.0 61.4

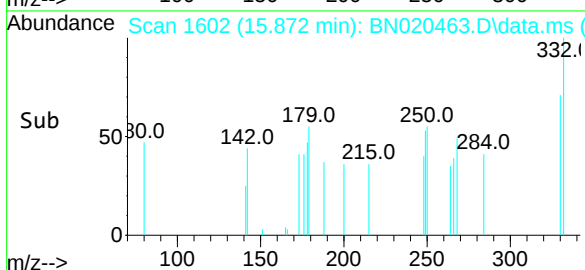
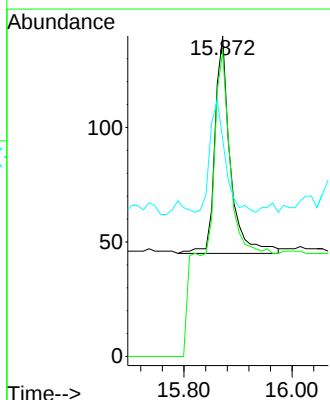
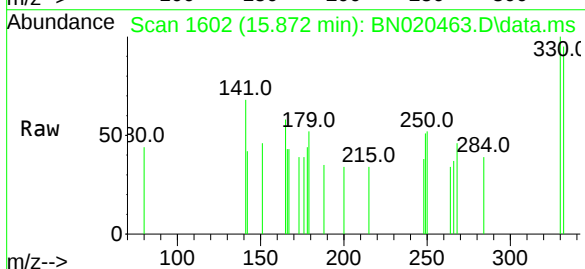




#15
2-Fluorobiphenyl
Concen: 0.118 ng
RT: 12.998 min Scan# 1333
Delta R.T. -0.000 min
Lab File: BN020463.D
Acq: 26 Jun 2022 13:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1

Tgt Ion:	172	Resp:	1988
Ion	Ratio	Lower	Upper
172	100		
171	37.5	27.2	40.8
170	26.0	18.2	27.4

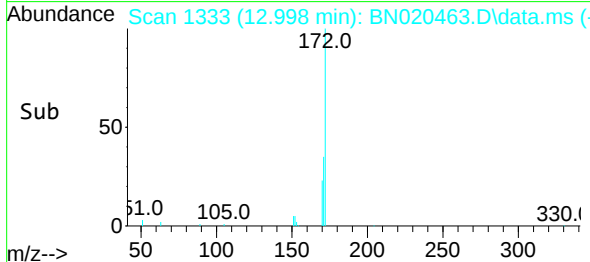

#16
Acenaphthylene
Concen: 0.098 ng
RT: 14.089 min Scan# 1435
Delta R.T. -0.000 min
Lab File: BN020463.D
Acq: 26 Jun 2022 13:05

Tgt Ion:	152	Resp:	2153
Ion	Ratio	Lower	Upper
152	100		
151	20.3	16.2	24.4
153	13.3	10.7	16.1

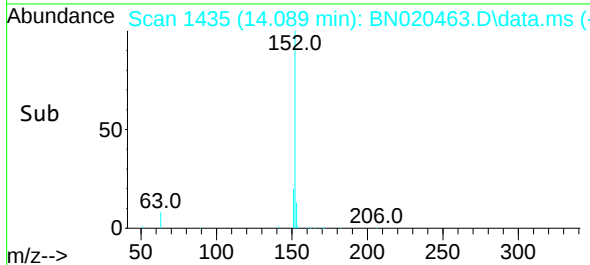

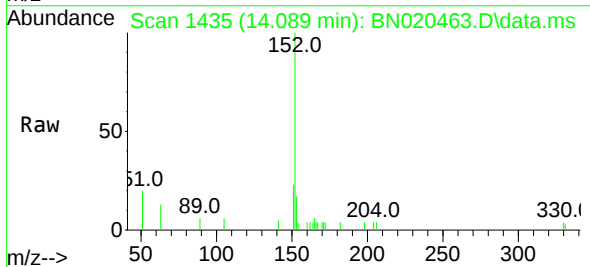




#17
Acenaphthene
Concen: 0.102 ng
RT: 14.431 min Scan# 1467
Delta R.T. -0.000 min
Lab File: BN020463.D
Acq: 26 Jun 2022 13:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1

Tgt Ion:154 Resp: 1572
Ion Ratio Lower Upper
154 100
153 114.8 87.5 131.3
152 56.3 43.8 65.6

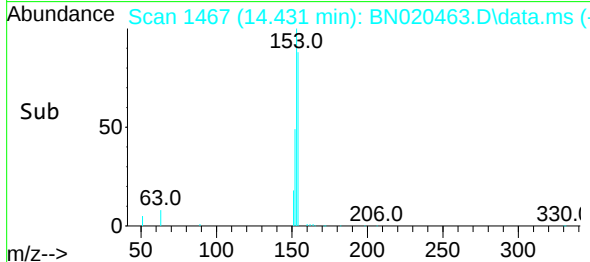

#18
Fluorene
Concen: 0.095 ng
RT: 15.425 min Scan# 1560
Delta R.T. 0.011 min
Lab File: BN020463.D
Acq: 26 Jun 2022 13:05

Tgt Ion:166 Resp: 2104
Ion Ratio Lower Upper
166 100
165 98.1 78.6 118.0
167 13.1 10.8 16.2


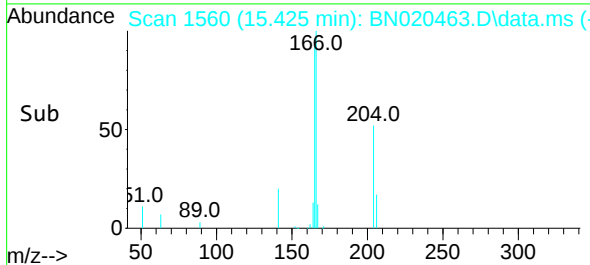

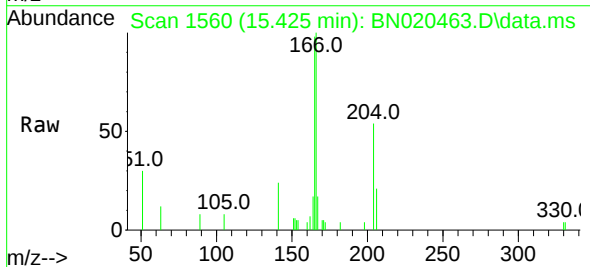




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.113 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN020463.D
Acq: 26 Jun 2022 13:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1

Tgt Ion:188 Resp: 9869
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 12.0 7.4 11.2#

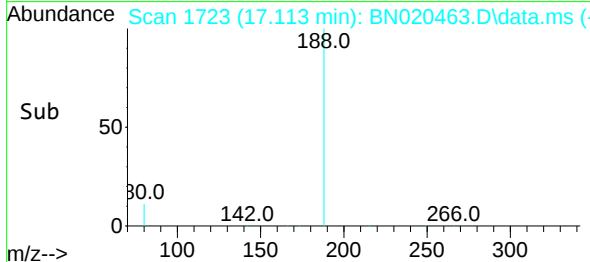

#20
4,6-Dinitro-2-methylphenol
Concen: 0.054 ng
RT: 15.532 min Scan# 1570
Delta R.T. 0.021 min
Lab File: BN020463.D
Acq: 26 Jun 2022 13:05

Tgt Ion:198 Resp: 84
Ion Ratio Lower Upper
198 100
182 75.0 12.1 18.1#
77 0.0 0.0 0.0

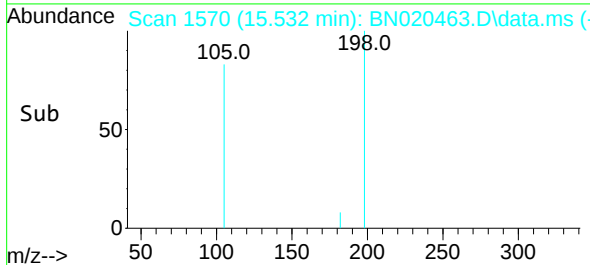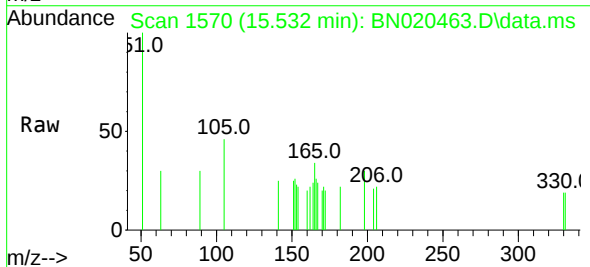



#21

4-Bromophenyl-phenylether

Concen: 0.108 ng

RT: 16.313 min Scan# 1645

Delta R.T. -0.000 min

Lab File: BN020463.D

Acq: 26 Jun 2022 13:05

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:248 Resp: 587

Ion Ratio Lower Upper

248 100

250 99.8 75.3 112.9

141 79.0 67.3 100.9

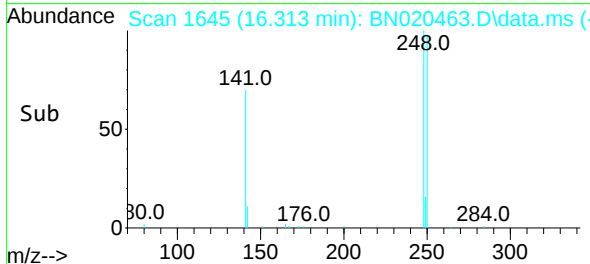

#22

Hexachlorobenzene

Concen: 0.109 ng

RT: 16.425 min Scan# 1656

Delta R.T. -0.000 min

Lab File: BN020463.D

Acq: 26 Jun 2022 13:05




Tgt Ion:284 Resp: 671

Ion Ratio Lower Upper

284 100

142 45.0 35.2 52.8

249 37.3 26.6 40.0

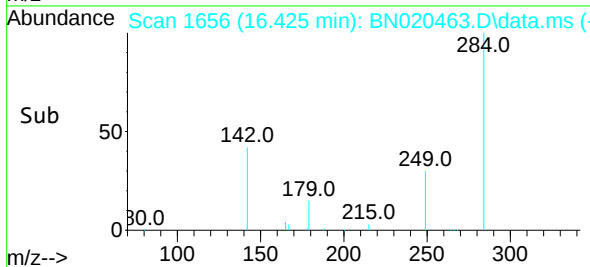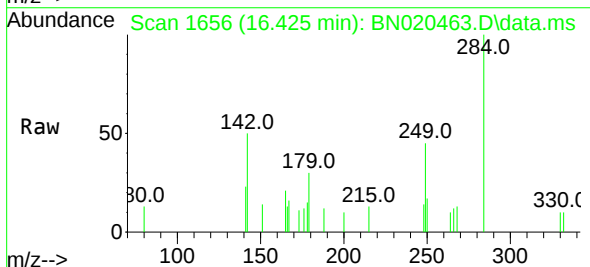



#23

Atrazine

Concen: 0.116 ng

RT: 16.579 min Scan# 1671

Delta R.T. -0.000 min

Lab File: BN020463.D

Acq: 26 Jun 2022 13:05

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:200 Resp: 471

Ion Ratio Lower Upper

200 100

173 41.7 23.6 35.4#

215 52.8 36.6 54.8

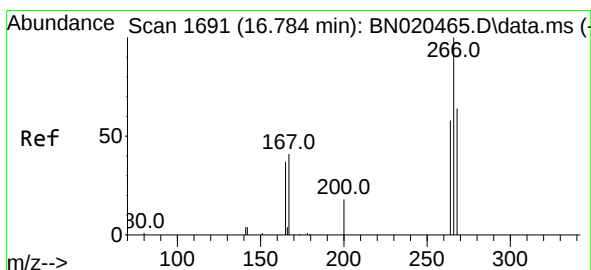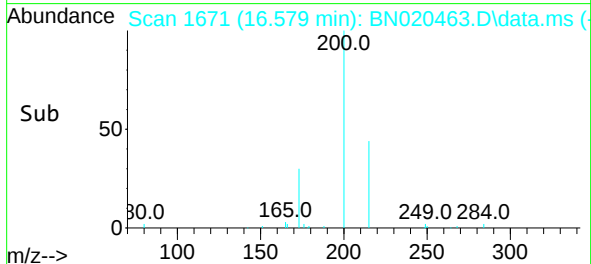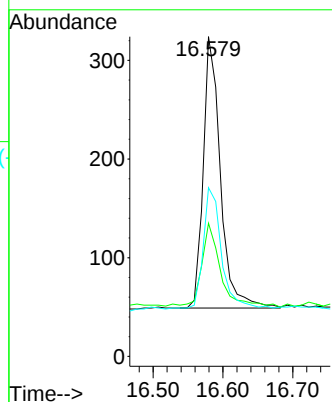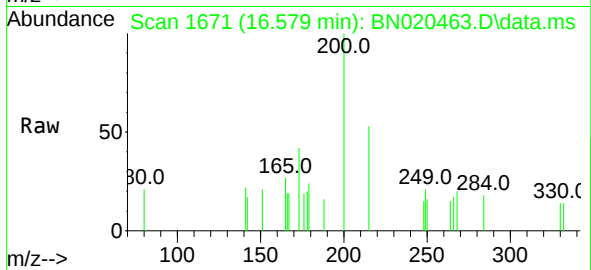

#24

Pentachlorophenol

Concen: 0.050 ng

RT: 16.784 min Scan# 1691

Delta R.T. -0.000 min

Lab File: BN020463.D

Acq: 26 Jun 2022 13:05




Tgt Ion:266 Resp: 135

Ion Ratio Lower Upper

266 100

264 62.2 51.3 76.9

268 68.9 52.6 79.0


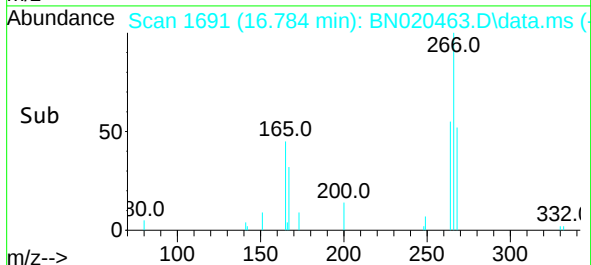

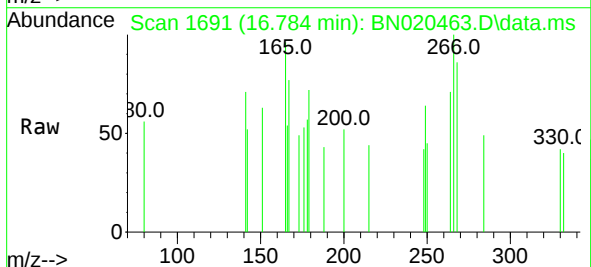




#25
Phenanthrene
Concen: 0.104 ng
RT: 17.154 min Scan# 1727
Delta R.T. -0.000 min
Lab File: BN020463.D
Acq: 26 Jun 2022 13:05




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1

Tgt Ion:178 Resp: 3518
Ion Ratio Lower Upper
178 100
176 19.5 15.3 22.9
179 16.5 12.2 18.4

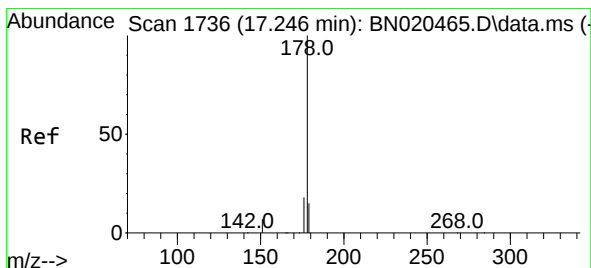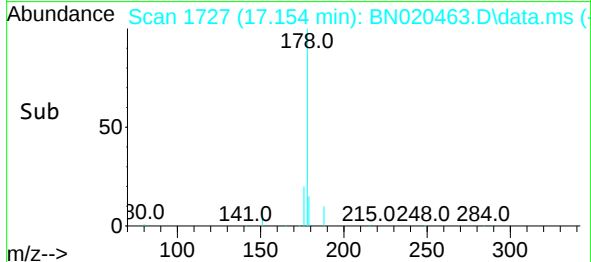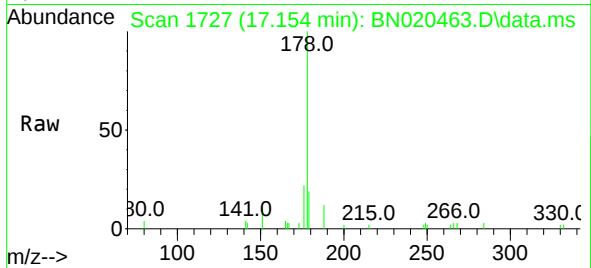

#26
Anthracene
Concen: 0.096 ng
RT: 17.246 min Scan# 1736
Delta R.T. -0.000 min
Lab File: BN020463.D
Acq: 26 Jun 2022 13:05

Tgt Ion:178 Resp: 2806
Ion Ratio Lower Upper
178 100
176 19.1 14.9 22.3
179 14.7 12.2 18.4

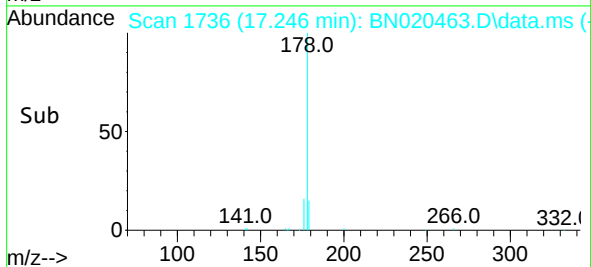

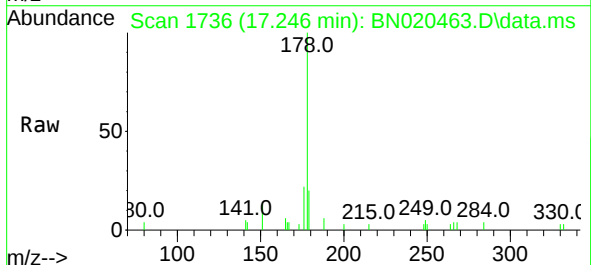




#27
Fluoranthene-d10
Concen: 0.088 ng
RT: 19.152 min Scan# 2082
Delta R.T. 0.004 min
Lab File: BN020463.D
Acq: 26 Jun 2022 13:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:212 Resp: 3043
Ion Ratio Lower Upper
212 100
106 16.4 12.6 19.0
104 10.0 7.2 10.8

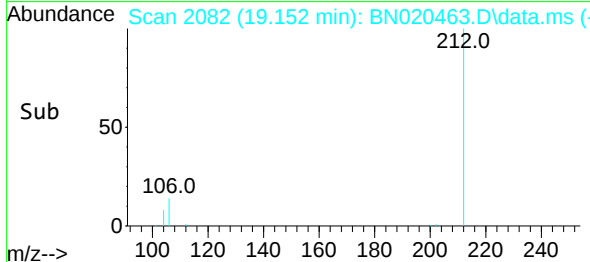

#28
Fluoranthene
Concen: 0.083 ng
RT: 19.181 min Scan# 2089
Delta R.T. -0.000 min
Lab File: BN020463.D
Acq: 26 Jun 2022 13:05

Tgt Ion:202 Resp: 3709
Ion Ratio Lower Upper
202 100
101 13.1 9.6 14.4
203 17.2 13.5 20.3

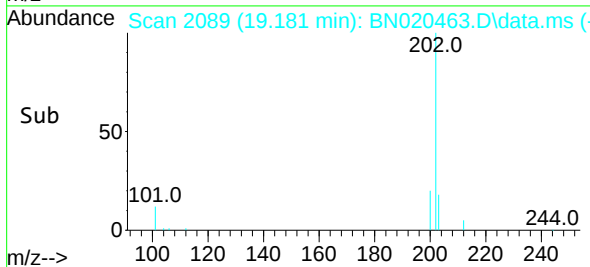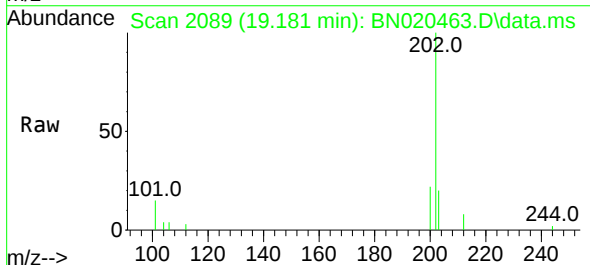

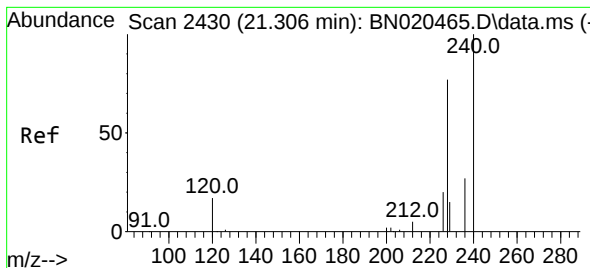

#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.306 min Scan# 2430

Delta R.T. -0.000 min

Lab File: BN020463.D

Acq: 26 Jun 2022 13:05

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:240 Resp: 8823

Ion Ratio Lower Upper

240 100

120 19.6 14.6 21.8

236 28.3 22.6 33.8

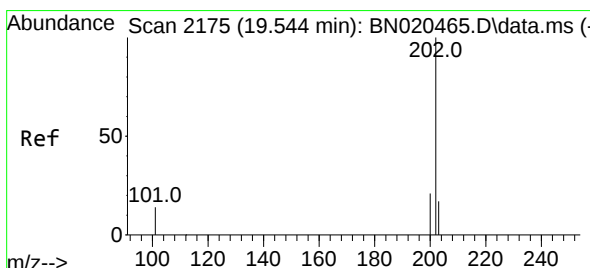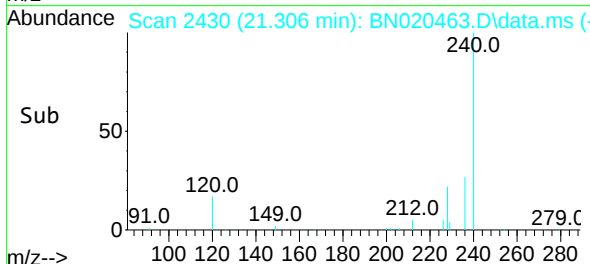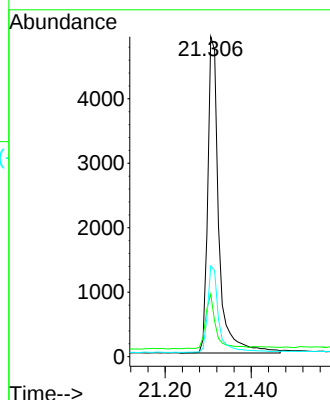

#30

Pyrene

Concen: 0.123 ng

RT: 19.544 min Scan# 2175

Delta R.T. -0.000 min

Lab File: BN020463.D

Acq: 26 Jun 2022 13:05




Tgt Ion:202 Resp: 4001

Ion Ratio Lower Upper

202 100

200 20.7 16.6 25.0

203 18.4 14.2 21.2

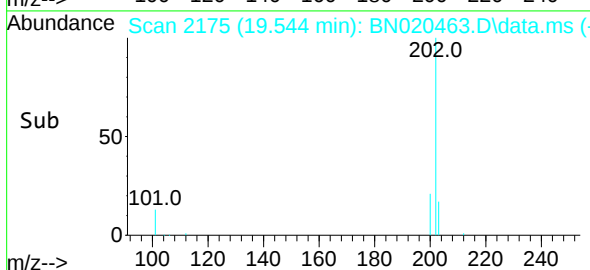
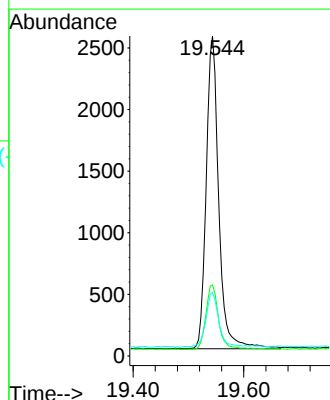
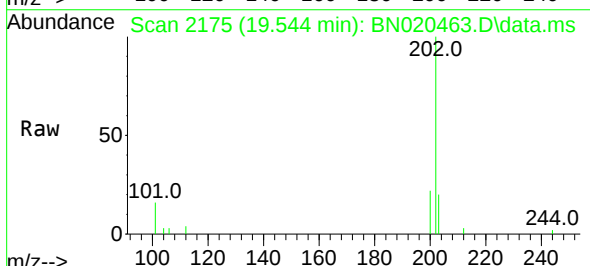




#31
 Terphenyl-d14
 Concen: 0.128 ng
 RT: 19.750 min Scan# 21
 Delta R.T. -0.004 min
 Lab File: BN020463.D
 Acq: 26 Jun 2022 13:05




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1

Tgt Ion:244 Resp: 2251
 Ion Ratio Lower Upper
 244 100
 212 12.0 7.1 10.7#
 122 0.0 0.0 0.0

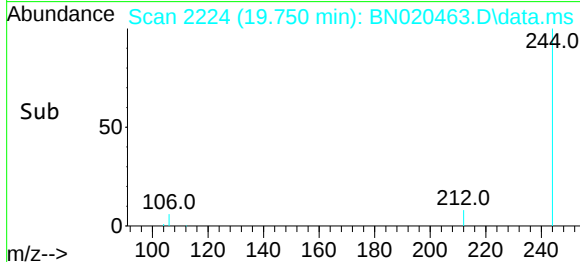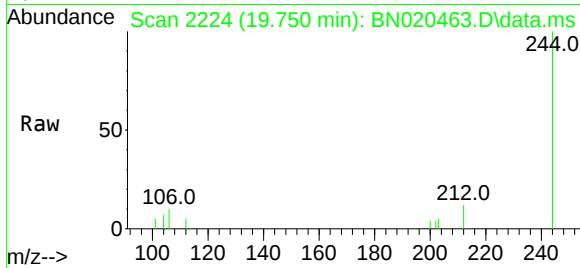

#32
 Benzo(a)anthracene
 Concen: 0.102 ng
 RT: 21.297 min Scan# 2429
 Delta R.T. -0.000 min
 Lab File: BN020463.D
 Acq: 26 Jun 2022 13:05

Tgt Ion:228 Resp: 3216
 Ion Ratio Lower Upper
 228 100
 226 28.3 21.2 31.8
 229 21.6 15.6 23.4


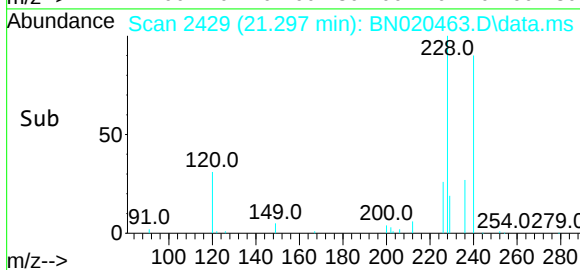

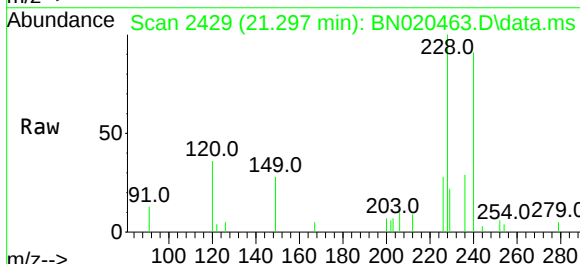




#33
Chrysene
Concen: 0.100 ng
RT: 21.351 min Scan# 2435
Delta R.T. 0.009 min
Lab File: BN020463.D
Acq: 26 Jun 2022 13:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1

Tgt Ion:228 Resp: 3617
Ion Ratio Lower Upper
228 100
226 32.1 23.4 35.0
229 22.3 15.7 23.5

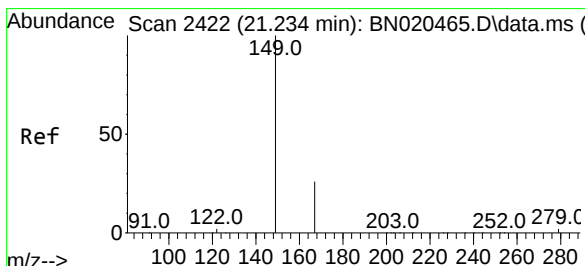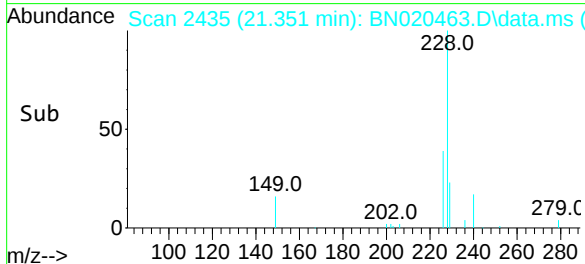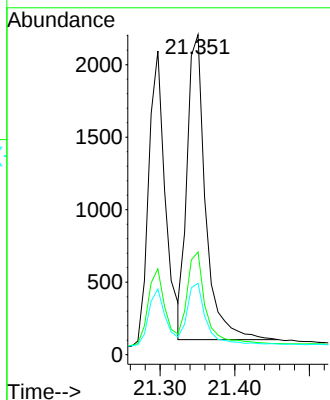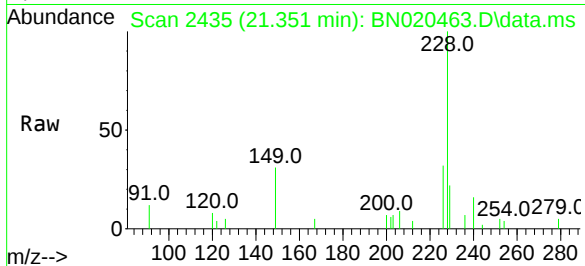

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.158 ng
RT: 21.234 min Scan# 2422
Delta R.T. -0.000 min
Lab File: BN020463.D
Acq: 26 Jun 2022 13:05

Tgt Ion:149 Resp: 2296
Ion Ratio Lower Upper
149 100
167 26.1 21.7 32.5
279 4.4 2.2 3.2#

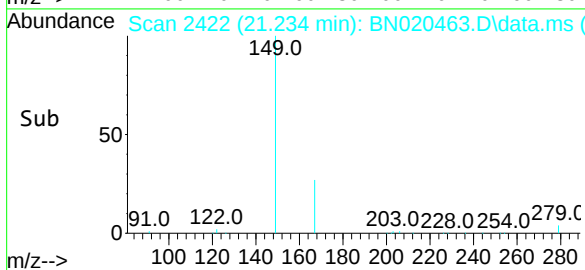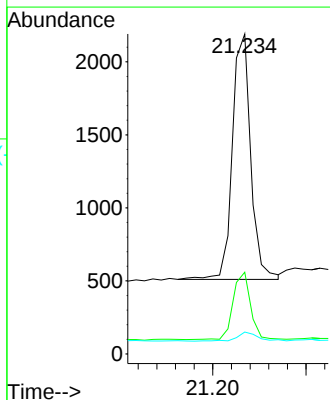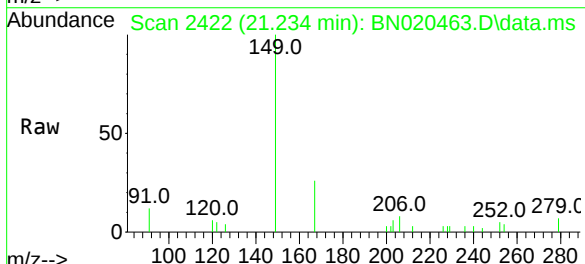



#35

Perylene-d12

Concen: 0.400 ng

RT: 23.597 min Scan# 2960

Delta R.T. -0.003 min

Lab File: BN020463.D

Acq: 26 Jun 2022 13:05

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:264 Resp: 8556

Ion Ratio Lower Upper

264 100

260 26.4 20.9 31.3

265 45.2 28.0 42.0#

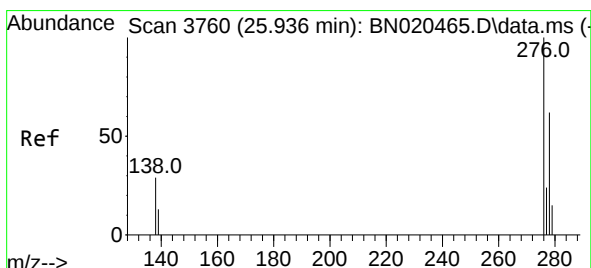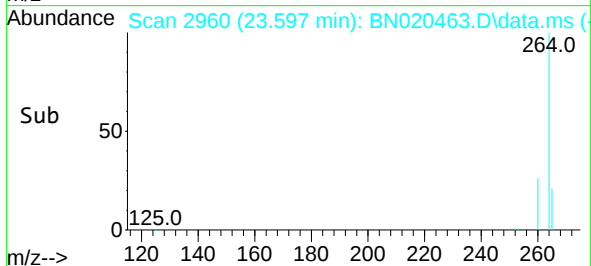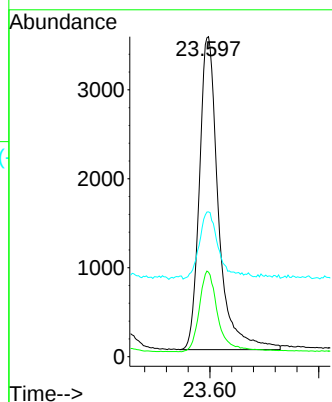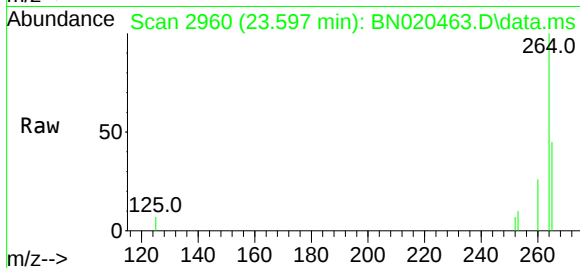

#36

Indeno(1,2,3-cd)pyrene

Concen: 0.087 ng

RT: 25.939 min Scan# 3761

Delta R.T. 0.003 min

Lab File: BN020463.D

Acq: 26 Jun 2022 13:05




Tgt Ion:276 Resp: 3648

Ion Ratio Lower Upper

276 100

138 27.3 25.9 38.9

277 24.7 19.8 29.8

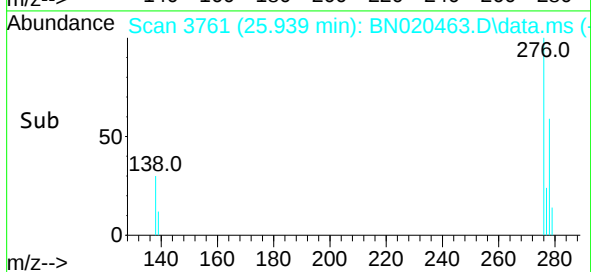
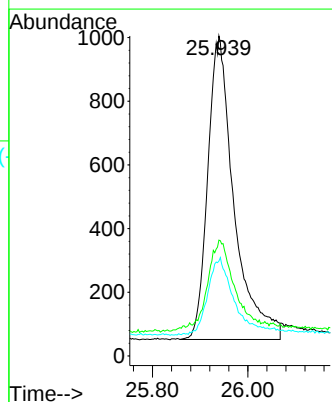
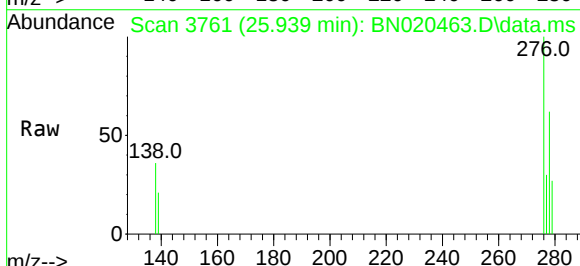




#37
Benzo(b)fluoranthene
Concen: 0.095 ng
RT: 22.910 min Scan# 21
Delta R.T. 0.003 min
Lab File: BN020463.D
Acq: 26 Jun 2022 13:05




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1

Tgt Ion:252 Resp: 3209
Ion Ratio Lower Upper
252 100
253 36.8 18.5 27.7#
125 30.0 11.4 17.0#

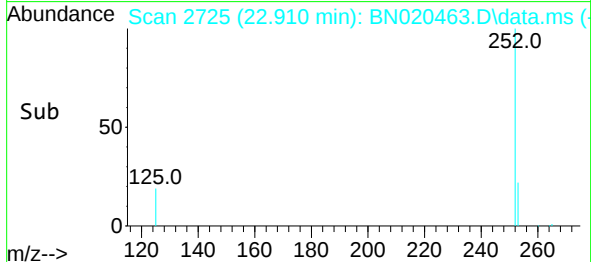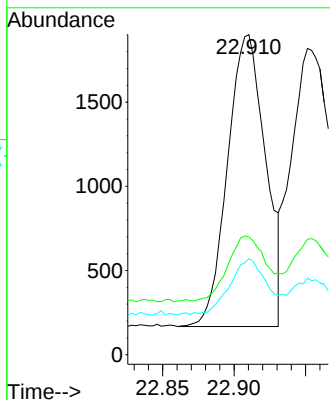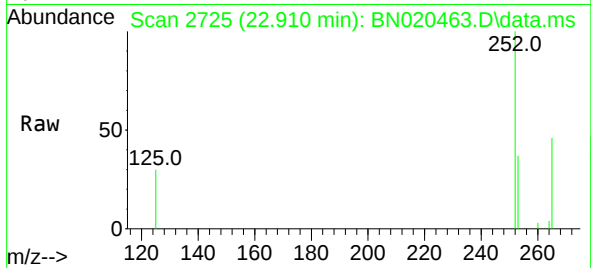

#38
Benzo(k)fluoranthene
Concen: 0.097 ng
RT: 22.951 min Scan# 2739
Delta R.T. -0.003 min
Lab File: BN020463.D
Acq: 26 Jun 2022 13:05

Tgt Ion:252 Resp: 3368
Ion Ratio Lower Upper
252 100
253 37.7 18.0 27.0#
125 25.0 11.0 16.4#

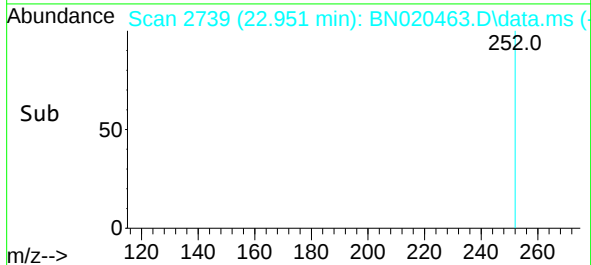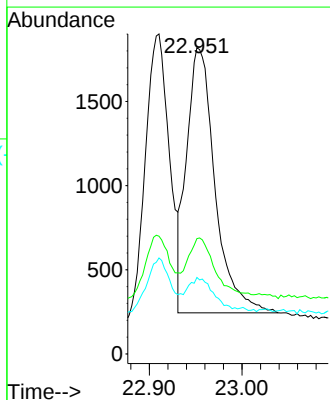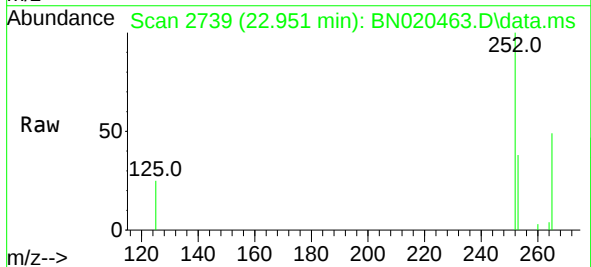



#39

Benzo(a)pyrene

Concen: 0.095 ng

RT: 23.495 min Scan# 2925

Delta R.T. -0.003 min

Lab File: BN020463.D

Acq: 26 Jun 2022 13:05

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1




Tgt Ion:252 Resp: 2789

Ion Ratio Lower Upper

252 100

253 43.3 19.0 28.4#

125 39.6 13.8 20.8#

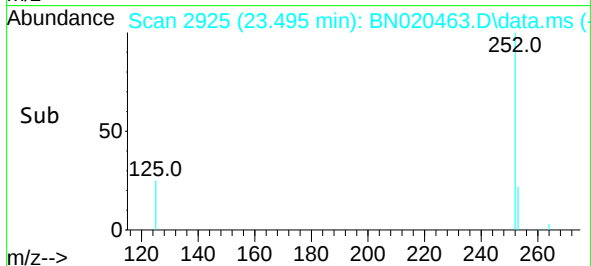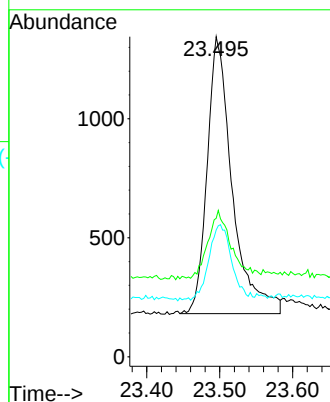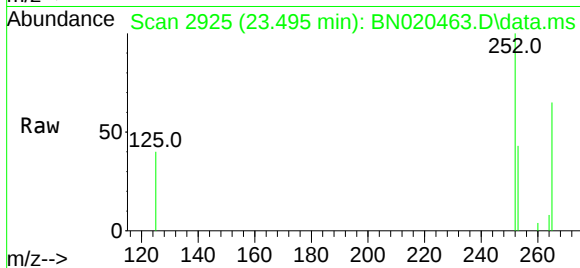

#40

Dibenzo(a,h)anthracene

Concen: 0.086 ng

RT: 25.951 min Scan# 3765

Delta R.T. 0.003 min

Lab File: BN020463.D

Acq: 26 Jun 2022 13:05




Tgt Ion:278 Resp: 2864

Ion Ratio Lower Upper

278 100

139 29.2 18.6 28.0#


279 38.5 19.7 29.5#

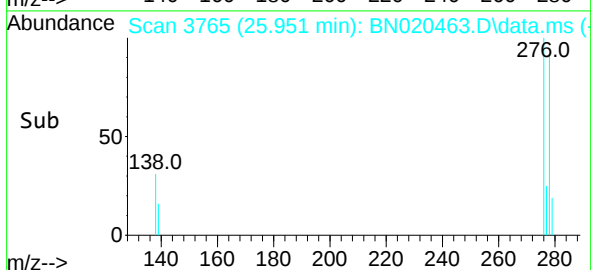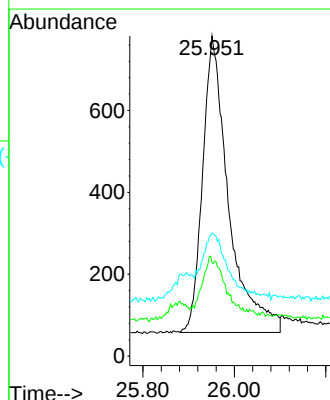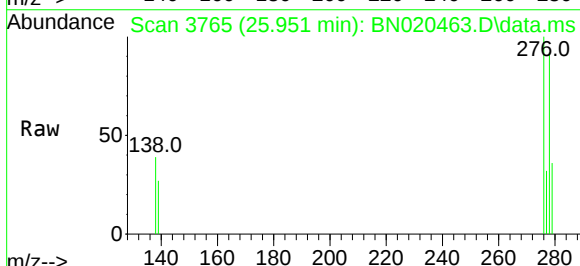



#41
 Benzo(g,h,i)perylene
 Concen: 0.088 ng
 RT: 26.656 min Scan# 40
 Delta R.T. 0.003 min
 Lab File: BN020463.D
 Acq: 26 Jun 2022 13:05

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1

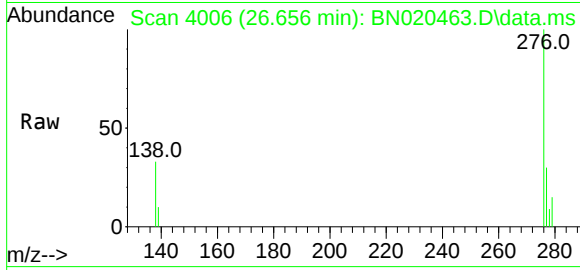

Tgt Ion: 276 Resp: 3264
 Ion Ratio Lower Upper
 276 100
 277 29.7 19.5 29.3#
 138 33.1 22.6 34.0

