

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062622\
 Data File : BN020464.D
 Acq On : 26 Jun 2022 13:57
 Operator : CG/JU
 Sample : SSTDICC0.2
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2

Quant Time: Jun 27 01:37:30 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 27 01:36:24 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.739	152	3177	0.400	ng	0.00
7) Naphthalene-d8	10.519	136	8949	0.400	ng	# 0.00
13) Acenaphthene-d10	14.367	164	5208	0.400	ng	0.00
19) Phenanthrene-d10	17.113	188	10988	0.400	ng	# 0.00
29) Chrysene-d12	21.315	240	9120	0.400	ng	# 0.00
35) Perylene-d12	23.600	264	8530	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.341	112	1816	0.195	ng	0.00
5) Phenol-d6	6.944	99	2052	0.171	ng	0.00
8) Nitrobenzene-d5	8.886	82	1448	0.232	ng	-0.01
11) 2-Methylnaphthalene-d10	12.117	152	2969	0.178	ng	0.00
14) 2,4,6-Tribromophenol	15.872	330	368	0.149	ng	0.01
15) 2-Fluorobiphenyl	12.998	172	4263	0.229	ng	0.00
27) Fluoranthene-d10	19.151	212	6296	0.163	ng	0.00
31) Terphenyl-d14	19.750	244	4522	0.249	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.232	88	853	0.234	ng	97
3) n-Nitrosodimethylamine	3.557	42	759	0.229	ng	# 92
6) bis(2-Chloroethyl)ether	7.168	93	1744	0.187	ng	99
9) Naphthalene	10.573	128	5316	0.199	ng	97
10) Hexachlorobutadiene	10.861	225	1003	0.223	ng	# 99
12) 2-Methylnaphthalene	12.189	142	3424	0.175	ng	98
16) Acenaphthylene	14.089	152	4610	0.189	ng	99
17) Acenaphthene	14.431	154	3356	0.197	ng	96
18) Fluorene	15.414	166	4369	0.179	ng	99
20) 4,6-Dinitro-2-methylph...	15.521	198	175	0.102	ng	# 21
21) 4-Bromophenyl-phenylether	16.313	248	1289	0.212	ng	88
22) Hexachlorobenzene	16.425	284	1422	0.208	ng	97
23) Atrazine	16.579	200	974	0.216	ng	# 94
24) Pentachlorophenol	16.784	266	263	0.087	ng	90
25) Phenanthrene	17.154	178	7533	0.199	ng	99
26) Anthracene	17.246	178	6070	0.186	ng	100
28) Fluoranthene	19.181	202	7635	0.153	ng	99
30) Pyrene	19.543	202	8044	0.239	ng	100
32) Benzo(a)anthracene	21.297	228	6296	0.192	ng	96
33) Chrysene	21.351	228	7337	0.197	ng	99
34) Bis(2-ethylhexyl)phtha...	21.234	149	3906	0.260	ng	97
36) Indeno(1,2,3-cd)pyrene	25.939	276	6865	0.164	ng	98
37) Benzo(b)fluoranthene	22.910	252	6156	0.183	ng	# 87
38) Benzo(k)fluoranthene	22.954	252	6410	0.185	ng	# 88
39) Benzo(a)pyrene	23.498	252	5345	0.182	ng	# 79
40) Dibenzo(a,h)anthracene	25.954	278	5472	0.164	ng	# 92
41) Benzo(g,h,i)perylene	26.650	276	6240	0.168	ng	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062622\
Data File : BN020464.D
Acq On : 26 Jun 2022 13:57
Operator : CG/JU
Sample : SSTDICC0.2
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2

Quant Time: Jun 27 01:37:30 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 01:36:24 2022
Response via : Initial Calibration








#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.739 min Scan# 64
 Delta R.T. -0.000 min
 Lab File: BN020464.D
 Acq: 26 Jun 2022 13:57




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2

Tgt Ion:152 Resp: 3177
 Ion Ratio Lower Upper
 152 100
 150 152.8 127.9 191.9
 115 64.2 51.4 77.2



#2
 1,4-Dioxane
 Concen: 0.234 ng
 RT: 3.232 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BN020464.D
 Acq: 26 Jun 2022 13:57

Tgt Ion: 88 Resp: 853
 Ion Ratio Lower Upper
 88 100
 43 33.9 30.2 45.2
 58 89.9 73.0 109.6








#3
 n-Nitrosodimethylamine
 Concen: 0.229 ng
 RT: 3.557 min Scan# 60
 Delta R.T. -0.000 min
 Lab File: BN020464.D
 Acq: 26 Jun 2022 13:57




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2

Tgt Ion: 42 Resp: 759
 Ion Ratio Lower Upper
 42 100
 74 108.4 84.0 126.0
 44 31.0 9.8 14.8#



#4
 2-Fluorophenol
 Concen: 0.195 ng
 RT: 5.341 min Scan# 313
 Delta R.T. -0.007 min
 Lab File: BN020464.D
 Acq: 26 Jun 2022 13:57


Tgt Ion: 112 Resp: 1816
 Ion Ratio Lower Upper
 112 100
 64 63.5 49.1 73.7
 63 30.4 26.3 39.5








#5
Phenol-d6
Concen: 0.171 ng
RT: 6.944 min Scan# 51
Delta R.T. -0.000 min
Lab File: BN020464.D
Acq: 26 Jun 2022 13:57

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2






Tgt Ion:	99	Resp:	2052
Ion	Ratio	Lower	Upper
99	100		
42	21.5	19.3	28.9
71	36.0	27.5	41.3



#6
bis(2-Chloroethyl)ether
Concen: 0.187 ng
RT: 7.168 min Scan# 566
Delta R.T. -0.000 min
Lab File: BN020464.D
Acq: 26 Jun 2022 13:57

Tgt Ion:	93	Resp:	1744
Ion	Ratio	Lower	Upper
93	100		
63	83.0	67.4	101.0
95	33.5	26.5	39.7








#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.519 min Scan# 91
Delta R.T. -0.000 min
Lab File: BN020464.D
Acq: 26 Jun 2022 13:57




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2

Tgt Ion:136 Resp: 8949
Ion Ratio Lower Upper
136 100
137 12.0 9.0 13.6
54 10.8 6.2 9.2#
68 7.0 4.4 6.6#



#8
Nitrobenzene-d5
Concen: 0.232 ng
RT: 8.886 min Scan# 778
Delta R.T. -0.011 min
Lab File: BN020464.D
Acq: 26 Jun 2022 13:57

Tgt Ion: 82 Resp: 1448
Ion Ratio Lower Upper
82 100
128 38.9 35.0 52.6
54 65.8 46.2 69.4









#9
Naphthalene
Concen: 0.199 ng
RT: 10.573 min Scan# 91
Delta R.T. -0.000 min
Lab File: BN020464.D
Acq: 26 Jun 2022 13:57




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2

Tgt Ion:	128	Resp:	5316
Ion Ratio	Lower	Upper	
128	100		
129	12.7	8.9	13.3
127	14.5	10.8	16.2



#10
Hexachlorobutadiene
Concen: 0.223 ng
RT: 10.861 min Scan# 963
Delta R.T. -0.011 min
Lab File: BN020464.D
Acq: 26 Jun 2022 13:57

Tgt Ion:	225	Resp:	1003
Ion Ratio	Lower	Upper	
225	100		
223	0.0	0.0	0.0
227	62.5	50.9	76.3





#11

2-Methylnaphthalene-d10

Concen: 0.178 ng

RT: 12.117 min Scan# 1184

Delta R.T. -0.004 min

Lab File: BN020464.D

Acq: 26 Jun 2022 13:57

Instrument :

BNA_N

ClientSampleId :





SSTDICC0.2

Tgt Ion:152 Resp: 2969

Ion Ratio Lower Upper

152 100

151 20.7 16.2 24.4



#12

2-Methylnaphthalene

Concen: 0.175 ng

RT: 12.189 min Scan# 1203

Delta R.T. -0.004 min

Lab File: BN020464.D

Acq: 26 Jun 2022 13:57




Tgt Ion:142 Resp: 3424

Ion Ratio Lower Upper

142 100

141 88.0 71.6 107.4

115 39.5 29.8 44.8





#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.367 min Scan# 1461

Delta R.T. -0.000 min

Lab File: BN020464.D

Acq: 26 Jun 2022 13:57

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2





Tgt Ion:164 Resp: 5208

Ion Ratio Lower Upper

164 100

162 104.4 82.1 123.1

160 49.6 38.6 58.0



#14

2,4,6-Tribromophenol

Concen: 0.149 ng

RT: 15.872 min Scan# 1602

Delta R.T. 0.010 min

Lab File: BN020464.D

Acq: 26 Jun 2022 13:57




Tgt Ion:330 Resp: 368

Ion Ratio Lower Upper

330 100

332 213.3 77.6 116.4#

141 56.8 41.0 61.4








#15
2-Fluorobiphenyl
Concen: 0.229 ng
RT: 12.998 min Scan# 1333
Delta R.T. -0.000 min
Lab File: BN020464.D
Acq: 26 Jun 2022 13:57




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2

Tgt Ion:172 Resp: 4263
Ion Ratio Lower Upper
172 100
171 36.7 27.2 40.8
170 23.7 18.2 27.4



#16
Acenaphthylene
Concen: 0.189 ng
RT: 14.089 min Scan# 1435
Delta R.T. -0.000 min
Lab File: BN020464.D
Acq: 26 Jun 2022 13:57

Tgt Ion:152 Resp: 4610
Ion Ratio Lower Upper
152 100
151 19.7 16.2 24.4
153 12.9 10.7 16.1








#17
Acenaphthene
Concen: 0.197 ng
RT: 14.431 min Scan# 1467
Delta R.T. -0.000 min
Lab File: BN020464.D
Acq: 26 Jun 2022 13:57




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2

Tgt Ion:154 Resp: 3356
Ion Ratio Lower Upper
154 100
153 114.8 87.5 131.3
152 56.3 43.8 65.6



#18
Fluorene
Concen: 0.179 ng
RT: 15.414 min Scan# 1559
Delta R.T. -0.000 min
Lab File: BN020464.D
Acq: 26 Jun 2022 13:57

Tgt Ion:166 Resp: 4369
Ion Ratio Lower Upper
166 100
165 99.6 78.6 118.0
167 13.9 10.8 16.2





#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.113 min Scan# 1723

Delta R.T. -0.000 min

Lab File: BN020464.D

Acq: 26 Jun 2022 13:57

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2





Tgt Ion:188 Resp: 10988

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 11.6 7.4 11.2#



#20

4,6-Dinitro-2-methylphenol

Concen: 0.102 ng

RT: 15.521 min Scan# 1569

Delta R.T. 0.011 min

Lab File: BN020464.D

Acq: 26 Jun 2022 13:57




Tgt Ion:198 Resp: 175

Ion Ratio Lower Upper

198 100

182 47.9 12.1 18.1#

77 0.0 0.0 0.0









#21
4-Bromophenyl-phenylether
Concen: 0.212 ng
RT: 16.313 min Scan# 1645
Delta R.T. -0.000 min
Lab File: BN020464.D
Acq: 26 Jun 2022 13:57




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2

Tgt Ion:	248	Resp:	1289
Ion	Ratio	Lower	Upper
248	100		
250	101.1	75.3	112.9
141	68.8	67.3	100.9

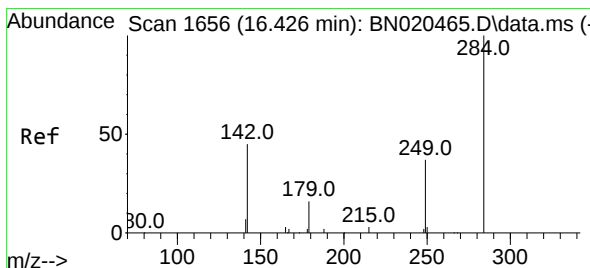

#22
Hexachlorobenzene
Concen: 0.208 ng
RT: 16.425 min Scan# 1656
Delta R.T. -0.000 min
Lab File: BN020464.D
Acq: 26 Jun 2022 13:57

Tgt Ion:	284	Resp:	1422
Ion	Ratio	Lower	Upper
284	100		
142	44.7	35.2	52.8
249	35.9	26.6	40.0





#23

Atrazine

Concen: 0.216 ng

RT: 16.579 min Scan# 1671

Delta R.T. -0.000 min

Lab File: BN020464.D

Acq: 26 Jun 2022 13:57

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2





Tgt Ion:200 Resp: 974

Ion Ratio Lower Upper

200 100

173 36.2 23.6 35.4#

215 46.9 36.6 54.8



#24

Pentachlorophenol

Concen: 0.087 ng

RT: 16.784 min Scan# 1691

Delta R.T. -0.000 min

Lab File: BN020464.D

Acq: 26 Jun 2022 13:57




Tgt Ion:266 Resp: 263


Ion Ratio Lower Upper

266 100

264 55.5 51.3 76.9

268 58.6 52.6 79.0





#25

Phenanthrene

Concen: 0.199 ng

RT: 17.154 min Scan# 1727

Delta R.T. -0.000 min

Lab File: BN020464.D

Acq: 26 Jun 2022 13:57

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2





Tgt Ion:178 Resp: 7533

Ion Ratio Lower Upper

178 100

176 19.6 15.3 22.9

179 15.8 12.2 18.4



#26

Anthracene

Concen: 0.186 ng

RT: 17.246 min Scan# 1736

Delta R.T. -0.000 min

Lab File: BN020464.D

Acq: 26 Jun 2022 13:57




Tgt Ion:178 Resp: 6070

Ion Ratio Lower Upper

178 100

176 18.9 14.9 22.3

179 15.2 12.2 18.4








#27
Fluoranthene-d10
Concen: 0.163 ng
RT: 19.151 min Scan# 2082
Delta R.T. 0.004 min
Lab File: BN020464.D
Acq: 26 Jun 2022 13:57




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:212 Resp: 6296
Ion Ratio Lower Upper
212 100
106 15.2 12.6 19.0
104 8.4 7.2 10.8



#28
Fluoranthene
Concen: 0.153 ng
RT: 19.181 min Scan# 2089
Delta R.T. -0.000 min
Lab File: BN020464.D
Acq: 26 Jun 2022 13:57

Tgt Ion:202 Resp: 7635
Ion Ratio Lower Upper
202 100
101 12.2 9.6 14.4
203 17.1 13.5 20.3





#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.315 min Scan# 2431

Delta R.T. 0.009 min

Lab File: BN020464.D

Acq: 26 Jun 2022 13:57

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2





Tgt Ion:240 Resp: 9120

Ion Ratio Lower Upper

240 100

120 11.8 14.6 21.8#

236 27.3 22.6 33.8



#30

Pyrene

Concen: 0.239 ng

RT: 19.543 min Scan# 2175

Delta R.T. -0.000 min

Lab File: BN020464.D

Acq: 26 Jun 2022 13:57




Tgt Ion:202 Resp: 8044

Ion Ratio Lower Upper

202 100

200 21.1 16.6 25.0

203 17.8 14.2 21.2








#31
 Terphenyl-d14
 Concen: 0.249 ng
 RT: 19.750 min Scan# 21
 Delta R.T. -0.004 min
 Lab File: BN020464.D
 Acq: 26 Jun 2022 13:57




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2

Tgt Ion:244 Resp: 4522
 Ion Ratio Lower Upper
 244 100
 212 10.5 7.1 10.7
 122 0.0 0.0 0.0



#32
 Benzo(a)anthracene
 Concen: 0.192 ng
 RT: 21.297 min Scan# 2429
 Delta R.T. -0.000 min
 Lab File: BN020464.D
 Acq: 26 Jun 2022 13:57

Tgt Ion:228 Resp: 6296
 Ion Ratio Lower Upper
 228 100
 226 28.5 21.2 31.8
 229 20.9 15.6 23.4





#33

Chrysene

Concen: 0.197 ng

RT: 21.351 min Scan# 2435

Delta R.T. 0.009 min

Lab File: BN020464.D

Acq: 26 Jun 2022 13:57

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2




Tgt Ion:228 Resp: 7337

Ion Ratio Lower Upper

228 100

226 30.0 23.4 35.0

229 19.8 15.7 23.5



#34

Bis(2-ethylhexyl)phthalate

Concen: 0.260 ng

RT: 21.234 min Scan# 2422

Delta R.T. -0.000 min

Lab File: BN020464.D

Acq: 26 Jun 2022 13:57




Tgt Ion:149 Resp: 3906

Ion Ratio Lower Upper

149 100

167 25.7 21.7 32.5

279 3.1 2.2 3.2








#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.600 min Scan# 2961
 Delta R.T. -0.000 min
 Lab File: BN020464.D
 Acq: 26 Jun 2022 13:57




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2

Tgt Ion:264 Resp: 8530
 Ion Ratio Lower Upper
 264 100
 260 26.6 20.9 31.3
 265 42.3 28.0 42.0#



#36
 Indeno(1,2,3-cd)pyrene
 Concen: 0.164 ng
 RT: 25.939 min Scan# 3761
 Delta R.T. 0.003 min
 Lab File: BN020464.D
 Acq: 26 Jun 2022 13:57

Tgt Ion:276 Resp: 6865
 Ion Ratio Lower Upper
 276 100
 138 31.2 25.9 38.9
 277 25.6 19.8 29.8





#37

Benzo(b)fluoranthene

Concen: 0.183 ng

RT: 22.910 min Scan# 21

Delta R.T. 0.003 min

Lab File: BN020464.D


Acq: 26 Jun 2022 13:57

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2





Tgt Ion:252 Resp: 6156

Ion Ratio Lower Upper

252 100

253 29.0 18.5 27.7#

125 19.9 11.4 17.0#



#38

Benzo(k)fluoranthene

Concen: 0.185 ng

RT: 22.954 min Scan# 2740

Delta R.T. -0.000 min

Lab File: BN020464.D

Acq: 26 Jun 2022 13:57




Tgt Ion:252 Resp: 6410

Ion Ratio Lower Upper

252 100

253 29.0 18.0 27.0#

125 17.2 11.0 16.4#





#39

Benzo(a)pyrene

Concen: 0.182 ng

RT: 23.498 min Scan# 2926

Delta R.T. -0.000 min

Lab File: BN020464.D


Acq: 26 Jun 2022 13:57

Instrument :



BN020464.D

ClientSampleId :

SSTDICC0.2



Tgt Ion:	252	Resp:	5345
Ion Ratio	Lower	Upper	
252	100		
253	34.1	19.0	28.4#
125	26.5	13.8	20.8#



#40

Dibenzo(a,h)anthracene

Concen: 0.164 ng




RT: 25.954 min Scan# 3766

Delta R.T. 0.006 min

Lab File: BN020464.D

Acq: 26 Jun 2022 13:57

Tgt Ion:	278	Resp:	5472
Ion Ratio	Lower	Upper	
278	100		
139	24.5	18.6	28.0
279	30.8	19.7	29.5#





#41
 Benzo(g,h,i)perylene
 Concen: 0.168 ng
 RT: 26.650 min Scan# 40
 Delta R.T. -0.003 min
 Lab File: BN020464.D
 Acq: 26 Jun 2022 13:57

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2

Tgt Ion:	276	Resp:	6240
Ion Ratio	Lower	Upper	
276	100		
277	26.6	19.5	29.3
138	31.1	22.6	34.0

