

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062622\
 Data File : BN020465.D
 Acq On : 26 Jun 2022 14:37
 Operator : CG/JU
 Sample : SSTDICCC0.4
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICCC0.4

Quant Time: Jun 27 01:37:41 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 27 01:36:24 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.739	152	3071	0.400	ng	0.00
7) Naphthalene-d8	10.520	136	9294	0.400	ng	# 0.00
13) Acenaphthene-d10	14.367	164	5419	0.400	ng	0.00
19) Phenanthrene-d10	17.113	188	11328	0.400	ng	0.00
29) Chrysene-d12	21.306	240	9666	0.400	ng	0.00
35) Perylene-d12	23.600	264	9060	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.348	112	3322	0.369	ng	0.00
5) Phenol-d6	6.944	99	3882	0.335	ng	0.00
8) Nitrobenzene-d5	8.897	82	2746	0.423	ng	0.00
11) 2-Methylnaphthalene-d10	12.121	152	6031	0.349	ng	0.00
14) 2,4,6-Tribromophenol	15.861	330	706	0.274	ng	0.00
15) 2-Fluorobiphenyl	12.998	172	8796	0.454	ng	0.00
27) Fluoranthene-d10	19.147	212	12414	0.313	ng	0.00
31) Terphenyl-d14	19.754	244	9038	0.469	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.232	88	1539	0.438	ng	98
3) n-Nitrosodimethylamine	3.557	42	1371	0.428	ng	# 91
6) bis(2-Chloroethyl)ether	7.168	93	3328	0.370	ng	99
9) Naphthalene	10.573	128	10672	0.385	ng	98
10) Hexachlorobutadiene	10.872	225	1962	0.420	ng	# 98
12) 2-Methylnaphthalene	12.193	142	7076	0.348	ng	98
16) Acenaphthylene	14.089	152	9542	0.376	ng	99
17) Acenaphthene	14.431	154	6843	0.387	ng	96
18) Fluorene	15.415	166	8804	0.346	ng	100
20) 4,6-Dinitro-2-methylph...	15.511	198	430	0.243	ng	# 68
21) 4-Bromophenyl-phenylether	16.313	248	2444	0.391	ng	# 86
22) Hexachlorobenzene	16.426	284	2711	0.384	ng	99
23) Atrazine	16.579	200	1870	0.402	ng	97
24) Pentachlorophenol	16.784	266	510	0.164	ng	97
25) Phenanthrene	17.154	178	14278	0.366	ng	100
26) Anthracene	17.246	178	11940	0.356	ng	99
28) Fluoranthene	19.181	202	15380	0.299	ng	100
30) Pyrene	19.544	202	15959	0.447	ng	100
32) Benzo(a)anthracene	21.297	228	12979	0.374	ng	99
33) Chrysene	21.342	228	14736	0.373	ng	98
34) Bis(2-ethylhexyl)phtha...	21.234	149	6899	0.433	ng	# 98
36) Indeno(1,2,3-cd)pyrene	25.936	276	15397	0.346	ng	98
37) Benzo(b)fluoranthene	22.907	252	13296	0.372	ng	95
38) Benzo(k)fluoranthene	22.954	252	13911	0.377	ng	96
39) Benzo(a)pyrene	23.498	252	11550	0.370	ng	93
40) Dibenzo(a,h)anthracene	25.948	278	12221	0.346	ng	97
41) Benzo(g,h,i)perylene	26.653	276	13712	0.347	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062622\
 Data File : BN020465.D
 Acq On : 26 Jun 2022 14:37
 Operator : CG/JU
 Sample : SSTDICCC0.4
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICCC0.4

Quant Time: Jun 27 01:37:41 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 27 01:36:24 2022
 Response via : Initial Calibration








#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.739 min Scan# 64
 Delta R.T. -0.000 min
 Lab File: BN020465.D
 Acq: 26 Jun 2022 14:37




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICCC0.4

Tgt Ion:152 Resp: 3071
 Ion Ratio Lower Upper
 152 100
 150 156.1 127.9 191.9
 115 65.8 51.4 77.2



#2
 1,4-Dioxane
 Concen: 0.438 ng
 RT: 3.232 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BN020465.D
 Acq: 26 Jun 2022 14:37

Tgt Ion: 88 Resp: 1539
 Ion Ratio Lower Upper
 88 100
 43 34.9 30.2 45.2
 58 92.1 73.0 109.6








#3
 n-Nitrosodimethylamine
 Concen: 0.428 ng
 RT: 3.557 min Scan# 66
 Delta R.T. 0.000 min
 Lab File: BN020465.D
 Acq: 26 Jun 2022 14:37




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.4

Tgt Ion: 42 Resp: 1371
 Ion Ratio Lower Upper
 42 100
 74 113.4 84.0 126.0
 44 4.5 9.8 14.8#



#4
 2-Fluorophenol
 Concen: 0.369 ng
 RT: 5.348 min Scan# 314
 Delta R.T. 0.000 min
 Lab File: BN020465.D
 Acq: 26 Jun 2022 14:37

Tgt Ion: 112 Resp: 3322
 Ion Ratio Lower Upper
 112 100
 64 61.1 49.1 73.7
 63 32.7 26.3 39.5








#5
Phenol-d6
Concen: 0.335 ng
RT: 6.944 min Scan# 51
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion: 99 Resp: 3882
Ion Ratio Lower Upper
99 100
42 22.4 19.3 28.9
71 35.6 27.5 41.3



#6
bis(2-Chloroethyl)ether
Concen: 0.370 ng
RT: 7.168 min Scan# 566
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37

Tgt Ion: 93 Resp: 3328
Ion Ratio Lower Upper
93 100
63 84.0 67.4 101.0
95 33.7 26.5 39.7








#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.520 min Scan# 931
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:	136	Resp:	9294
Ion Ratio	Lower	Upper	
136	100		
137	11.7	9.0	13.6
54	10.8	6.2	9.2#
68	7.3	4.4	6.6#



#8
Nitrobenzene-d5
Concen: 0.423 ng
RT: 8.897 min Scan# 779
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37

Tgt Ion:	82	Resp:	2746
Ion Ratio	Lower	Upper	
82	100		
128	45.7	35.0	52.6
54	57.9	46.2	69.4









#9
Naphthalene
Concen: 0.385 ng
RT: 10.573 min Scan# 91
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:128 Resp: 10672
Ion Ratio Lower Upper
128 100
129 11.8 8.9 13.3
127 14.3 10.8 16.2



#10
Hexachlorobutadiene
Concen: 0.420 ng
RT: 10.872 min Scan# 964
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37

Tgt Ion:225 Resp: 1962
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 62.1 50.9 76.3









#11
2-Methylnaphthalene-d10
Concen: 0.349 ng
RT: 12.121 min Scan# 1185
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:152 Resp: 6031
Ion Ratio Lower Upper
152 100
151 20.4 16.2 24.4

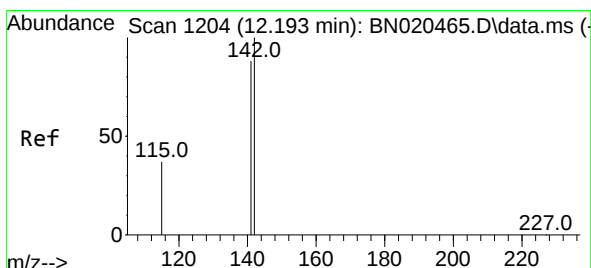

#12
2-Methylnaphthalene
Concen: 0.348 ng
RT: 12.193 min Scan# 1204
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37

Tgt Ion:142 Resp: 7076
Ion Ratio Lower Upper
142 100
141 87.9 71.6 107.4
115 37.9 29.8 44.8





#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.367 min Scan# 1461

Delta R.T. 0.000 min

Lab File: BN020465.D

Acq: 26 Jun 2022 14:37

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:164 Resp: 5419

Ion Ratio Lower Upper

164 100

162 105.3 82.1 123.1

160 49.3 38.6 58.0

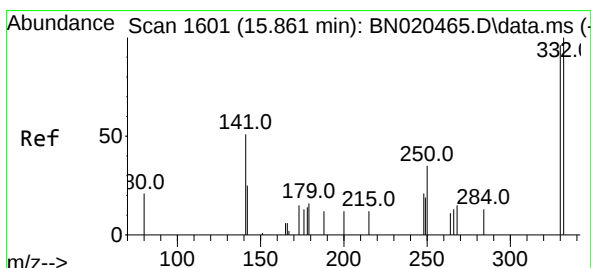

#14

2,4,6-Tribromophenol

Concen: 0.274 ng

RT: 15.861 min Scan# 1601

Delta R.T. 0.000 min

Lab File: BN020465.D

Acq: 26 Jun 2022 14:37




Tgt Ion:330 Resp: 706

Ion Ratio Lower Upper

330 100

332 161.9 77.6 116.4#

141 55.8 41.0 61.4








#15
2-Fluorobiphenyl
Concen: 0.454 ng
RT: 12.998 min Scan# 1333
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:172 Resp: 8796
Ion Ratio Lower Upper
172 100
171 34.9 27.2 40.8
170 23.1 18.2 27.4



#16
Acenaphthylene
Concen: 0.376 ng
RT: 14.089 min Scan# 1435
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37

Tgt Ion:152 Resp: 9542
Ion Ratio Lower Upper
152 100
151 19.6 16.2 24.4
153 12.9 10.7 16.1








#17
Acenaphthene
Concen: 0.387 ng
RT: 14.431 min Scan# 1467
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:154 Resp: 6843
Ion Ratio Lower Upper
154 100
153 114.5 87.5 131.3
152 56.9 43.8 65.6



#18
Fluorene
Concen: 0.346 ng
RT: 15.415 min Scan# 1559
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37

Tgt Ion:166 Resp: 8804
Ion Ratio Lower Upper
166 100
165 98.6 78.6 118.0
167 13.4 10.8 16.2





#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.113 min Scan# 11

Delta R.T. 0.000 min

Lab File: BN020465.D

Acq: 26 Jun 2022 14:37

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:188 Resp: 11328

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 10.7 7.4 11.2



#20

4,6-Dinitro-2-methylphenol

Concen: 0.243 ng

RT: 15.511 min Scan# 1568

Delta R.T. 0.000 min

Lab File: BN020465.D

Acq: 26 Jun 2022 14:37




Tgt Ion:198 Resp: 430


Ion Ratio Lower Upper

198 100

182 28.3 12.1 18.1#

77 0.0 0.0 0.0









#21
4-Bromophenyl-phenylether
Concen: 0.391 ng
RT: 16.313 min Scan# 1645
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:248 Resp: 2444
Ion Ratio Lower Upper
248 100
250 100.9 75.3 112.9
141 64.6 67.3 100.9#



#22
Hexachlorobenzene
Concen: 0.384 ng
RT: 16.426 min Scan# 1656
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37

Tgt Ion:284 Resp: 2711
Ion Ratio Lower Upper
284 100
142 44.6 35.2 52.8
249 34.1 26.6 40.0





#23

Atrazine

Concen: 0.402 ng

RT: 16.579 min Scan# 1671

Delta R.T. 0.000 min

Lab File: BN020465.D

Acq: 26 Jun 2022 14:37

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:200 Resp: 1870

Ion Ratio Lower Upper

200 100

173 33.1 23.6 35.4

215 45.9 36.6 54.8

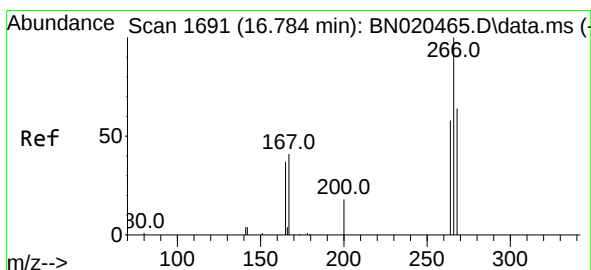

#24

Pentachlorophenol

Concen: 0.164 ng

RT: 16.784 min Scan# 1691

Delta R.T. 0.000 min

Lab File: BN020465.D

Acq: 26 Jun 2022 14:37




Tgt Ion:266 Resp: 510

Ion Ratio Lower Upper

266 100

264 61.4 51.3 76.9

268 67.1 52.6 79.0









#25
Phenanthrene
Concen: 0.366 ng
RT: 17.154 min Scan# 1727
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:178 Resp: 14278
Ion Ratio Lower Upper
178 100
176 19.1 15.3 22.9
179 15.5 12.2 18.4

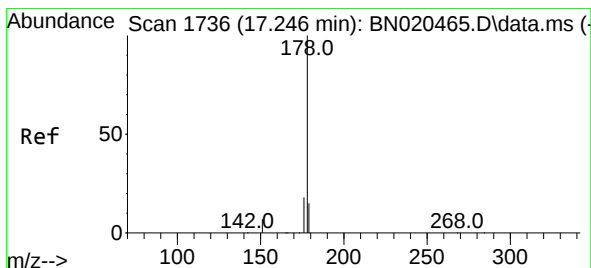

#26
Anthracene
Concen: 0.356 ng
RT: 17.246 min Scan# 1736
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37

Tgt Ion:178 Resp: 11940
Ion Ratio Lower Upper
178 100
176 18.2 14.9 22.3
179 15.0 12.2 18.4








#27
Fluoranthene-d10
Concen: 0.313 ng
RT: 19.147 min Scan# 2081
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:212 Resp: 12414
Ion Ratio Lower Upper
212 100
106 15.5 12.6 19.0
104 8.4 7.2 10.8



#28
Fluoranthene
Concen: 0.299 ng
RT: 19.181 min Scan# 2089
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37

Tgt Ion:202 Resp: 15380
Ion Ratio Lower Upper
202 100
101 11.7 9.6 14.4
203 16.8 13.5 20.3





#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.306 min Scan# 2430

Delta R.T. 0.000 min

Lab File: BN020465.D

Acq: 26 Jun 2022 14:37

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:240 Resp: 9666

Ion Ratio Lower Upper

240 100

120 18.4 14.6 21.8

236 27.8 22.6 33.8



#30

Pyrene

Concen: 0.447 ng

RT: 19.544 min Scan# 2175

Delta R.T. 0.000 min

Lab File: BN020465.D

Acq: 26 Jun 2022 14:37




Tgt Ion:202 Resp: 15959

Ion Ratio Lower Upper

202 100

200 21.0 16.6 25.0

203 17.5 14.2 21.2








#31
 Terphenyl-d14
 Concen: 0.469 ng
 RT: 19.754 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BN020465.D
 Acq: 26 Jun 2022 14:37




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.4


Tgt Ion:244 Resp: 9038
 Ion Ratio Lower Upper
 244 100
 212 9.3 7.1 10.7
 122 0.0 0.0 0.0



#32
 Benzo(a)anthracene
 Concen: 0.374 ng
 RT: 21.297 min Scan# 2429
 Delta R.T. 0.000 min
 Lab File: BN020465.D
 Acq: 26 Jun 2022 14:37

Tgt Ion:228 Resp: 12979
 Ion Ratio Lower Upper
 228 100
 226 27.0 21.2 31.8
 229 20.1 15.6 23.4





#33

Chrysene

Concen: 0.373 ng

RT: 21.342 min Scan# 2434

Delta R.T. 0.000 min

Lab File: BN020465.D

Acq: 26 Jun 2022 14:37

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:228 Resp: 14736

Ion Ratio Lower Upper

228 100

226 31.0 23.4 35.0

229 19.6 15.7 23.5



#34

Bis(2-ethylhexyl)phthalate

Concen: 0.433 ng

RT: 21.234 min Scan# 2422

Delta R.T. 0.000 min

Lab File: BN020465.D

Acq: 26 Jun 2022 14:37




Tgt Ion:149 Resp: 6899


Ion Ratio Lower Upper

149 100

167 26.0 21.7 32.5

279 3.5 2.2 3.2#





#35

Perylene-d12

Concen: 0.400 ng

RT: 23.600 min Scan# 2961

Delta R.T. 0.000 min

Lab File: BN020465.D

Acq: 26 Jun 2022 14:37

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:264 Resp: 9060

Ion Ratio Lower Upper

264 100

260 26.2 20.9 31.3

265 41.1 28.0 42.0

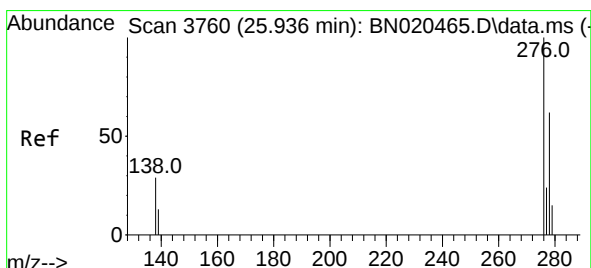

#36

Indeno(1,2,3-cd)pyrene

Concen: 0.346 ng

RT: 25.936 min Scan# 3760

Delta R.T. 0.000 min

Lab File: BN020465.D

Acq: 26 Jun 2022 14:37




Tgt Ion:276 Resp: 15397

Ion Ratio Lower Upper

276 100

138 30.9 25.9 38.9

277 25.3 19.8 29.8








#37
Benzo(b)fluoranthene
Concen: 0.372 ng
RT: 22.907 min Scan# 2724
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:252 Resp: 13296
Ion Ratio Lower Upper
252 100
253 25.6 18.5 27.7
125 16.2 11.4 17.0



#38
Benzo(k)fluoranthene
Concen: 0.377 ng
RT: 22.954 min Scan# 2740
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37

Tgt Ion:252 Resp: 13911
Ion Ratio Lower Upper
252 100
253 25.1 18.0 27.0
125 14.8 11.0 16.4








#39
Benzo(a)pyrene
Concen: 0.370 ng
RT: 23.498 min Scan# 2926
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:	252	Resp:	11550
Ion Ratio	Lower	Upper	
252	100		
253	26.9	19.0	28.4
125	20.7	13.8	20.8



#40
Dibenzo(a,h)anthracene
Concen: 0.346 ng
RT: 25.948 min Scan# 3764
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37

Tgt Ion:	278	Resp:	12221
Ion Ratio	Lower	Upper	
278	100		
139	22.7	18.6	28.0
279	26.6	19.7	29.5





#41
 Benzo(g,h,i)perylene
 Concen: 0.347 ng
 RT: 26.653 min Scan# 40
 Delta R.T. 0.000 min
 Lab File: BN020465.D
 Acq: 26 Jun 2022 14:37

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICCC0.4

Tgt Ion:	276	Resp:	13712
Ion	Ratio	Lower	Upper
276	100		
277	25.3	19.5	29.3
138	28.2	22.6	34.0

