

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062622\
 Data File : BN020469.D
 Acq On : 26 Jun 2022 17:03
 Operator : CG/JU
 Sample : SSTDICC5.0
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Quant Time: Jun 27 01:38:20 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 27 01:36:24 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.739	152	2947	0.400	ng	0.00
7) Naphthalene-d8	10.520	136	8105	0.400	ng	# 0.00
13) Acenaphthene-d10	14.367	164	4826	0.400	ng	0.00
19) Phenanthrene-d10	17.113	188	9789	0.400	ng	0.00
29) Chrysene-d12	21.306	240	9539	0.400	ng	0.00
35) Perylene-d12	23.595	264	8389	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.341	112	36307	4.205	ng	0.00
5) Phenol-d6	6.937	99	47357	4.255	ng	0.00
8) Nitrobenzene-d5	8.886	82	34817	6.153	ng	-0.01
11) 2-Methylnaphthalene-d10	12.117	152	68560	4.550	ng	0.00
14) 2,4,6-Tribromophenol	15.861	330	9965	4.345	ng	0.00
15) 2-Fluorobiphenyl	12.998	172	94513	5.473	ng	0.00
27) Fluoranthene-d10	19.147	212	147161	4.287	ng	0.00
31) Terphenyl-d14	19.750	244	104189	5.480	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.225	88	16776	4.970	ng	93
3) n-Nitrosodimethylamine	3.543	42	17638	5.735	ng	# 92
6) bis(2-Chloroethyl)ether	7.168	93	40373	4.672	ng	98
9) Naphthalene	10.573	128	117275	4.854	ng	99
10) Hexachlorobutadiene	10.872	225	20458	5.024	ng	# 100
12) 2-Methylnaphthalene	12.189	142	79348	4.478	ng	100
16) Acenaphthylene	14.089	152	124330	5.496	ng	99
17) Acenaphthene	14.431	154	76952	4.884	ng	97
18) Fluorene	15.415	166	100064	4.415	ng	100
20) 4,6-Dinitro-2-methylph...	15.500	198	10976	7.178	ng	# 87
21) 4-Bromophenyl-phenylether	16.302	248	28400	5.253	ng	# 87
22) Hexachlorobenzene	16.426	284	30788	5.051	ng	99
23) Atrazine	16.579	200	24062	5.981	ng	98
24) Pentachlorophenol	16.774	266	10112	3.773	ng	98
25) Phenanthrene	17.154	178	161641	4.798	ng	100
26) Anthracene	17.246	178	149687	5.160	ng	100
28) Fluoranthene	19.177	202	182322	4.096	ng	99
30) Pyrene	19.539	202	186583	5.300	ng	100
32) Benzo(a)anthracene	21.288	228	171935	5.025	ng	98
33) Chrysene	21.342	228	176995	4.539	ng	98
34) Bis(2-ethylhexyl)phtha...	21.234	149	96067	6.113	ng	100
36) Indeno(1,2,3-cd)pyrene	25.925	276	197875	4.804	ng	99
37) Benzo(b)fluoranthene	22.902	252	168495	5.086	ng	97
38) Benzo(k)fluoranthene	22.948	252	172150	5.044	ng	98
39) Benzo(a)pyrene	23.492	252	144089	4.985	ng	95
40) Dibenzo(a,h)anthracene	25.945	278	159260	4.866	ng	97
41) Benzo(g,h,i)perylene	26.638	276	167446	4.581	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062622\
 Data File : BN020469.D
 Acq On : 26 Jun 2022 17:03
 Operator : CG/JU
 Sample : SSTDICC5.0
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0


Quant Time: Jun 27 01:38:20 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 27 01:36:24 2022
 Response via : Initial Calibration

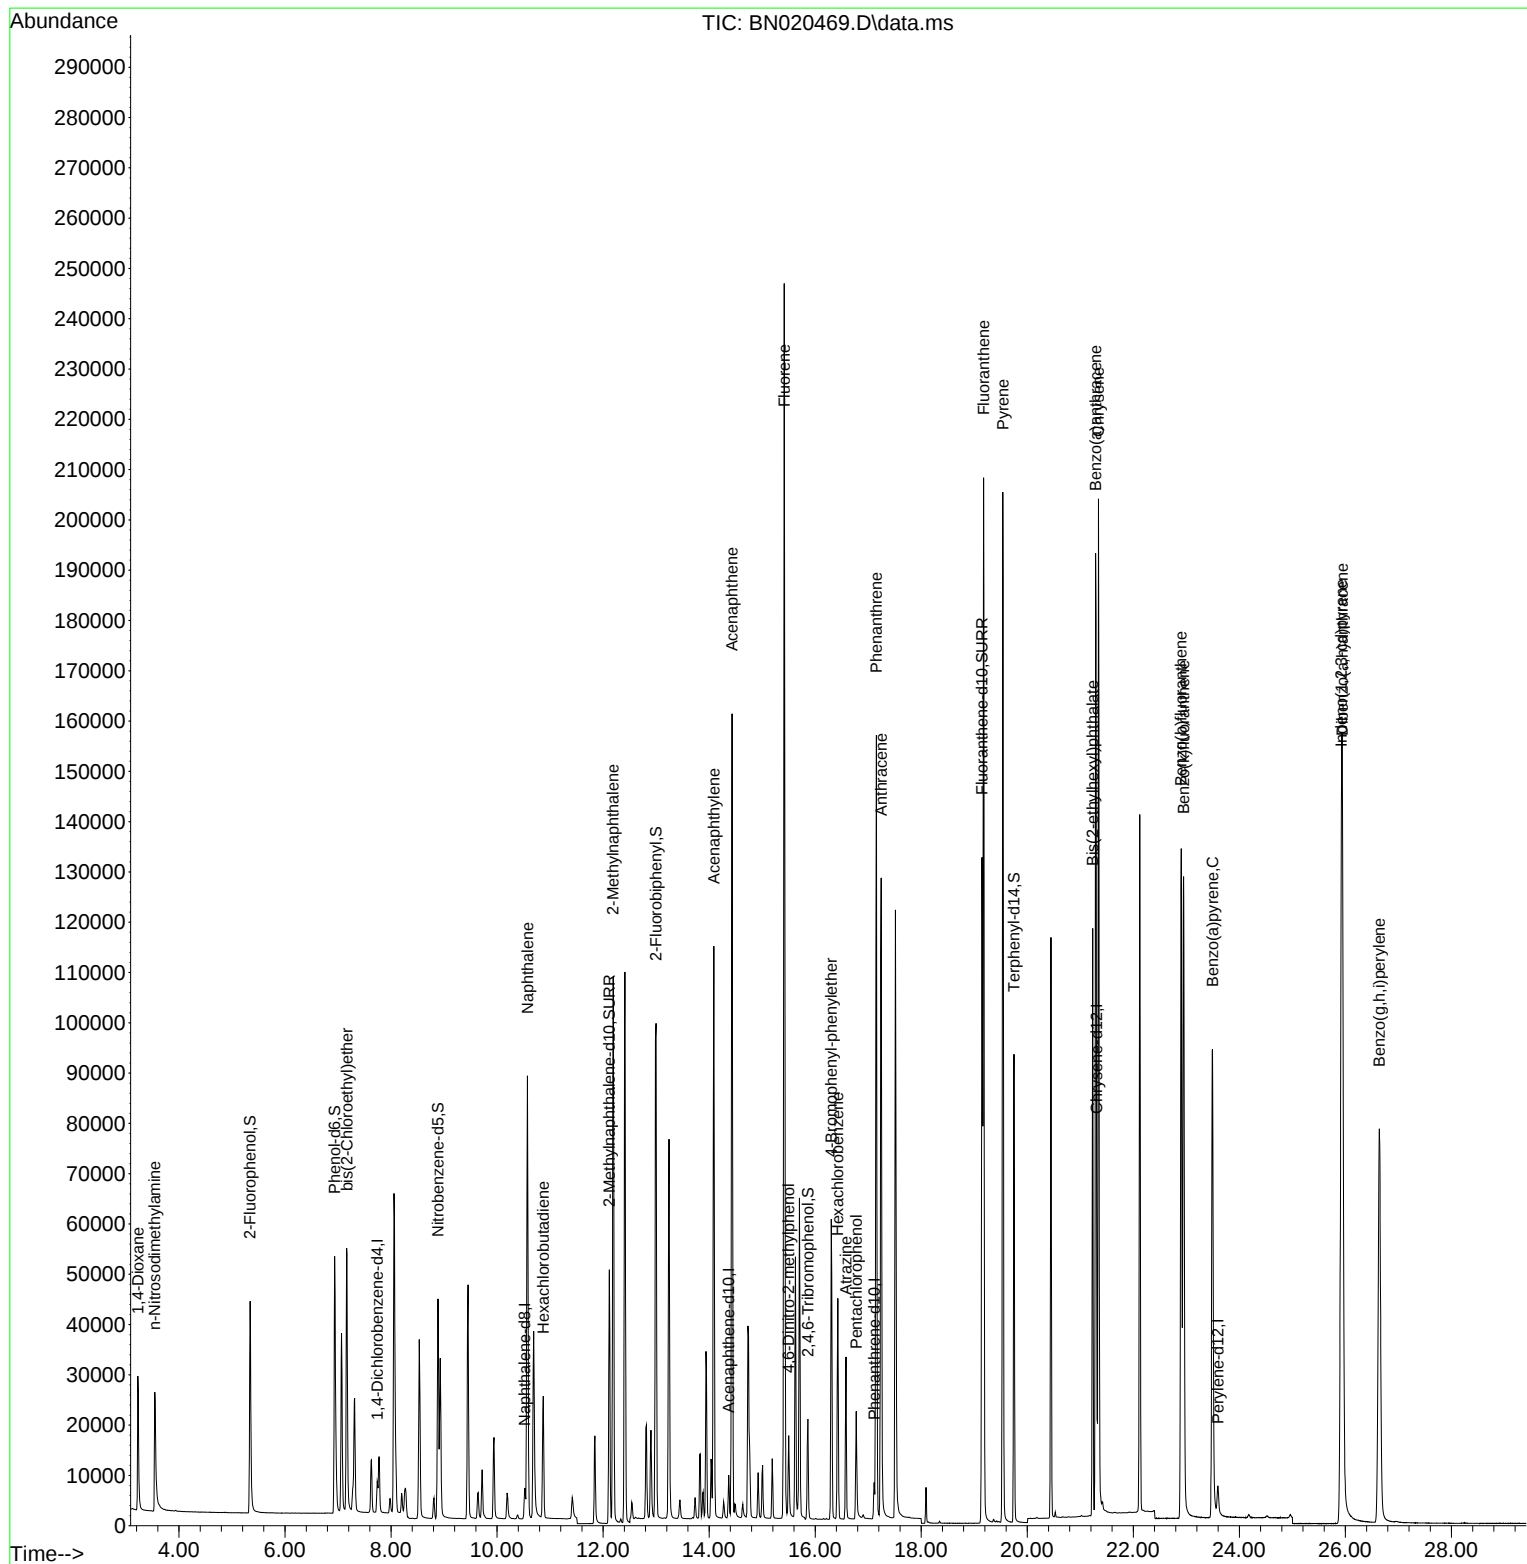





#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.739 min Scan# 64
 Delta R.T. -0.000 min
 Lab File: BN020469.D
 Acq: 26 Jun 2022 17:03

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0



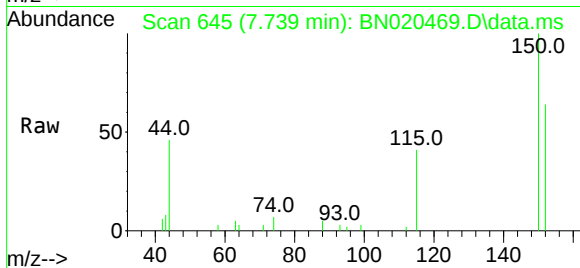


Tgt Ion:152 Resp: 2947
 Ion Ratio Lower Upper
 152 100
 150 155.1 127.9 191.9
 115 64.2 51.4 77.2

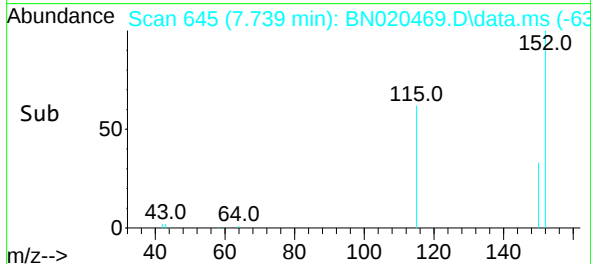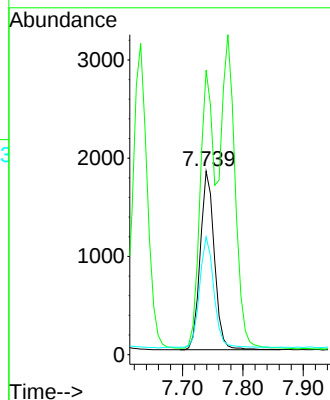

#2
 1,4-Dioxane
 Concen: 4.970 ng
 RT: 3.225 min Scan# 20
 Delta R.T. -0.007 min
 Lab File: BN020469.D
 Acq: 26 Jun 2022 17:03

Tgt Ion: 88 Resp: 16776
 Ion Ratio Lower Upper
 88 100
 43 33.5 30.2 45.2
 58 84.9 73.0 109.6


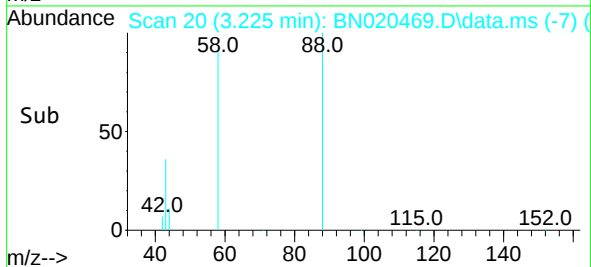
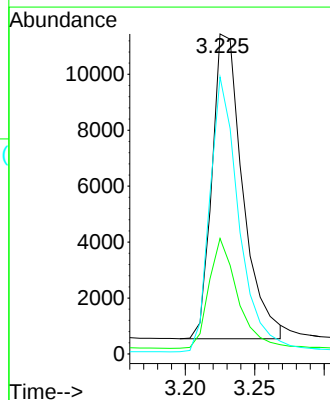
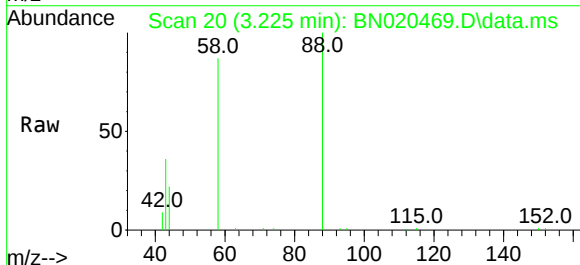




#3
 n-Nitrosodimethylamine
 Concen: 5.735 ng
 RT: 3.543 min Scan# 64
 Delta R.T. -0.014 min
 Lab File: BN020469.D
 Acq: 26 Jun 2022 17:03




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Tgt Ion: 42 Resp: 17638
 Ion Ratio Lower Upper
 42 100
 74 112.6 84.0 126.0
 44 7.5 9.8 14.8#

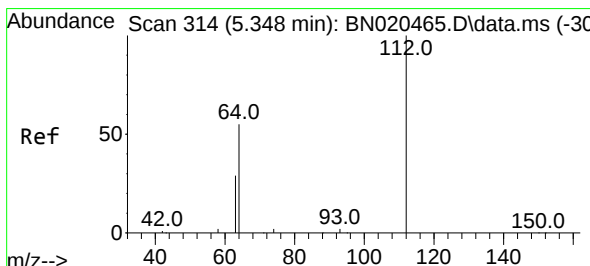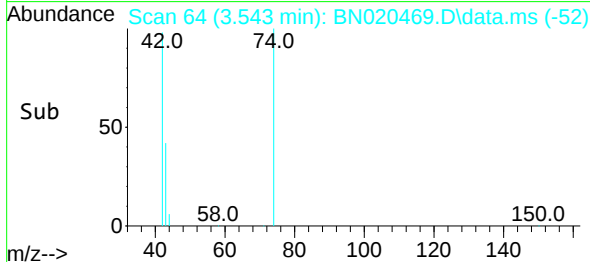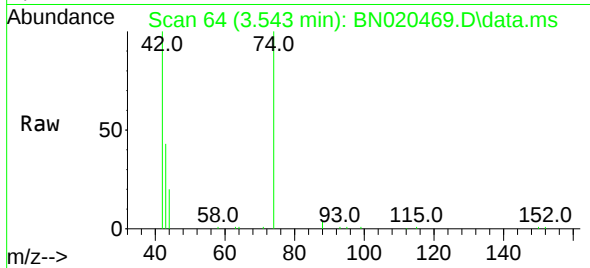

#4
 2-Fluorophenol
 Concen: 4.205 ng
 RT: 5.341 min Scan# 313
 Delta R.T. -0.007 min
 Lab File: BN020469.D
 Acq: 26 Jun 2022 17:03


Tgt Ion: 112 Resp: 36307
 Ion Ratio Lower Upper
 112 100
 64 61.7 49.1 73.7
 63 32.5 26.3 39.5

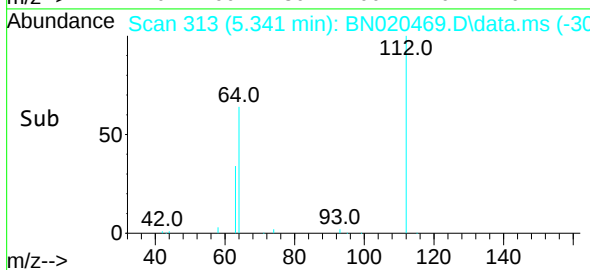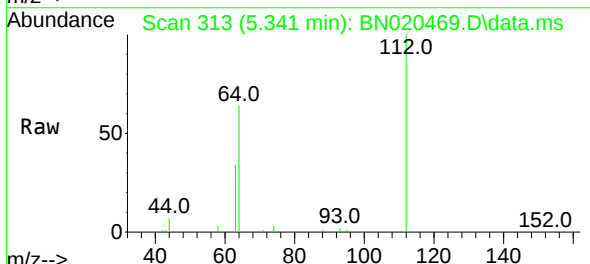






#5
Phenol-d6
Concen: 4.255 ng
RT: 6.937 min Scan# 511
Delta R.T. -0.007 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0



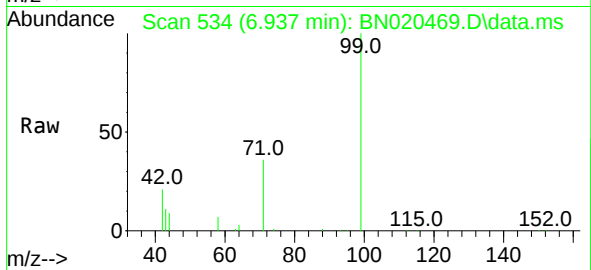


Tgt Ion: 99 Resp: 47357
Ion Ratio Lower Upper
99 100
42 21.6 19.3 28.9
71 35.3 27.5 41.3

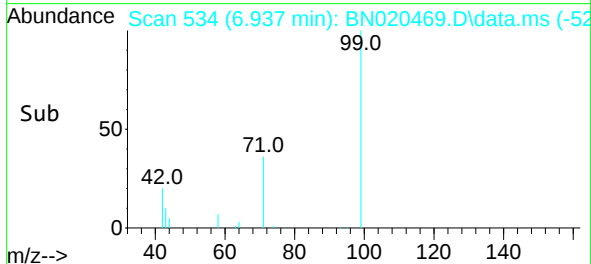

#6
bis(2-Chloroethyl)ether
Concen: 4.672 ng
RT: 7.168 min Scan# 566
Delta R.T. 0.000 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03

Tgt Ion: 93 Resp: 40373
Ion Ratio Lower Upper
93 100
63 82.3 67.4 101.0
95 32.7 26.5 39.7


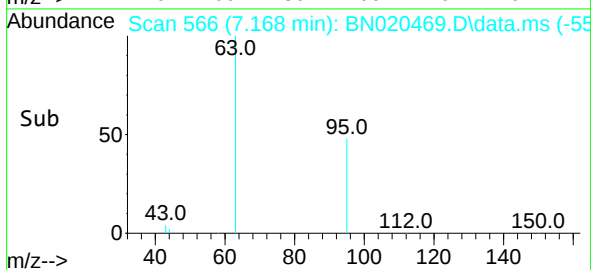

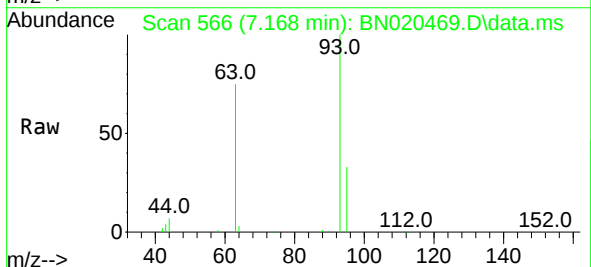




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.520 min Scan# 91
Delta R.T. 0.000 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:136 Resp: 8105
Ion Ratio Lower Upper
136 100
137 11.9 9.0 13.6
54 11.5 6.2 9.2#
68 7.5 4.4 6.6#

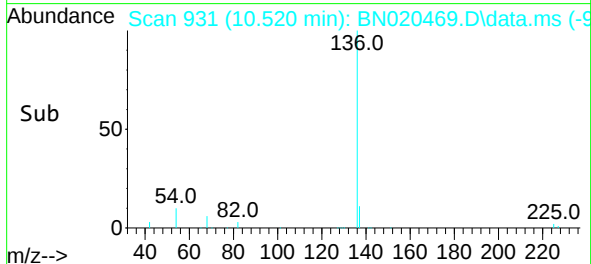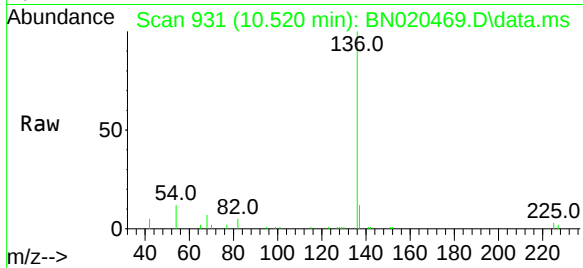

#8
Nitrobenzene-d5
Concen: 6.153 ng
RT: 8.886 min Scan# 778
Delta R.T. -0.011 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03

Tgt Ion: 82 Resp: 34817
Ion Ratio Lower Upper
82 100
128 40.7 35.0 52.6
54 57.5 46.2 69.4


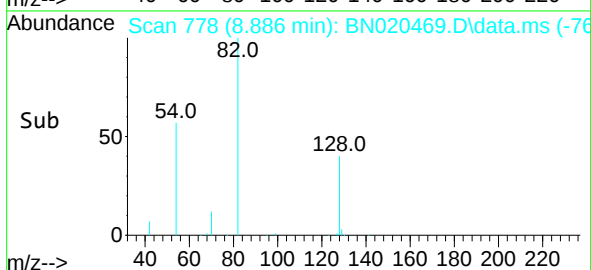

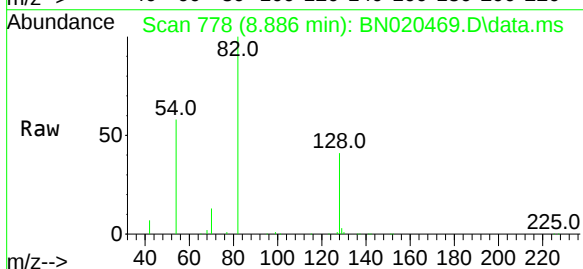




#9
Naphthalene
Concen: 4.854 ng
RT: 10.573 min Scan# 91
Delta R.T. 0.000 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:128 Resp: 117275
Ion Ratio Lower Upper
128 100
129 11.0 8.9 13.3
127 13.1 10.8 16.2

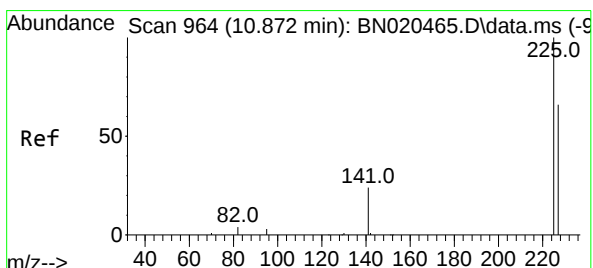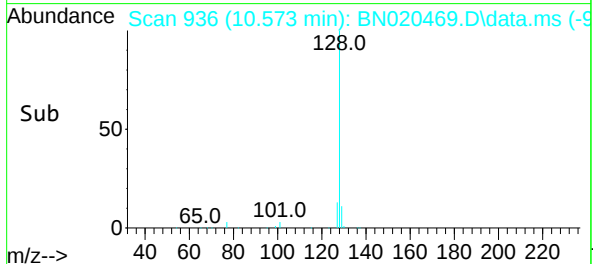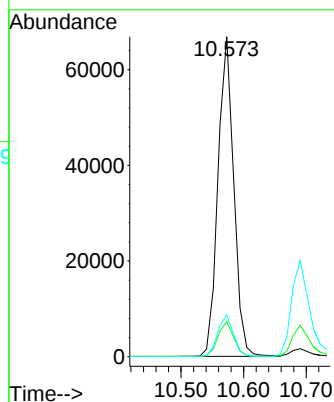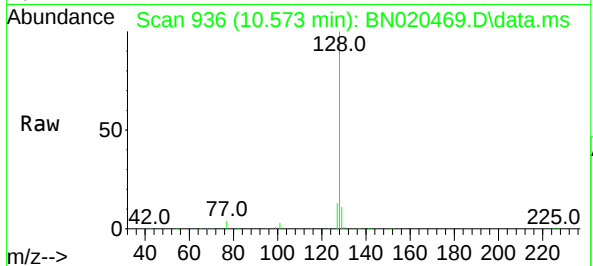

#10
Hexachlorobutadiene
Concen: 5.024 ng
RT: 10.872 min Scan# 964
Delta R.T. 0.000 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03

Tgt Ion:225 Resp: 20458
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.7 50.9 76.3


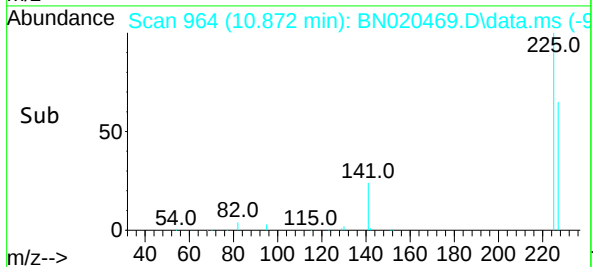
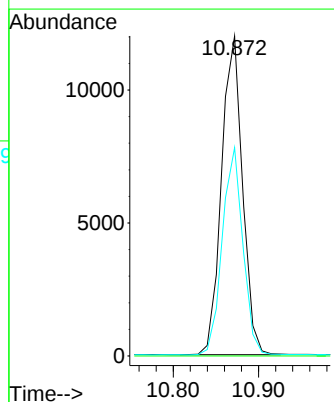
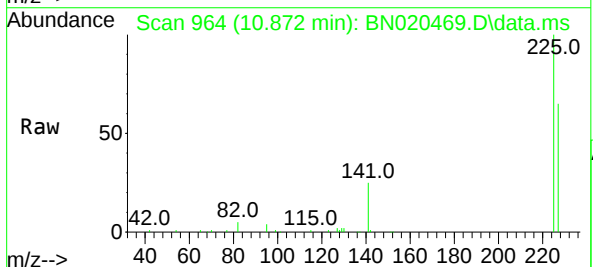




#11
2-Methylnaphthalene-d10
Concen: 4.550 ng
RT: 12.117 min Scan# 1184
Delta R.T. -0.004 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:152 Resp: 68560
Ion Ratio Lower Upper
152 100
151 20.5 16.2 24.4

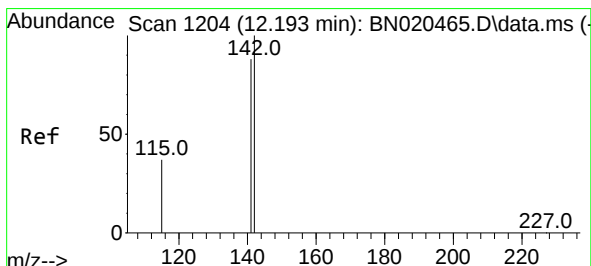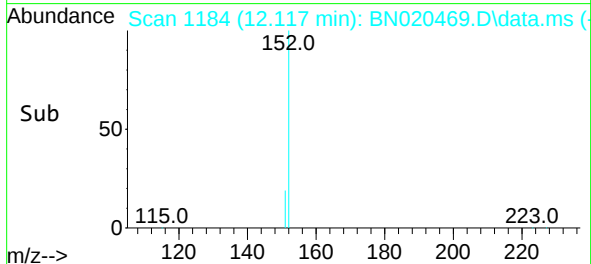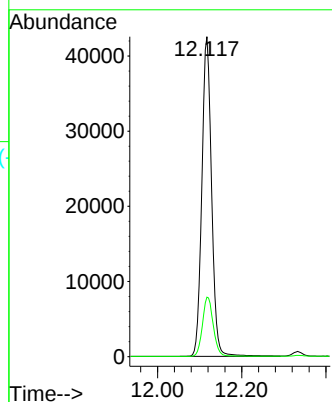

#12
2-Methylnaphthalene
Concen: 4.478 ng
RT: 12.189 min Scan# 1203
Delta R.T. -0.004 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03

Tgt Ion:142 Resp: 79348
Ion Ratio Lower Upper
142 100
141 89.6 71.6 107.4
115 37.7 29.8 44.8

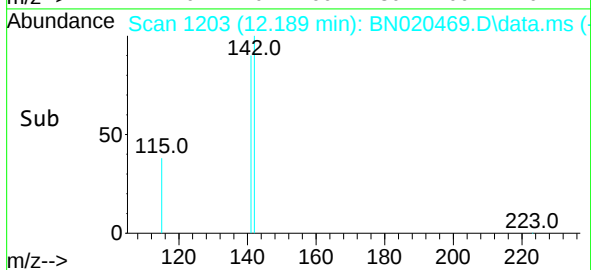

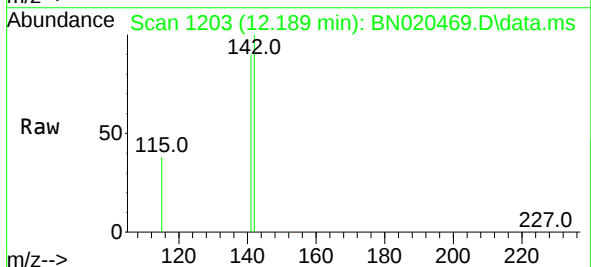




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.367 min Scan# 1461
Delta R.T. 0.000 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:164 Resp: 4826
Ion Ratio Lower Upper
164 100
162 102.3 82.1 123.1
160 48.1 38.6 58.0

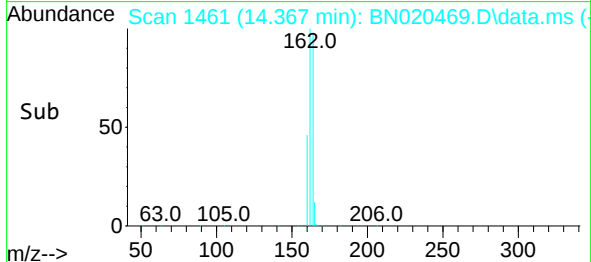

#14
2,4,6-Tribromophenol
Concen: 4.345 ng
RT: 15.861 min Scan# 1601
Delta R.T. 0.000 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03

Tgt Ion:330 Resp: 9965
Ion Ratio Lower Upper
330 100
332 100.0 77.6 116.4
141 54.5 41.0 61.4

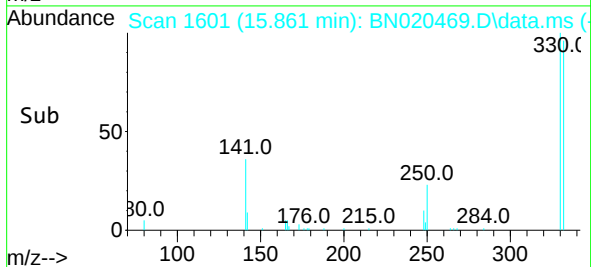

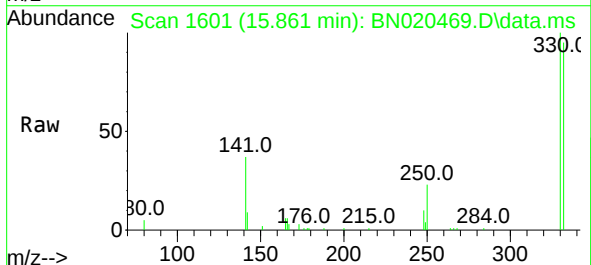




#15
2-Fluorobiphenyl
Concen: 5.473 ng
RT: 12.998 min Scan# 1333
Delta R.T. 0.000 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:172 Resp: 94513
Ion Ratio Lower Upper
172 100
171 34.4 27.2 40.8
170 22.5 18.2 27.4

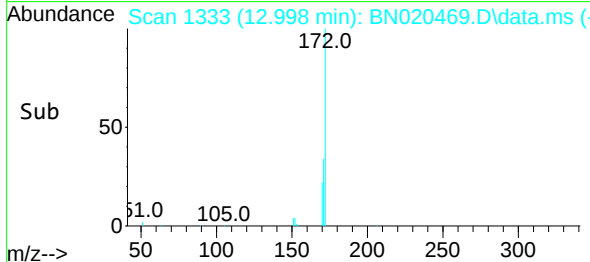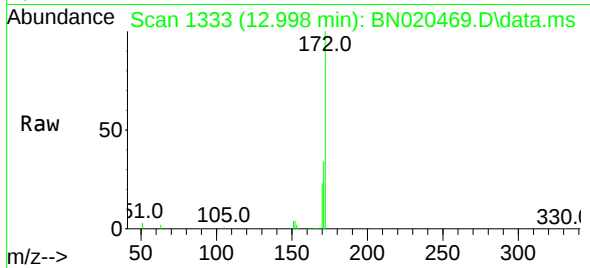

#16
Acenaphthylene
Concen: 5.496 ng
RT: 14.089 min Scan# 1435
Delta R.T. 0.000 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03

Tgt Ion:152 Resp: 124330
Ion Ratio Lower Upper
152 100
151 19.5 16.2 24.4
153 12.9 10.7 16.1

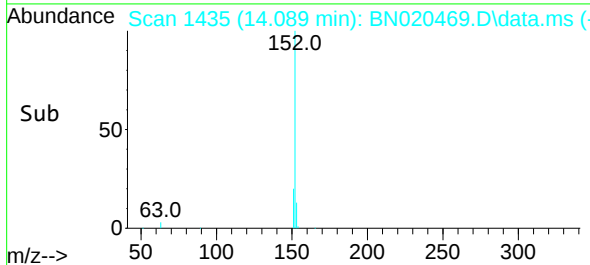

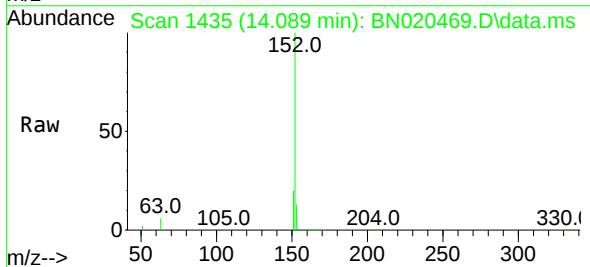




#17
Acenaphthene
Concen: 4.884 ng
RT: 14.431 min Scan# 1467
Delta R.T. 0.000 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:154 Resp: 76952
Ion Ratio Lower Upper
154 100
153 113.7 87.5 131.3
152 54.8 43.8 65.6

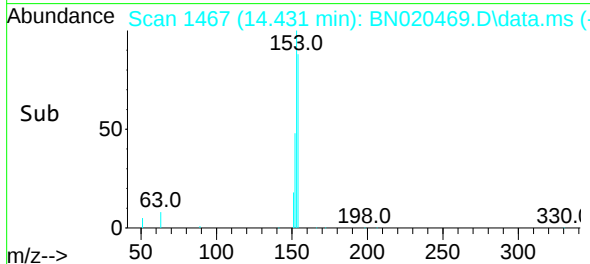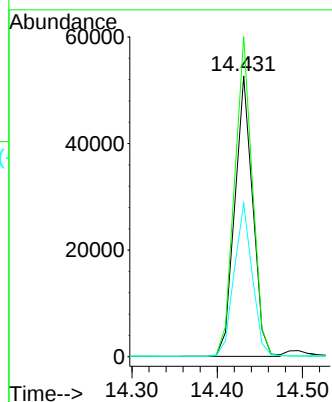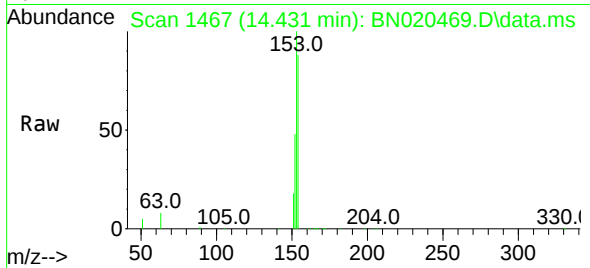

#18
Fluorene
Concen: 4.415 ng
RT: 15.415 min Scan# 1559
Delta R.T. 0.000 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03

Tgt Ion:166 Resp: 100064
Ion Ratio Lower Upper
166 100
165 98.0 78.6 118.0
167 13.4 10.8 16.2


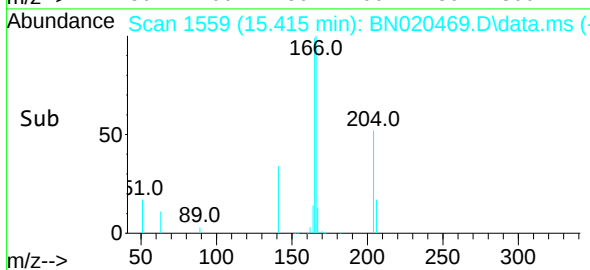
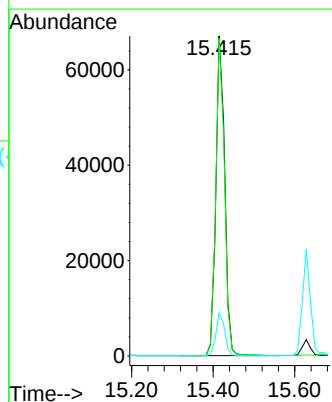
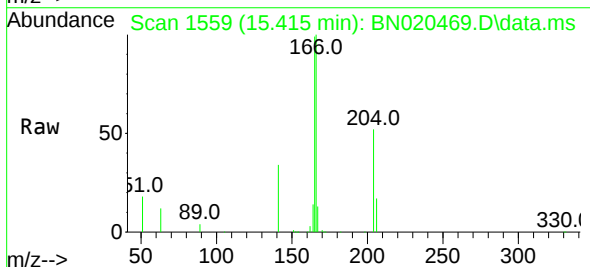




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.113 min Scan# 1723
Delta R.T. 0.000 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:188 Resp: 9789
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 11.0 7.4 11.2

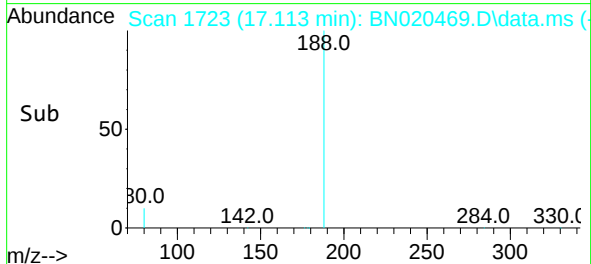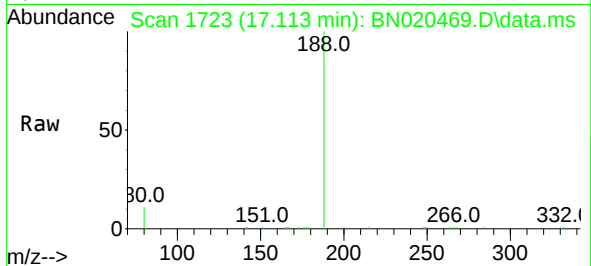

#20
4,6-Dinitro-2-methylphenol
Concen: 7.178 ng
RT: 15.500 min Scan# 1567
Delta R.T. -0.011 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03

Tgt Ion:198 Resp: 10976
Ion Ratio Lower Upper
198 100
182 9.6 12.1 18.1#
77 0.0 0.0 0.0


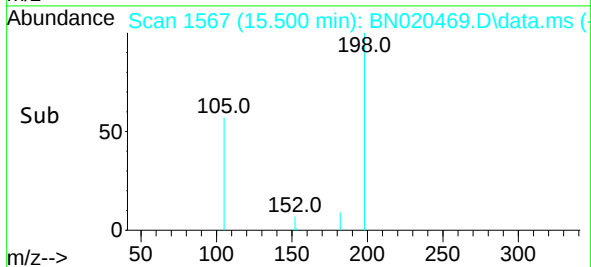

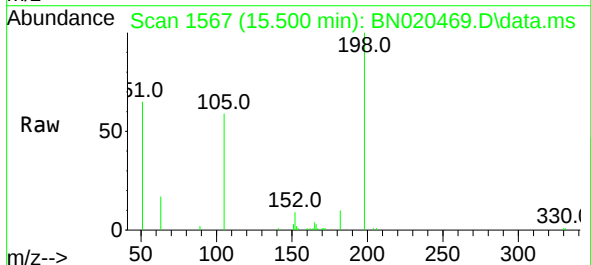


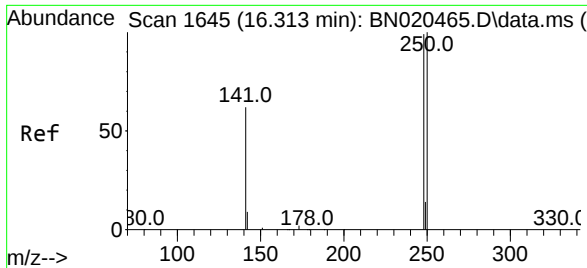

#21
4-Bromophenyl-phenylether
Concen: 5.253 ng
RT: 16.302 min Scan# 1644
Delta R.T. -0.010 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:248 Resp: 28400
Ion Ratio Lower Upper
248 100
250 92.8 75.3 112.9
141 107.5 67.3 100.9#

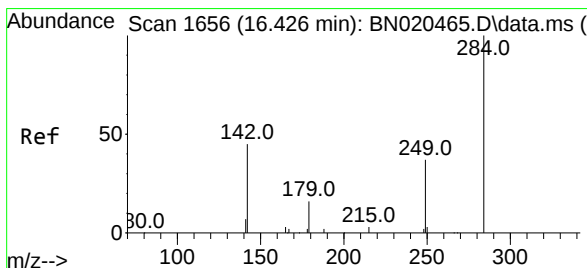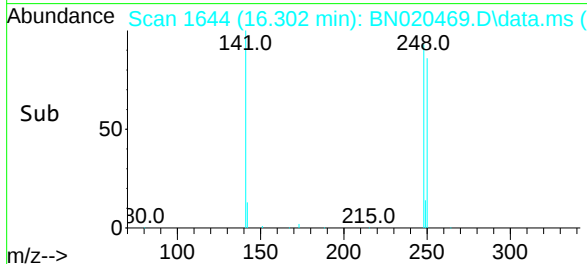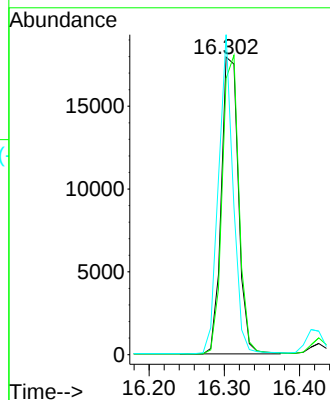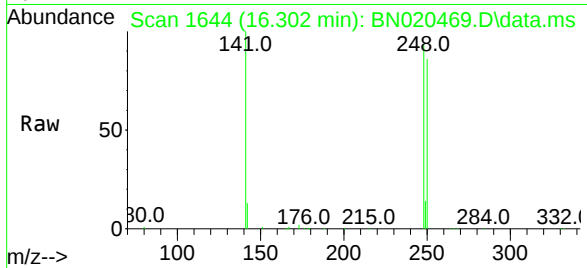

#22
Hexachlorobenzene
Concen: 5.051 ng
RT: 16.426 min Scan# 1656
Delta R.T. 0.000 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03

Tgt Ion:284 Resp: 30788
Ion Ratio Lower Upper
284 100
142 43.8 35.2 52.8
249 34.2 26.6 40.0

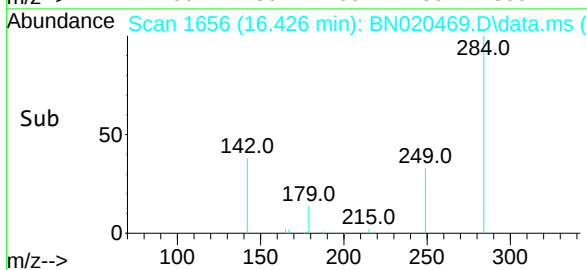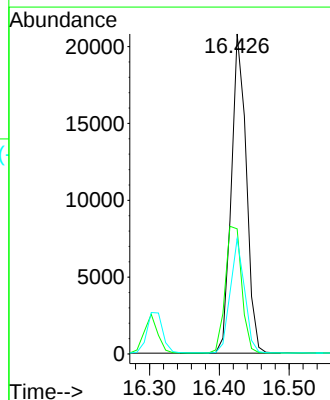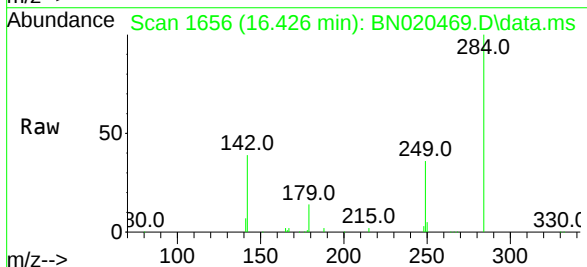



#23

Atrazine

Concen: 5.981 ng

RT: 16.579 min Scan# 1671

Delta R.T. 0.000 min

Lab File: BN020469.D

Acq: 26 Jun 2022 17:03

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:200 Resp: 24062

Ion Ratio Lower Upper

200 100

173 28.1 23.6 35.4

215 45.0 36.6 54.8

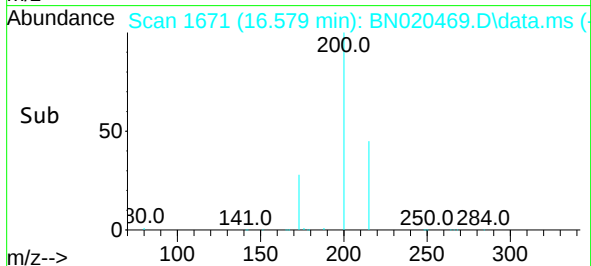

#24

Pentachlorophenol

Concen: 3.773 ng

RT: 16.774 min Scan# 1690

Delta R.T. -0.010 min

Lab File: BN020469.D

Acq: 26 Jun 2022 17:03




Tgt Ion:266 Resp: 10112


Ion Ratio Lower Upper

266 100

264 63.2 51.3 76.9

268 63.8 52.6 79.0

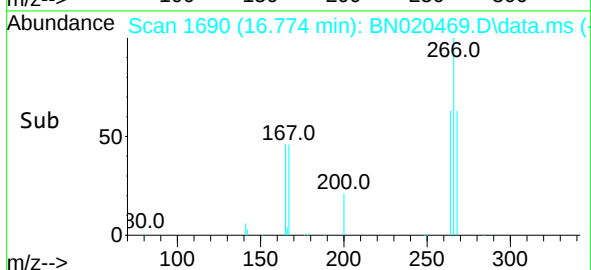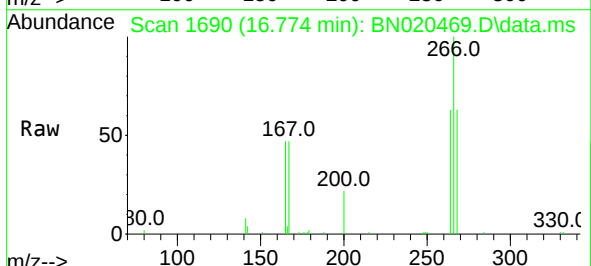

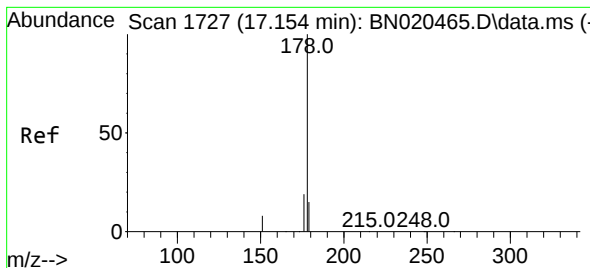

#25

Phenanthrene

Concen: 4.798 ng

RT: 17.154 min Scan# 1727

Delta R.T. 0.000 min

Lab File: BN020469.D

Acq: 26 Jun 2022 17:03

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:178 Resp: 161641

Ion Ratio Lower Upper

178 100

176 19.1 15.3 22.9

179 15.3 12.2 18.4

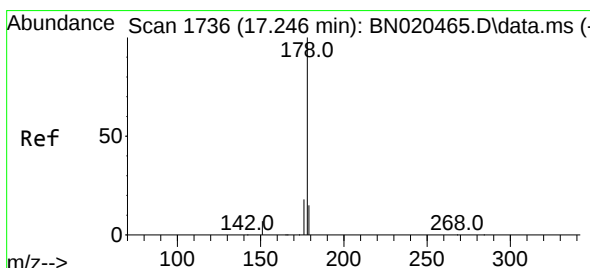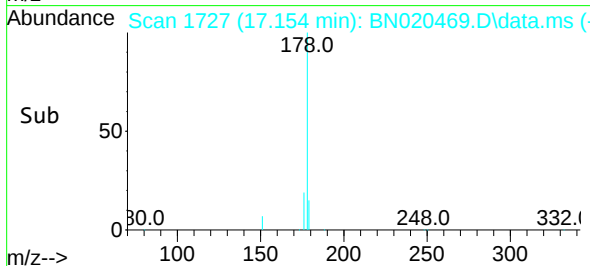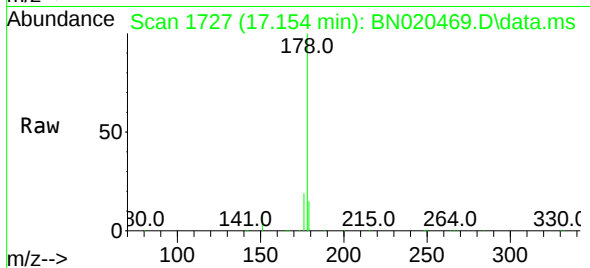

#26

Anthracene

Concen: 5.160 ng

RT: 17.246 min Scan# 1736

Delta R.T. 0.000 min

Lab File: BN020469.D

Acq: 26 Jun 2022 17:03




Tgt Ion:178 Resp: 149687

Ion Ratio Lower Upper

178 100

176 18.4 14.9 22.3

179 15.2 12.2 18.4

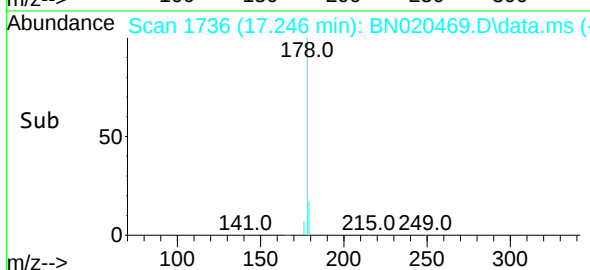

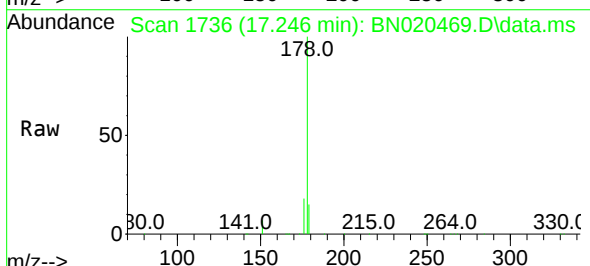




#27
Fluoranthene-d10
Concen: 4.287 ng
RT: 19.147 min Scan# 2081
Delta R.T. 0.000 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:212 Resp: 147161
Ion Ratio Lower Upper
212 100
106 15.7 12.6 19.0
104 8.8 7.2 10.8

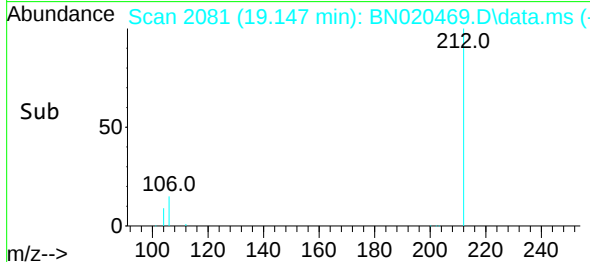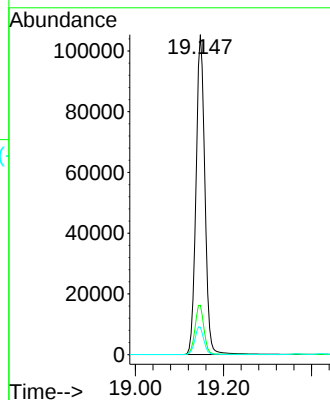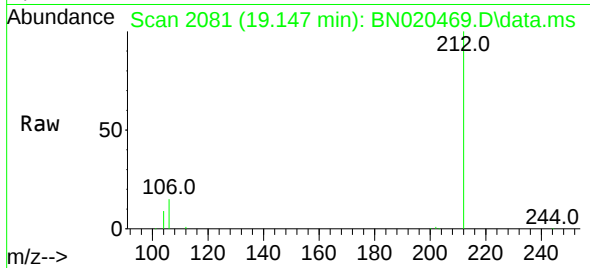

#28
Fluoranthene
Concen: 4.096 ng
RT: 19.177 min Scan# 2088
Delta R.T. -0.004 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03

Tgt Ion:202 Resp: 182322
Ion Ratio Lower Upper
202 100
101 12.5 9.6 14.4
203 17.3 13.5 20.3

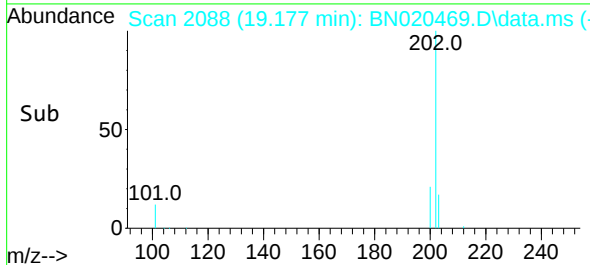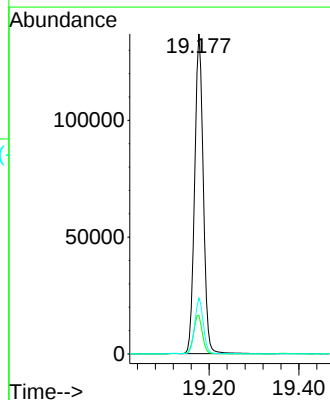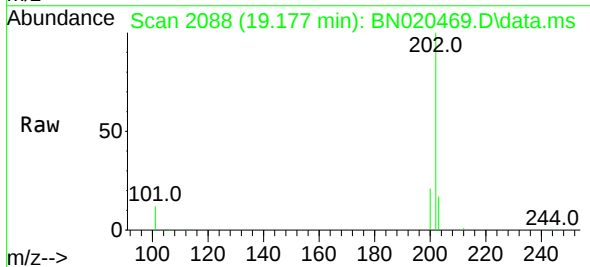



#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.306 min Scan# 2430

Delta R.T. 0.000 min

Lab File: BN020469.D

Acq: 26 Jun 2022 17:03

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:240 Resp: 9539

Ion Ratio Lower Upper

240 100

120 15.5 14.6 21.8

236 27.9 22.6 33.8

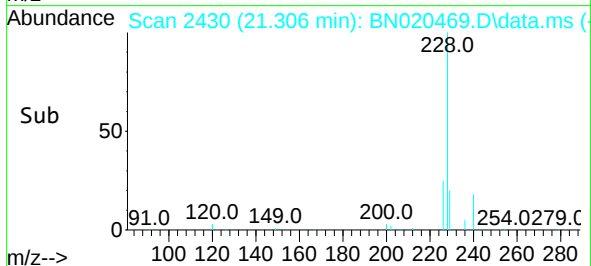

#30

Pyrene

Concen: 5.300 ng

RT: 19.539 min Scan# 2174

Delta R.T. -0.004 min

Lab File: BN020469.D

Acq: 26 Jun 2022 17:03




Tgt Ion:202 Resp: 186583

Ion Ratio Lower Upper

202 100

200 20.9 16.6 25.0

203 17.7 14.2 21.2

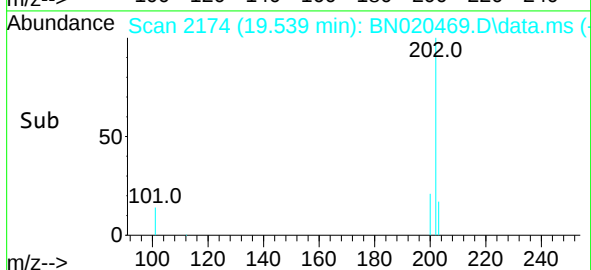

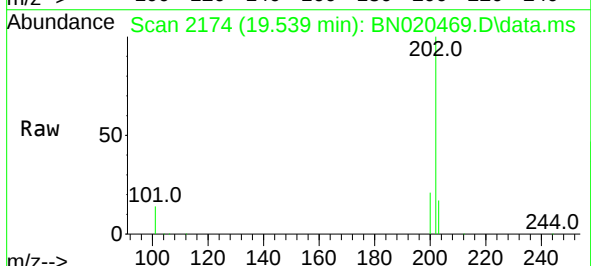




#31
 Terphenyl-d14
 Concen: 5.480 ng
 RT: 19.750 min Scan# 21
 Delta R.T. -0.004 min
 Lab File: BN020469.D
 Acq: 26 Jun 2022 17:03




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Tgt Ion:244 Resp: 104189
 Ion Ratio Lower Upper
 244 100
 212 8.6 7.1 10.7
 122 0.0 0.0 0.0

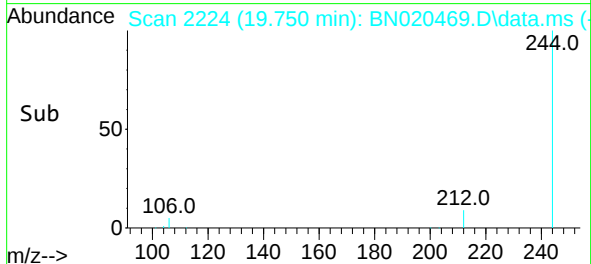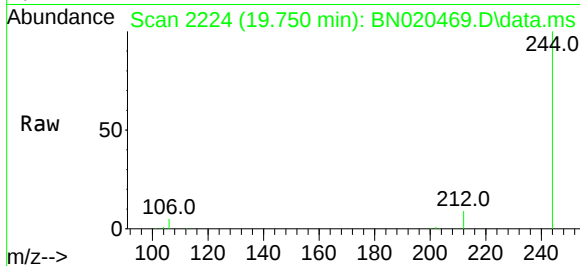

#32
 Benzo(a)anthracene
 Concen: 5.025 ng
 RT: 21.288 min Scan# 2428
 Delta R.T. -0.009 min
 Lab File: BN020469.D
 Acq: 26 Jun 2022 17:03

Tgt Ion:228 Resp: 171935
 Ion Ratio Lower Upper
 228 100
 226 27.9 21.2 31.8
 229 19.4 15.6 23.4

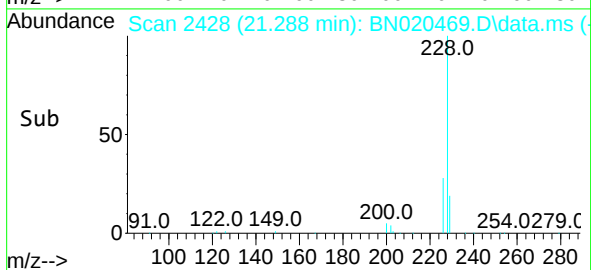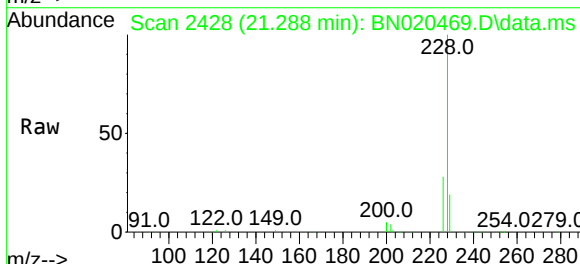



#33

Chrysene

Concen: 4.539 ng

RT: 21.342 min Scan# 2434

Delta R.T. 0.000 min

Lab File: BN020469.D

Acq: 26 Jun 2022 17:03

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:228 Resp: 176995

Ion Ratio Lower Upper

228 100

226 30.5 23.4 35.0

229 19.4 15.7 23.5

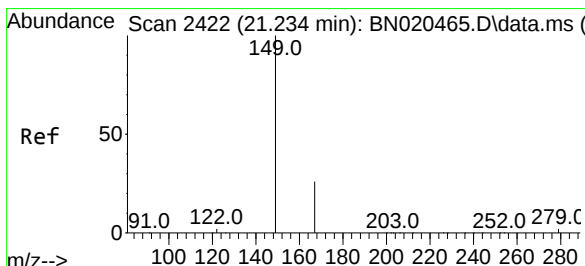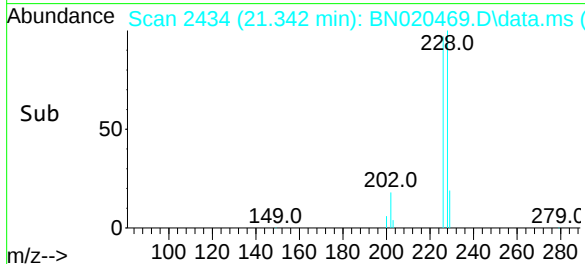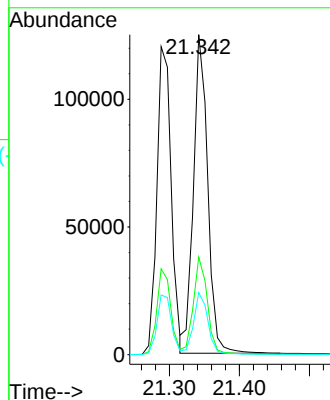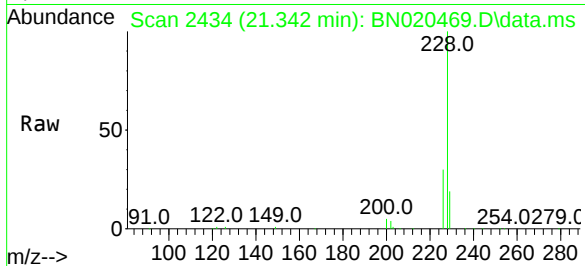

#34

Bis(2-ethylhexyl)phthalate

Concen: 6.113 ng

RT: 21.234 min Scan# 2422

Delta R.T. 0.000 min

Lab File: BN020469.D

Acq: 26 Jun 2022 17:03




Tgt Ion:149 Resp: 96067

Ion Ratio Lower Upper

149 100

167 27.0 21.7 32.5

279 2.9 2.2 3.2

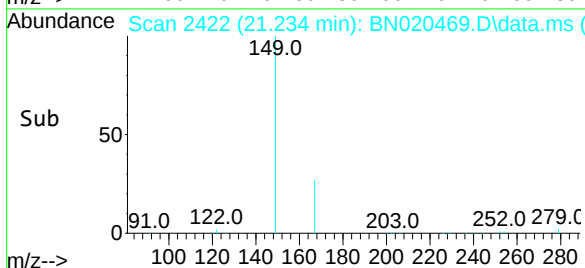
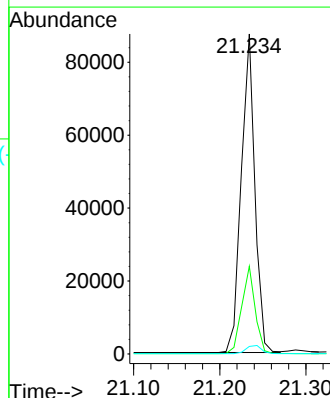
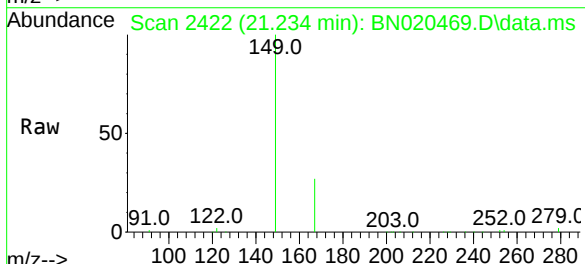




#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.595 min Scan# 2961
 Delta R.T. -0.006 min
 Lab File: BN020469.D
 Acq: 26 Jun 2022 17:03




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Tgt Ion:264 Resp: 8389
 Ion Ratio Lower Upper
 264 100
 260 25.8 20.9 31.3
 265 39.8 28.0 42.0

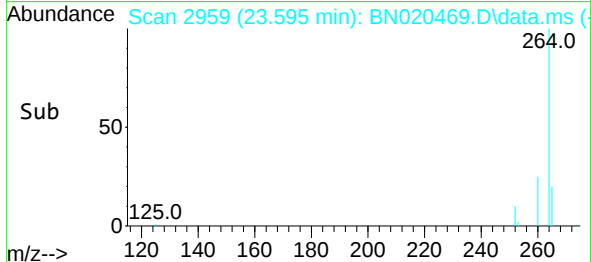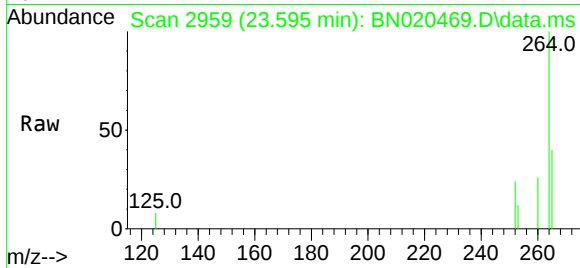

#36
 Indeno(1,2,3-cd)pyrene
 Concen: 4.804 ng
 RT: 25.925 min Scan# 3756
 Delta R.T. -0.012 min
 Lab File: BN020469.D
 Acq: 26 Jun 2022 17:03

Tgt Ion:276 Resp: 197875
 Ion Ratio Lower Upper
 276 100
 138 31.9 25.9 38.9
 277 25.0 19.8 29.8

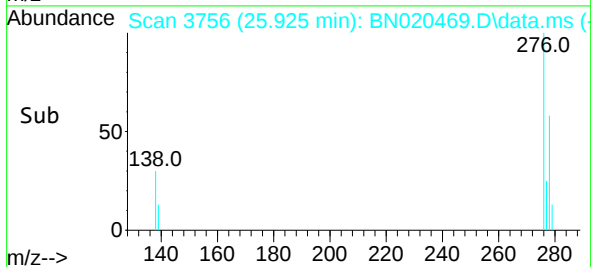

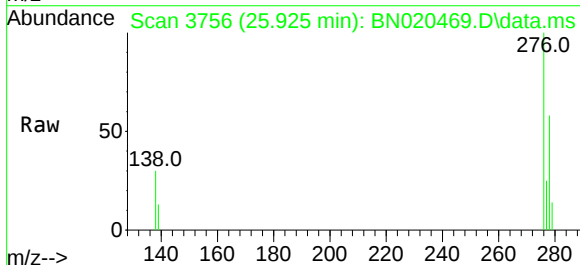




#37
Benzo(b)fluoranthene
Concen: 5.086 ng
RT: 22.902 min Scan# 21
Delta R.T. -0.006 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:252 Resp: 168495
Ion Ratio Lower Upper
252 100
253 21.6 18.5 27.7
125 12.7 11.4 17.0

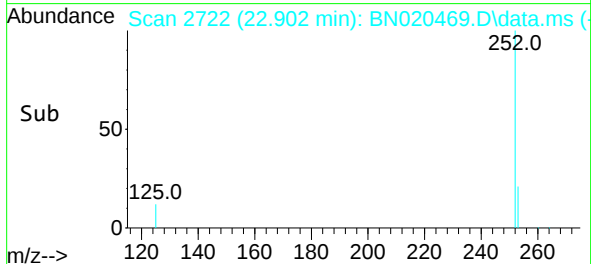

#38
Benzo(k)fluoranthene
Concen: 5.044 ng
RT: 22.948 min Scan# 2738
Delta R.T. -0.006 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03

Tgt Ion:252 Resp: 172150
Ion Ratio Lower Upper
252 100
253 22.0 18.0 27.0
125 12.5 11.0 16.4

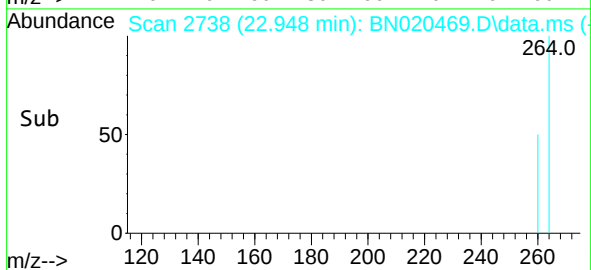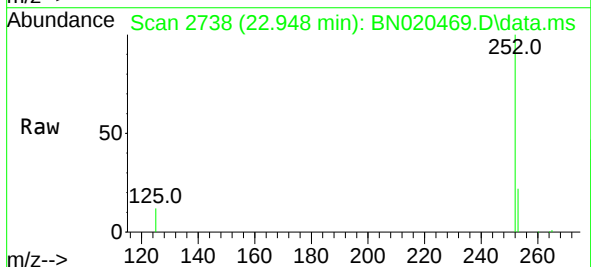



#39

Benzo(a)pyrene

Concen: 4.985 ng

RT: 23.492 min Scan# 2924

Delta R.T. -0.006 min

Lab File: BN020469.D

Acq: 26 Jun 2022 17:03

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0




Tgt Ion:252 Resp: 144089

Ion Ratio Lower Upper

252 100

253 22.1 19.0 28.4

125 14.4 13.8 20.8

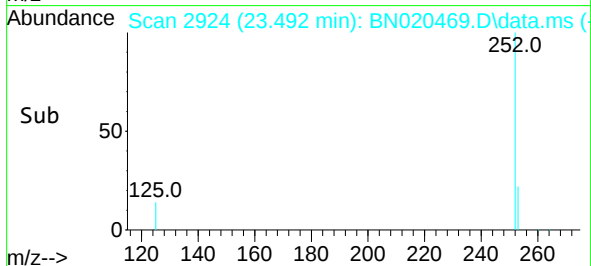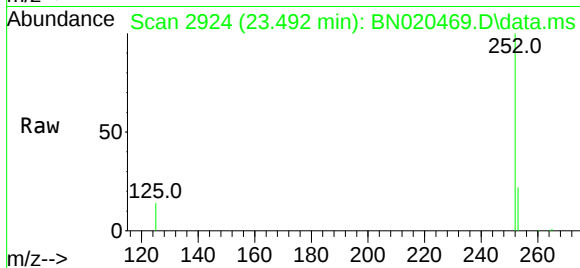

#40

Dibenzo(a,h)anthracene

Concen: 4.866 ng

RT: 25.945 min Scan# 3763

Delta R.T. -0.003 min

Lab File: BN020469.D

Acq: 26 Jun 2022 17:03




Tgt Ion:278 Resp: 159260


Ion Ratio Lower Upper

278 100

139 21.1 18.6 28.0

279 23.3 19.7 29.5

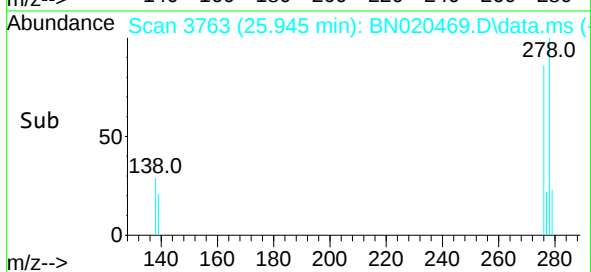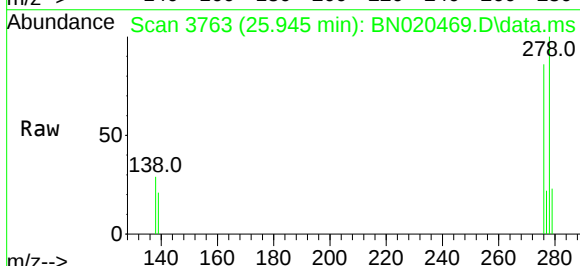

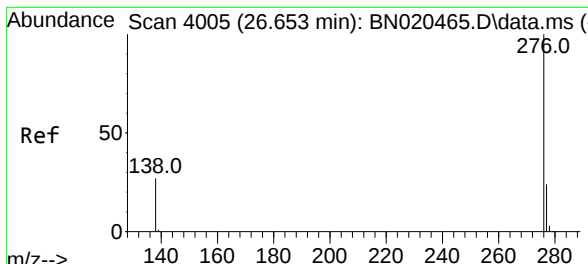

#41

Benzo(g,h,i)perylene

Concen: 4.581 ng

RT: 26.638 min Scan# 40

Delta R.T. -0.015 min

Lab File: BN020469.D


Acq: 26 Jun 2022 17:03

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0

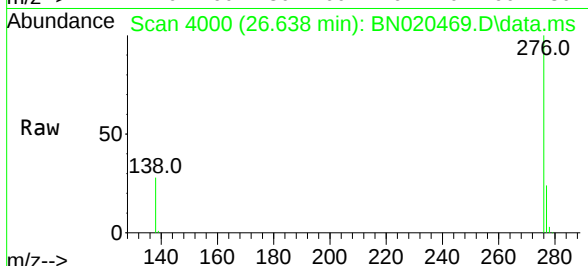

Tgt Ion:276 Resp: 167446

Ion Ratio Lower Upper

276 100

277 23.6 19.5 29.3

138 27.6 22.6 34.0

