
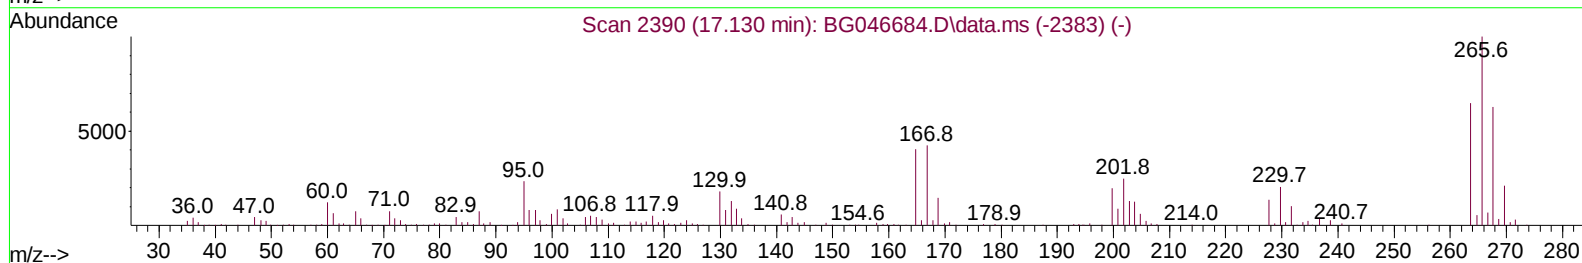
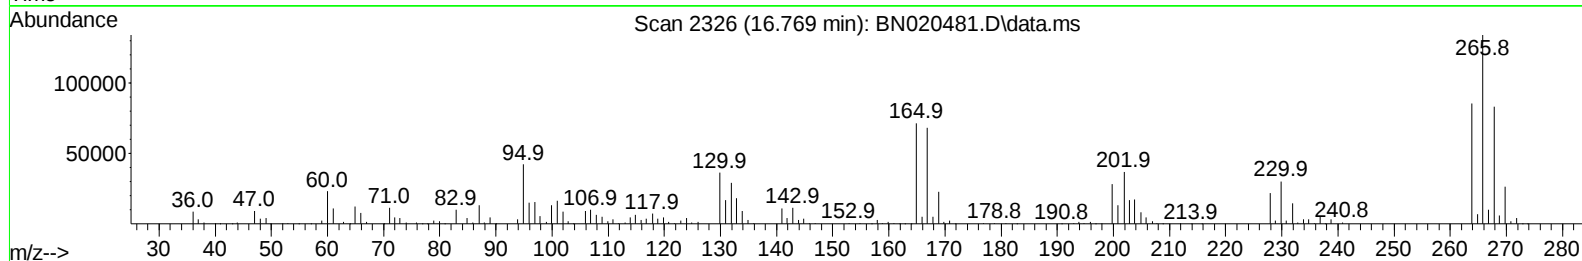


Quant Time: Jun 27 04:42:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 02:09:13 2022
Response via : Initial Calibration

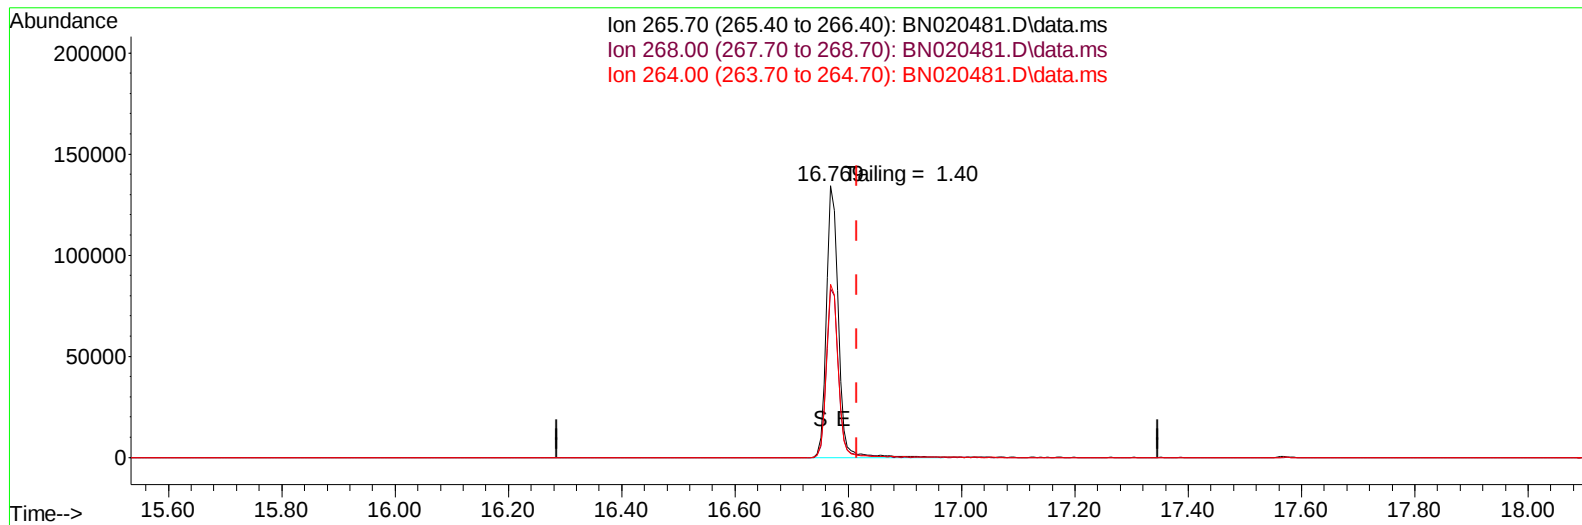

TIC: BN020481.D\data.ms

(70) Pentachlorophenol (C)




16.769min (-0.047) 16478.77 ng

response **196439**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.12
264.00	61.60	63.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062622\
 Data File : BN020481.D
 Acq On : 27 Jun 2022 03:20
 Operator : CG/JU
 Sample : DFTTP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 27 04:42:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 27 02:09:13 2022
 Response via : Initial Calibration

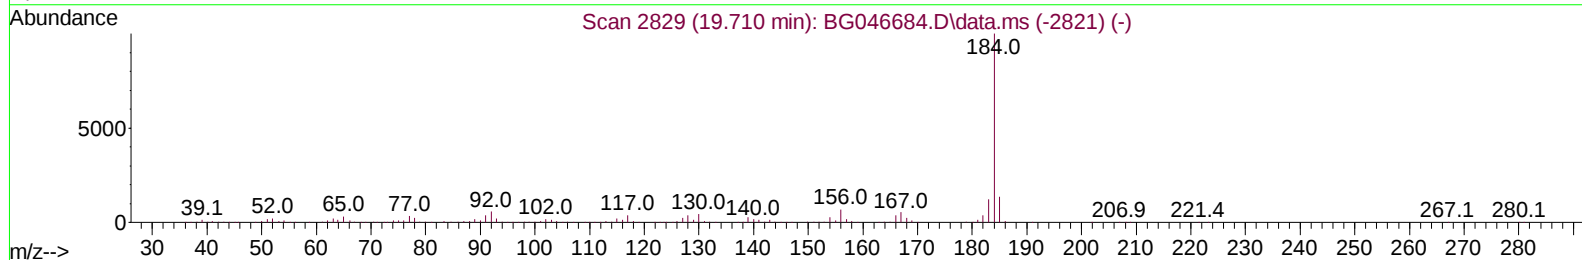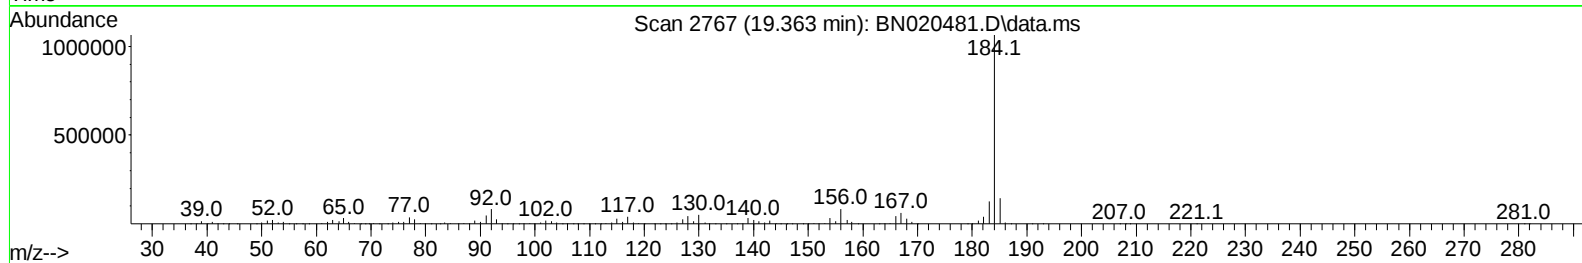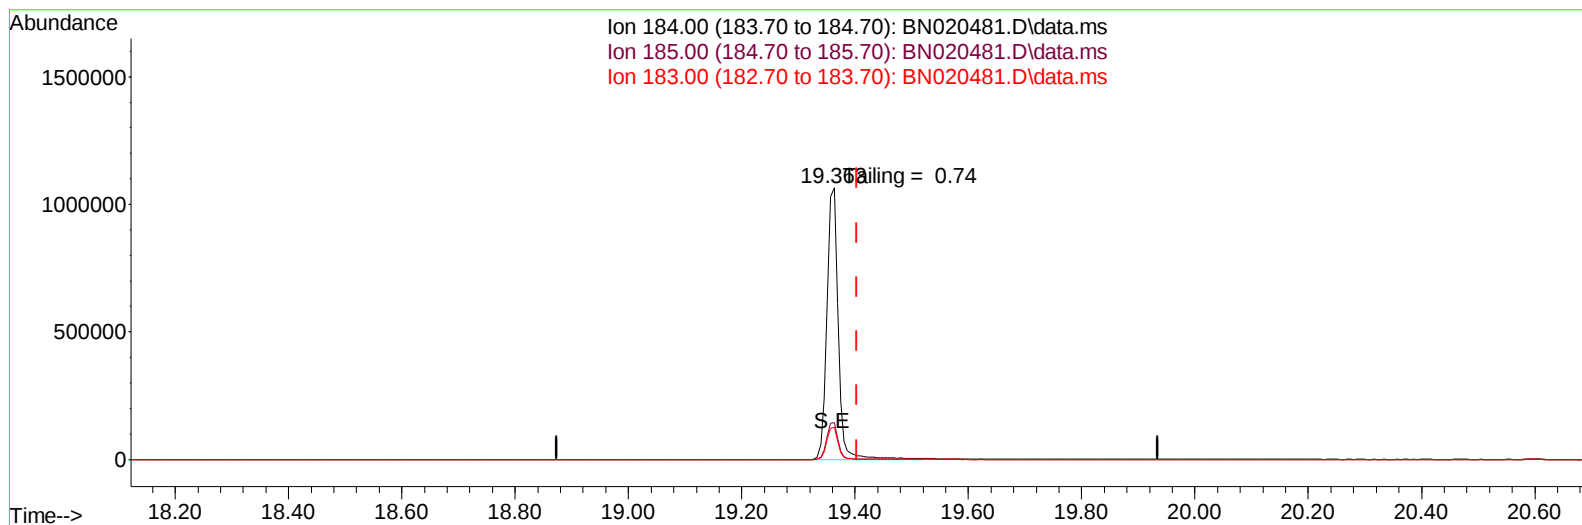

TIC: BN020481.D\data.ms

(77) Benzidine**19.363min (-0.041) 0.00 ng****response 1469558**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.59
183.00	13.20	11.96
0.00	0.00	0.00