

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062622\
 Data File : BN020465.D
 Acq On : 26 Jun 2022 14:37
 Operator : CG/JU
 Sample : SSTDICCC0.4
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICCC0.4

Quant Time: Jun 27 01:37:41 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 27 01:36:24 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.739	152	3071	0.400	ng	0.00
7) Naphthalene-d8	10.520	136	9294	0.400	ng	# 0.00
13) Acenaphthene-d10	14.367	164	5419	0.400	ng	0.00
19) Phenanthrene-d10	17.113	188	11328	0.400	ng	0.00
29) Chrysene-d12	21.306	240	9666	0.400	ng	0.00
35) Perylene-d12	23.600	264	9060	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.348	112	3322	0.369	ng	0.00
5) Phenol-d6	6.944	99	3882	0.335	ng	0.00
8) Nitrobenzene-d5	8.897	82	2746	0.423	ng	0.00
11) 2-Methylnaphthalene-d10	12.121	152	6031	0.349	ng	0.00
14) 2,4,6-Tribromophenol	15.861	330	706	0.274	ng	0.00
15) 2-Fluorobiphenyl	12.998	172	8796	0.454	ng	0.00
27) Fluoranthene-d10	19.147	212	12414	0.313	ng	0.00
31) Terphenyl-d14	19.754	244	9038	0.469	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.232	88	1539	0.438	ng	98
3) n-Nitrosodimethylamine	3.557	42	1371	0.428	ng	# 91
6) bis(2-Chloroethyl)ether	7.168	93	3328	0.370	ng	99
9) Naphthalene	10.573	128	10672	0.385	ng	98
10) Hexachlorobutadiene	10.872	225	1962	0.420	ng	# 98
12) 2-Methylnaphthalene	12.193	142	7076	0.348	ng	98
16) Acenaphthylene	14.089	152	9542	0.376	ng	99
17) Acenaphthene	14.431	154	6843	0.387	ng	96
18) Fluorene	15.415	166	8804	0.346	ng	100
20) 4,6-Dinitro-2-methylph...	15.511	198	430	0.243	ng	# 68
21) 4-Bromophenyl-phenylether	16.313	248	2444	0.391	ng	# 86
22) Hexachlorobenzene	16.426	284	2711	0.384	ng	99
23) Atrazine	16.579	200	1870	0.402	ng	97
24) Pentachlorophenol	16.784	266	510	0.164	ng	97
25) Phenanthrene	17.154	178	14278	0.366	ng	100
26) Anthracene	17.246	178	11940	0.356	ng	99
28) Fluoranthene	19.181	202	15380	0.299	ng	100
30) Pyrene	19.544	202	15959	0.447	ng	100
32) Benzo(a)anthracene	21.297	228	12979	0.374	ng	99
33) Chrysene	21.342	228	14736	0.373	ng	98
34) Bis(2-ethylhexyl)phtha...	21.234	149	6899	0.433	ng	# 98
36) Indeno(1,2,3-cd)pyrene	25.936	276	15397	0.346	ng	98
37) Benzo(b)fluoranthene	22.907	252	13296	0.372	ng	95
38) Benzo(k)fluoranthene	22.954	252	13911	0.377	ng	96
39) Benzo(a)pyrene	23.498	252	11550	0.370	ng	93
40) Dibenzo(a,h)anthracene	25.948	278	12221	0.346	ng	97
41) Benzo(g,h,i)perylene	26.653	276	13712	0.347	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062622\
Data File : BN020465.D
Acq On : 26 Jun 2022 14:37
Operator : CG/JU
Sample : SSTDICC0.4
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.4

Quant Time: Jun 27 01:37:41 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 01:36:24 2022
Response via : Initial Calibration








#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.739 min Scan# 64
 Delta R.T. -0.000 min
 Lab File: BN020465.D
 Acq: 26 Jun 2022 14:37




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICCC0.4

Tgt Ion:152 Resp: 3071
 Ion Ratio Lower Upper
 152 100
 150 156.1 127.9 191.9
 115 65.8 51.4 77.2



#2
 1,4-Dioxane
 Concen: 0.438 ng
 RT: 3.232 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BN020465.D
 Acq: 26 Jun 2022 14:37

Tgt Ion: 88 Resp: 1539
 Ion Ratio Lower Upper
 88 100
 43 34.9 30.2 45.2
 58 92.1 73.0 109.6








#3
n-Nitrosodimethylamine
Concen: 0.428 ng
RT: 3.557 min Scan# 66
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion: 42 Resp: 1371
Ion Ratio Lower Upper
42 100
74 113.4 84.0 126.0
44 4.5 9.8 14.8#



#4
2-Fluorophenol
Concen: 0.369 ng
RT: 5.348 min Scan# 314
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37

Tgt Ion: 112 Resp: 3322
Ion Ratio Lower Upper
112 100
64 61.1 49.1 73.7
63 32.7 26.3 39.5








#5
Phenol-d6
Concen: 0.335 ng
RT: 6.944 min Scan# 51
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion: 99 Resp: 3882
Ion Ratio Lower Upper
99 100
42 22.4 19.3 28.9
71 35.6 27.5 41.3



#6
bis(2-Chloroethyl)ether
Concen: 0.370 ng
RT: 7.168 min Scan# 566
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37

Tgt Ion: 93 Resp: 3328
Ion Ratio Lower Upper
93 100
63 84.0 67.4 101.0
95 33.7 26.5 39.7








#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.520 min Scan# 931
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:	136	Resp:	9294
Ion	Ratio	Lower	Upper
136	100		
137	11.7	9.0	13.6
54	10.8	6.2	9.2#
68	7.3	4.4	6.6#



#8
Nitrobenzene-d5
Concen: 0.423 ng
RT: 8.897 min Scan# 779
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37

Tgt Ion:	82	Resp:	2746
Ion	Ratio	Lower	Upper
82	100		
128	45.7	35.0	52.6
54	57.9	46.2	69.4









#9
Naphthalene
Concen: 0.385 ng
RT: 10.573 min Scan# 91
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:128 Resp: 10672
Ion Ratio Lower Upper
128 100
129 11.8 8.9 13.3
127 14.3 10.8 16.2



#10
Hexachlorobutadiene
Concen: 0.420 ng
RT: 10.872 min Scan# 964
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37

Tgt Ion:225 Resp: 1962
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 62.1 50.9 76.3








#11
2-Methylnaphthalene-d10
Concen: 0.349 ng
RT: 12.121 min Scan# 1185
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:152 Resp: 6031
Ion Ratio Lower Upper
152 100
151 20.4 16.2 24.4



#12
2-Methylnaphthalene
Concen: 0.348 ng
RT: 12.193 min Scan# 1204
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37

Tgt Ion:142 Resp: 7076
Ion Ratio Lower Upper
142 100
141 87.9 71.6 107.4
115 37.9 29.8 44.8





#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.367 min Scan# 1461

Delta R.T. 0.000 min

Lab File: BN020465.D

Acq: 26 Jun 2022 14:37

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:164 Resp: 5419

Ion Ratio Lower Upper

164 100

162 105.3 82.1 123.1

160 49.3 38.6 58.0



#14

2,4,6-Tribromophenol

Concen: 0.274 ng

RT: 15.861 min Scan# 1601

Delta R.T. 0.000 min

Lab File: BN020465.D

Acq: 26 Jun 2022 14:37




Tgt Ion:330 Resp: 706


Ion Ratio Lower Upper

330 100

332 161.9 77.6 116.4#

141 55.8 41.0 61.4








#15
2-Fluorobiphenyl
Concen: 0.454 ng
RT: 12.998 min Scan# 1333
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:	172	Resp:	8796
Ion Ratio	Lower	Upper	
172	100		
171	34.9	27.2	40.8
170	23.1	18.2	27.4



#16
Acenaphthylene
Concen: 0.376 ng
RT: 14.089 min Scan# 1435
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37

Tgt Ion:	152	Resp:	9542
Ion Ratio	Lower	Upper	
152	100		
151	19.6	16.2	24.4
153	12.9	10.7	16.1








#17
Acenaphthene
Concen: 0.387 ng
RT: 14.431 min Scan# 1467
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:154 Resp: 6843
Ion Ratio Lower Upper
154 100
153 114.5 87.5 131.3
152 56.9 43.8 65.6



#18
Fluorene
Concen: 0.346 ng
RT: 15.415 min Scan# 1559
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37

Tgt Ion:166 Resp: 8804
Ion Ratio Lower Upper
166 100
165 98.6 78.6 118.0
167 13.4 10.8 16.2





#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.113 min Scan# 11

Delta R.T. 0.000 min

Lab File: BN020465.D

Acq: 26 Jun 2022 14:37

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:188 Resp: 11328

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 10.7 7.4 11.2



#20

4,6-Dinitro-2-methylphenol

Concen: 0.243 ng

RT: 15.511 min Scan# 1568

Delta R.T. 0.000 min

Lab File: BN020465.D

Acq: 26 Jun 2022 14:37




Tgt Ion:198 Resp: 430


Ion Ratio Lower Upper

198 100

182 28.3 12.1 18.1#

77 0.0 0.0 0.0









#21
4-Bromophenyl-phenylether
Concen: 0.391 ng
RT: 16.313 min Scan# 1645
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:248 Resp: 2444
Ion Ratio Lower Upper
248 100
250 100.9 75.3 112.9
141 64.6 67.3 100.9#



#22
Hexachlorobenzene
Concen: 0.384 ng
RT: 16.426 min Scan# 1656
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37

Tgt Ion:284 Resp: 2711
Ion Ratio Lower Upper
284 100
142 44.6 35.2 52.8
249 34.1 26.6 40.0









#23
 Atrazine
 Concen: 0.402 ng
 RT: 16.579 min Scan# 1671
 Delta R.T. 0.000 min
 Lab File: BN020465.D
 Acq: 26 Jun 2022 14:37




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICCC0.4

Tgt Ion:200 Resp: 1870
 Ion Ratio Lower Upper
 200 100
 173 33.1 23.6 35.4
 215 45.9 36.6 54.8

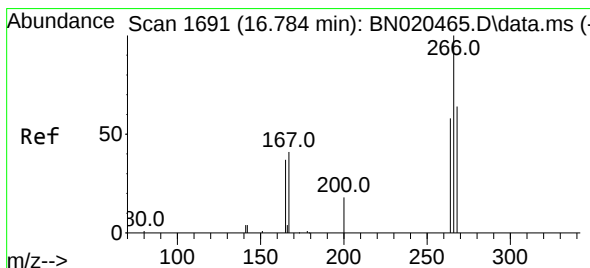

#24
 Pentachlorophenol
 Concen: 0.164 ng
 RT: 16.784 min Scan# 1691
 Delta R.T. 0.000 min
 Lab File: BN020465.D
 Acq: 26 Jun 2022 14:37

Tgt Ion:266 Resp: 510
 Ion Ratio Lower Upper
 266 100
 264 61.4 51.3 76.9
 268 67.1 52.6 79.0









#25
Phenanthrene
Concen: 0.366 ng
RT: 17.154 min Scan# 1727
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:178 Resp: 14278
Ion Ratio Lower Upper
178 100
176 19.1 15.3 22.9
179 15.5 12.2 18.4

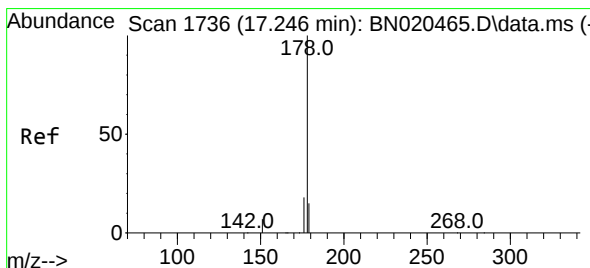

#26
Anthracene
Concen: 0.356 ng
RT: 17.246 min Scan# 1736
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37

Tgt Ion:178 Resp: 11940
Ion Ratio Lower Upper
178 100
176 18.2 14.9 22.3
179 15.0 12.2 18.4








#27
Fluoranthene-d10
Concen: 0.313 ng
RT: 19.147 min Scan# 2081
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:212 Resp: 12414
Ion Ratio Lower Upper
212 100
106 15.5 12.6 19.0
104 8.4 7.2 10.8



#28
Fluoranthene
Concen: 0.299 ng
RT: 19.181 min Scan# 2089
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37

Tgt Ion:202 Resp: 15380
Ion Ratio Lower Upper
202 100
101 11.7 9.6 14.4
203 16.8 13.5 20.3









#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.306 min Scan# 2430
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:240 Resp: 9666
Ion Ratio Lower Upper
240 100
120 18.4 14.6 21.8
236 27.8 22.6 33.8



#30
Pyrene
Concen: 0.447 ng
RT: 19.544 min Scan# 2175
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37

Tgt Ion:202 Resp: 15959
Ion Ratio Lower Upper
202 100
200 21.0 16.6 25.0
203 17.5 14.2 21.2








#31
 Terphenyl-d14
 Concen: 0.469 ng
 RT: 19.754 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BN020465.D
 Acq: 26 Jun 2022 14:37




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.4


Tgt Ion:244 Resp: 9038
 Ion Ratio Lower Upper
 244 100
 212 9.3 7.1 10.7
 122 0.0 0.0 0.0



#32
 Benzo(a)anthracene
 Concen: 0.374 ng
 RT: 21.297 min Scan# 2429
 Delta R.T. 0.000 min
 Lab File: BN020465.D
 Acq: 26 Jun 2022 14:37

Tgt Ion:228 Resp: 12979
 Ion Ratio Lower Upper
 228 100
 226 27.0 21.2 31.8
 229 20.1 15.6 23.4





#33

Chrysene

Concen: 0.373 ng

RT: 21.342 min Scan# 2434

Delta R.T. 0.000 min

Lab File: BN020465.D

Acq: 26 Jun 2022 14:37

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:228 Resp: 14736

Ion Ratio Lower Upper

228 100

226 31.0 23.4 35.0

229 19.6 15.7 23.5



#34

Bis(2-ethylhexyl)phthalate

Concen: 0.433 ng

RT: 21.234 min Scan# 2422

Delta R.T. 0.000 min

Lab File: BN020465.D

Acq: 26 Jun 2022 14:37




Tgt Ion:149 Resp: 6899

Ion Ratio Lower Upper

149 100

167 26.0 21.7 32.5

279 3.5 2.2 3.2#








#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.600 min Scan# 2961
 Delta R.T. 0.000 min
 Lab File: BN020465.D
 Acq: 26 Jun 2022 14:37




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICCC0.4

Tgt Ion:264 Resp: 9060
 Ion Ratio Lower Upper
 264 100
 260 26.2 20.9 31.3
 265 41.1 28.0 42.0



#36
 Indeno(1,2,3-cd)pyrene
 Concen: 0.346 ng
 RT: 25.936 min Scan# 3760
 Delta R.T. 0.000 min
 Lab File: BN020465.D
 Acq: 26 Jun 2022 14:37

Tgt Ion:276 Resp: 15397
 Ion Ratio Lower Upper
 276 100
 138 30.9 25.9 38.9
 277 25.3 19.8 29.8








#37
Benzo(b)fluoranthene
Concen: 0.372 ng
RT: 22.907 min Scan# 2724
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:252 Resp: 13296
Ion Ratio Lower Upper
252 100
253 25.6 18.5 27.7
125 16.2 11.4 17.0



#38
Benzo(k)fluoranthene
Concen: 0.377 ng
RT: 22.954 min Scan# 2740
Delta R.T. 0.000 min
Lab File: BN020465.D
Acq: 26 Jun 2022 14:37

Tgt Ion:252 Resp: 13911
Ion Ratio Lower Upper
252 100
253 25.1 18.0 27.0
125 14.8 11.0 16.4





#39

Benzo(a)pyrene

Concen: 0.370 ng

RT: 23.498 min Scan# 2926

Delta R.T. 0.000 min

Lab File: BN020465.D

Acq: 26 Jun 2022 14:37

Instrument :

BN020465.D

ClientSampleId :

SSTDICCC0.4




Tgt Ion:252 Resp: 11550

Ion Ratio Lower Upper

252 100

253 26.9 19.0 28.4

125 20.7 13.8 20.8



#40

Dibenzo(a,h)anthracene

Concen: 0.346 ng

RT: 25.948 min Scan# 3764

Delta R.T. 0.000 min

Lab File: BN020465.D

Acq: 26 Jun 2022 14:37




Tgt Ion:278 Resp: 12221


Ion Ratio Lower Upper

278 100

139 22.7 18.6 28.0

279 26.6 19.7 29.5





#41
 Benzo(g,h,i)perylene
 Concen: 0.347 ng
 RT: 26.653 min Scan# 40
 Delta R.T. 0.000 min
 Lab File: BN020465.D
 Acq: 26 Jun 2022 14:37

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.4

Tgt Ion:	276	Resp:	13712
Ion	Ratio	Lower	Upper
276	100		
277	25.3	19.5	29.3
138	28.2	22.6	34.0

