

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062622\
 Data File : BN020469.D
 Acq On : 26 Jun 2022 17:03
 Operator : CG/JU
 Sample : SSTDICC5.0
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Quant Time: Jun 27 01:38:20 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 27 01:36:24 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.739	152	2947	0.400	ng	0.00
7) Naphthalene-d8	10.520	136	8105	0.400	ng	# 0.00
13) Acenaphthene-d10	14.367	164	4826	0.400	ng	0.00
19) Phenanthrene-d10	17.113	188	9789	0.400	ng	0.00
29) Chrysene-d12	21.306	240	9539	0.400	ng	0.00
35) Perylene-d12	23.595	264	8389	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.341	112	36307	4.205	ng	0.00
5) Phenol-d6	6.937	99	47357	4.255	ng	0.00
8) Nitrobenzene-d5	8.886	82	34817	6.153	ng	-0.01
11) 2-Methylnaphthalene-d10	12.117	152	68560	4.550	ng	0.00
14) 2,4,6-Tribromophenol	15.861	330	9965	4.345	ng	0.00
15) 2-Fluorobiphenyl	12.998	172	94513	5.473	ng	0.00
27) Fluoranthene-d10	19.147	212	147161	4.287	ng	0.00
31) Terphenyl-d14	19.750	244	104189	5.480	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.225	88	16776	4.970	ng	93
3) n-Nitrosodimethylamine	3.543	42	17638	5.735	ng	# 92
6) bis(2-Chloroethyl)ether	7.168	93	40373	4.672	ng	98
9) Naphthalene	10.573	128	117275	4.854	ng	99
10) Hexachlorobutadiene	10.872	225	20458	5.024	ng	# 100
12) 2-Methylnaphthalene	12.189	142	79348	4.478	ng	100
16) Acenaphthylene	14.089	152	124330	5.496	ng	99
17) Acenaphthene	14.431	154	76952	4.884	ng	97
18) Fluorene	15.415	166	100064	4.415	ng	100
21) 4-Bromophenyl-phenylether	16.302	248	28400	5.253	ng	# 87
22) Hexachlorobenzene	16.426	284	30788	5.051	ng	99
23) Atrazine	16.579	200	24062	5.981	ng	98
24) Pentachlorophenol	16.774	266	10112	3.773	ng	98
25) Phenanthrene	17.154	178	161641	4.798	ng	100
26) Anthracene	17.246	178	149687	5.160	ng	100
28) Fluoranthene	19.177	202	182322	4.096	ng	99
30) Pyrene	19.539	202	186583	5.300	ng	100
32) Benzo(a)anthracene	21.288	228	171935	5.025	ng	98
33) Chrysene	21.342	228	176995	4.539	ng	98
34) Bis(2-ethylhexyl)phtha...	21.234	149	96067	6.113	ng	100
36) Indeno(1,2,3-cd)pyrene	25.925	276	197875	4.804	ng	99
37) Benzo(b)fluoranthene	22.902	252	168495	5.086	ng	97
38) Benzo(k)fluoranthene	22.948	252	172150	5.044	ng	98
39) Benzo(a)pyrene	23.492	252	144089	4.985	ng	95
40) Dibenzo(a,h)anthracene	25.945	278	159260	4.866	ng	97
41) Benzo(g,h,i)perylene	26.638	276	167446	4.581	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062622\
Data File : BN020469.D
Acq On : 26 Jun 2022 17:03
Operator : CG/JU
Sample : SSTDICC5.0
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Quant Time: Jun 27 01:38:20 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 01:36:24 2022
Response via : Initial Calibration

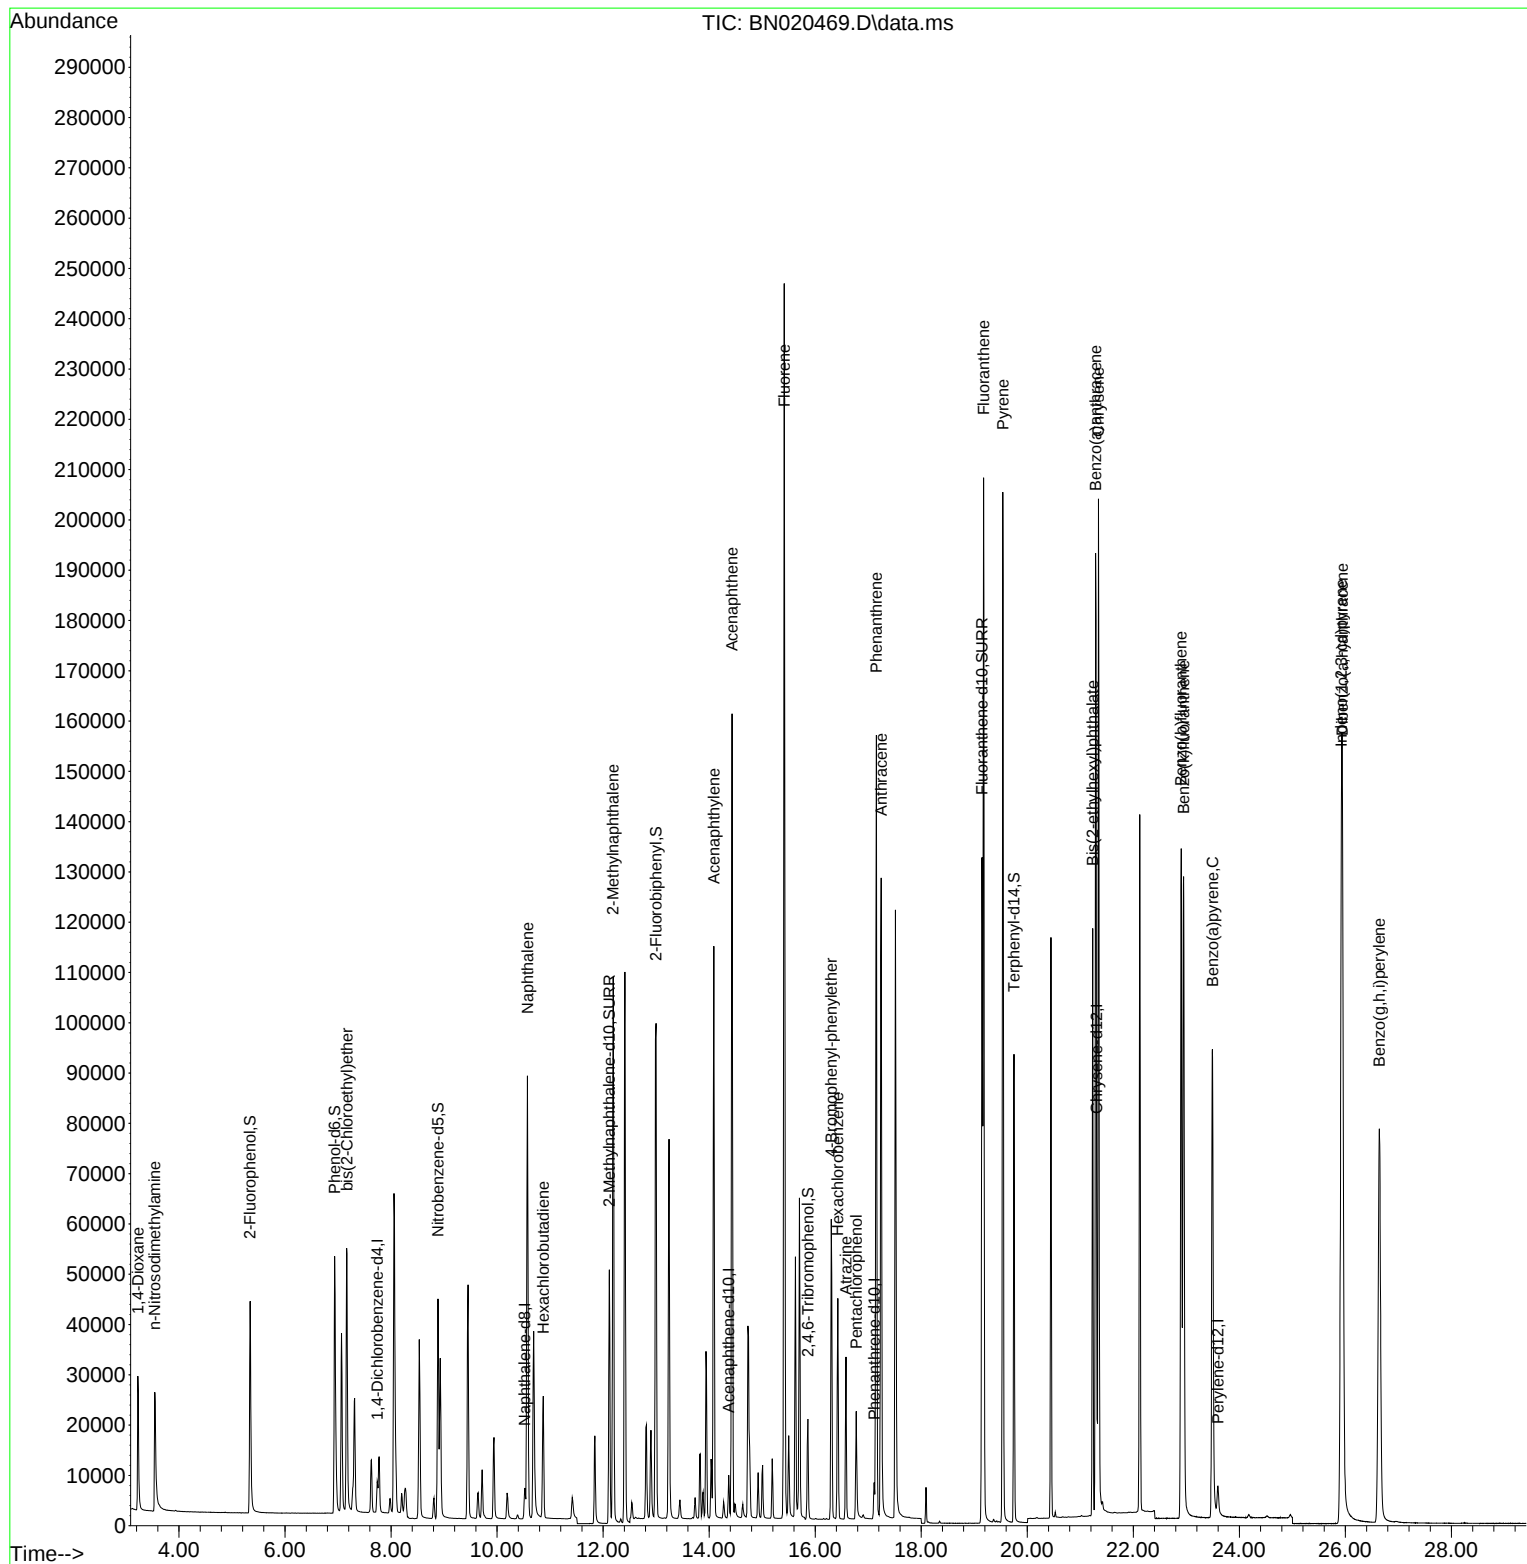





#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.739 min Scan# 64
 Delta R.T. -0.000 min
 Lab File: BN020469.D
 Acq: 26 Jun 2022 17:03

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0



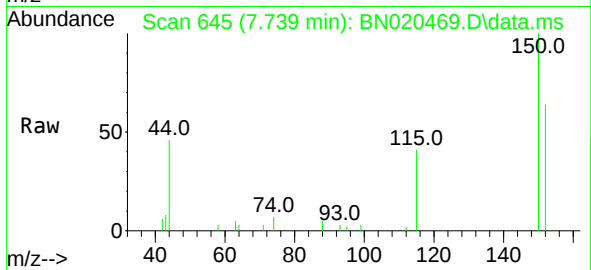



Tgt Ion:152 Resp: 2947
 Ion Ratio Lower Upper
 152 100
 150 155.1 127.9 191.9
 115 64.2 51.4 77.2

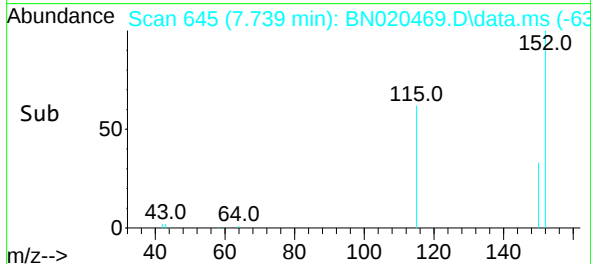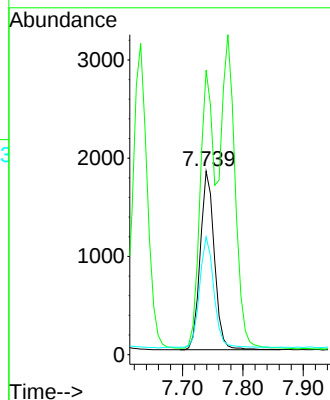

#2
 1,4-Dioxane
 Concen: 4.970 ng
 RT: 3.225 min Scan# 20
 Delta R.T. -0.007 min
 Lab File: BN020469.D
 Acq: 26 Jun 2022 17:03

Tgt Ion: 88 Resp: 16776
 Ion Ratio Lower Upper
 88 100
 43 33.5 30.2 45.2
 58 84.9 73.0 109.6

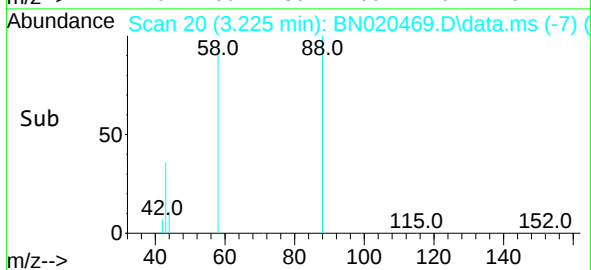
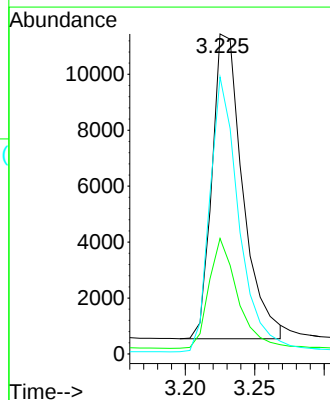
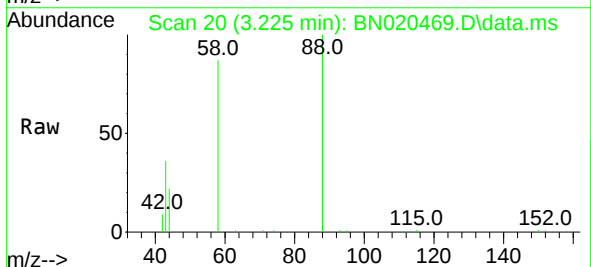




#3
n-Nitrosodimethylamine
Concen: 5.735 ng
RT: 3.543 min Scan# 64
Delta R.T. -0.014 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion: 42 Resp: 17638
Ion Ratio Lower Upper
42 100
74 112.6 84.0 126.0
44 7.5 9.8 14.8#

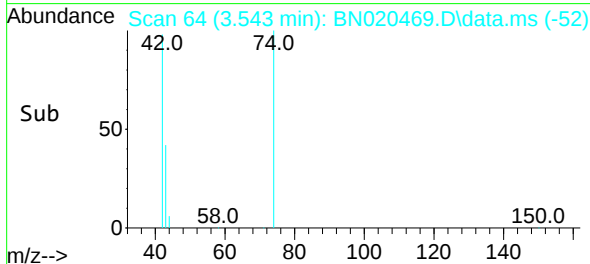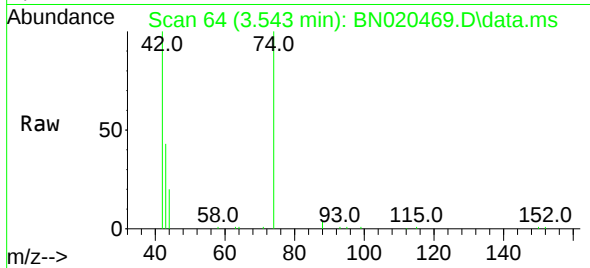

#4
2-Fluorophenol
Concen: 4.205 ng
RT: 5.341 min Scan# 313
Delta R.T. -0.007 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03

Tgt Ion: 112 Resp: 36307
Ion Ratio Lower Upper
112 100
64 61.7 49.1 73.7
63 32.5 26.3 39.5

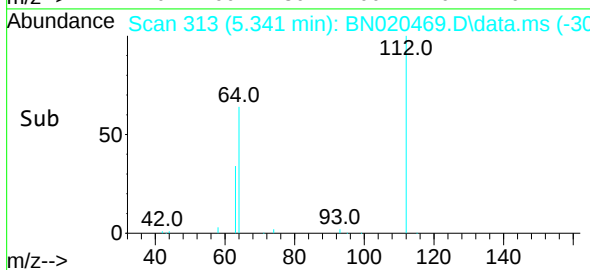

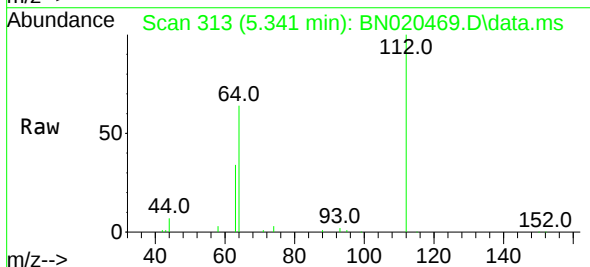




#5
Phenol-d6
Concen: 4.255 ng
RT: 6.937 min Scan# 51
Delta R.T. -0.007 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion: 99 Resp: 47357
Ion Ratio Lower Upper
99 100
42 21.6 19.3 28.9
71 35.3 27.5 41.3

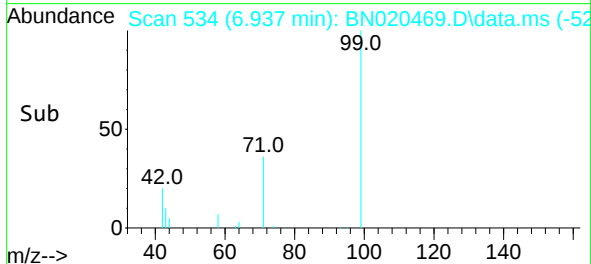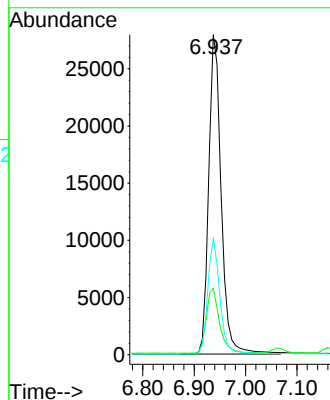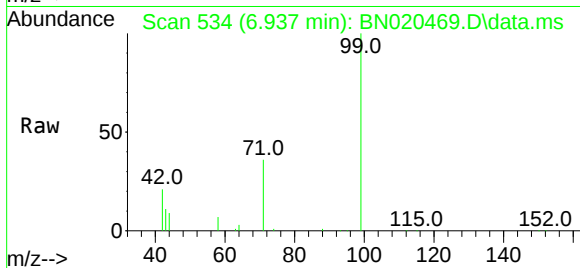

#6
bis(2-Chloroethyl)ether
Concen: 4.672 ng
RT: 7.168 min Scan# 566
Delta R.T. 0.000 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03

Tgt Ion: 93 Resp: 40373
Ion Ratio Lower Upper
93 100
63 82.3 67.4 101.0
95 32.7 26.5 39.7

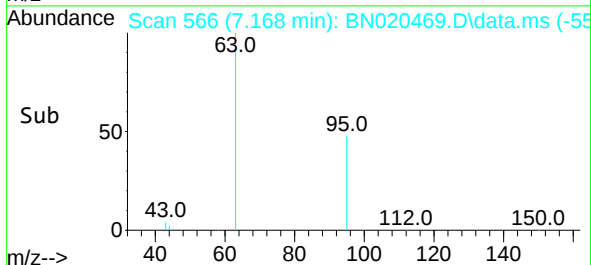
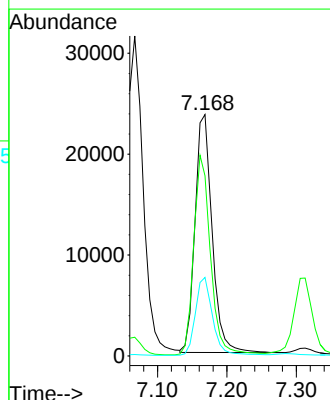
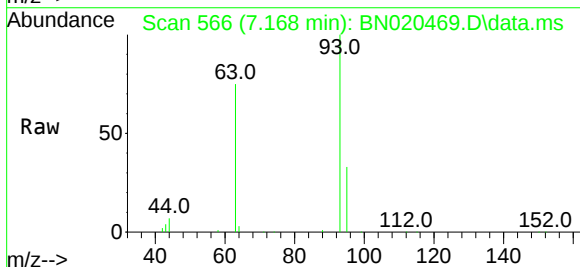




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.520 min Scan# 91
Delta R.T. 0.000 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:136 Resp: 8105
Ion Ratio Lower Upper
136 100
137 11.9 9.0 13.6
54 11.5 6.2 9.2#
68 7.5 4.4 6.6#

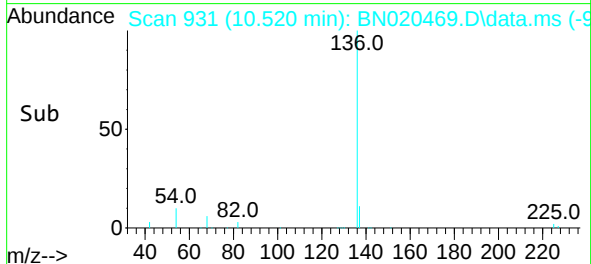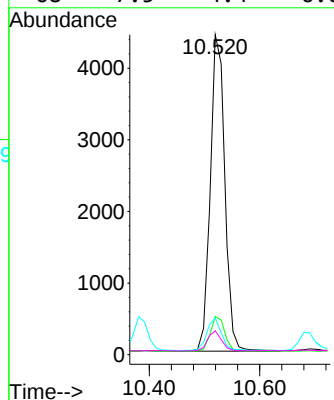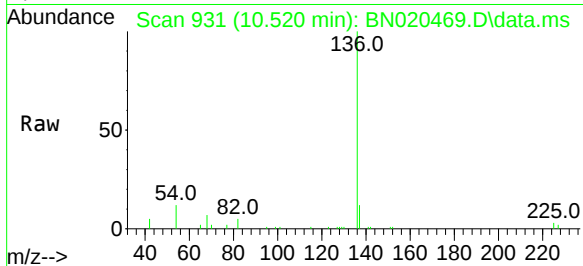

#8
Nitrobenzene-d5
Concen: 6.153 ng
RT: 8.886 min Scan# 778
Delta R.T. -0.011 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03

Tgt Ion: 82 Resp: 34817
Ion Ratio Lower Upper
82 100
128 40.7 35.0 52.6
54 57.5 46.2 69.4


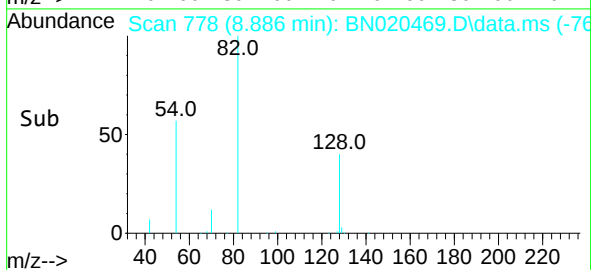
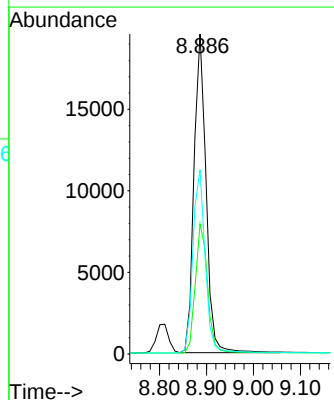
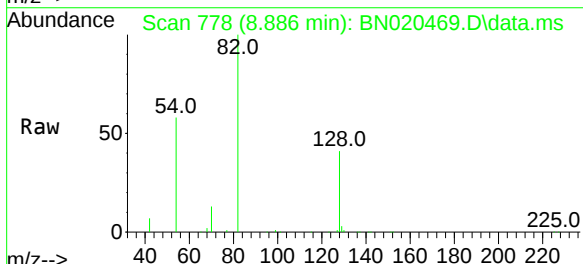




#9
Naphthalene
Concen: 4.854 ng
RT: 10.573 min Scan# 91
Delta R.T. 0.000 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:128 Resp: 117275
Ion Ratio Lower Upper
128 100
129 11.0 8.9 13.3
127 13.1 10.8 16.2

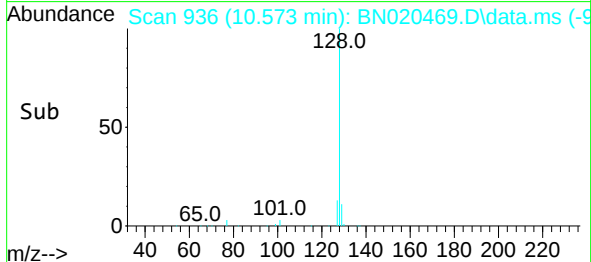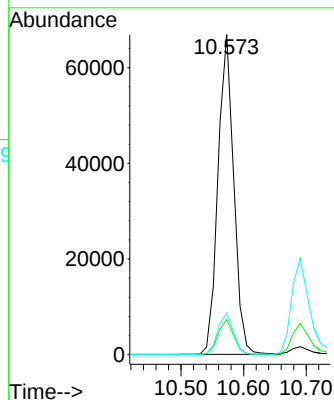

#10
Hexachlorobutadiene
Concen: 5.024 ng
RT: 10.872 min Scan# 964
Delta R.T. 0.000 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03

Tgt Ion:225 Resp: 20458
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.7 50.9 76.3

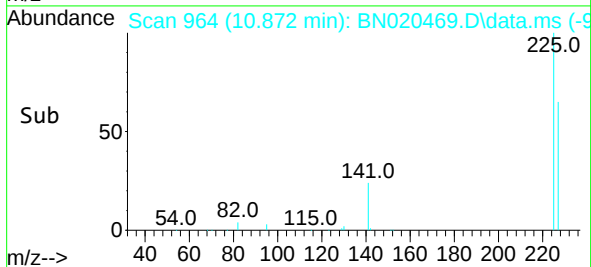
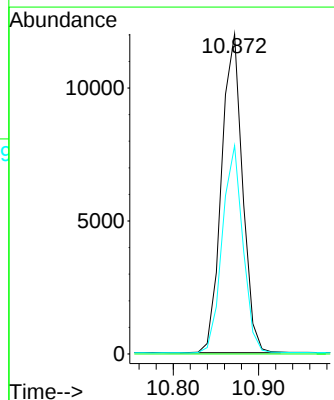
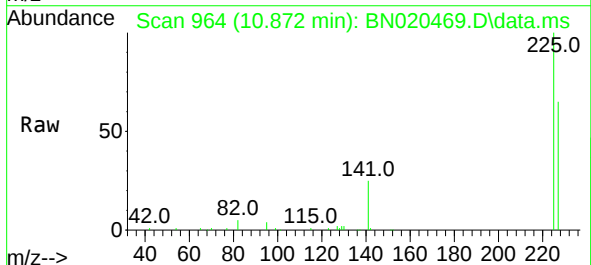




#11
2-Methylnaphthalene-d10
Concen: 4.550 ng
RT: 12.117 min Scan# 1184
Delta R.T. -0.004 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:152 Resp: 68560
Ion Ratio Lower Upper
152 100
151 20.5 16.2 24.4

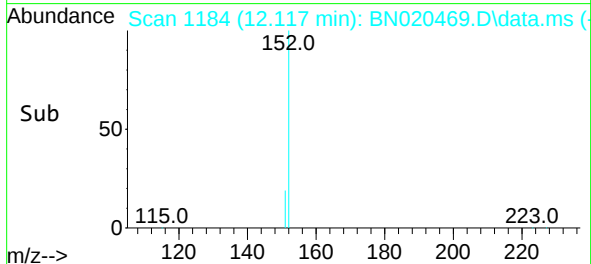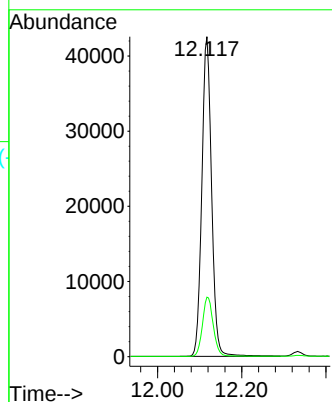

#12
2-Methylnaphthalene
Concen: 4.478 ng
RT: 12.189 min Scan# 1203
Delta R.T. -0.004 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03

Tgt Ion:142 Resp: 79348
Ion Ratio Lower Upper
142 100
141 89.6 71.6 107.4
115 37.7 29.8 44.8

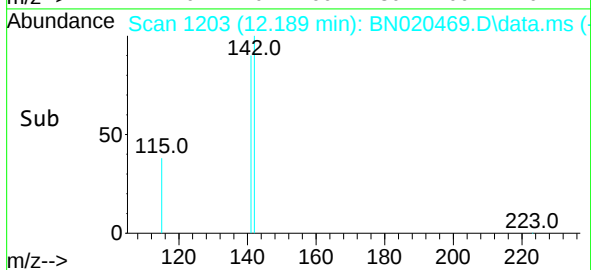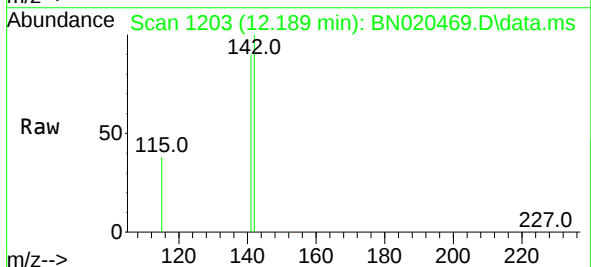



#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.367 min Scan# 1461

Delta R.T. 0.000 min

Lab File: BN020469.D

Acq: 26 Jun 2022 17:03

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:164 Resp: 4826

Ion Ratio Lower Upper

164 100

162 102.3 82.1 123.1

160 48.1 38.6 58.0

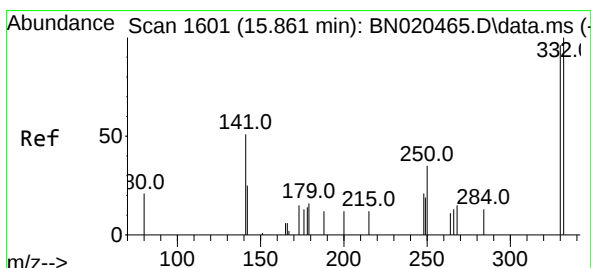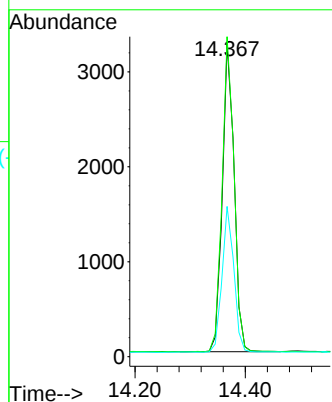

#14

2,4,6-Tribromophenol

Concen: 4.345 ng

RT: 15.861 min Scan# 1601

Delta R.T. 0.000 min

Lab File: BN020469.D

Acq: 26 Jun 2022 17:03




Tgt Ion:330 Resp: 9965

Ion Ratio Lower Upper

330 100

332 100.0 77.6 116.4

141 54.5 41.0 61.4

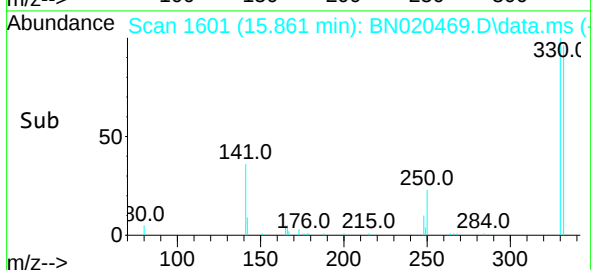






#15
2-Fluorobiphenyl
Concen: 5.473 ng
RT: 12.998 min Scan# 1333
Delta R.T. 0.000 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:172 Resp: 94513
Ion Ratio Lower Upper
172 100
171 34.4 27.2 40.8
170 22.5 18.2 27.4

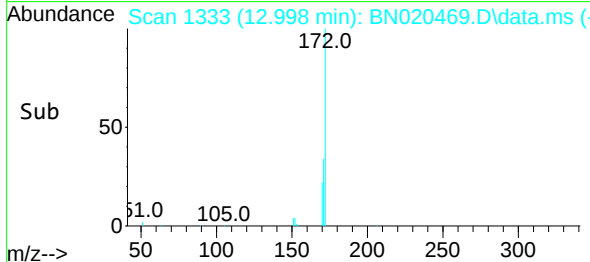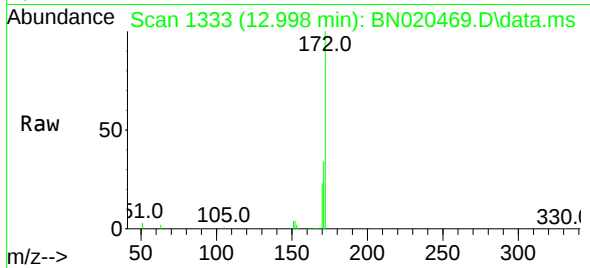

#16
Acenaphthylene
Concen: 5.496 ng
RT: 14.089 min Scan# 1435
Delta R.T. 0.000 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03

Tgt Ion:152 Resp: 124330
Ion Ratio Lower Upper
152 100
151 19.5 16.2 24.4
153 12.9 10.7 16.1


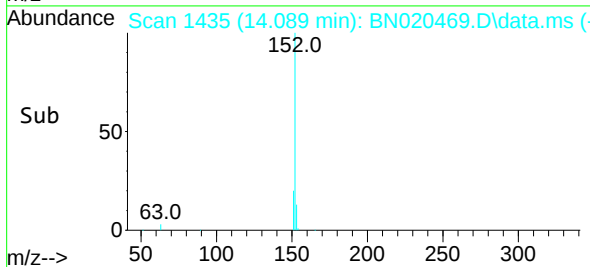

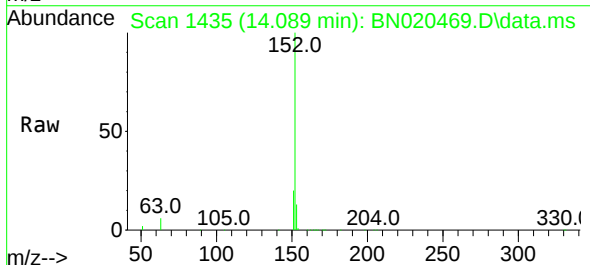




#17
Acenaphthene
Concen: 4.884 ng
RT: 14.431 min Scan# 1467
Delta R.T. 0.000 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:154 Resp: 76952
Ion Ratio Lower Upper
154 100
153 113.7 87.5 131.3
152 54.8 43.8 65.6

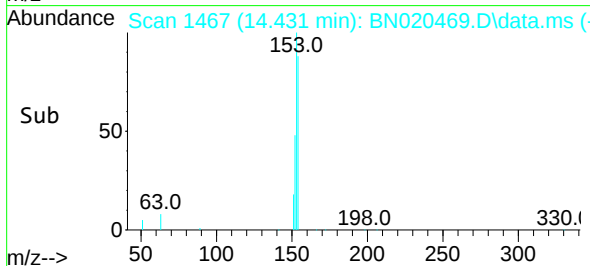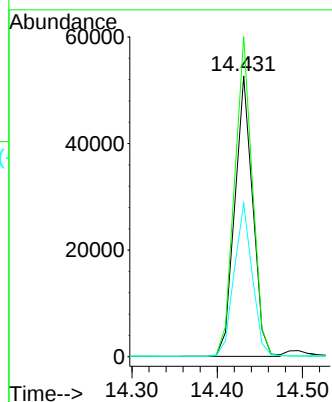

#18
Fluorene
Concen: 4.415 ng
RT: 15.415 min Scan# 1559
Delta R.T. 0.000 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03

Tgt Ion:166 Resp: 100064
Ion Ratio Lower Upper
166 100
165 98.0 78.6 118.0
167 13.4 10.8 16.2


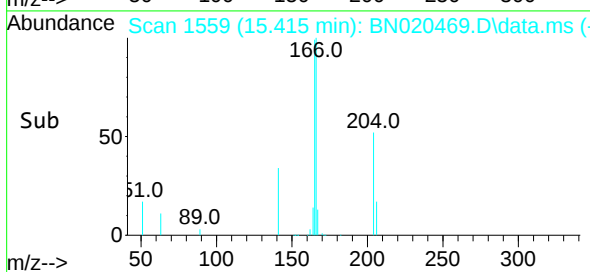
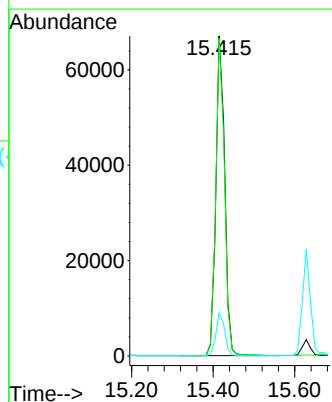
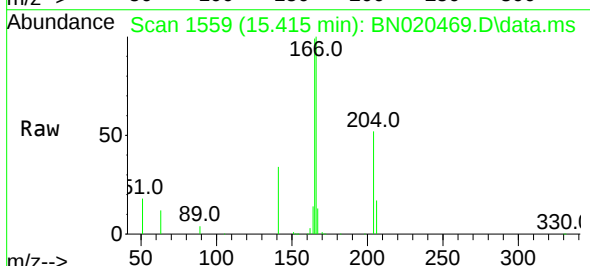




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.113 min Scan# 1723
Delta R.T. 0.000 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:188 Resp: 9789
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 11.0 7.4 11.2

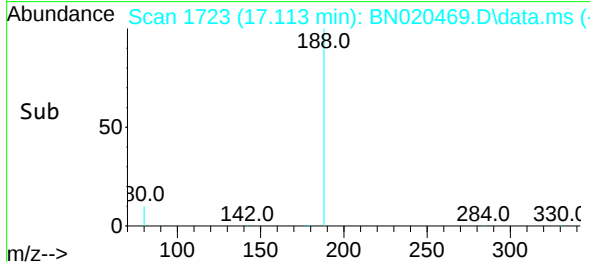

#21
4-Bromophenyl-phenylether
Concen: 5.253 ng
RT: 16.302 min Scan# 1644
Delta R.T. -0.010 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03

Tgt Ion:248 Resp: 28400
Ion Ratio Lower Upper
248 100
250 92.8 75.3 112.9
141 107.5 67.3 100.9#


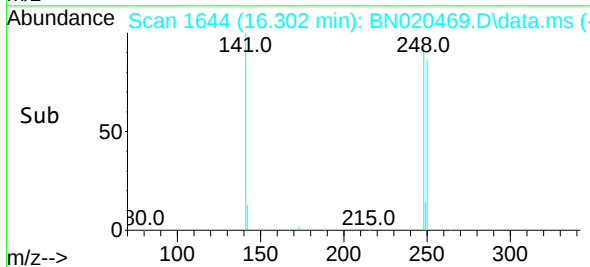

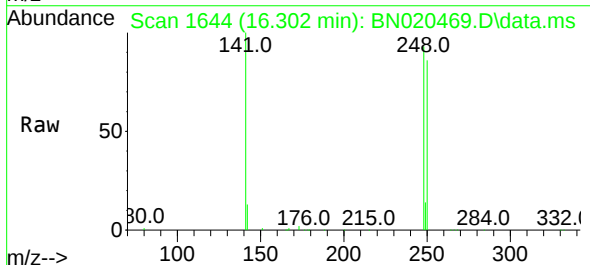




#22
Hexachlorobenzene
Concen: 5.051 ng
RT: 16.426 min Scan# 1656
Delta R.T. 0.000 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:284 Resp: 30788
Ion Ratio Lower Upper
284 100
142 43.8 35.2 52.8
249 34.2 26.6 40.0

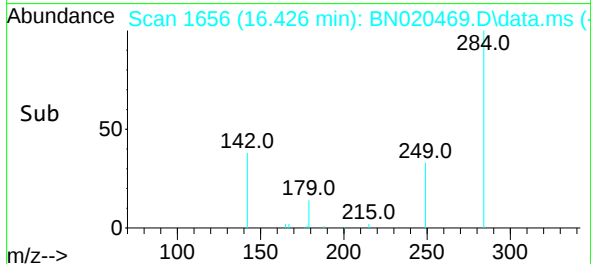

#23
Atrazine
Concen: 5.981 ng
RT: 16.579 min Scan# 1671
Delta R.T. 0.000 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03

Tgt Ion:200 Resp: 24062
Ion Ratio Lower Upper
200 100
173 28.1 23.6 35.4
215 45.0 36.6 54.8


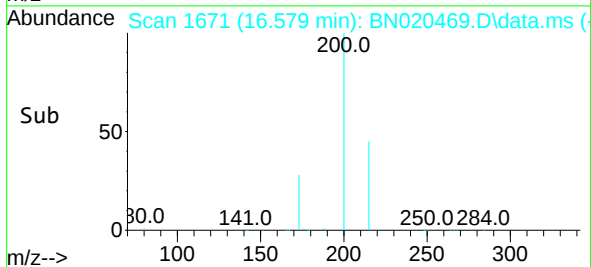

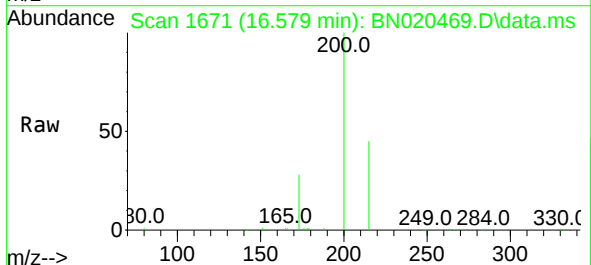




#24
 Pentachlorophenol
 Concen: 3.773 ng
 RT: 16.774 min Scan# 1690
 Delta R.T. -0.010 min
 Lab File: BN020469.D
 Acq: 26 Jun 2022 17:03




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:266 Resp: 10112
 Ion Ratio Lower Upper
 266 100
 264 63.2 51.3 76.9
 268 63.8 52.6 79.0

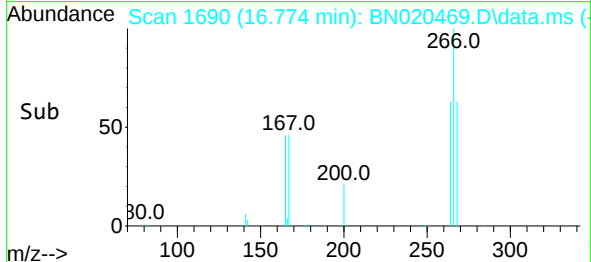

#25
 Phenanthrene
 Concen: 4.798 ng
 RT: 17.154 min Scan# 1727
 Delta R.T. 0.000 min
 Lab File: BN020469.D
 Acq: 26 Jun 2022 17:03

Tgt Ion:178 Resp: 161641
 Ion Ratio Lower Upper
 178 100
 176 19.1 15.3 22.9
 179 15.3 12.2 18.4


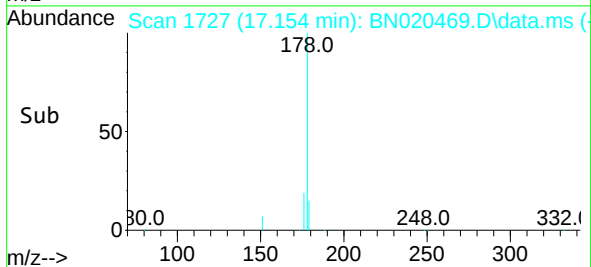

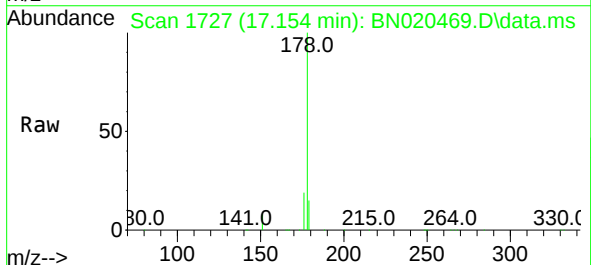




#26
 Anthracene
 Concen: 5.160 ng
 RT: 17.246 min Scan# 1736
 Delta R.T. 0.000 min
 Lab File: BN020469.D
 Acq: 26 Jun 2022 17:03




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:178 Resp: 149687
 Ion Ratio Lower Upper
 178 100
 176 18.4 14.9 22.3
 179 15.2 12.2 18.4

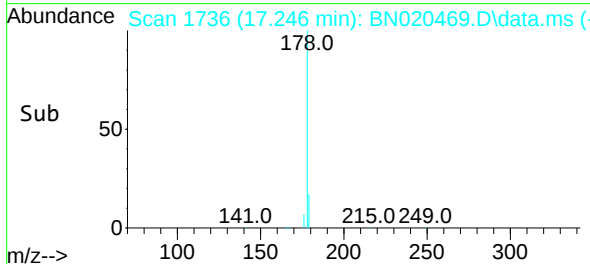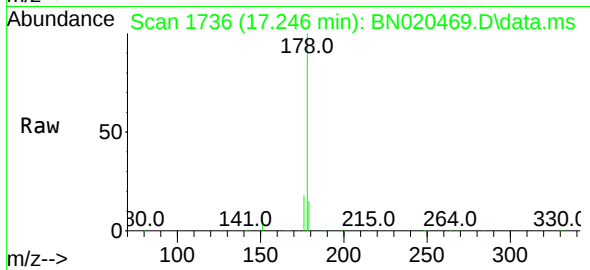

#27
 Fluoranthene-d10
 Concen: 4.287 ng
 RT: 19.147 min Scan# 2081
 Delta R.T. 0.000 min
 Lab File: BN020469.D
 Acq: 26 Jun 2022 17:03

Tgt Ion:212 Resp: 147161
 Ion Ratio Lower Upper
 212 100
 106 15.7 12.6 19.0
 104 8.8 7.2 10.8


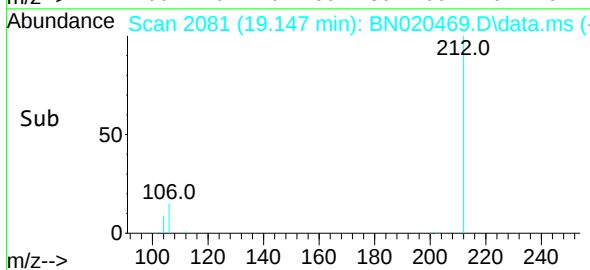

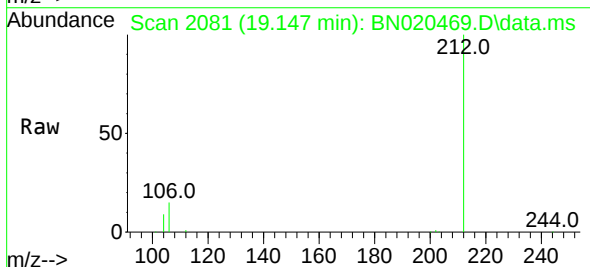


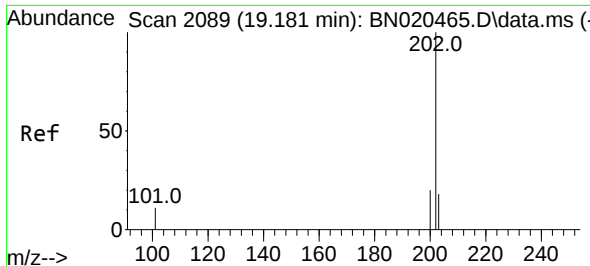

#28
Fluoranthene
Concen: 4.096 ng
RT: 19.177 min Scan# 2088
Delta R.T. -0.004 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:202 Resp: 182322
Ion Ratio Lower Upper
202 100
101 12.5 9.6 14.4
203 17.3 13.5 20.3

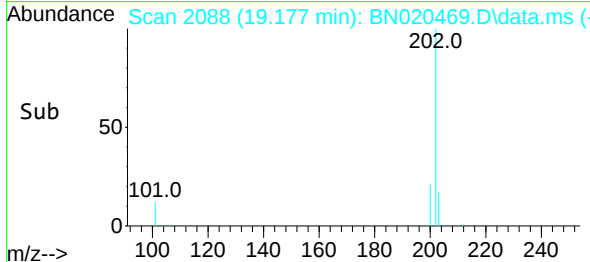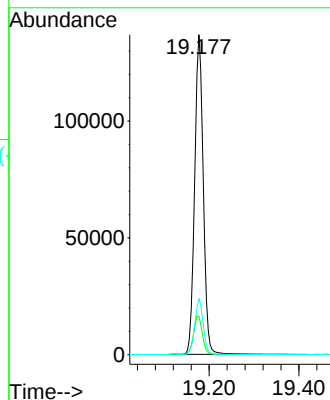

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.306 min Scan# 2430
Delta R.T. 0.000 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03

Tgt Ion:240 Resp: 9539
Ion Ratio Lower Upper
240 100
120 15.5 14.6 21.8
236 27.9 22.6 33.8


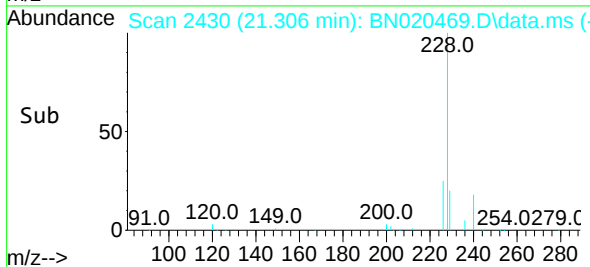
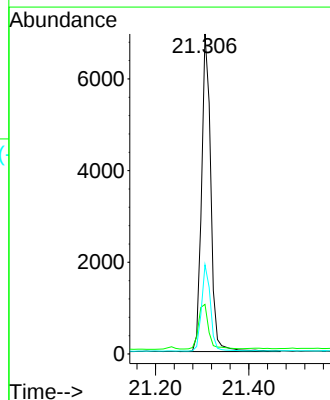
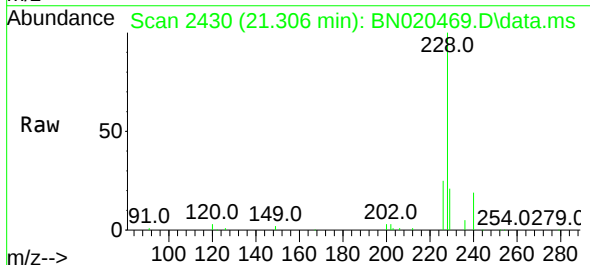




#30
Pyrene
Concen: 5.300 ng
RT: 19.539 min Scan# 2174
Delta R.T. -0.004 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:202 Resp: 186583
Ion Ratio Lower Upper
202 100
200 20.9 16.6 25.0
203 17.7 14.2 21.2

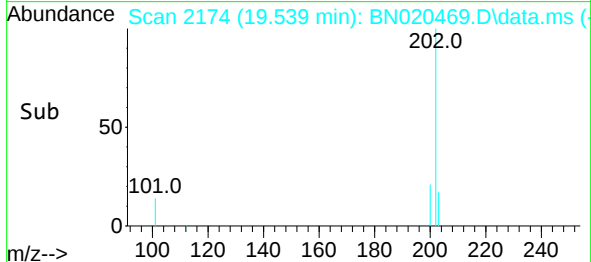

#31
Terphenyl-d14
Concen: 5.480 ng
RT: 19.750 min Scan# 2224
Delta R.T. -0.004 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03

Tgt Ion:244 Resp: 104189
Ion Ratio Lower Upper
244 100
212 8.6 7.1 10.7
122 0.0 0.0 0.0


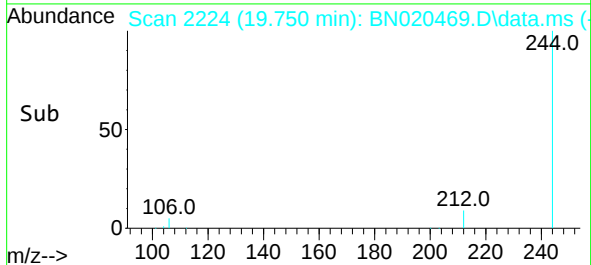

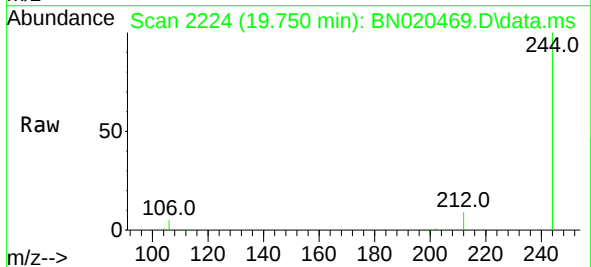




#32
Benzo(a)anthracene
Concen: 5.025 ng
RT: 21.288 min Scan# 2428
Delta R.T. -0.009 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:228 Resp: 171935
Ion Ratio Lower Upper
228 100
226 27.9 21.2 31.8
229 19.4 15.6 23.4

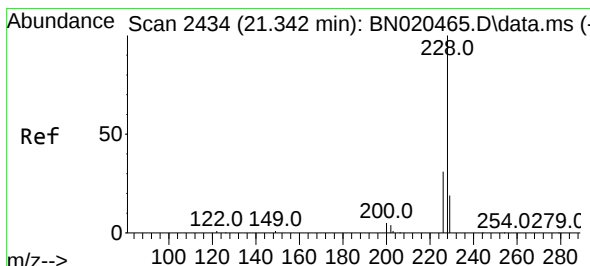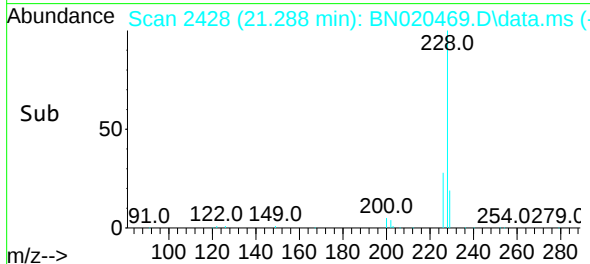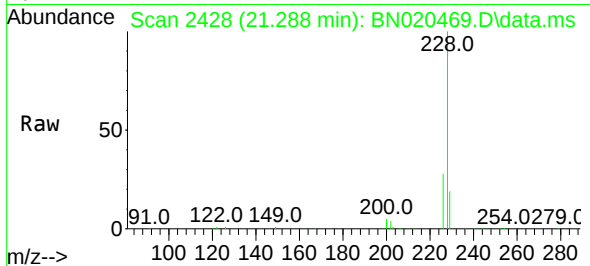

#33
Chrysene
Concen: 4.539 ng
RT: 21.342 min Scan# 2434
Delta R.T. 0.000 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03

Tgt Ion:228 Resp: 176995
Ion Ratio Lower Upper
228 100
226 30.5 23.4 35.0
229 19.4 15.7 23.5



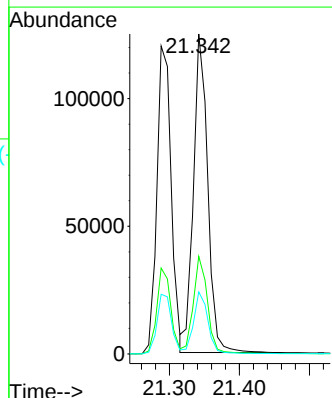
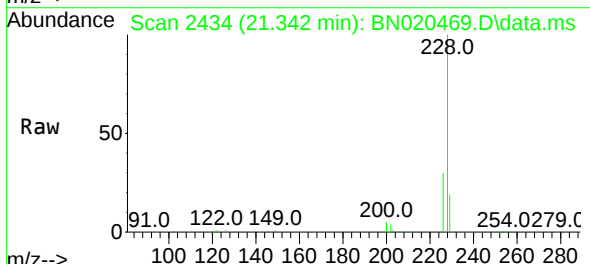


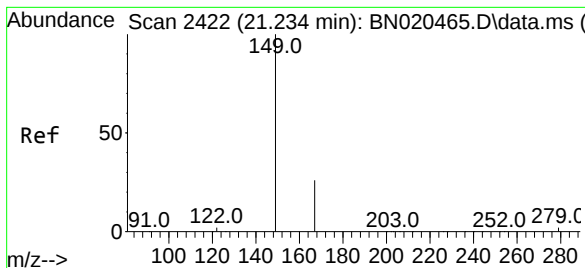

#34
Bis(2-ethylhexyl)phthalate
Concen: 6.113 ng
RT: 21.234 min Scan# 2422
Delta R.T. 0.000 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:149 Resp: 96067
Ion Ratio Lower Upper
149 100
167 27.0 21.7 32.5
279 2.9 2.2 3.2

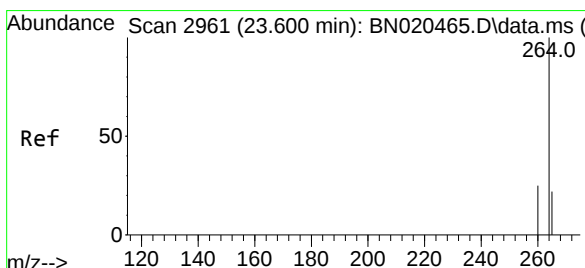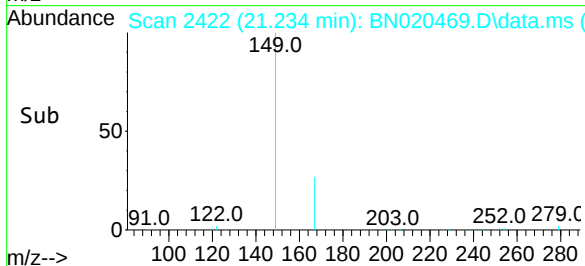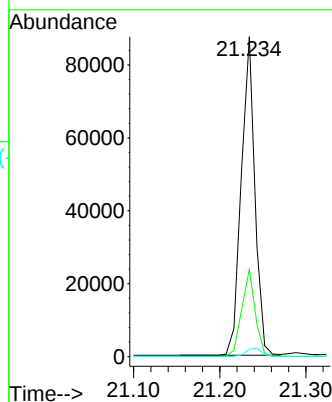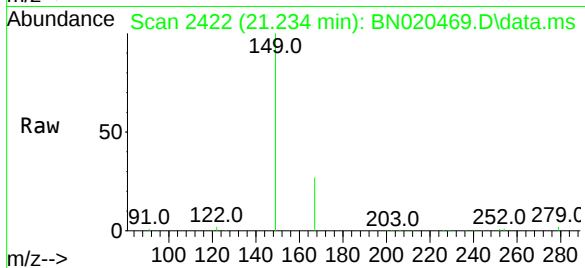

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.595 min Scan# 2959
Delta R.T. -0.006 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03

Tgt Ion:264 Resp: 8389
Ion Ratio Lower Upper
264 100
260 25.8 20.9 31.3
265 39.8 28.0 42.0


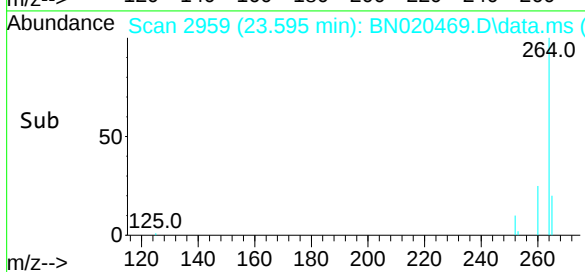
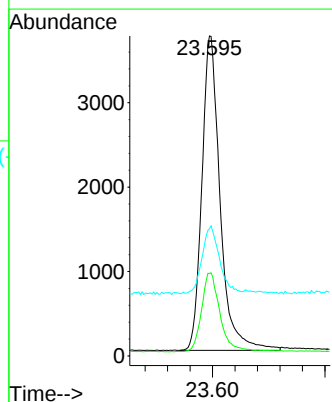
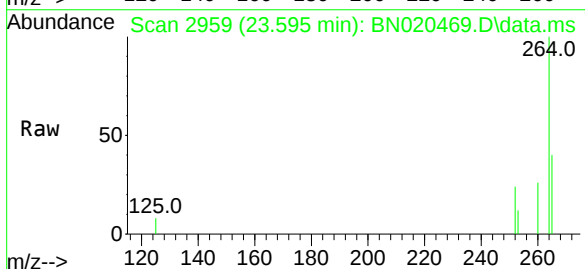




#36
Indeno(1,2,3-cd)pyrene
Concen: 4.804 ng
RT: 25.925 min Scan# 31
Delta R.T. -0.012 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:276 Resp: 197875
Ion Ratio Lower Upper
276 100
138 31.9 25.9 38.9
277 25.0 19.8 29.8

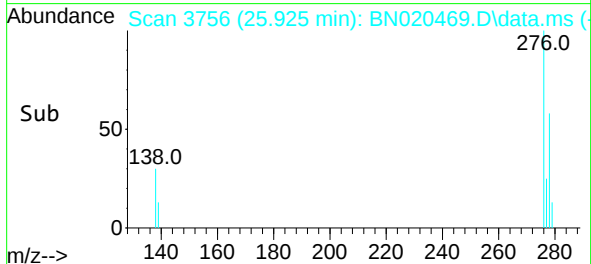

#37
Benzo(b)fluoranthene
Concen: 5.086 ng
RT: 22.902 min Scan# 2722
Delta R.T. -0.006 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03

Tgt Ion:252 Resp: 168495
Ion Ratio Lower Upper
252 100
253 21.6 18.5 27.7
125 12.7 11.4 17.0


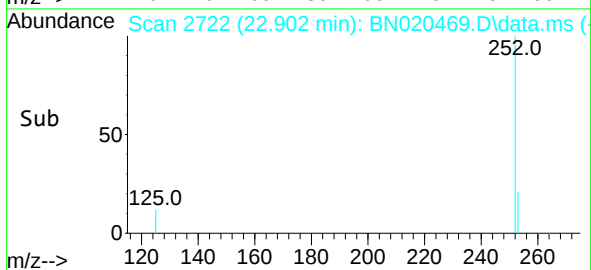

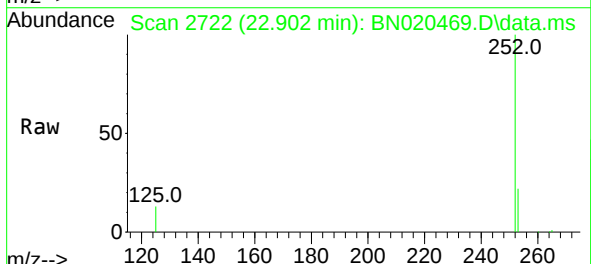




#38
Benzo(k)fluoranthene
Concen: 5.044 ng
RT: 22.948 min Scan# 21
Delta R.T. -0.006 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:252 Resp: 172150
Ion Ratio Lower Upper
252 100
253 22.0 18.0 27.0
125 12.5 11.0 16.4

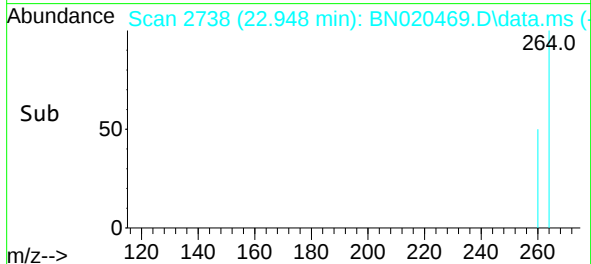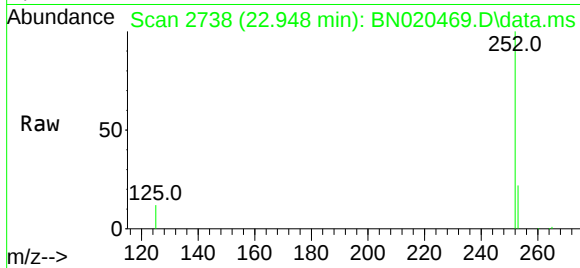

#39
Benzo(a)pyrene
Concen: 4.985 ng
RT: 23.492 min Scan# 2924
Delta R.T. -0.006 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03

Tgt Ion:252 Resp: 144089
Ion Ratio Lower Upper
252 100
253 22.1 19.0 28.4
125 14.4 13.8 20.8


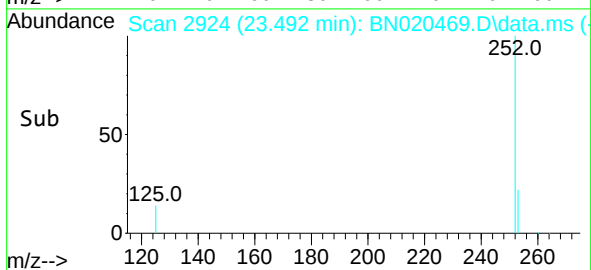

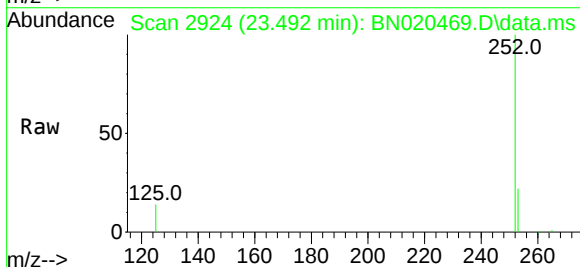




#40
Dibenzo(a,h)anthracene
Concen: 4.866 ng
RT: 25.945 min Scan# 31
Delta R.T. -0.003 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:278 Resp: 159260
Ion Ratio Lower Upper
278 100
139 21.1 18.6 28.0
279 23.3 19.7 29.5

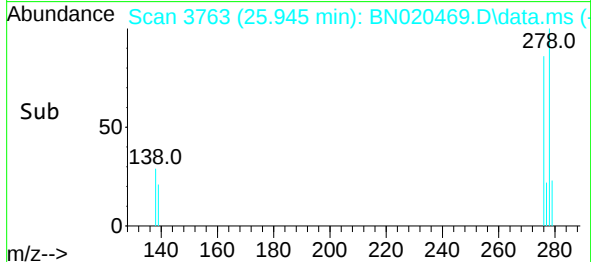

#41
Benzo(g,h,i)perylene
Concen: 4.581 ng
RT: 26.638 min Scan# 4000
Delta R.T. -0.015 min
Lab File: BN020469.D
Acq: 26 Jun 2022 17:03

Tgt Ion:276 Resp: 167446
Ion Ratio Lower Upper
276 100
277 23.6 19.5 29.3
138 27.6 22.6 34.0

