

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062622\
 Data File : BN020475.D
 Acq On : 26 Jun 2022 21:18
 Operator : CG/JU
 Sample : N3354-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MW-48

Manual Integrations
 APPROVED

Reviewed By : Christian Giraldo 06/28/2022
 Supervised By : Jagrut Upadhyay 06/30/2022

Quant Time: Jun 27 02:51:57 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 27 02:03:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.739	152	2882	0.400	ng	0.00
7) Naphthalene-d8	10.519	136	9865	0.400	ng	# 0.00
13) Acenaphthene-d10	14.367	164	11472	0.400	ng	# 0.00
19) Phenanthrene-d10	17.113	188	12327	0.400	ng	# 0.00
29) Chrysene-d12	21.306	240	10614	0.400	ng	0.00
35) Perylene-d12	23.583	264	9494	0.400	ng	-0.02
System Monitoring Compounds						
4) 2-Fluorophenol	5.355	112	1171	0.146	ng	0.00
5) Phenol-d6	6.952	99	783	0.082	ng	0.00
8) Nitrobenzene-d5	8.886	82	2017	0.252	ng	-0.01
11) 2-Methylnaphthalene-d10	12.117	152	6019	0.356	ng	0.00
14) 2,4,6-Tribromophenol	15.861	330	1004	0.232	ng	0.00
15) 2-Fluorobiphenyl	12.998	172	7256	0.153	ng	0.00
27) Fluoranthene-d10	19.147	212	13067	0.357	ng	0.00
31) Terphenyl-d14	19.746	244	10316	0.407	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.232	88	169	0.045	ng	# 1
9) Naphthalene	10.573	128	2298	0.078	ng	# 20
12) 2-Methylnaphthalene	12.189	142	1195	0.061	ng	# 56
16) Acenaphthylene	14.089	152	5525	0.100	ng	# 1
17) Acenaphthene	14.431	154	19918	0.531	ng	98
18) Fluorene	15.414	166	5163	0.105	ng	# 93
25) Phenanthrene	17.154	178	1005	0.024	ng	# 45
26) Anthracene	17.246	178	2067	0.058	ng	# 1
28) Fluoranthene	19.177	202	1014	0.022	ng	# 84
30) Pyrene	19.539	202	1775m	0.039	ng	
34) Bis(2-ethylhexyl)phtha...	21.225	149	1789	0.084	ng	# 87

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062622\
Data File : BN020475.D
Acq On : 26 Jun 2022 21:18
Operator : CG/JU
Sample : N3354-03
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
MW-48

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 06/28/2022
Supervised By :Jagrut Upadhyay 06/30/2022


Quant Time: Jun 27 02:51:57 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 02:03:21 2022
Response via : Initial Calibration

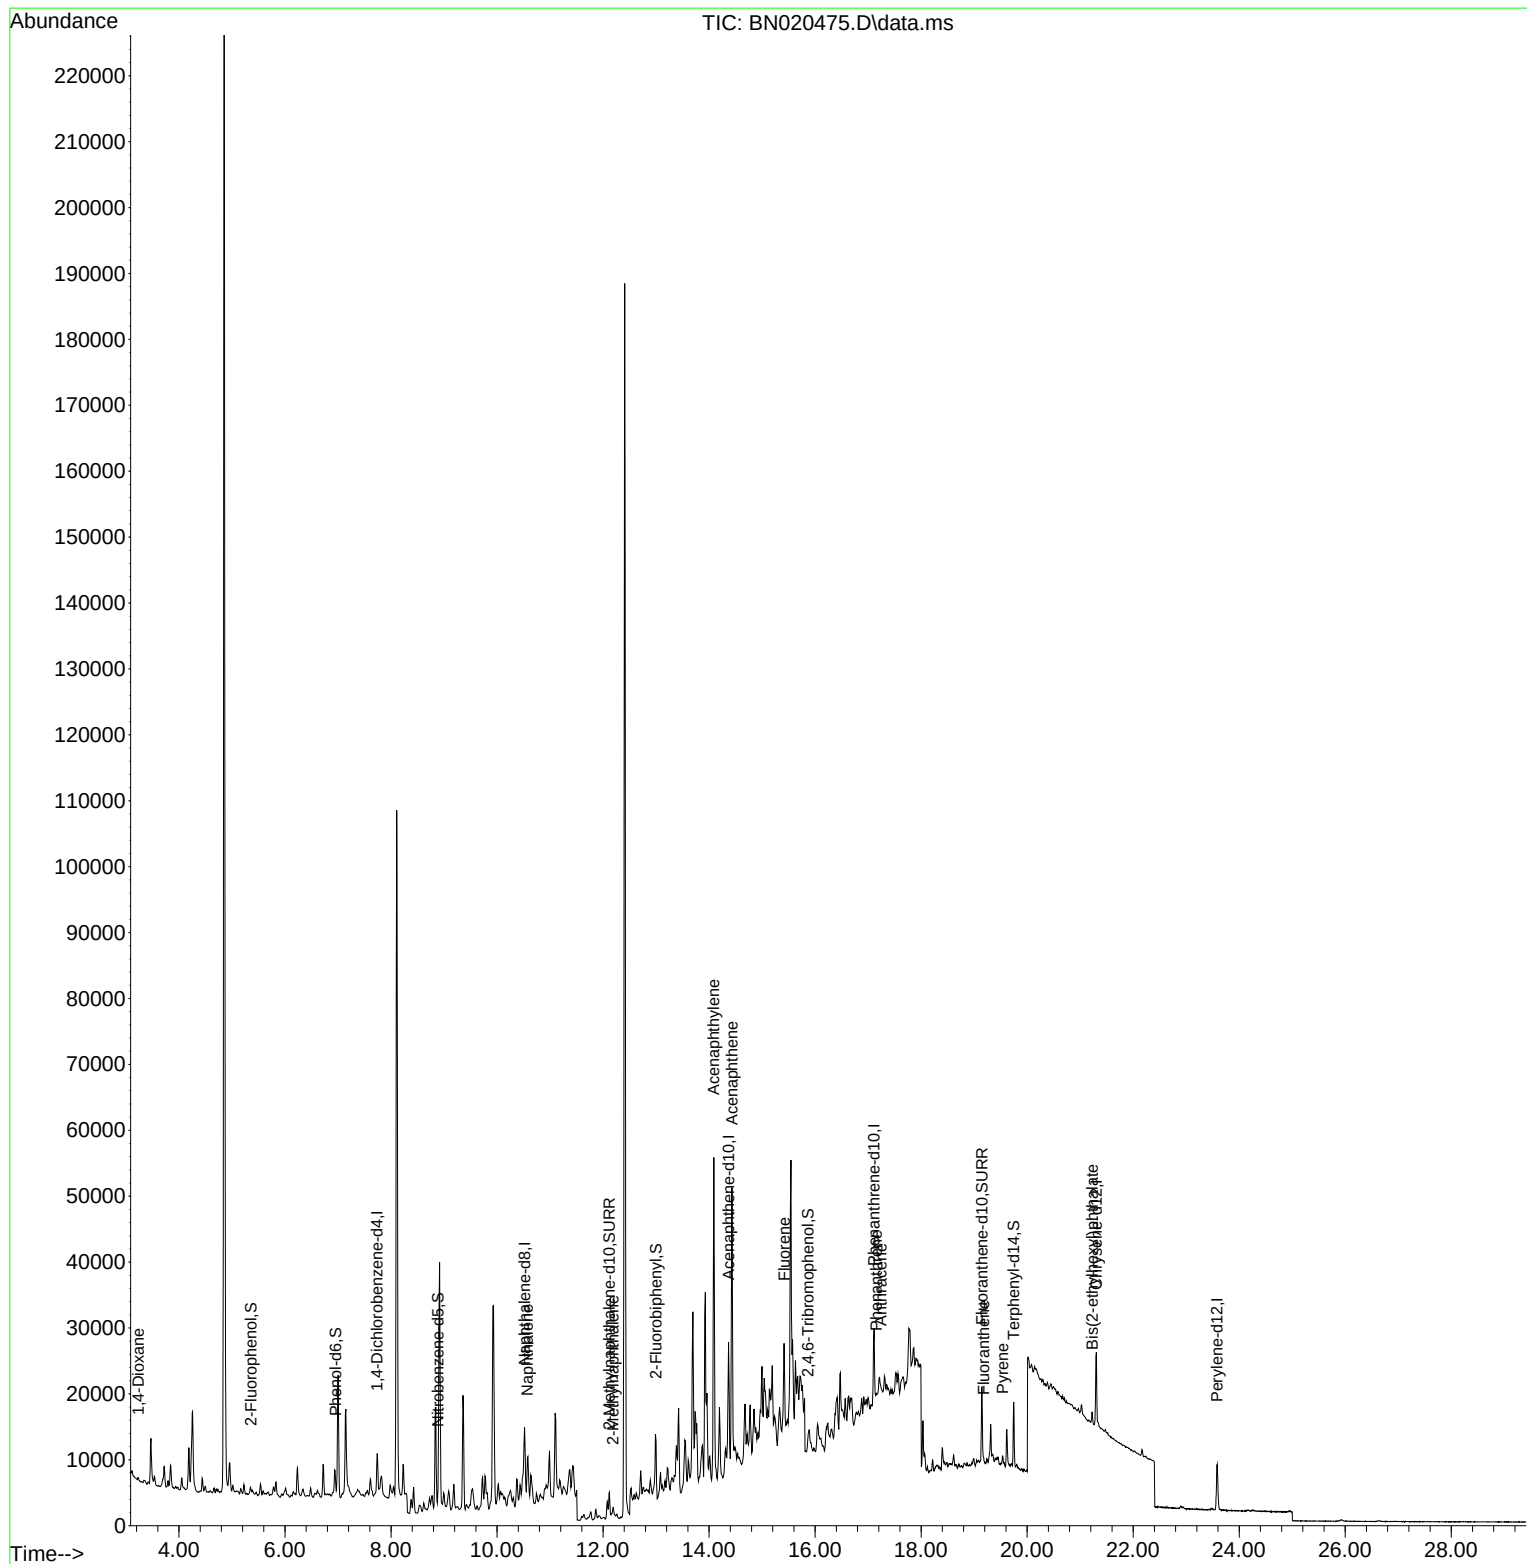

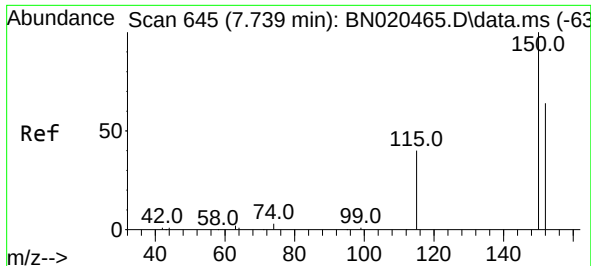

#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.739 min Scan# 645
 Delta R.T. -0.000 min
 Lab File: BN020475.D
 Acq: 26 Jun 2022 21:18




Instrument :
 BNA_N
 ClientSampleId :
 MW-48

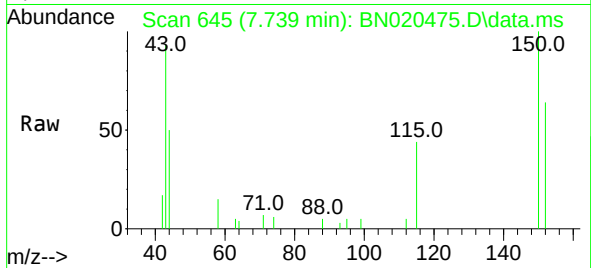


Tgt Ion: 152 Resp: 288
 Ion Ratio Lower Upper
 152 100
 150 155.4 127.9 191.9
 115 67.8 51.4 77.2

Manual Integrations
 APPROVED



Reviewed By : Christian Giraldo 06/28/2022
 Supervised By : Jagrut Upadhyay 06/30/2022

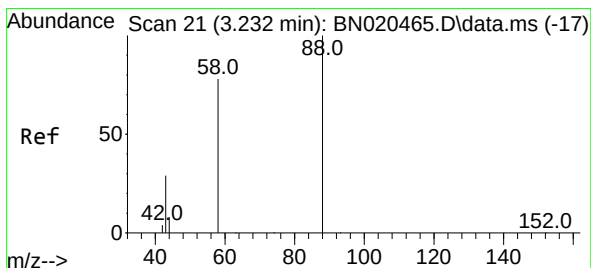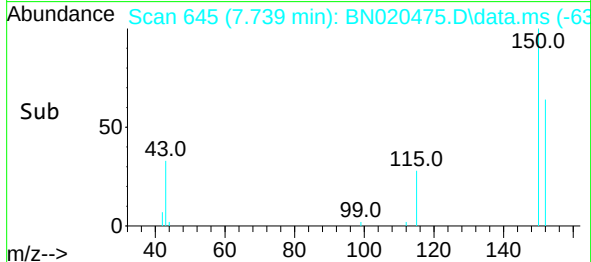


#2
 1,4-Dioxane
 Concen: 0.045 ng
 RT: 3.232 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BN020475.D
 Acq: 26 Jun 2022 21:18

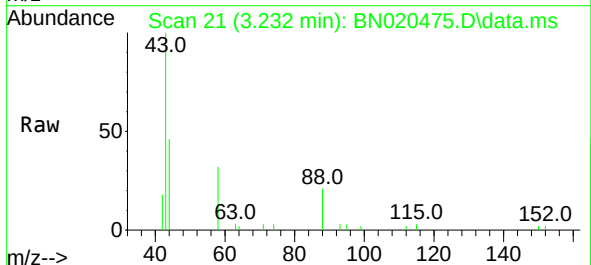

Tgt Ion: 88 Resp: 169
 Ion Ratio Lower Upper
 88 100
 43 286.4 30.2 45.2#
 58 161.5 73.0 109.6#

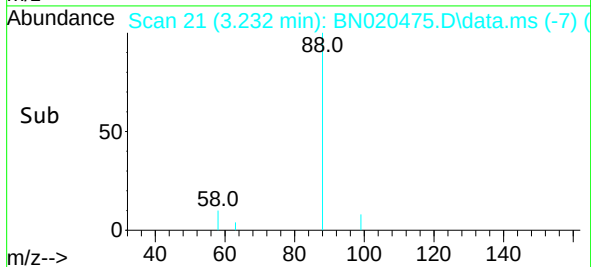

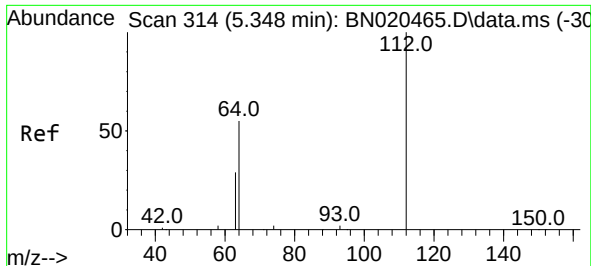





#4
2-Fluorophenol
Concen: 0.146 ng
RT: 5.355 min Scan# 314
Delta R.T. 0.007 min
Lab File: BN020475.D
Acq: 26 Jun 2022 21:18

Instrument :
BNA_N
ClientSampleId :
MW-48

Tgt Ion: 112 Resp: 117
Ion Ratio Lower Upper
112 100
64 68.1 49.1 73.7
63 29.8 26.3 39.5




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 06/28/2022
Supervised By :Jagrut Upadhyay 06/30/2022

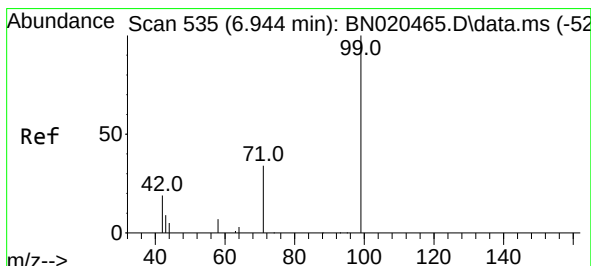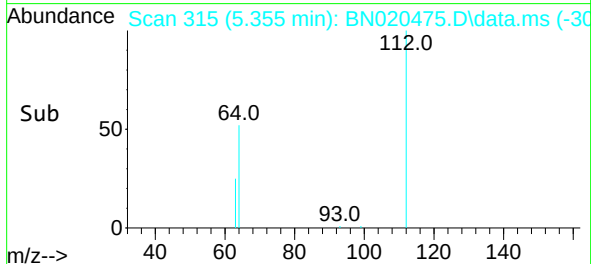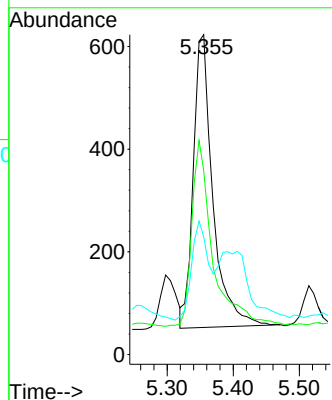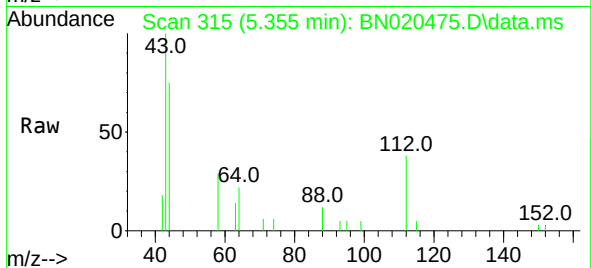

#5
Phenol-d6
Concen: 0.082 ng
RT: 6.952 min Scan# 536
Delta R.T. 0.007 min
Lab File: BN020475.D
Acq: 26 Jun 2022 21:18


Tgt Ion: 99 Resp: 783
Ion Ratio Lower Upper
99 100
42 60.2 19.3 28.9#
71 274.5 27.5 41.3#

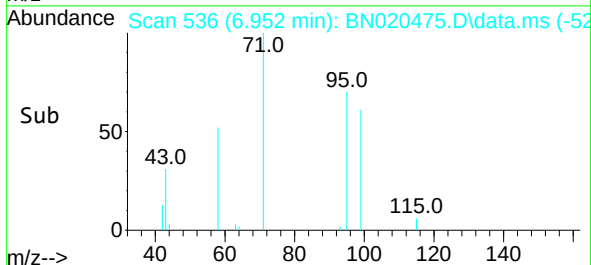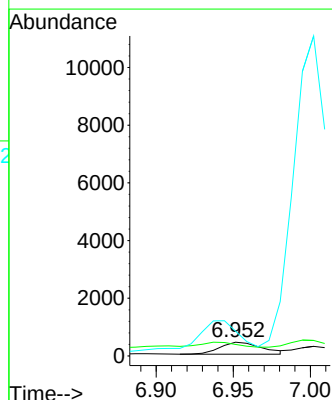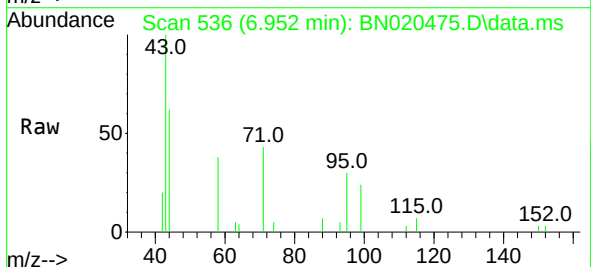

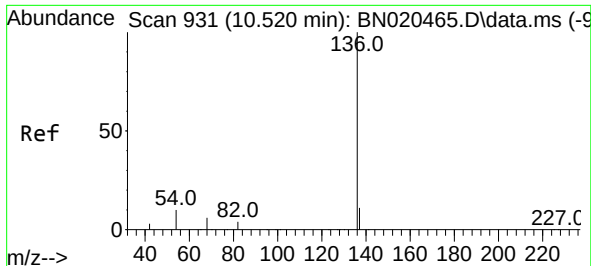

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.519 min Scan# 91
Delta R.T. -0.000 min
Lab File: BN020475.D
Acq: 26 Jun 2022 21:18




Instrument :
BNA_N
ClientSampleId :
MW-48

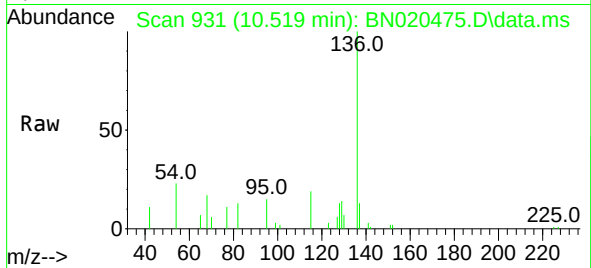

Tgt Ion	Ratio	Lower	Upper
136	100		
137	12.5	9.0	13.6
54	23.2	6.2	9.2
68	17.4	4.4	6.6




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 06/28/2022
Supervised By :Jagrut Upadhyay 06/30/2022

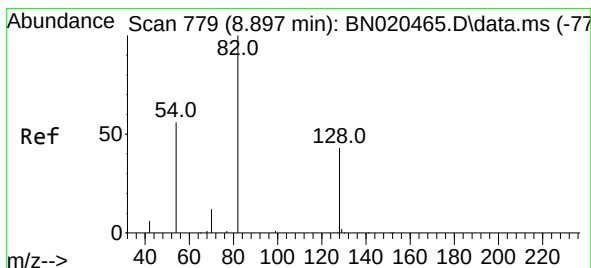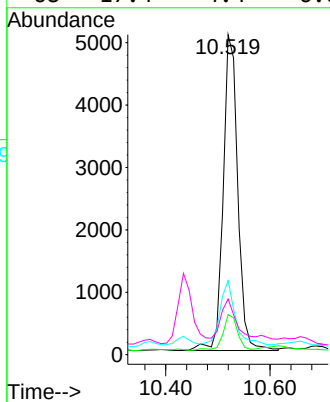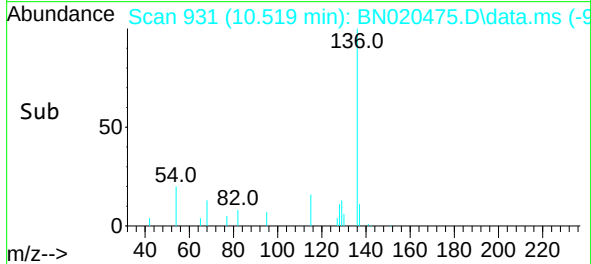

#8
Nitrobenzene-d5
Concen: 0.252 ng
RT: 8.886 min Scan# 778
Delta R.T. -0.011 min
Lab File: BN020475.D
Acq: 26 Jun 2022 21:18


Tgt Ion	Ratio	Lower	Upper
82	100		
128	41.3	35.0	52.6
54	64.4	46.2	69.4

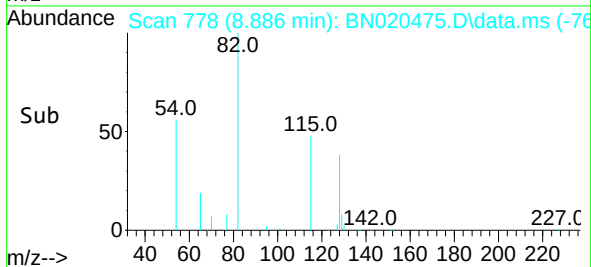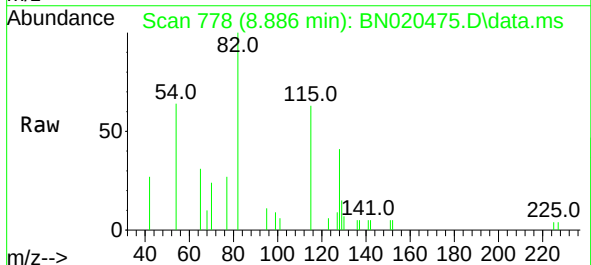

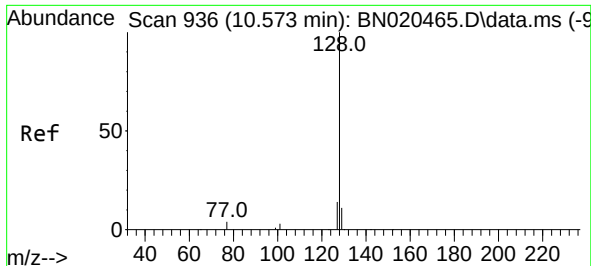

#9
Naphthalene
Concen: 0.078 ng
RT: 10.573 min Scan# 91
Delta R.T. -0.000 min
Lab File: BN020475.D
Acq: 26 Jun 2022 21:18




Instrument :
BNA_N
ClientSampleId :
MW-48

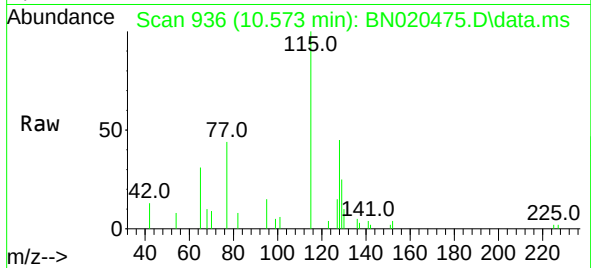

Tgt Ion:128 Resp: 2298
Ion Ratio Lower Upper
128 100
129 56.8 8.9 13.3
127 32.4 10.8 16.2




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 06/28/2022
Supervised By :Jagrut Upadhyay 06/30/2022

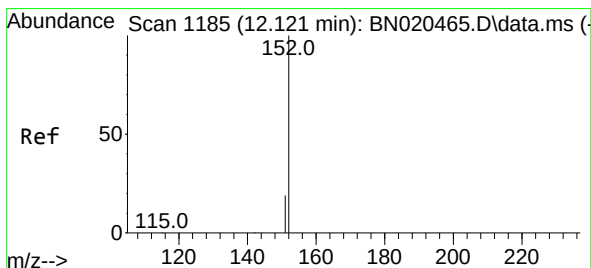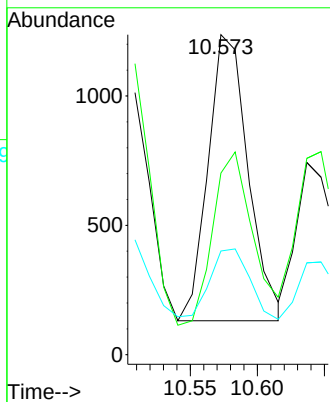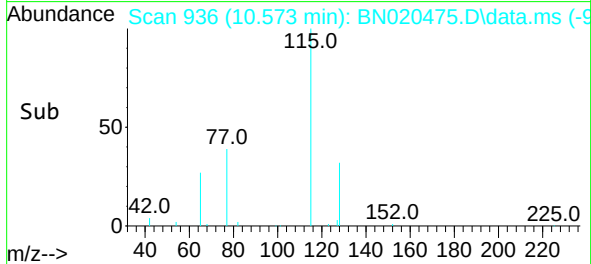

#11
2-Methylnaphthalene-d10
Concen: 0.356 ng
RT: 12.117 min Scan# 1184
Delta R.T. -0.004 min
Lab File: BN020475.D
Acq: 26 Jun 2022 21:18


Tgt Ion:152 Resp: 6019
Ion Ratio Lower Upper
152 100
151 23.4 16.2 24.4

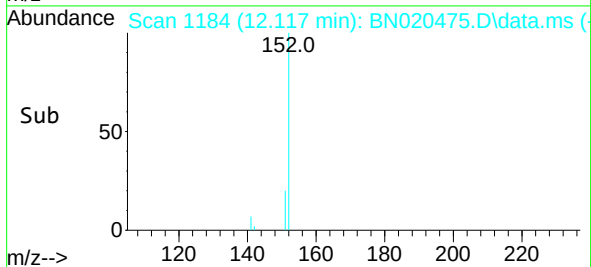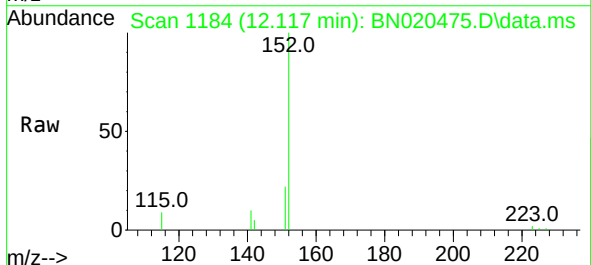



#12
2-Methylnaphthalene
Concen: 0.061 ng
RT: 12.189 min Scan# 1203
Delta R.T. -0.004 min
Lab File: BN020475.D
Acq: 26 Jun 2022 21:18




Instrument :
BNA_N
ClientSampleId :
MW-48




Tgt Ion:142 Resp: 119
Ion Ratio Lower Upper
142 100
141 102.9 71.6 107.4
115 107.2 29.8 44.8

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 06/28/2022
Supervised By :Jagrut Upadhyay 06/30/2022

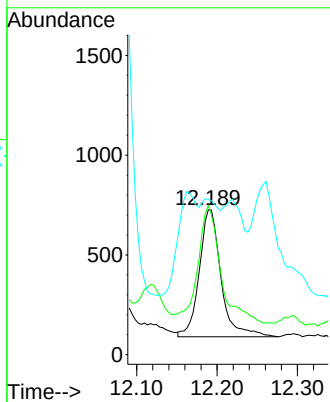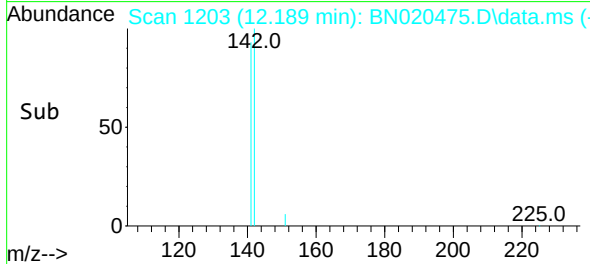


#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.367 min Scan# 1461
Delta R.T. -0.000 min
Lab File: BN020475.D
Acq: 26 Jun 2022 21:18

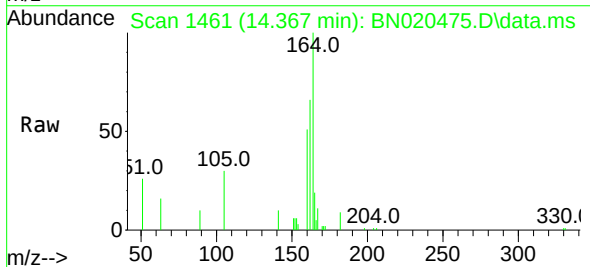


Tgt Ion:164 Resp: 11472
Ion Ratio Lower Upper
164 100
162 65.9 82.1 123.1#
160 50.6 38.6 58.0

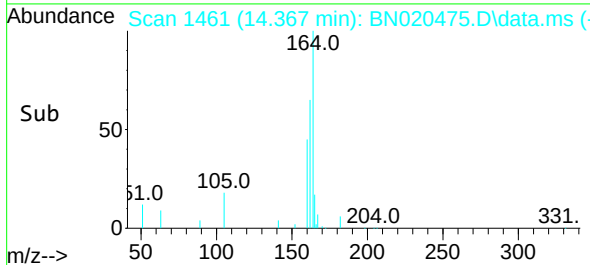



#14
2,4,6-Tribromophenol
Concen: 0.232 ng
RT: 15.861 min Scan# 1601
Delta R.T. -0.000 min
Lab File: BN020475.D
Acq: 26 Jun 2022 21:18




Instrument :
BNA_N
ClientSampleId :
MW-48




Tgt Ion: 330 Resp: 1004
Ion Ratio Lower Upper
330 100
332 132.1 77.6 116.4
141 100.2 41.0 61.4

Manual Integrations
APPROVED



Reviewed By : Christian Giraldo 06/28/2022
Supervised By : Jagrut Upadhyay 06/30/2022

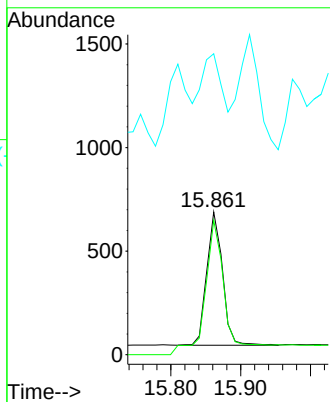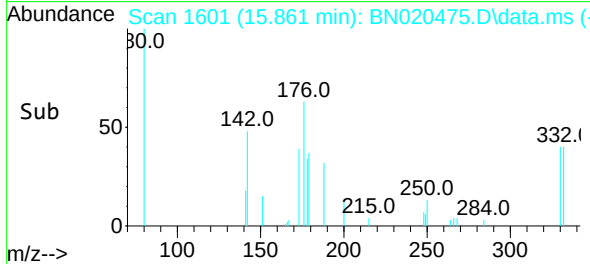


#15
2-Fluorobiphenyl
Concen: 0.153 ng
RT: 12.998 min Scan# 1333
Delta R.T. -0.000 min
Lab File: BN020475.D
Acq: 26 Jun 2022 21:18

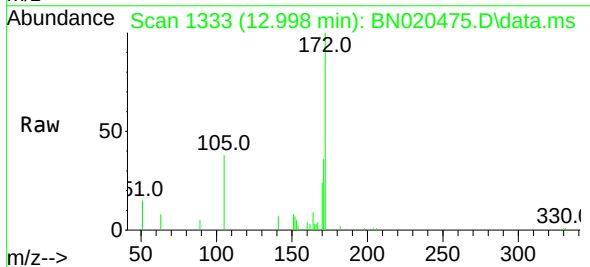


Tgt Ion: 172 Resp: 7256
Ion Ratio Lower Upper
172 100
171 35.6 27.2 40.8
170 23.6 18.2 27.4

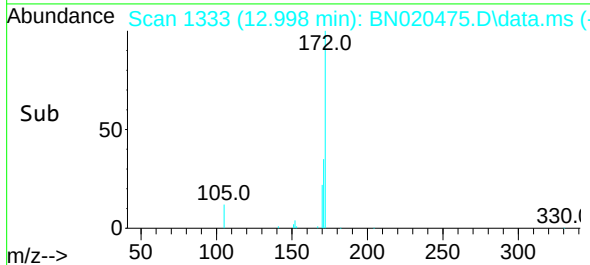



#16
Acenaphthylene
Concen: 0.100 ng
RT: 14.089 min Scan# 1435
Delta R.T. -0.000 min
Lab File: BN020475.D
Acq: 26 Jun 2022 21:18




Instrument :
BNA_N
ClientSampleId :
MW-48




Tgt Ion:152 Resp: 552
Ion Ratio Lower Upper
152 100
151 46.9 16.2 24.4
153 97.6 10.7 16.1

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 06/28/2022
Supervised By :Jagrut Upadhyay 06/30/2022

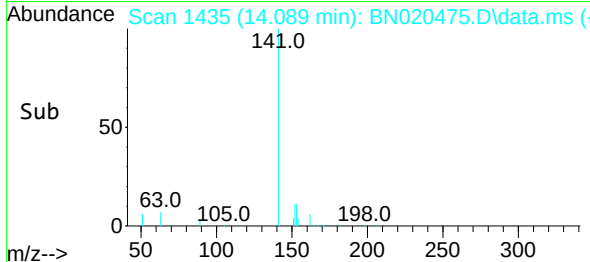


#17
Acenaphthene
Concen: 0.531 ng
RT: 14.431 min Scan# 1467
Delta R.T. -0.000 min
Lab File: BN020475.D
Acq: 26 Jun 2022 21:18

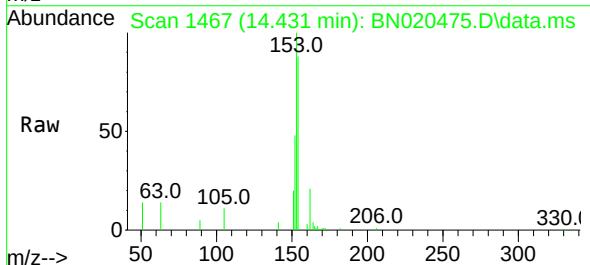


Tgt Ion:154 Resp: 19918
Ion Ratio Lower Upper
154 100
153 111.6 87.5 131.3
152 52.8 43.8 65.6

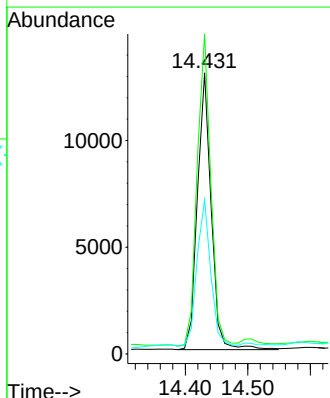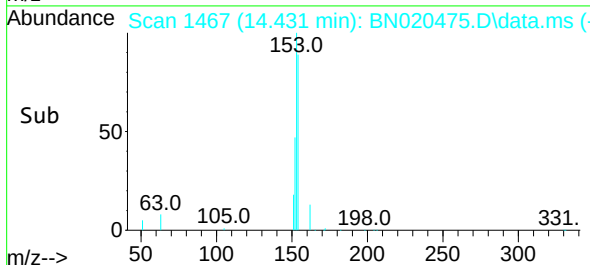



#18
Fluorene
Concen: 0.105 ng
RT: 15.414 min Scan# 1559
Delta R.T. -0.000 min
Lab File: BN020475.D
Acq: 26 Jun 2022 21:18




Instrument :
BNA_N
ClientSampleId :
MW-48



Tgt Ion:166 Resp: 516
Ion Ratio Lower Upper
166 100
165 102.1 78.6 118.0
167 26.0 10.8 16.2




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 06/28/2022
Supervised By :Jagrut Upadhyay 06/30/2022

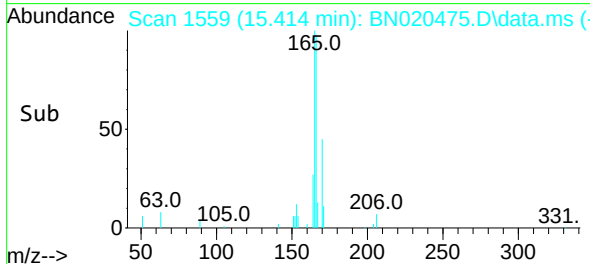

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.113 min Scan# 1723
Delta R.T. -0.000 min
Lab File: BN020475.D
Acq: 26 Jun 2022 21:18

Tgt Ion:188 Resp: 12327
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 27.3 7.4 11.2

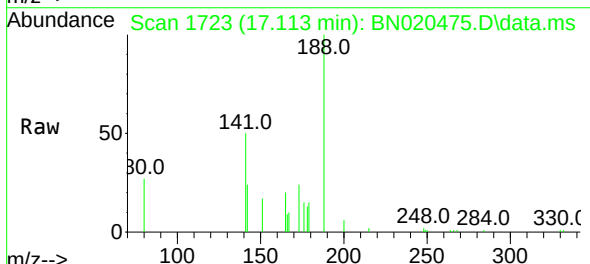







#25
Phenanthrene
Concen: 0.024 ng
RT: 17.154 min Scan# 1727
Delta R.T. -0.000 min
Lab File: BN020475.D
Acq: 26 Jun 2022 21:18

Instrument :
BNA_N
ClientSampleId :
MW-48

Tgt Ion:178 Resp: 100
Ion Ratio Lower Upper
178 100
176 0.0 15.3 22.9#
179 45.0 12.2 18.4#




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 06/28/2022
Supervised By :Jagrut Upadhyay 06/30/2022

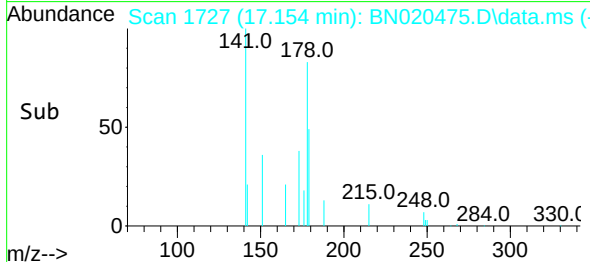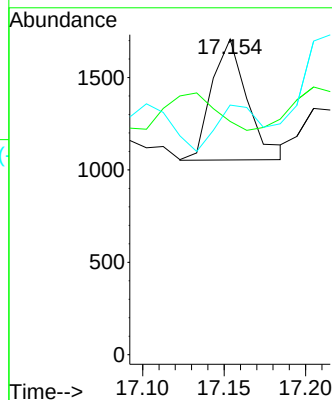

#26
Anthracene
Concen: 0.058 ng
RT: 17.246 min Scan# 1736
Delta R.T. -0.000 min
Lab File: BN020475.D
Acq: 26 Jun 2022 21:18


Tgt Ion:178 Resp: 2067
Ion Ratio Lower Upper
178 100
176 115.6 14.9 22.3#
179 0.0 12.2 18.4#

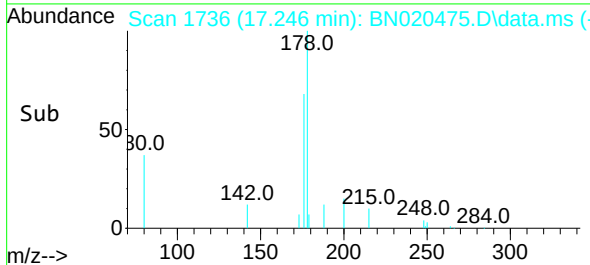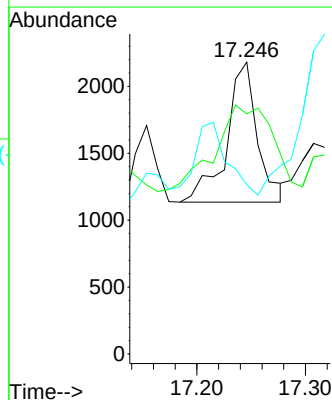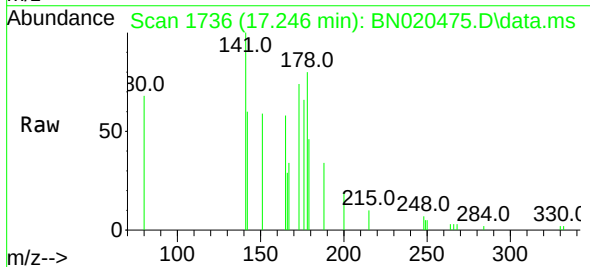



#27
Fluoranthene-d10
Concen: 0.357 ng
RT: 19.147 min Scan# 2081
Delta R.T. -0.000 min
Lab File: BN020475.D
Acq: 26 Jun 2022 21:18




Instrument :
BNA_N
ClientSampleId :
MW-48




Tgt Ion:212 Resp: 1306
Ion Ratio Lower Upper
212 100
106 16.7 12.6 19.0
104 8.6 7.2 10.8

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 06/28/2022
Supervised By :Jagrut Upadhyay 06/30/2022

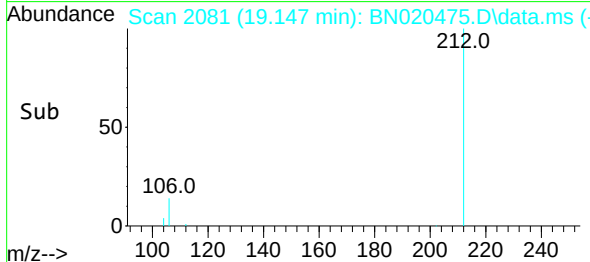


#28
Fluoranthene
Concen: 0.022 ng
RT: 19.177 min Scan# 2088
Delta R.T. -0.004 min
Lab File: BN020475.D
Acq: 26 Jun 2022 21:18

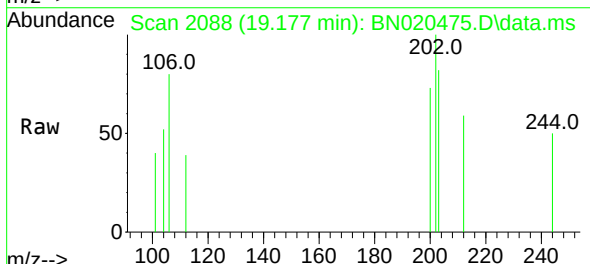


Tgt Ion:202 Resp: 1014
Ion Ratio Lower Upper
202 100
101 18.5 9.6 14.4#
203 23.5 13.5 20.3#

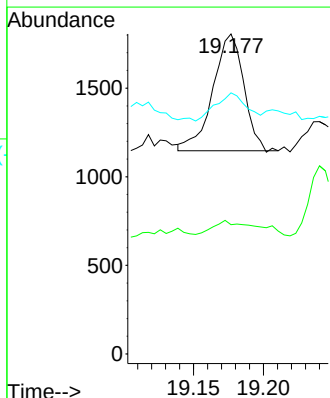



#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.306 min Scan# 2430
Delta R.T. -0.000 min
Lab File: BN020475.D
Acq: 26 Jun 2022 21:18




Instrument :
BNA_N
ClientSampleId :
MW-48




Tgt Ion:240 Resp: 10614
Ion Ratio Lower Upper
240 100
120 17.6 14.6 21.8
236 29.0 22.6 33.8

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 06/28/2022
Supervised By :Jagrut Upadhyay 06/30/2022

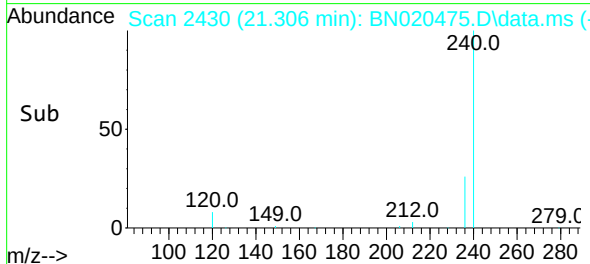


#30
Pyrene
Concen: 0.039 ng m
RT: 19.539 min Scan# 2174
Delta R.T. -0.004 min
Lab File: BN020475.D
Acq: 26 Jun 2022 21:18

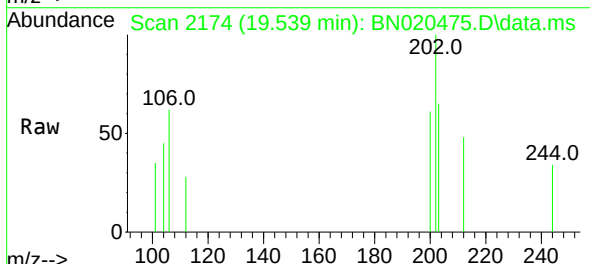


Tgt Ion:202 Resp: 1775
Ion Ratio Lower Upper
202 100
200 16.4 16.6 25.0#
203 16.3 14.2 21.2

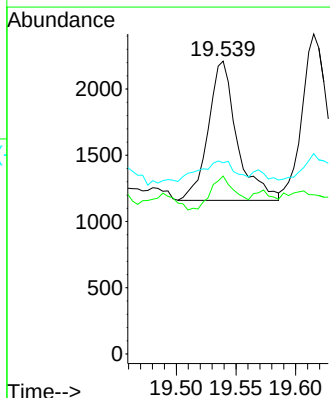



#31
 Terphenyl-d14
 Concen: 0.407 ng
 RT: 19.746 min Scan# 21
 Delta R.T. -0.009 min
 Lab File: BN020475.D
 Acq: 26 Jun 2022 21:18




Instrument :
 BNA_N
 ClientSampleId :
 MW-48




Tgt Ion:244 Resp: 10310
 Ion Ratio Lower Upper
 244 100
 212 18.7 7.1 10.7
 122 0.0 0.0 0.0

Manual Integrations
 APPROVED



Reviewed By :Christian Giraldo 06/28/2022
 Supervised By :Jagrut Upadhyay 06/30/2022

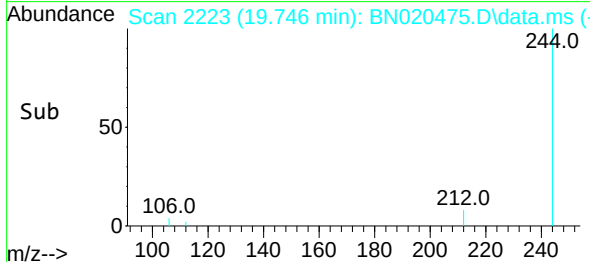


#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.084 ng
 RT: 21.225 min Scan# 2421
 Delta R.T. -0.009 min
 Lab File: BN020475.D
 Acq: 26 Jun 2022 21:18

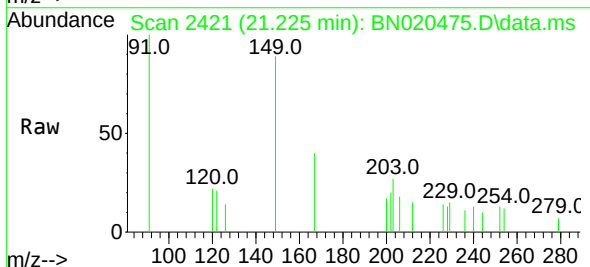


Tgt Ion:149 Resp: 1789
 Ion Ratio Lower Upper
 149 100
 167 34.8 21.7 32.5
 279 2.9 2.2 3.2

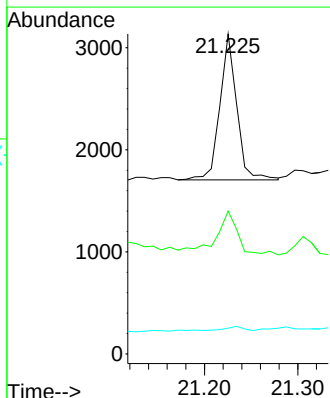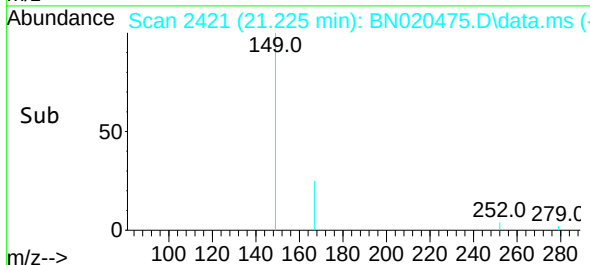

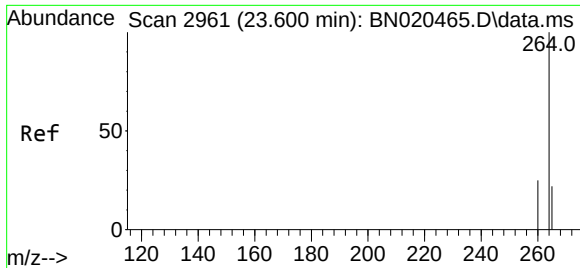

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.583 min Scan# 2961
 Delta R.T. -0.018 min
 Lab File: BN020475.D
 Acq: 26 Jun 2022 21:18

Instrument :
 BNA_N
 ClientSampleId :
 MW-48

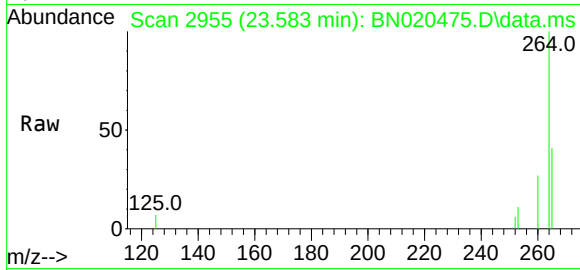

Tgt Ion:264 Resp: 9494

Ion	Ratio	Lower	Upper
264	100		
260	27.0	20.9	31.3
265	41.3	28.0	42.0

Manual Integrations
 APPROVED

Reviewed By :Christian Giraldo 06/28/2022
 Supervised By :Jagrut Upadhyay 06/30/2022

