

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062622\
 Data File : BN020499.D
 Acq On : 27 Jun 2022 14:13
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Quant Time: Jun 28 00:34:20 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 27 02:03:21 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.739	152	3203	0.400	ng	0.00
7) Naphthalene-d8	10.519	136	10336	0.400	ng	# 0.00
13) Acenaphthene-d10	14.367	164	6575	0.400	ng	0.00
19) Phenanthrene-d10	17.113	188	14181	0.400	ng	0.00
29) Chrysene-d12	21.306	240	11622	0.400	ng	# 0.00
35) Perylene-d12	23.586	264	9212	0.400	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.348	112	3727	0.419	ng	0.00
5) Phenol-d6	6.944	99	4667	0.439	ng	0.00
8) Nitrobenzene-d5	8.897	82	3252	0.388	ng	0.00
11) 2-Methylnaphthalene-d10	12.117	152	7165	0.404	ng	0.00
14) 2,4,6-Tribromophenol	15.861	330	979	0.395	ng	0.00
15) 2-Fluorobiphenyl	12.998	172	10376	0.382	ng	0.00
27) Fluoranthene-d10	19.147	212	15713	0.373	ng	0.00
31) Terphenyl-d14	19.746	244	11159	0.402	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.232	88	1659	0.395	ng	95
3) n-Nitrosodimethylamine	3.564	42	1411	0.369	ng	# 91
6) bis(2-Chloroethyl)ether	7.168	93	3689	0.404	ng	98
9) Naphthalene	10.573	128	12208	0.395	ng	99
10) Hexachlorobutadiene	10.872	225	2214	0.394	ng	# 100
12) 2-Methylnaphthalene	12.193	142	8290	0.404	ng	100
16) Acenaphthylene	14.089	152	12162	0.385	ng	99
17) Acenaphthene	14.431	154	8377	0.390	ng	97
18) Fluorene	15.414	166	10912	0.389	ng	100
20) 4,6-Dinitro-2-methylph...	15.511	198	709	0.480	ng	# 82
21) 4-Bromophenyl-phenylether	16.313	248	3047	0.370	ng	# 83
22) Hexachlorobenzene	16.425	284	3360	0.368	ng	99
23) Atrazine	16.579	200	2322	0.357	ng	96
24) Pentachlorophenol	16.784	266	1058	0.545	ng	99
25) Phenanthrene	17.154	178	17708	0.370	ng	100
26) Anthracene	17.246	178	15277	0.371	ng	99
28) Fluoranthene	19.177	202	19453	0.373	ng	100
30) Pyrene	19.539	202	19994	0.406	ng	100
32) Benzo(a)anthracene	21.288	228	16206	0.390	ng	98
33) Chrysene	21.342	228	17751	0.386	ng	99
34) Bis(2-ethylhexyl)phtha...	21.225	149	9944	0.425	ng	99
36) Indeno(1,2,3-cd)pyrene	25.916	276	13422	0.327	ng	99
37) Benzo(b)fluoranthene	22.896	252	14396	0.406	ng	94
38) Benzo(k)fluoranthene	22.942	252	14549	0.385	ng	96
39) Benzo(a)pyrene	23.483	252	11986	0.389	ng	# 93
40) Dibenzo(a,h)anthracene	25.936	278	10348	0.314	ng	96
41) Benzo(g,h,i)perylene	26.629	276	11514	0.320	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062622\
Data File : BN020499.D
Acq On : 27 Jun 2022 14:13
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Quant Time: Jun 28 00:34:20 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 02:03:21 2022
Response via : Initial Calibration

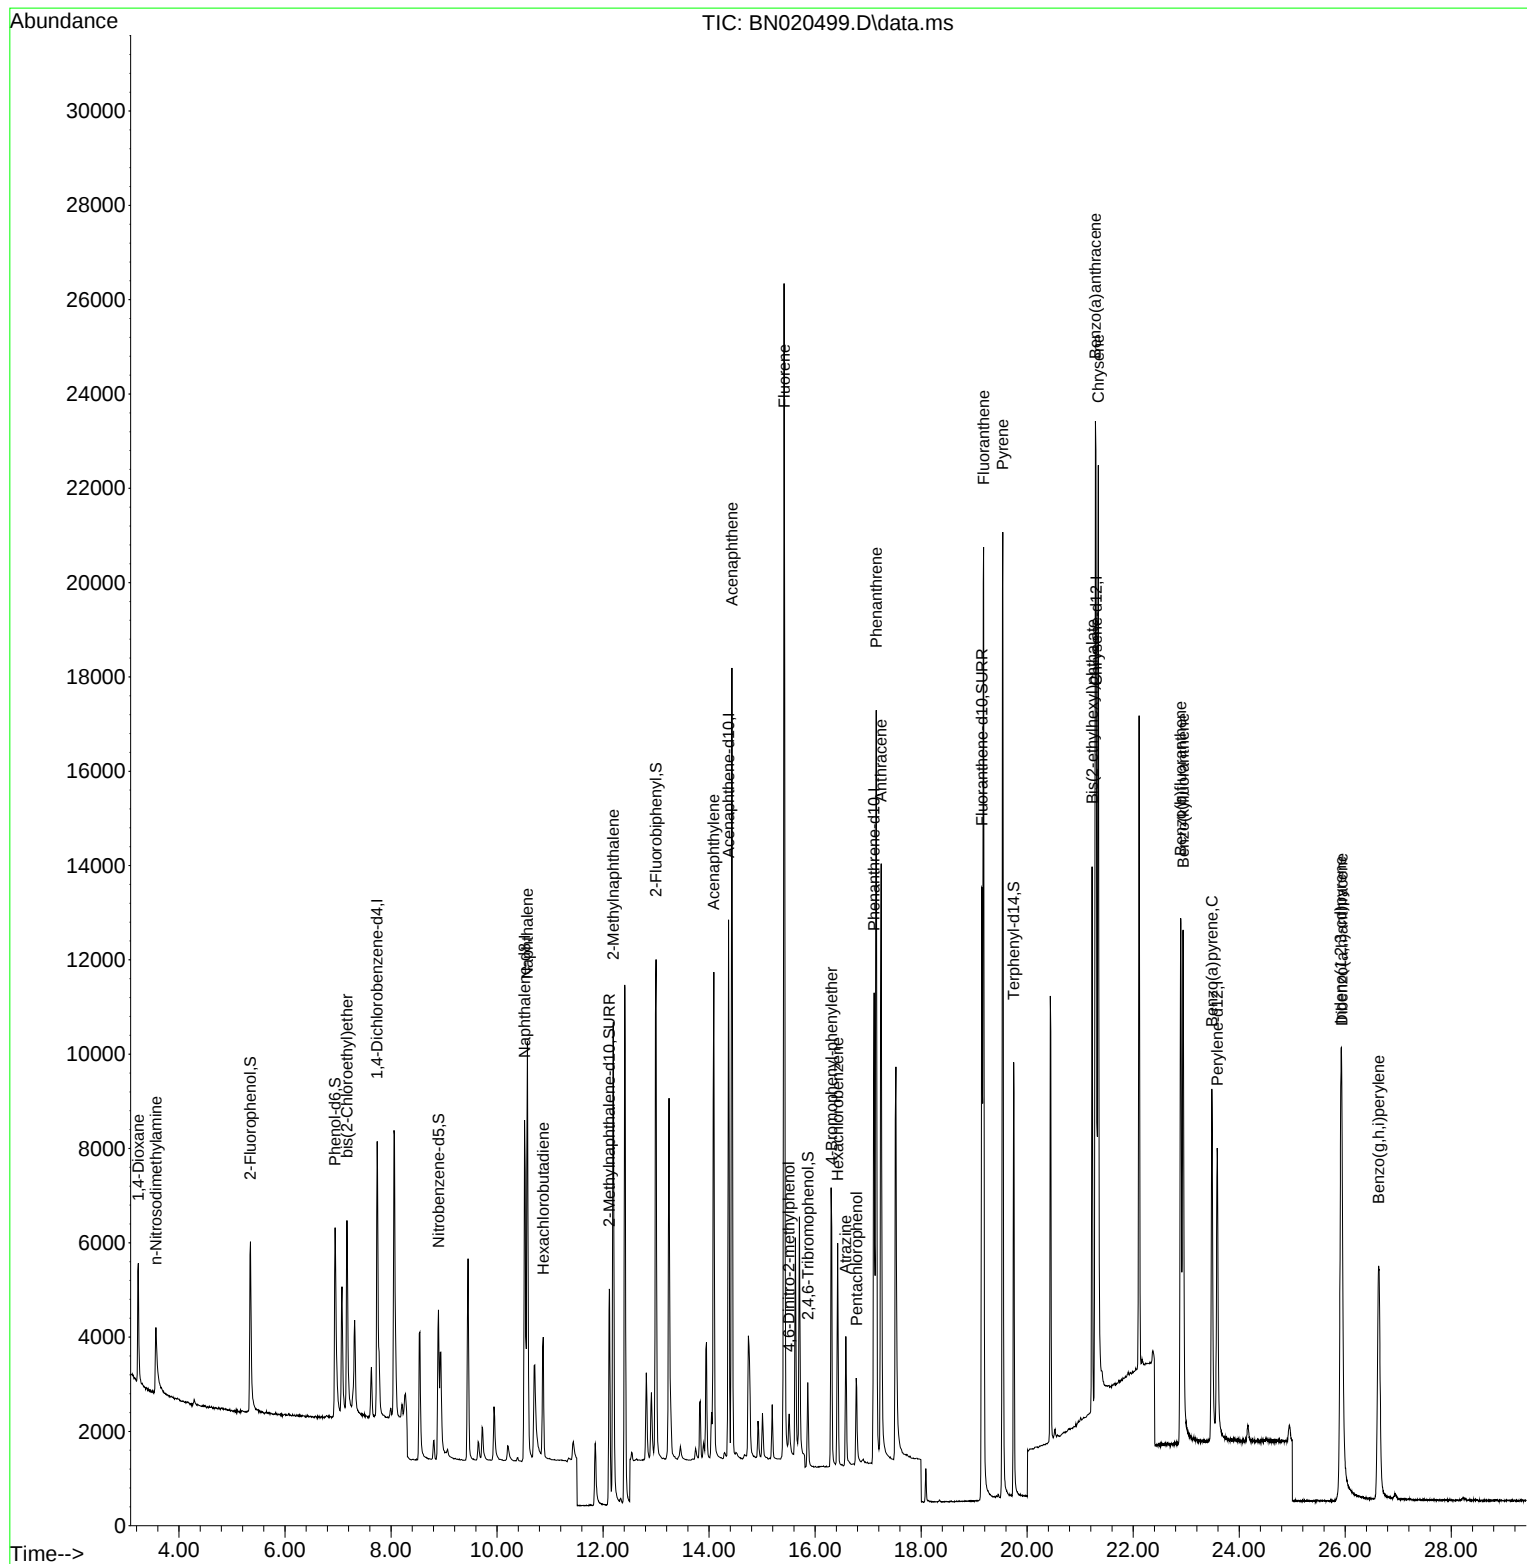






#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.739 min Scan# 64
 Delta R.T. -0.000 min
 Lab File: BN020499.D
 Acq: 27 Jun 2022 14:13

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC







Tgt Ion:152 Resp: 3203
 Ion Ratio Lower Upper
 152 100
 150 155.2 127.9 191.9
 115 65.4 51.4 77.2

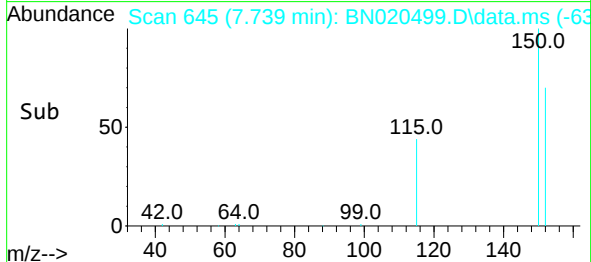

#2
 1,4-Dioxane
 Concen: 0.395 ng
 RT: 3.232 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BN020499.D
 Acq: 27 Jun 2022 14:13

Tgt Ion: 88 Resp: 1659
 Ion Ratio Lower Upper
 88 100
 43 34.1 30.2 45.2
 58 87.3 73.0 109.6


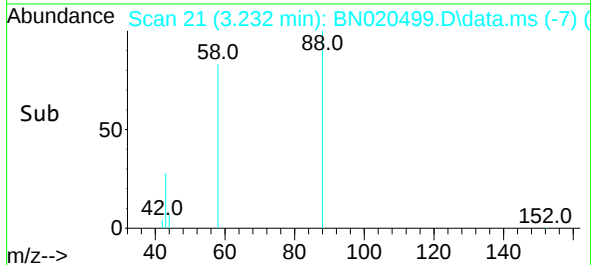

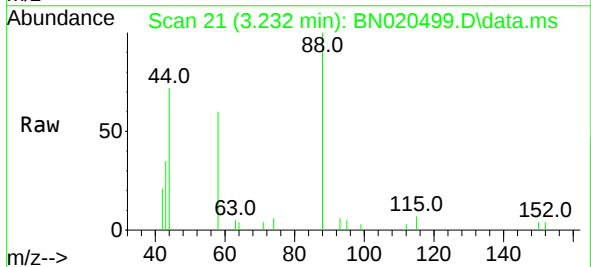


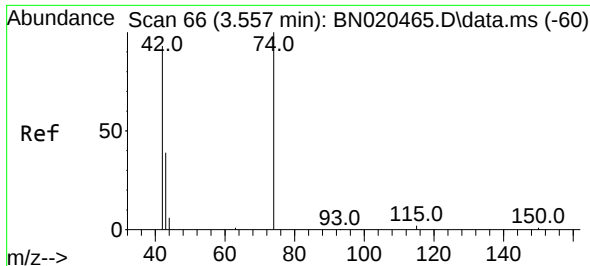

#3
 n-Nitrosodimethylamine
 Concen: 0.369 ng
 RT: 3.564 min Scan# 61
 Delta R.T. 0.007 min
 Lab File: BN020499.D
 Acq: 27 Jun 2022 14:13




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC


Tgt Ion: 42 Resp: 1411
 Ion Ratio Lower Upper
 42 100
 74 112.5 84.0 126.0
 44 4.5 9.8 14.8#

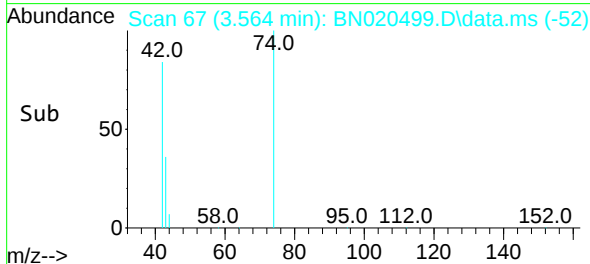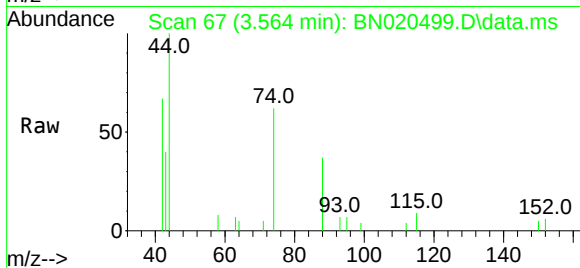

#4
 2-Fluorophenol
 Concen: 0.419 ng
 RT: 5.348 min Scan# 314
 Delta R.T. -0.000 min
 Lab File: BN020499.D
 Acq: 27 Jun 2022 14:13


Tgt Ion: 112 Resp: 3727
 Ion Ratio Lower Upper
 112 100
 64 61.3 49.1 73.7
 63 32.8 26.3 39.5

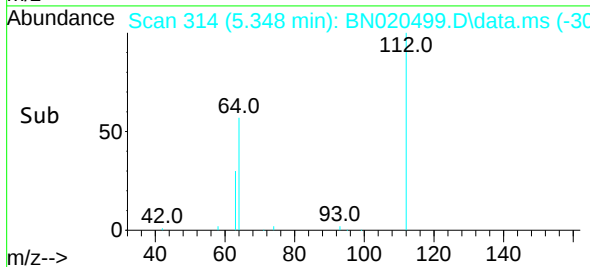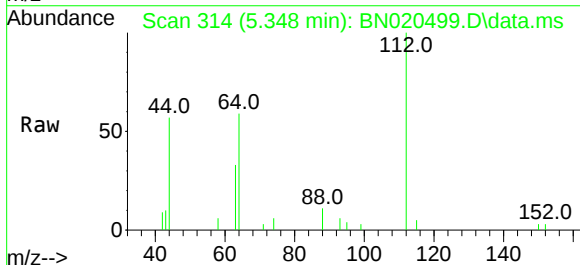






#5
Phenol-d6
Concen: 0.439 ng
RT: 6.944 min Scan# 511
Delta R.T. -0.000 min
Lab File: BN020499.D
Acq: 27 Jun 2022 14:13

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC



Tgt Ion: 99 Resp: 4667




Ion	Ratio	Lower	Upper
99	100		
42	21.6	19.3	28.9
71	35.2	27.5	41.3

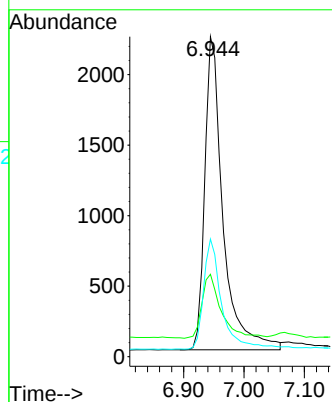


#6
bis(2-Chloroethyl)ether
Concen: 0.404 ng
RT: 7.168 min Scan# 566
Delta R.T. -0.000 min
Lab File: BN020499.D
Acq: 27 Jun 2022 14:13

Tgt Ion: 93 Resp: 3689

Ion	Ratio	Lower	Upper
93	100		
63	82.7	67.4	101.0
95	34.1	26.5	39.7


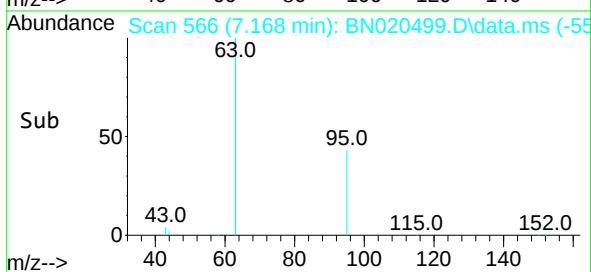
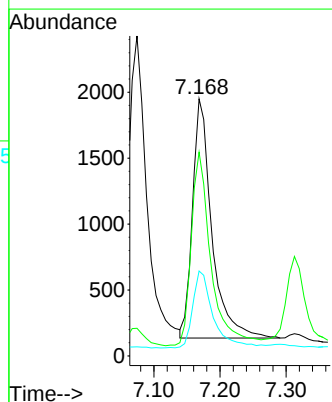





#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.519 min Scan# 91
Delta R.T. -0.000 min
Lab File: BN020499.D
Acq: 27 Jun 2022 14:13




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:	136	Resp:	10336
Ion Ratio	Lower	Upper	
136	100		
137	11.6	9.0	13.6
54	11.4	6.2	9.2#
68	7.4	4.4	6.6#

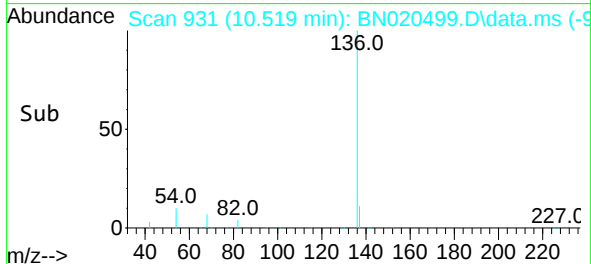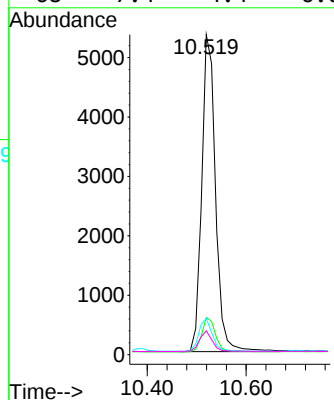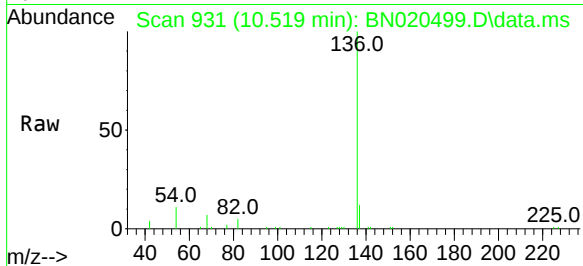

#8
Nitrobenzene-d5
Concen: 0.388 ng
RT: 8.897 min Scan# 779
Delta R.T. -0.000 min
Lab File: BN020499.D
Acq: 27 Jun 2022 14:13

Tgt Ion:	82	Resp:	3252
Ion Ratio	Lower	Upper	
82	100		
128	44.4	35.0	52.6
54	54.8	46.2	69.4


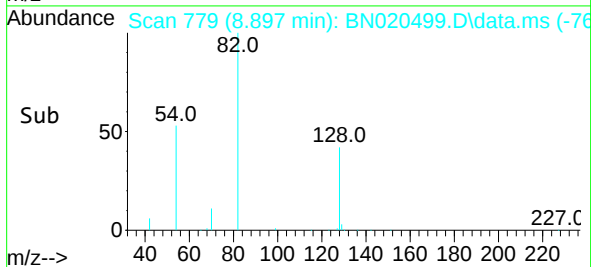
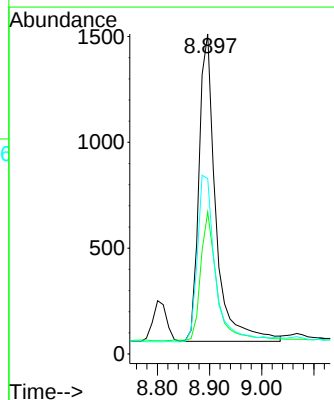
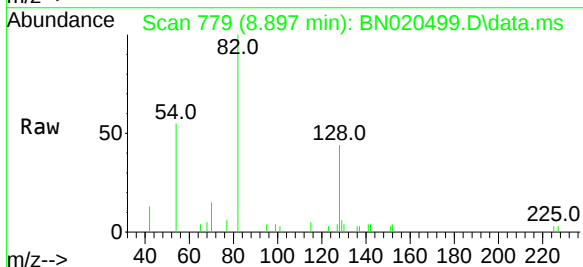


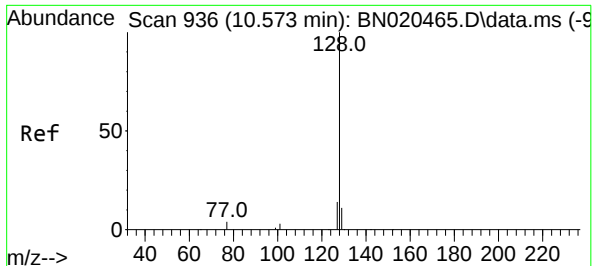

#9
Naphthalene
Concen: 0.395 ng
RT: 10.573 min Scan# 91
Delta R.T. -0.000 min
Lab File: BN020499.D
Acq: 27 Jun 2022 14:13




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:128 Resp: 12208
Ion Ratio Lower Upper
128 100
129 11.6 8.9 13.3
127 13.7 10.8 16.2

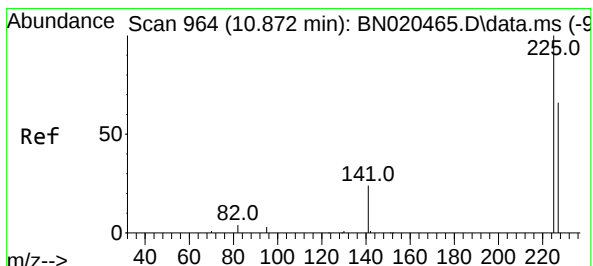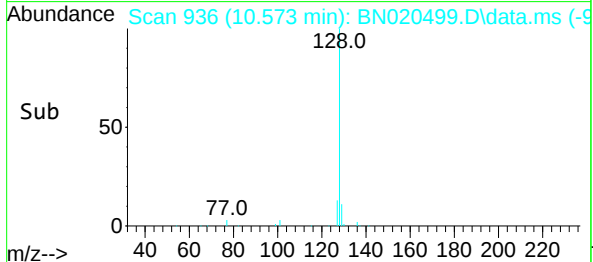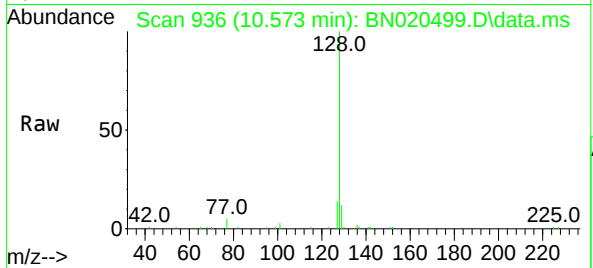

#10
Hexachlorobutadiene
Concen: 0.394 ng
RT: 10.872 min Scan# 964
Delta R.T. -0.000 min
Lab File: BN020499.D
Acq: 27 Jun 2022 14:13

Tgt Ion:225 Resp: 2214
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.9 50.9 76.3


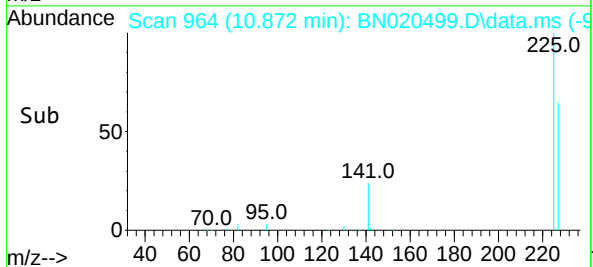

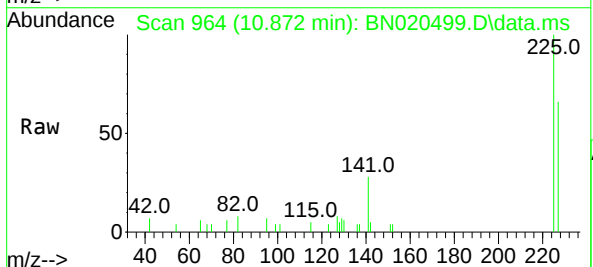




#11
2-Methylnaphthalene-d10
Concen: 0.404 ng
RT: 12.117 min Scan# 1185
Delta R.T. -0.004 min
Lab File: BN020499.D
Acq: 27 Jun 2022 14:13




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:152 Resp: 7165
Ion Ratio Lower Upper
152 100
151 20.3 16.2 24.4

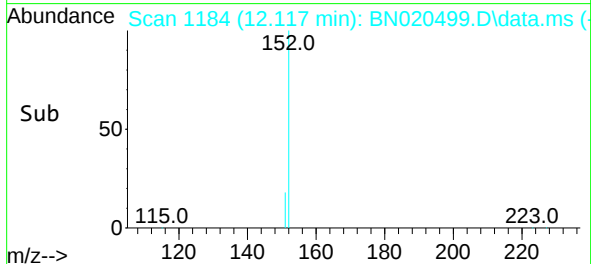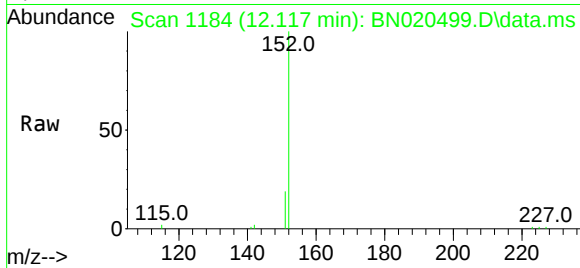

#12
2-Methylnaphthalene
Concen: 0.404 ng
RT: 12.193 min Scan# 1204
Delta R.T. -0.000 min
Lab File: BN020499.D
Acq: 27 Jun 2022 14:13

Tgt Ion:142 Resp: 8290
Ion Ratio Lower Upper
142 100
141 88.9 71.6 107.4
115 37.4 29.8 44.8

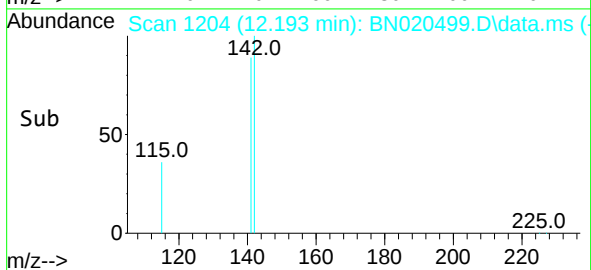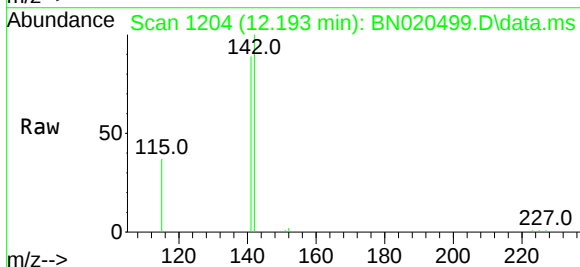



#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.367 min Scan# 1461

Delta R.T. -0.000 min

Lab File: BN020499.D

Acq: 27 Jun 2022 14:13

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion:164 Resp: 6575

Ion Ratio Lower Upper

164 100

162 104.3 82.1 123.1

160 48.0 38.6 58.0

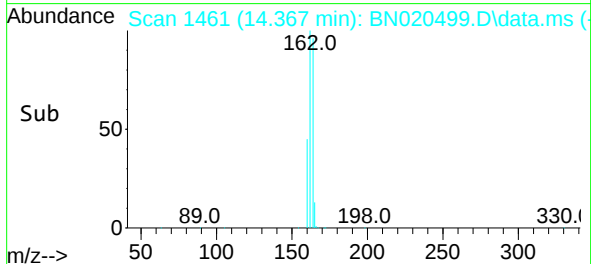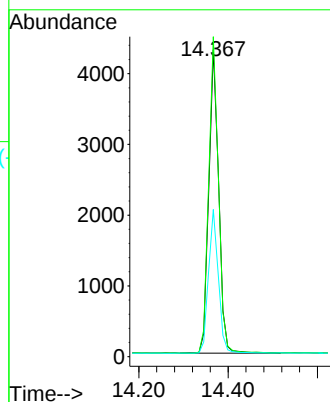

#14

2,4,6-Tribromophenol

Concen: 0.395 ng

RT: 15.861 min Scan# 1601

Delta R.T. -0.000 min

Lab File: BN020499.D

Acq: 27 Jun 2022 14:13




Tgt Ion:330 Resp: 979


Ion Ratio Lower Upper

330 100

332 144.3 77.6 116.4#

141 56.4 41.0 61.4


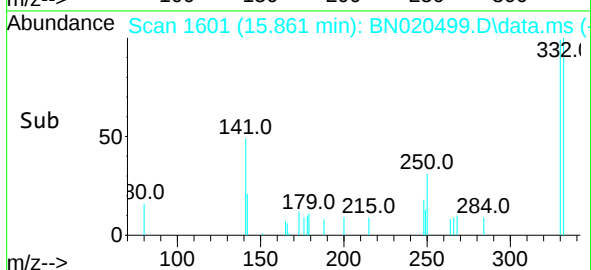
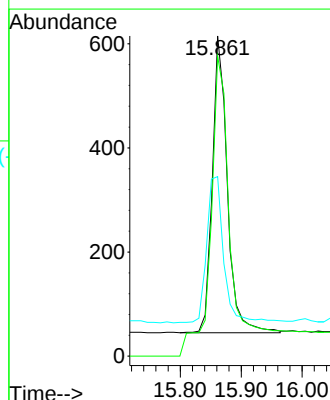





#15
2-Fluorobiphenyl
Concen: 0.382 ng
RT: 12.998 min Scan# 1333
Delta R.T. -0.000 min
Lab File: BN020499.D
Acq: 27 Jun 2022 14:13




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:	172	Resp:	10376
Ion Ratio	Lower	Upper	
172	100		
171	34.9	27.2	40.8
170	23.0	18.2	27.4

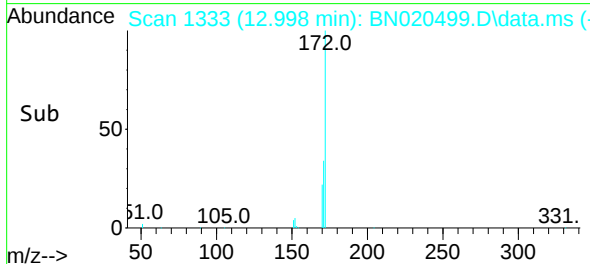

#16
Acenaphthylene
Concen: 0.385 ng
RT: 14.089 min Scan# 1435
Delta R.T. -0.000 min
Lab File: BN020499.D
Acq: 27 Jun 2022 14:13

Tgt Ion:	152	Resp:	12162
Ion Ratio	Lower	Upper	
152	100		
151	19.6	16.2	24.4
153	13.2	10.7	16.1


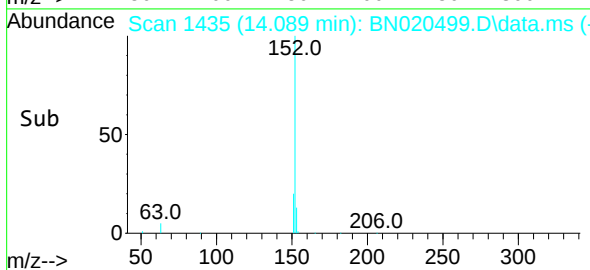

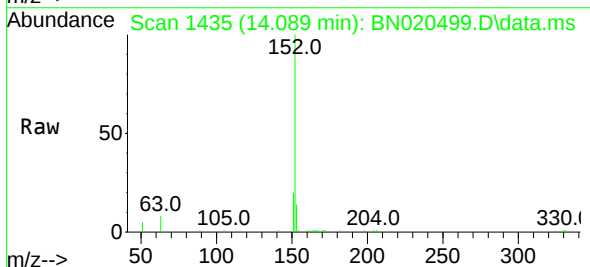




#17
Acenaphthene
Concen: 0.390 ng
RT: 14.431 min Scan# 1467
Delta R.T. -0.000 min
Lab File: BN020499.D
Acq: 27 Jun 2022 14:13




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:154 Resp: 8377
Ion Ratio Lower Upper
154 100
153 114.0 87.5 131.3
152 55.0 43.8 65.6

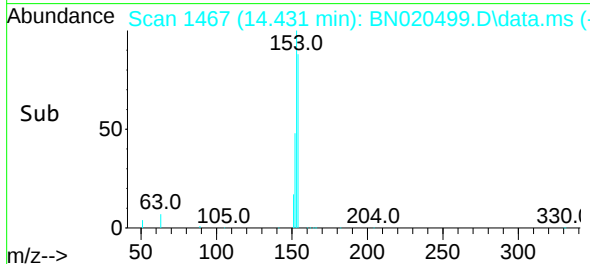

#18
Fluorene
Concen: 0.389 ng
RT: 15.414 min Scan# 1559
Delta R.T. -0.000 min
Lab File: BN020499.D
Acq: 27 Jun 2022 14:13

Tgt Ion:166 Resp: 10912
Ion Ratio Lower Upper
166 100
165 98.0 78.6 118.0
167 13.3 10.8 16.2

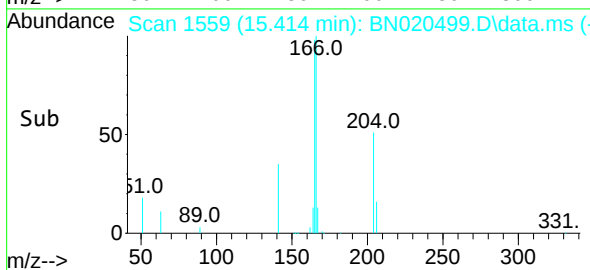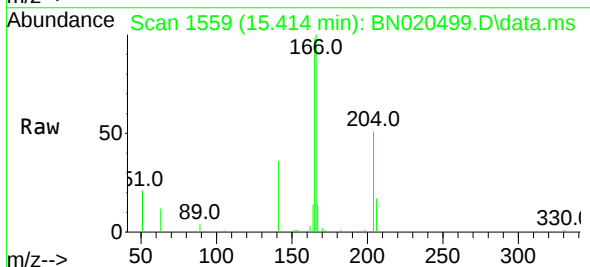



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.113 min Scan# 1723

Delta R.T. -0.000 min

Lab File: BN020499.D

Acq: 27 Jun 2022 14:13

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion:188 Resp: 14181

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 9.6 7.4 11.2

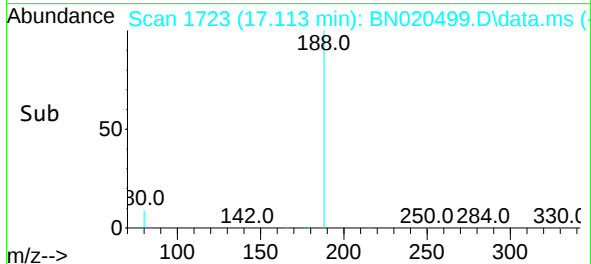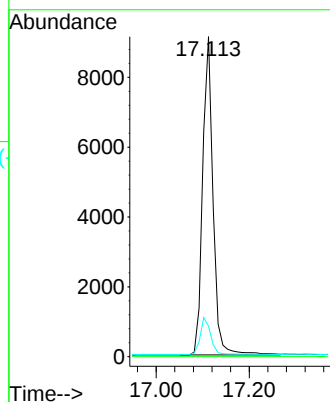

#20

4,6-Dinitro-2-methylphenol

Concen: 0.480 ng

RT: 15.511 min Scan# 1568

Delta R.T. -0.000 min

Lab File: BN020499.D

Acq: 27 Jun 2022 14:13




Tgt Ion:198 Resp: 709


Ion Ratio Lower Upper

198 100

182 22.8 12.1 18.1#

77 0.0 0.0 0.0


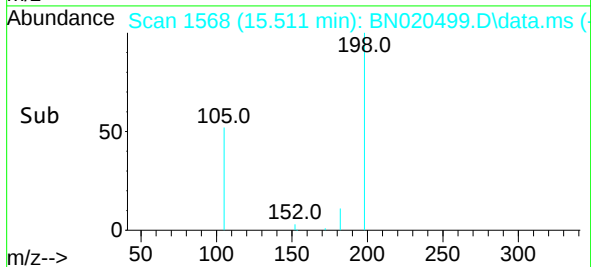
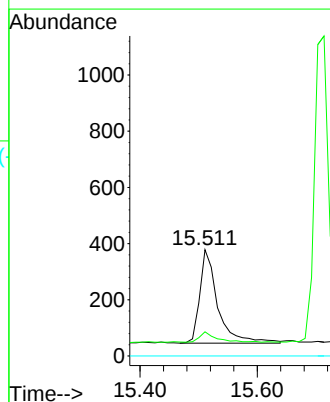
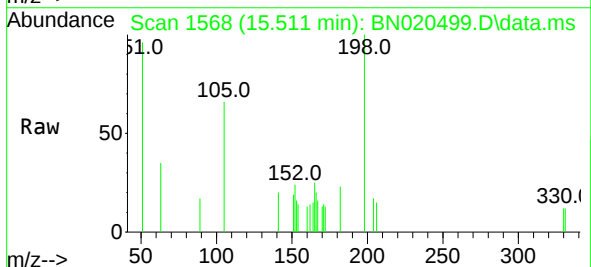


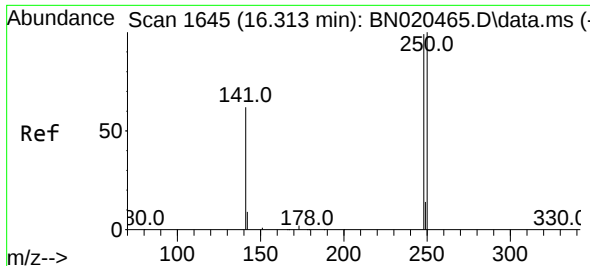

#21
4-Bromophenyl-phenylether
Concen: 0.370 ng
RT: 16.313 min Scan# 1645
Delta R.T. -0.000 min
Lab File: BN020499.D
Acq: 27 Jun 2022 14:13




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:248 Resp: 3047
Ion Ratio Lower Upper
248 100
250 101.1 75.3 112.9
141 58.8 67.3 100.9#

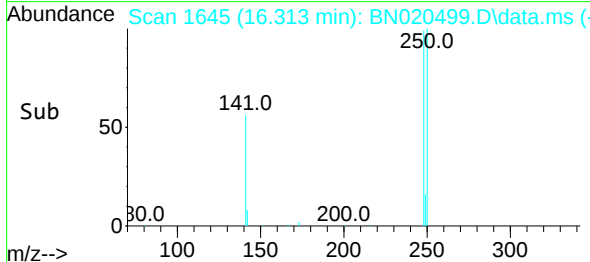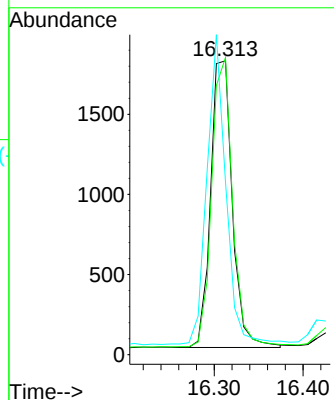

#22
Hexachlorobenzene
Concen: 0.368 ng
RT: 16.425 min Scan# 1656
Delta R.T. -0.000 min
Lab File: BN020499.D
Acq: 27 Jun 2022 14:13

Tgt Ion:284 Resp: 3360
Ion Ratio Lower Upper
284 100
142 43.6 35.2 52.8
249 34.6 26.6 40.0


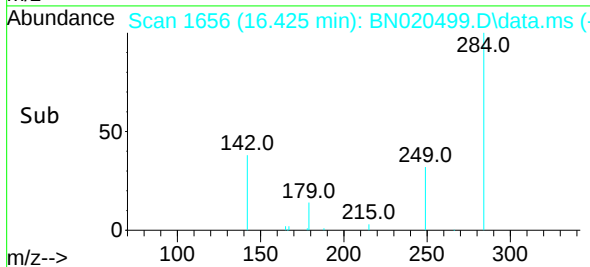
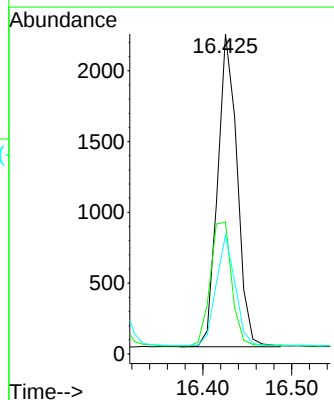
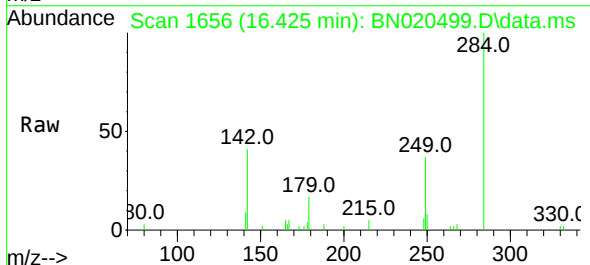




#23
 Atrazine
 Concen: 0.357 ng
 RT: 16.579 min Scan# 1671
 Delta R.T. -0.000 min
 Lab File: BN020499.D
 Acq: 27 Jun 2022 14:13




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC


Tgt Ion:	200	Resp:	2322
Ion Ratio	Lower	Upper	
200	100		
173	32.8	23.6	35.4
215	46.9	36.6	54.8

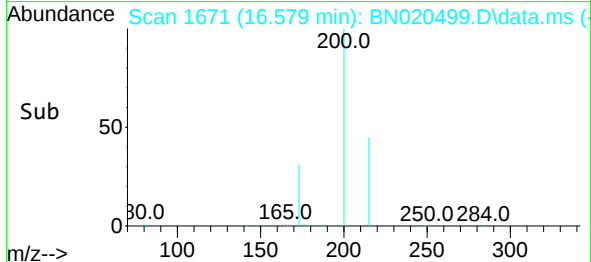

#24
 Pentachlorophenol
 Concen: 0.545 ng
 RT: 16.784 min Scan# 1691
 Delta R.T. 0.000 min
 Lab File: BN020499.D
 Acq: 27 Jun 2022 14:13

Tgt Ion:	266	Resp:	1058
Ion Ratio	Lower	Upper	
266	100		
264	63.3	51.3	76.9
268	64.6	52.6	79.0


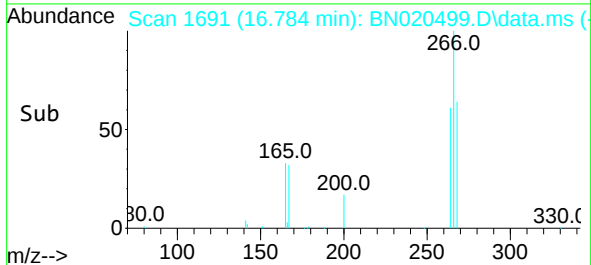

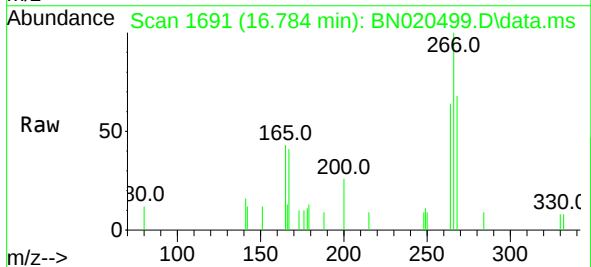




#25
Phenanthrene
Concen: 0.370 ng
RT: 17.154 min Scan# 1727
Delta R.T. -0.000 min
Lab File: BN020499.D
Acq: 27 Jun 2022 14:13




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:178 Resp: 17708
Ion Ratio Lower Upper
178 100
176 18.9 15.3 22.9
179 15.5 12.2 18.4

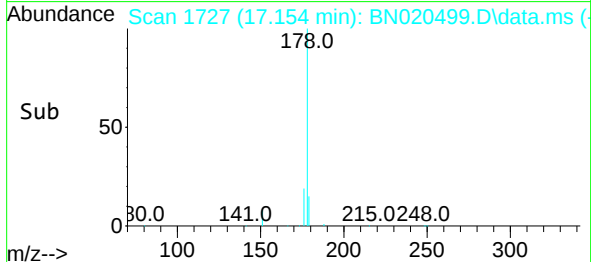

#26
Anthracene
Concen: 0.371 ng
RT: 17.246 min Scan# 1736
Delta R.T. -0.000 min
Lab File: BN020499.D
Acq: 27 Jun 2022 14:13

Tgt Ion:178 Resp: 15277
Ion Ratio Lower Upper
178 100
176 18.6 14.9 22.3
179 14.7 12.2 18.4


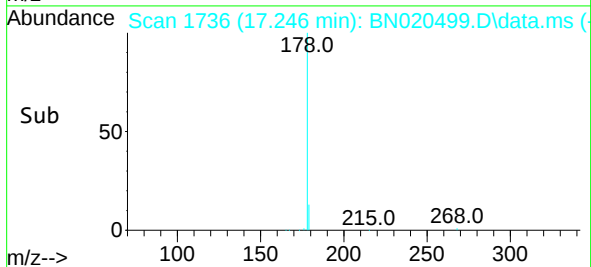

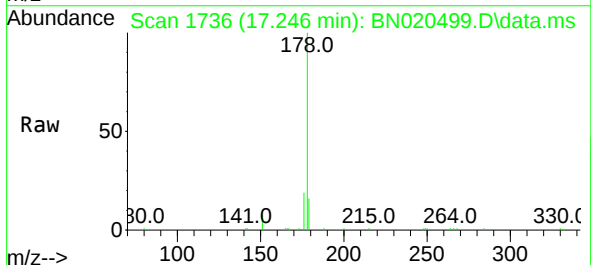


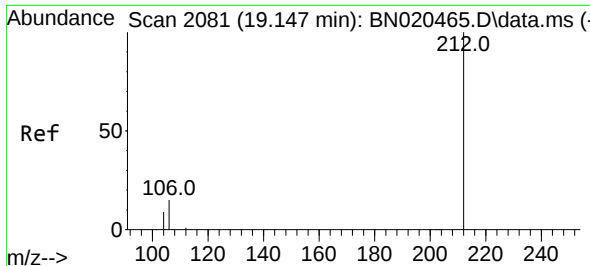

#27
Fluoranthene-d10
Concen: 0.373 ng
RT: 19.147 min Scan# 2081
Delta R.T. -0.000 min
Lab File: BN020499.D
Acq: 27 Jun 2022 14:13




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:212 Resp: 15713
Ion Ratio Lower Upper
212 100
106 15.1 12.6 19.0
104 8.5 7.2 10.8

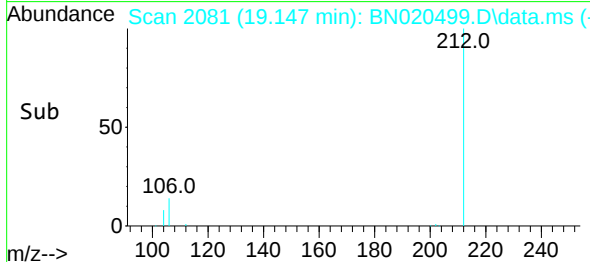

#28
Fluoranthene
Concen: 0.373 ng
RT: 19.177 min Scan# 2088
Delta R.T. -0.004 min
Lab File: BN020499.D
Acq: 27 Jun 2022 14:13

Tgt Ion:202 Resp: 19453
Ion Ratio Lower Upper
202 100
101 12.2 9.6 14.4
203 16.8 13.5 20.3


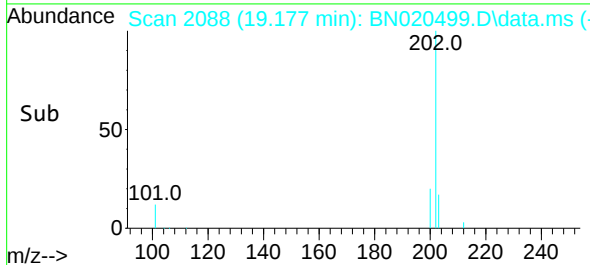

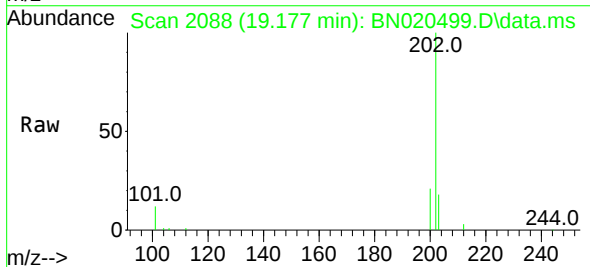




#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.306 min Scan# 2430
Delta R.T. -0.000 min
Lab File: BN020499.D
Acq: 27 Jun 2022 14:13




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:240 Resp: 11622
Ion Ratio Lower Upper
240 100
120 11.5 14.6 21.8#
236 27.1 22.6 33.8

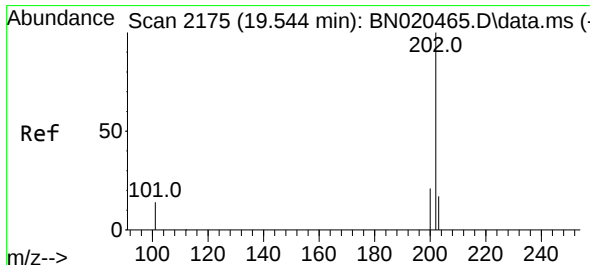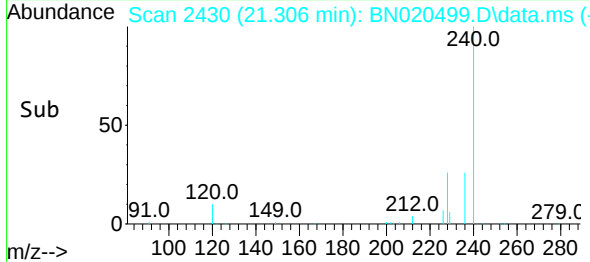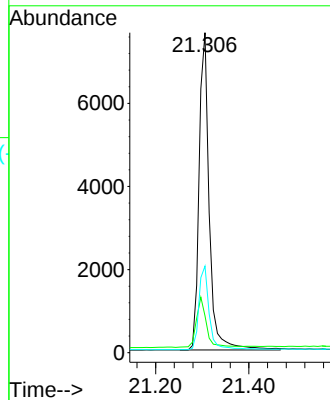

#30
Pyrene
Concen: 0.406 ng
RT: 19.539 min Scan# 2174
Delta R.T. -0.004 min
Lab File: BN020499.D
Acq: 27 Jun 2022 14:13

Tgt Ion:202 Resp: 19994
Ion Ratio Lower Upper
202 100
200 20.6 16.6 25.0
203 17.6 14.2 21.2


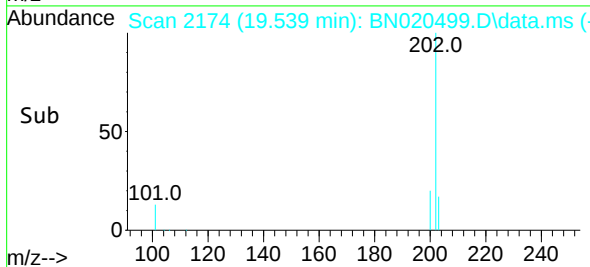
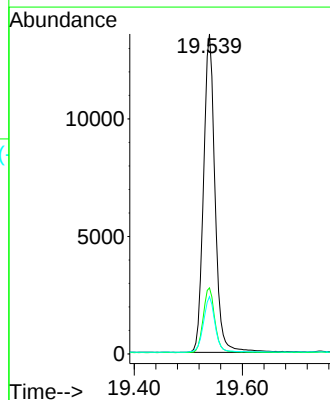
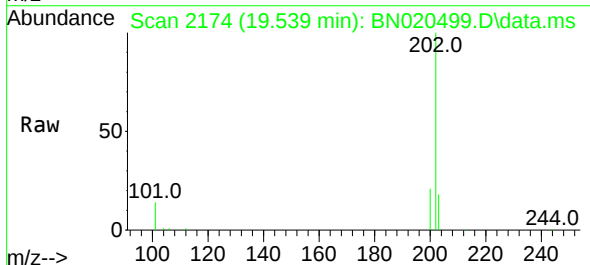




#31
 Terphenyl-d14
 Concen: 0.402 ng
 RT: 19.746 min Scan# 21159
 Delta R.T. -0.009 min
 Lab File: BN020499.D
 Acq: 27 Jun 2022 14:13




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC


Tgt Ion:244 Resp: 11159
 Ion Ratio Lower Upper
 244 100
 212 9.4 7.1 10.7
 122 0.0 0.0 0.0

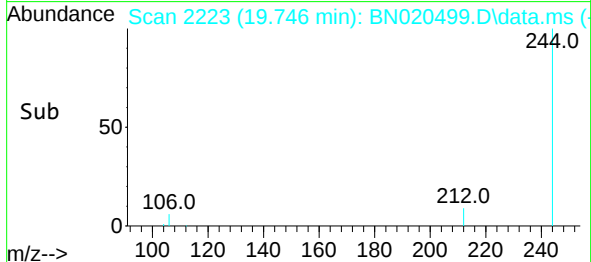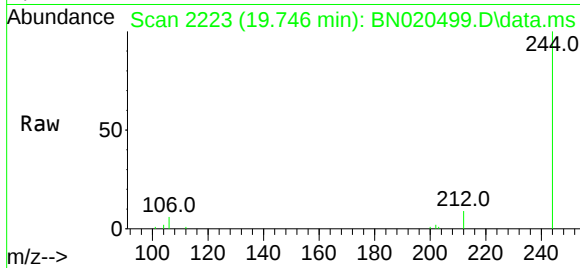

#32
 Benzo(a)anthracene
 Concen: 0.390 ng
 RT: 21.288 min Scan# 2428
 Delta R.T. -0.009 min
 Lab File: BN020499.D
 Acq: 27 Jun 2022 14:13

Tgt Ion:228 Resp: 16206
 Ion Ratio Lower Upper
 228 100
 226 27.5 21.2 31.8
 229 20.6 15.6 23.4

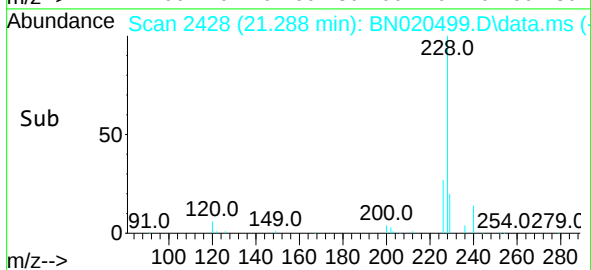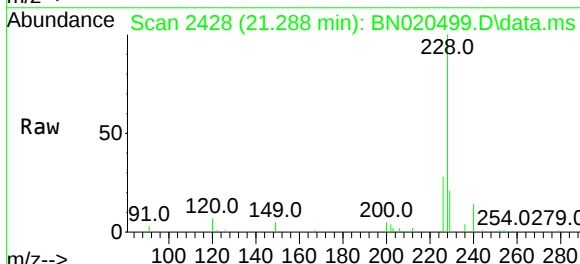

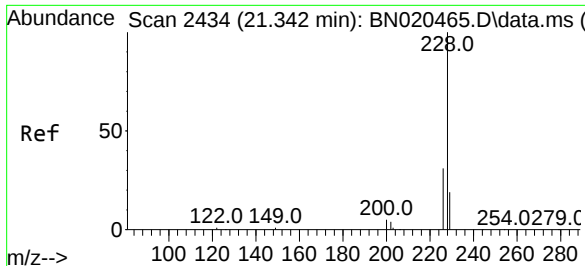

#33

Chrysene

Concen: 0.386 ng

RT: 21.342 min Scan# 2434

Delta R.T. -0.000 min

Lab File: BN020499.D

Acq: 27 Jun 2022 14:13

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion:228 Resp: 17751

Ion Ratio Lower Upper

228 100

226 29.0 23.4 35.0

229 20.1 15.7 23.5

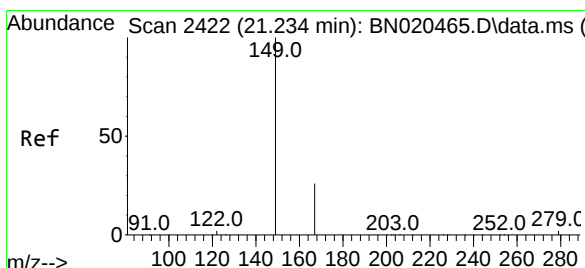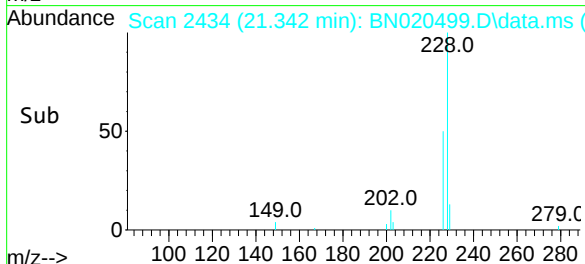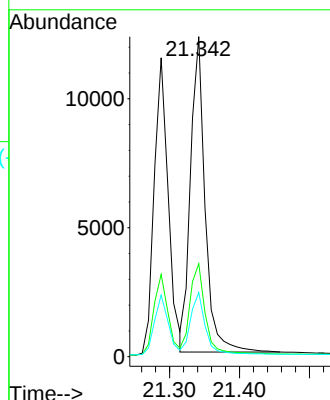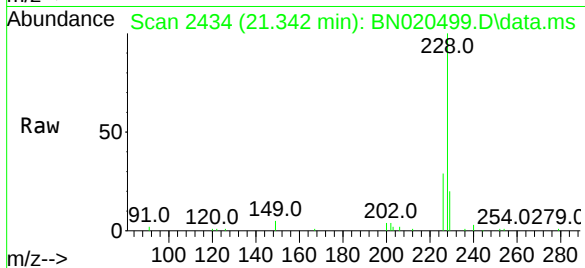

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.425 ng

RT: 21.225 min Scan# 2421

Delta R.T. -0.009 min

Lab File: BN020499.D

Acq: 27 Jun 2022 14:13




Tgt Ion:149 Resp: 9944


Ion Ratio Lower Upper

149 100

167 26.9 21.7 32.5

279 3.1 2.2 3.2


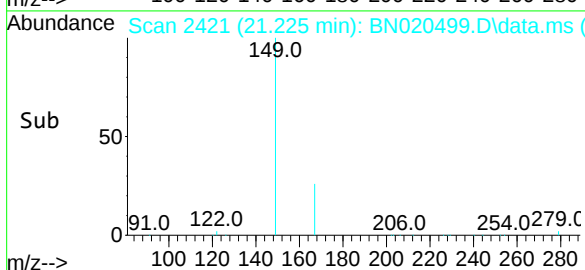
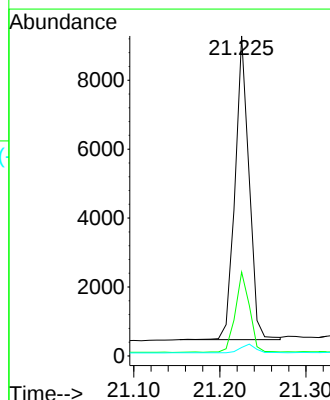
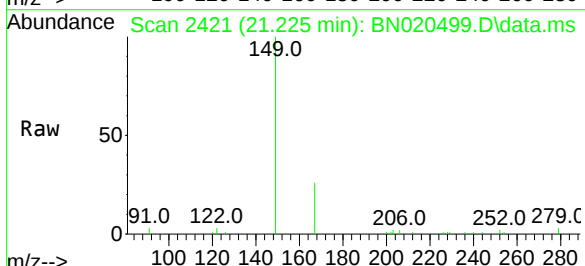




#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.586 min Scan# 2961
 Delta R.T. -0.015 min
 Lab File: BN020499.D
 Acq: 27 Jun 2022 14:13




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC


Tgt Ion:264 Resp: 9212
 Ion Ratio Lower Upper
 264 100
 260 25.8 20.9 31.3
 265 41.3 28.0 42.0

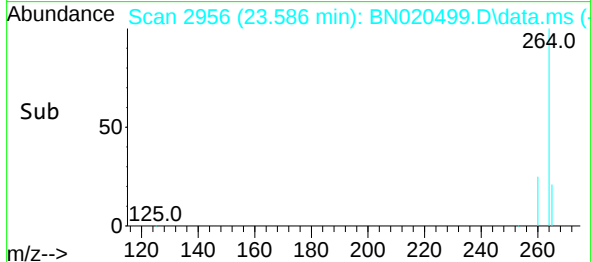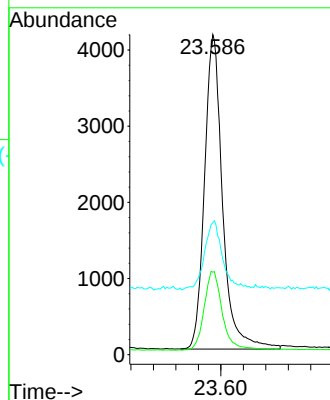

#36
 Indeno(1,2,3-cd)pyrene
 Concen: 0.327 ng
 RT: 25.916 min Scan# 3753
 Delta R.T. -0.021 min
 Lab File: BN020499.D
 Acq: 27 Jun 2022 14:13


Tgt Ion:276 Resp: 13422
 Ion Ratio Lower Upper
 276 100
 138 31.9 25.9 38.9
 277 24.8 19.8 29.8

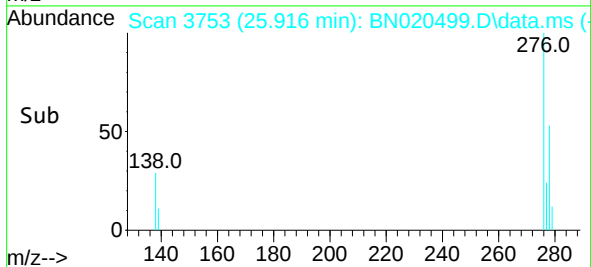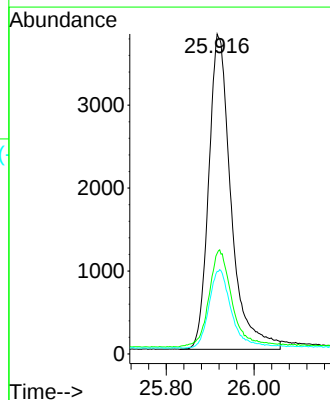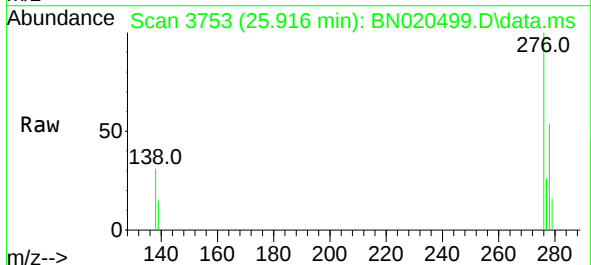






#37
Benzo(b)fluoranthene
Concen: 0.406 ng
RT: 22.896 min Scan# 21
Delta R.T. -0.012 min
Lab File: BN020499.D
Acq: 27 Jun 2022 14:13

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC







Tgt Ion:252 Resp: 14396
Ion Ratio Lower Upper
252 100
253 25.7 18.5 27.7
125 16.6 11.4 17.0

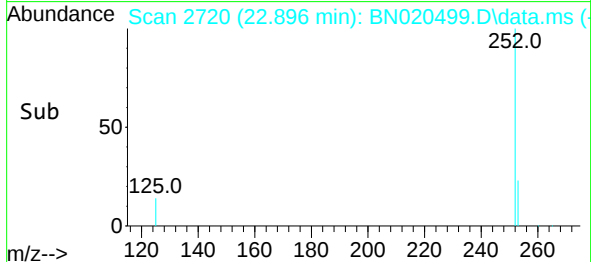

#38
Benzo(k)fluoranthene
Concen: 0.385 ng
RT: 22.942 min Scan# 2736
Delta R.T. -0.012 min
Lab File: BN020499.D
Acq: 27 Jun 2022 14:13

Tgt Ion:252 Resp: 14549
Ion Ratio Lower Upper
252 100
253 25.0 18.0 27.0
125 14.6 11.0 16.4

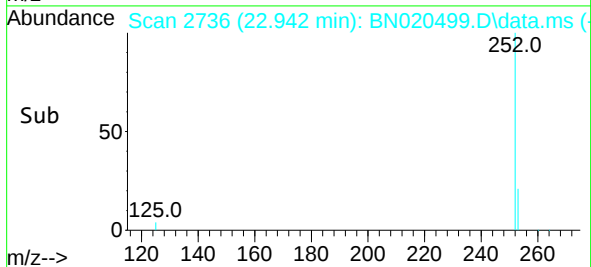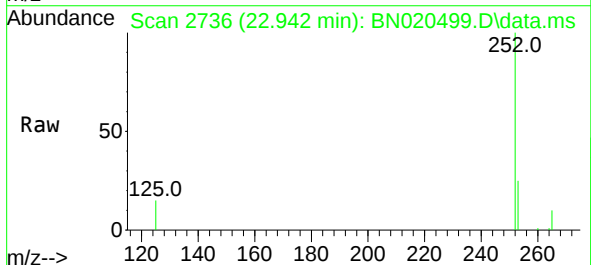



#39

Benzo(a)pyrene

Concen: 0.389 ng

RT: 23.483 min Scan# 2921

Delta R.T. -0.015 min

Lab File: BN020499.D

Acq: 27 Jun 2022 14:13





Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC

Tgt Ion:252	Resp:	11986
Ion Ratio	Lower	Upper
252	100	
253	27.0	19.0 28.4
125	20.9	13.8 20.8#

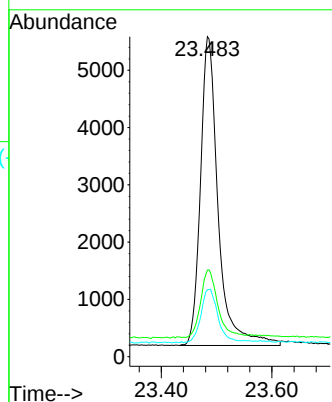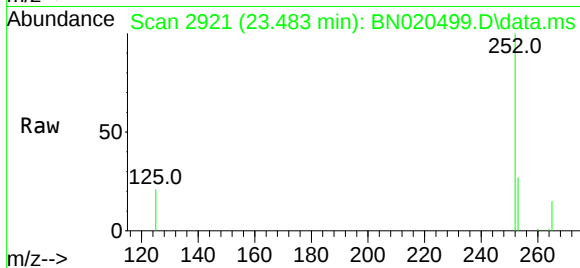

#40

Dibenzo(a,h)anthracene

Concen: 0.314 ng




RT: 25.936 min Scan# 3760


Delta R.T. -0.012 min

Lab File: BN020499.D

Acq: 27 Jun 2022 14:13


Tgt Ion:278	Resp:	10348
Ion Ratio	Lower	Upper
278	100	
139	24.1	18.6 28.0
279	27.4	19.7 29.5

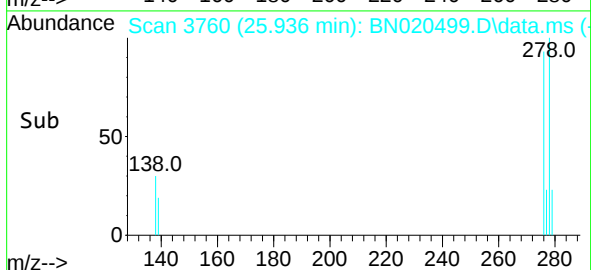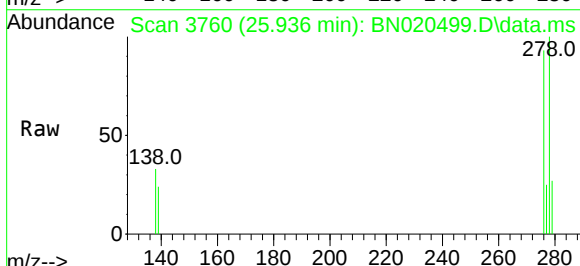

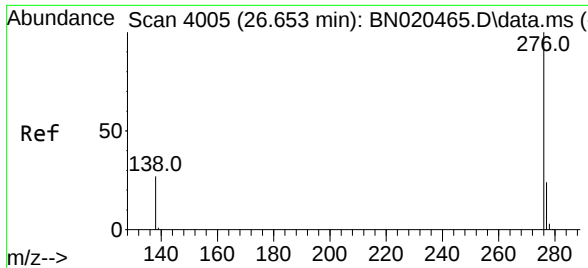

#41
Benzo(g,h,i)perylene
Concen: 0.320 ng
RT: 26.629 min Scan# 3997
Delta R.T. -0.023 min
Lab File: BN020499.D
Acq: 27 Jun 2022 14:13

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

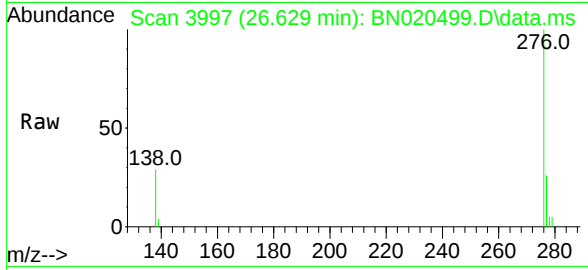

Tgt Ion:276 Resp: 11514
Ion Ratio Lower Upper
276 100
277 25.7 19.5 29.3
138 29.3 22.6 34.0

