


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062622\
 Data File : BN020462.D
 Acq On : 26 Jun 2022 12:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 27 02:03:21 2022

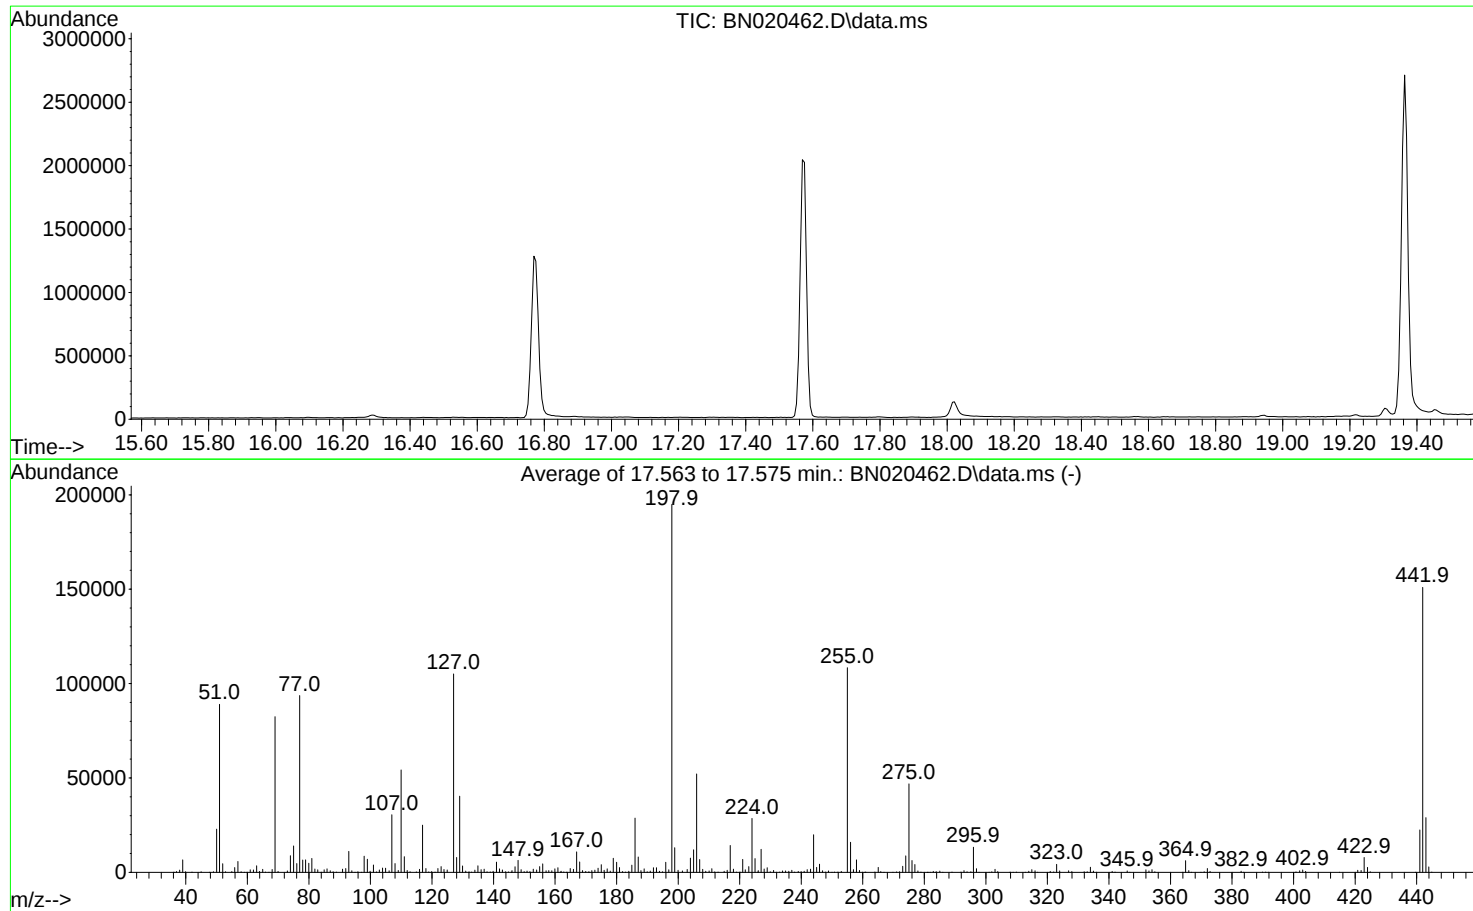




AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.7	89010	PASS
68	69	0.00	2	1.9	1544	PASS
69	198	0.00	100	42.3	82492	PASS
70	69	0.00	2	0.6	506	PASS
127	198	10	80	54.0	105141	PASS
197	198	0.00	2	0.7	1366	PASS
198	198	100	100	100.0	194880	PASS
199	198	5	9	6.7	13074	PASS
275	198	10	60	24.1	46923	PASS
365	198	1	100	3.2	6177	PASS
441	198	0.01	100	11.5	22483	PASS
442	442	50	100	100.0	150984	PASS
443	442	15	24	19.2	29028	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062622\
 Data File : BN020462.D
 Acq On : 26 Jun 2022 12:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jun 27 02:09:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 27 02:09:13 2022
 Response via : Initial Calibration

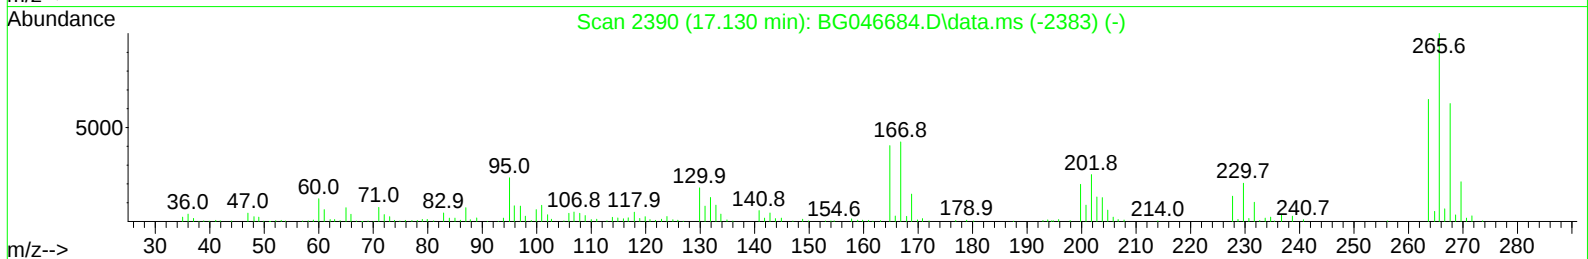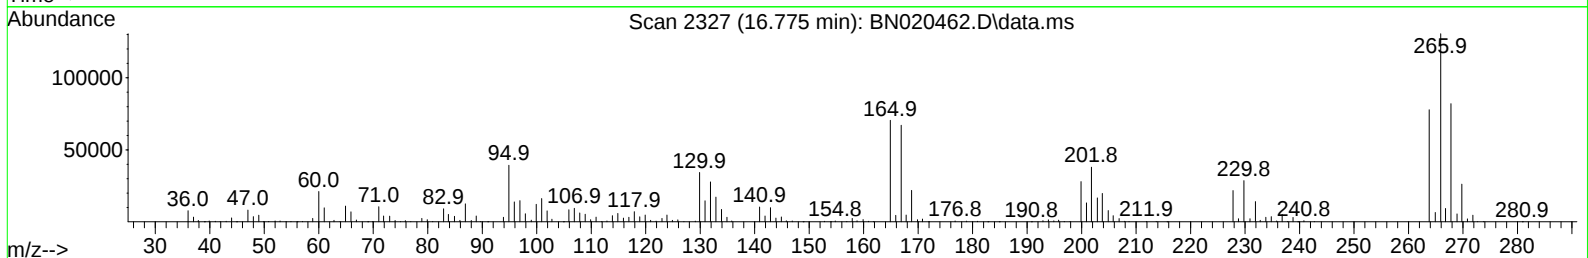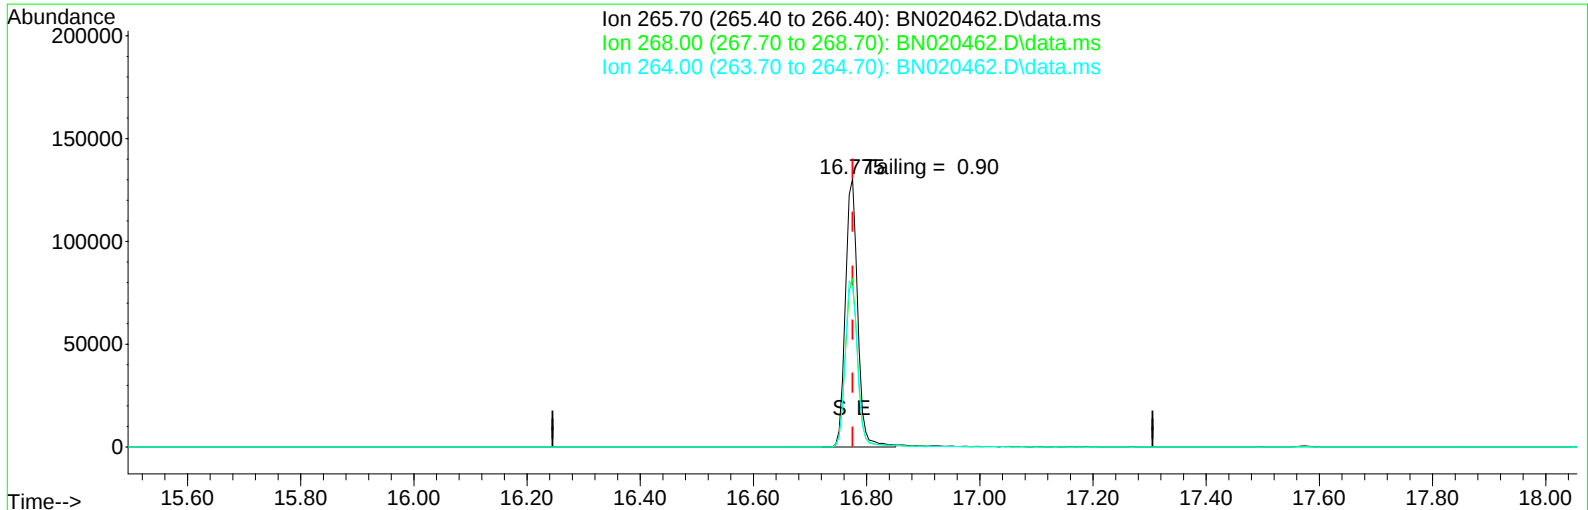

TIC: BN020462.D\data.ms

(70) Pentachlorophenol (C)

16.775min (0.000) 18095.27 ng




response 199094

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.84
264.00	61.60	59.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062622\
Data File : BN020462.D
Acq On : 26 Jun 2022 12:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 27 02:09:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 02:09:13 2022
Response via : Initial Calibration

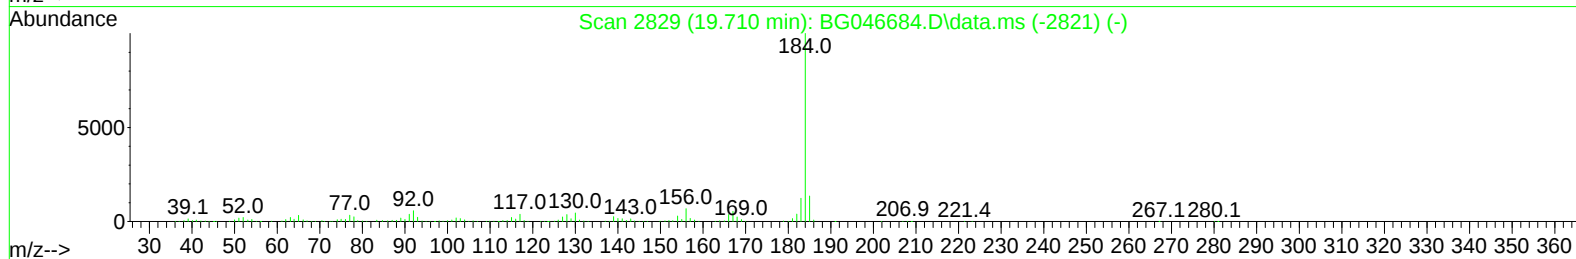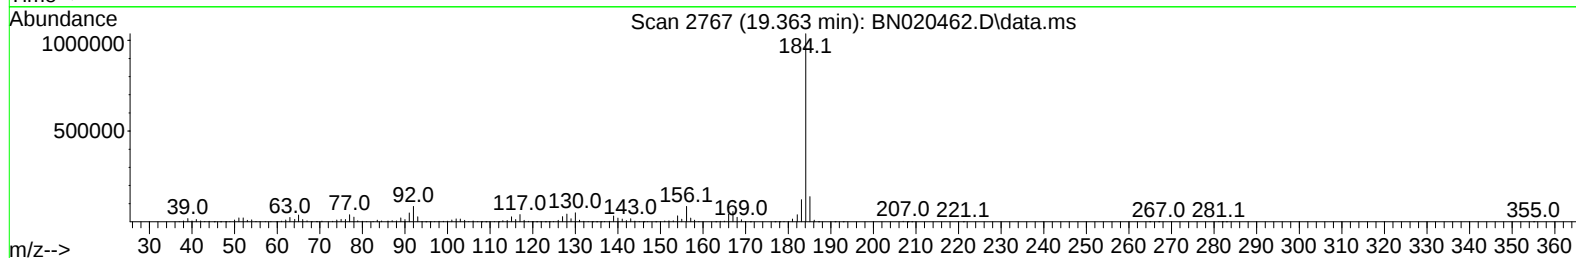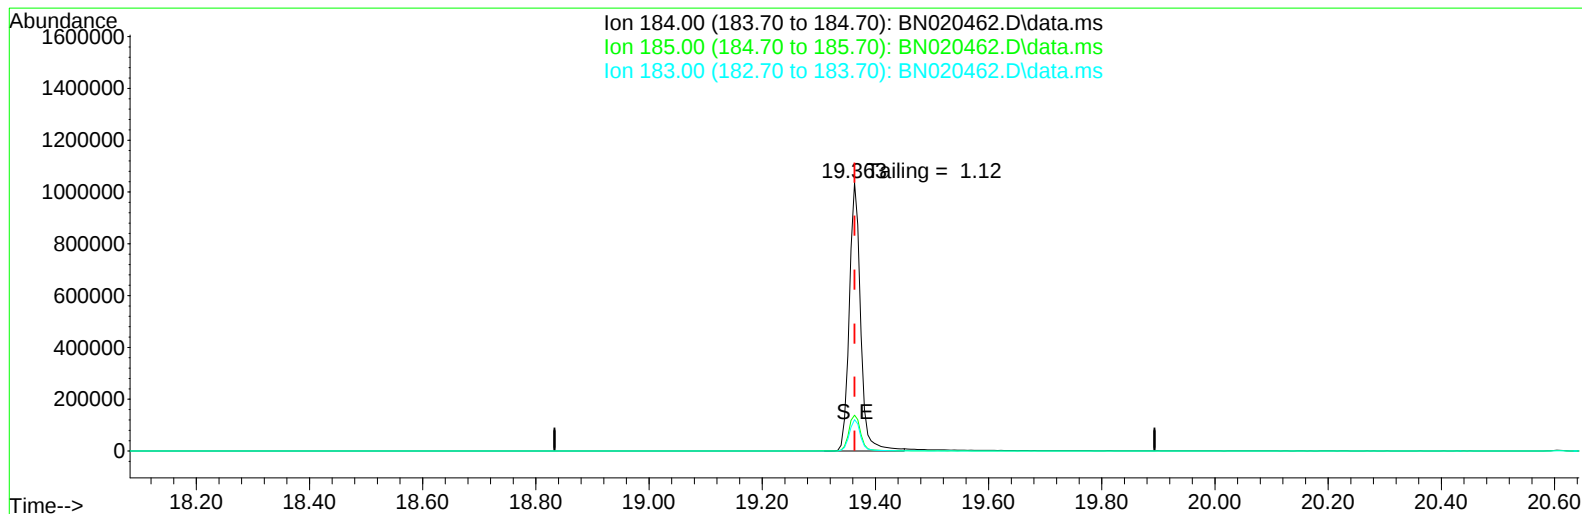

TIC: BN020462.D\data.ms

(77) Benzidine

19.363min (0.000) 0.00 ng

response 1473691

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.36
183.00	13.20	11.72
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/26/2022	BNA_N	<u>BN020462.D</u>
Compound Name	Response	Retention Time
DDT	687187	20.61
DDD	2125	20.16
DDE	0	19.75
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2125	689312	0.31

Instrument :
BNA_N
ClientSampleId :
DFTPP