


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062622\
 Data File : BN020481.D
 Acq On : 27 Jun 2022 03:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 27 02:03:21 2022

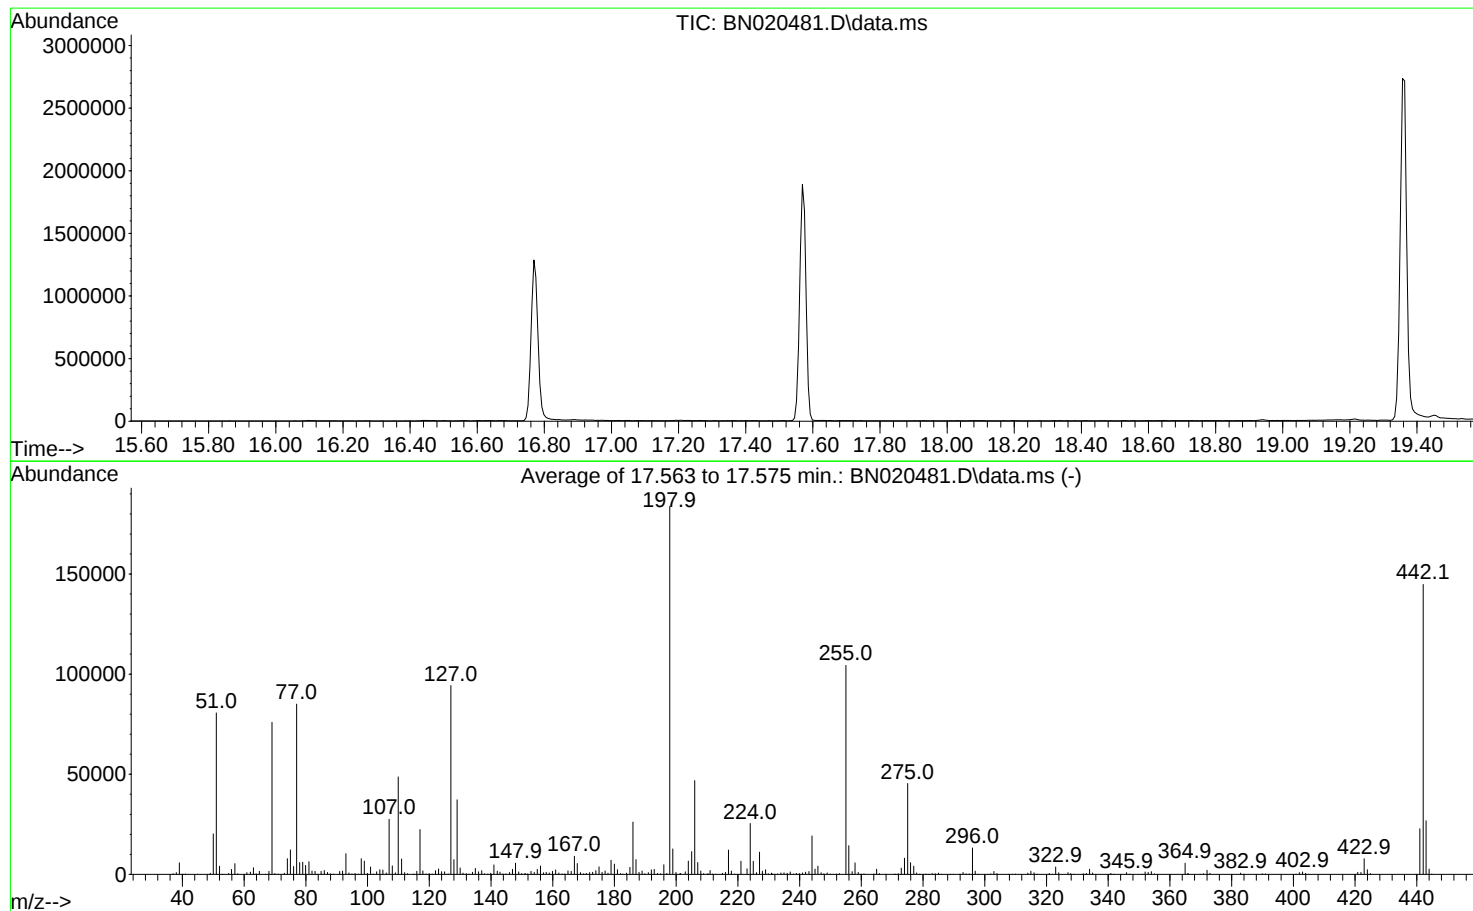




AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.9	80619	PASS
68	69	0.00	2	2.0	1496	PASS
69	198	0.00	100	41.3	75885	PASS
70	69	0.00	2	0.6	430	PASS
127	198	10	80	51.3	94280	PASS
197	198	0.00	2	0.3	504	PASS
198	198	100	100	100.0	183723	PASS
199	198	5	9	6.9	12748	PASS
275	198	10	60	24.7	45352	PASS
365	198	1	100	3.1	5619	PASS
441	198	0.01	100	12.4	22754	PASS
442	442	50	100	100.0	144805	PASS
443	442	15	24	18.5	26779	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062622\
Data File : BN020481.D
Acq On : 27 Jun 2022 03:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 27 04:42:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 02:09:13 2022
Response via : Initial Calibration

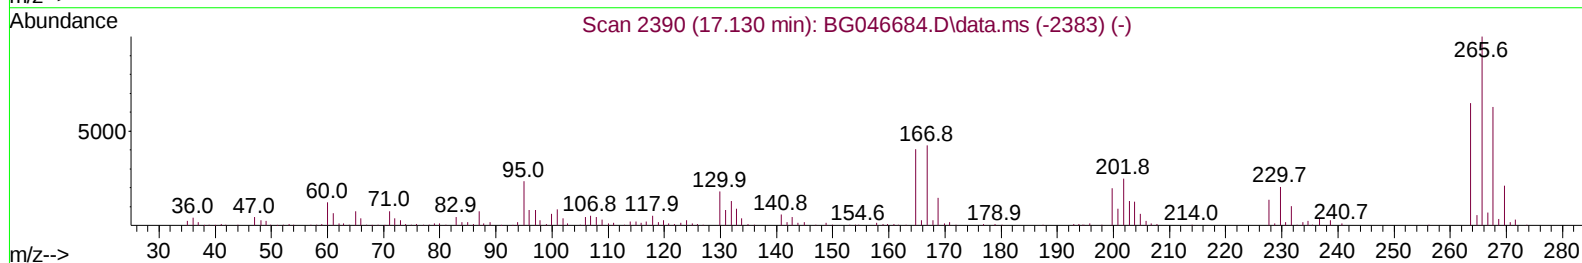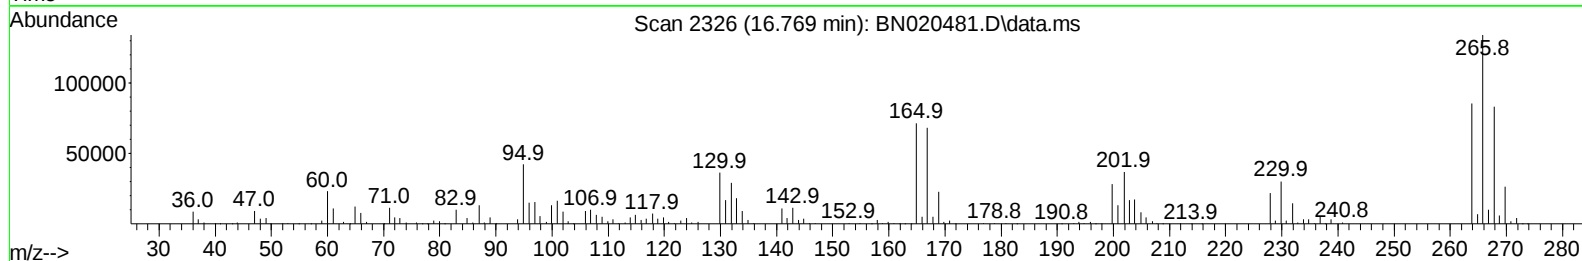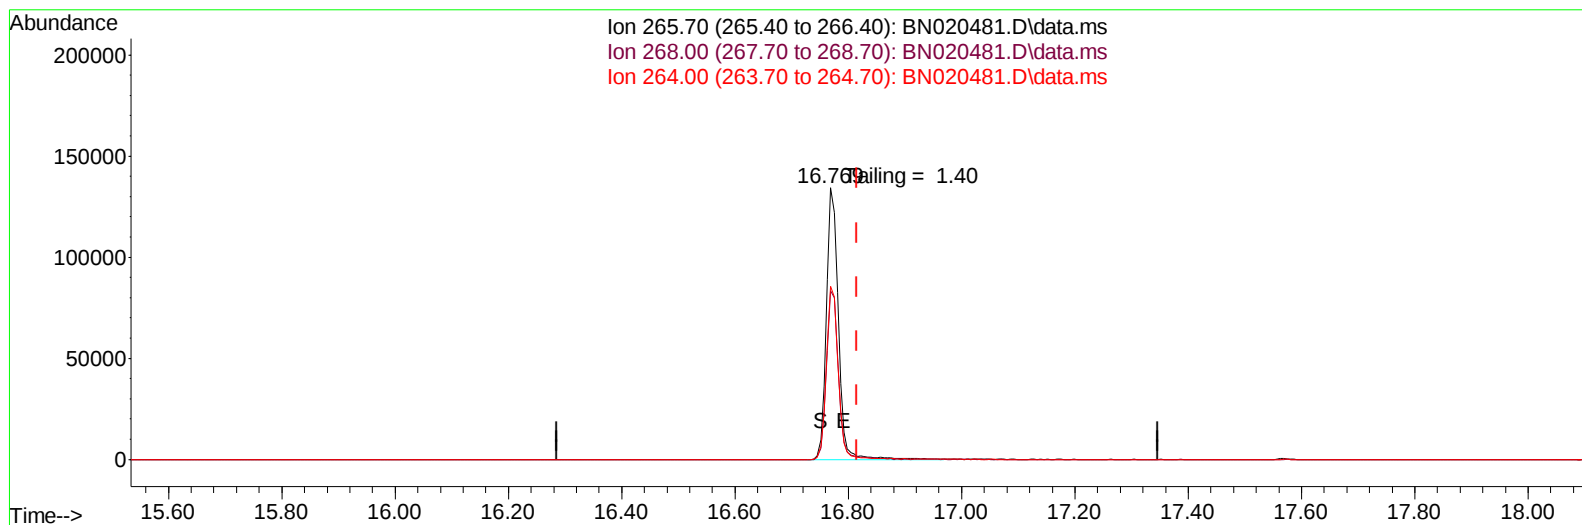

TIC: BN020481.D\data.ms

(70) Pentachloropheno1 (C)

16.769min (-0.047) 16478.77 ng




response 196439

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.12
264.00	61.60	63.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062622\
Data File : BN020481.D
Acq On : 27 Jun 2022 03:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 27 04:42:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 02:09:13 2022
Response via : Initial Calibration

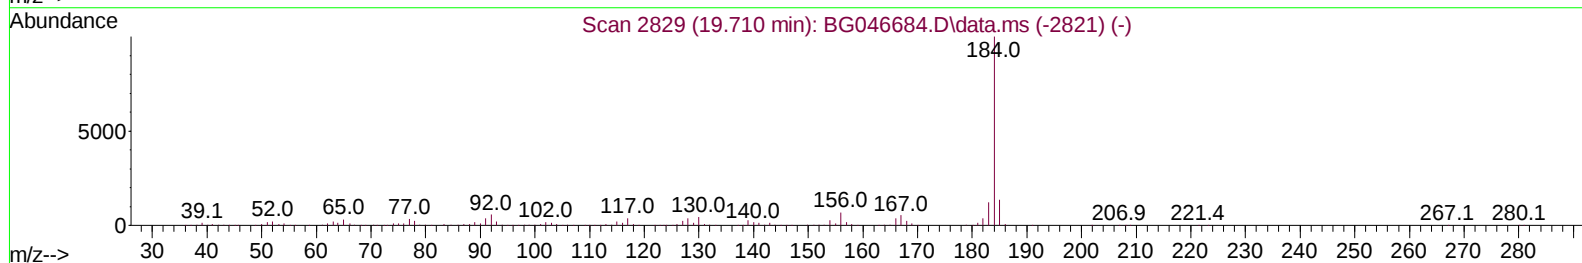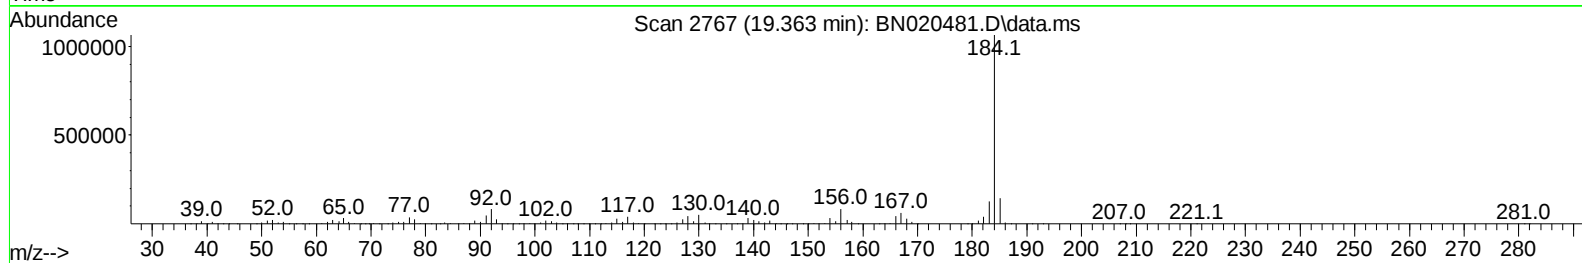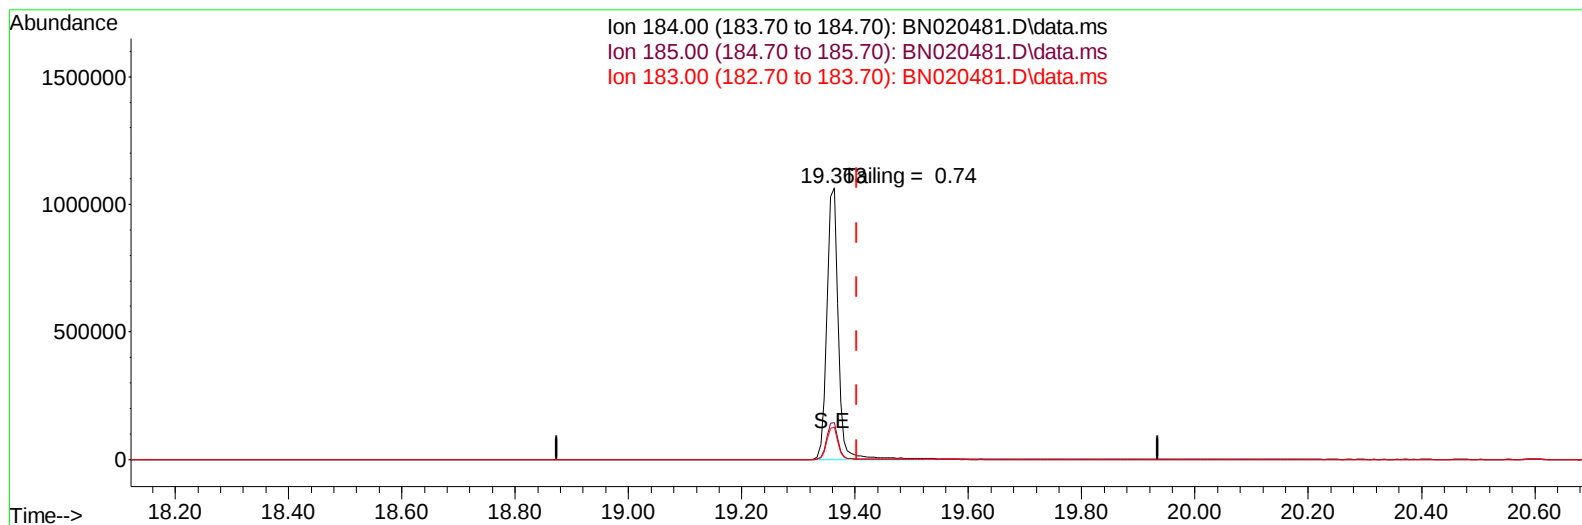

TIC: BN020481.D\data.ms

(77) Benzidine

19.363min (-0.041) 0.00 ng

response 1469558

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.59
183.00	13.20	11.96
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/26/2022	BNA_N	<u>BN020481.D</u>
Compound Name	Response	Retention Time
DDT	655682	20.59
DDD	9761	20.16
DDE	469	19.65
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10230	665912	1.54

Instrument :
BNA_N
ClientSampleId :
DFTPP