
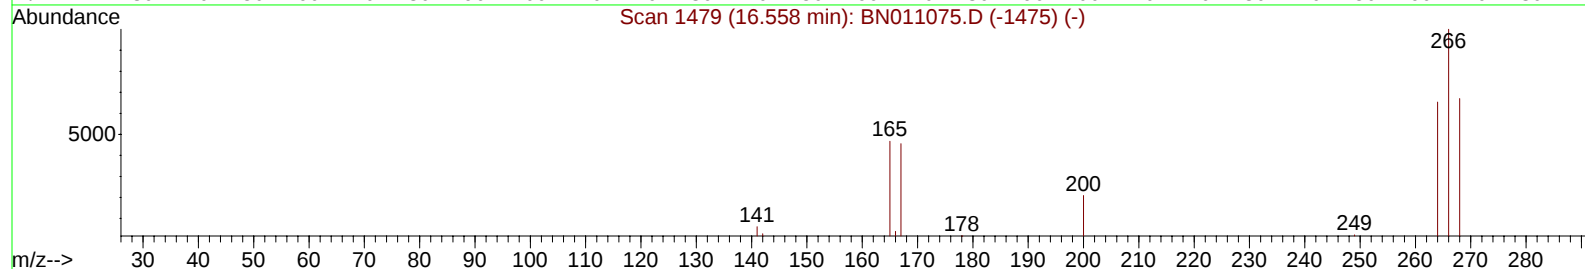
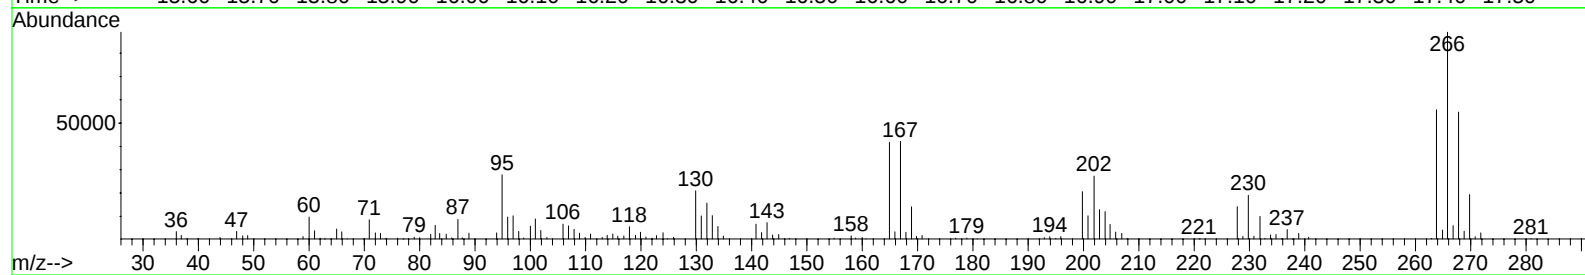


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN063020\
 Data File : BN011072.D
 Acq On : 30 Jun 2020 08:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 30 18:57:02 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN063020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 30 14:12:13 2020
 Response via : Initial Calibration

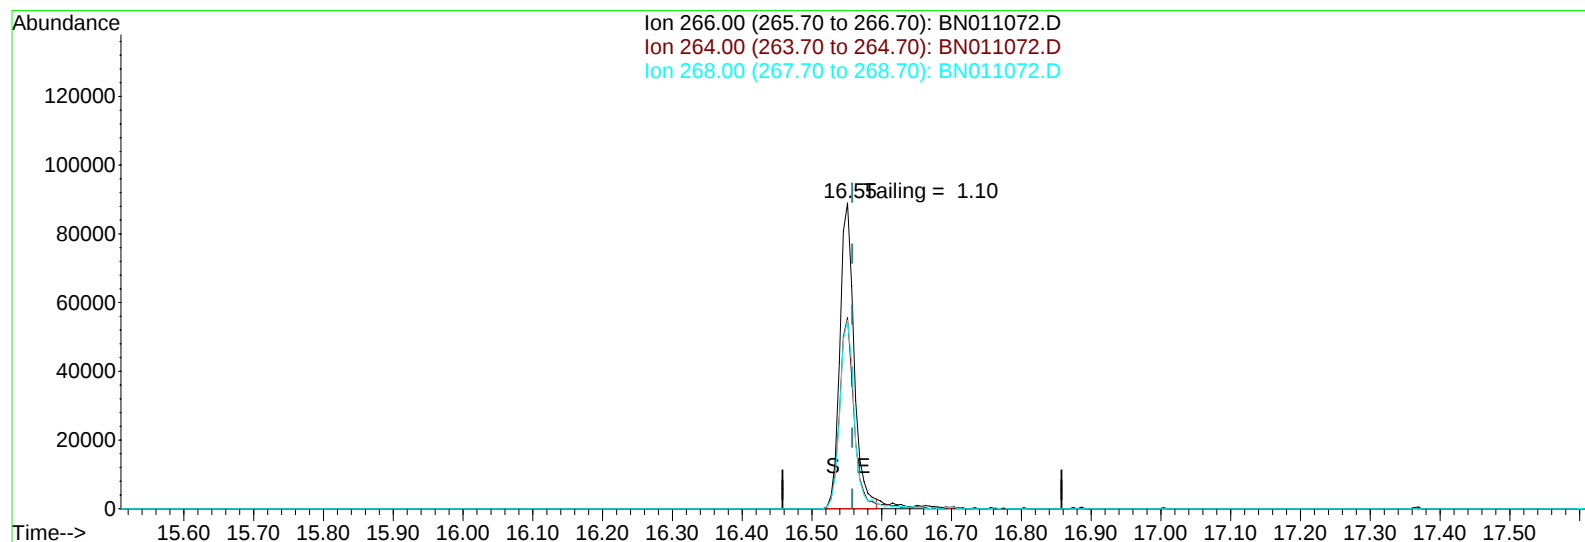

TIC: BN011072.D

(24) Pentachlorophenol

16.551min (-0.007) 0.00ng

response 128643

Ion	Exp%	Act%
266.00	100	100
264.00	59.20	63.37
268.00	68.70	63.25
0.00	0.00	0.00