


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN063020\
 Data File : BN011072.D
 Acq On : 30 Jun 2020 08:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN063020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 30 14:12:13 2020

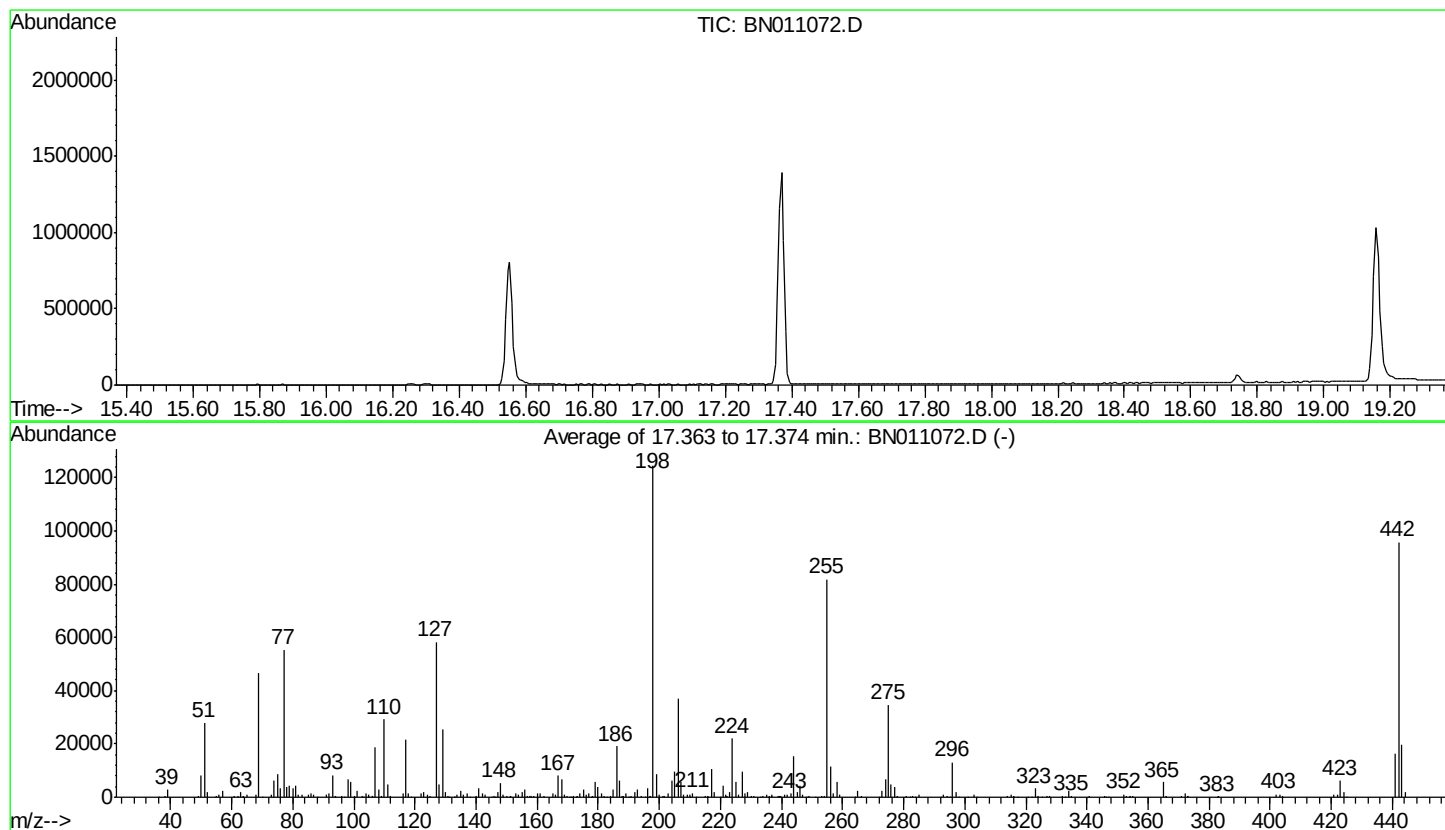

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.4	27933	PASS
68	69	0.00	2	1.9	901	PASS
69	198	0.00	100	37.6	46813	PASS
70	69	0.00	2	0.2	114	PASS
127	198	10	80	46.8	58277	PASS
197	198	0.00	2	0.5	625	PASS
198	198	100	100	100.0	124496	PASS
199	198	5	9	7.1	8889	PASS
275	198	10	60	27.9	34738	PASS
365	198	1	100	4.5	5604	PASS
441	198	0.01	100	13.3	16555	PASS
442	198	50	100	76.8	95658	PASS
443	442	15	24	20.6	19751	PASS