

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070121\
 Data File : BN015285.D
 Acq On : 02 Jul 2021 07:20
 Operator : CG/JU
 Sample : PB137445BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB137445BL

Quant Time: Jul 02 08:29:24 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN063021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 01 09:06:31 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.735	152	24848	0.40	ng	# 0.00
7) Naphthalene-d8	10.495	136	110901	0.40	ng	0.00
13) Acenaphthene-d10	14.345	164	54206	0.40	ng	0.00
19) Phenanthrene-d10	17.091	188	97752	0.40	ng	0.00
29) Chrysene-d12	21.291	240	63185	0.40	ng	#-0.01
35) Perylene-d12	23.539	264	51033	0.40	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.374	112	23210	0.37	ng	0.01
5) Phenol-d6	6.914	99	25545	0.32	ng	0.01
8) Nitrobenzene-d5	8.861	82	28091	0.45	ng	0.00
11) 2-Methylnaphthalene-d10	12.083	152	57745	0.31	ng	0.00
14) 2,4,6-Tribromophenol	15.842	330	3769	0.38	ng	0.00
15) 2-Fluorobiphenyl	12.962	172	80247	0.36	ng	0.00
27) Fluoranthene-d10	19.127	212	85265	0.30	ng	0.00
31) Terphenyl-d14	19.733	244	98928	0.67	ng	0.00
Target Compounds						Qvalue
20) 4,6-Dinitro-2-methylph...	15.525	198	5	0.19	ng	# 14
23) Atrazine	16.555	200	9	0.17	ng	# 16
24) Pentachlorophenol	16.750	266	168	0.26	ng	91
34) Bis(2-ethylhexyl)phtha...	21.217	149	1506	0.16	ng	# 90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070121\
Data File : BN015285.D
Acq On : 02 Jul 2021 07:20
Operator : CG/JU
Sample : PB137445BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB137445BL

Quant Time: Jul 02 08:29:24 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN063021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 01 09:06:31 2021
Response via : Initial Calibration




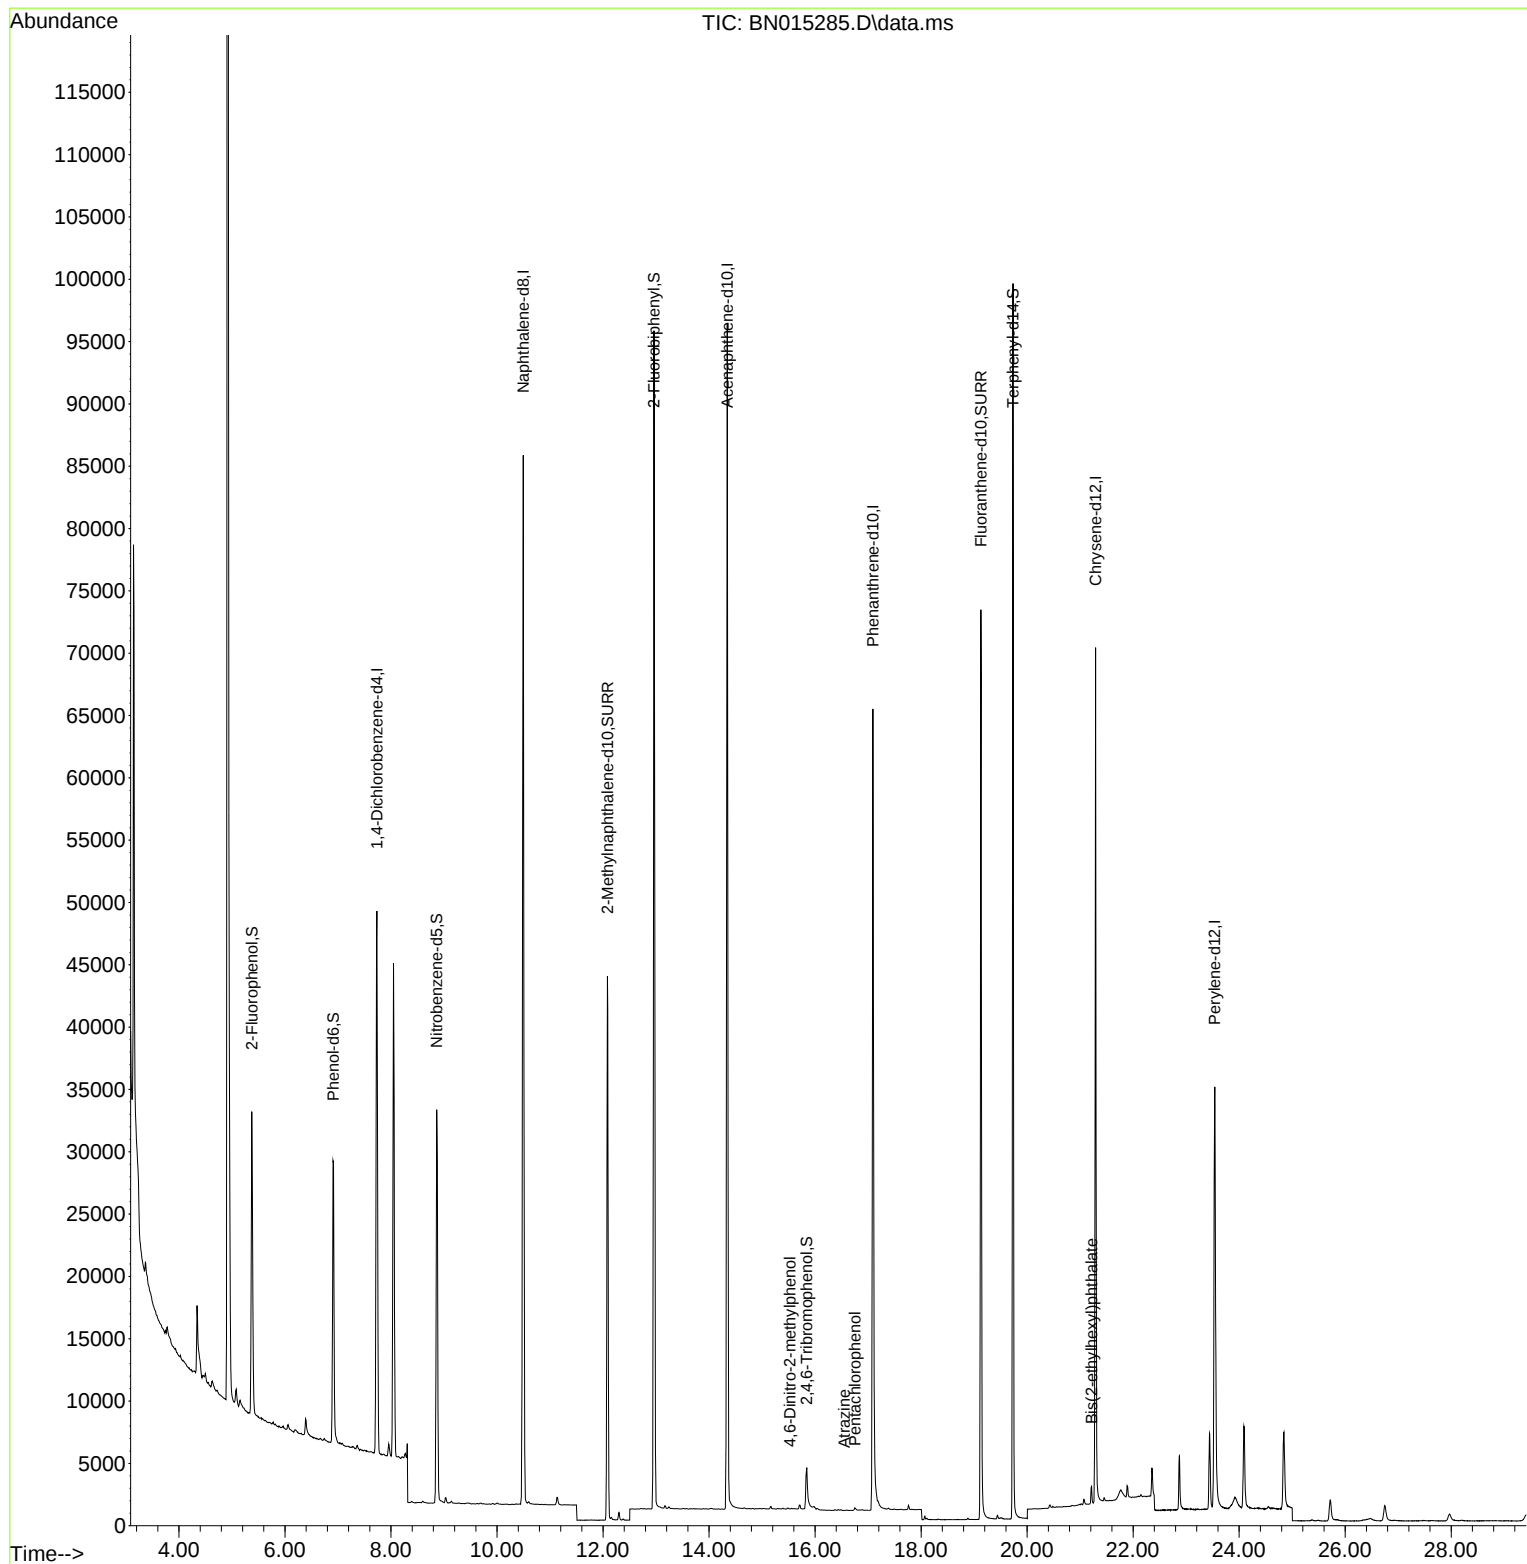




#1
1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.735 min Scan# 505
Delta R.T. 0.003 min
Lab File: BN015285.D
Acq: 02 Jul 2021 07:20




Instrument :
BNA_N
ClientSampleId :
PB137445BL


Tgt Ion:152 Resp: 24848
Ion Ratio Lower Upper
152 100
150 153.7 119.0 178.6
115 58.7 62.2 93.4#

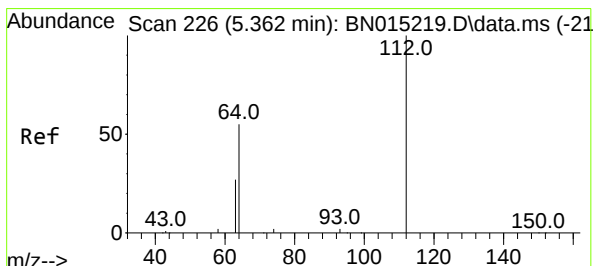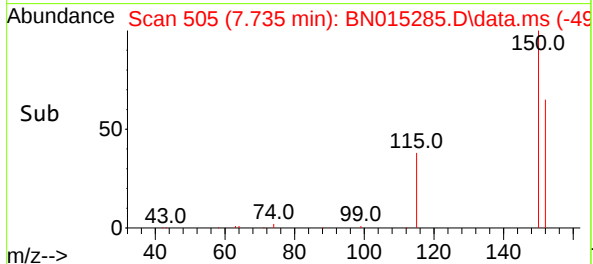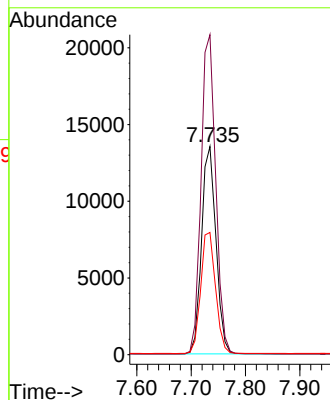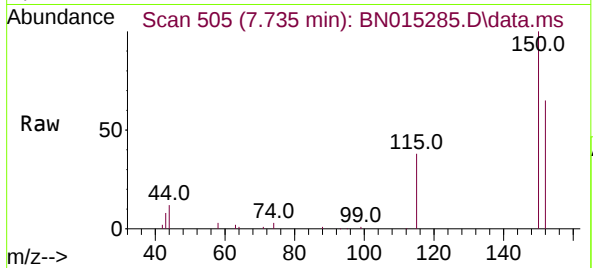

#4
2-Fluorophenol
Concen: 0.37 ng
RT: 5.374 min Scan# 249
Delta R.T. 0.012 min
Lab File: BN015285.D
Acq: 02 Jul 2021 07:20

Tgt Ion:112 Resp: 23210
Ion Ratio Lower Upper
112 100
64 55.9 39.0 58.6
63 28.2 20.6 30.8


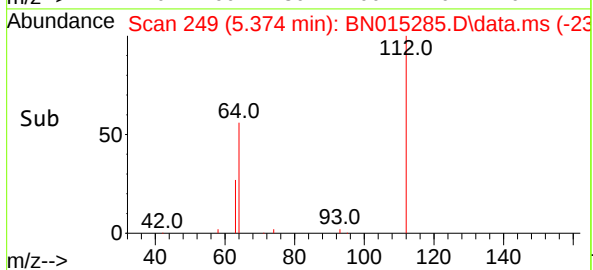
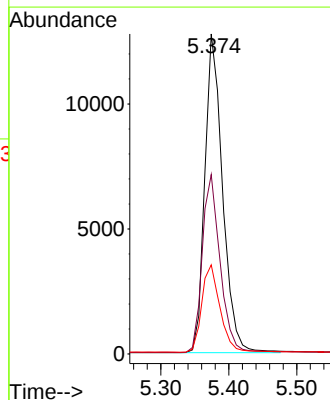
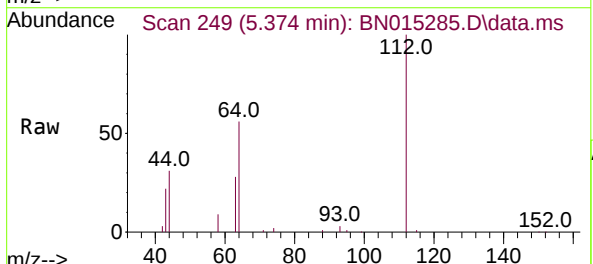


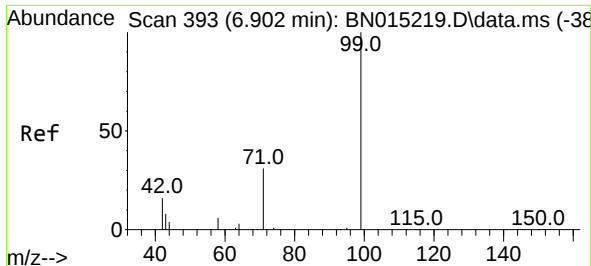

#5
Phenol-d6
Concen: 0.32 ng
RT: 6.914 min Scan# 416
Delta R.T. 0.012 min
Lab File: BN015285.D
Acq: 02 Jul 2021 07:20




Instrument :
BNA_N
ClientSampleId :
PB137445BL

Tgt Ion: 99 Resp: 25545
Ion Ratio Lower Upper
99 100
42 16.4 8.9 13.3#
71 30.2 35.6 53.4#

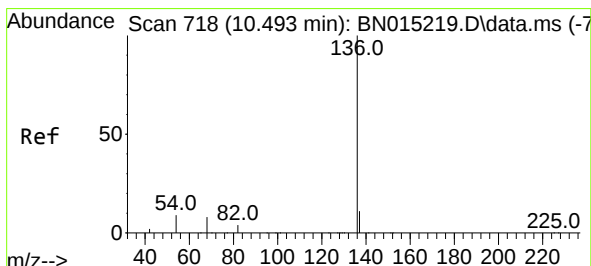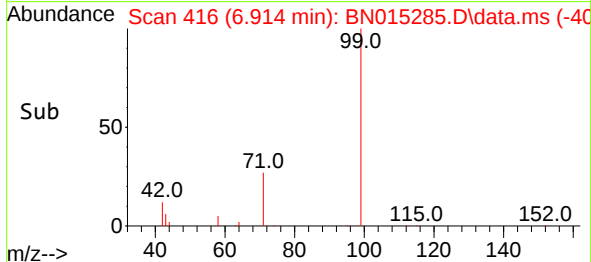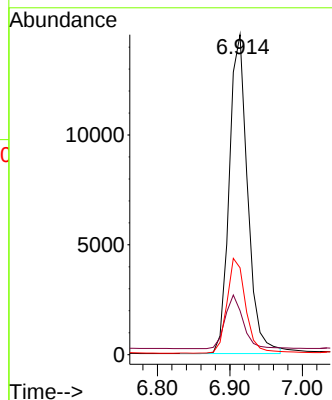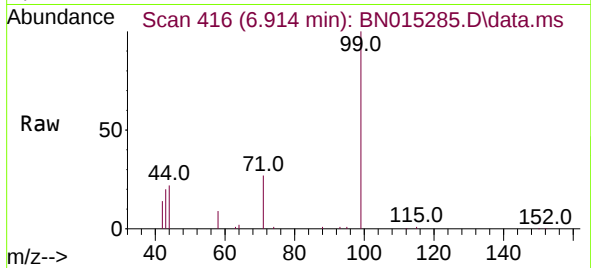

#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.495 min Scan# 740
Delta R.T. 0.003 min
Lab File: BN015285.D
Acq: 02 Jul 2021 07:20

Tgt Ion: 136 Resp: 110901
Ion Ratio Lower Upper
136 100
137 10.9 9.8 14.8
54 5.9 5.4 8.2
68 5.0 4.9 7.3


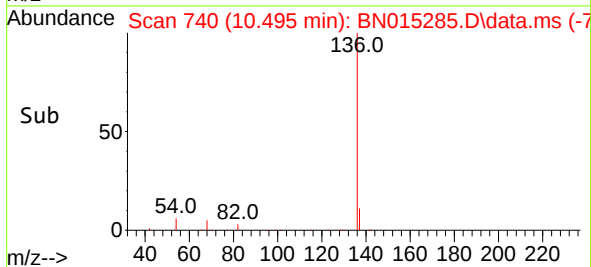
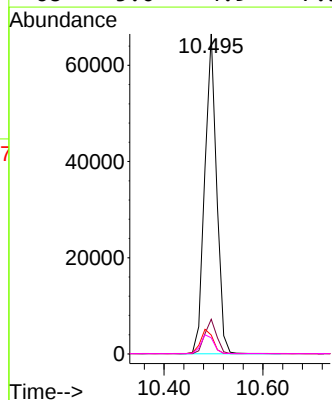
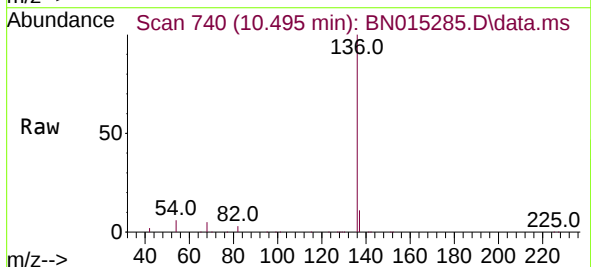




#8
Nitrobenzene-d5
Concen: 0.45 ng
RT: 8.861 min Scan# 611
Delta R.T. -0.009 min
Lab File: BN015285.D
Acq: 02 Jul 2021 07:20




Instrument :
BNA_N
ClientSampleId :
PB137445BL


Tgt Ion: 82 Resp: 28091
Ion Ratio Lower Upper
82 100
128 34.2 31.6 47.4
54 54.2 29.0 43.4#

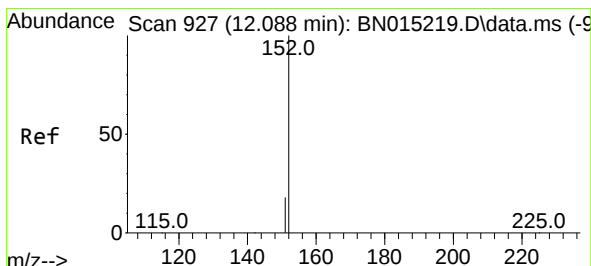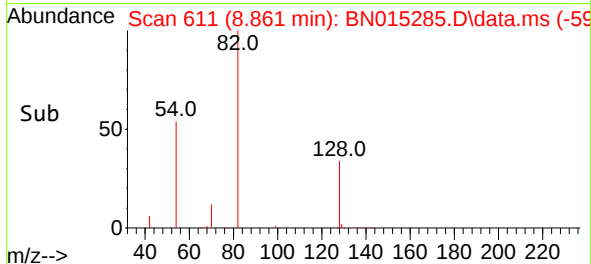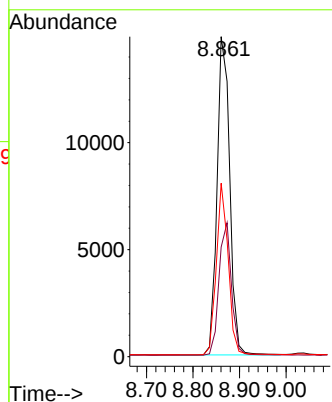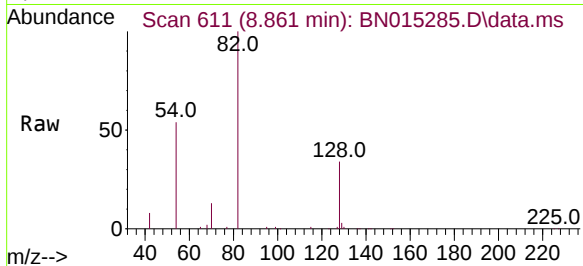

#11
2-Methylnaphthalene-d10
Concen: 0.31 ng
RT: 12.083 min Scan# 949
Delta R.T. -0.005 min
Lab File: BN015285.D
Acq: 02 Jul 2021 07:20

Tgt Ion: 152 Resp: 57745
Ion Ratio Lower Upper
152 100
151 20.5 16.7 25.1


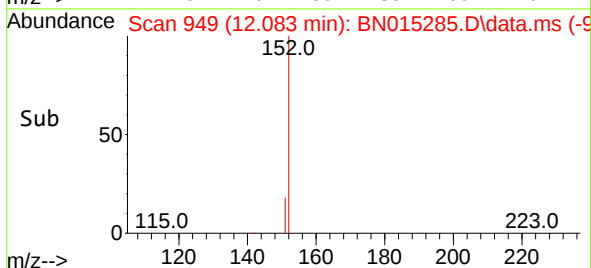
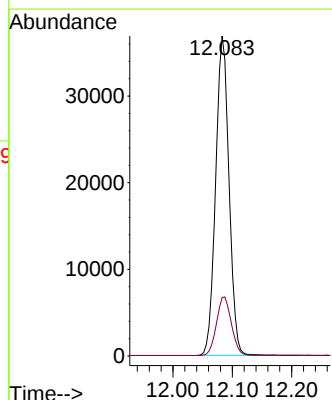
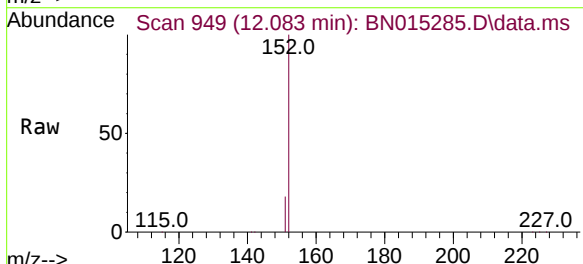


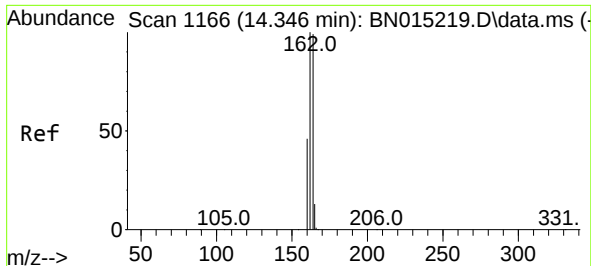

#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.345 min Scan# 1189
Delta R.T. -0.001 min
Lab File: BN015285.D
Acq: 02 Jul 2021 07:20




Instrument :
BNA_N
ClientSampleId :
PB137445BL


Tgt Ion:164 Resp: 54206
Ion Ratio Lower Upper
164 100
162 100.1 83.8 125.6
160 45.3 37.4 56.0

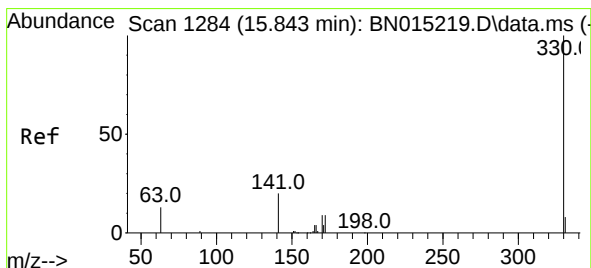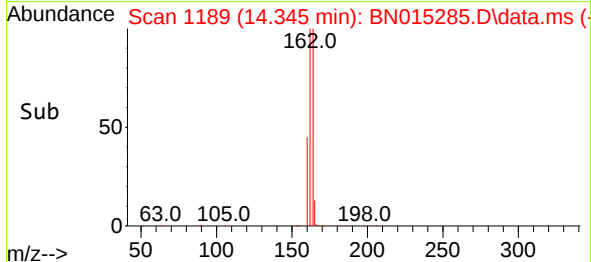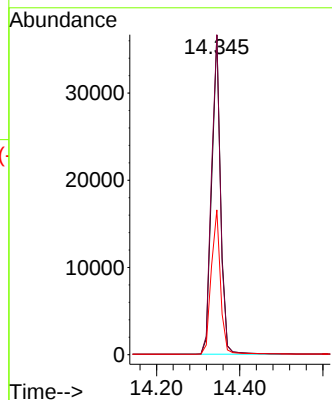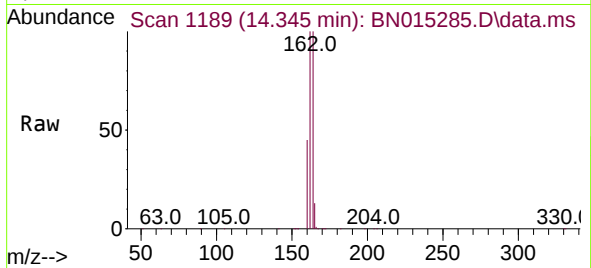

#14
2,4,6-Tribromophenol
Concen: 0.38 ng
RT: 15.842 min Scan# 1307
Delta R.T. -0.001 min
Lab File: BN015285.D
Acq: 02 Jul 2021 07:20

Tgt Ion:330 Resp: 3769
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 37.9 22.4 33.6#


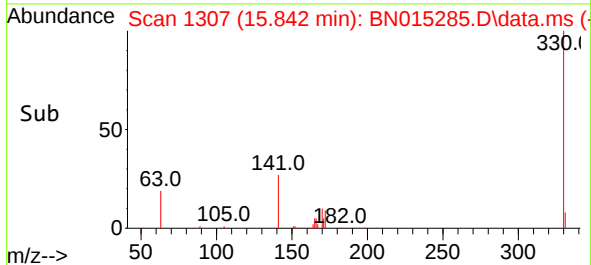
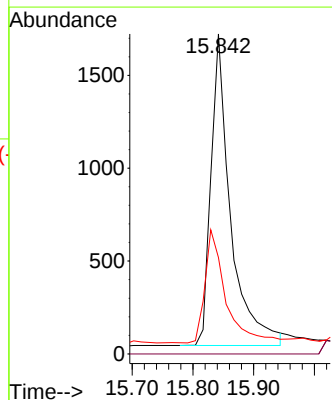
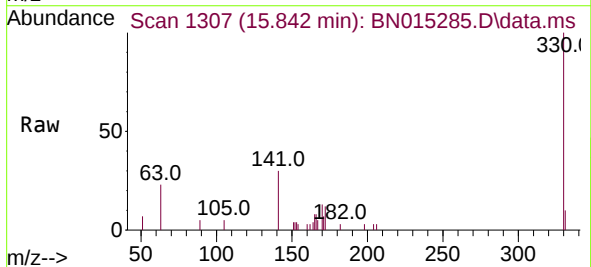


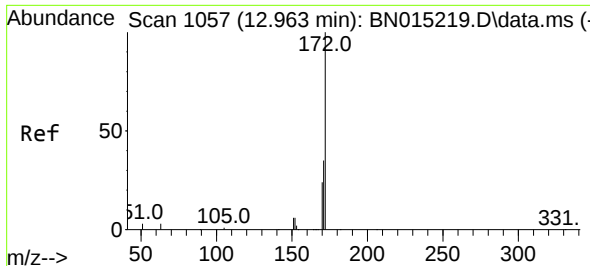

#15
2-Fluorobiphenyl
Concen: 0.36 ng
RT: 12.962 min Scan# 1080
Delta R.T. -0.001 min
Lab File: BN015285.D
Acq: 02 Jul 2021 07:20




Instrument :
BNA_N
ClientSampleId :
PB137445BL


Tgt Ion:172 Resp: 80247
Ion Ratio Lower Upper
172 100
171 34.9 30.6 45.8
170 23.4 20.2 30.4

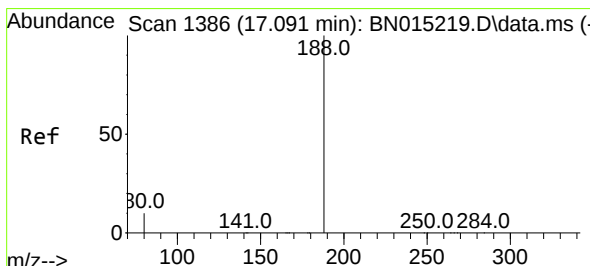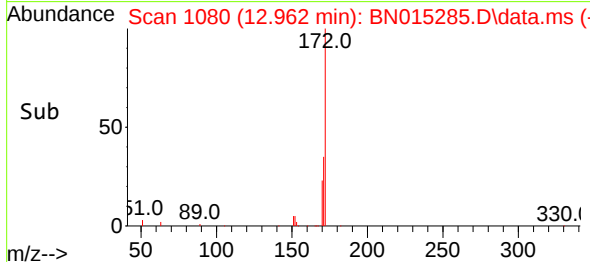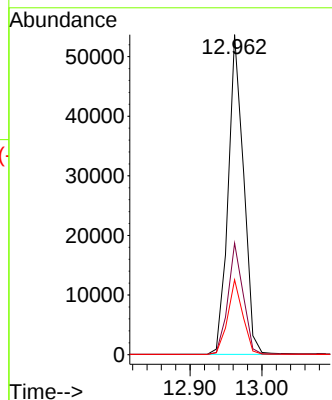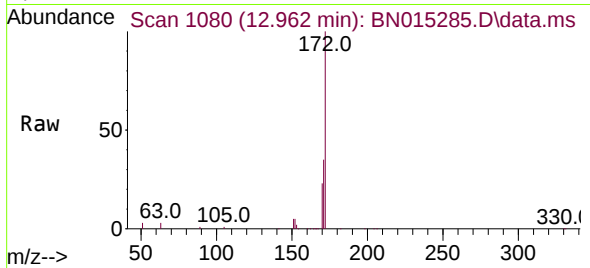

#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.091 min Scan# 1409
Delta R.T. -0.000 min
Lab File: BN015285.D
Acq: 02 Jul 2021 07:20

Tgt Ion:188 Resp: 97752
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 10.5 9.0 13.4


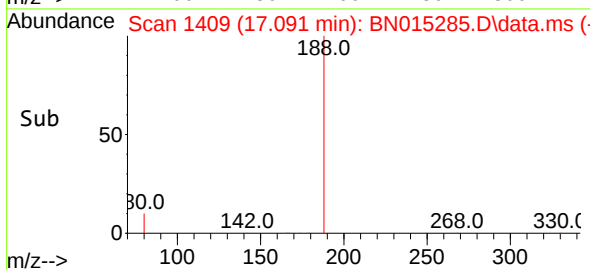
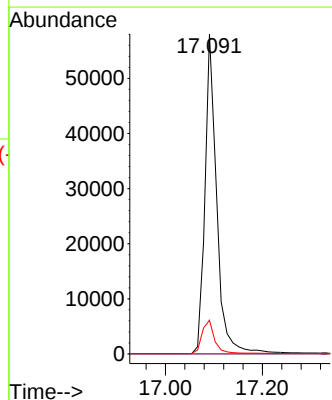
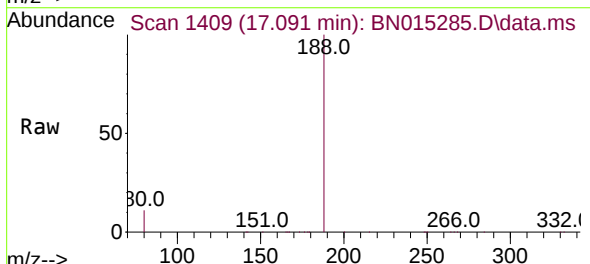


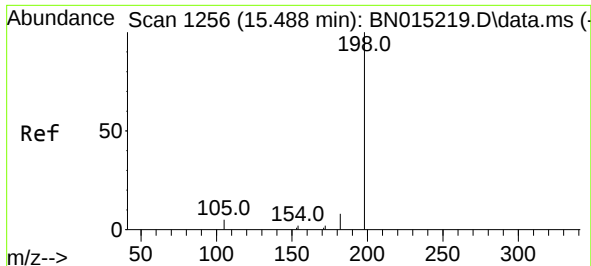

#20
4,6-Dinitro-2-methylphenol
Concen: 0.19 ng
RT: 15.525 min Scan# 1282
Delta R.T. 0.037 min
Lab File: BN015285.D
Acq: 02 Jul 2021 07:20




Instrument :
BNA_N
ClientSampleId :
PB137445BL


Tgt Ion:198 Resp: 5
Ion Ratio Lower Upper
198 100
182 97.9 34.5 51.7#
77 0.0 0.0 0.0

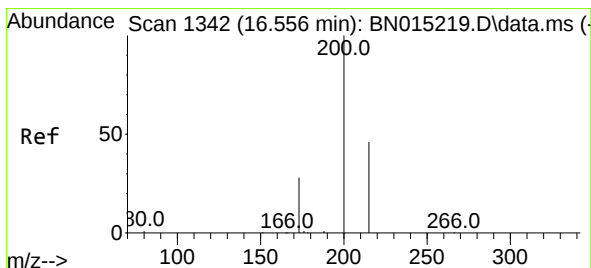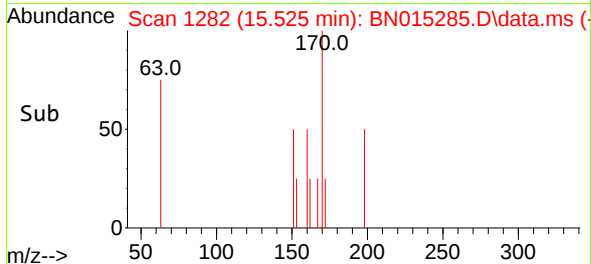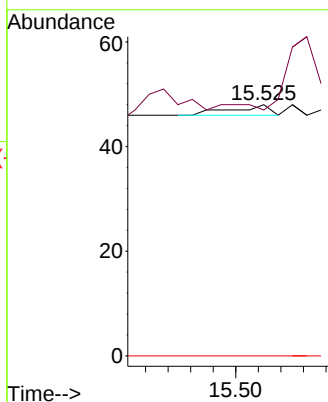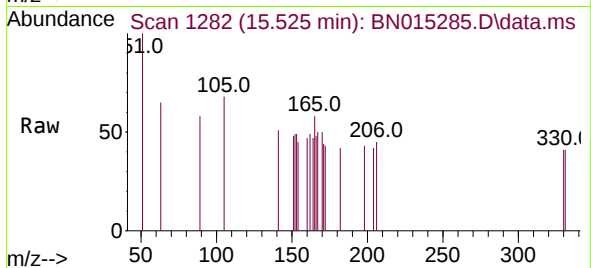

#23
Atrazine
Concen: 0.17 ng
RT: 16.555 min Scan# 1365
Delta R.T. -0.001 min
Lab File: BN015285.D
Acq: 02 Jul 2021 07:20

Tgt Ion:200 Resp: 9
Ion Ratio Lower Upper
200 100
173 96.1 21.7 32.5#
215 96.1 43.1 64.7#


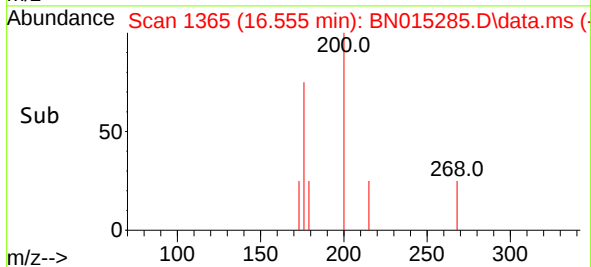
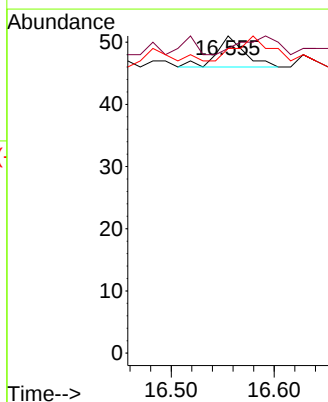
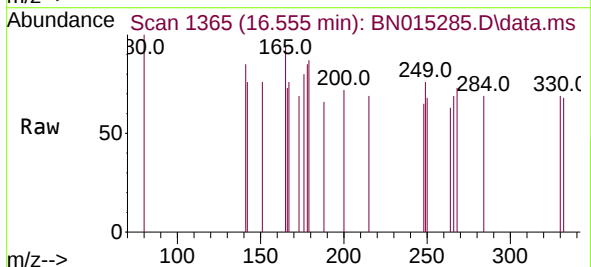


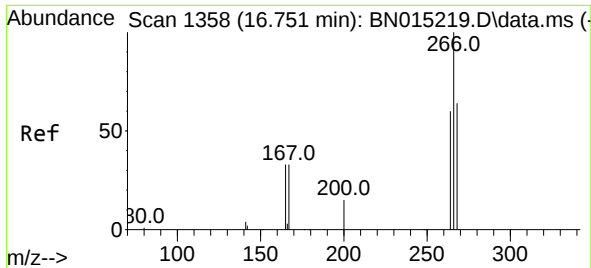

#24
Pentachlorophenol
Concen: 0.26 ng
RT: 16.750 min Scan# 1381
Delta R.T. -0.001 min
Lab File: BN015285.D
Acq: 02 Jul 2021 07:20




Instrument :
BNA_N
ClientSampleId :
PB137445BL


Tgt Ion:	266	Resp:	168
Ion Ratio	Lower	Upper	
266	100		
264	55.4	51.0	76.4
268	68.5	50.6	76.0

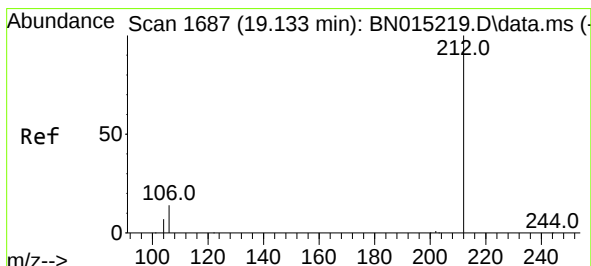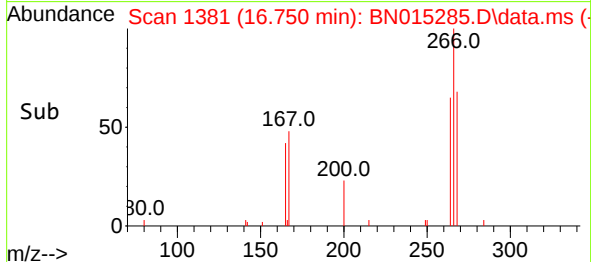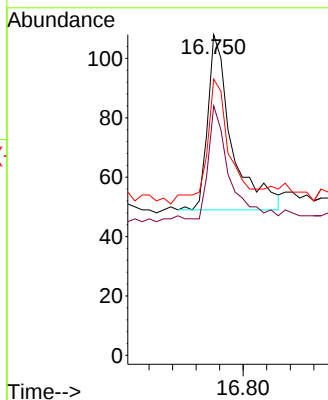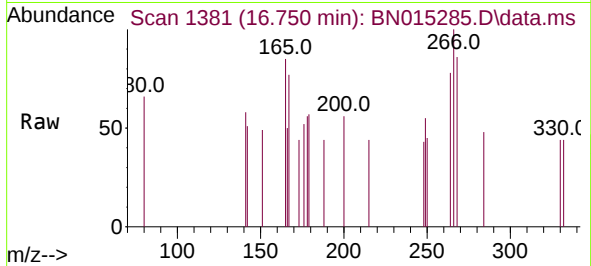

#27
Fluoranthene-d10
Concen: 0.30 ng
RT: 19.127 min Scan# 1709
Delta R.T. -0.006 min
Lab File: BN015285.D
Acq: 02 Jul 2021 07:20

Tgt Ion:	212	Resp:	85265
Ion Ratio	Lower	Upper	
212	100		
106	14.2	7.0	10.6#
104	7.7	4.1	6.1#


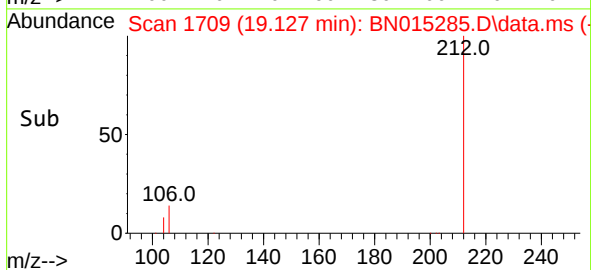
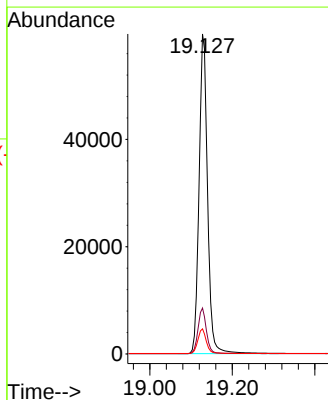
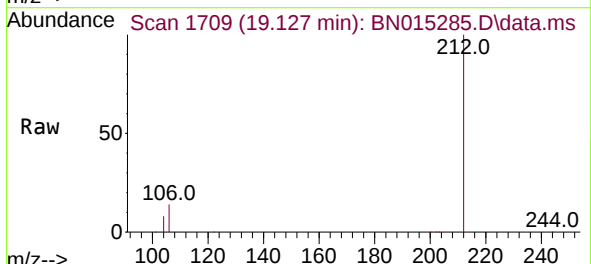


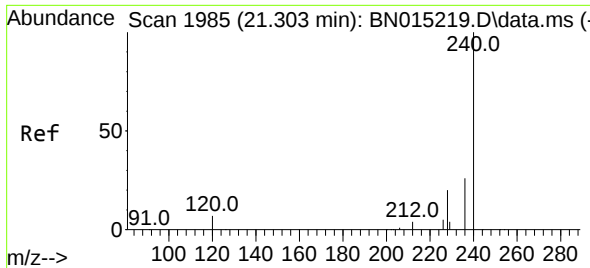

#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.291 min Scan# 2007
Delta R.T. -0.012 min
Lab File: BN015285.D
Acq: 02 Jul 2021 07:20




Instrument :
BNA_N
ClientSampleId :
PB137445BL


Tgt Ion:240 Resp: 63185
Ion Ratio Lower Upper
240 100
120 9.4 4.2 6.4#
236 26.3 21.4 32.2

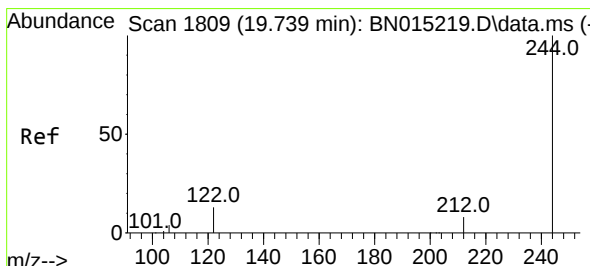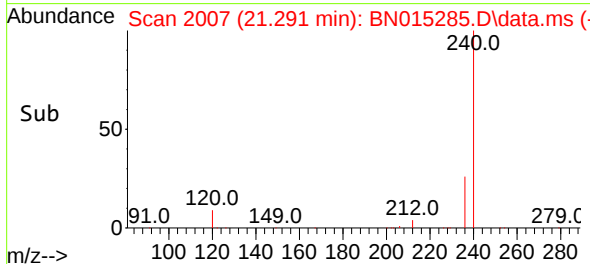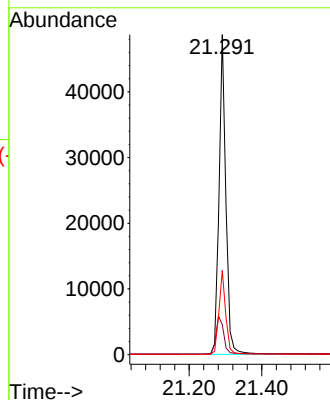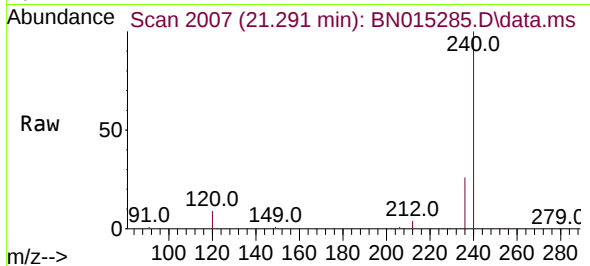

#31
Terphenyl-d14
Concen: 0.67 ng
RT: 19.733 min Scan# 1831
Delta R.T. -0.006 min
Lab File: BN015285.D
Acq: 02 Jul 2021 07:20

Tgt Ion:244 Resp: 98928
Ion Ratio Lower Upper
244 100
212 7.7 6.3 9.5
122 12.7 6.2 9.2#


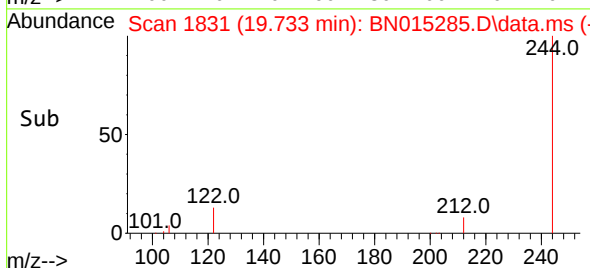
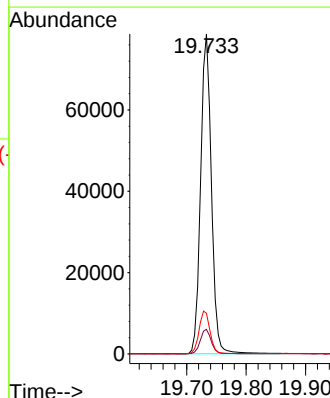
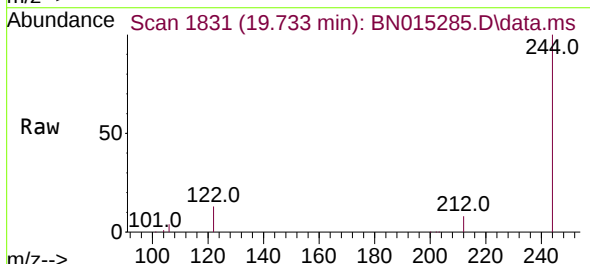


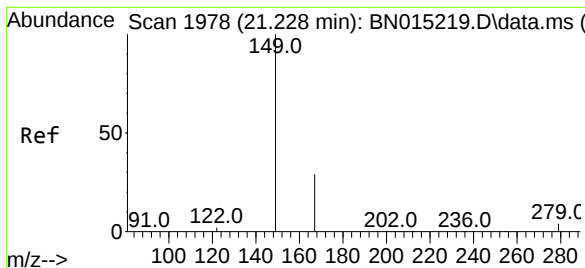

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.16 ng
 RT: 21.217 min Scan# 2000
 Delta R.T. -0.011 min
 Lab File: BN015285.D
 Acq: 02 Jul 2021 07:20

Instrument :
 BNA_N
 ClientSampleId :
 PB137445BL

Tgt Ion:149 Resp: 1506
 Ion Ratio Lower Upper
 149 100
 167 29.9 28.9 43.3
 279 4.4 4.9 7.3#

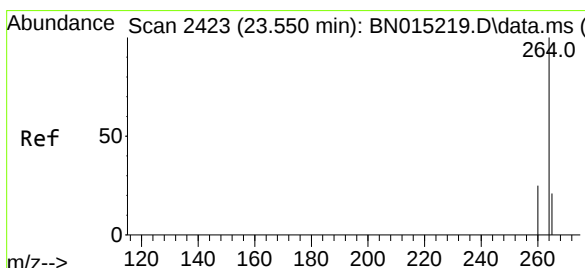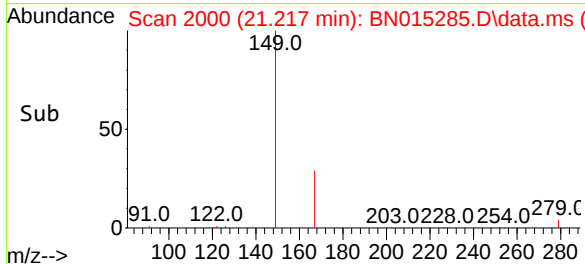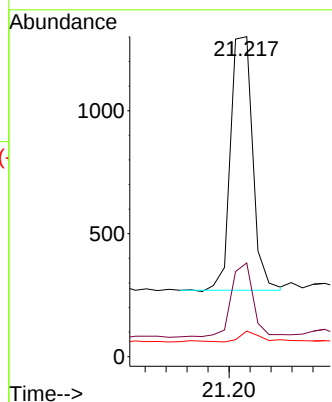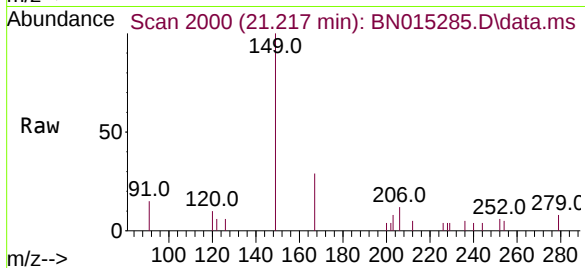

#35
 Perylene-d12
 Concen: 0.40 ng
 RT: 23.539 min Scan# 2443
 Delta R.T. -0.011 min
 Lab File: BN015285.D
 Acq: 02 Jul 2021 07:20

Tgt Ion:264 Resp: 51033
 Ion Ratio Lower Upper
 264 100
 260 25.0 20.6 31.0
 265 23.9 21.4 32.2

