
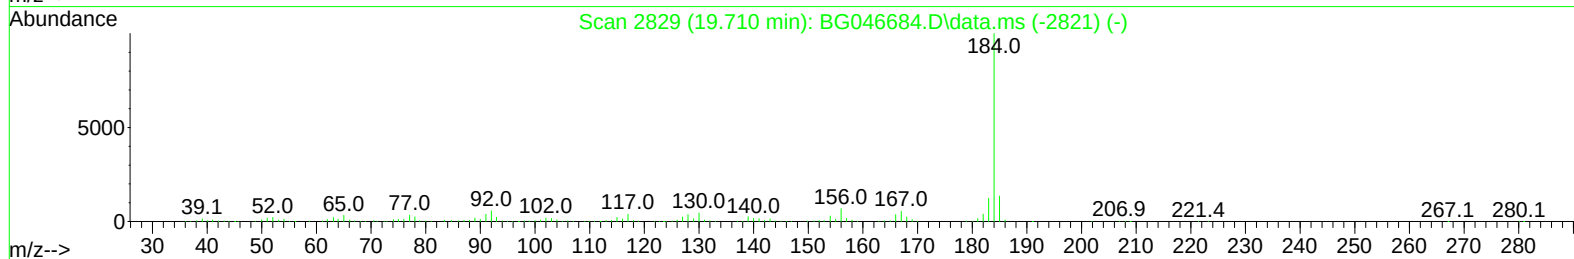
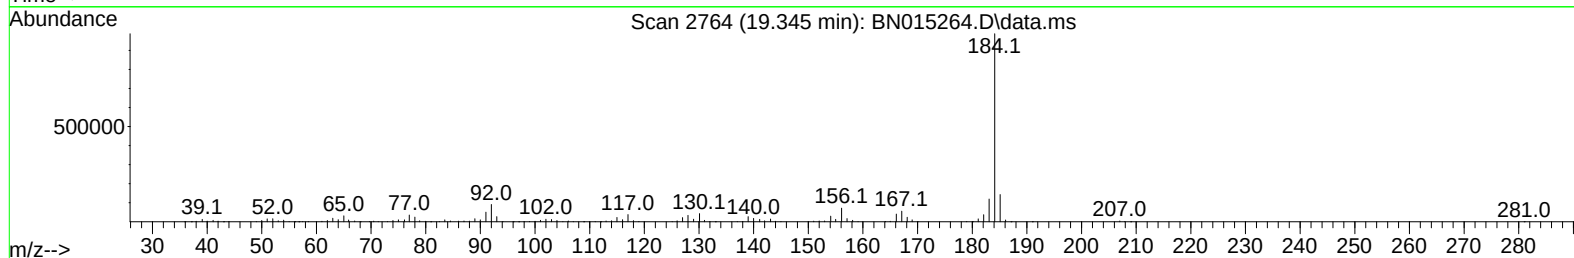


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070121\
Data File : BN015264.D
Acq On : 01 Jul 2021 17:30
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 01 18:51:16 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 10:10:58 2021
Response via : Initial Calibration

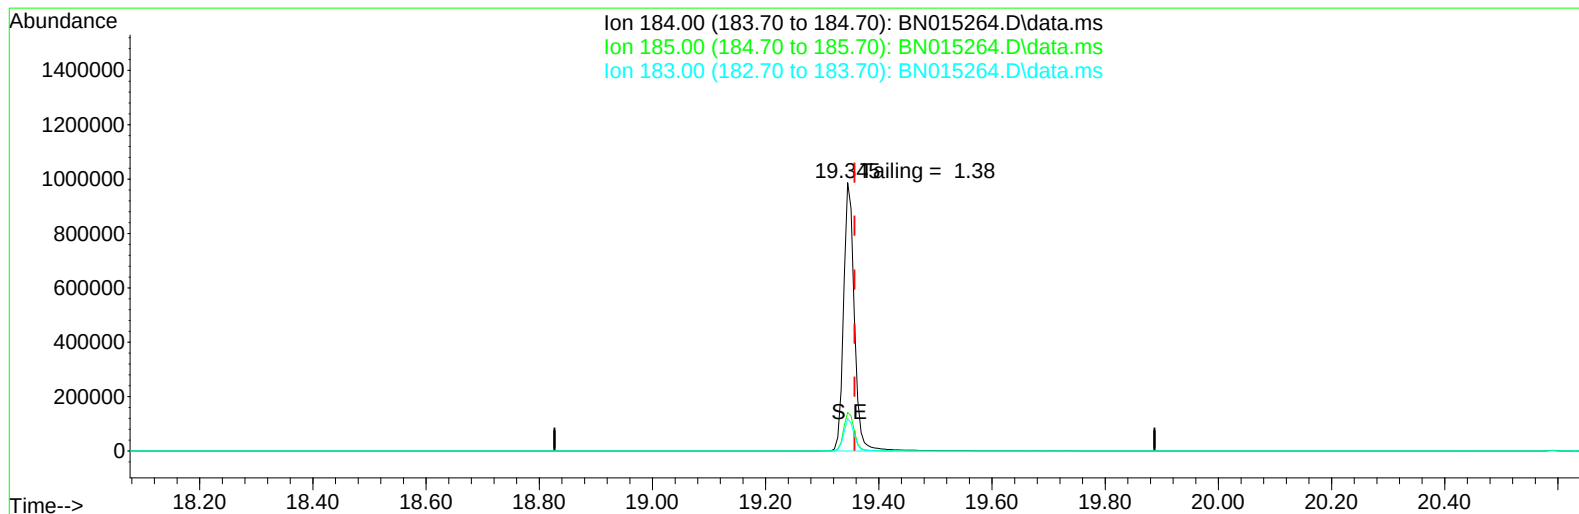

TIC: BN015264.D\data.ms

(77) Benzidine




19.345min (-0.012) 0.00 ng

response 1302641

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.46
183.00	13.20	12.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070121\
Data File : BN015264.D
Acq On : 01 Jul 2021 17:30
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 01 18:51:16 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 10:10:58 2021
Response via : Initial Calibration

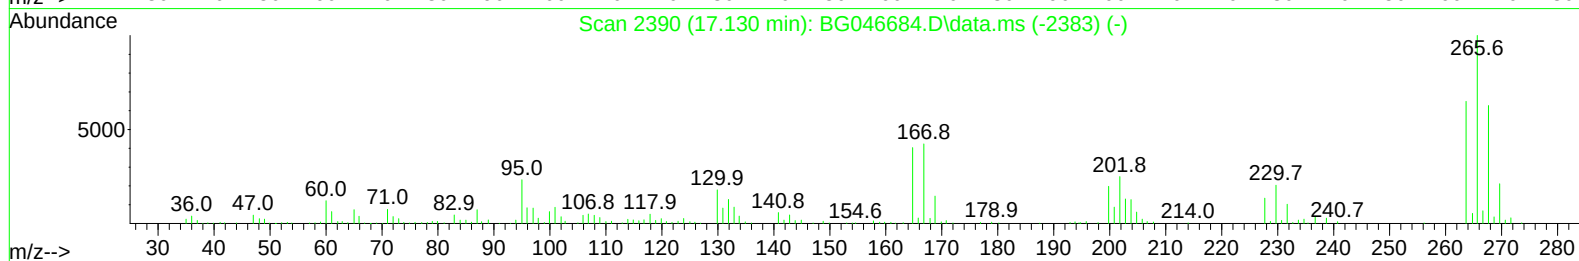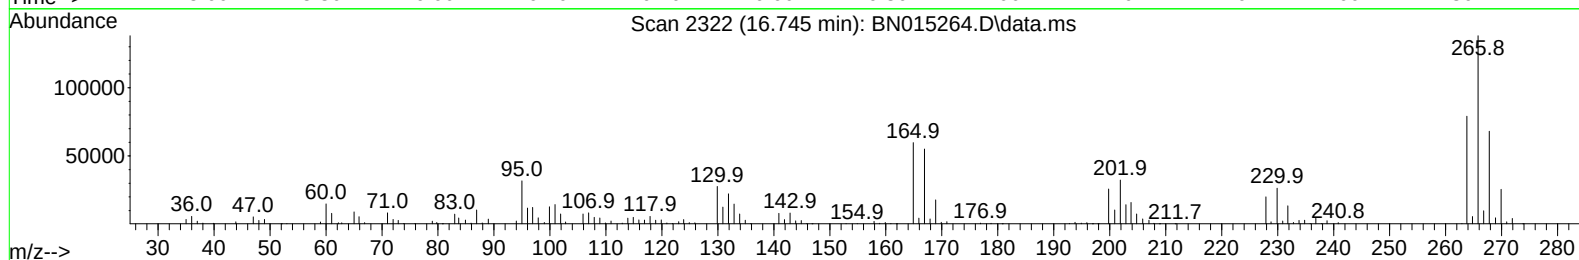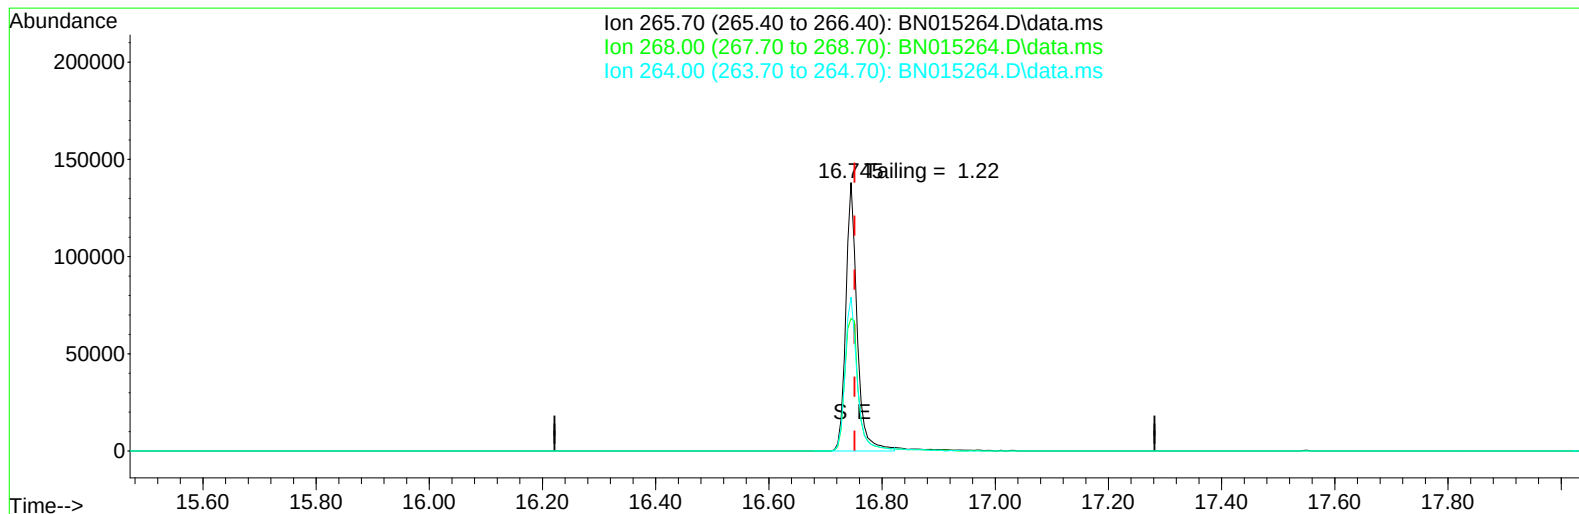

TIC: BN015264.D\data.ms

(70) Pentachlorophenol (C)

16.745min (-0.006) 20871.45 ng

response 193113

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	49.36#
264.00	61.60	57.32
0.00	0.00	0.00