

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070121\
 Data File : BN015265.D
 Acq On : 01 Jul 2021 18:07
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Quant Time: Jul 01 18:57:25 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN063021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 01 09:06:31 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.731	152	17223	0.40	ng	# 0.00
7) Naphthalene-d8	10.492	136	74562	0.40	ng	# 0.00
13) Acenaphthene-d10	14.345	164	37160	0.40	ng	0.00
19) Phenanthrene-d10	17.091	188	68783	0.40	ng	0.00
29) Chrysene-d12	21.291	240	53594	0.40	ng	#-0.01
35) Perylene-d12	23.539	264	44324	0.40	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.343	112	21323	0.49	ng	-0.02
5) Phenol-d6	6.901	99	26579	0.48	ng	0.00
8) Nitrobenzene-d5	8.870	82	23917	0.57	ng	0.00
11) 2-Methylnaphthalene-d10	12.083	152	47795	0.39	ng	0.00
14) 2,4,6-Tribromophenol	15.842	330	4255	0.49	ng	0.00
15) 2-Fluorobiphenyl	12.962	172	61323	0.41	ng	0.00
27) Fluoranthene-d10	19.133	212	71277	0.35	ng	0.00
31) Terphenyl-d14	19.733	244	50665	0.40	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.351	88	3092	0.38	ng	# 54
3) n-Nitrosodimethylamine	3.692	42	6738	0.45	ng	# 67
6) bis(2-Chloroethyl)ether	7.169	93	22669	0.42	ng	# 83
9) Naphthalene	10.543	128	84813	0.40	ng	97
10) Hexachlorobutadiene	10.834	225	16880	0.42	ng	# 99
12) 2-Methylnaphthalene	12.159	142	54245	0.40	ng	# 90
16) Acenaphthylene	14.066	152	64765	0.39	ng	98
17) Acenaphthene	14.409	154	44462	0.39	ng	100
18) Fluorene	15.398	166	53628	0.38	ng	99
20) 4,6-Dinitro-2-methylph...	15.474	198	281	0.41	ng	# 81
21) 4-Bromophenyl-phenylether	16.288	248	17386	0.40	ng	# 87
22) Hexachlorobenzene	16.397	284	20845	0.42	ng	# 92
23) Atrazine	16.555	200	9678	0.43	ng	94
24) Pentachlorophenol	16.750	266	2616	0.55	ng	98
25) Phenanthrene	17.127	178	87047	0.39	ng	99
26) Anthracene	17.225	178	67156	0.35	ng	99
28) Fluoranthene	19.157	202	91647	0.38	ng	# 97
30) Pyrene	19.525	202	85516	0.42	ng	99
32) Benzo(a)anthracene	21.281	228	58968	0.32	ng	96
33) Chrysene	21.323	228	79138	0.40	ng	98
34) Bis(2-ethylhexyl)phtha...	21.217	149	18200	0.43	ng	# 85
36) Indeno(1,2,3-cd)pyrene	25.802	276	51638	0.33	ng	# 90
37) Benzo(b)fluoranthene	22.869	252	65026	0.37	ng	# 94
38) Benzo(k)fluoranthene	22.910	252	78267	0.42	ng	# 94
39) Benzo(a)pyrene	23.444	252	62880	0.40	ng	# 86
40) Dibenzo(a,h)anthracene	25.816	278	37300	0.30	ng	# 91
41) Benzo(g,h,i)perylene	26.487	276	44730	0.33	ng	# 89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070121\
Data File : BN015265.D
Acq On : 01 Jul 2021 18:07
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Quant Time: Jul 01 18:57:25 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN063021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 01 09:06:31 2021
Response via : Initial Calibration








#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.731 min Scan# 827
 Delta R.T. -0.001 min
 Lab File: BN015265.D
 Acq: 01 Jul 2021 18:07




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4


Tgt Ion: 152 Resp: 17223
 Ion Ratio Lower Upper
 152 100
 150 156.5 119.0 178.6
 115 61.3 62.2 93.4#



#2
 1,4-Dioxane
 Concen: 0.38 ng
 RT: 3.351 min Scan# 352
 Delta R.T. -0.001 min
 Lab File: BN015265.D
 Acq: 01 Jul 2021 18:07

Tgt Ion: 88 Resp: 3092
 Ion Ratio Lower Upper
 88 100
 43 30.7 12.9 19.3#
 58 81.5 38.1 57.1#







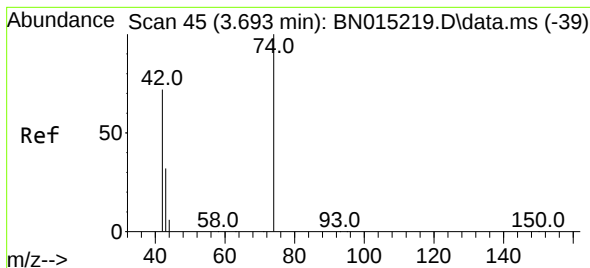

#3
n-Nitrosodimethylamine
Concen: 0.45 ng
RT: 3.692 min Scan# 389
Delta R.T. -0.001 min
Lab File: BN015265.D
Acq: 01 Jul 2021 18:07




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion: 42 Resp: 6738
Ion Ratio Lower Upper
42 100
74 138.3 149.5 224.3#
44 6.9 4.2 6.2#



#4
2-Fluorophenol
Concen: 0.49 ng
RT: 5.343 min Scan# 568
Delta R.T. -0.019 min
Lab File: BN015265.D
Acq: 01 Jul 2021 18:07

Tgt Ion: 112 Resp: 21323
Ion Ratio Lower Upper
112 100
64 58.0 39.0 58.6
63 30.0 20.6 30.8









#5
Phenol-d6
Concen: 0.48 ng
RT: 6.901 min Scan# 737
Delta R.T. -0.001 min
Lab File: BN015265.D
Acq: 01 Jul 2021 18:07




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion: 99 Resp: 26579
Ion Ratio Lower Upper
99 100
42 18.7 8.9 13.3#
71 31.9 35.6 53.4#



#6
bis(2-Chloroethyl)ether
Concen: 0.42 ng
RT: 7.169 min Scan# 766
Delta R.T. -0.001 min
Lab File: BN015265.D
Acq: 01 Jul 2021 18:07

Tgt Ion: 93 Resp: 22669
Ion Ratio Lower Upper
93 100
63 76.7 46.6 70.0#
95 32.9 28.6 42.8









#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.492 min Scan# 1062
Delta R.T. -0.001 min
Lab File: BN015265.D
Acq: 01 Jul 2021 18:07




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:136	Resp:	74562
Ion Ratio	Lower	Upper
136	100	
137	11.1	9.8 14.8
54	9.1	5.4 8.2#
68	7.1	4.9 7.3



#8
Nitrobenzene-d5
Concen: 0.57 ng
RT: 8.870 min Scan# 934
Delta R.T. -0.000 min
Lab File: BN015265.D
Acq: 01 Jul 2021 18:07

Tgt Ion: 82	Resp:	23917
Ion Ratio	Lower	Upper
82	100	
128	42.8	31.6 47.4
54	47.6	29.0 43.4#









#9
Naphthalene
Concen: 0.40 ng
RT: 10.543 min Scan# 1066
Delta R.T. -0.001 min
Lab File: BN015265.D
Acq: 01 Jul 2021 18:07




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:128 Resp: 84813
Ion Ratio Lower Upper
128 100
129 11.0 9.1 13.7
127 13.1 11.8 17.6



#10
Hexachlorobutadiene
Concen: 0.42 ng
RT: 10.834 min Scan# 1089
Delta R.T. -0.001 min
Lab File: BN015265.D
Acq: 01 Jul 2021 18:07

Tgt Ion:225 Resp: 16880
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.7 50.2 75.2









#11
2-Methylnaphthalene-d10
Concen: 0.39 ng
RT: 12.083 min Scan# 1270
Delta R.T. -0.005 min
Lab File: BN015265.D
Acq: 01 Jul 2021 18:07




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:152 Resp: 47795
Ion Ratio Lower Upper
152 100
151 20.3 16.7 25.1



#12
2-Methylnaphthalene
Concen: 0.40 ng
RT: 12.159 min Scan# 1287
Delta R.T. -0.001 min
Lab File: BN015265.D
Acq: 01 Jul 2021 18:07

Tgt Ion:142 Resp: 54245
Ion Ratio Lower Upper
142 100
141 88.3 72.3 108.5
115 34.0 40.7 61.1#









#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.345 min Scan# 1510
Delta R.T. -0.001 min
Lab File: BN015265.D
Acq: 01 Jul 2021 18:07




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:164 Resp: 37160
Ion Ratio Lower Upper
164 100
162 100.8 83.8 125.6
160 46.2 37.4 56.0



#14
2,4,6-Tribromophenol
Concen: 0.49 ng
RT: 15.842 min Scan# 1628
Delta R.T. -0.001 min
Lab File: BN015265.D
Acq: 01 Jul 2021 18:07

Tgt Ion:330 Resp: 4255
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 38.0 22.4 33.6#









#15
2-Fluorobiphenyl
Concen: 0.41 ng
RT: 12.962 min Scan# 1401
Delta R.T. -0.001 min
Lab File: BN015265.D
Acq: 01 Jul 2021 18:07




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:172 Resp: 61323
Ion Ratio Lower Upper
172 100
171 35.0 30.6 45.8
170 23.8 20.2 30.4



#16
Acenaphthylene
Concen: 0.39 ng
RT: 14.066 min Scan# 1488
Delta R.T. -0.001 min
Lab File: BN015265.D
Acq: 01 Jul 2021 18:07

Tgt Ion:152 Resp: 64765
Ion Ratio Lower Upper
152 100
151 19.5 16.7 25.1
153 13.1 10.5 15.7









#17
Acenaphthene
Concen: 0.39 ng
RT: 14.409 min Scan# 1515
Delta R.T. -0.000 min
Lab File: BN015265.D
Acq: 01 Jul 2021 18:07




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:154 Resp: 44462
Ion Ratio Lower Upper
154 100
153 113.6 90.9 136.3
152 57.4 45.8 68.8



#18
Fluorene
Concen: 0.38 ng
RT: 15.398 min Scan# 1593
Delta R.T. -0.001 min
Lab File: BN015265.D
Acq: 01 Jul 2021 18:07

Tgt Ion:166 Resp: 53628
Ion Ratio Lower Upper
166 100
165 98.3 79.2 118.8
167 13.5 10.7 16.1









#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.091 min Scan# 1730
Delta R.T. -0.000 min
Lab File: BN015265.D
Acq: 01 Jul 2021 18:07




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:188 Resp: 68783
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 10.0 9.0 13.4



#20
4,6-Dinitro-2-methylphenol
Concen: 0.41 ng
RT: 15.474 min Scan# 1599
Delta R.T. -0.014 min
Lab File: BN015265.D
Acq: 01 Jul 2021 18:07

Tgt Ion:198 Resp: 281
Ion Ratio Lower Upper
198 100
182 31.1 34.5 51.7#
77 0.0 0.0 0.0









#21
4-Bromophenyl-phenylether
Concen: 0.40 ng
RT: 16.288 min Scan# 1664
Delta R.T. -0.000 min
Lab File: BN015265.D
Acq: 01 Jul 2021 18:07




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:248 Resp: 17386
Ion Ratio Lower Upper
248 100
250 94.4 86.2 129.4
141 54.3 36.2 54.2#



#22
Hexachlorobenzene
Concen: 0.42 ng
RT: 16.397 min Scan# 1673
Delta R.T. -0.013 min
Lab File: BN015265.D
Acq: 01 Jul 2021 18:07

Tgt Ion:284 Resp: 20845
Ion Ratio Lower Upper
284 100
142 35.2 22.2 33.2#
249 31.3 26.6 39.8





#23

Atrazine

Concen: 0.43 ng

RT: 16.555 min Scan# 1686

Delta R.T. -0.001 min

Lab File: BN015265.D

Acq: 01 Jul 2021 18:07





Tgt Ion:200 Resp: 9678

Ion Ratio Lower Upper

200 100

173 27.2 21.7 32.5

215 47.8 43.1 64.7



#24

Pentachlorophenol

Concen: 0.55 ng

RT: 16.750 min Scan# 1702

Delta R.T. -0.001 min

Lab File: BN015265.D

Acq: 01 Jul 2021 18:07




Tgt Ion:266 Resp: 2616

Ion Ratio Lower Upper

266 100

264 62.0 51.0 76.4

268 64.9 50.6 76.0









#25
Phenanthrene
Concen: 0.39 ng
RT: 17.127 min Scan# 1733
Delta R.T. -0.001 min
Lab File: BN015265.D
Acq: 01 Jul 2021 18:07




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:178 Resp: 87047
Ion Ratio Lower Upper
178 100
176 18.9 15.6 23.4
179 15.4 12.1 18.1



#26
Anthracene
Concen: 0.35 ng
RT: 17.225 min Scan# 1741
Delta R.T. -0.000 min
Lab File: BN015265.D
Acq: 01 Jul 2021 18:07

Tgt Ion:178 Resp: 67156
Ion Ratio Lower Upper
178 100
176 18.3 15.1 22.7
179 15.2 12.2 18.2







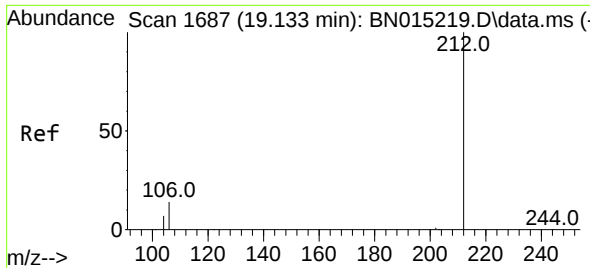

#27
Fluoranthene-d10
Concen: 0.35 ng
RT: 19.133 min Scan# 2031
Delta R.T. -0.000 min
Lab File: BN015265.D
Acq: 01 Jul 2021 18:07




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:212 Resp: 71277
Ion Ratio Lower Upper
212 100
106 14.1 7.0 10.6#
104 7.8 4.1 6.1#

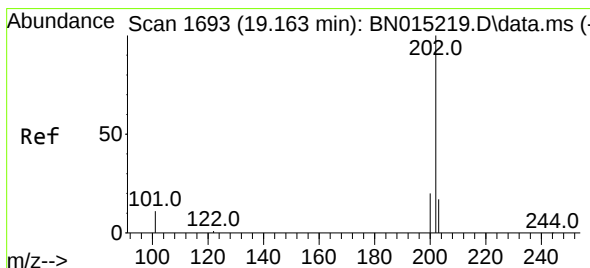

#28
Fluoranthene
Concen: 0.38 ng
RT: 19.157 min Scan# 2036
Delta R.T. -0.006 min
Lab File: BN015265.D
Acq: 01 Jul 2021 18:07

Tgt Ion:202 Resp: 91647
Ion Ratio Lower Upper
202 100
101 11.6 6.6 10.0#
203 17.3 13.9 20.9





#29

Chrysene-d12

Concen: 0.40 ng

RT: 21.291 min Scan# 2328

Delta R.T. -0.012 min

Lab File: BN015265.D

Acq: 01 Jul 2021 18:07





Tgt Ion:240	Resp:	53594
Ion Ratio	Lower	Upper
240	100	
120	10.6	4.2 6.4#
236	26.4	21.4 32.2

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4



#30

Pyrene

Concen: 0.42 ng




RT: 19.525 min Scan# 2110


Delta R.T. -0.005 min

Lab File: BN015265.D

Acq: 01 Jul 2021 18:07

Tgt Ion:202	Resp:	85516
Ion Ratio	Lower	Upper
202	100	
200	20.5	16.9 25.3
203	17.3	13.9 20.9









#31
 Terphenyl-d14
 Concen: 0.40 ng
 RT: 19.733 min Scan# 2152
 Delta R.T. -0.006 min
 Lab File: BN015265.D
 Acq: 01 Jul 2021 18:07




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Tgt Ion:244 Resp: 50665
 Ion Ratio Lower Upper
 244 100
 212 7.9 6.3 9.5
 122 13.7 6.2 9.2#



#32
 Benzo(a)anthracene
 Concen: 0.32 ng
 RT: 21.281 min Scan# 2327
 Delta R.T. -0.000 min
 Lab File: BN015265.D
 Acq: 01 Jul 2021 18:07

Tgt Ion:228 Resp: 58968
 Ion Ratio Lower Upper
 228 100
 226 25.8 23.0 34.6
 229 19.8 15.7 23.5









#33
Chrysene
Concen: 0.40 ng
RT: 21.323 min Scan# 2331
Delta R.T. -0.012 min
Lab File: BN015265.D
Acq: 01 Jul 2021 18:07




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:	228	Resp:	79138
Ion Ratio	Lower	Upper	
228	100		
226	30.6	25.0	37.6
229	19.0	15.9	23.9

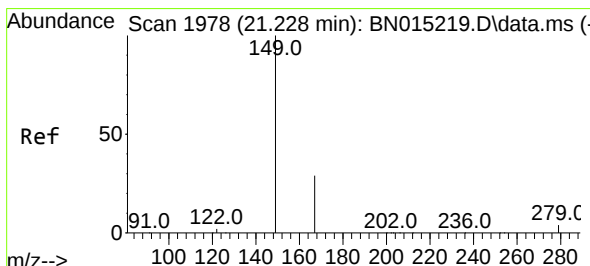

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.43 ng
RT: 21.217 min Scan# 2321
Delta R.T. -0.011 min
Lab File: BN015265.D
Acq: 01 Jul 2021 18:07


Tgt Ion:	149	Resp:	18200
Ion Ratio	Lower	Upper	
149	100		
167	26.6	28.9	43.3#
279	3.2	4.9	7.3#








#35
Perylene-d12
Concen: 0.40 ng
RT: 23.539 min Scan# 2764
Delta R.T. -0.011 min
Lab File: BN015265.D
Acq: 01 Jul 2021 18:07


Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4





Tgt Ion:264 Resp: 44324
Ion Ratio Lower Upper
264 100
260 25.4 20.6 31.0
265 24.1 21.4 32.2



#36
Indeno(1,2,3-cd)pyrene
Concen: 0.33 ng
RT: 25.802 min Scan# 3425
Delta R.T. -0.011 min
Lab File: BN015265.D
Acq: 01 Jul 2021 18:07



Tgt Ion:276 Resp: 51638
Ion Ratio Lower Upper
276 100
138 23.1 10.0 15.0#
277 24.7 20.4 30.6









#37
Benzo(b)fluoranthene
Concen: 0.37 ng
RT: 22.869 min Scan# 2568
Delta R.T. -0.008 min
Lab File: BN015265.D
Acq: 01 Jul 2021 18:07




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:252 Resp: 65026
Ion Ratio Lower Upper
252 100
253 22.6 18.5 27.7
125 14.8 5.8 8.6#



#38
Benzo(k)fluoranthene
Concen: 0.42 ng
RT: 22.910 min Scan# 2580
Delta R.T. -0.011 min
Lab File: BN015265.D
Acq: 01 Jul 2021 18:07

Tgt Ion:252 Resp: 78267
Ion Ratio Lower Upper
252 100
253 22.2 19.1 28.7
125 11.1 5.4 8.0#





#39

Benzo(a)pyrene

Concen: 0.40 ng

RT: 23.444 min Scan# 2736

Delta R.T. -0.011 min

Lab File: BN015265.D

Acq: 01 Jul 2021 18:07





Tgt Ion:252	Resp:	62880
Ion Ratio	Lower	Upper
252	100	
253	23.7	19.4 29.2
125	26.3	7.4 11.2#

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4



#40

Dibenzo(a,h)anthracene

Concen: 0.30 ng




RT: 25.816 min Scan# 3429


Delta R.T. -0.011 min

Lab File: BN015265.D

Acq: 01 Jul 2021 18:07

Tgt Ion:278	Resp:	37300
Ion Ratio	Lower	Upper
278	100	
139	18.9	9.0 13.4#
279	24.0	21.0 31.4





#41
Benzo(g,h,i)perylene
Concen: 0.33 ng
RT: 26.487 min Scan# 3625
Delta R.T. -0.011 min
Lab File: BN015265.D
Acq: 01 Jul 2021 18:07

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:276 Resp: 44730
Ion Ratio Lower Upper
276 100
277 23.8 19.7 29.5
138 24.4 9.8 14.6#

