


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070121\
 Data File : BN015264.D
 Acq On : 01 Jul 2021 17:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN063021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 01 09:06:31 2021

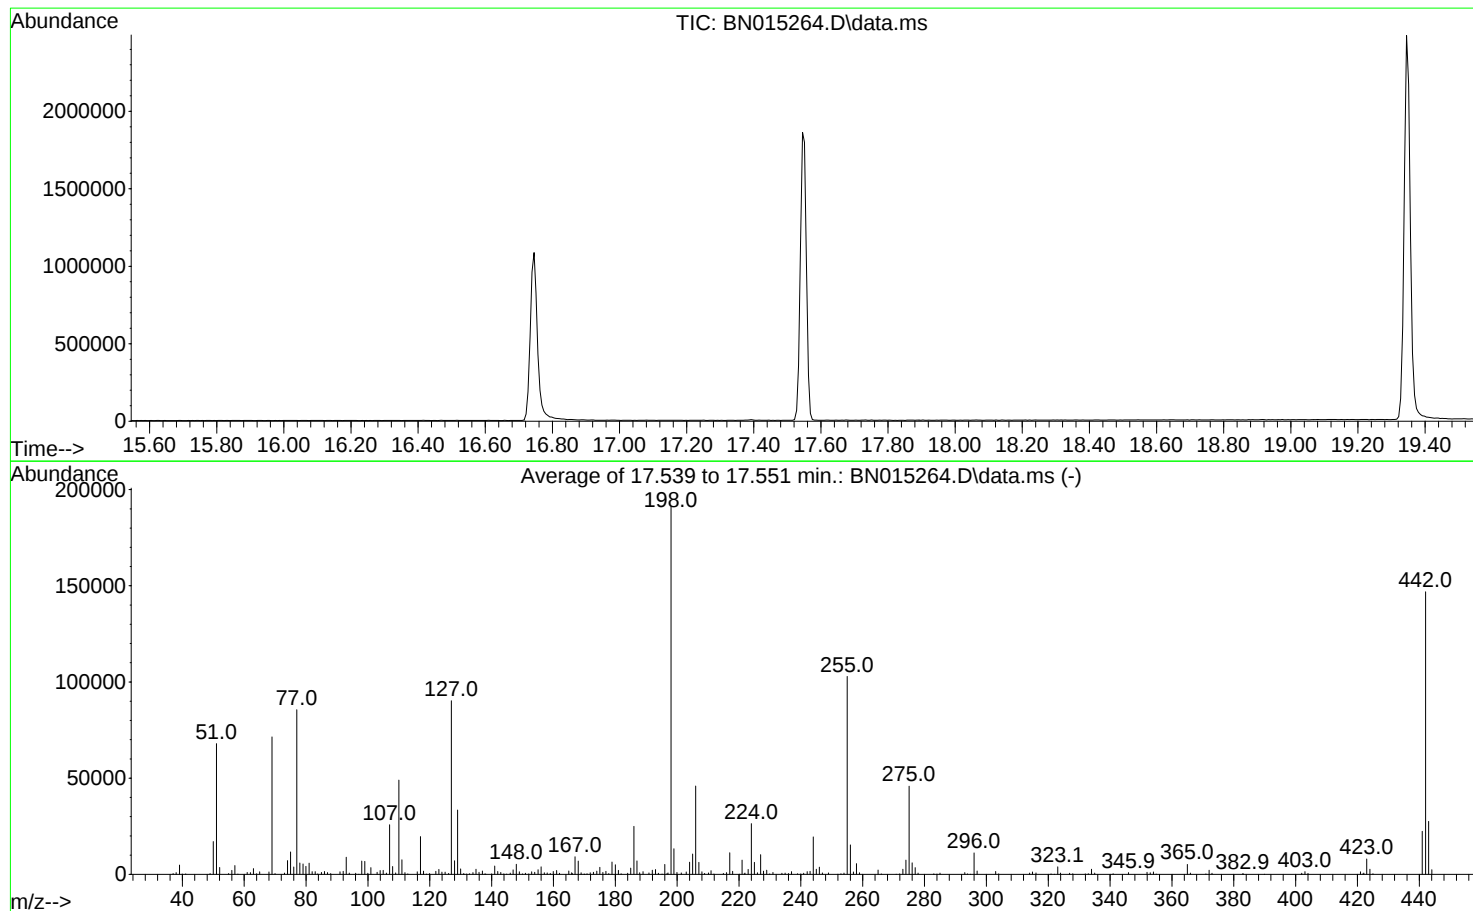




AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	67963	PASS
68	69	0.00	2	1.8	1268	PASS
69	198	0.00	100	37.4	71421	PASS
70	69	0.00	2	0.6	398	PASS
127	198	10	80	47.2	90221	PASS
197	198	0.00	2	0.4	758	PASS
198	198	100	100	100.0	191211	PASS
199	198	5	9	7.0	13292	PASS
275	198	10	60	24.0	45800	PASS
365	198	1	100	2.7	5181	PASS
441	198	0.01	100	11.7	22388	PASS
442	442	50	100	100.0	146904	PASS
443	442	15	24	18.7	27539	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070121\
Data File : BN015264.D
Acq On : 01 Jul 2021 17:30
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 01 18:51:16 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 10:10:58 2021
Response via : Initial Calibration

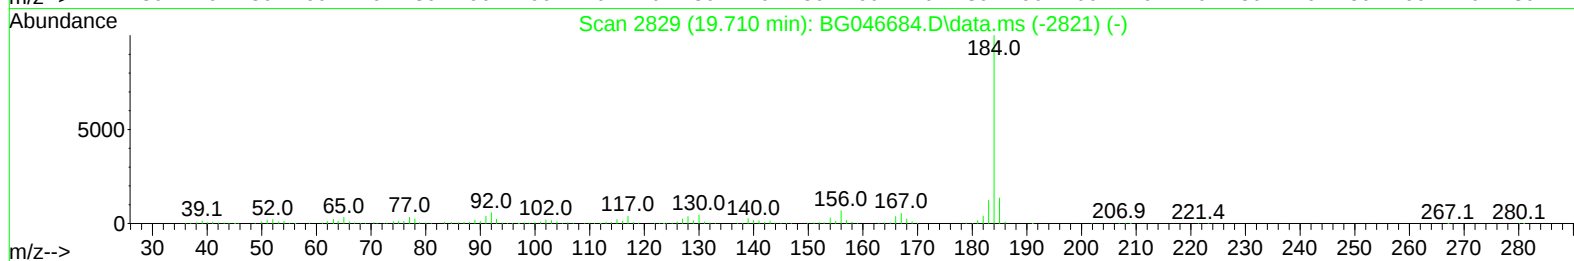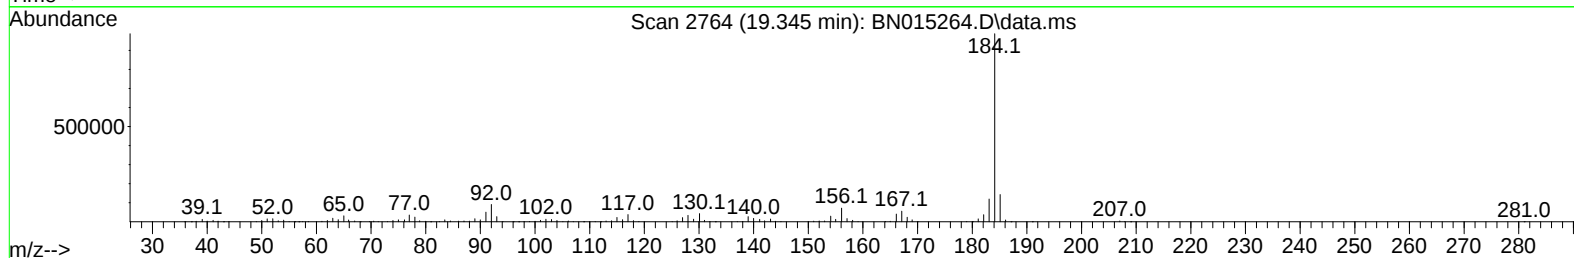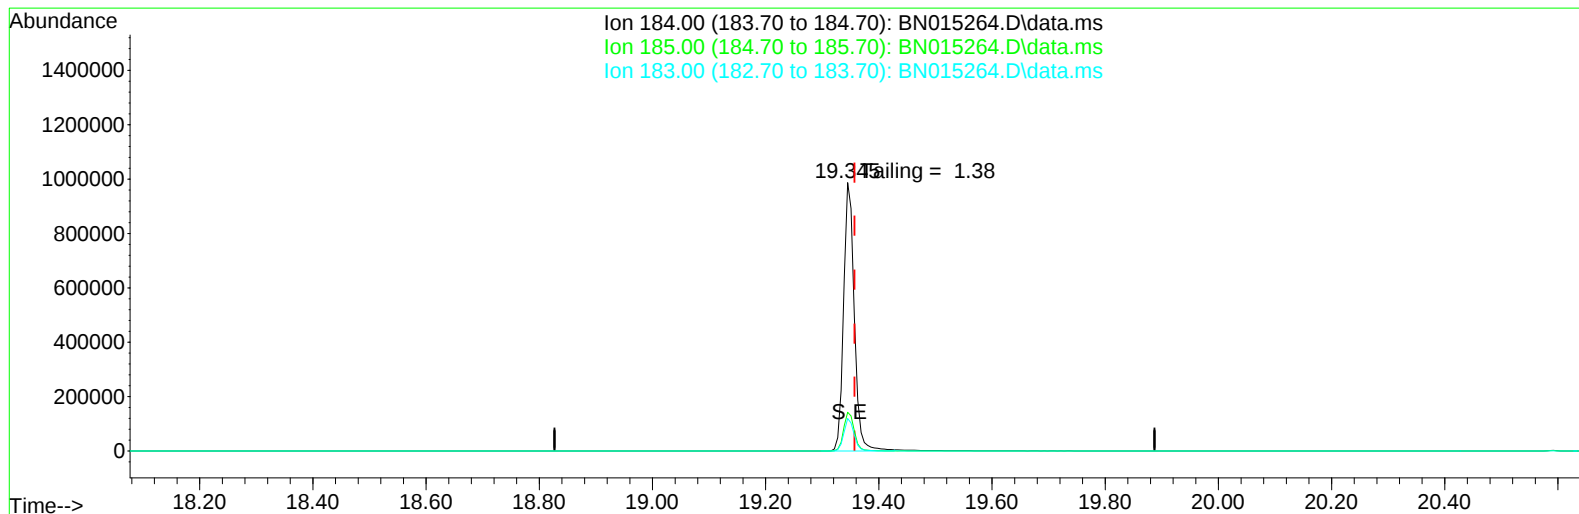

TIC: BN015264.D\data.ms

(77) Benzidine

19.345min (-0.012) 0.00 ng




response 1302641

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.46
183.00	13.20	12.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070121\
Data File : BN015264.D
Acq On : 01 Jul 2021 17:30
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 01 18:51:16 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 10:10:58 2021
Response via : Initial Calibration

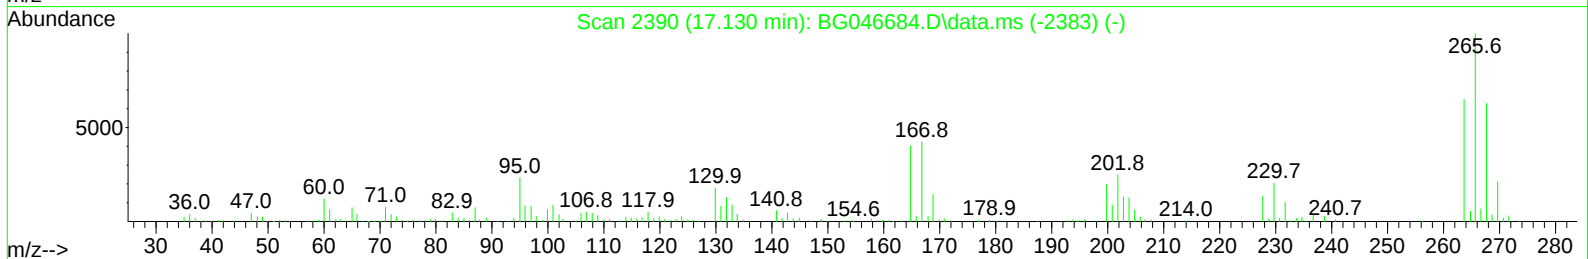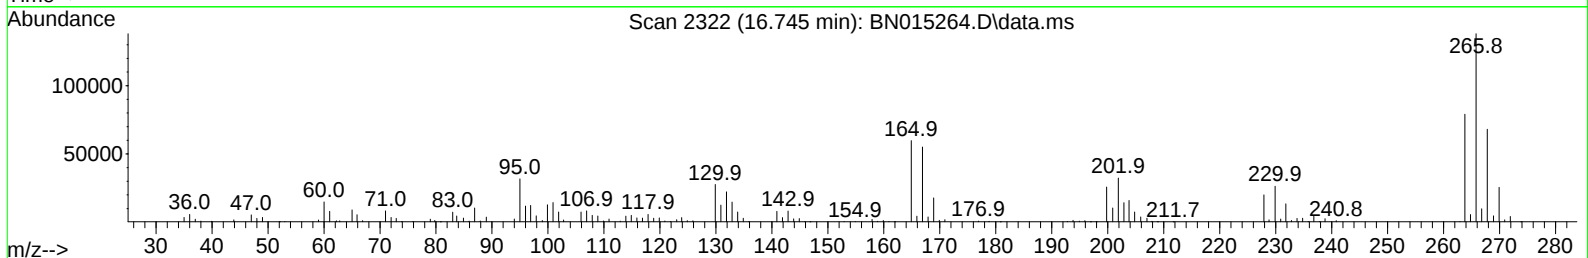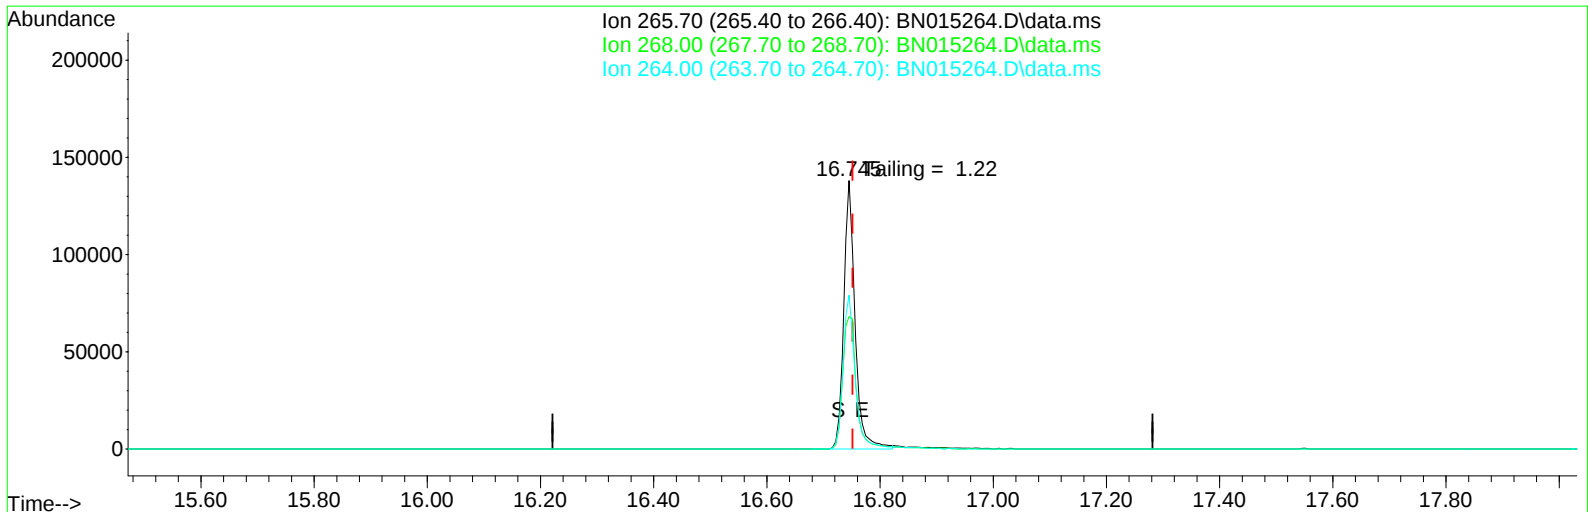

TIC: BN015264.D\data.ms

(70) Pentachlorophenol (C)

16.745min (-0.006) 20871.45 ng

response 193113

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	49.36#
264.00	61.60	57.32
0.00	0.00	0.00

Instrument :
BNA_N
ClientSampleId :
DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/1/2021	BNA_N	<u>BN015264.D</u>
Compound Name	Response	Retention Time
DDT	522919	20.59
DDD	20544	20.15
DDE	1275	19.63
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21819	544738	4.01