


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070121\
 Data File : BN015283.D
 Acq On : 02 Jul 2021 06:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN063021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 01 09:06:31 2021

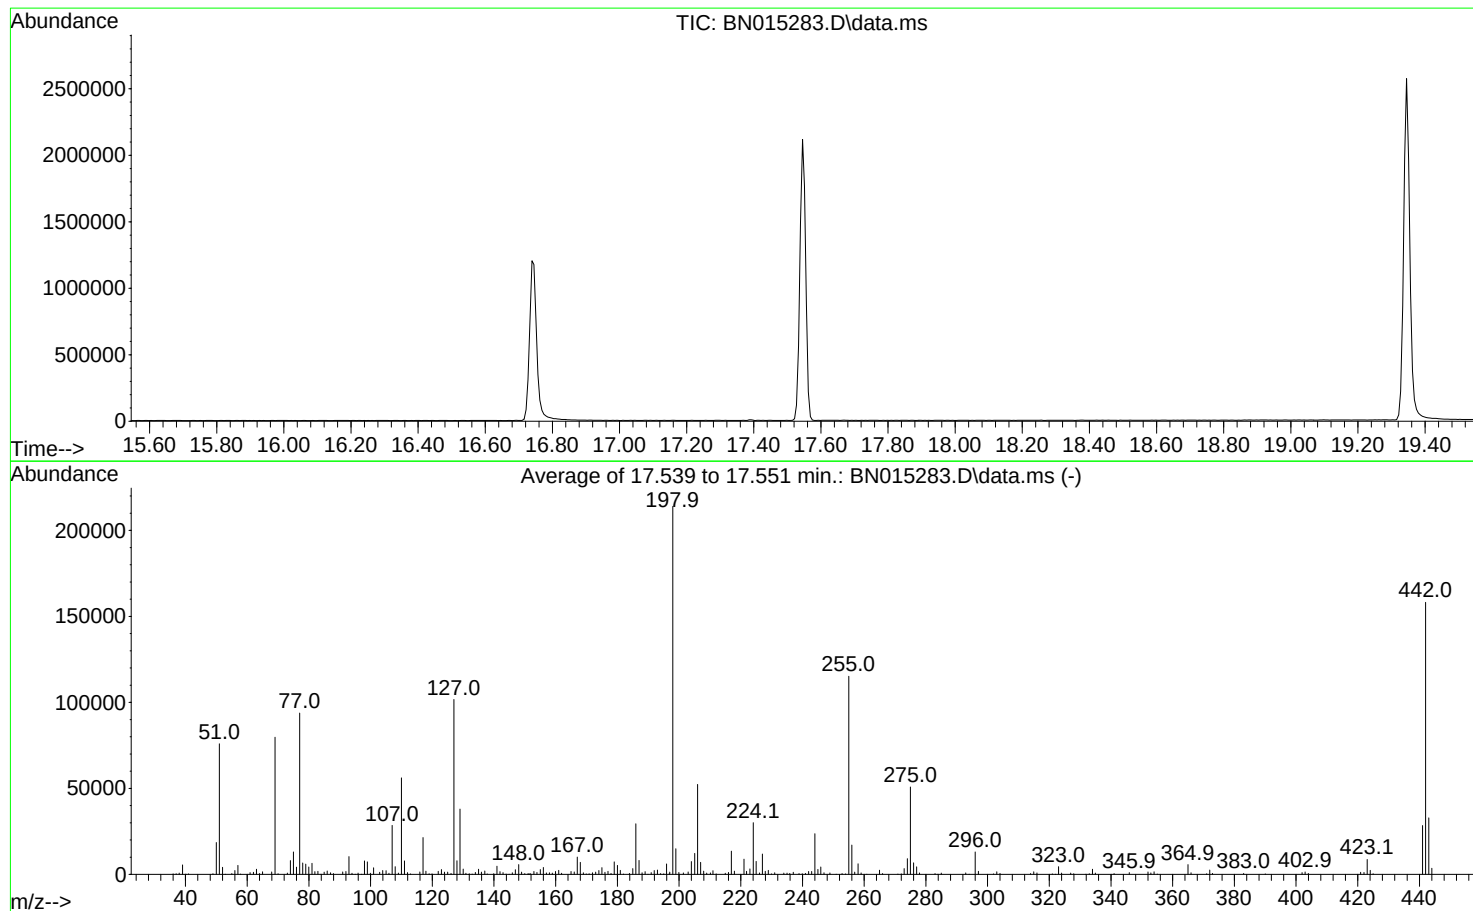

AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	75912	PASS
68	69	0.00	2	1.8	1406	PASS
69	198	0.00	100	37.3	79709	PASS
70	69	0.00	2	0.5	417	PASS
127	198	10	80	47.6	101736	PASS
197	198	0.00	2	0.6	1314	PASS
198	198	100	100	100.0	213909	PASS
199	198	5	9	7.0	14869	PASS
275	198	10	60	23.7	50776	PASS
365	198	1	100	2.7	5674	PASS
441	198	0.01	100	13.3	28406	PASS
442	442	50	100	100.0	158205	PASS
443	442	15	24	20.8	32851	PASS

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/1/2021	BNA_N	<u>BN015283.D</u>
Compound Name	Response	Retention Time
DDT	600347	20.586
DDD	19993	20.145
DDE	1582	19.639
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21575	621922	3.47

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070121\
Data File : BN015283.D
Acq On : 02 Jul 2021 06:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 02 07:52:34 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 10:10:58 2021
Response via : Initial Calibration

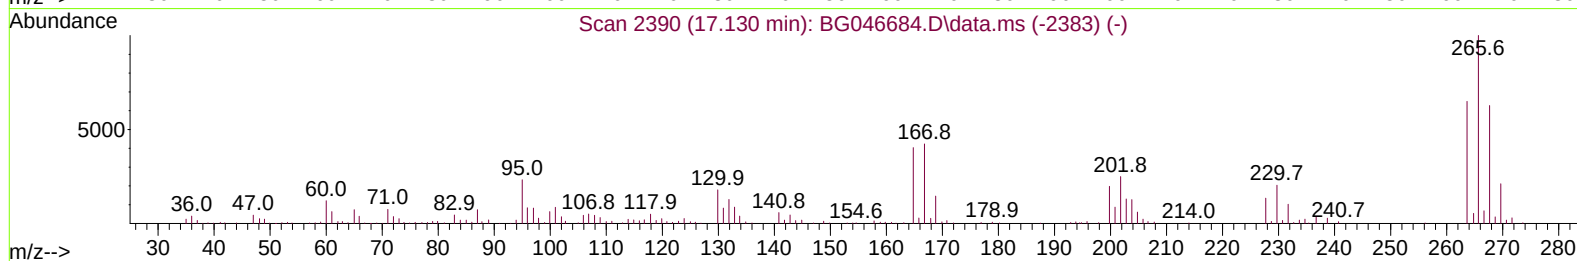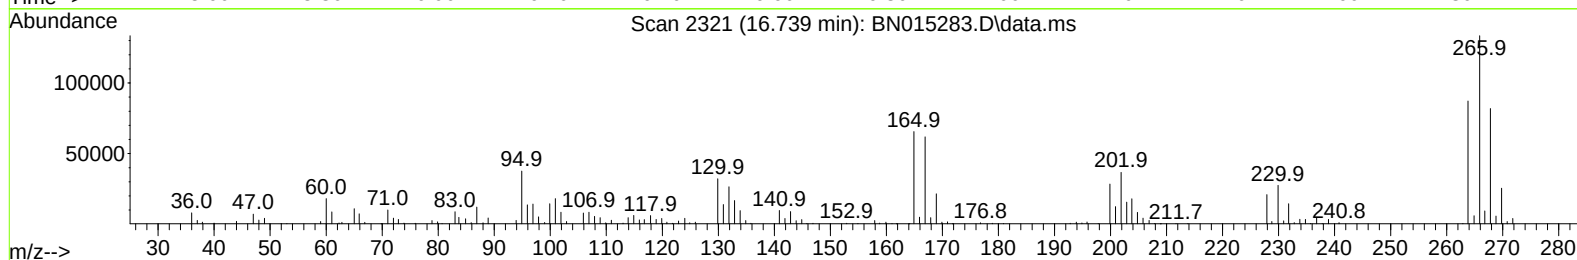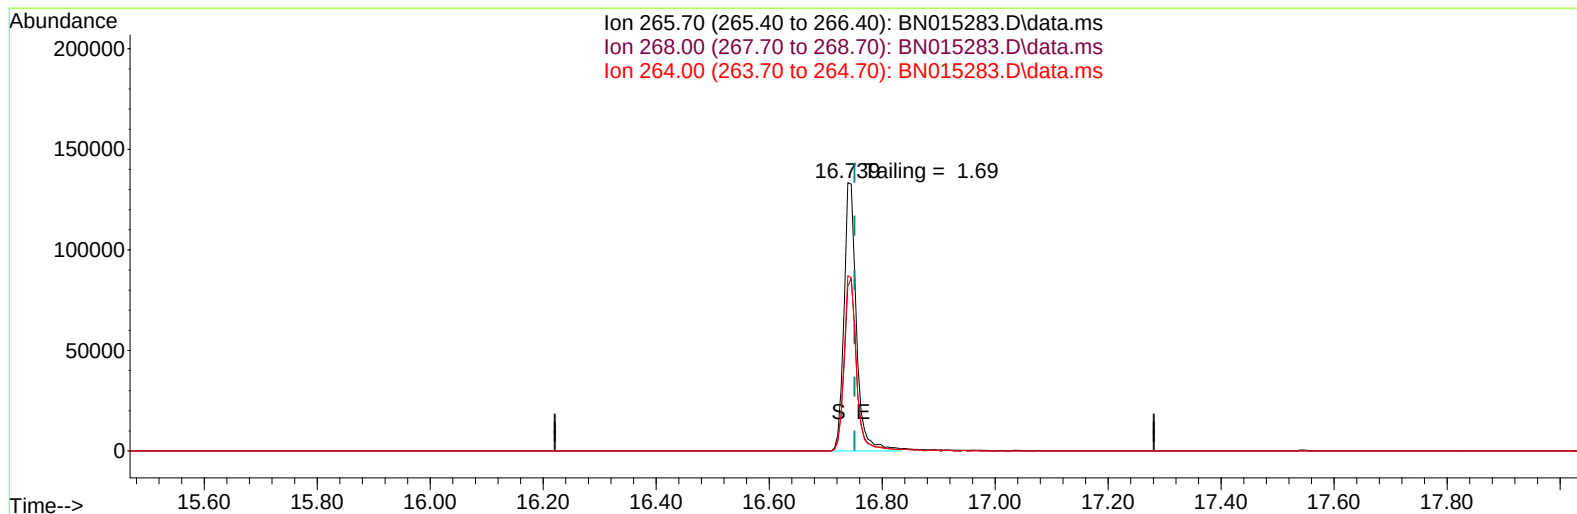

TIC: BN015283.D\data.ms

(70) Pentachlorophenol (C)

16.739min (-0.012) 24061.85 ng




response 206015

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.40
264.00	61.60	65.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070121\
Data File : BN015283.D
Acq On : 02 Jul 2021 06:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 02 07:52:34 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 10:10:58 2021
Response via : Initial Calibration

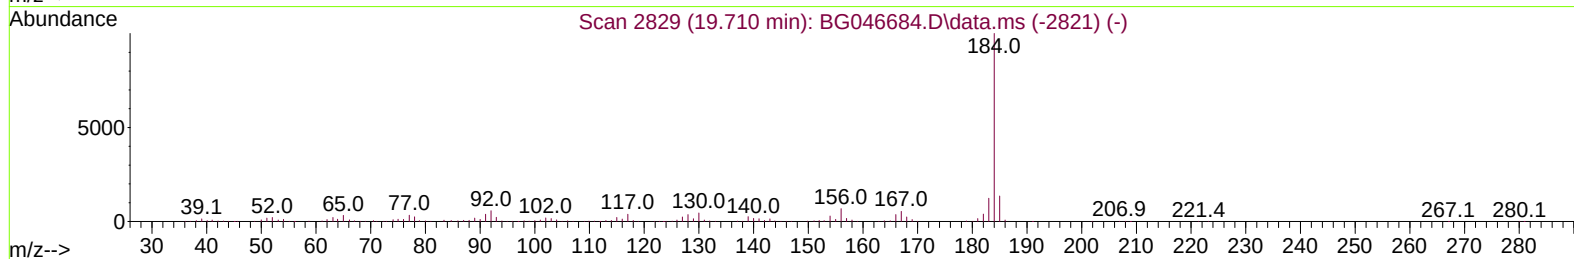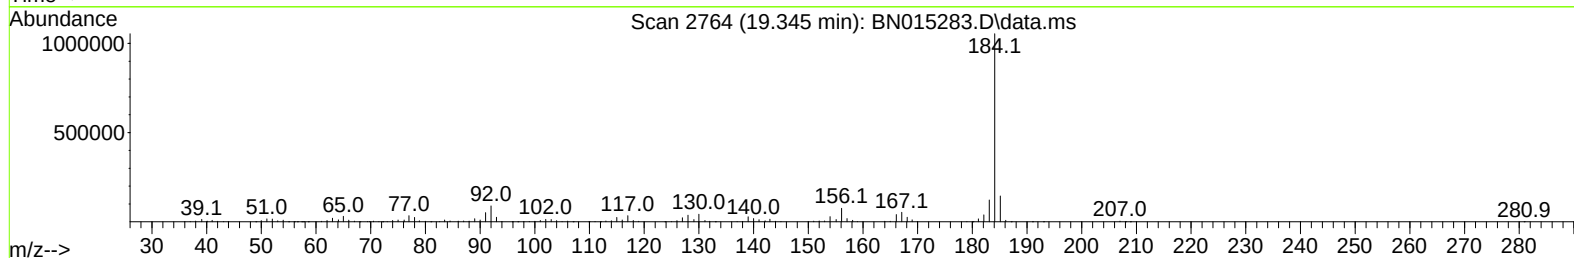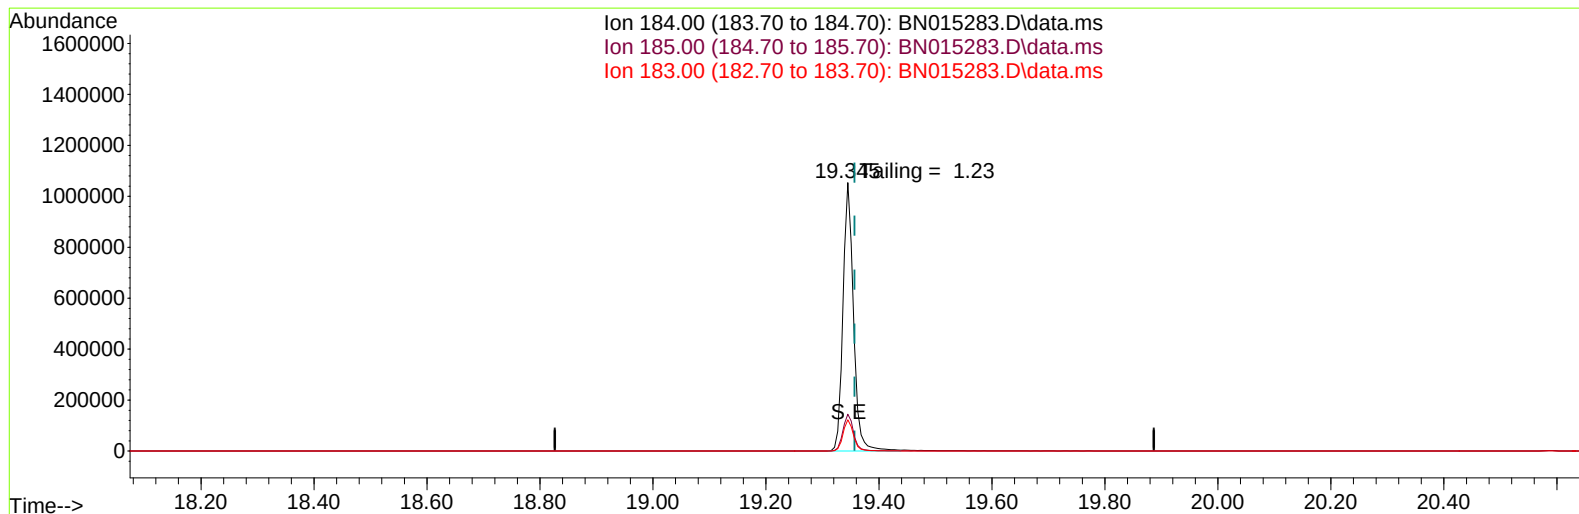

TIC: BN015283.D\data.ms

(77) Benzidine

19.345min (-0.012) 0.00 ng

response 1364779

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.70
183.00	13.20	11.63
0.00	0.00	0.00