


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070621\
 Data File : BN015335.D
 Acq On : 06 Jul 2021 11:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN063021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 01 09:06:31 2021

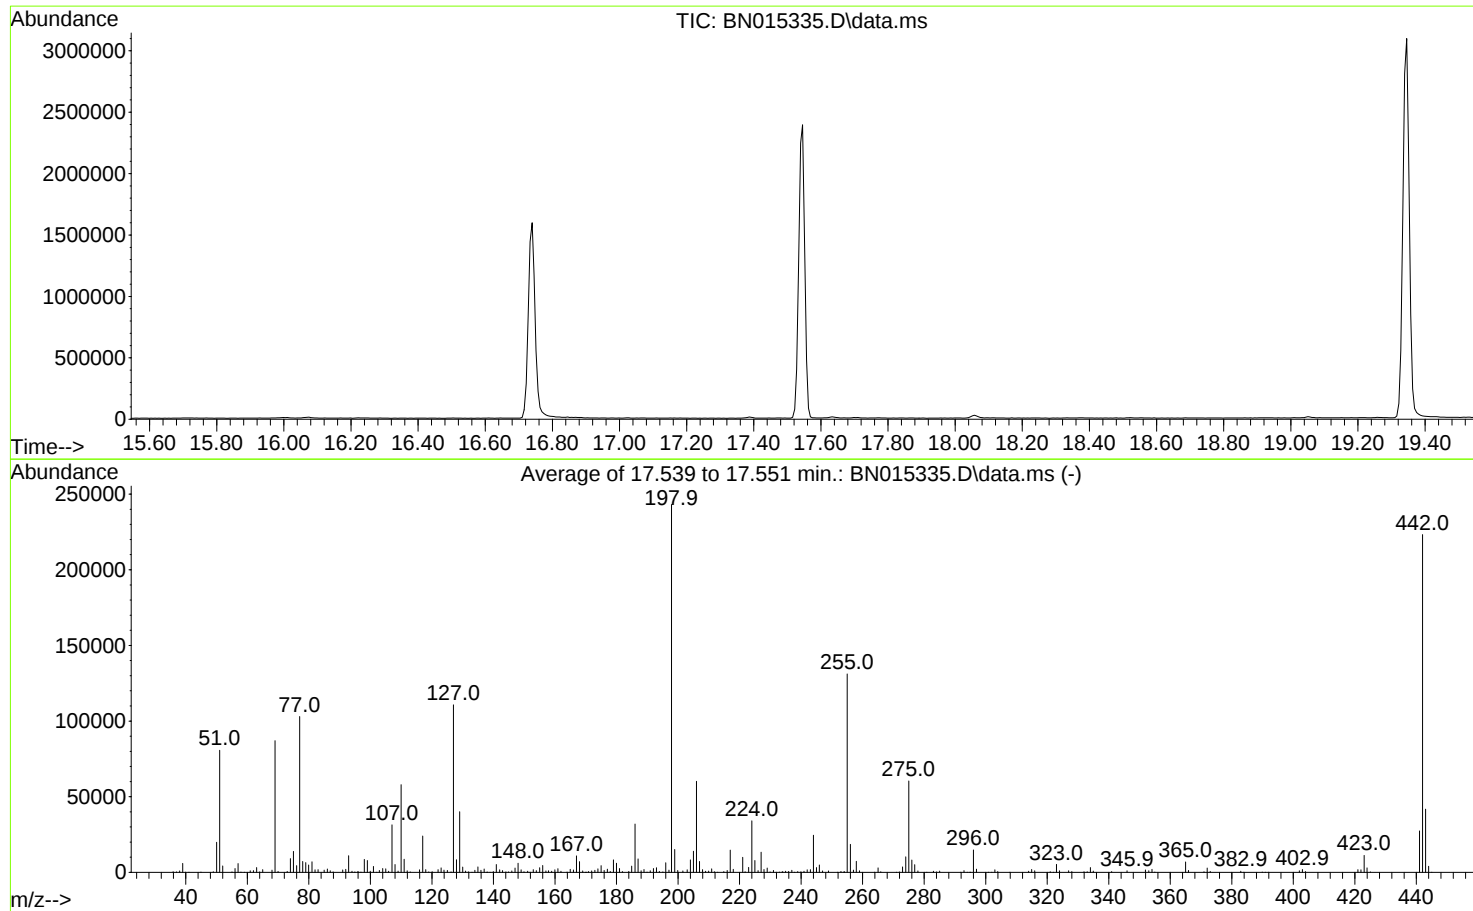

AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	80653	PASS
68	69	0.00	2	1.7	1472	PASS
69	198	0.00	100	35.8	87051	PASS
70	69	0.00	2	0.7	637	PASS
127	198	10	80	45.6	110768	PASS
197	198	0.00	2	0.6	1527	PASS
198	198	100	100	100.0	243157	PASS
199	198	5	9	6.2	15182	PASS
275	198	10	60	24.8	60376	PASS
365	198	1	100	2.8	6888	PASS
441	198	0.01	100	11.2	27355	PASS
442	442	50	100	100.0	223275	PASS
443	442	15	24	18.7	41829	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/6/2021	BNA_N	<u>BN015335.D</u>
Compound Name	Response	Retention Time
DDT	728522	20.59
DDD	1101	20.14
DDE	1082	19.63
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2183	730705	0.30

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070621\
Data File : BN015335.D
Acq On : 06 Jul 2021 11:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 06 13:13:17 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 10:10:58 2021
Response via : Initial Calibration

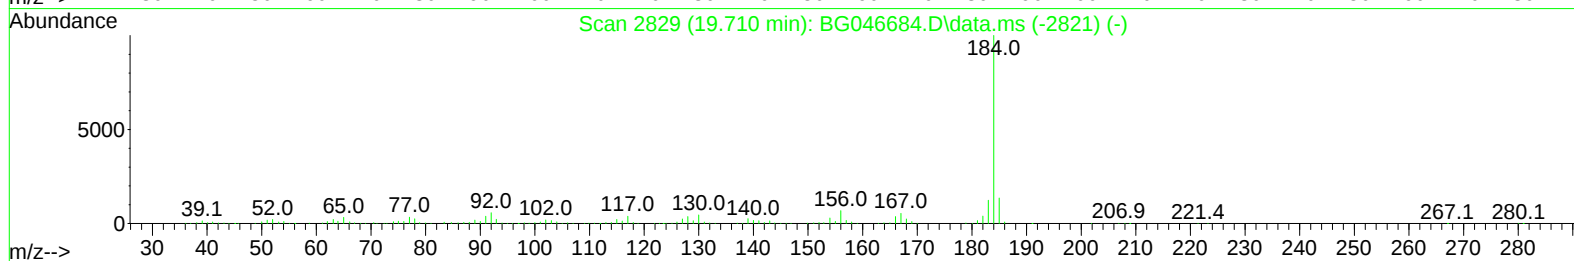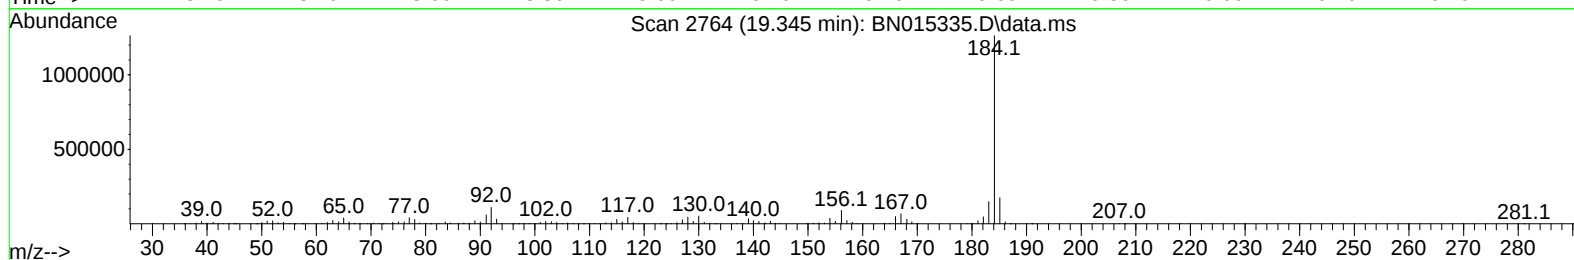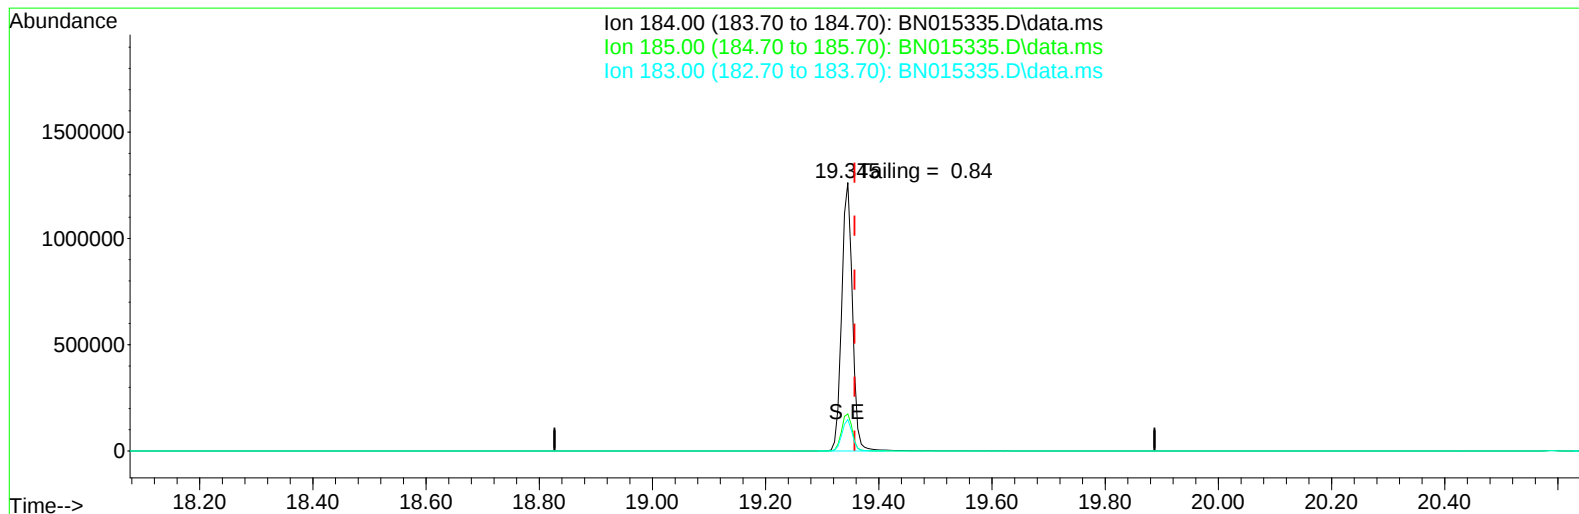

TIC: BN015335.D\data.ms

(77) Benzidine

19.345min (-0.012) 0.00 ng




response 1666989

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.84
183.00	13.20	11.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070621\
 Data File : BN015335.D
 Acq On : 06 Jul 2021 11:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jul 06 13:13:17 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 23 10:10:58 2021
 Response via : Initial Calibration

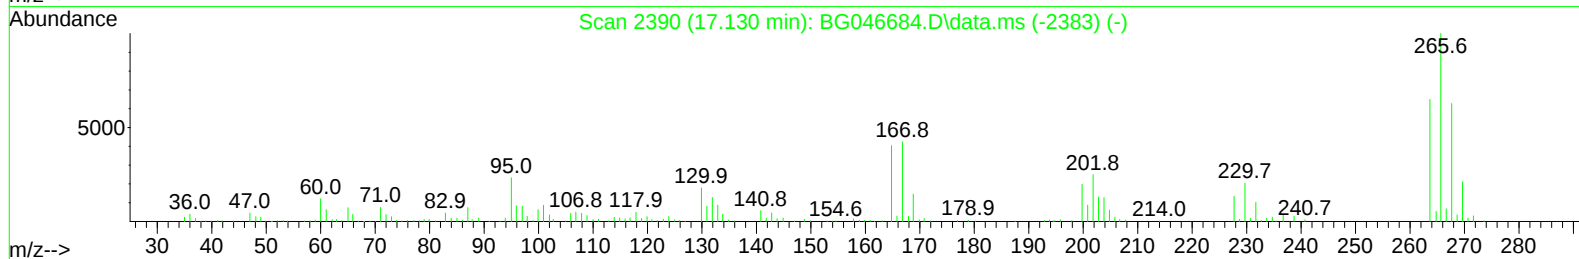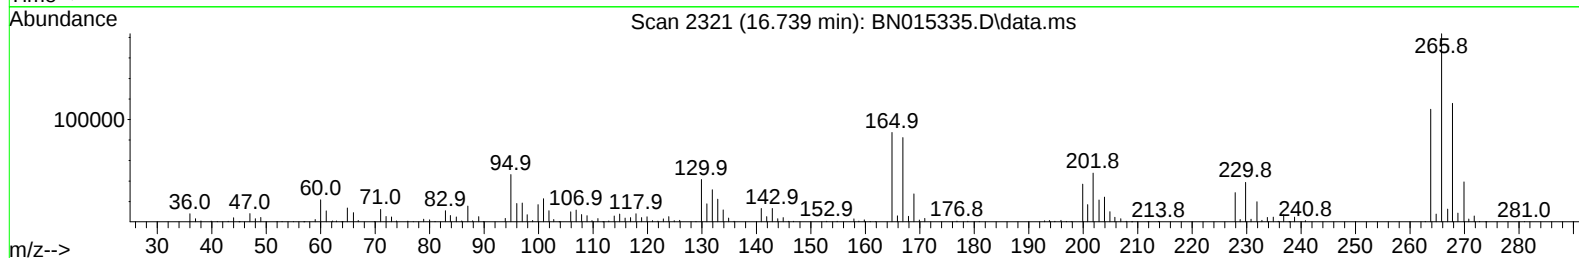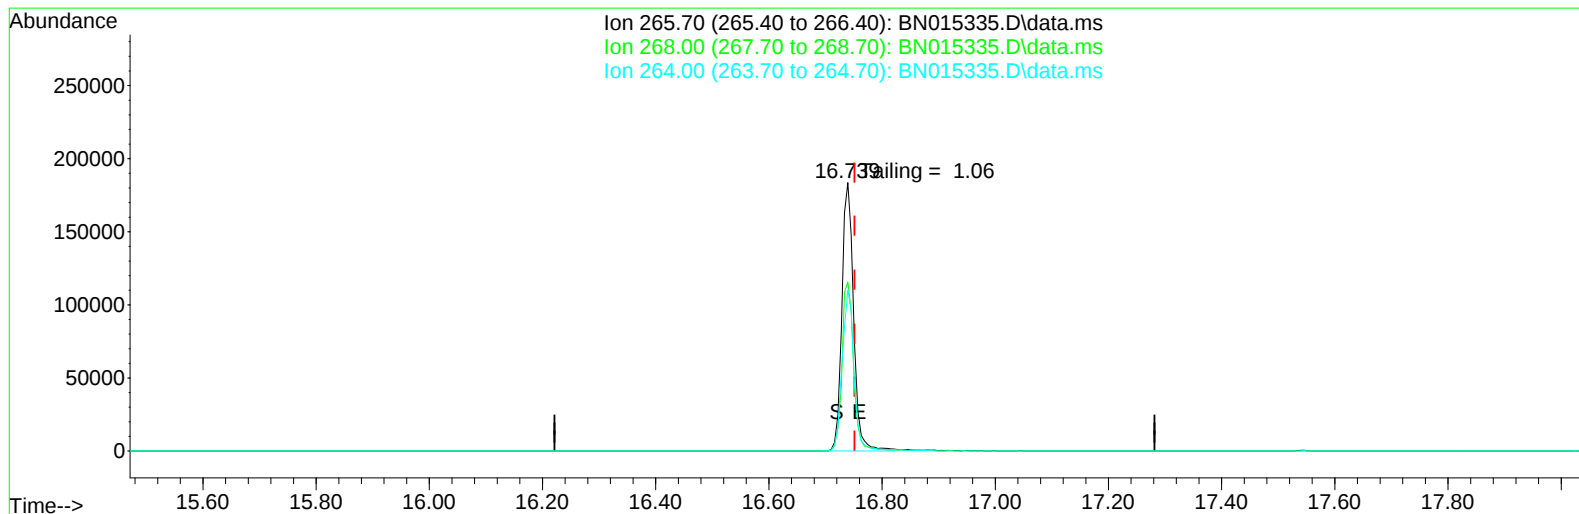

TIC: BN015335.D\data.ms

(70) Pentachlorophenol (C)

16.739min (-0.012) 22575.42 ng

response 265395

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.02
264.00	61.60	59.92
0.00	0.00	0.00