
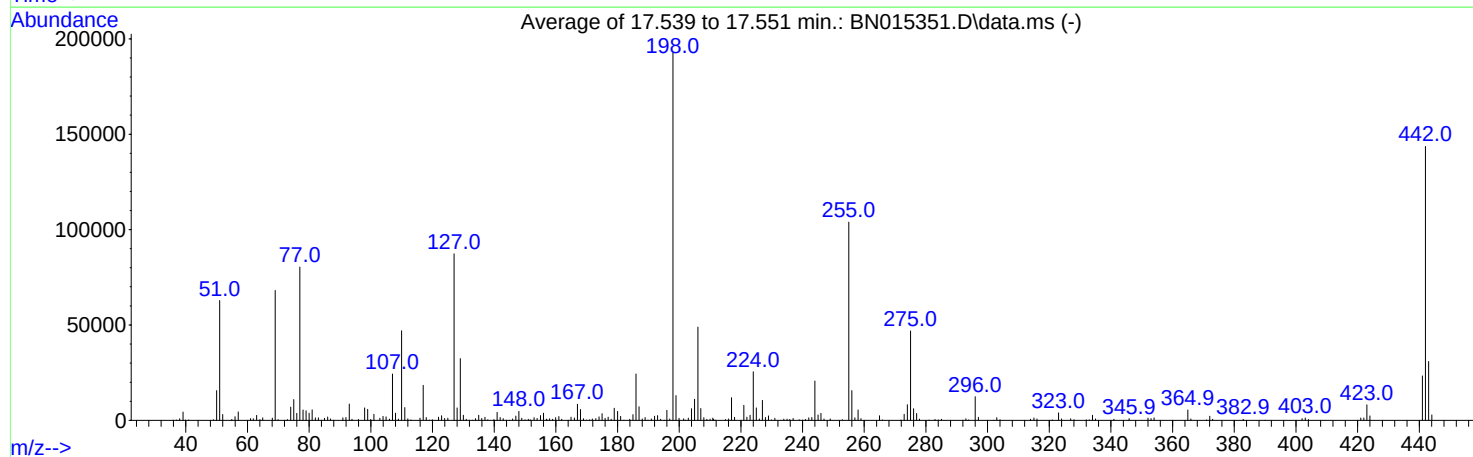


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070621\
 Data File : BN015351.D
 Acq On : 07 Jul 2021 00:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN063021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 07 11:11:38 2021

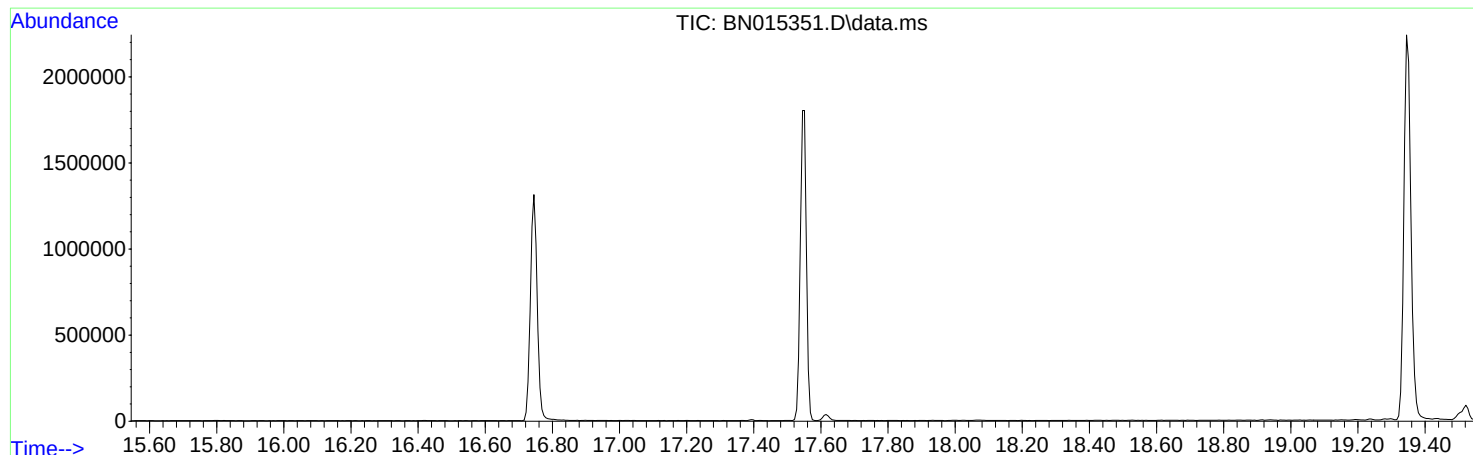




AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.6	62800	PASS
68	69	0.00	2	1.7	1147	PASS
69	198	0.00	100	35.3	68085	PASS
70	69	0.00	2	0.7	444	PASS
127	198	10	80	45.3	87280	PASS
197	198	0.00	2	0.4	757	PASS
198	198	100	100	100.0	192832	PASS
199	198	5	9	6.8	13043	PASS
275	198	10	60	24.3	46883	PASS
365	198	1	100	2.8	5470	PASS
441	198	0.01	100	12.1	23298	PASS
442	442	50	100	100.0	143619	PASS
443	442	15	24	21.5	30880	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070621\
 Data File : BN015351.D
 Acq On : 07 Jul 2021 00:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jul 07 06:44:25 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 23 10:10:58 2021
 Response via : Initial Calibration

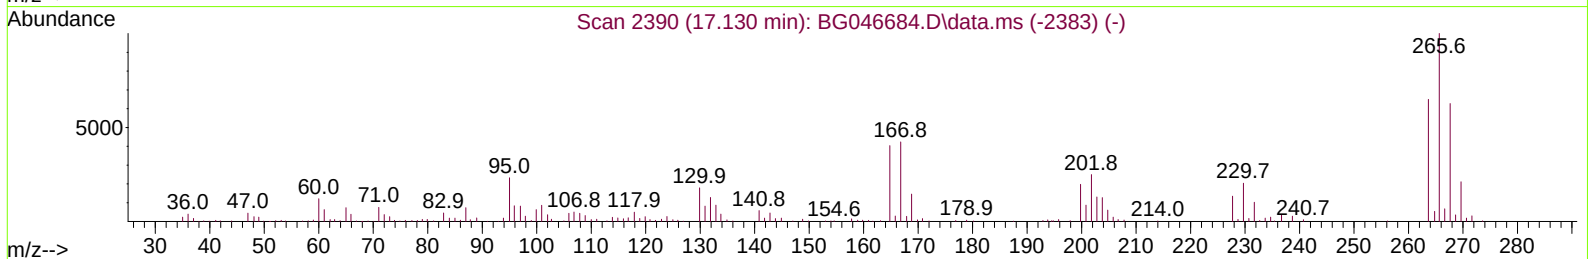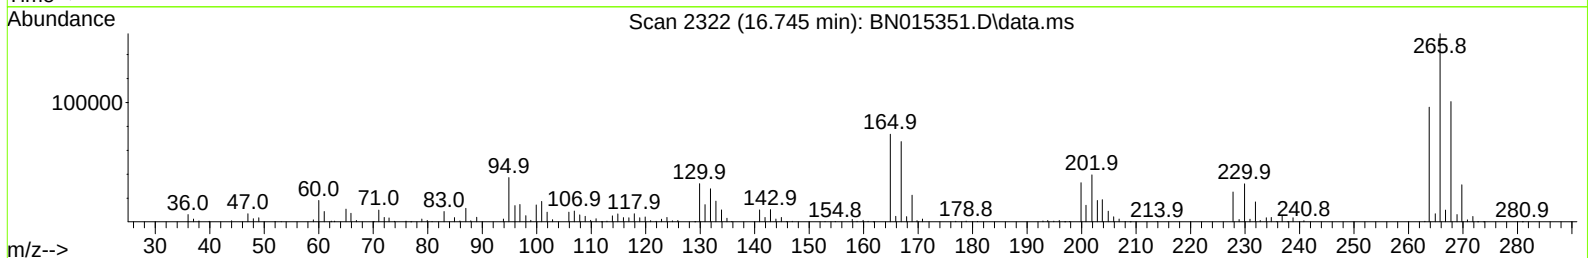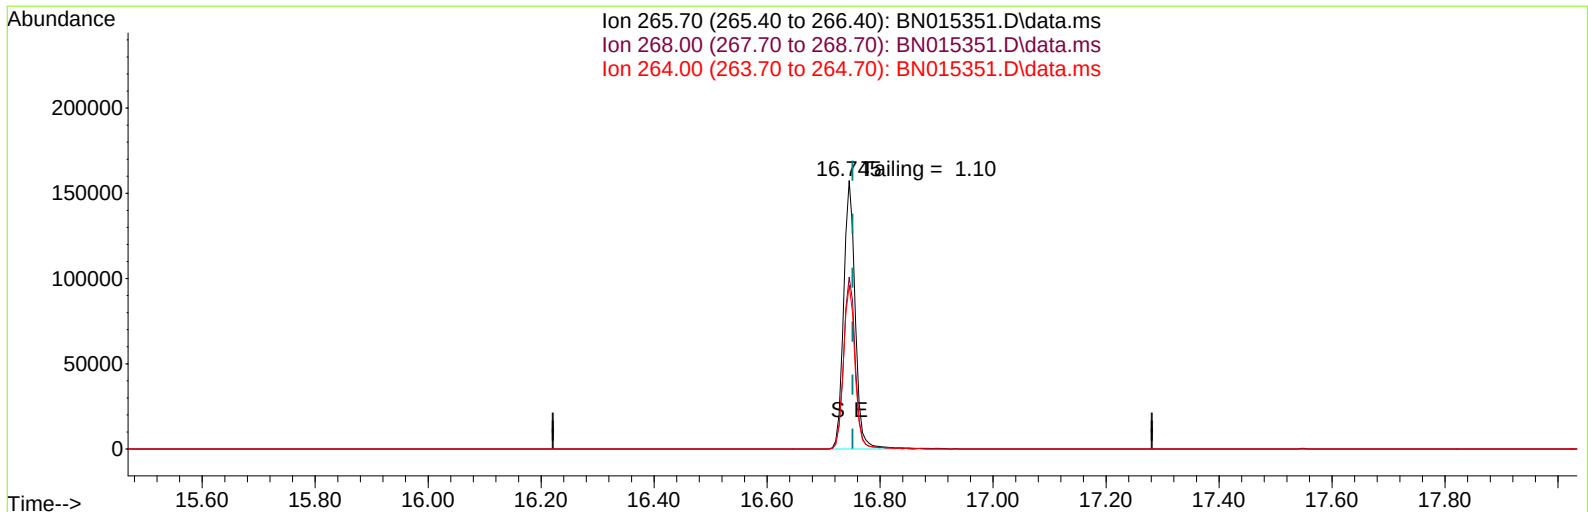

TIC: BN015351.D\data.ms

(70) Pentachlorophenol (C)

16.745min (-0.006) 27669.27 ng




response 224090

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.02
264.00	61.60	61.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070621\
Data File : BN015351.D
Acq On : 07 Jul 2021 00:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 07 06:44:25 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 10:10:58 2021
Response via : Initial Calibration

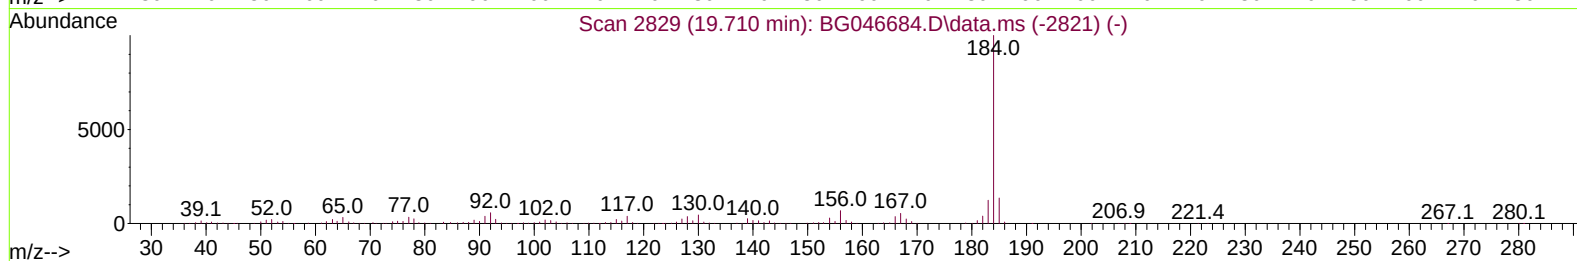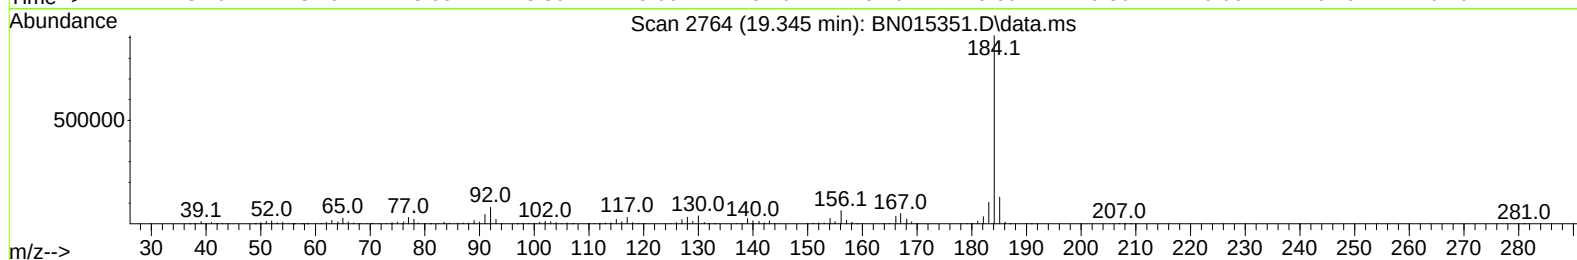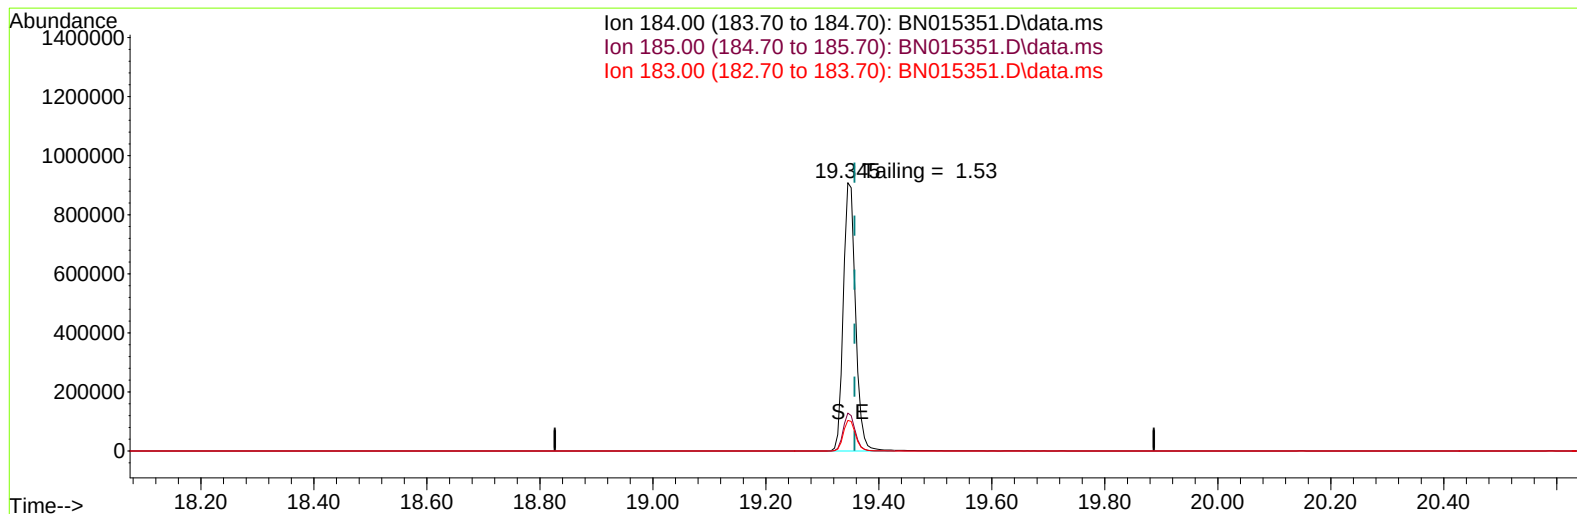

TIC: BN015351.D\data.ms

(77) Benzidine

19.345min (-0.012) 0.00 ng

response 1359226

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.14
183.00	13.20	11.40
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/6/2021	BNA_N	<u>BN015351.D</u>
Compound Name	Response	Retention Time
DDT	146902	20.586
DDD	320694	20.145
DDE	1452	19.639
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
322146	469048	68.68

Instrument :
BNA_N
ClientSampleId :
DFTPP