

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070722\
 Data File : BN020677.D
 Acq On : 07 Jul 2022 13:55
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Quant Time: Jul 08 01:31:03 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 02 03:10:12 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.818	152	4833	0.400	ng	0.00
7) Naphthalene-d8	10.616	136	14499	0.400	ng	#-0.01
13) Acenaphthene-d10	14.474	164	8057	0.400	ng	0.00
19) Phenanthrene-d10	17.226	188	15912	0.400	ng	0.00
29) Chrysene-d12	21.431	240	11010	0.400	ng	# 0.00
35) Perylene-d12	23.788	264	8242	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.406	112	4227	0.315	ng	0.00
5) Phenol-d6	7.017	99	5233	0.326	ng	-0.01
8) Nitrobenzene-d5	8.982	82	3978	0.339	ng	-0.01
11) 2-Methylnaphthalene-d10	12.219	152	8759	0.352	ng	0.00
14) 2,4,6-Tribromophenol	15.974	330	790	0.260	ng	0.00
15) 2-Fluorobiphenyl	13.095	172	12544	0.377	ng	-0.01
27) Fluoranthene-d10	19.265	212	15540	0.329	ng	0.00
31) Terphenyl-d14	19.868	244	10748	0.408	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.261	88	2274	0.359	ng	100
3) n-Nitrosodimethylamine	3.608	42	1769	0.306	ng	# 98
6) bis(2-Chloroethyl)ether	7.248	93	4830	0.350	ng	97
9) Naphthalene	10.669	128	16064	0.371	ng	99
10) Hexachlorobutadiene	10.968	225	2872	0.364	ng	# 100
12) 2-Methylnaphthalene	12.295	142	10273	0.357	ng	99
16) Acenaphthylene	14.185	152	13128	0.339	ng	98
17) Acenaphthene	14.527	154	9520	0.361	ng	96
18) Fluorene	15.522	166	11905	0.346	ng	99
20) 4,6-Dinitro-2-methylph...	15.639	198	441	0.367	ng	# 65
21) 4-Bromophenyl-phenylether	16.415	248	3495	0.378	ng	98
22) Hexachlorobenzene	16.538	284	3983	0.389	ng	98
23) Atrazine	16.692	200	2133	0.292	ng	97
24) Pentachlorophenol	16.897	266	885	0.453	ng	98
25) Phenanthrene	17.267	178	18901	0.352	ng	100
26) Anthracene	17.359	178	14984	0.324	ng	100
28) Fluoranthene	19.295	202	19779	0.338	ng	99
30) Pyrene	19.657	202	19717	0.423	ng	100
32) Benzo(a)anthracene	21.413	228	12570	0.320	ng	98
33) Chrysene	21.467	228	16718	0.384	ng	99
34) Bis(2-ethylhexyl)phtha...	21.351	149	7798	0.352	ng	98
36) Indeno(1,2,3-cd)pyrene	26.223	276	11743	0.320	ng	100
37) Benzo(b)fluoranthene	23.071	252	12850	0.405	ng	97
38) Benzo(k)fluoranthene	23.118	252	13331	0.394	ng	97
39) Benzo(a)pyrene	23.682	252	9692	0.352	ng	95
40) Dibenzo(a,h)anthracene	26.238	278	9285	0.315	ng	96
41) Benzo(g,h,i)perylene	26.963	276	11167	0.347	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070722\
Data File : BN020677.D
Acq On : 07 Jul 2022 13:55
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Quant Time: Jul 08 01:31:03 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 02 03:10:12 2022
Response via : Initial Calibration



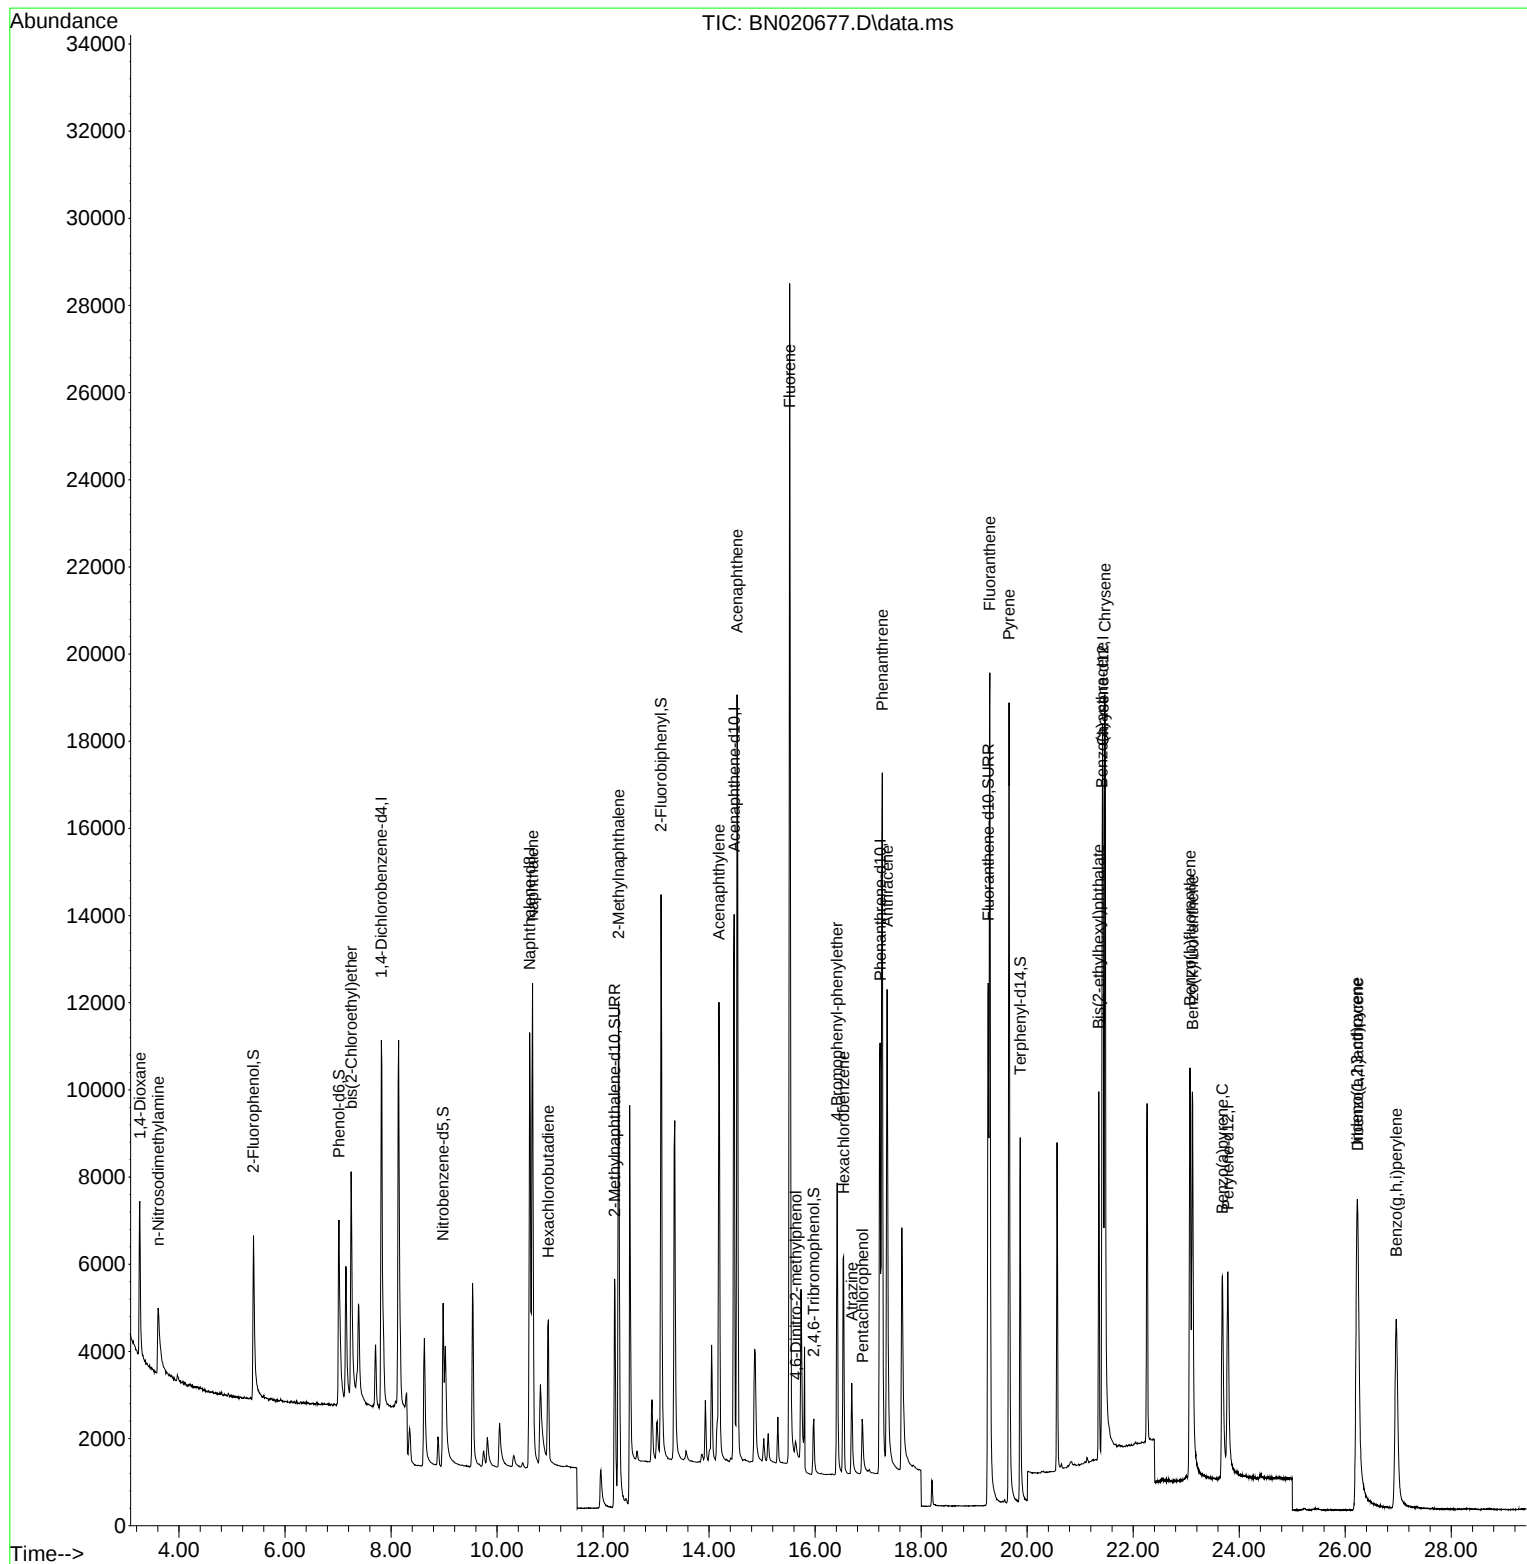




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.818 min Scan# 61
 Delta R.T. -0.007 min
 Lab File: BN020677.D
 Acq: 07 Jul 2022 13:55




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Tgt Ion:152 Resp: 4833
 Ion Ratio Lower Upper
 152 100
 150 158.8 127.9 191.9
 115 65.5 51.4 77.2

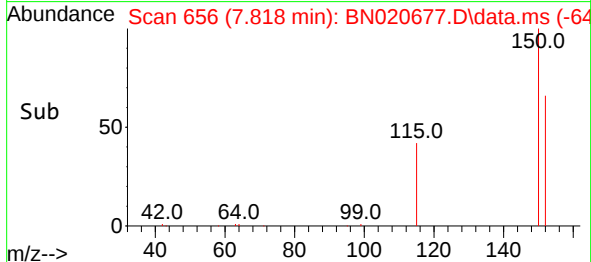

#2
 1,4-Dioxane
 Concen: 0.359 ng
 RT: 3.261 min Scan# 25
 Delta R.T. 0.000 min
 Lab File: BN020677.D
 Acq: 07 Jul 2022 13:55

Tgt Ion: 88 Resp: 2274
 Ion Ratio Lower Upper
 88 100
 43 37.5 30.2 45.2
 58 91.1 73.0 109.6

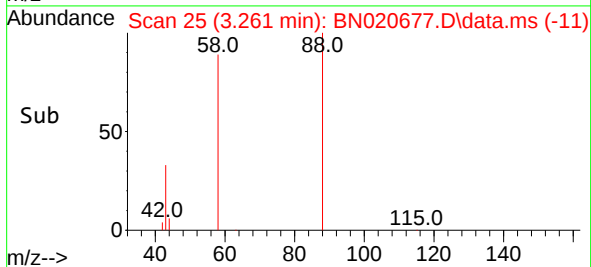

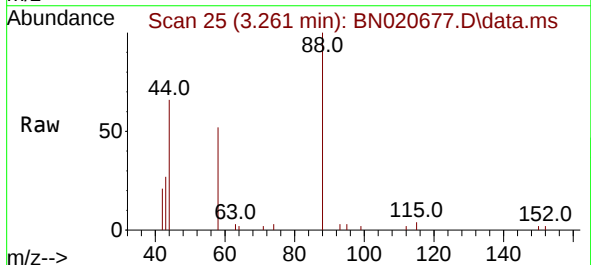




#3
n-Nitrosodimethylamine
Concen: 0.306 ng
RT: 3.608 min Scan# 71
Delta R.T. 0.000 min
Lab File: BN020677.D
Acq: 07 Jul 2022 13:55




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion: 42 Resp: 1769
Ion Ratio Lower Upper
42 100
74 105.7 84.0 126.0
44 8.4 9.8 14.8#

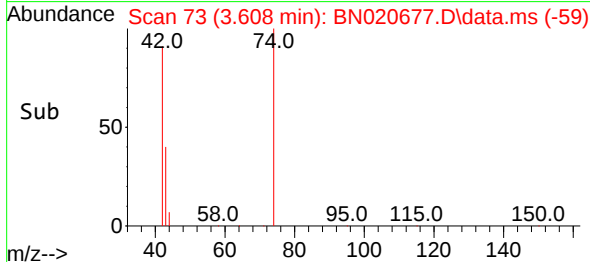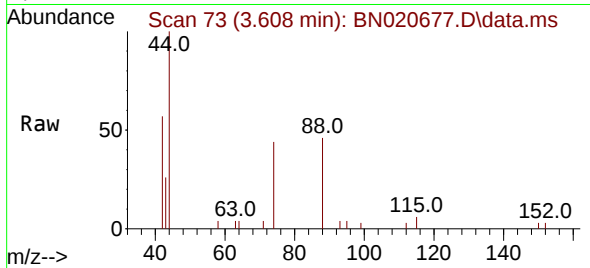

#4
2-Fluorophenol
Concen: 0.315 ng
RT: 5.406 min Scan# 322
Delta R.T. -0.007 min
Lab File: BN020677.D
Acq: 07 Jul 2022 13:55

Tgt Ion: 112 Resp: 4227
Ion Ratio Lower Upper
112 100
64 63.9 49.1 73.7
63 33.4 26.3 39.5

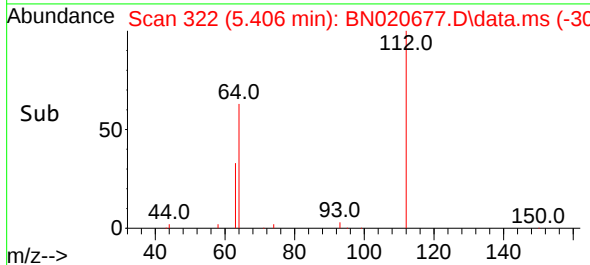

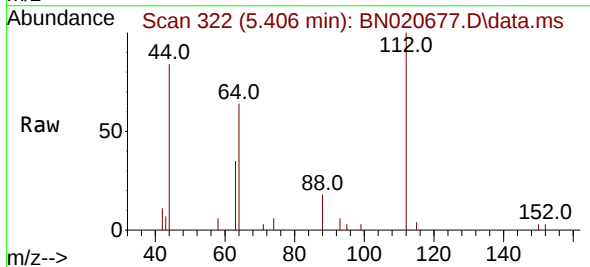




#5
Phenol-d6
Concen: 0.326 ng
RT: 7.017 min Scan# 54
Delta R.T. -0.014 min
Lab File: BN020677.D
Acq: 07 Jul 2022 13:55




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion: 99 Resp: 5233
Ion Ratio Lower Upper
99 100
42 22.9 19.3 28.9
71 34.9 27.5 41.3

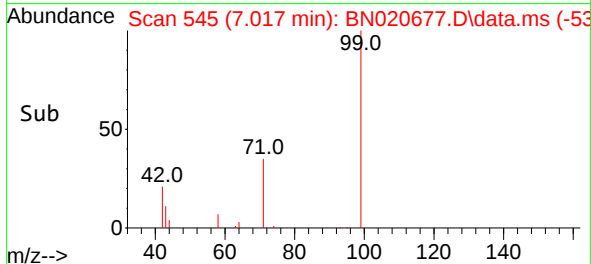

#6
bis(2-Chloroethyl)ether
Concen: 0.350 ng
RT: 7.248 min Scan# 577
Delta R.T. -0.007 min
Lab File: BN020677.D
Acq: 07 Jul 2022 13:55

Tgt Ion: 93 Resp: 4830
Ion Ratio Lower Upper
93 100
63 87.8 67.4 101.0
95 34.3 26.5 39.7

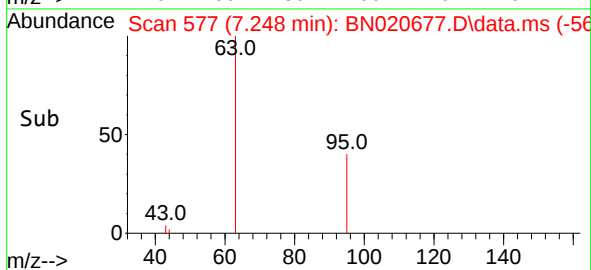

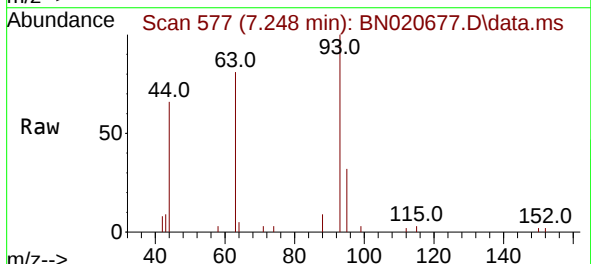




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.616 min Scan# 94
Delta R.T. -0.010 min
Lab File: BN020677.D
Acq: 07 Jul 2022 13:55




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:136	Resp:	14499
Ion Ratio	Lower	Upper
136	100	
137	11.6	9.0 13.6
54	11.4	6.2 9.2#
68	7.3	4.4 6.6#

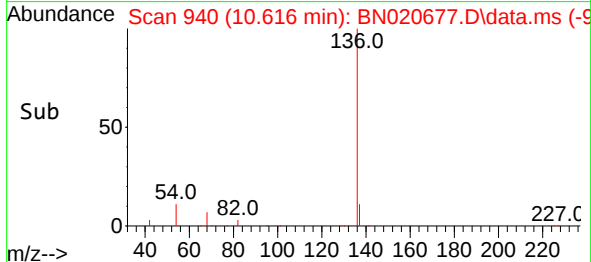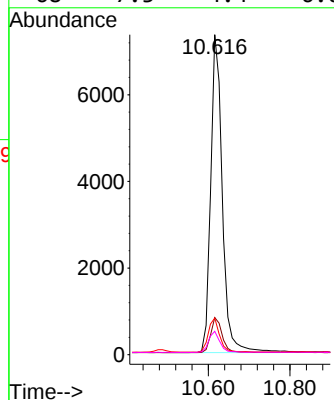

#8
Nitrobenzene-d5
Concen: 0.339 ng
RT: 8.982 min Scan# 787
Delta R.T. -0.010 min
Lab File: BN020677.D
Acq: 07 Jul 2022 13:55

Tgt Ion: 82	Resp:	3978
Ion Ratio	Lower	Upper
82	100	
128	39.5	35.0 52.6
54	60.6	46.2 69.4


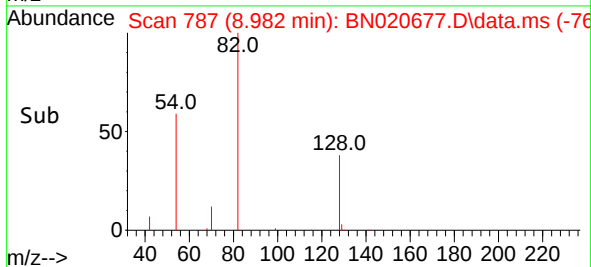
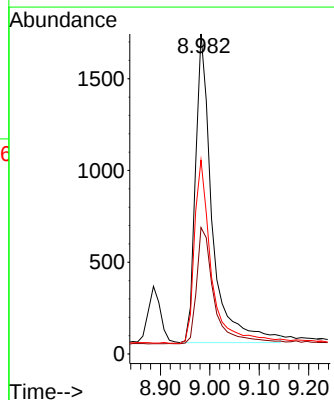
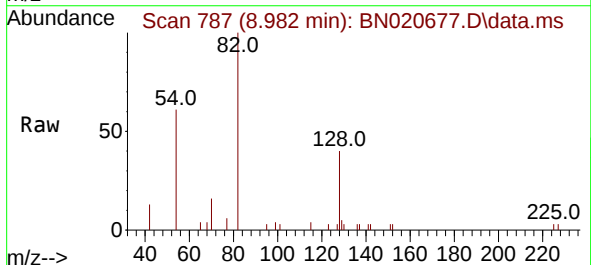




#9
Naphthalene
Concen: 0.371 ng
RT: 10.669 min Scan# 945
Delta R.T. -0.010 min
Lab File: BN020677.D
Acq: 07 Jul 2022 13:55




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:128	Resp:	16064
Ion Ratio	Lower	Upper
128	100	
129	11.5	8.9 13.3
127	13.6	10.8 16.2

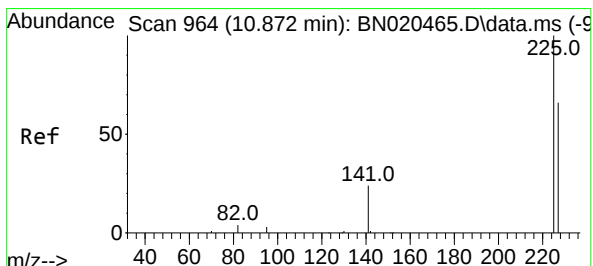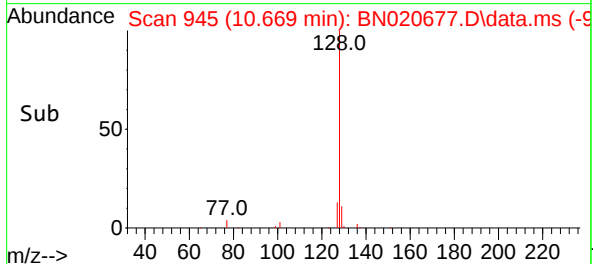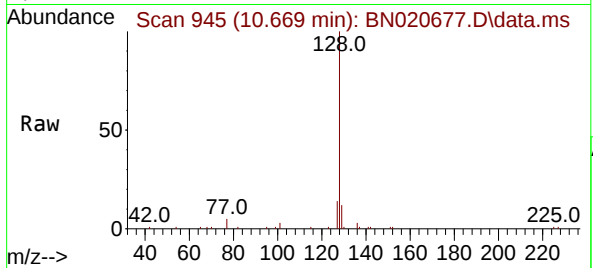

#10
Hexachlorobutadiene
Concen: 0.364 ng
RT: 10.968 min Scan# 973
Delta R.T. 0.000 min
Lab File: BN020677.D
Acq: 07 Jul 2022 13:55

Tgt Ion:225	Resp:	2872
Ion Ratio	Lower	Upper
225	100	
223	0.0	0.0 0.0
227	63.3	50.9 76.3

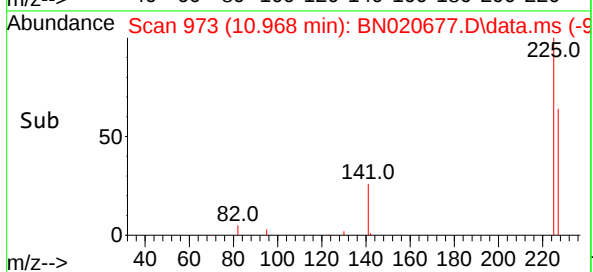

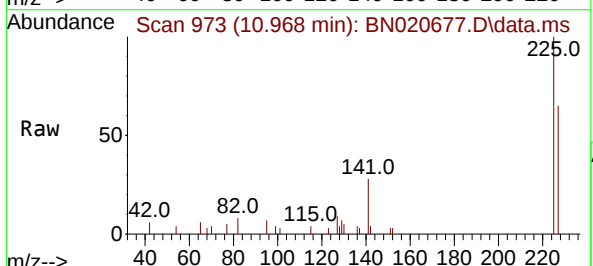




#11
2-Methylnaphthalene-d10
Concen: 0.352 ng
RT: 12.219 min Scan# 1185
Delta R.T. -0.007 min
Lab File: BN020677.D
Acq: 07 Jul 2022 13:55




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:152 Resp: 8759
Ion Ratio Lower Upper
152 100
151 20.5 16.2 24.4

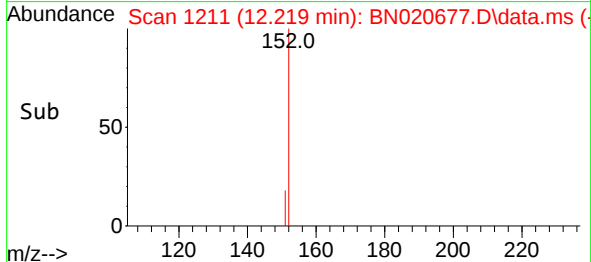

#12
2-Methylnaphthalene
Concen: 0.357 ng
RT: 12.295 min Scan# 1231
Delta R.T. -0.004 min
Lab File: BN020677.D
Acq: 07 Jul 2022 13:55

Tgt Ion:142 Resp: 10273
Ion Ratio Lower Upper
142 100
141 89.2 71.6 107.4
115 38.1 29.8 44.8

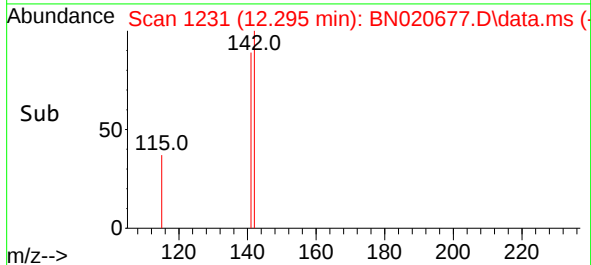

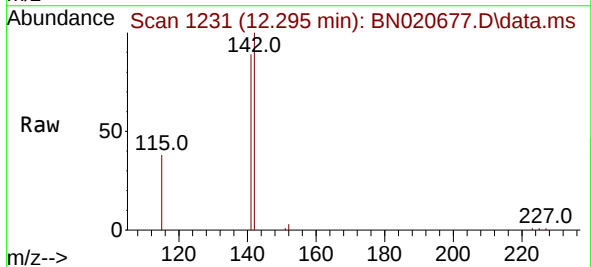




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.474 min Scan# 14
Delta R.T. 0.000 min
Lab File: BN020677.D
Acq: 07 Jul 2022 13:55




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:164 Resp: 8057
Ion Ratio Lower Upper
164 100
162 100.1 82.1 123.1
160 46.9 38.6 58.0

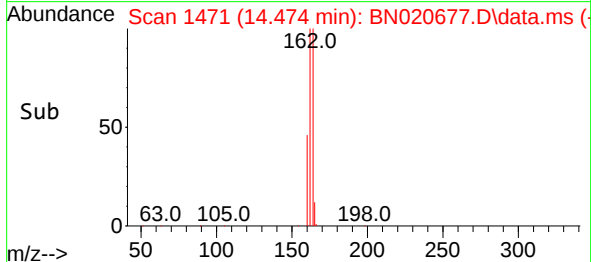

#14
2,4,6-Tribromophenol
Concen: 0.260 ng
RT: 15.974 min Scan# 1612
Delta R.T. 0.000 min
Lab File: BN020677.D
Acq: 07 Jul 2022 13:55

Tgt Ion:330 Resp: 790
Ion Ratio Lower Upper
330 100
332 97.2 77.6 116.4
141 57.6 41.0 61.4

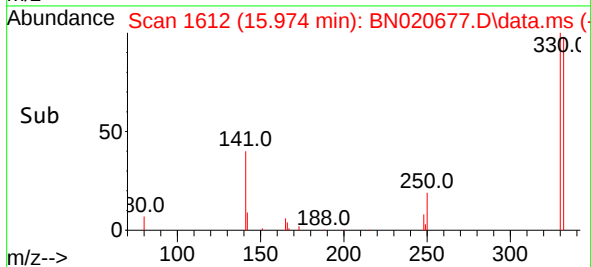

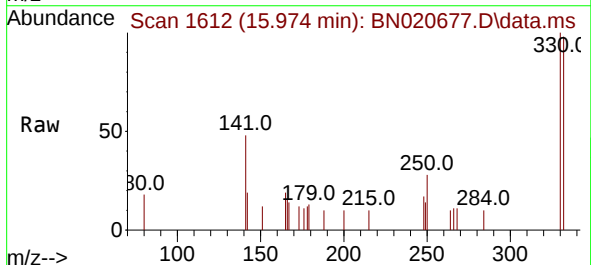




#15
2-Fluorobiphenyl
Concen: 0.377 ng
RT: 13.095 min Scan# 11
Delta R.T. -0.010 min
Lab File: BN020677.D
Acq: 07 Jul 2022 13:55




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:	172	Resp:	12544
Ion Ratio	Lower	Upper	
172	100		
171	36.0	27.2	40.8
170	24.1	18.2	27.4

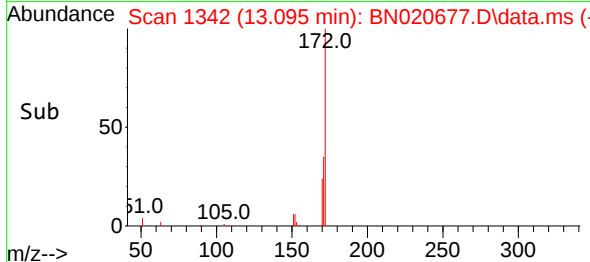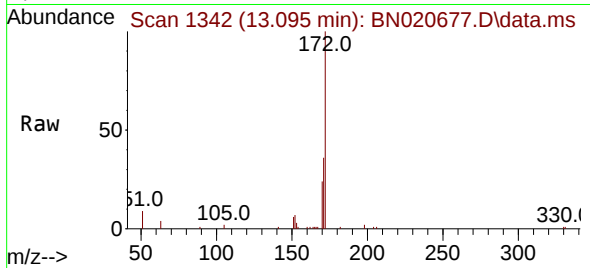

#16
Acenaphthylene
Concen: 0.339 ng
RT: 14.185 min Scan# 1444
Delta R.T. -0.011 min
Lab File: BN020677.D
Acq: 07 Jul 2022 13:55

Tgt Ion:	152	Resp:	13128
Ion Ratio	Lower	Upper	
152	100		
151	19.5	16.2	24.4
153	12.9	10.7	16.1

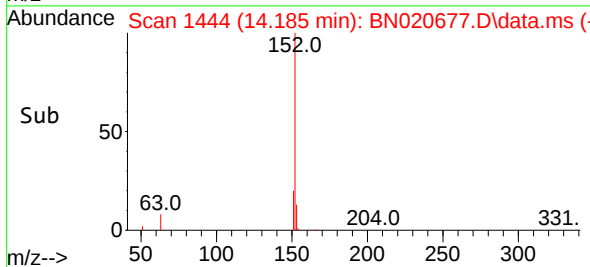

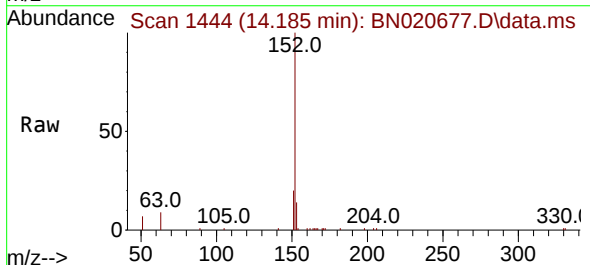




#17
Acenaphthene
Concen: 0.361 ng
RT: 14.527 min Scan# 1467
Delta R.T. -0.011 min
Lab File: BN020677.D
Acq: 07 Jul 2022 13:55




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:154 Resp: 9520
Ion Ratio Lower Upper
154 100
153 114.4 87.5 131.3
152 56.6 43.8 65.6

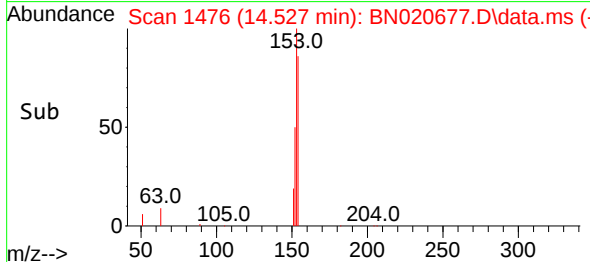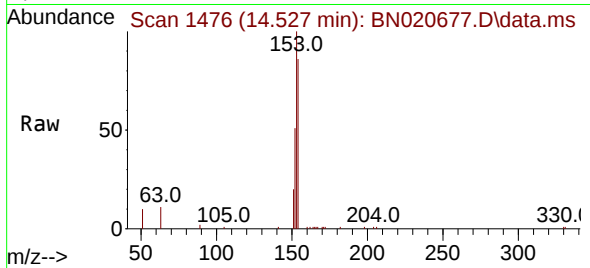

#18
Fluorene
Concen: 0.346 ng
RT: 15.522 min Scan# 1569
Delta R.T. -0.010 min
Lab File: BN020677.D
Acq: 07 Jul 2022 13:55

Tgt Ion:166 Resp: 11905
Ion Ratio Lower Upper
166 100
165 99.2 78.6 118.0
167 13.4 10.8 16.2

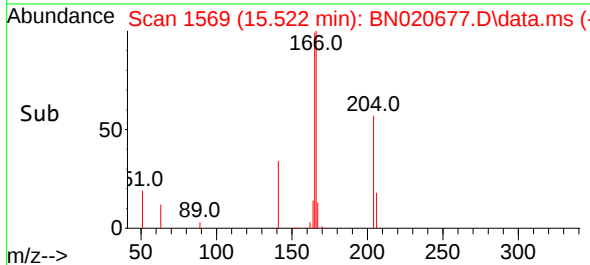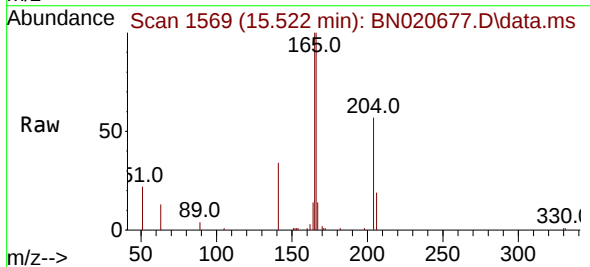



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.226 min Scan# 11

Delta R.T. 0.000 min

Lab File: BN020677.D

Acq: 07 Jul 2022 13:55

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:188 Resp: 15912

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 9.9 7.4 11.2

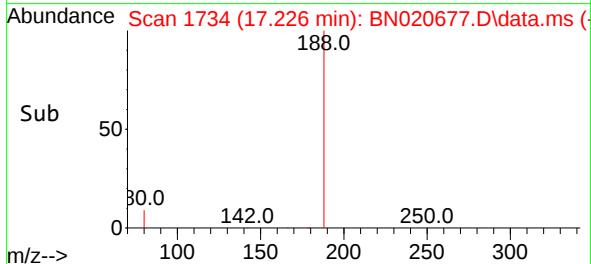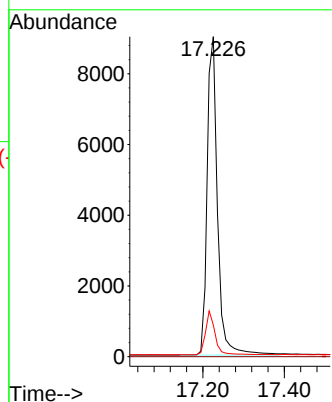

#20

4,6-Dinitro-2-methylphenol

Concen: 0.367 ng

RT: 15.639 min Scan# 1580

Delta R.T. 0.000 min

Lab File: BN020677.D

Acq: 07 Jul 2022 13:55




Tgt Ion:198 Resp: 441

Ion Ratio Lower Upper

198 100

182 29.7 12.1 18.1#

77 0.0 0.0 0.0


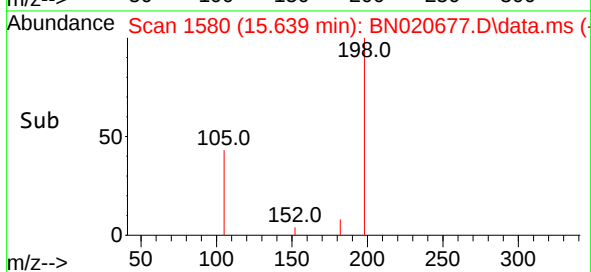
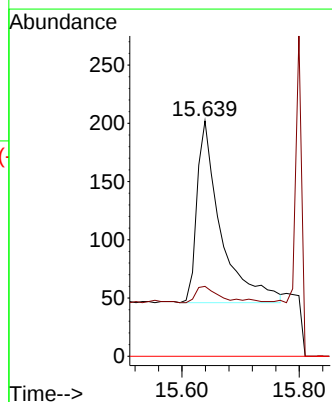
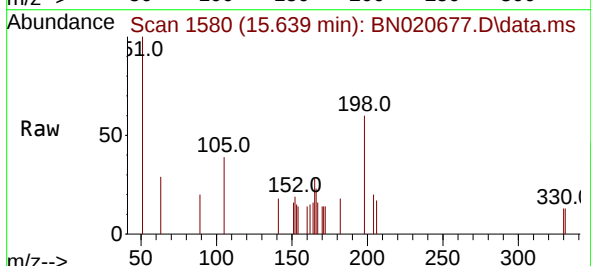




#21
4-Bromophenyl-phenylether
Concen: 0.378 ng
RT: 16.415 min Scan# 1665
Delta R.T. -0.010 min
Lab File: BN020677.D
Acq: 07 Jul 2022 13:55




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:248 Resp: 3495
Ion Ratio Lower Upper
248 100
250 95.1 75.3 112.9
141 80.7 67.3 100.9

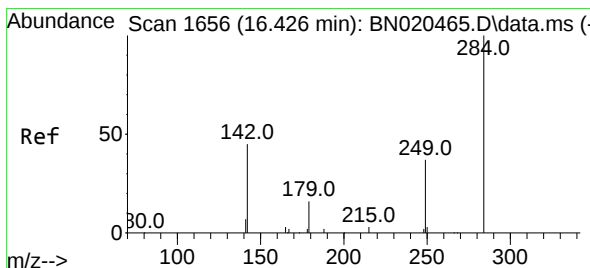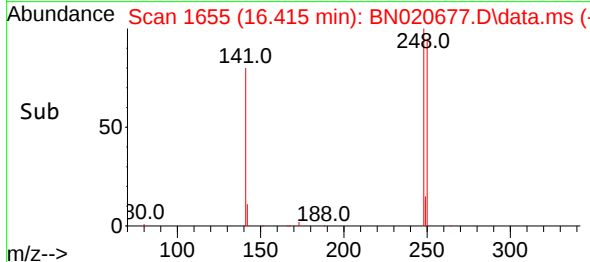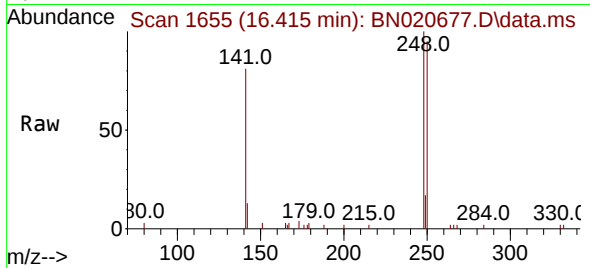

#22
Hexachlorobenzene
Concen: 0.389 ng
RT: 16.538 min Scan# 1667
Delta R.T. 0.000 min
Lab File: BN020677.D
Acq: 07 Jul 2022 13:55

Tgt Ion:284 Resp: 3983
Ion Ratio Lower Upper
284 100
142 45.6 35.2 52.8
249 33.7 26.6 40.0


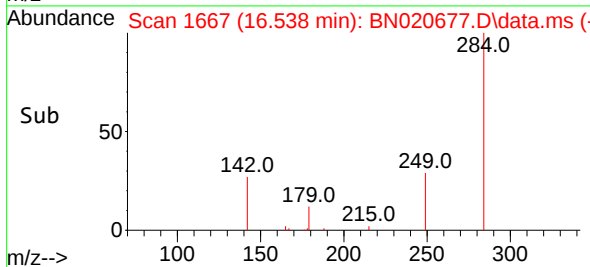

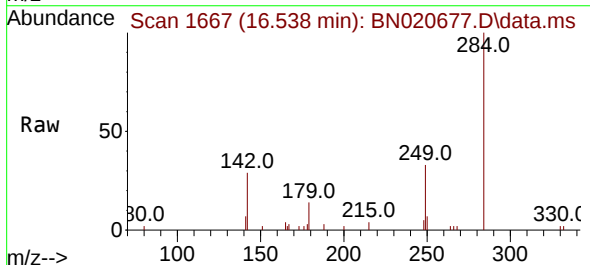


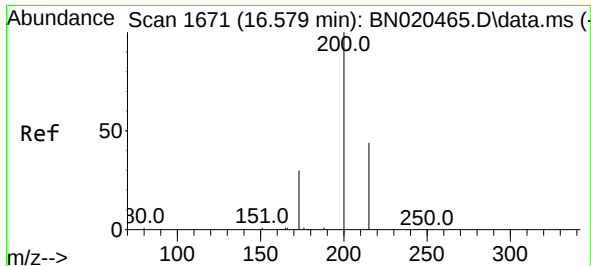

#23
 Atrazine
 Concen: 0.292 ng
 RT: 16.692 min Scan# 1702
 Delta R.T. 0.000 min
 Lab File: BN020677.D
 Acq: 07 Jul 2022 13:55




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Tgt Ion:	200	Resp:	2133
Ion Ratio	Lower	Upper	
200	100		
173	30.6	23.6	35.4
215	47.9	36.6	54.8

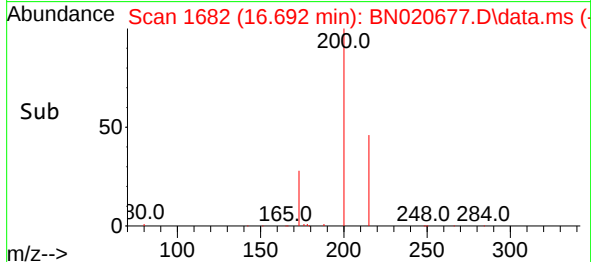

#24
 Pentachlorophenol
 Concen: 0.453 ng
 RT: 16.897 min Scan# 1702
 Delta R.T. 0.000 min
 Lab File: BN020677.D
 Acq: 07 Jul 2022 13:55

Tgt Ion:	266	Resp:	885
Ion Ratio	Lower	Upper	
266	100		
264	62.0	51.3	76.9
268	64.9	52.6	79.0


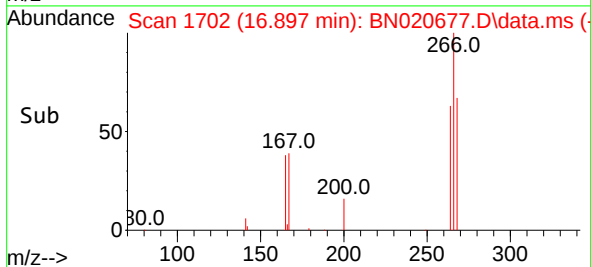

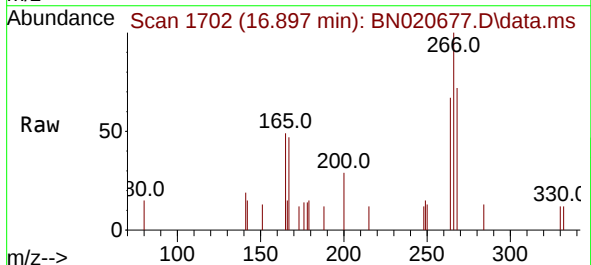




#25
Phenanthrene
Concen: 0.352 ng
RT: 17.267 min Scan# 1747
Delta R.T. 0.000 min
Lab File: BN020677.D
Acq: 07 Jul 2022 13:55




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:178 Resp: 18901
Ion Ratio Lower Upper
178 100
176 19.1 15.3 22.9
179 15.3 12.2 18.4

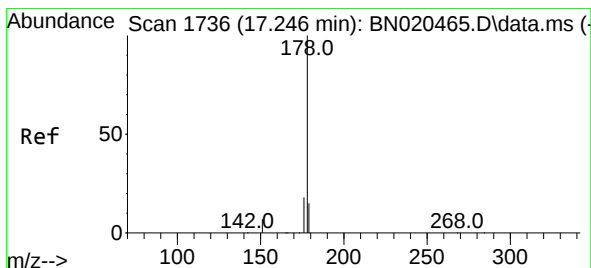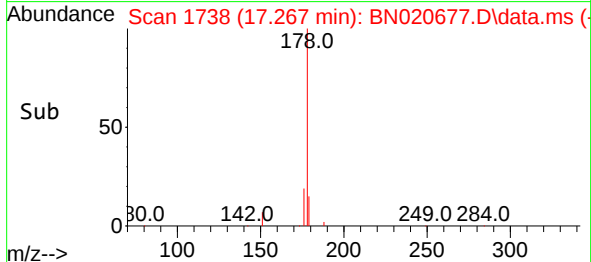

#26
Anthracene
Concen: 0.324 ng
RT: 17.359 min Scan# 1747
Delta R.T. 0.000 min
Lab File: BN020677.D
Acq: 07 Jul 2022 13:55

Tgt Ion:178 Resp: 14984
Ion Ratio Lower Upper
178 100
176 18.5 14.9 22.3
179 15.5 12.2 18.4

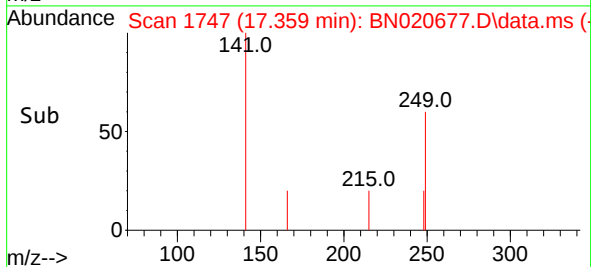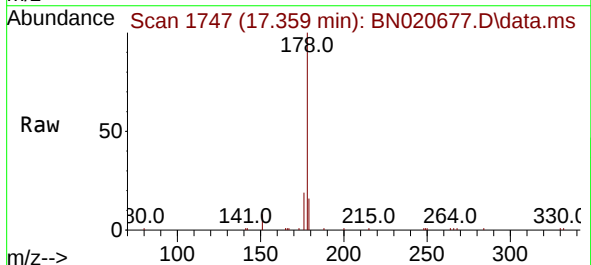



#27

Fluoranthene-d10

Concen: 0.329 ng

RT: 19.265 min Scan# 2116

Delta R.T. -0.004 min

Lab File: BN020677.D

Acq: 07 Jul 2022 13:55

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:212 Resp: 15540

Ion Ratio Lower Upper

212 100

106 16.1 12.6 19.0

104 9.0 7.2 10.8

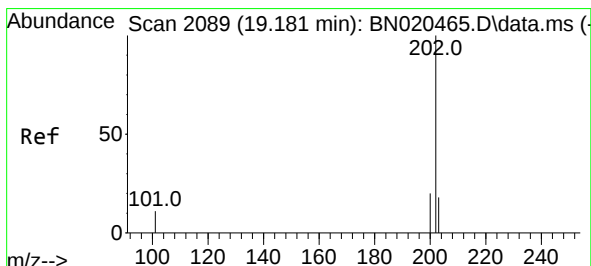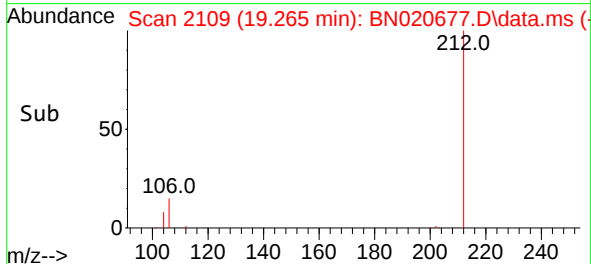

#28

Fluoranthene

Concen: 0.338 ng

RT: 19.295 min Scan# 2116

Delta R.T. -0.004 min

Lab File: BN020677.D

Acq: 07 Jul 2022 13:55




Tgt Ion:202 Resp: 19779


Ion Ratio Lower Upper

202 100

101 12.5 9.6 14.4

203 16.7 13.5 20.3

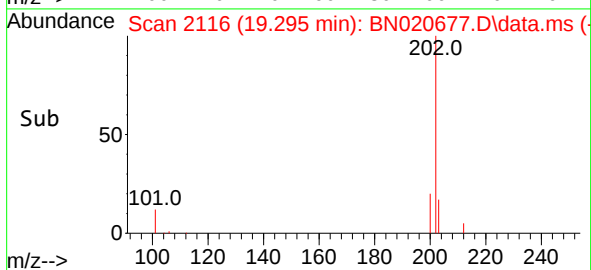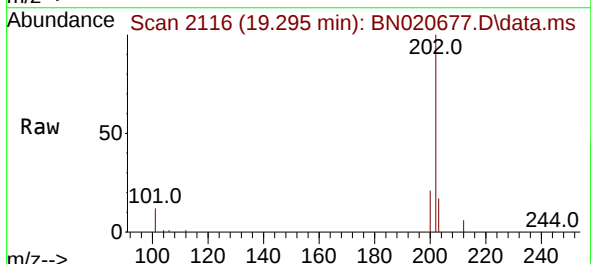

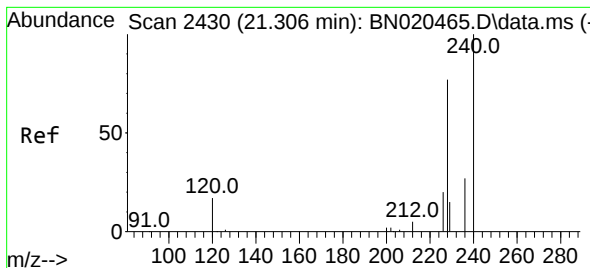

#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.431 min Scan# 2444

Delta R.T. 0.000 min

Lab File: BN020677.D

Acq: 07 Jul 2022 13:55

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:240 Resp: 11010

Ion Ratio Lower Upper

240 100

120 14.1 14.6 21.8#

236 26.6 22.6 33.8

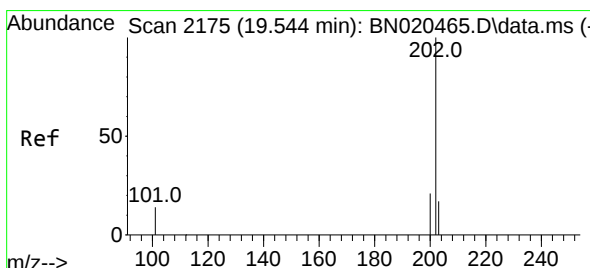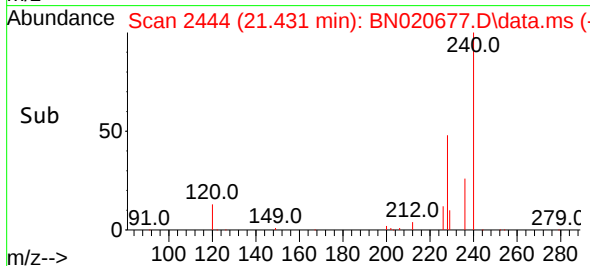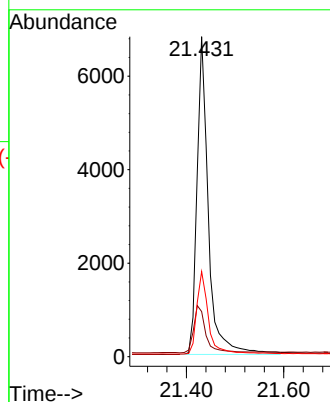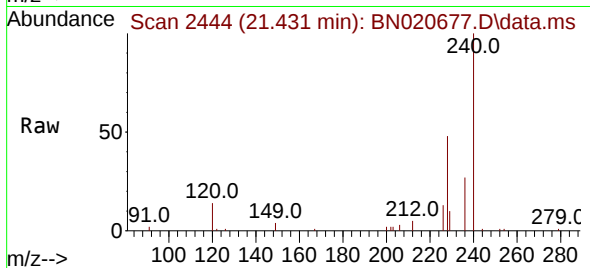

#30

Pyrene

Concen: 0.423 ng

RT: 19.657 min Scan# 2202

Delta R.T. -0.004 min

Lab File: BN020677.D

Acq: 07 Jul 2022 13:55




Tgt Ion:202 Resp: 19717

Ion Ratio Lower Upper

202 100

200 20.8 16.6 25.0

203 17.7 14.2 21.2

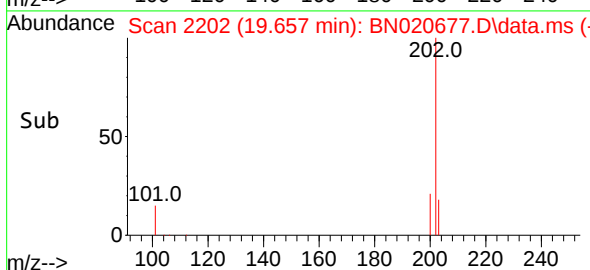

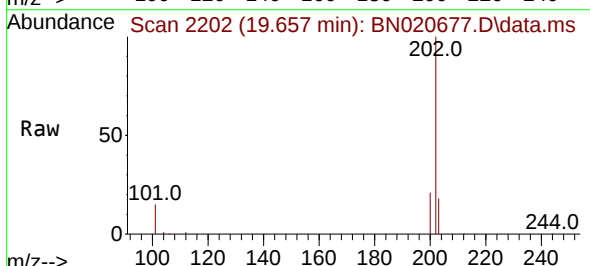




#31
 Terphenyl-d14
 Concen: 0.408 ng
 RT: 19.868 min Scan# 21
 Delta R.T. -0.004 min
 Lab File: BN020677.D
 Acq: 07 Jul 2022 13:55




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Tgt Ion:244 Resp: 10748
 Ion Ratio Lower Upper
 244 100
 212 9.3 7.1 10.7
 122 0.0 0.0 0.0

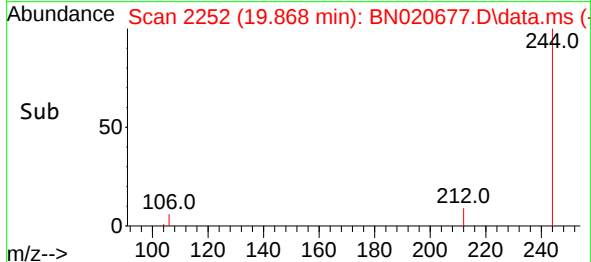

#32
 Benzo(a)anthracene
 Concen: 0.320 ng
 RT: 21.413 min Scan# 2442
 Delta R.T. -0.009 min
 Lab File: BN020677.D
 Acq: 07 Jul 2022 13:55

Tgt Ion:228 Resp: 12570
 Ion Ratio Lower Upper
 228 100
 226 28.2 21.2 31.8
 229 20.1 15.6 23.4

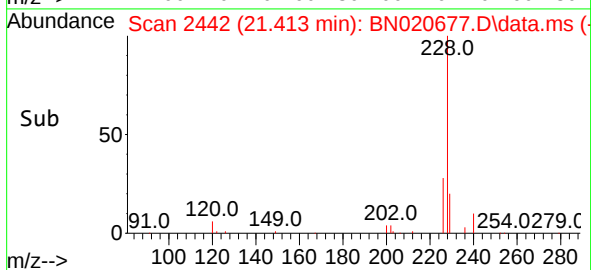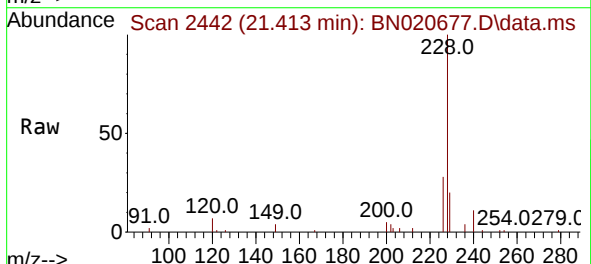



#33

Chrysene

Concen: 0.384 ng

RT: 21.467 min Scan# 2448

Delta R.T. 0.000 min

Lab File: BN020677.D

Acq: 07 Jul 2022 13:55

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4




Tgt Ion:228 Resp: 16718

Ion Ratio Lower Upper

228 100

226 30.3 23.4 35.0

229 19.5 15.7 23.5

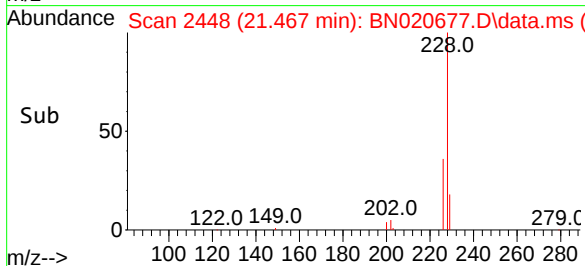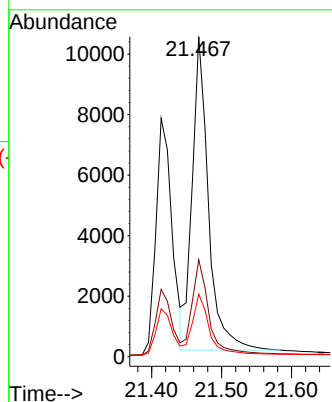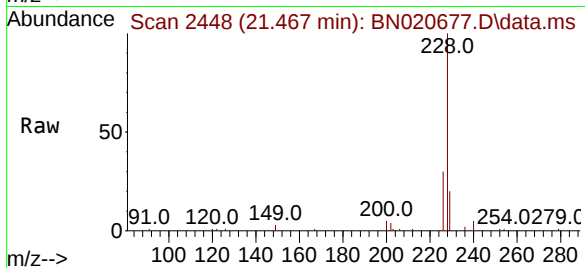

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.352 ng

RT: 21.351 min Scan# 2435

Delta R.T. 0.000 min

Lab File: BN020677.D

Acq: 07 Jul 2022 13:55




Tgt Ion:149 Resp: 7798

Ion Ratio Lower Upper

149 100

167 25.7 21.7 32.5

279 2.7 2.2 3.2

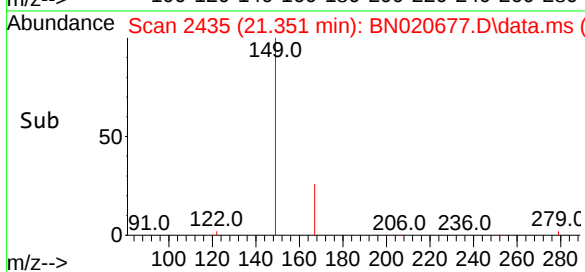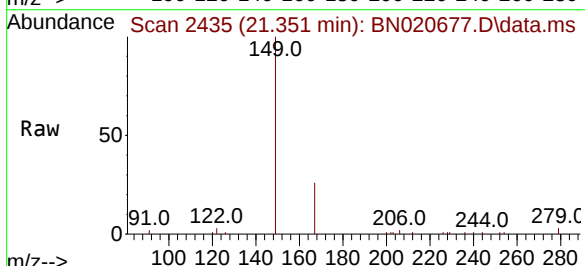



#35

Perylene-d12

Concen: 0.400 ng

RT: 23.788 min Scan# 30

Delta R.T. -0.003 min

Lab File: BN020677.D

Acq: 07 Jul 2022 13:55

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:264 Resp: 8242

Ion Ratio Lower Upper

264 100

260 26.3 20.9 31.3

265 36.2 28.0 42.0

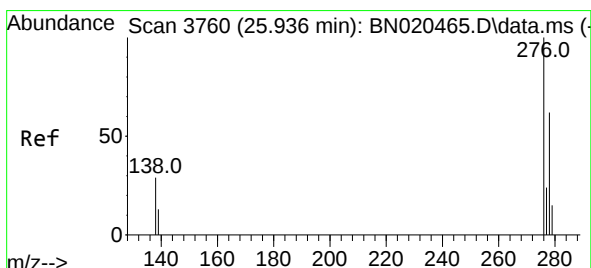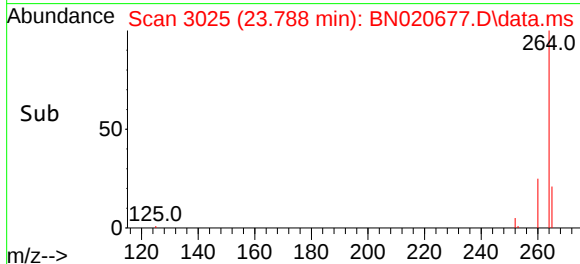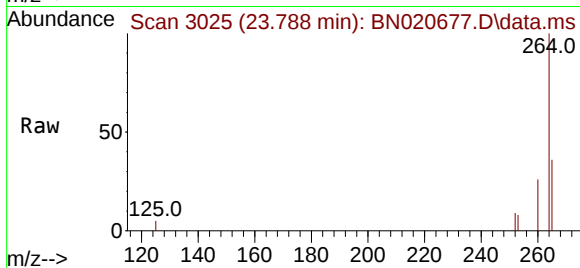

#36

Indeno(1,2,3-cd)pyrene

Concen: 0.320 ng

RT: 26.223 min Scan# 3858

Delta R.T. 0.000 min

Lab File: BN020677.D

Acq: 07 Jul 2022 13:55




Tgt Ion:276 Resp: 11743

Ion Ratio Lower Upper

276 100

138 32.2 25.9 38.9

277 25.1 19.8 29.8

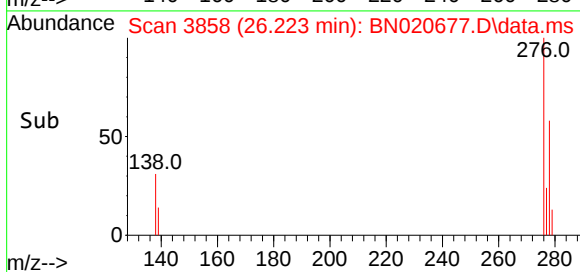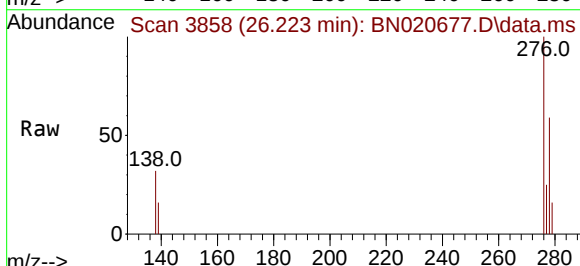



#37

Benzo(b)fluoranthene

Concen: 0.405 ng

RT: 23.071 min Scan# 21

Delta R.T. -0.003 min

Lab File: BN020677.D

Acq: 07 Jul 2022 13:55

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:252 Resp: 12850

Ion Ratio Lower Upper

252 100

253 24.7 18.5 27.7

125 15.3 11.4 17.0

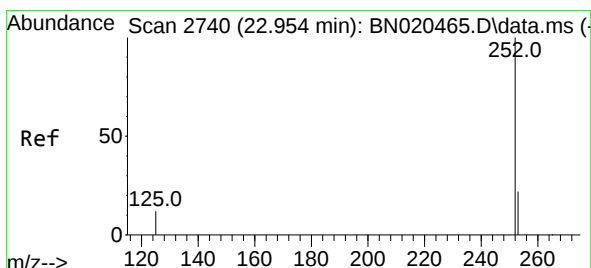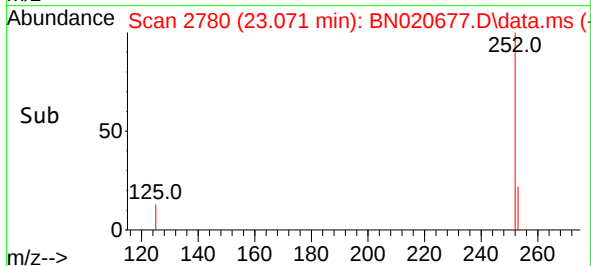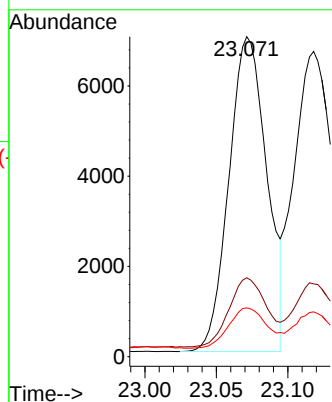

#38

Benzo(k)fluoranthene

Concen: 0.394 ng

RT: 23.118 min Scan# 2796

Delta R.T. -0.003 min

Lab File: BN020677.D

Acq: 07 Jul 2022 13:55




Tgt Ion:252 Resp: 13331

Ion Ratio Lower Upper

252 100

253 23.9 18.0 27.0

125 14.7 11.0 16.4

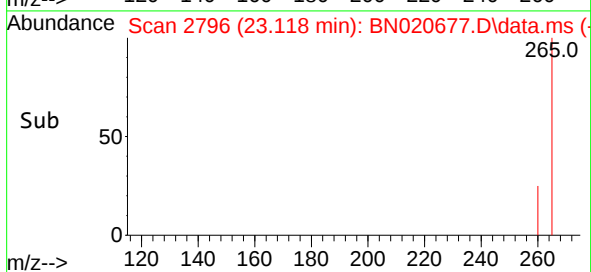
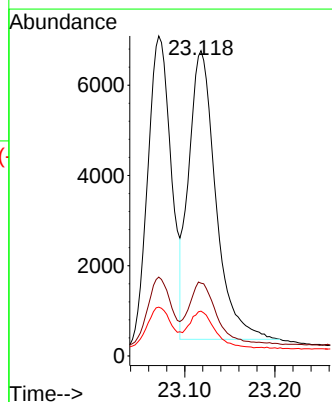
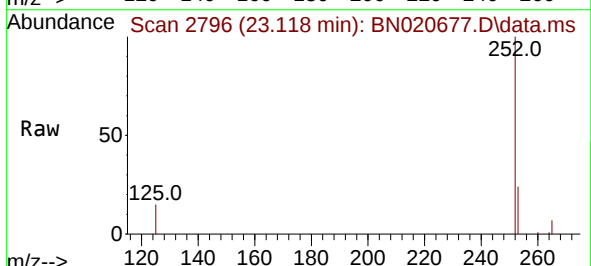




#39
Benzo(a)pyrene
Concen: 0.352 ng
RT: 23.682 min Scan# 2926
Delta R.T. -0.003 min
Lab File: BN020677.D
Acq: 07 Jul 2022 13:55




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:	252	Resp:	9692
Ion Ratio	Lower	Upper	
252	100		
253	27.1	19.0	28.4
125	18.0	13.8	20.8

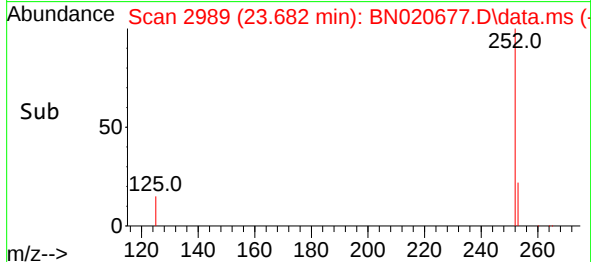

#40
Dibenzo(a,h)anthracene
Concen: 0.315 ng
RT: 26.238 min Scan# 3863
Delta R.T. -0.009 min
Lab File: BN020677.D
Acq: 07 Jul 2022 13:55


Tgt Ion:	278	Resp:	9285
Ion Ratio	Lower	Upper	
278	100		
139	23.9	18.6	28.0
279	27.5	19.7	29.5

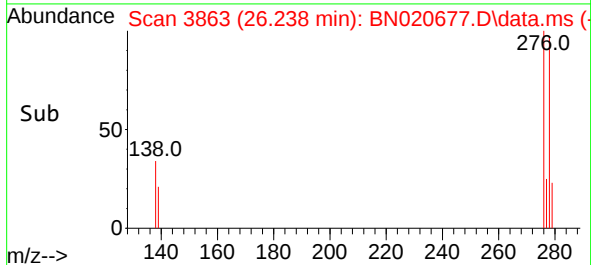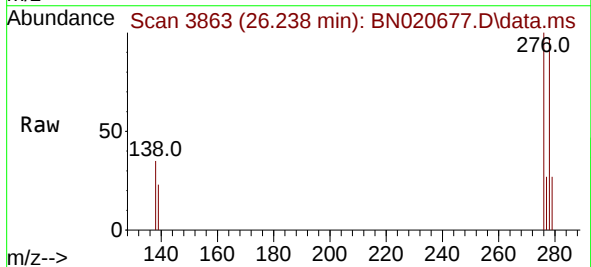



#41
Benzo(g,h,i)perylene
Concen: 0.347 ng
RT: 26.963 min Scan# 41
Delta R.T. -0.006 min
Lab File: BN020677.D
Acq: 07 Jul 2022 13:55

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

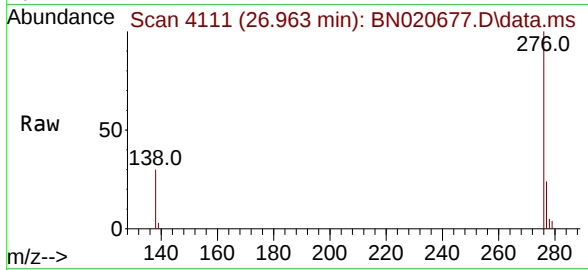

Tgt Ion:	276	Resp:	11167
Ion	Ratio	Lower	Upper
276	100		
277	24.3	19.5	29.3
138	29.7	22.6	34.0

