
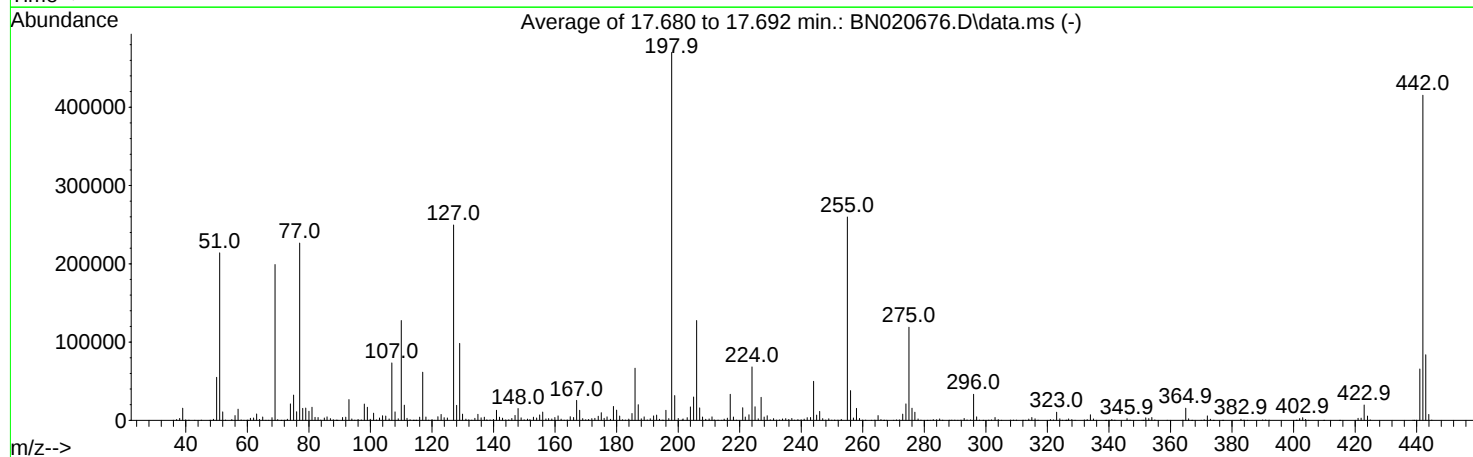


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070722\
 Data File : BN020676.D
 Acq On : 07 Jul 2022 13:19
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jul 02 03:10:12 2022

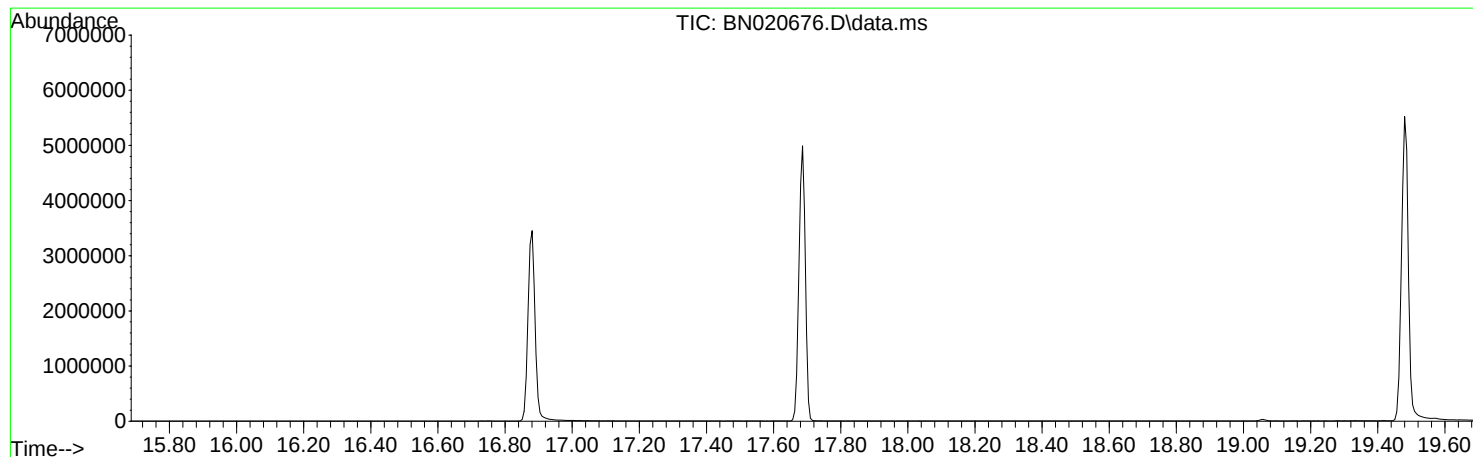




AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.5	214002	PASS
68	69	0.00	2	1.8	3562	PASS
69	198	0.00	100	42.4	199211	PASS
70	69	0.00	2	0.6	1103	PASS
127	198	10	80	53.1	249600	PASS
197	198	0.00	2	0.5	2160	PASS
198	198	100	100	100.0	469952	PASS
199	198	5	9	6.7	31648	PASS
275	198	10	60	25.3	118984	PASS
365	198	1	100	3.3	15467	PASS
441	198	0.01	100	14.0	65589	PASS
442	442	50	100	100.0	415317	PASS
443	442	15	24	20.2	83752	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070722\
 Data File : BN020676.D
 Acq On : 07 Jul 2022 13:19
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jul 08 05:25:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 05:25:05 2022
 Response via : Initial Calibration

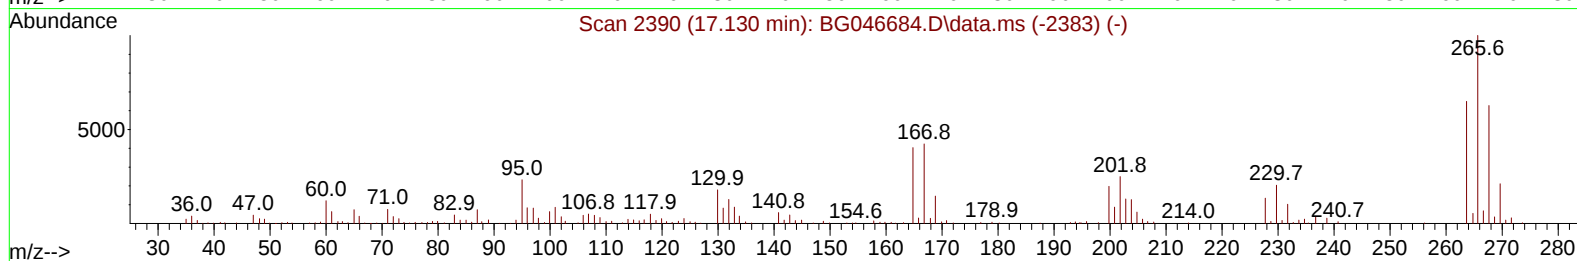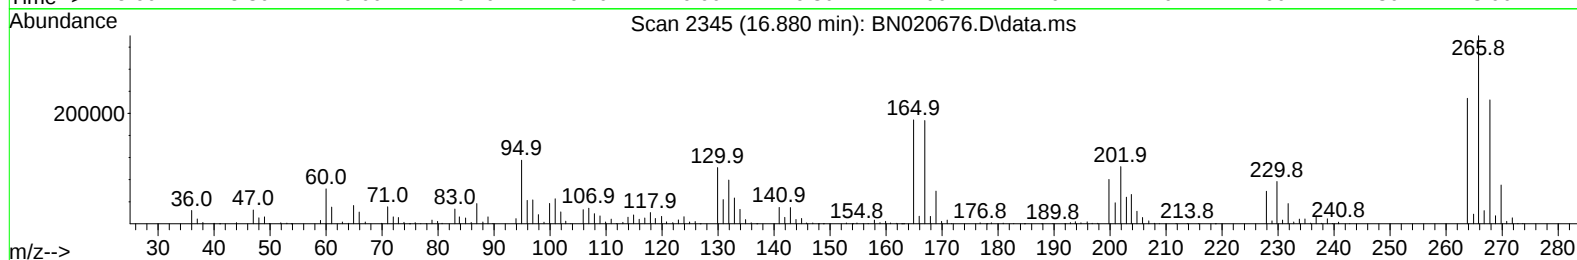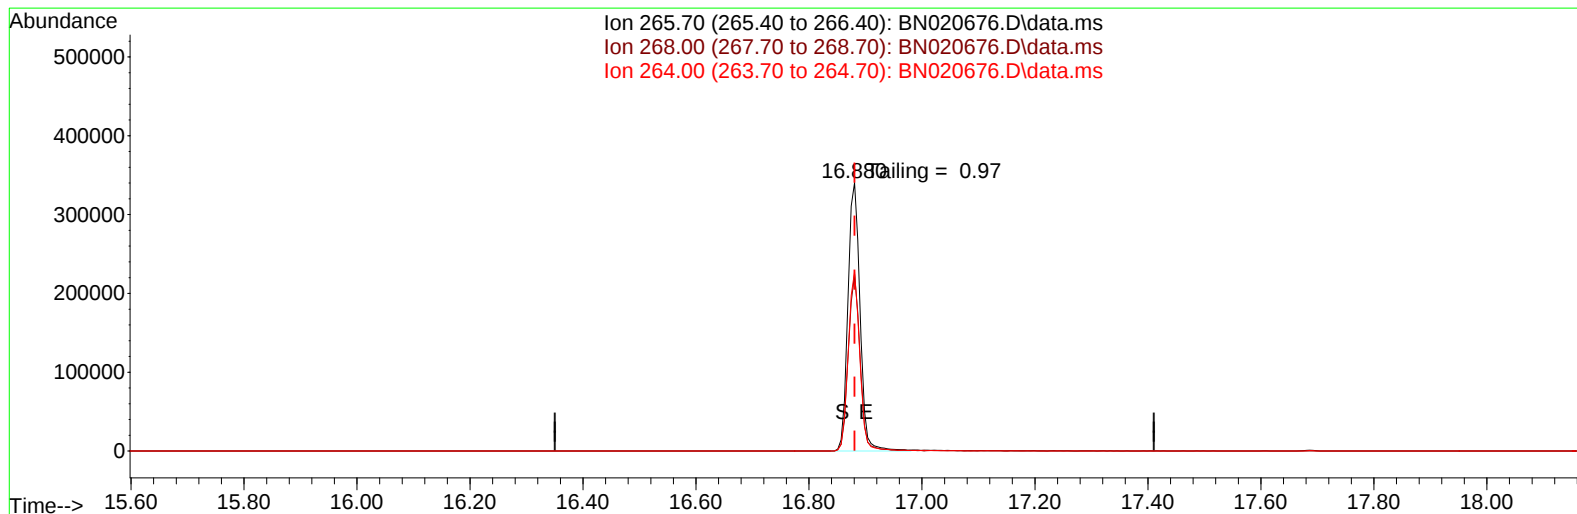

TIC: BN020676.D\data.ms

(70) Pentachlorophenol (C)

16.880min (0.000) 18962.23 ng




response 508189

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.93
264.00	61.60	66.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070722\
Data File : BN020676.D
Acq On : 07 Jul 2022 13:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 08 05:25:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 08 05:25:05 2022
Response via : Initial Calibration

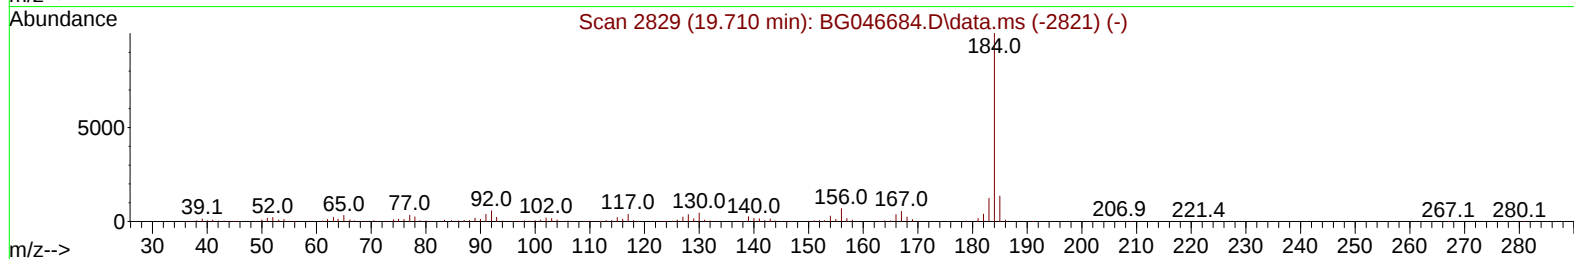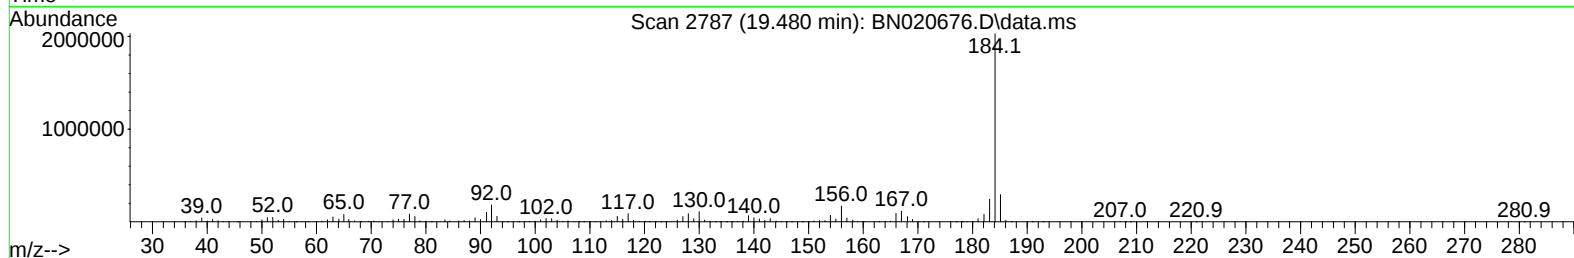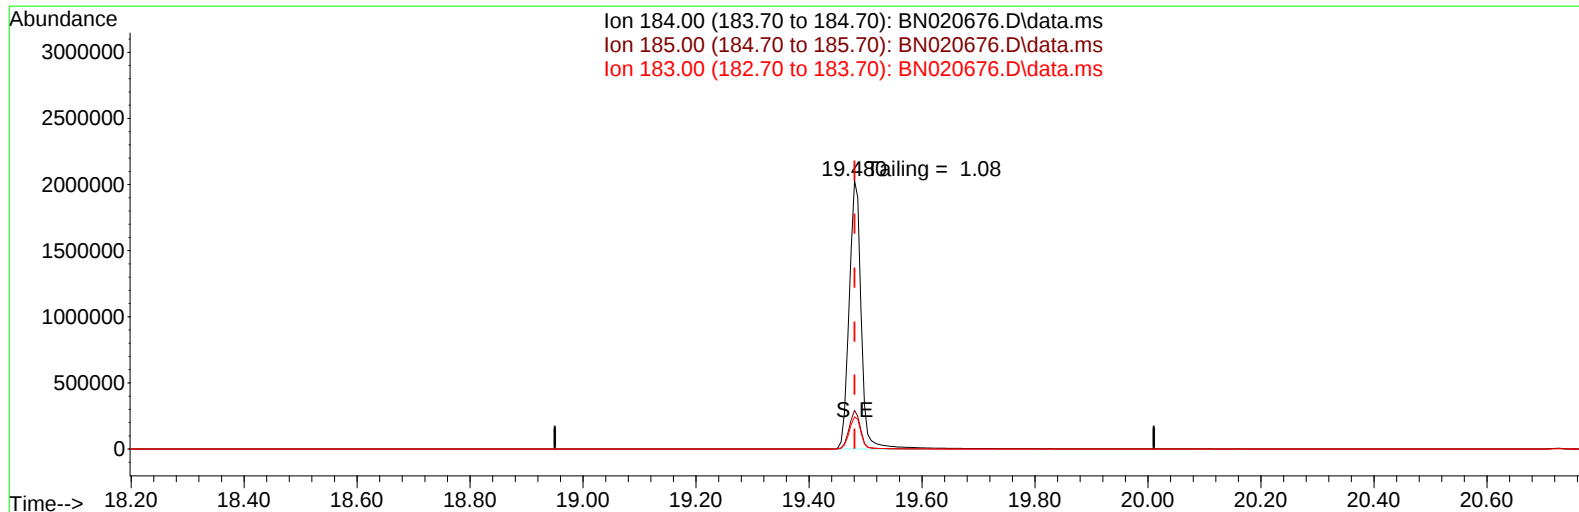

TIC: BN020676.D\data.ms

(77) Benzidine

19.480min (0.000) 0.00 ng

response 3021542

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.45
183.00	13.20	11.98
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/7/2022	BNA_N	<u>BN020676.D</u>
Compound Name	Response	Retention Time
DDT	1499588	20.727
DDD	25507	20.28
DDE	2312	19.774
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27819	1527407	1.82

Instrument :
BNA_N
ClientSampleId :
DFTPP