
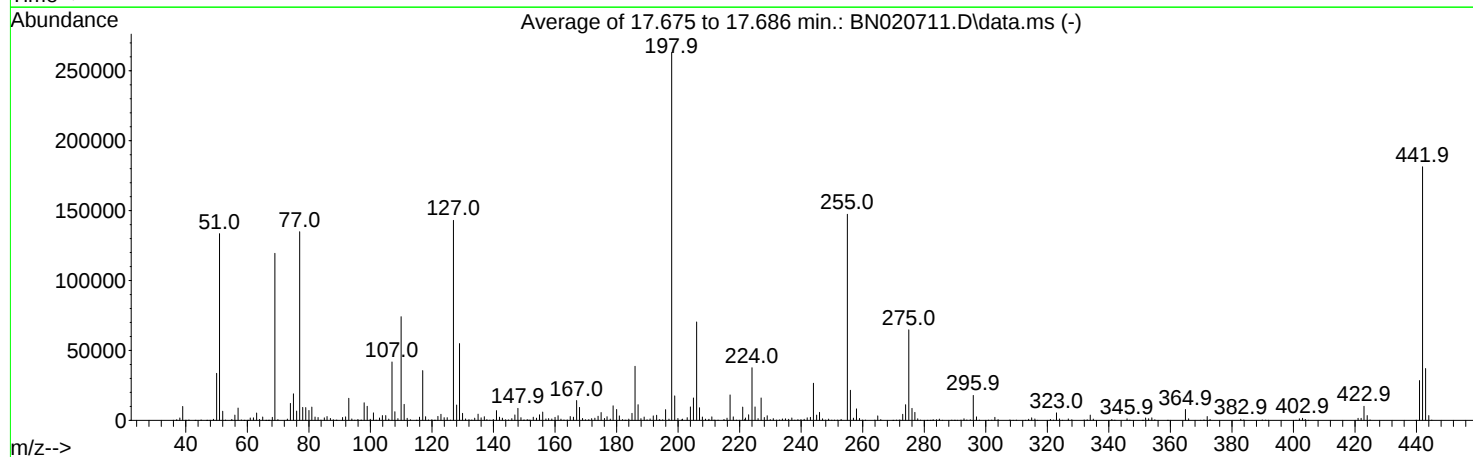


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071222\
 Data File : BN020711.D
 Acq On : 12 Jul 2022 10:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jul 02 03:10:12 2022

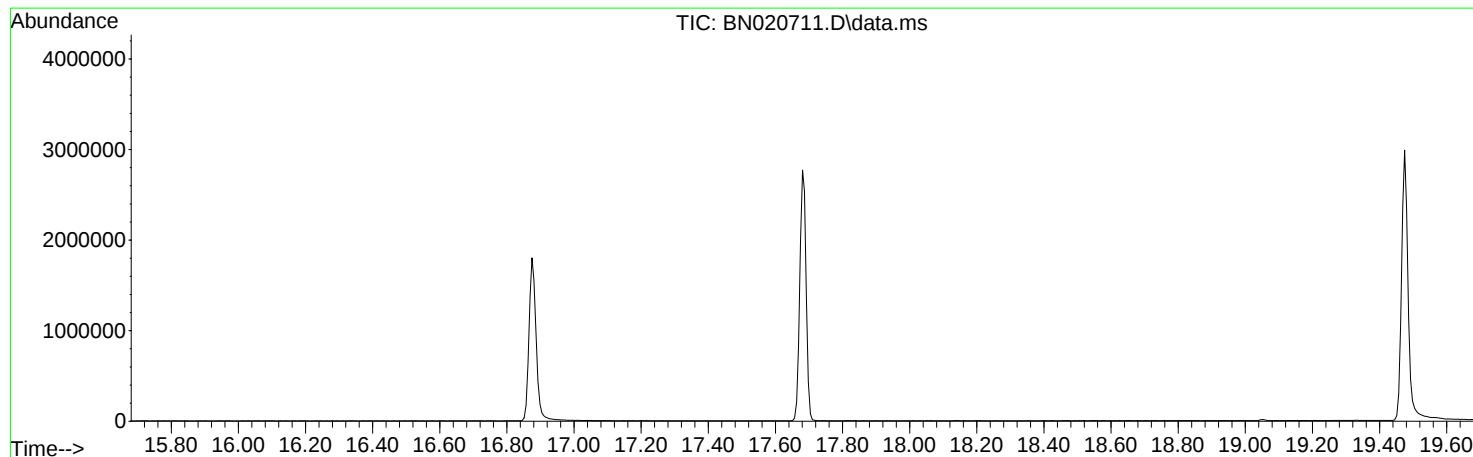




AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.7	133505	PASS
68	69	0.00	2	1.8	2129	PASS
69	198	0.00	100	45.4	119485	PASS
70	69	0.00	2	0.5	592	PASS
127	198	10	80	54.4	143059	PASS
197	198	0.00	2	0.4	987	PASS
198	198	100	100	100.0	263104	PASS
199	198	5	9	6.6	17486	PASS
275	198	10	60	24.6	64755	PASS
365	198	1	100	3.0	7839	PASS
441	198	0.01	100	10.8	28467	PASS
442	442	50	100	100.0	181347	PASS
443	442	15	24	20.5	37112	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071222\
Data File : BN020711.D
Acq On : 12 Jul 2022 10:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 13 03:13:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 13 03:13:12 2022
Response via : Initial Calibration

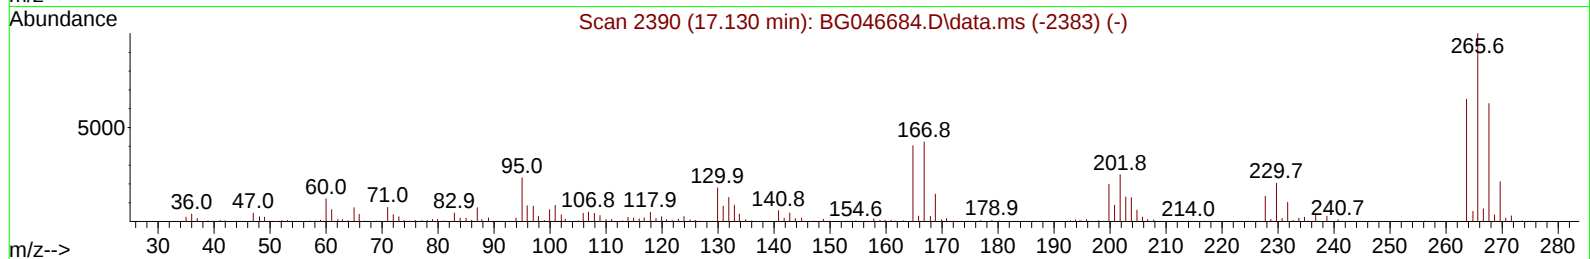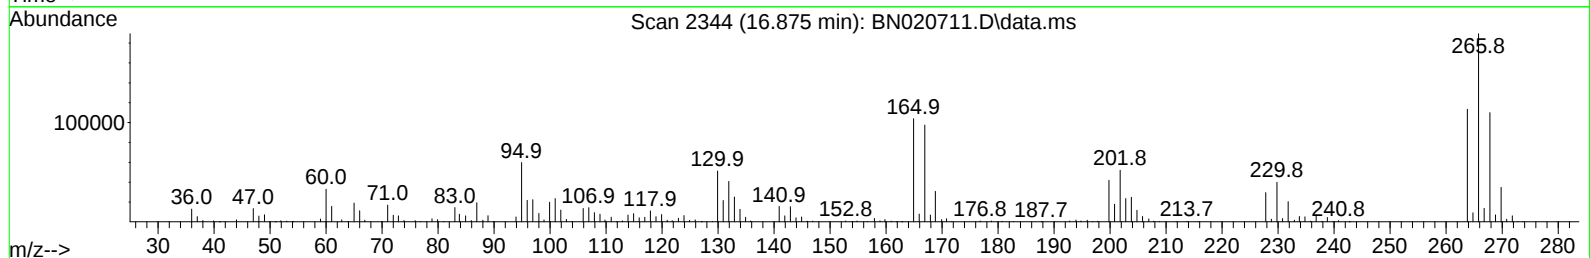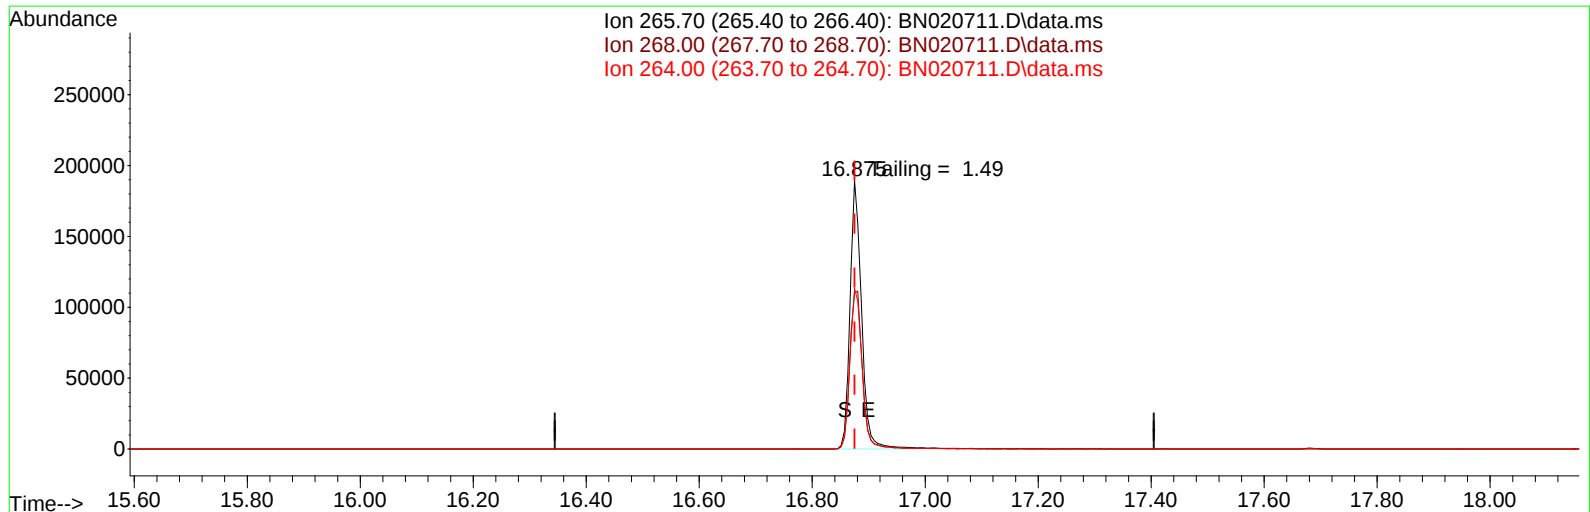

TIC: BN020711.D\data.ms

(70) Pentachlorophenol (C)

16.875min (0.000) 17219.65 ng




response 271352

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.04
264.00	61.60	59.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071222\
Data File : BN020711.D
Acq On : 12 Jul 2022 10:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 13 03:13:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 13 03:13:12 2022
Response via : Initial Calibration

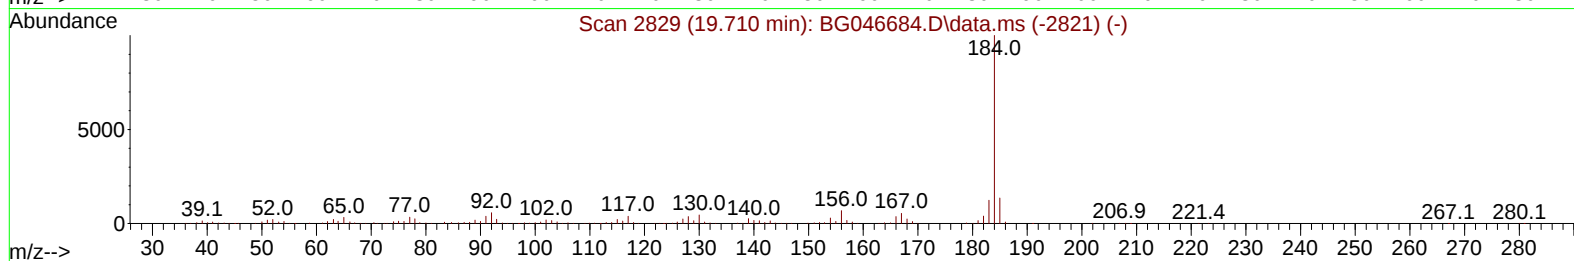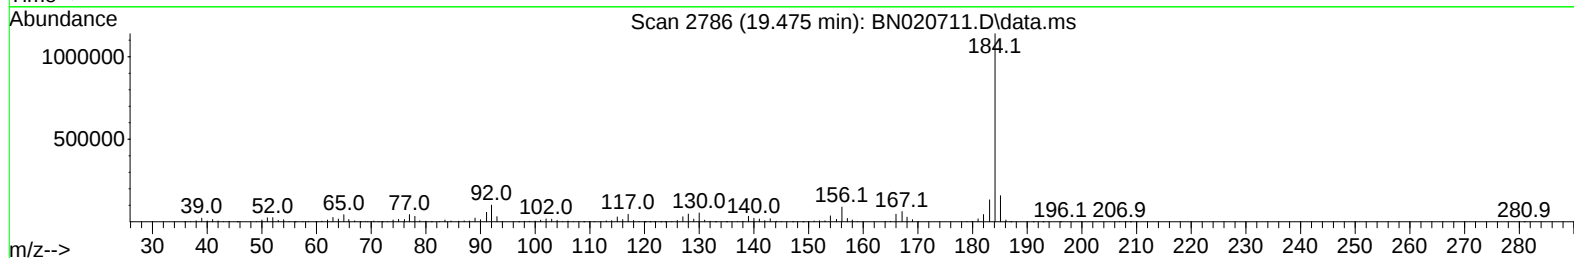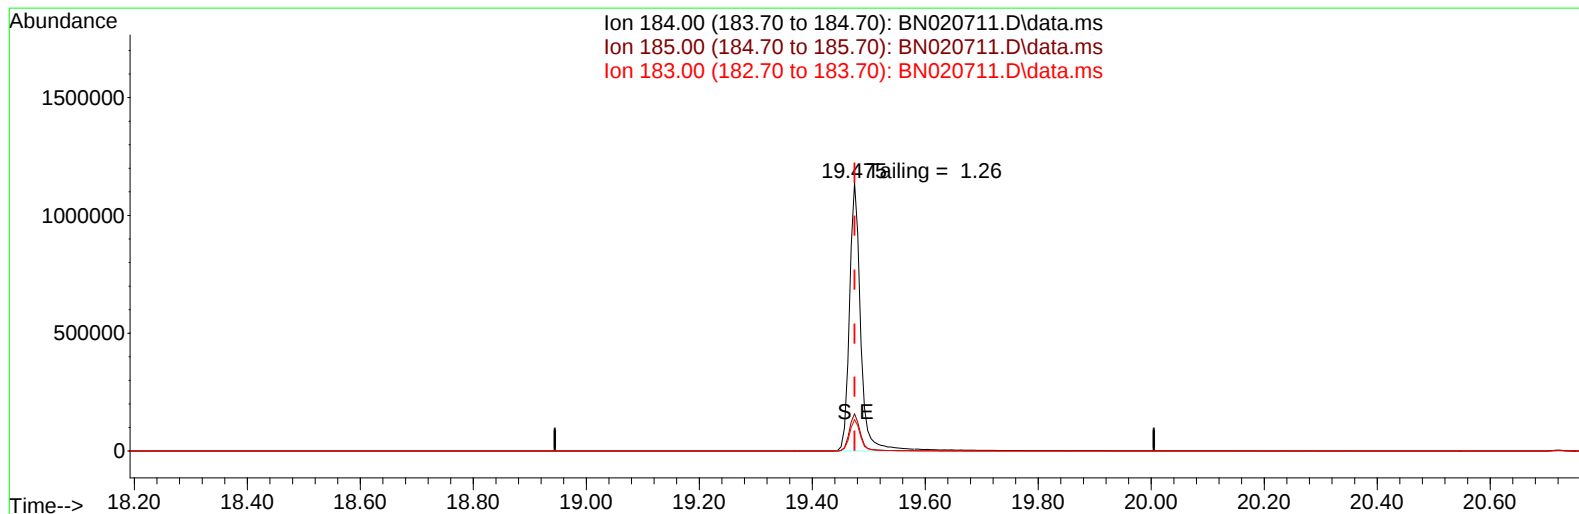

TIC: BN020711.D\data.ms

(77) Benzidine

19.475min (0.000) 0.00 ng

response 1598949

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.89
183.00	13.20	11.70
0.00	0.00	0.00

P

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/12/2022	BNA_N	<u>BN020711.D</u>
Compound Name	Response	Retention Time
DDT	878833	20.722
DDD	15481	20.2
DDE	1252	19.769
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16733	895566	1.87

Instrument :
BNA_N
ClientSampleId :
DFTPP