
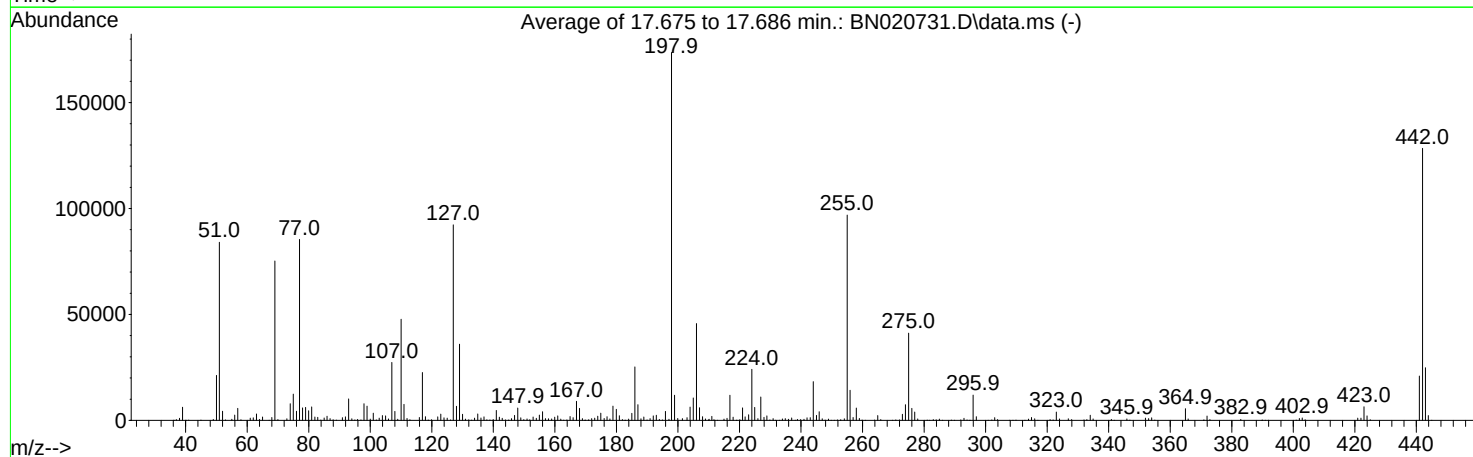


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071422\
 Data File : BN020731.D
 Acq On : 14 Jul 2022 11:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jul 02 03:10:12 2022

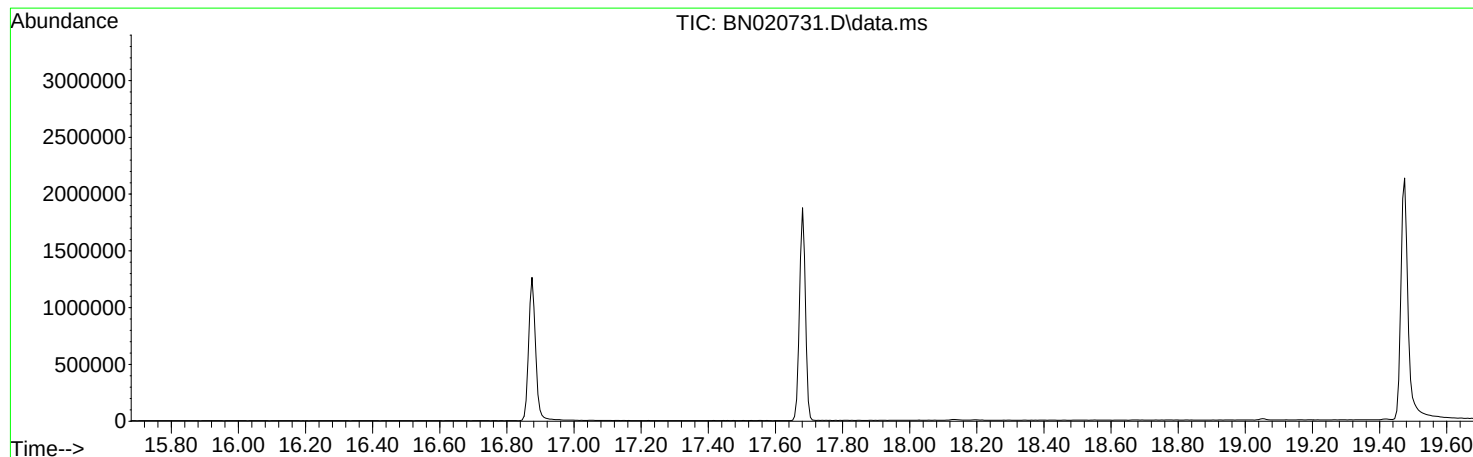




AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.4	84082	PASS
68	69	0.00	2	1.8	1355	PASS
69	198	0.00	100	43.3	75253	PASS
70	69	0.00	2	0.5	354	PASS
127	198	10	80	53.2	92304	PASS
197	198	0.00	2	0.3	496	PASS
198	198	100	100	100.0	173632	PASS
199	198	5	9	6.8	11826	PASS
275	198	10	60	23.7	41163	PASS
365	198	1	100	3.2	5484	PASS
441	198	0.01	100	12.1	20949	PASS
442	442	50	100	100.0	128384	PASS
443	442	15	24	19.4	24853	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071422\
 Data File : BN020731.D
 Acq On : 14 Jul 2022 11:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jul 15 05:47:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 15 05:47:26 2022
 Response via : Initial Calibration

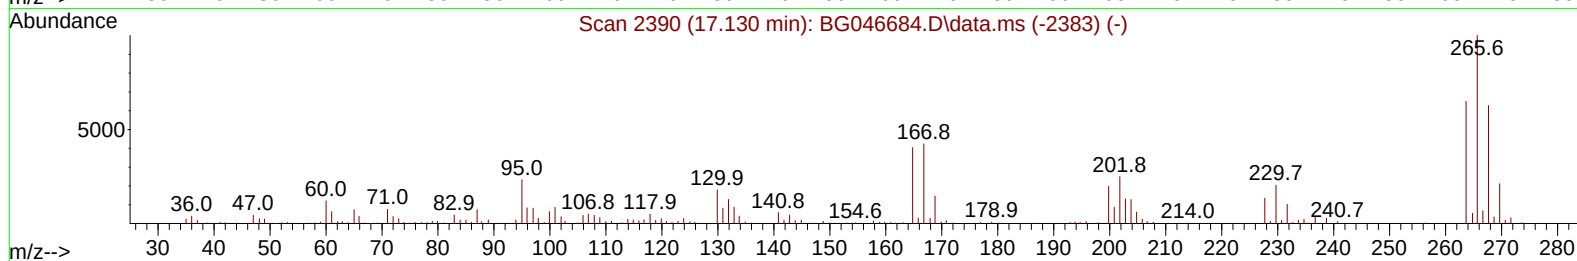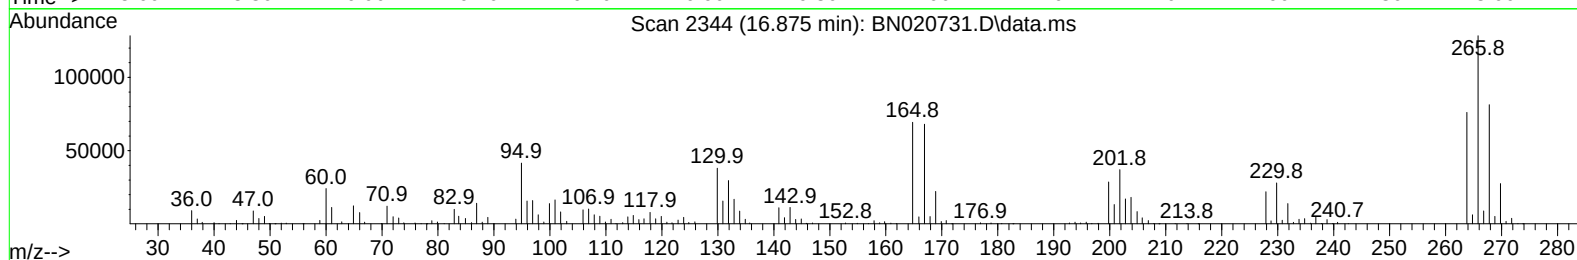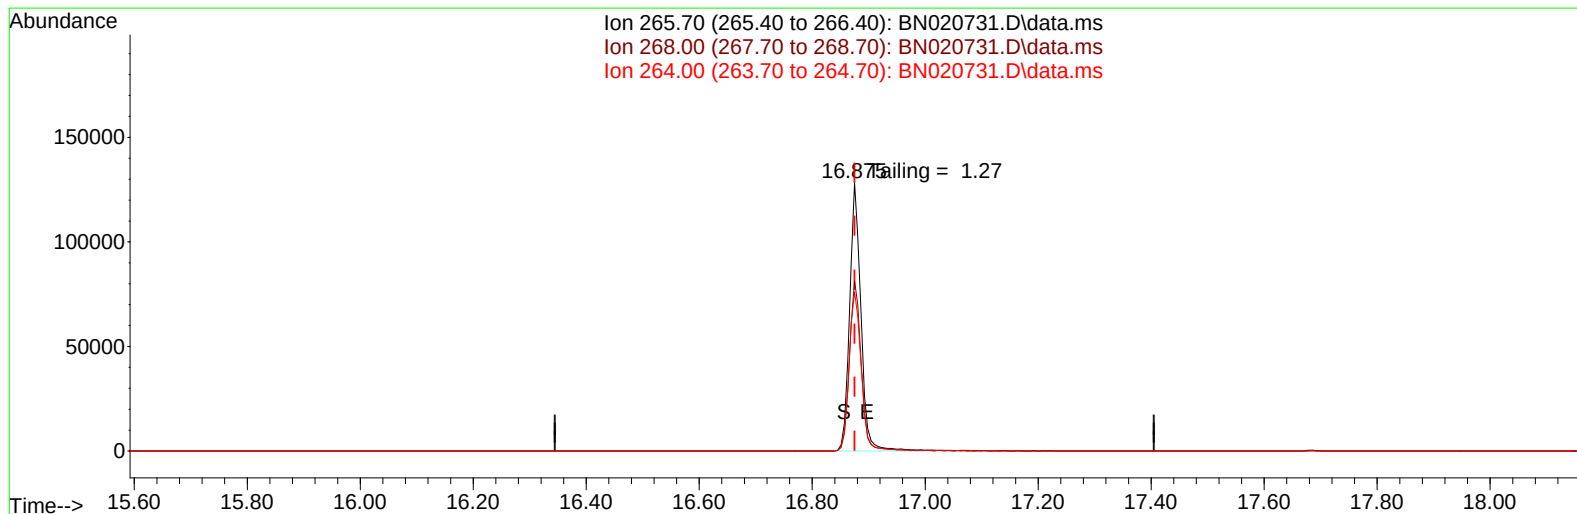

TIC: BN020731.D\data.ms

(70) Pentachlorophenol (C)

16.875min (0.000) 20511.80 ng




response 180288

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.36
264.00	61.60	59.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071422\
Data File : BN020731.D
Acq On : 14 Jul 2022 11:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 15 05:47:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 15 05:47:26 2022
Response via : Initial Calibration

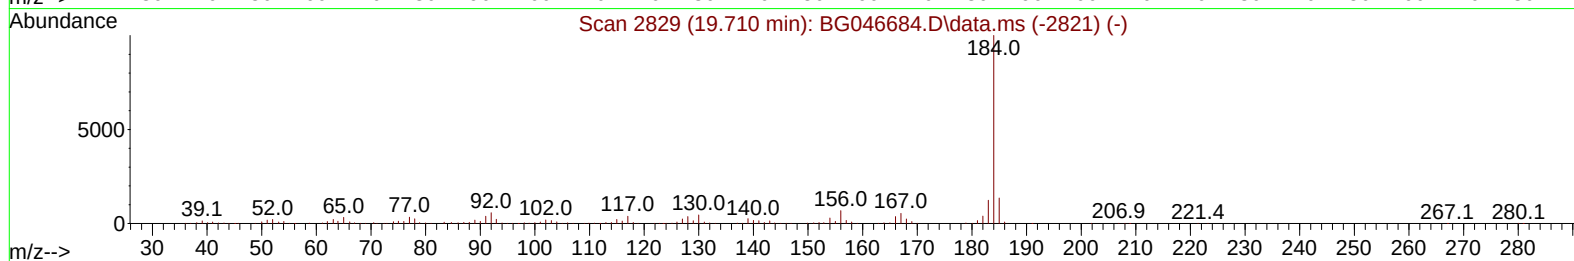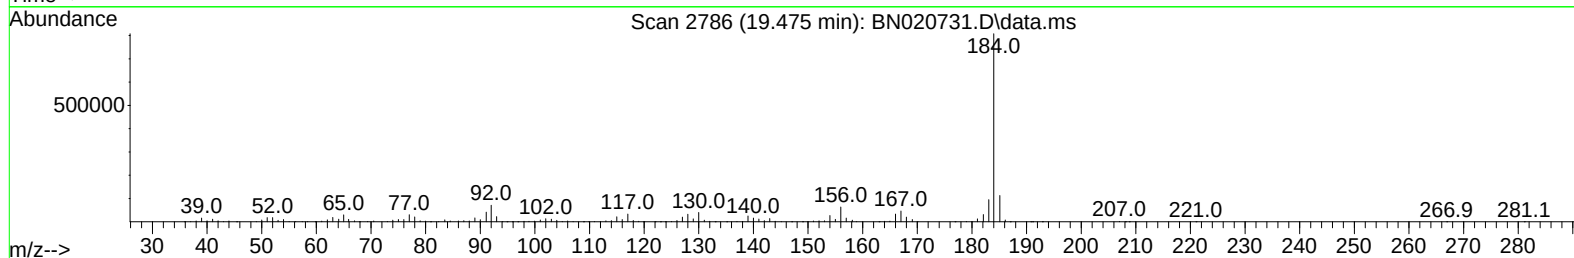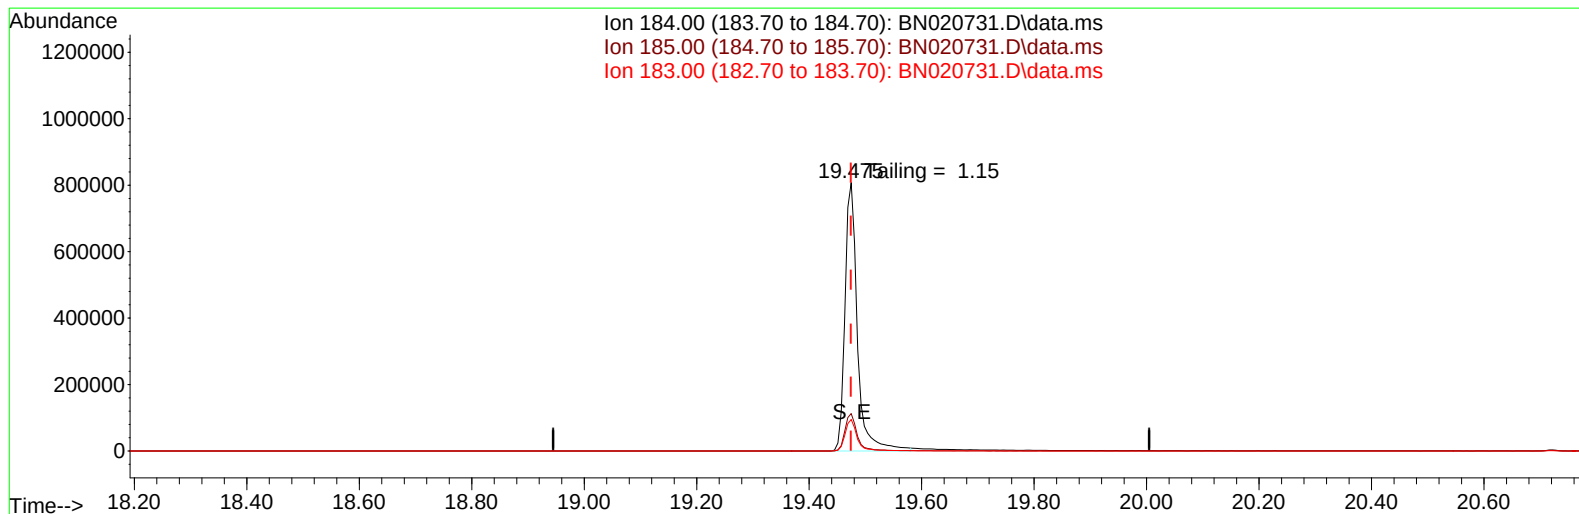

TIC: BN020731.D\data.ms

(77) Benzidine

19.475min (0.000) 0.00 ng

response 1283710

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.00
183.00	13.20	11.77
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/14/2022	BNA_N	<u>BN020731.D</u>
Compound Name	Response	Retention Time
DDT	715224	20.722
DDD	10976	20.28
DDE	782	19.775
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11758	726982	1.62

Instrument :
BNA_N
ClientSampleId :
DFTPP