

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN071520\
 Data File : BN011181.D
 Acq On : 15 Jul 2020 18:15
 Operator : CG/JU
 Sample : L3295-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG098

Quant Time: Jul 16 00:43:25 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071520MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 15 14:43:41 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.49	152	151131	20.00	ng/ul	0.00
18) Naphthalene-d8	10.24	136	628503	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.12	164	396596	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.87	188	921816	20.00	ng/ul	0.00
78) Chrysene-d12	21.09	240	1044794	20.00	ng/ul	0.00
86) Perylene-d12	23.22	264	961742	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.15	96	17830	4.51	ng/uL	0.00
5) Phenol-d5	6.69	99	21583	1.80	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.85	67	188030	29.28	ng/ul	0.00
9) 2-Chlorophenol-d4	7.03	132	192566	18.34	ng/ul	0.00
13) 4-Methylphenol-d8	8.20	113	48019	4.85	ng/ul	0.00
19) Nitrobenzene-d5	8.63	128	150879	29.56	ng/ul	0.00
22) 2-Nitrophenol-d4	9.34	143	155385	28.66	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.87	165	266056	25.30	ng/ul	0.00
29) 4-Chloroaniline-d4	10.25	131	752	0.07	ng/ul	-0.14
44) Dimethylphthalate-d6	13.55	166	1148985	35.73	ng/ul	0.00
47) Acenaphthylene-d8	13.80	160	26644	0.70	ng/ul	0.00
52) 4-Nitrophenol-d4	14.35	143	35019	6.09	ng/ul	0.00
58) Fluorene-d10	15.12	176	984173	34.60	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.25	200	184229	32.75	ng/ul	0.00
71) Anthracene-d10	16.97	188	175398	3.91	ng/ul	0.00
79) Pyrene-d10	19.28	212	770100	14.78	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.09	264	492089	9.44	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.59	163	133133	3.918	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN071520\
Data File : BN011181.D
Acq On : 15 Jul 2020 18:15
Operator : CG/JU
Sample : L3295-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG098

Quant Time: Jul 16 00:43:25 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 15 14:43:41 2020
Response via : Initial Calibration

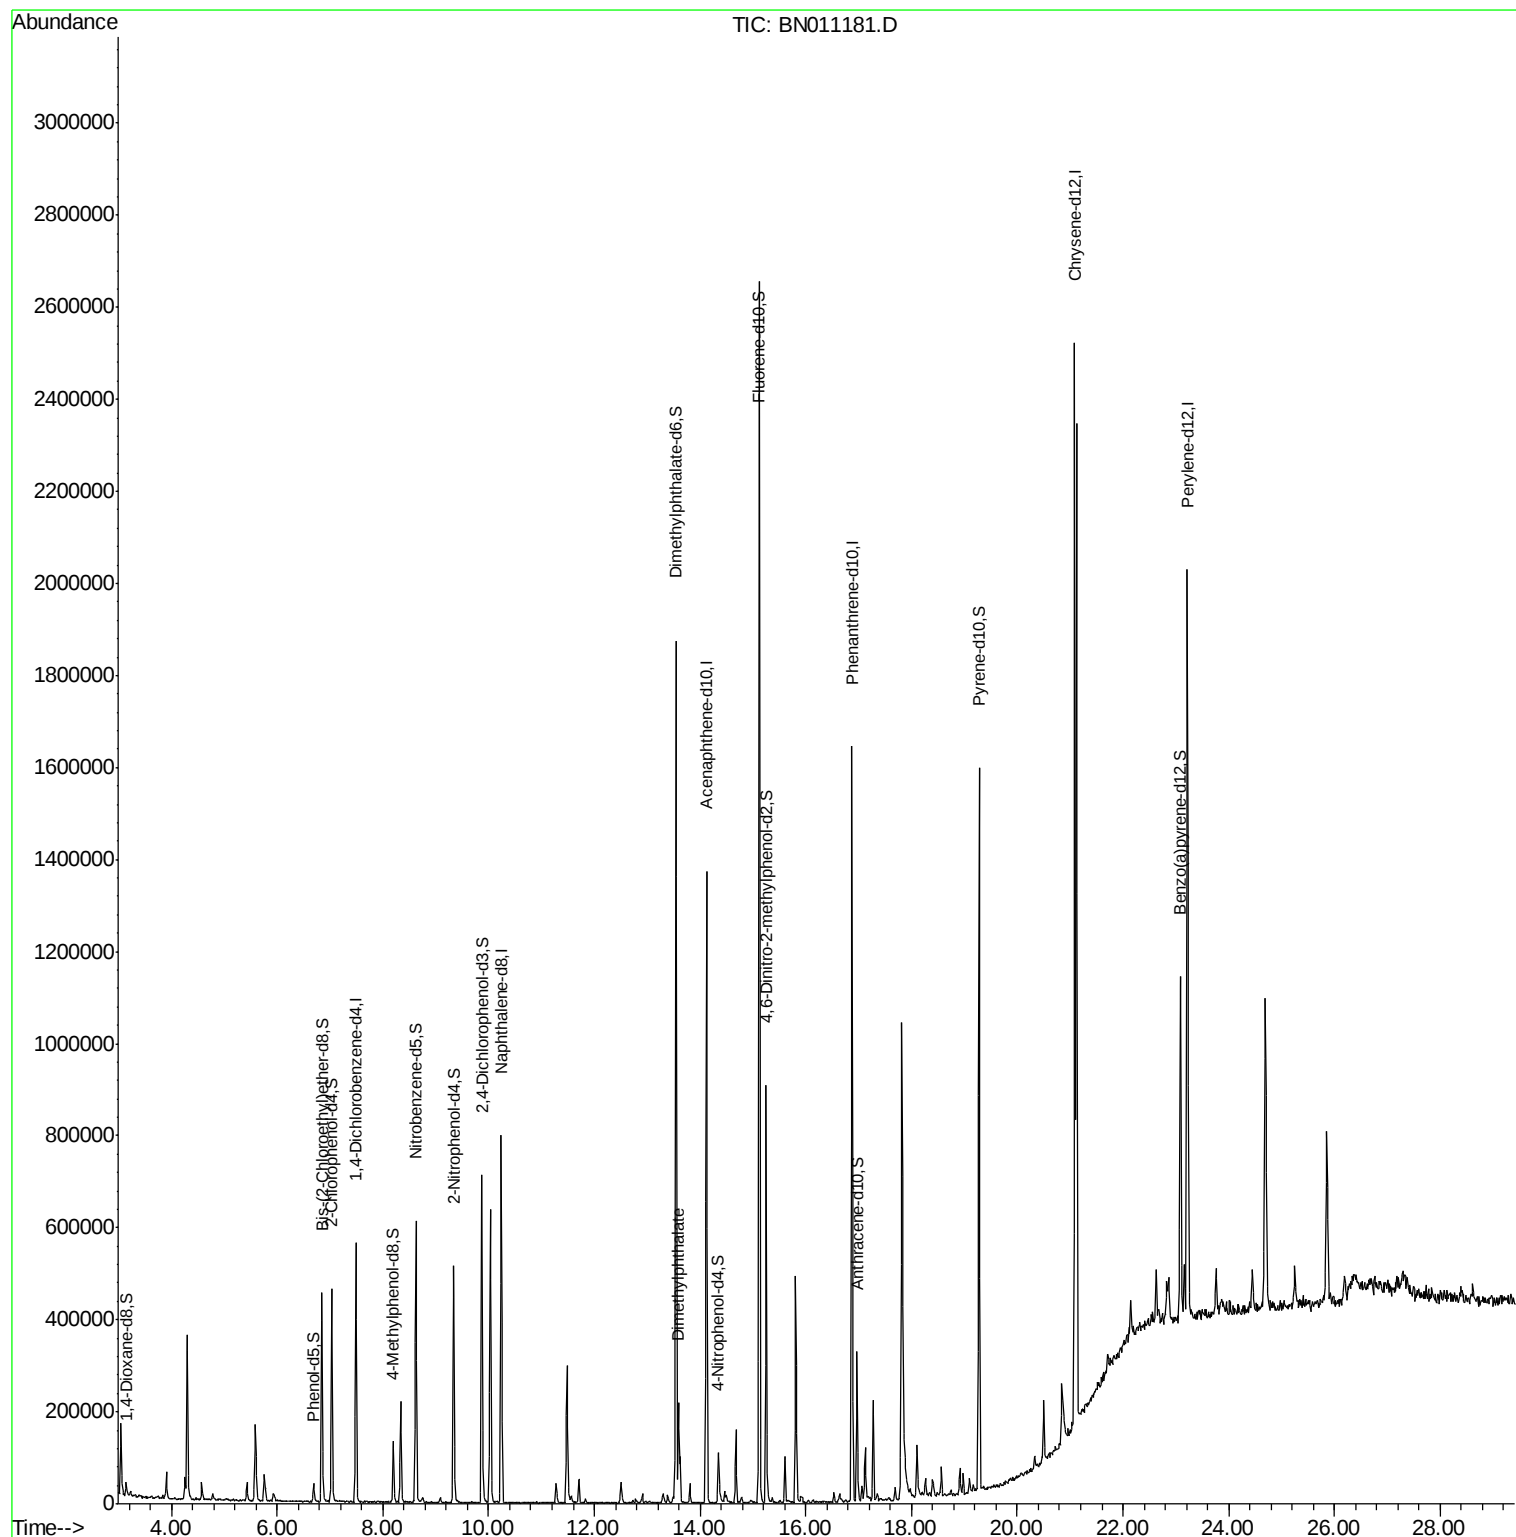

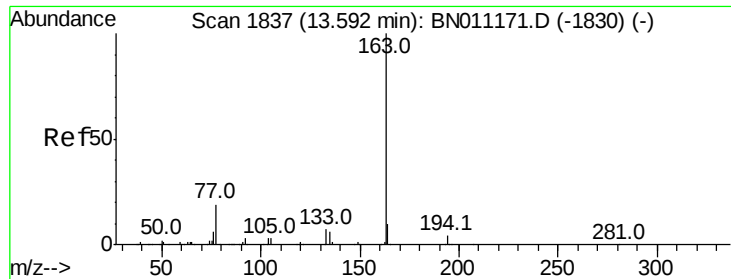

#45

Dimethylphthalate

Concen: 3.918 ng/ul

RT: 13.59 min Scan# 1803

Delta R.T. -0.00 min

Lab File: BN011181.D

Acq: 15 Jul 2020 18:15

Instrument :

BNA_N

ClientSampleId :

BG098


Tot Ion:163 Resp: 133133

Ion Ratio Lower Upper

163 100

194 3.8 3.4 5.0

164 9.7 7.8 11.8

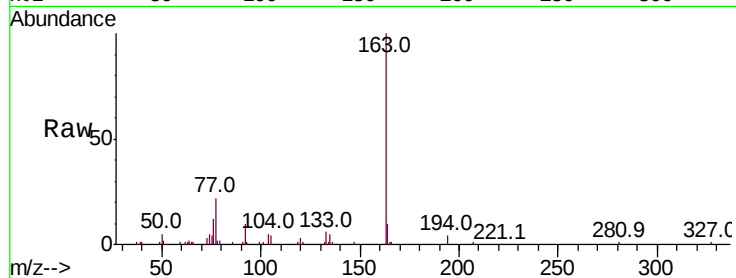

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

