
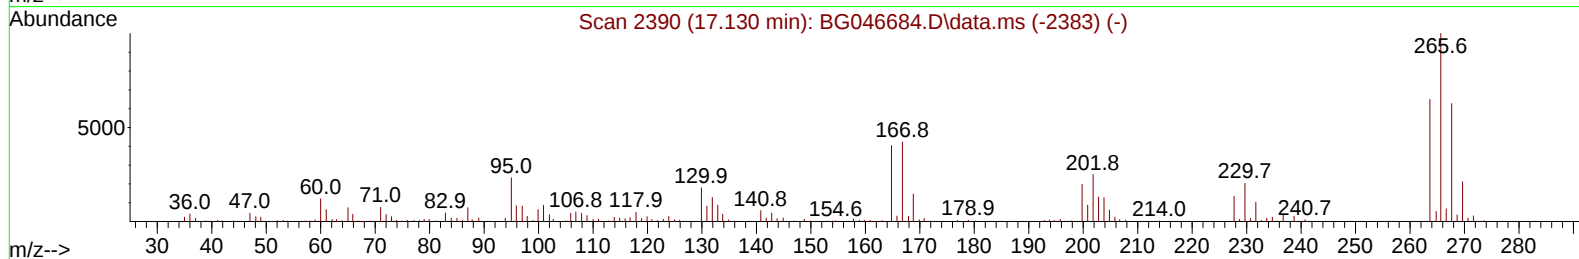
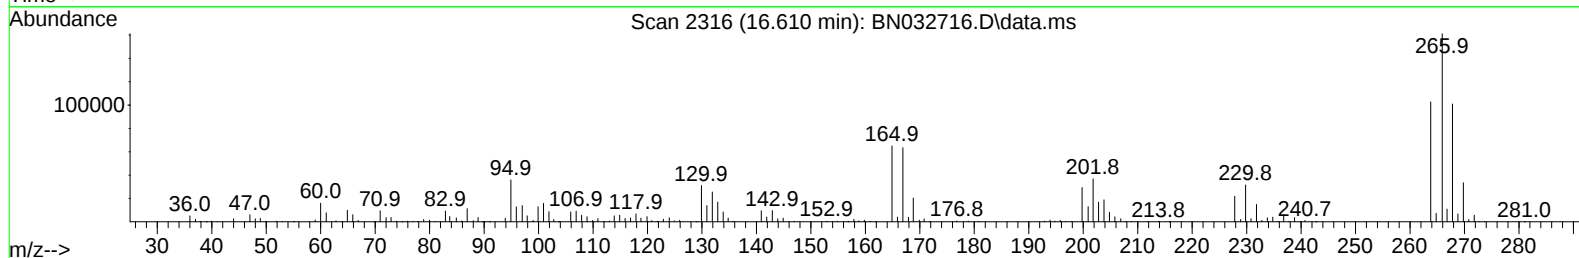


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071524\
Data File : BN032716.D
Acq On : 15 Jul 2024 10:01
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 11:22:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 11 03:07:33 2024
Response via : Initial Calibration

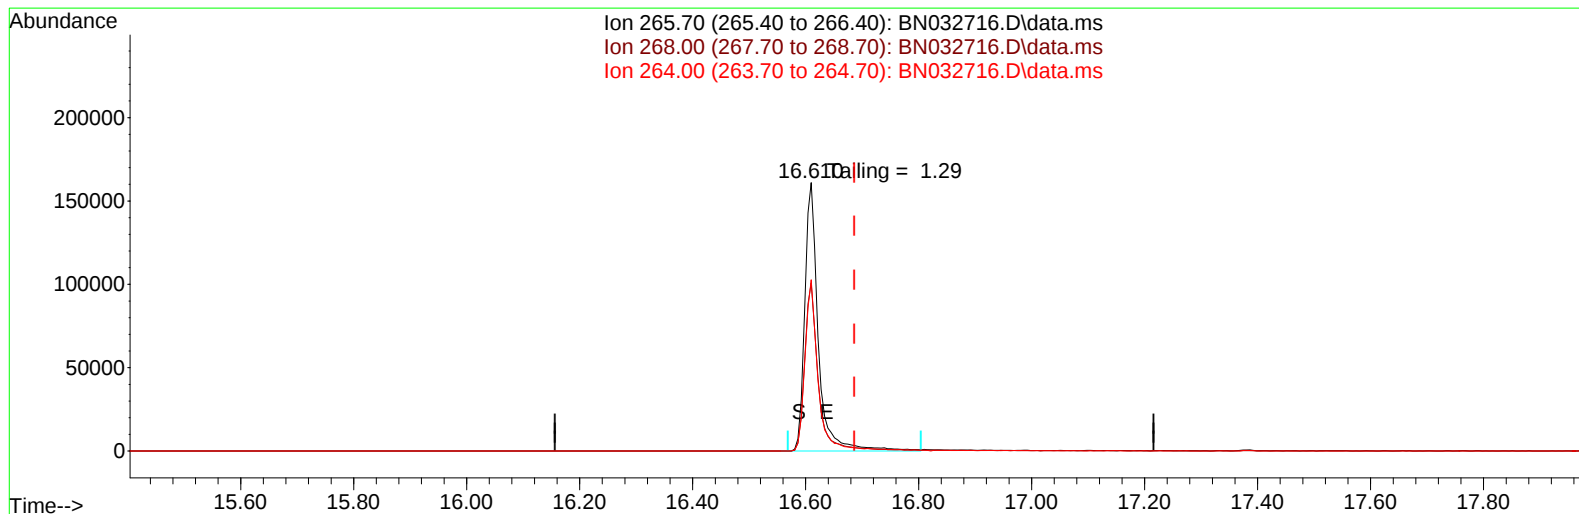

TIC: BN032716.D\data.ms

(70) Pentachlorophenol (C)




16.610min (-0.076) 22788.89 ng m

response 270766

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.63
264.00	61.60	63.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071524\
Data File : BN032716.D
Acq On : 15 Jul 2024 10:01
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 11:22:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 11 03:07:33 2024
Response via : Initial Calibration

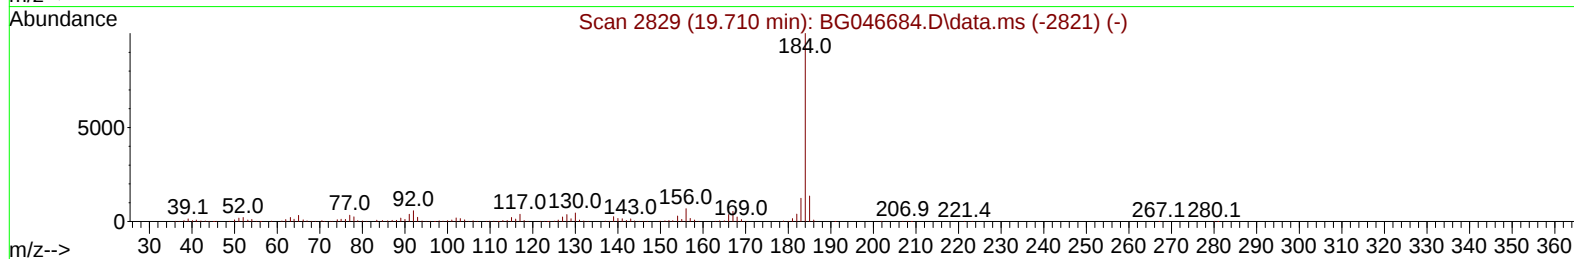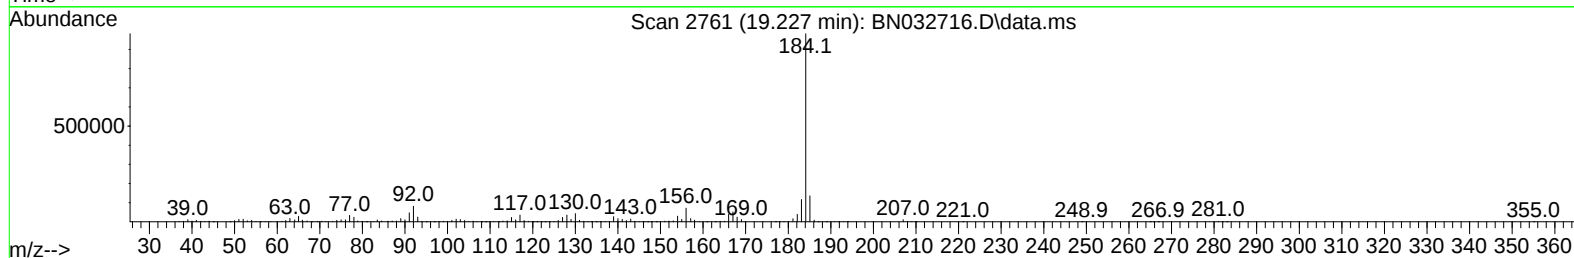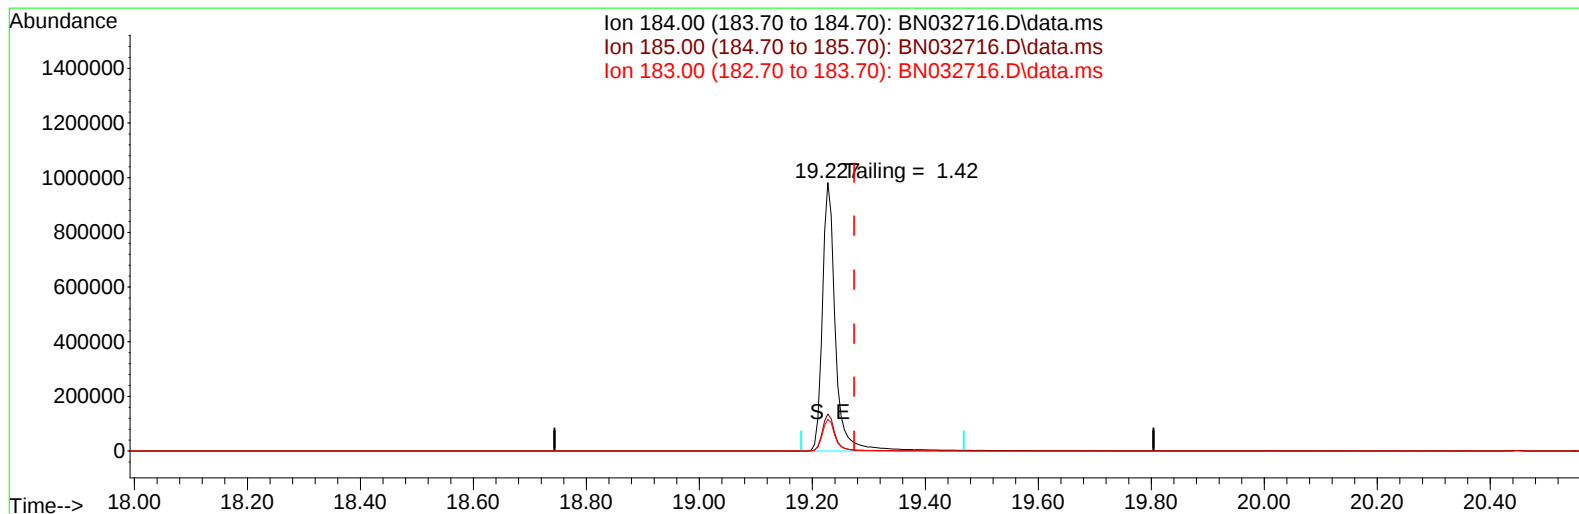

TIC: BN032716.D\data.ms

(77) Benzidine**19.227min (-0.047) 935218.39 ng****response 1585565**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.81
183.00	13.20	11.81
0.00	0.00	0.00