


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071524\
Data File : BN032716.D
Acq On : 15 Jul 2024 10:01
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN071124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jul 10 23:45:48 2024

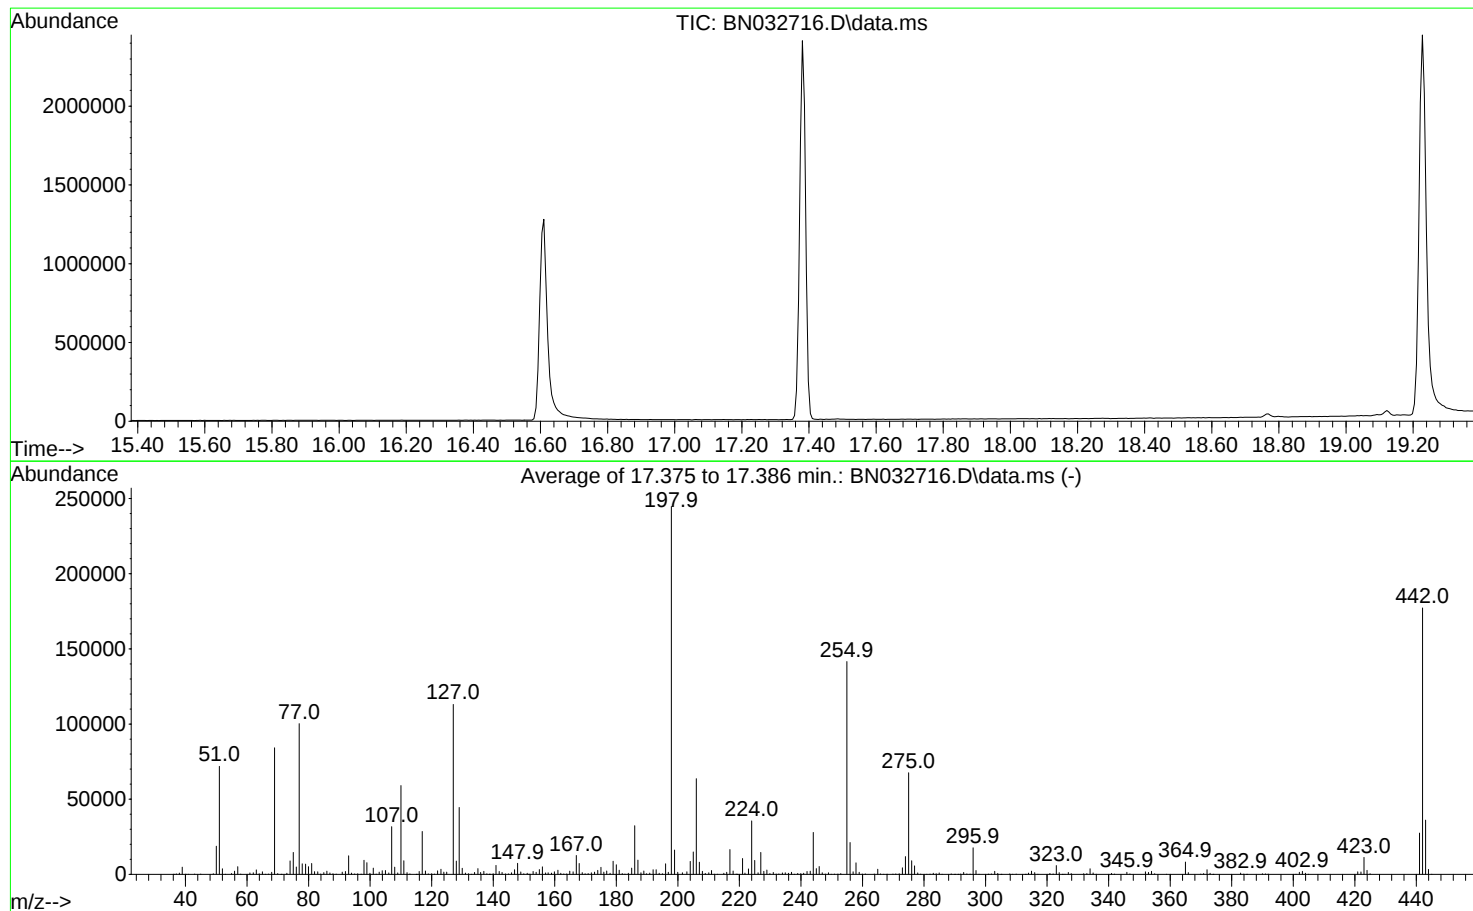

AutoFind: Scans 2446, 2447, 2448; Background Corrected with Scan 2439

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.4	71880	PASS
68	69	0.00	2	1.7	1437	PASS
69	198	0.00	100	34.4	84240	PASS
70	69	0.00	2	0.6	507	PASS
127	198	10	80	46.2	113096	PASS
197	198	0.00	2	0.6	1397	PASS
198	198	100	100	100.0	244736	PASS
199	198	5	9	6.6	16177	PASS
275	198	10	60	27.6	67603	PASS
365	198	1	100	3.4	8221	PASS
441	198	0.01	100	11.2	27523	PASS
442	442	50	100	100.0	177192	PASS
443	442	15	24	20.3	36048	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/15/2024	BNA_N	<u>BN032716.D</u>
Compound Name	Response	Retention Time
DDT	528904	20.445
DDD	224489	20.016
DDE	2683	19.492
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
227172	756076	30.05

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071524\
Data File : BN032716.D
Acq On : 15 Jul 2024 10:01
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 15 11:22:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 11 03:07:33 2024
Response via : Initial Calibration

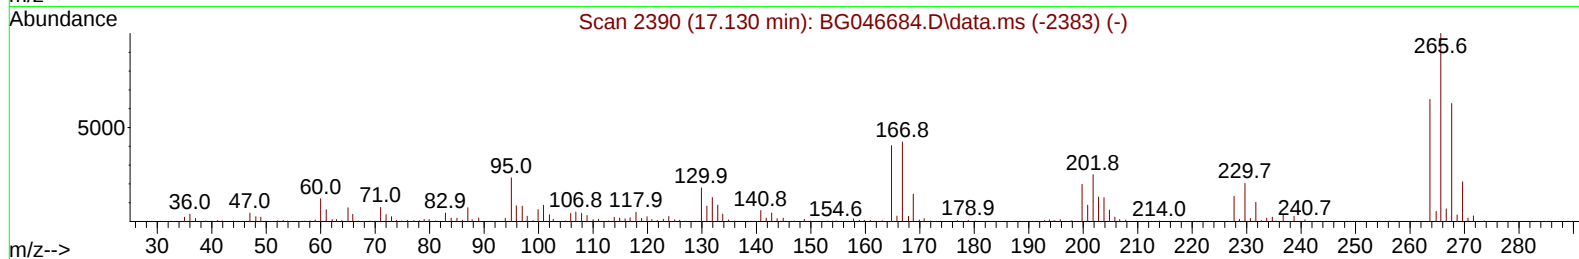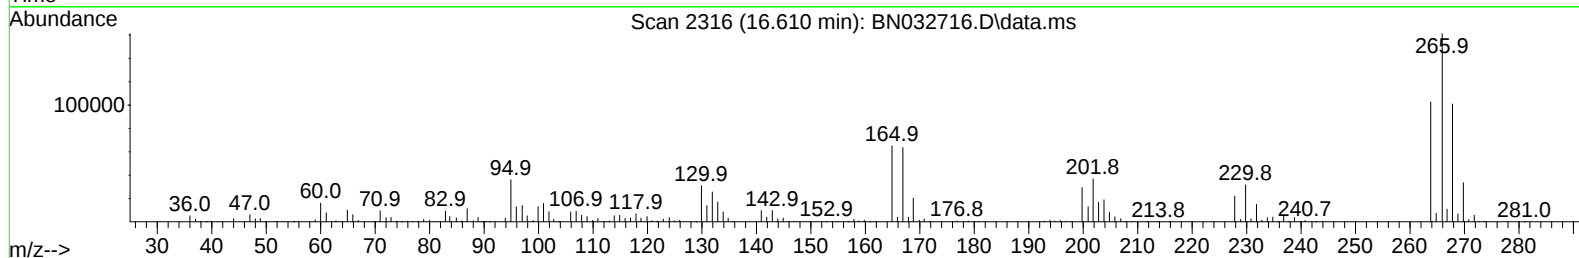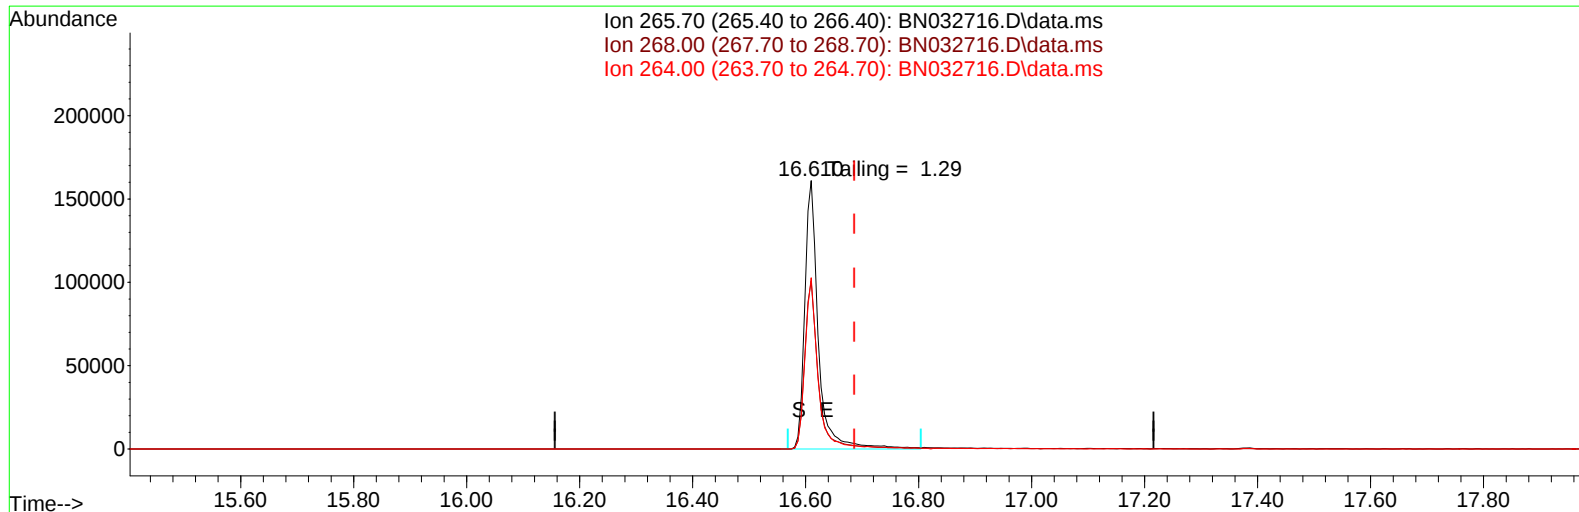

TIC: BN032716.D\data.ms

(70) Pentachlorophenol (C)

16.610min (-0.076) 22788.89 ng m




response 270766

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.63
264.00	61.60	63.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071524\
Data File : BN032716.D
Acq On : 15 Jul 2024 10:01
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 15 11:22:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 11 03:07:33 2024
Response via : Initial Calibration

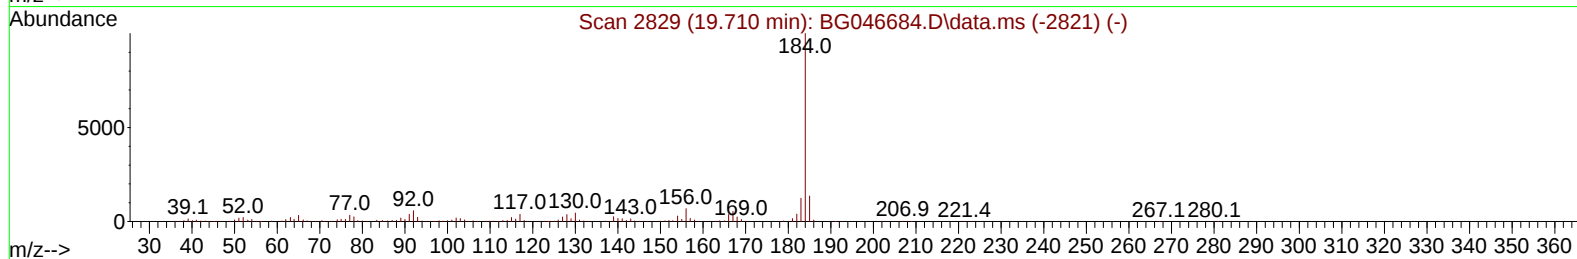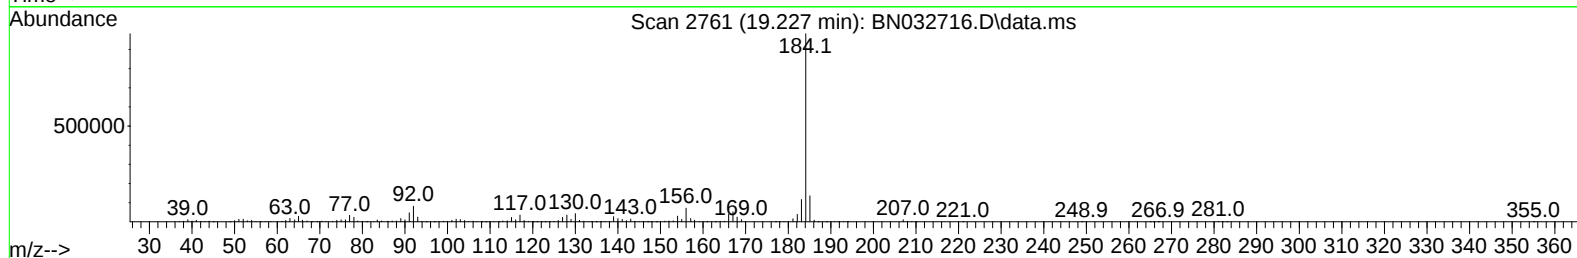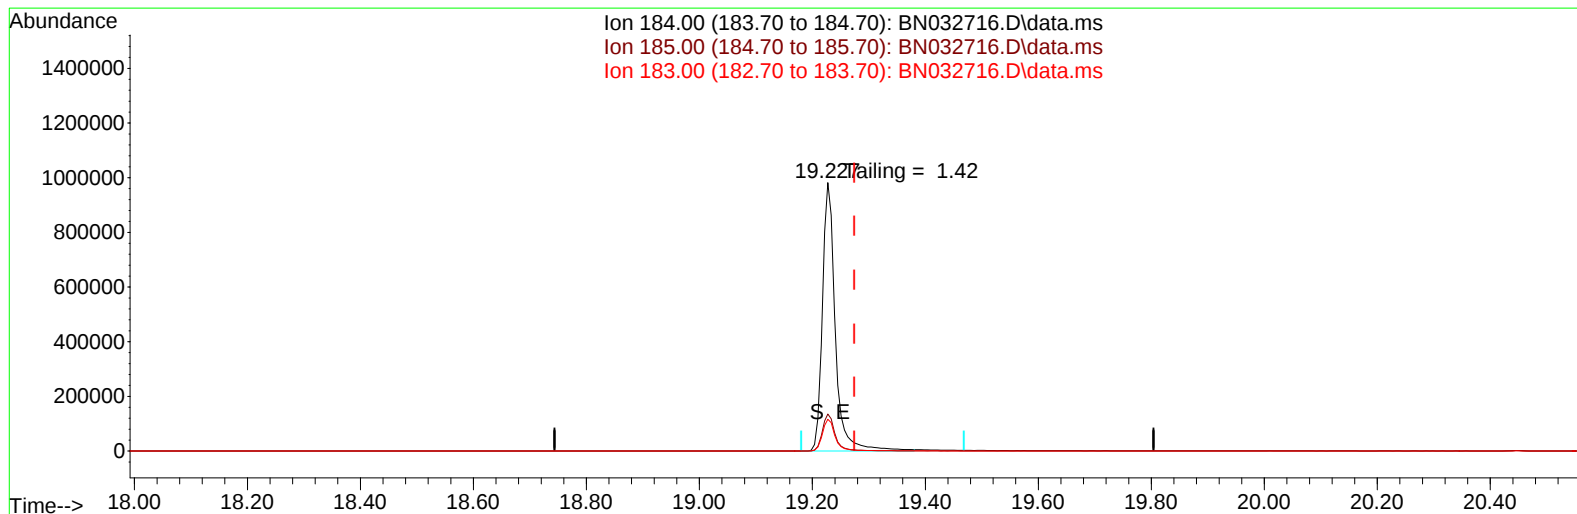

TIC: BN032716.D\data.ms

(77) Benzidine

19.227min (-0.047) 935218.39 ng

response 1585565

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.81
183.00	13.20	11.81
0.00	0.00	0.00