
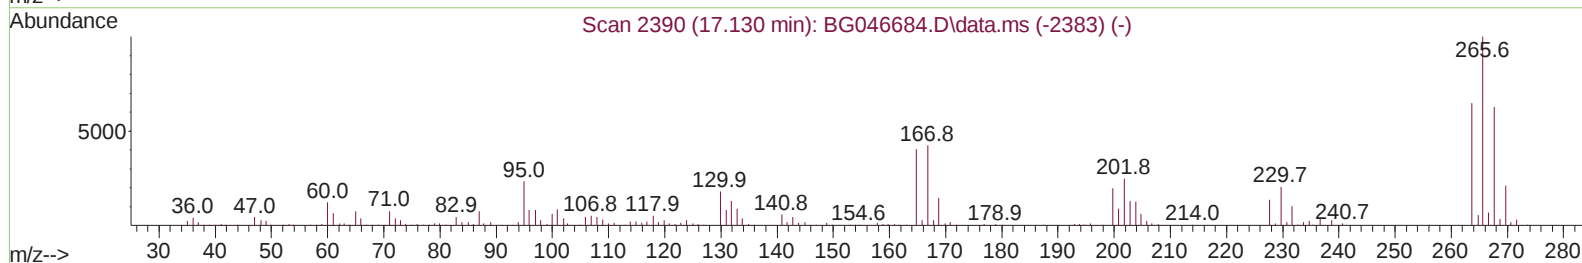
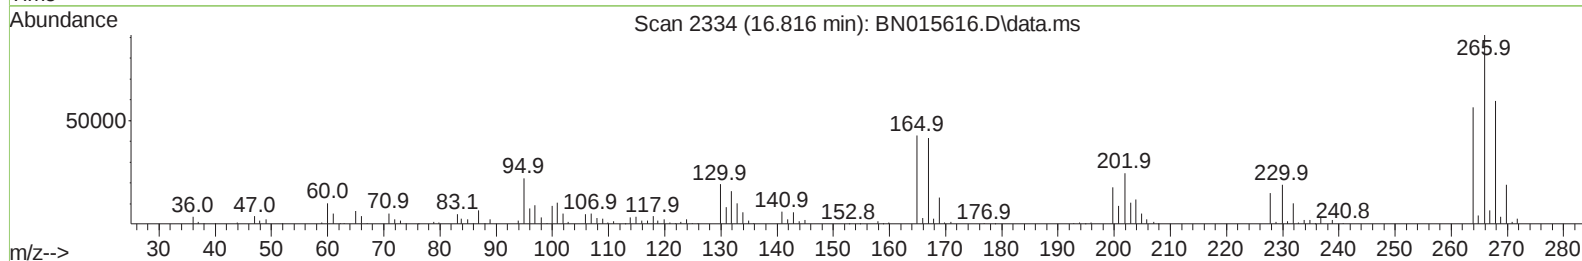


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072021\
Data File : BN015616.D
Acq On : 20 Jul 2021 08:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 20 11:32:34 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 15 05:41:44 2021
Response via : Initial Calibration

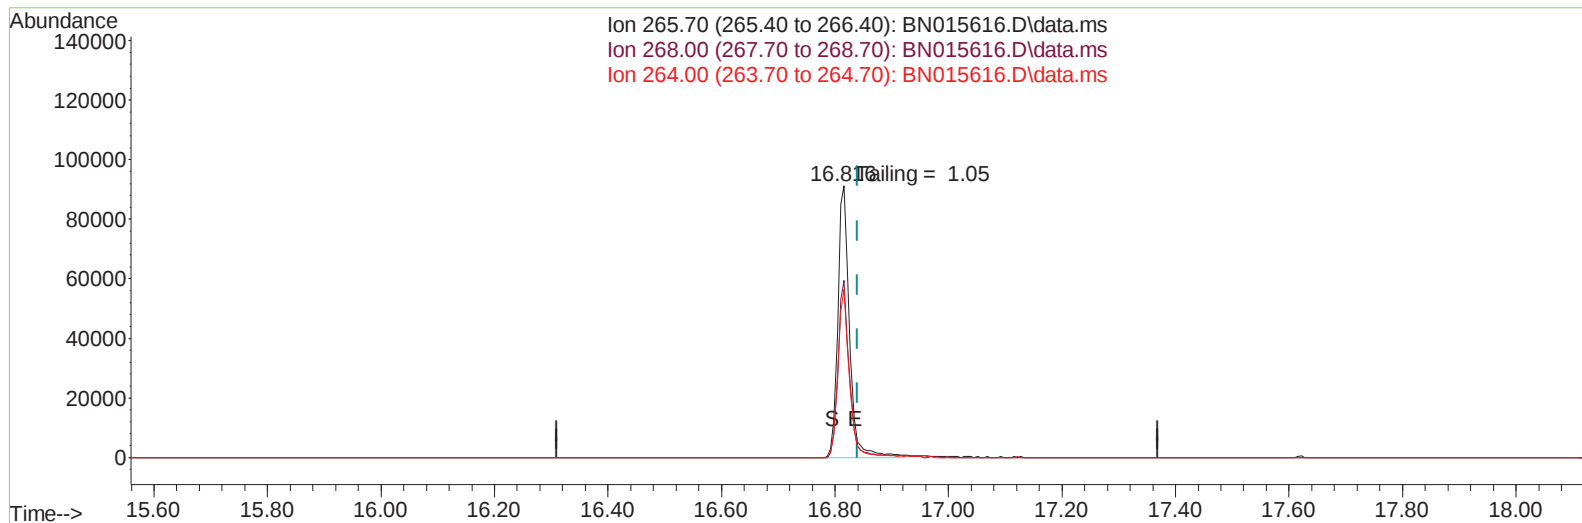




TIC: BN015616.D\data.ms

(70) Pentachlorophenol (C)**16.816min (-0.024) 19344.97 ng****response 132534**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.16
264.00	61.60	61.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072021\
Data File : BN015616.D
Acq On : 20 Jul 2021 08:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 20 11:32:34 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 15 05:41:44 2021
Response via : Initial Calibration

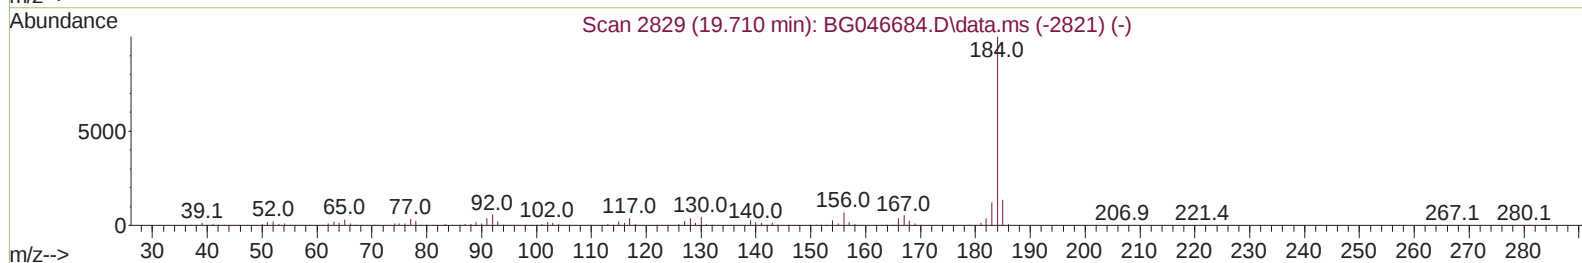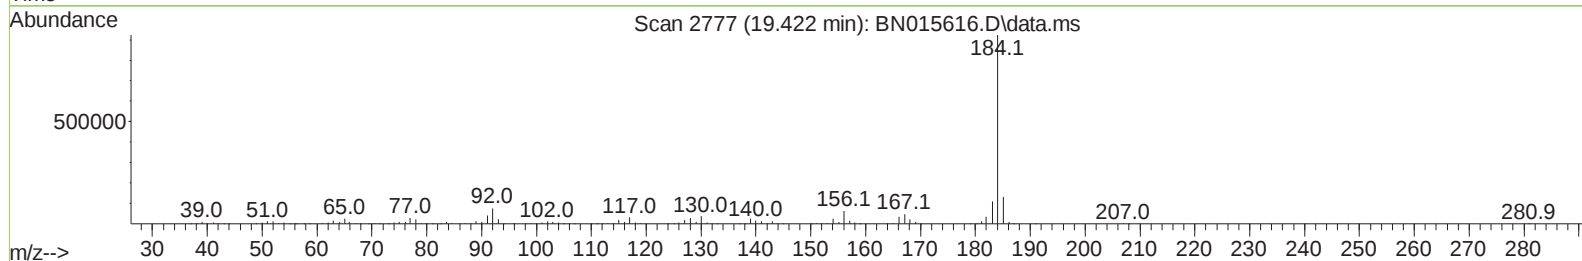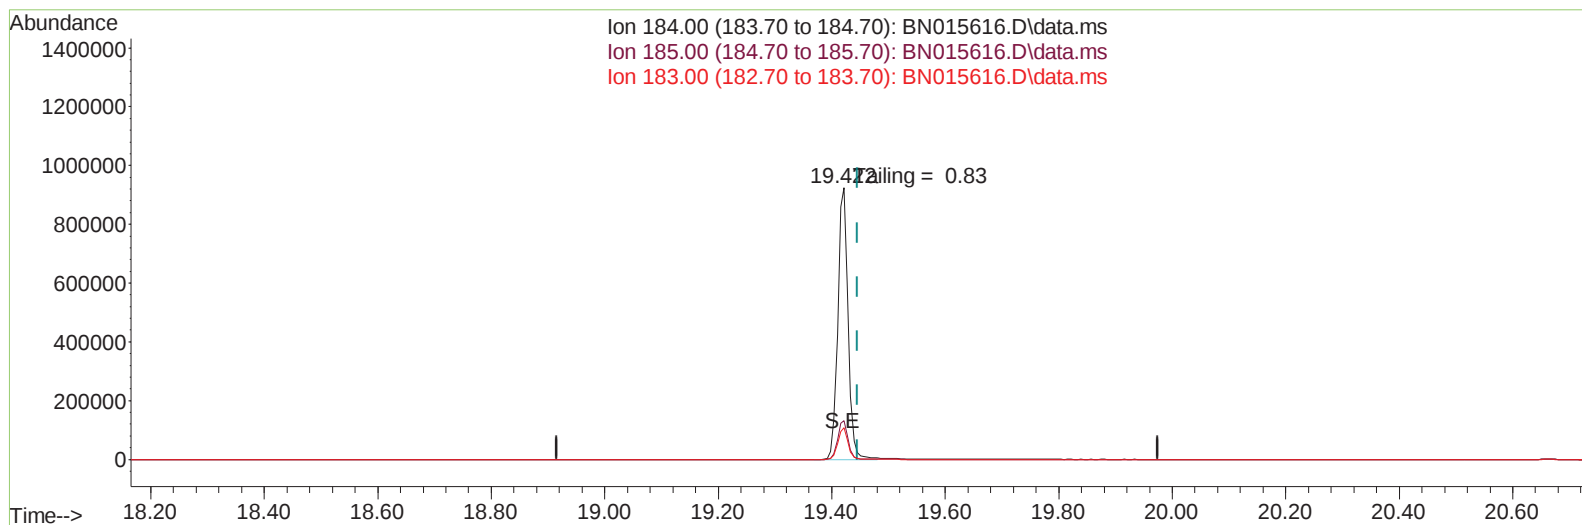

TIC: BN015616.D\data.ms

(77) Benzidine**19.422min (-0.024) 0.00 ng****response 1181408**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.39
183.00	13.20	11.75
0.00	0.00	0.00