


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072021\
 Data File : BN015616.D
 Acq On : 20 Jul 2021 08:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN071521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 20 11:13:03 2021

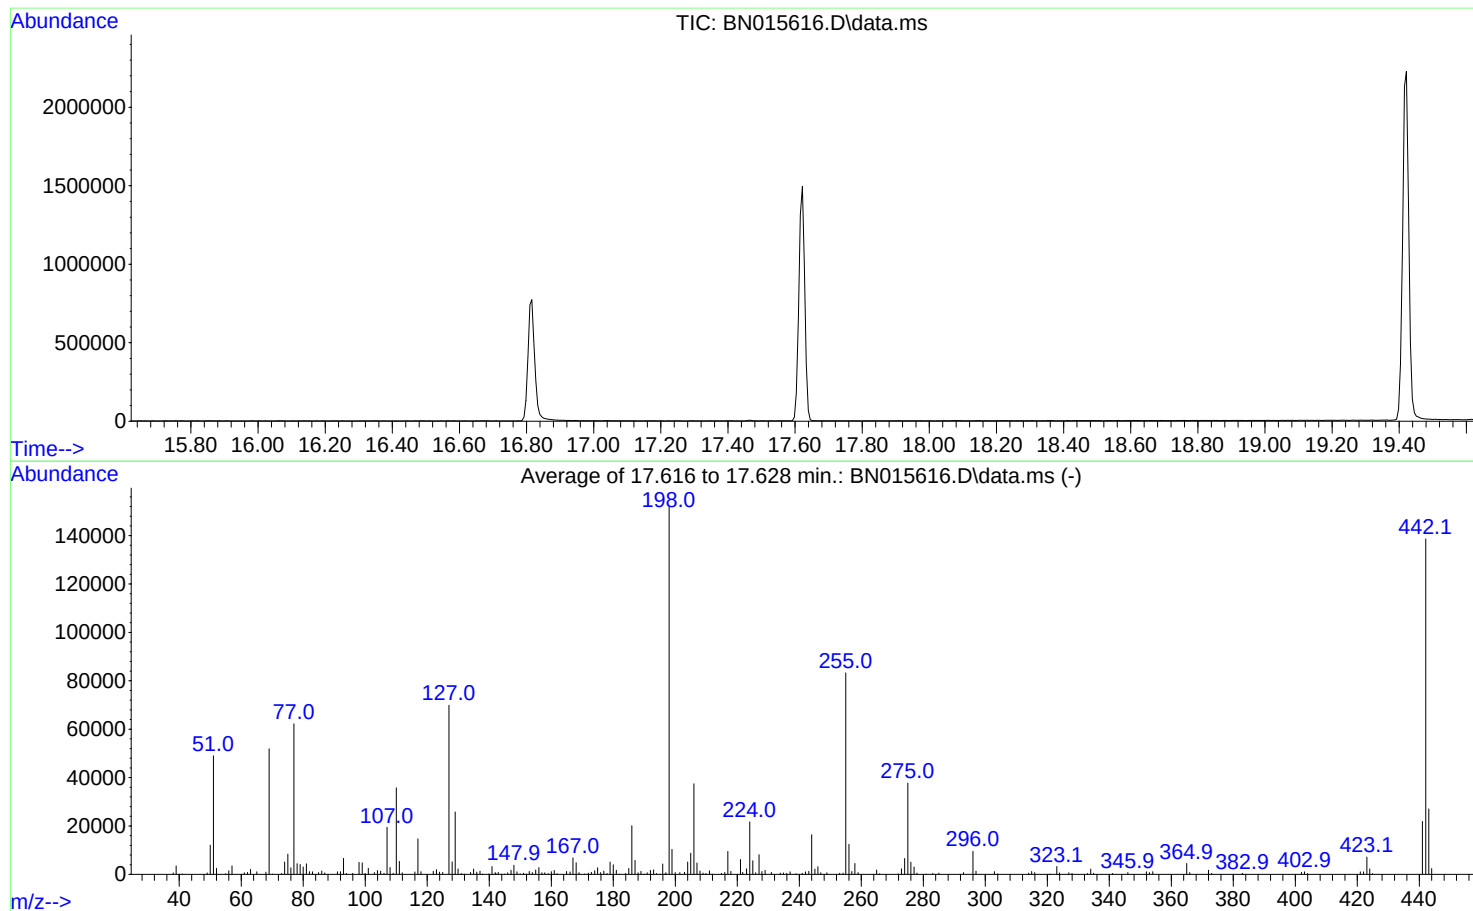




AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.2	48976	PASS
68	69	0.00	2	1.8	933	PASS
69	198	0.00	100	34.1	51883	PASS
70	69	0.00	2	0.2	116	PASS
127	198	10	80	46.0	69888	PASS
197	198	0.00	2	0.5	690	PASS
198	198	100	100	100.0	152035	PASS
199	198	5	9	6.8	10304	PASS
275	198	10	60	24.8	37739	PASS
365	198	1	100	3.0	4514	PASS
441	198	0.01	100	14.4	21872	PASS
442	442	50	100	100.0	138579	PASS
443	442	15	24	19.5	27019	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072021\
Data File : BN015616.D
Acq On : 20 Jul 2021 08:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 20 11:32:34 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 15 05:41:44 2021
Response via : Initial Calibration

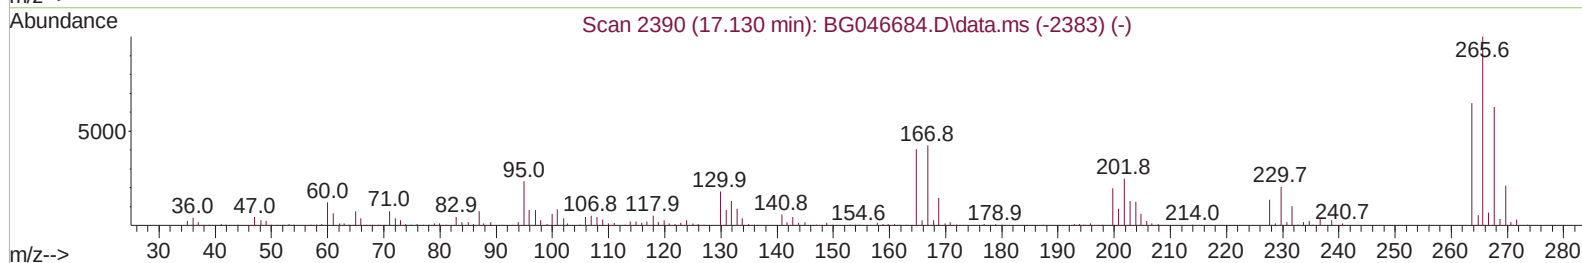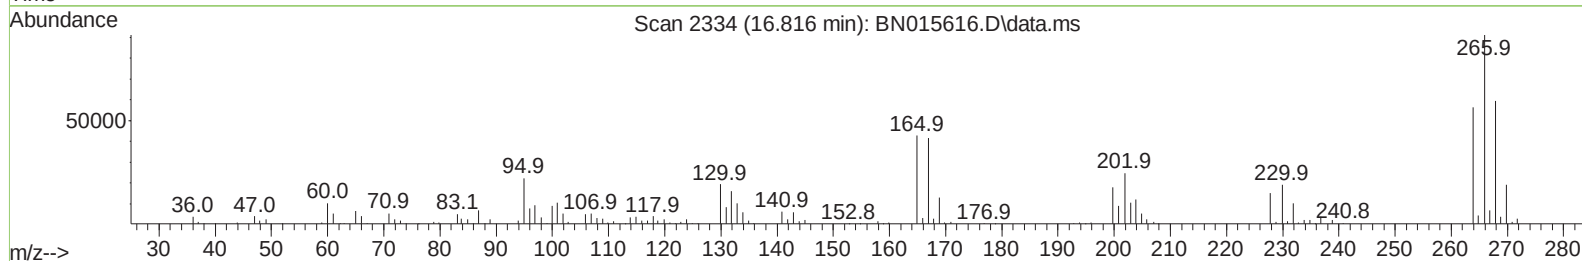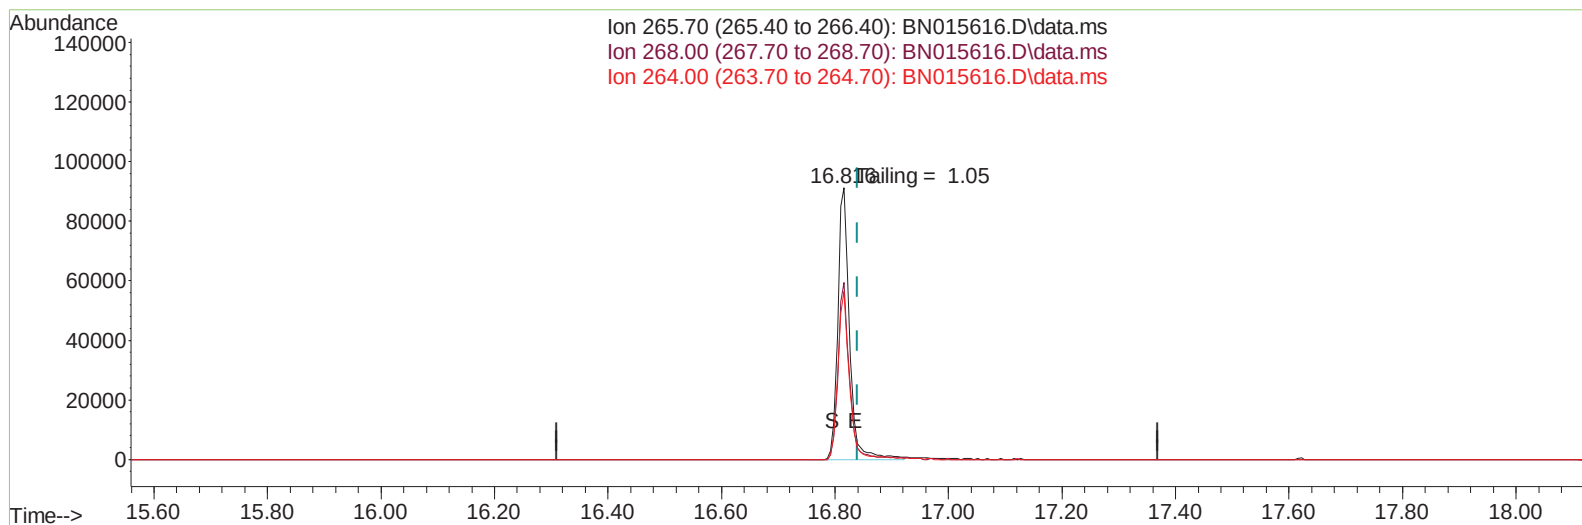

TIC: BN015616.D\data.ms

(70) Pentachlorophenol (C)

16.816min (-0.024) 19344.97 ng




response 132534

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.16
264.00	61.60	61.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072021\
Data File : BN015616.D
Acq On : 20 Jul 2021 08:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 20 11:32:34 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 15 05:41:44 2021
Response via : Initial Calibration

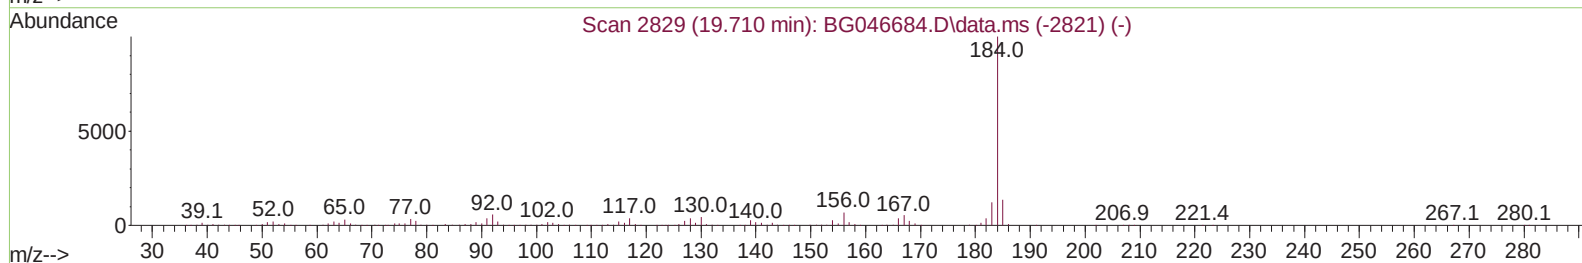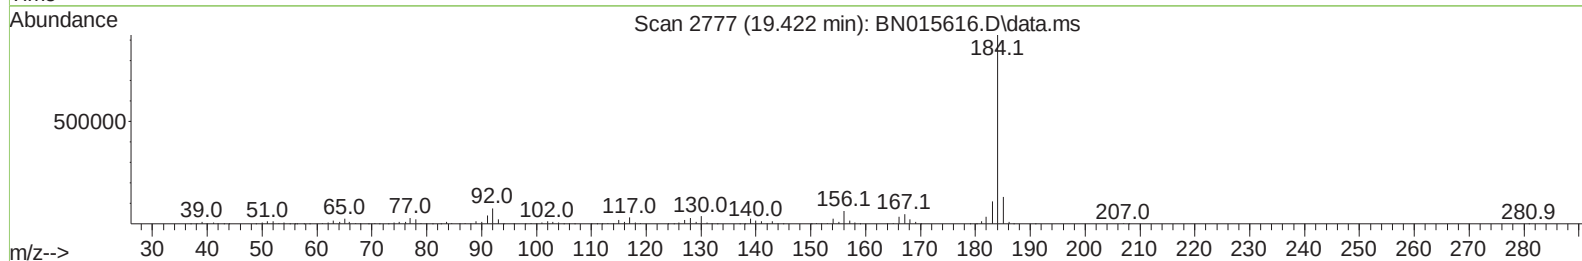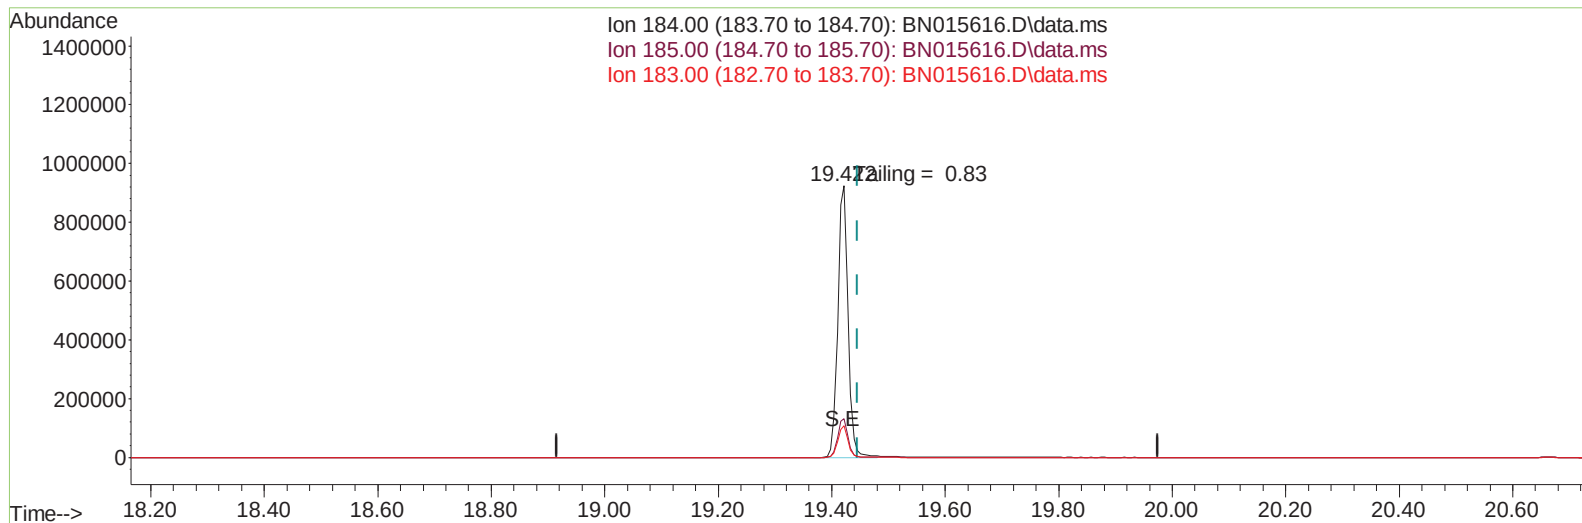

TIC: BN015616.D\data.ms

(77) Benzidine

19.422min (-0.024) 0.00 ng

response 1181408

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.39
183.00	13.20	11.75
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/20/2021	BNA_N	<u>BN015616.D</u>
Compound Name	Response	Retention Time
DDT	522605	20.66
DDD	418	20.22
DDE	392	19.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
810	523415	0.15

Instrument :
BNA_N
ClientSampleId :
DFTPP