

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080124\
 Data File : BN033136.D
 Acq On : 31 Jul 2024 18:26
 Operator : MA/JU
 Sample : P3359-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1G66

Quant Time: Jul 31 23:33:44 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 30 14:49:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.495	152	2769	0.400	ng/ul	-0.05
4) Naphthalene-d8	10.246	136	9847	0.400	ng/ul	-0.07
9) Acenaphthene-d10	14.134	164	5952	0.400	ng/ul	#-0.03
13) Phenanthrene-d10	16.996	188	734090	0.400	ng/ul	0.06
17) Chrysene-d12	21.158	240	11718	0.400	ng/ul	0.00
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.34
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.052	96	14353	4.098	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.895	152	3752	0.234	ng/ul	-0.03
18) Fluoranthene-d10	18.954	212	10920	0.329	ng/ul	-0.02
Target Compounds						
					Qvalue	
12) Fluorene	15.138	166	1094	0.051	ng/ul#	18
20) Pyrene	19.307	202	1546	0.037	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080124\
Data File : BN033136.D
Acq On : 31 Jul 2024 18:26
Operator : MA/JU
Sample : P3359-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1G66

Quant Time: Jul 31 23:33:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration




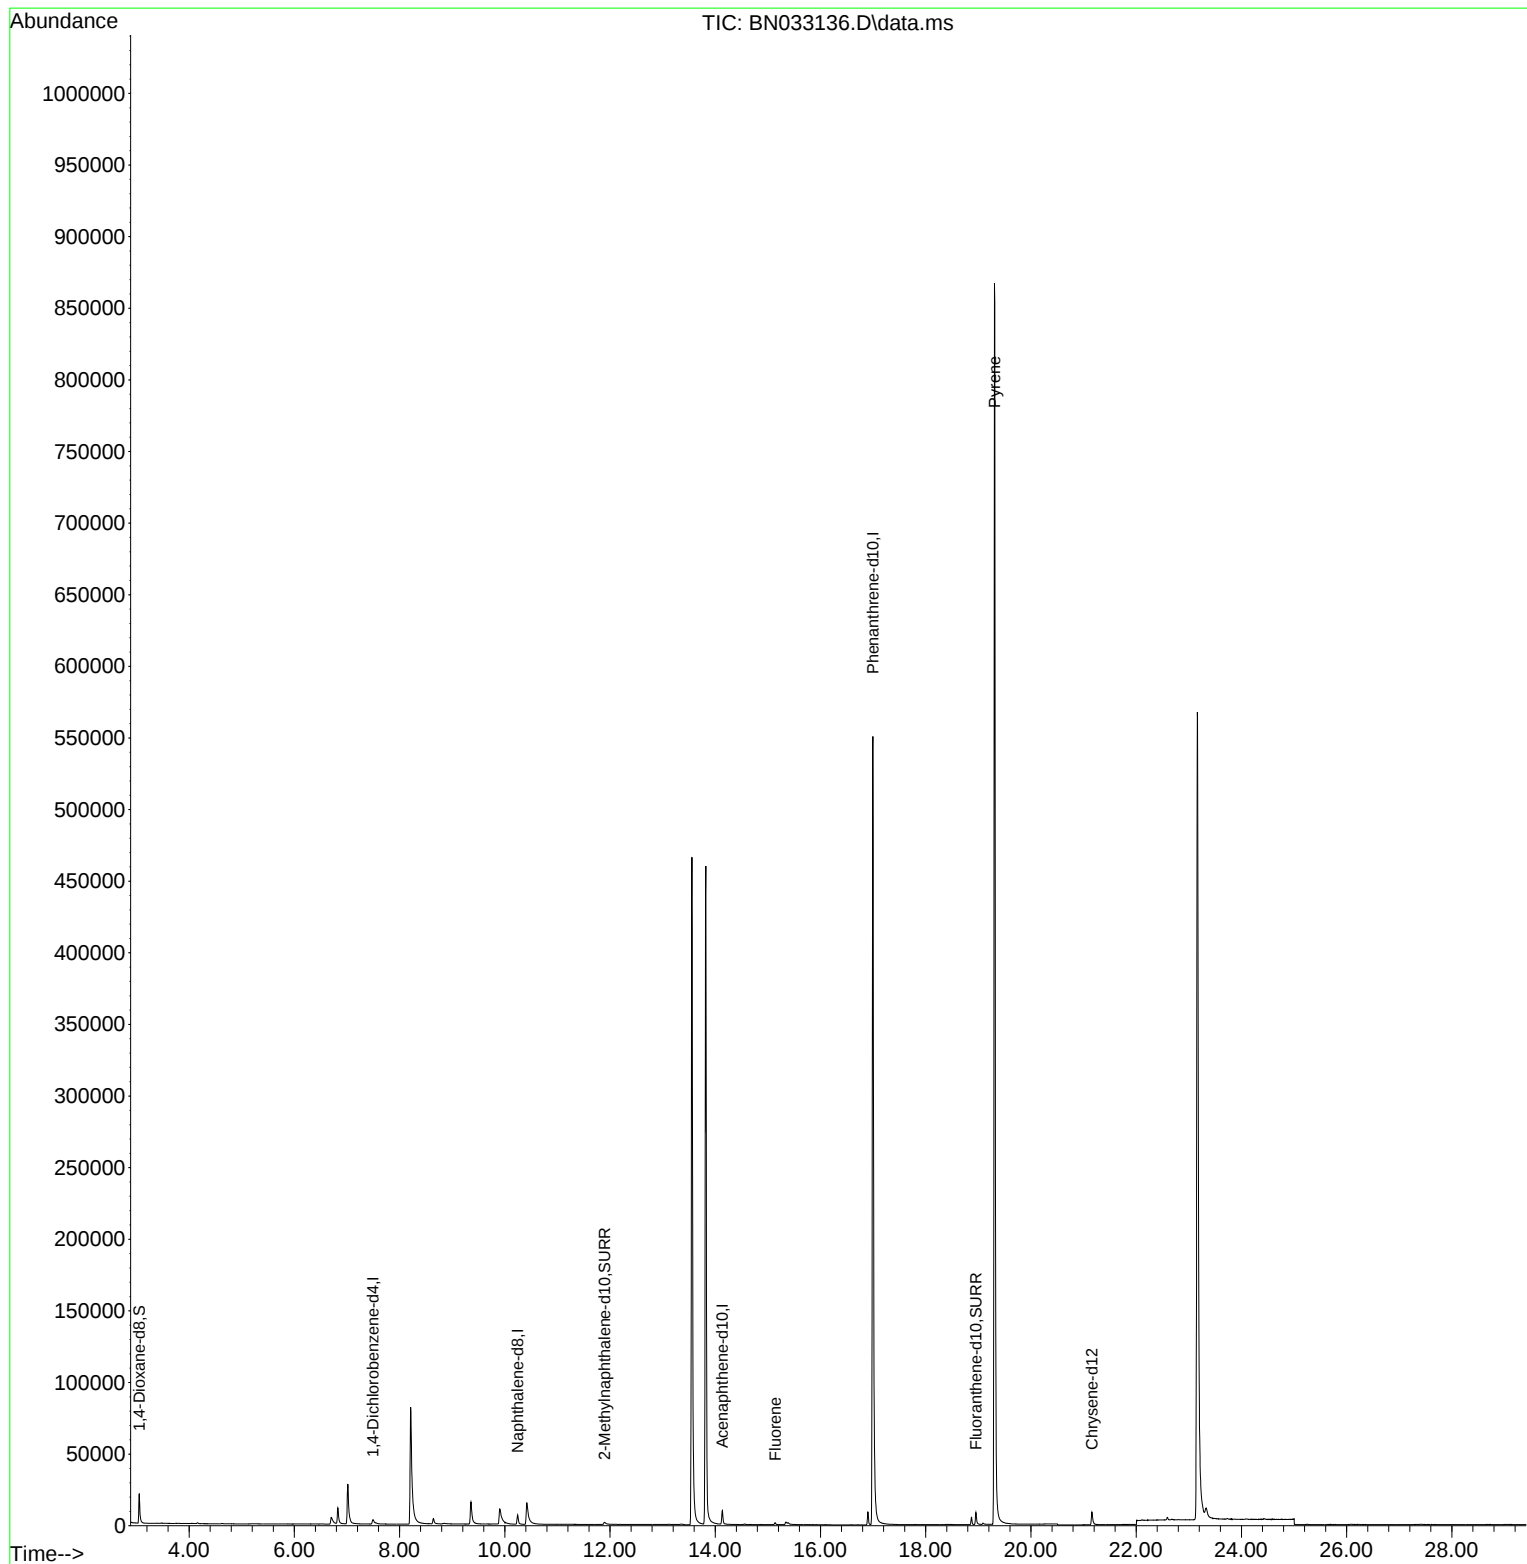


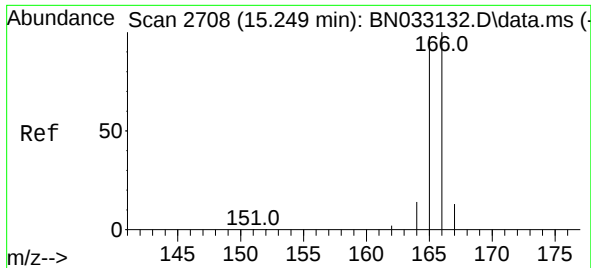

#12
Fluorene
Concen: 0.051 ng/ul
RT: 15.138 min Scan# 20
Delta R.T. -0.111 min
Lab File: BN033136.D
Acq: 31 Jul 2024 18:26

Instrument :
BNA_N
ClientSampleId :
E1G66

Tgt Ion:166 Resp: 1094
Ion Ratio Lower Upper
166 100
165 13.6 79.6 119.4#
167 38.7 12.2 18.4#

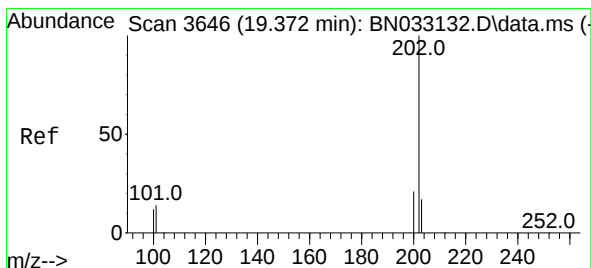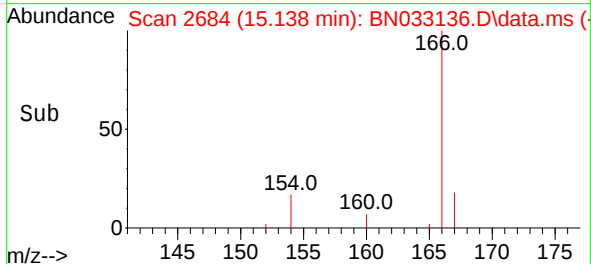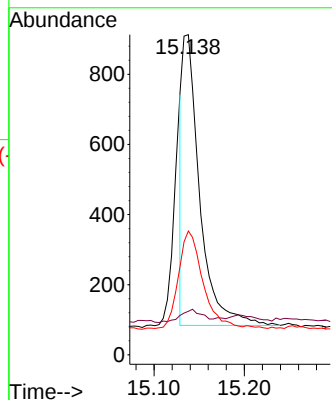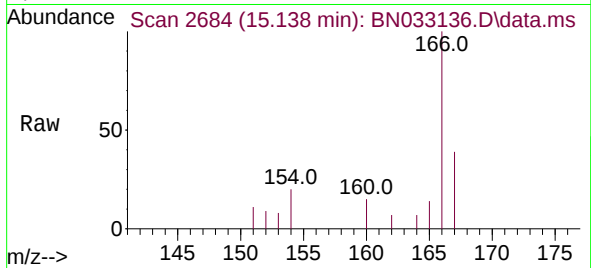

#20
Pyrene
Concen: 0.037 ng/ul
RT: 19.307 min Scan# 3632
Delta R.T. -0.064 min
Lab File: BN033136.D
Acq: 31 Jul 2024 18:26

Tgt Ion:202 Resp: 1546
Ion Ratio Lower Upper
202 100
101 179.8 12.6 18.8#
100 1335.1 9.9 14.9#

