

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080124\
 Data File : BN033137.D
 Acq On : 31 Jul 2024 19:02
 Operator : MA/JU
 Sample : P3359-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1G76

Quant Time: Jul 31 23:33:57 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 30 14:49:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.495	152	2977	0.400	ng/ul	-0.05
4) Naphthalene-d8	10.246	136	10581	0.400	ng/ul	#-0.07
9) Acenaphthene-d10	14.134	164	6312	0.400	ng/ul	#-0.03
13) Phenanthrene-d10	16.996	188	933049	0.400	ng/ul	0.06
17) Chrysene-d12	21.158	240	12138	0.400	ng/ul	0.00
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.34
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.052	96	17009	4.517	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.895	152	4304	0.249	ng/ul	-0.03
18) Fluoranthene-d10	18.954	212	11950	0.348	ng/ul	-0.02
Target Compounds						
					Qvalue	
12) Fluorene	15.133	166	1224	0.054	ng/ul#	18
20) Pyrene	19.307	202	1712	0.040	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080124\
Data File : BN033137.D
Acq On : 31 Jul 2024 19:02
Operator : MA/JU
Sample : P3359-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1G76

Quant Time: Jul 31 23:33:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration




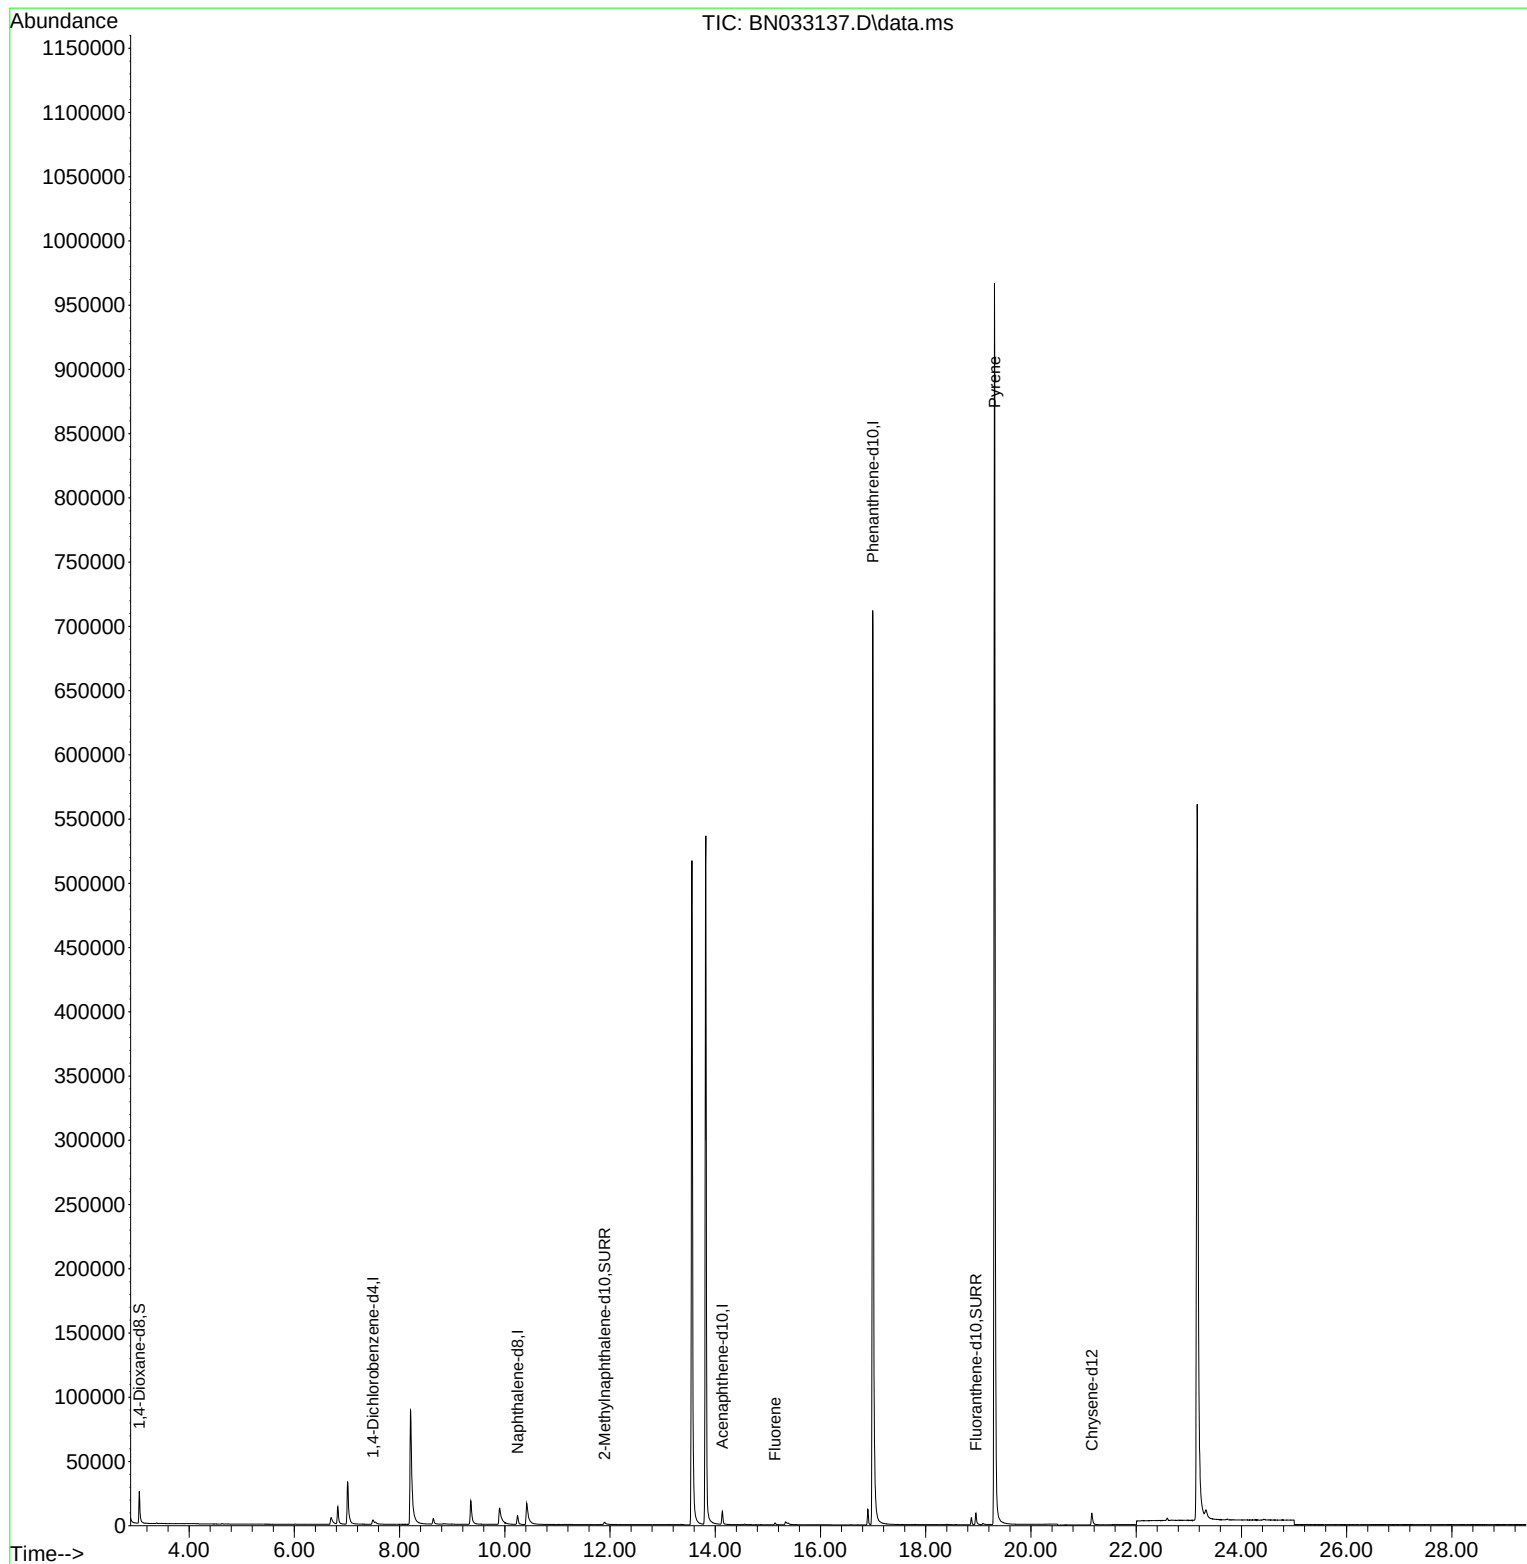


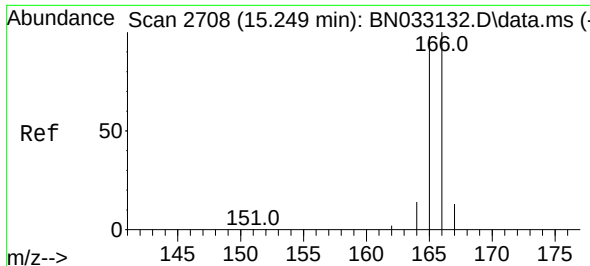

#12
Fluorene
Concen: 0.054 ng/ul
RT: 15.133 min Scan# 21
Delta R.T. -0.115 min
Lab File: BN033137.D
Acq: 31 Jul 2024 19:02

Instrument :
BNA_N
ClientSampleId :
E1G76

Tgt Ion:166 Resp: 1224
Ion Ratio Lower Upper
166 100
165 12.3 79.6 119.4#
167 34.9 12.2 18.4#

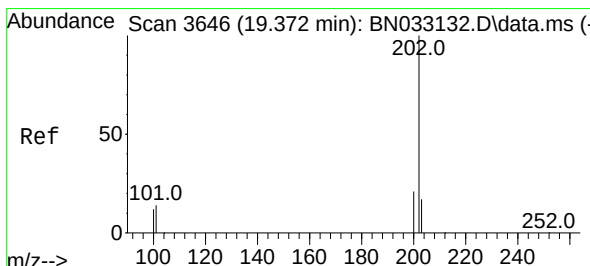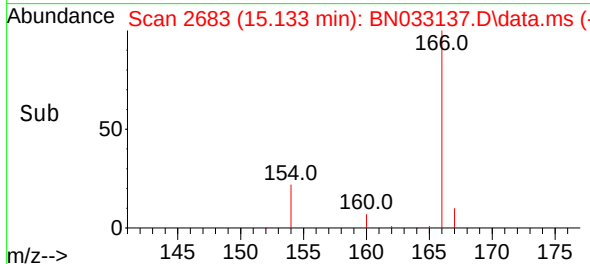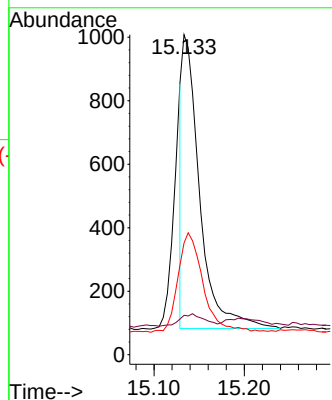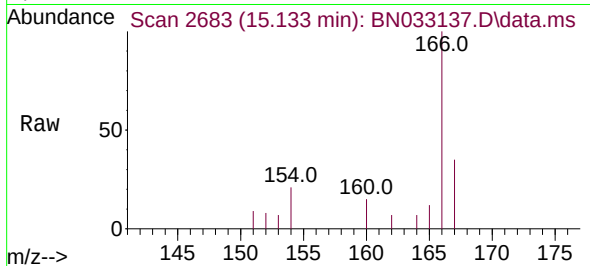

#20
Pyrene
Concen: 0.040 ng/ul
RT: 19.307 min Scan# 3632
Delta R.T. -0.064 min
Lab File: BN033137.D
Acq: 31 Jul 2024 19:02

Tgt Ion:202 Resp: 1712
Ion Ratio Lower Upper
202 100
101 176.5 12.6 18.8#
100 1292.5 9.9 14.9#

