

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080124\
Data File : BN033138.D
Acq On : 31 Jul 2024 19:38
Operator : MA/JU
Sample : P3359-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1G77

Quant Time: Jul 31 23:34:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.499	152	2271	0.400	ng/ul	-0.05
4) Naphthalene-d8	10.245	136	7979	0.400	ng/ul	-0.07
9) Acenaphthene-d10	14.134	164	4819	0.400	ng/ul	#-0.03
13) Phenanthrene-d10	16.992	188	746741	0.400	ng/ul	0.05
17) Chrysene-d12	21.154	240	10569	0.400	ng/ul	0.00
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.34
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.052	96	13375	4.656	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.901	152	3224	0.248	ng/ul	-0.03
18) Fluoranthene-d10	18.953	212	10066	0.336	ng/ul	-0.02
Target Compounds					Qvalue	
12) Fluorene	15.138	166	985	0.057	ng/ul#	20
20) Pyrene	19.307	202	1464	0.039	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080124\
Data File : BN033138.D
Acq On : 31 Jul 2024 19:38
Operator : MA/JU
Sample : P3359-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1G77

Quant Time: Jul 31 23:34:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

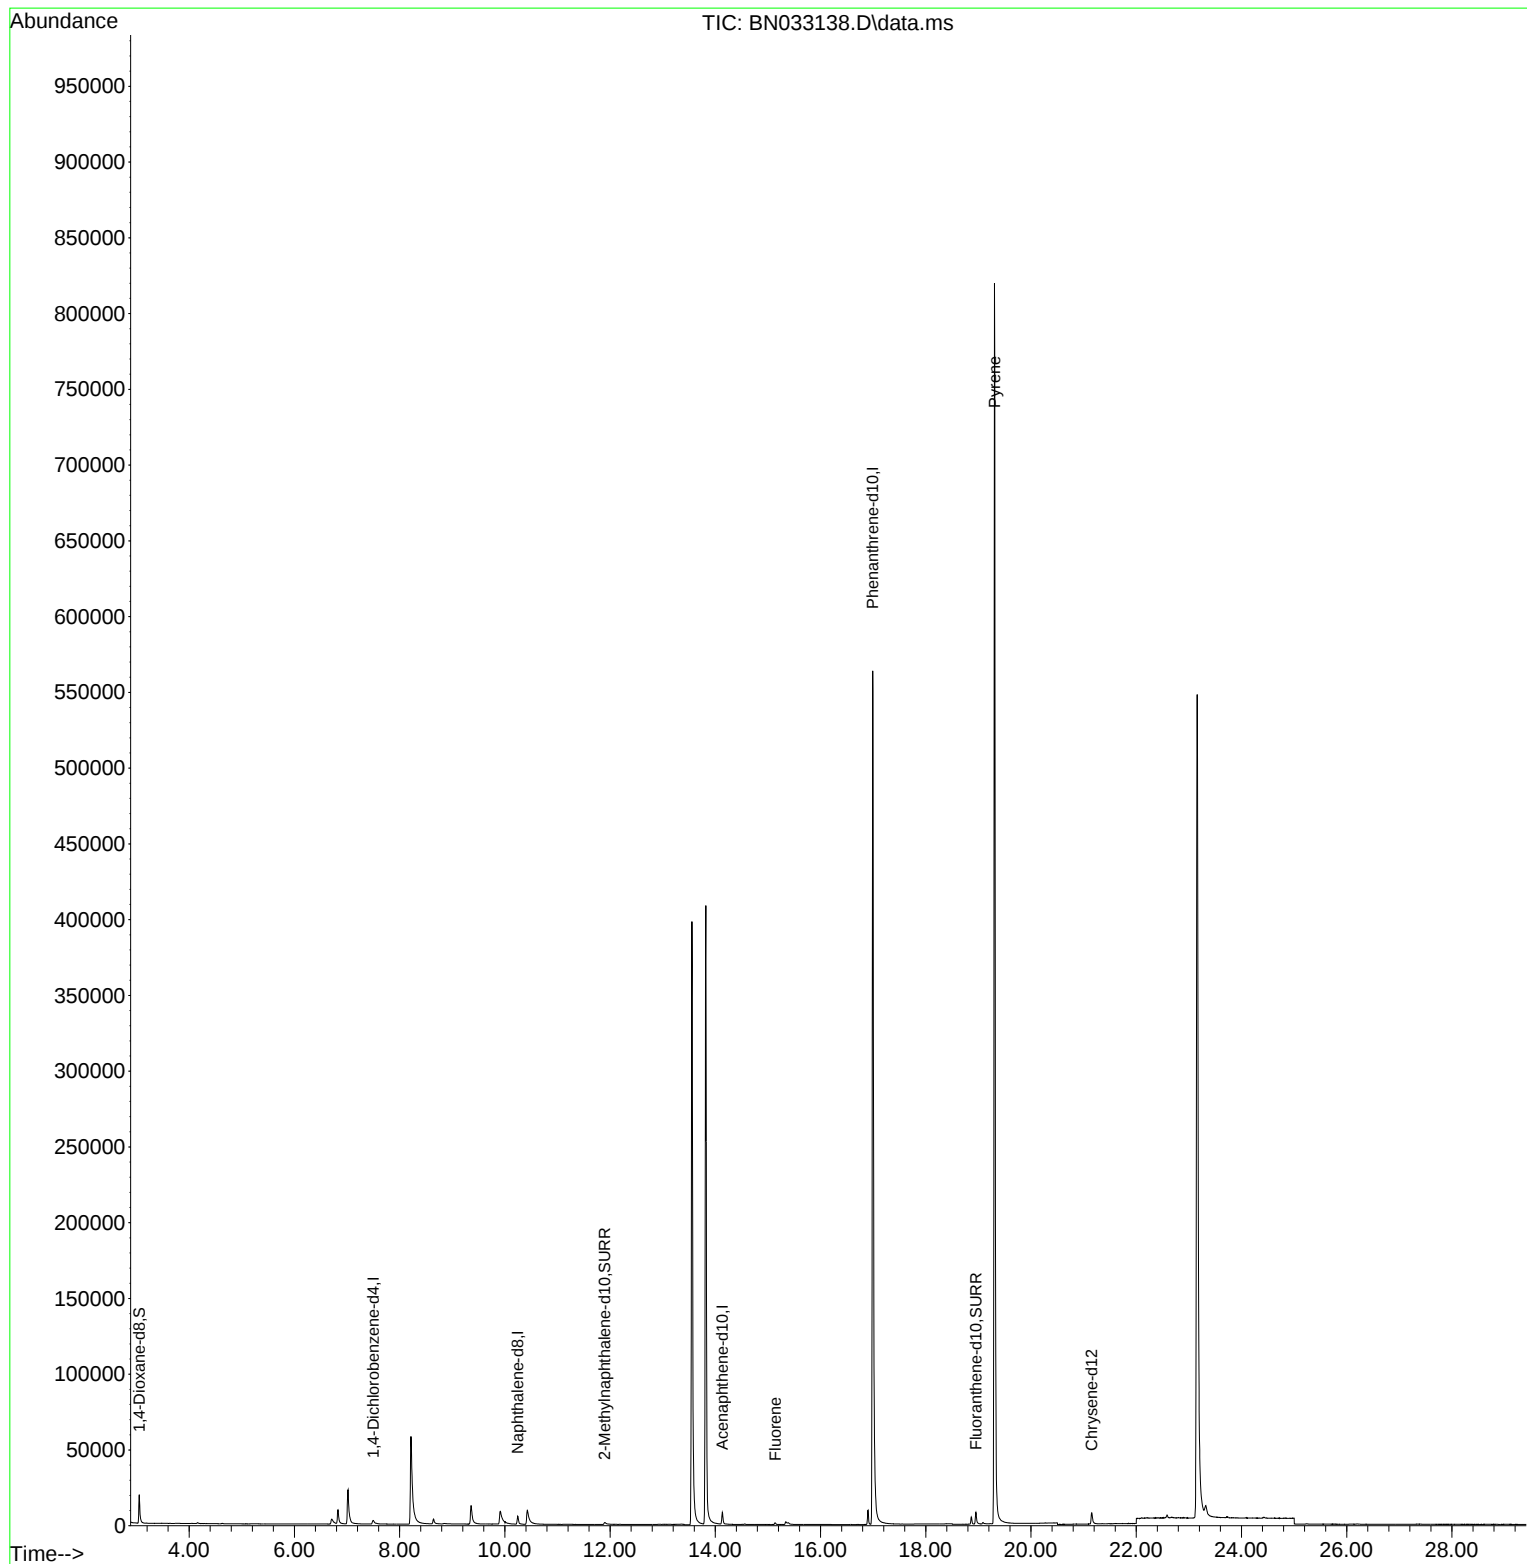

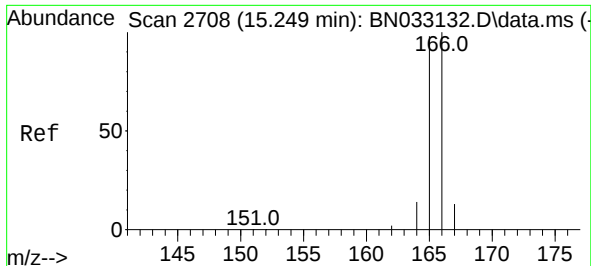

#12

Fluorene

Concen: 0.057 ng/ul

RT: 15.138 min Scan# 2

Delta R.T. -0.111 min

Lab File: BN033138.D

Acq: 31 Jul 2024 19:38

Instrument :

BNA_N

ClientSampleId :

E1G77





Tgt Ion:166 Resp: 985

Ion Ratio Lower Upper

166 100

165 16.2 79.6 119.4#

167 39.3 12.2 18.4#

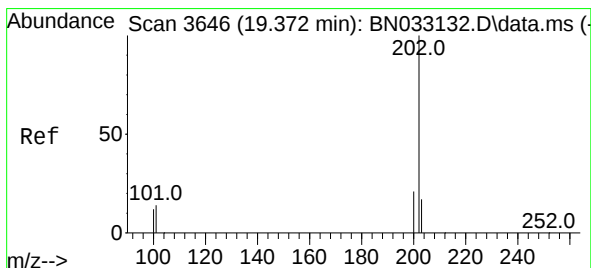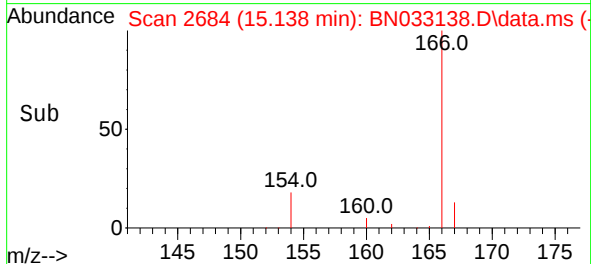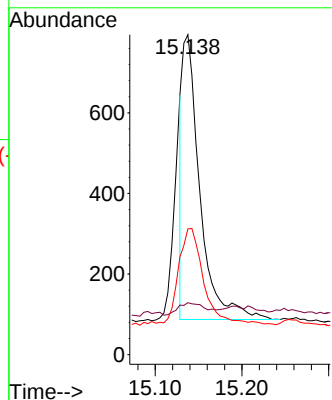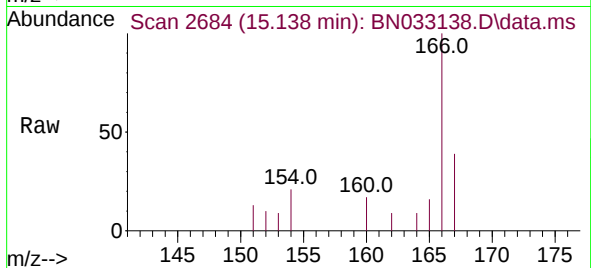

#20

Pyrene

Concen: 0.039 ng/ul

RT: 19.307 min Scan# 3632

Delta R.T. -0.065 min

Lab File: BN033138.D

Acq: 31 Jul 2024 19:38

Tgt Ion:202 Resp: 1464

Ion Ratio Lower Upper

202 100

101 173.8 12.6 18.8#

100 1262.5 9.9 14.9#

