

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080124\
 Data File : BN033142.D
 Acq On : 31 Jul 2024 22:03
 Operator : MA/JU
 Sample : P3359-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1G98

Quant Time: Jul 31 23:34:52 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 30 14:49:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.495	152	2702	0.400	ng/ul	-0.05
4) Naphthalene-d8	10.246	136	9735	0.400	ng/ul	#-0.07
9) Acenaphthene-d10	14.134	164	5915	0.400	ng/ul	#-0.03
13) Phenanthrene-d10	16.996	188	780281	0.400	ng/ul	0.06
17) Chrysene-d12	21.157	240	11840	0.400	ng/ul	0.00
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.34
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.052	96	13156	3.849	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.895	152	3272	0.206	ng/ul	-0.03
18) Fluoranthene-d10	18.954	212	10167	0.303	ng/ul	-0.02
Target Compounds						Qvalue
5) Naphthalene	10.295	128	569	0.023	ng/ul#	63
12) Fluorene	15.133	166	1041	0.049	ng/ul#	19
20) Pyrene	19.307	202	1499	0.036	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080124\
Data File : BN033142.D
Acq On : 31 Jul 2024 22:03
Operator : MA/JU
Sample : P3359-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1G98


Quant Time: Jul 31 23:34:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

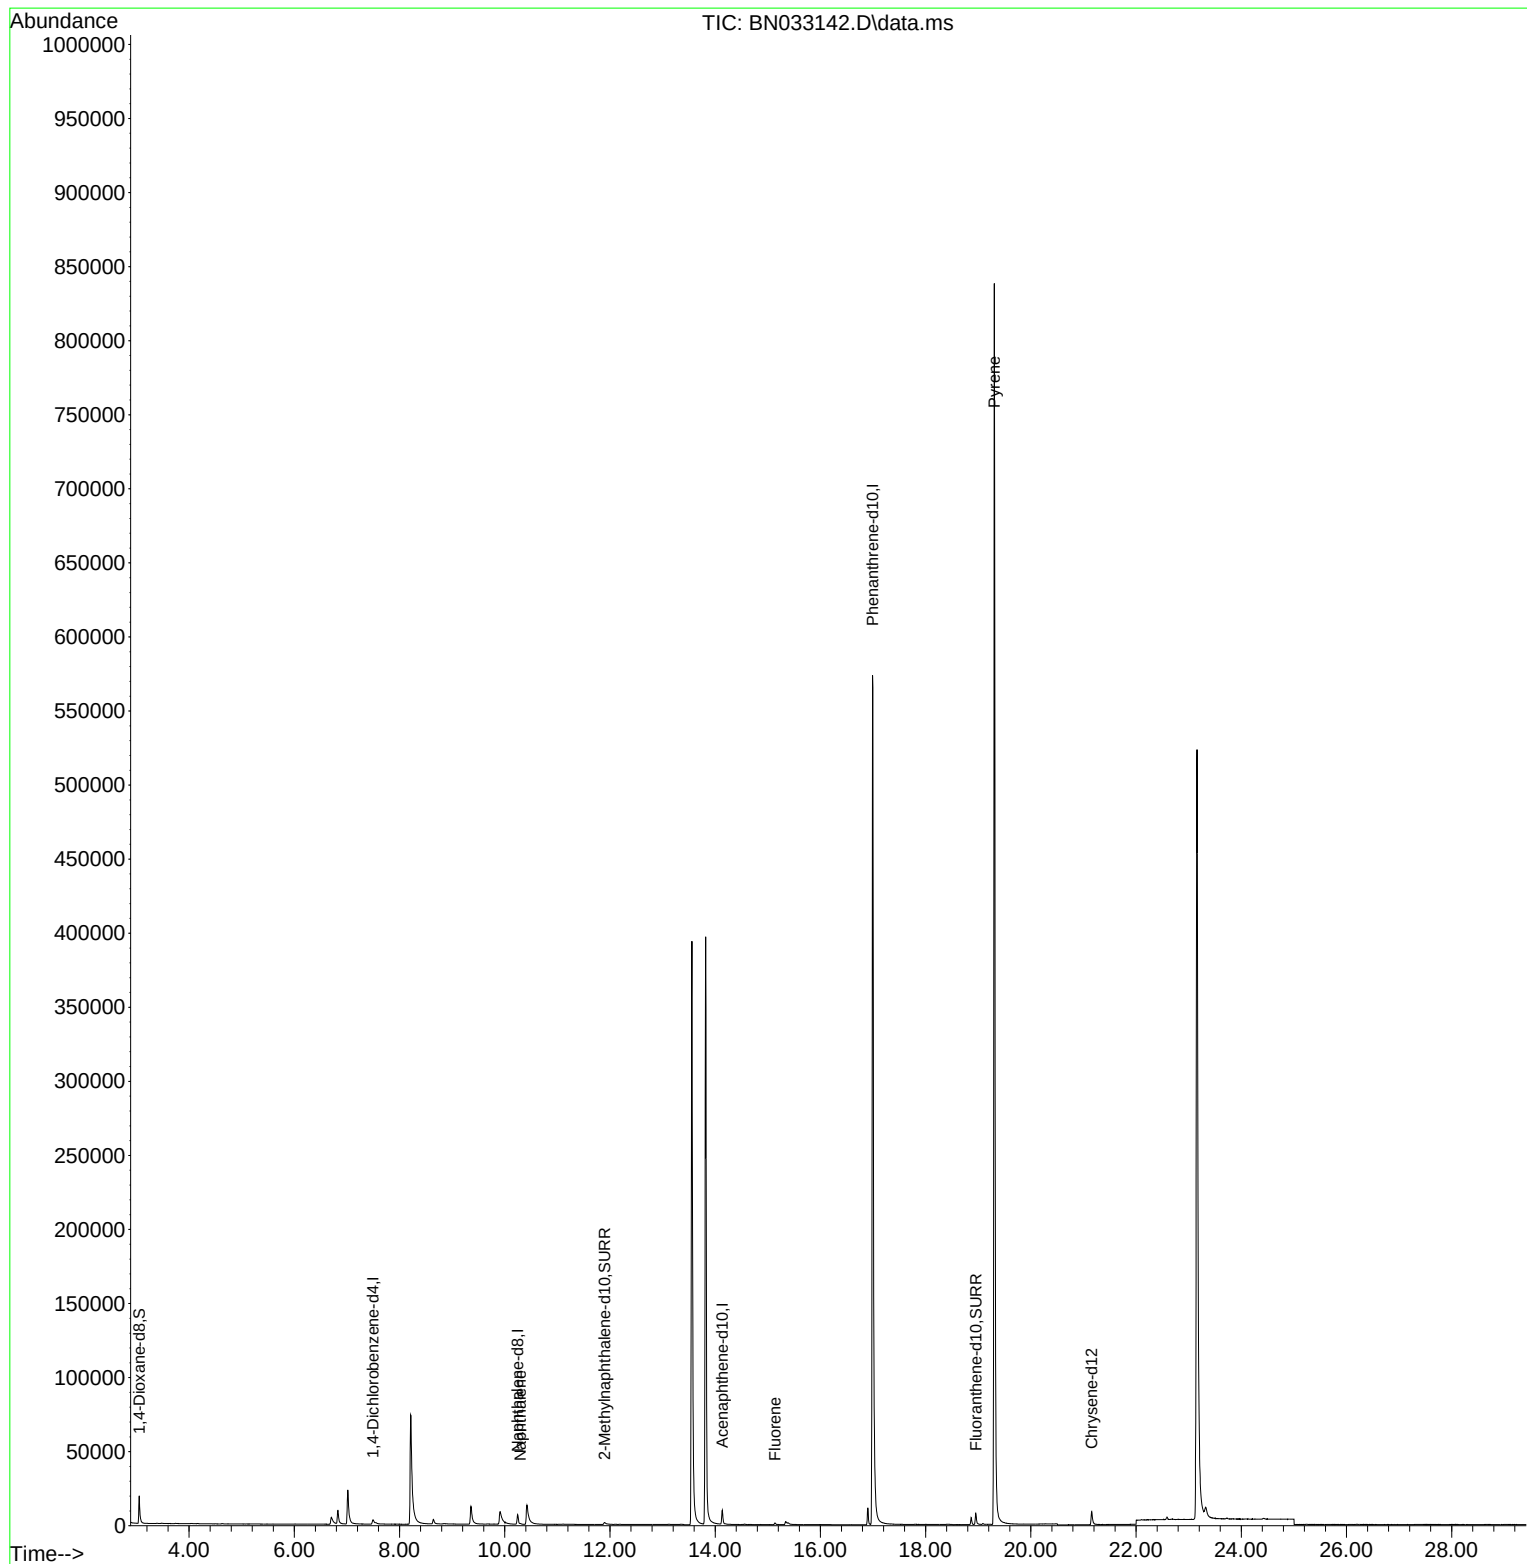



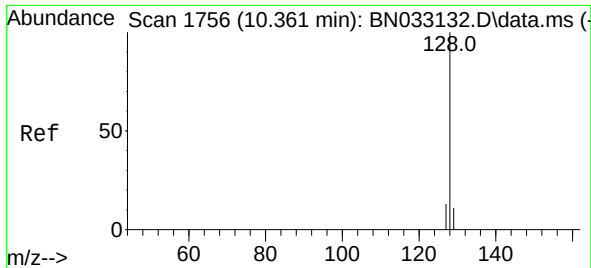


#5
Naphthalene
Concen: 0.023 ng/ul
RT: 10.295 min Scan# 1744
Delta R.T. -0.082 min
Lab File: BN033142.D
Acq: 31 Jul 2024 22:03

Instrument :
BNA_N
ClientSampleId :
E1G98



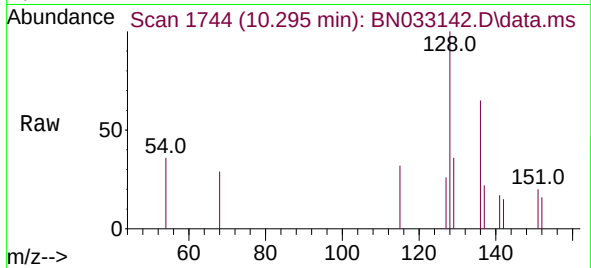



Tgt Ion:128 Resp: 569
Ion Ratio Lower Upper
128 100
129 36.4 12.0 18.0#
127 25.9 12.7 19.1#

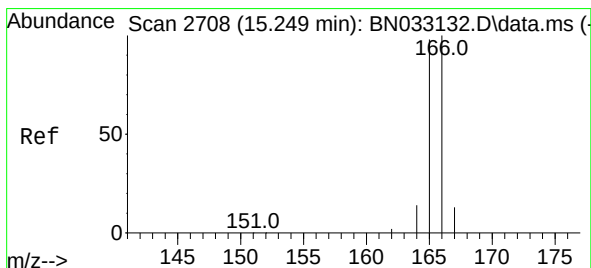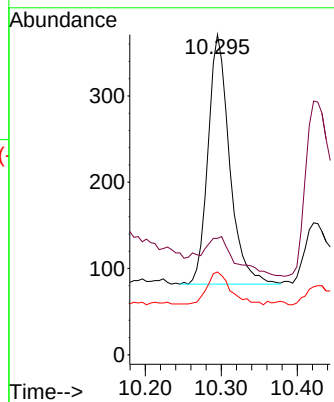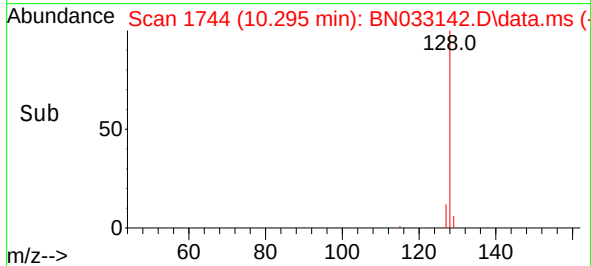

#12
Fluorene
Concen: 0.049 ng/ul
RT: 15.133 min Scan# 2683
Delta R.T. -0.115 min
Lab File: BN033142.D
Acq: 31 Jul 2024 22:03

Tgt Ion:166 Resp: 1041
Ion Ratio Lower Upper
166 100
165 13.6 79.6 119.4#
167 35.4 12.2 18.4#

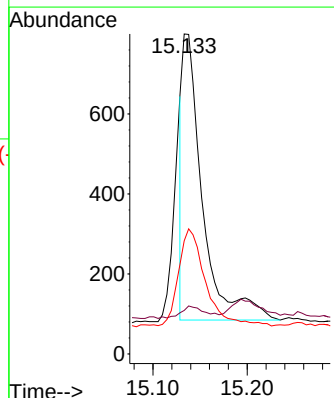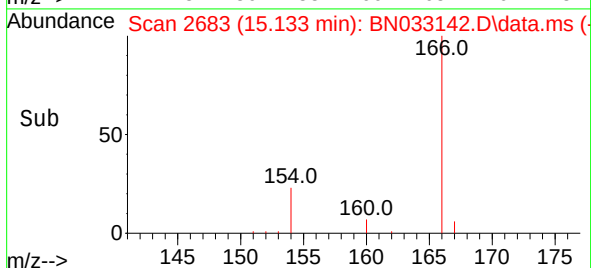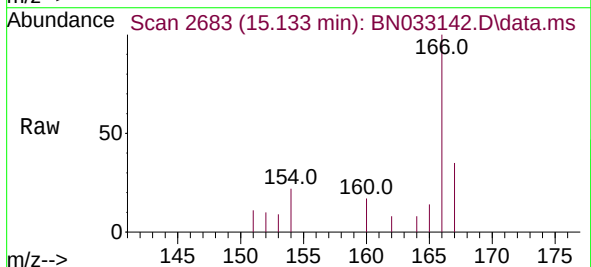

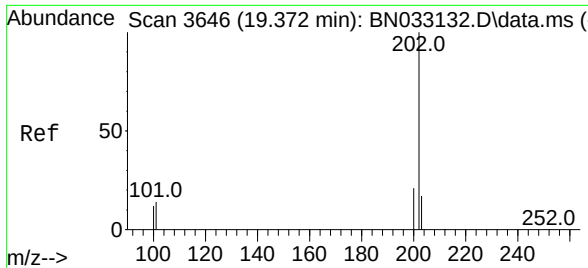

#20
 Pyrene
 Concen: 0.036 ng/ul
 RT: 19.307 min Scan# 30
 Delta R.T. -0.065 min
 Lab File: BN033142.D
 Acq: 31 Jul 2024 22:03

Instrument :
 BNA_N
 ClientSampleId :
 E1G98

Tgt Ion:202 Resp: 1499
 Ion Ratio Lower Upper
 202 100
 101 172.9 12.6 18.8#
 100 1235.2 9.9 14.9#

