

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080124\
 Data File : BN033143.D
 Acq On : 31 Jul 2024 22:39
 Operator : MA/JU
 Sample : P3359-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1G99

Quant Time: Jul 31 23:35:02 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 30 14:49:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.495	152	3067	0.400	ng/ul	-0.05
4) Naphthalene-d8	10.240	136	10731	0.400	ng/ul	-0.08
9) Acenaphthene-d10	14.134	164	6524	0.400	ng/ul	#-0.03
13) Phenanthrene-d10	16.992	188	975910	0.400	ng/ul	0.05
17) Chrysene-d12	21.148	240	12683	0.400	ng/ul	0.00
23) Perylene-d12	23.320	264	17922	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.052	96	15259	3.933	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.884	152	4070	0.232	ng/ul	-0.04
18) Fluoranthene-d10	18.949	212	12643	0.352	ng/ul	-0.02
Target Compounds						Qvalue
20) Pyrene	19.307	202	1863	0.042	ng/ul#	1
26) Benzo(a)pyrene	23.153	252	3085	0.063	ng/ul#	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080124\
Data File : BN033143.D
Acq On : 31 Jul 2024 22:39
Operator : MA/JU
Sample : P3359-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1G99

Quant Time: Jul 31 23:35:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

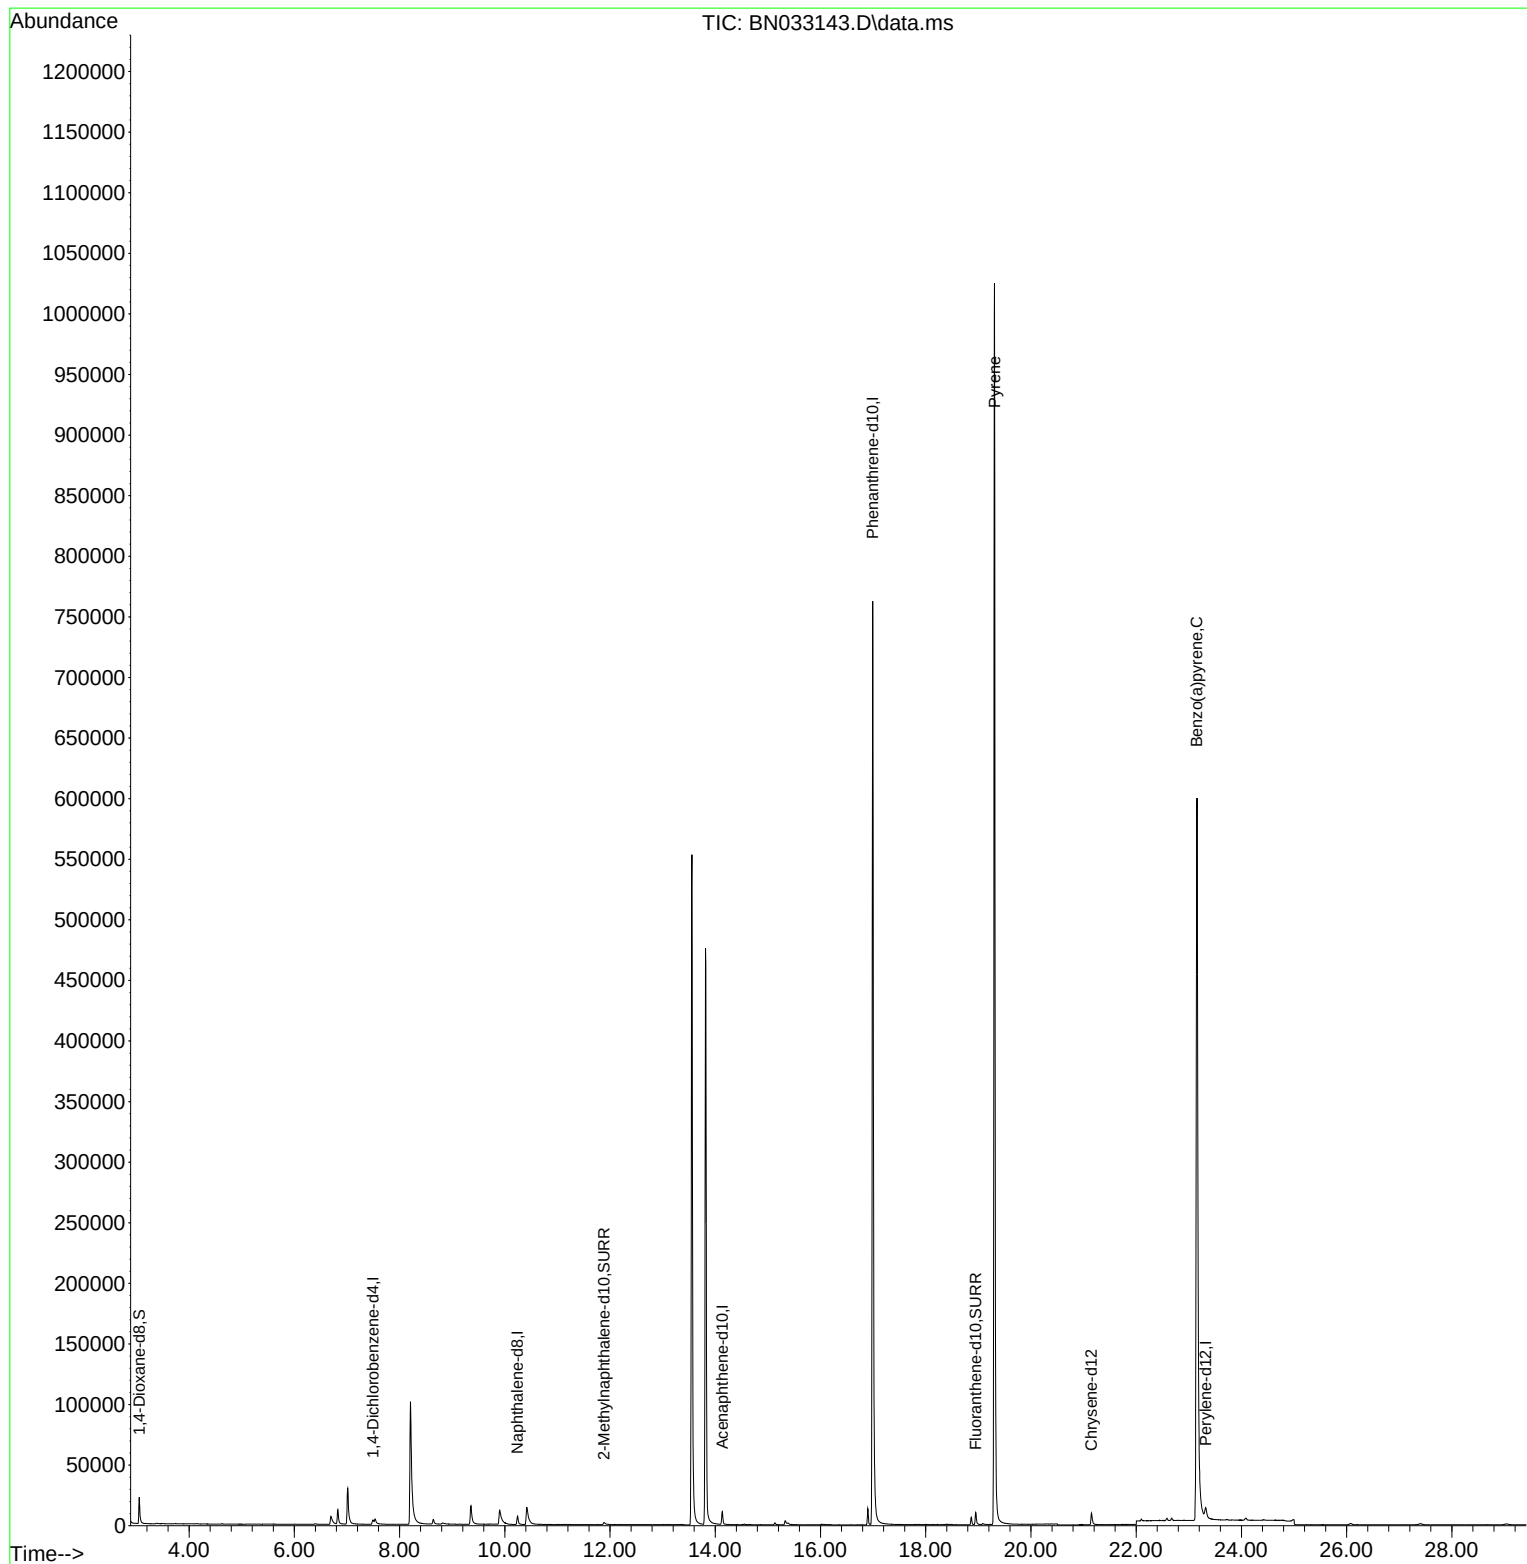

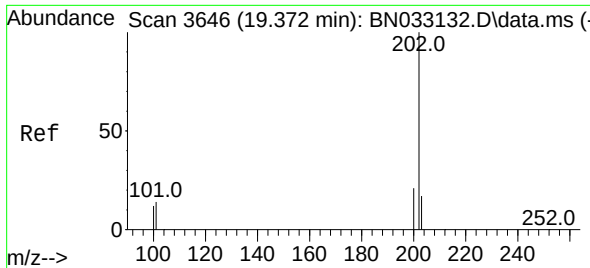

#20

Pyrene

Concen: 0.042 ng/ul

RT: 19.307 min Scan# 3

Delta R.T. -0.065 min

Lab File: BN033143.D

Acq: 31 Jul 2024 22:39

Instrument :

BNA_N

ClientSampleId :

E1G99





Tgt Ion:202 Resp: 1863

Ion Ratio Lower Upper

202 100

101 171.7 12.6 18.8#

100 1226.7 9.9 14.9#

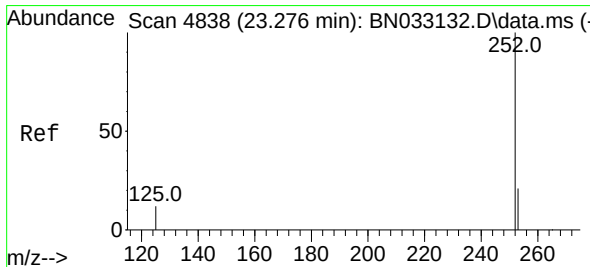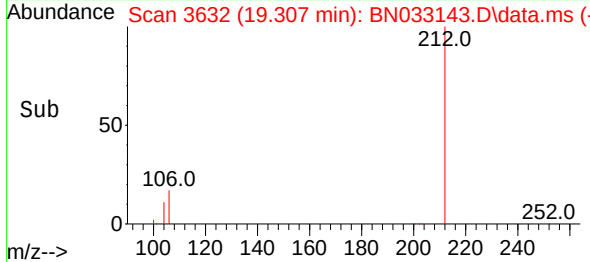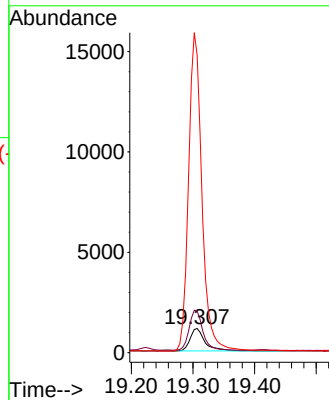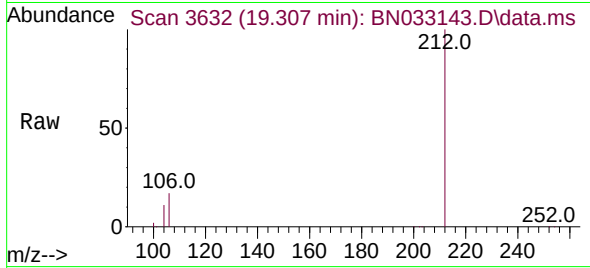

#26

Benzo(a)pyrene

Concen: 0.063 ng/ul

RT: 23.153 min Scan# 4796

Delta R.T. -0.096 min

Lab File: BN033143.D

Acq: 31 Jul 2024 22:39

Tgt Ion:252 Resp: 3085

Ion Ratio Lower Upper

252 100

253 54.1 27.5 41.3#

125 57.0 27.0 40.6#

