




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080124\
Data File : BN033160.D
Acq On : 01 Aug 2024 09:31
Operator : MA/JU
Sample : P3378-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B10

Manual IntegrationsAPPROVED

Quant Time: Aug 01 10:54:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/01/2024
Supervised By :mohammad ahmed 08/13/2024

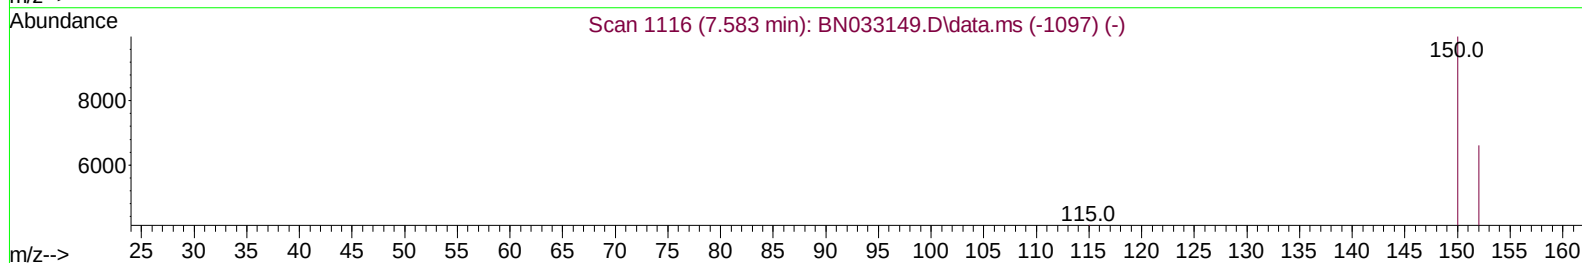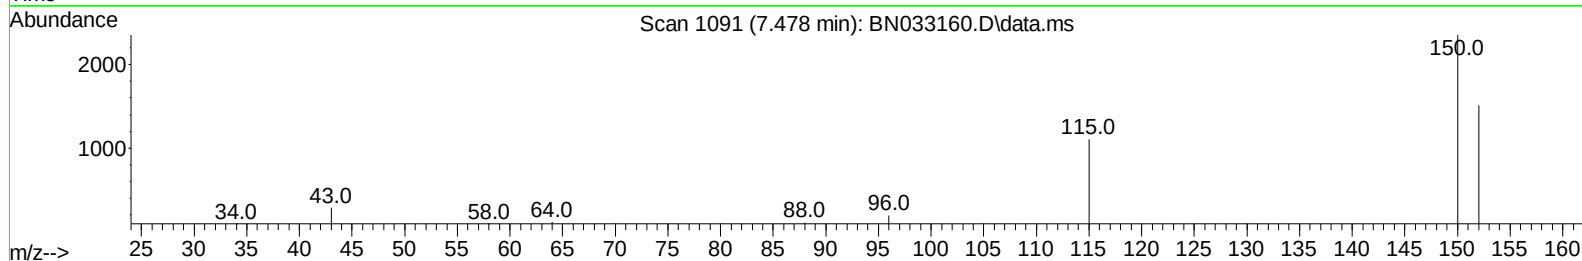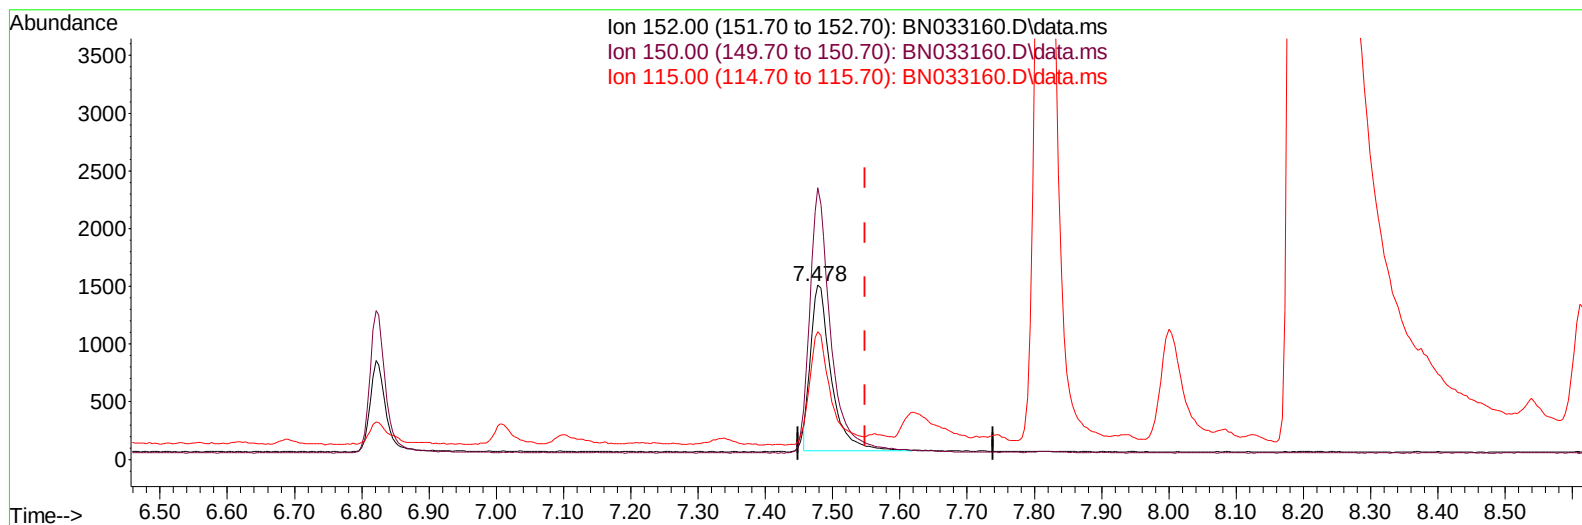

TIC: BN033160.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.478min (-0.071) 0.40 ng/ul

response 3034

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	143.10	155.76
115.00	84.50	73.38
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080124\
Data File : BN033160.D
Acq On : 01 Aug 2024 09:31
Operator : MA/JU
Sample : P3378-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B10

Manual IntegrationsAPPROVED

Quant Time: Aug 01 10:54:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/01/2024
Supervised By :mohammad ahmed 08/13/2024

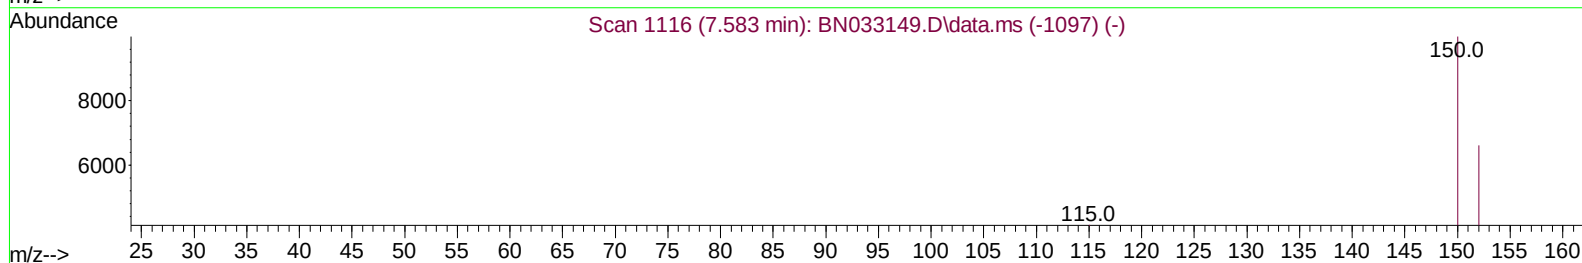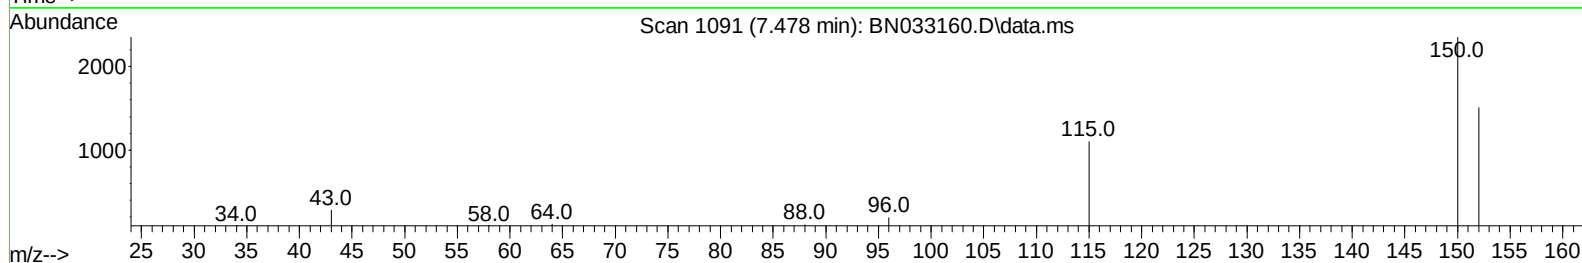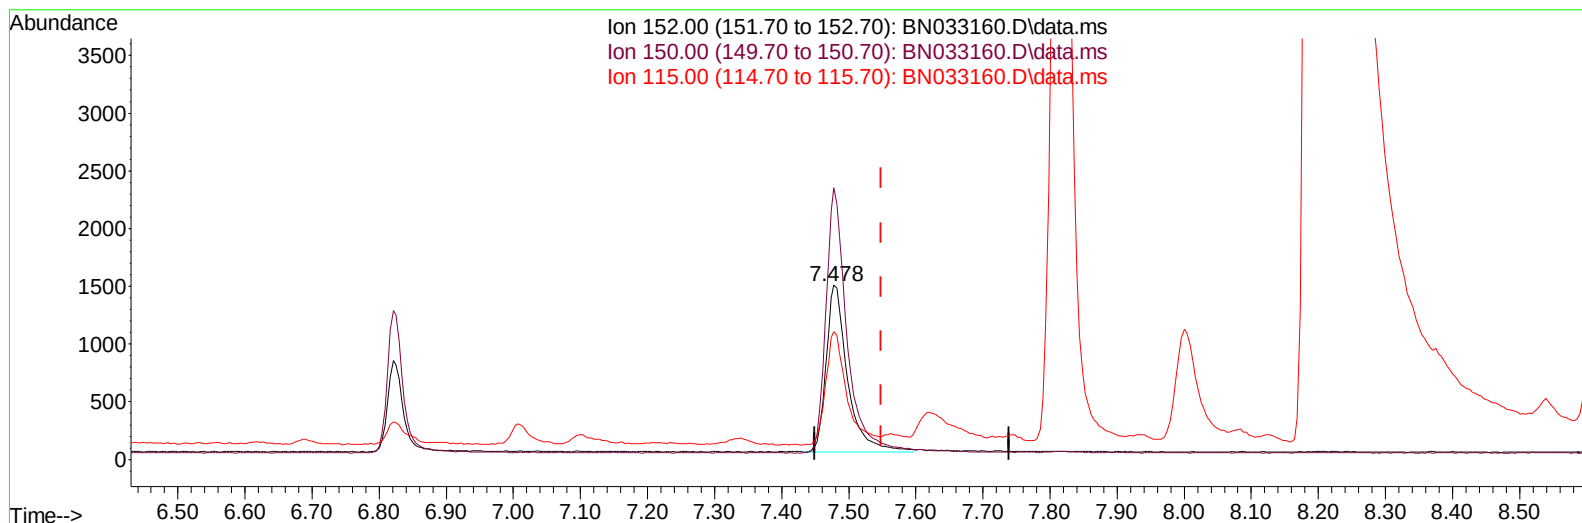

TIC: BN033160.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.478min (-0.071) 0.40 ng/ul m

response 3248

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	143.10	155.76
115.00	84.50	73.38
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080124\
Data File : BN033160.D
Acq On : 01 Aug 2024 09:31
Operator : MA/JU
Sample : P3378-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B10

Manual IntegrationsAPPROVED

Quant Time: Aug 01 10:54:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/01/2024
Supervised By :mohammad ahmed 08/13/2024

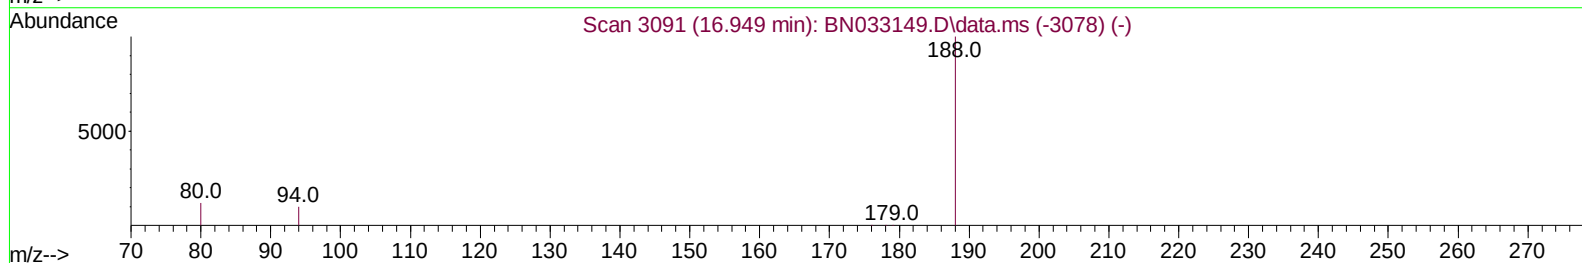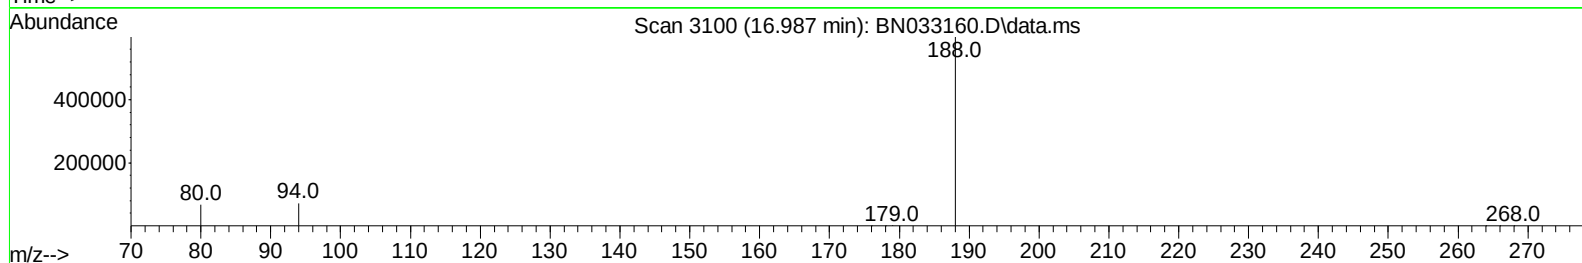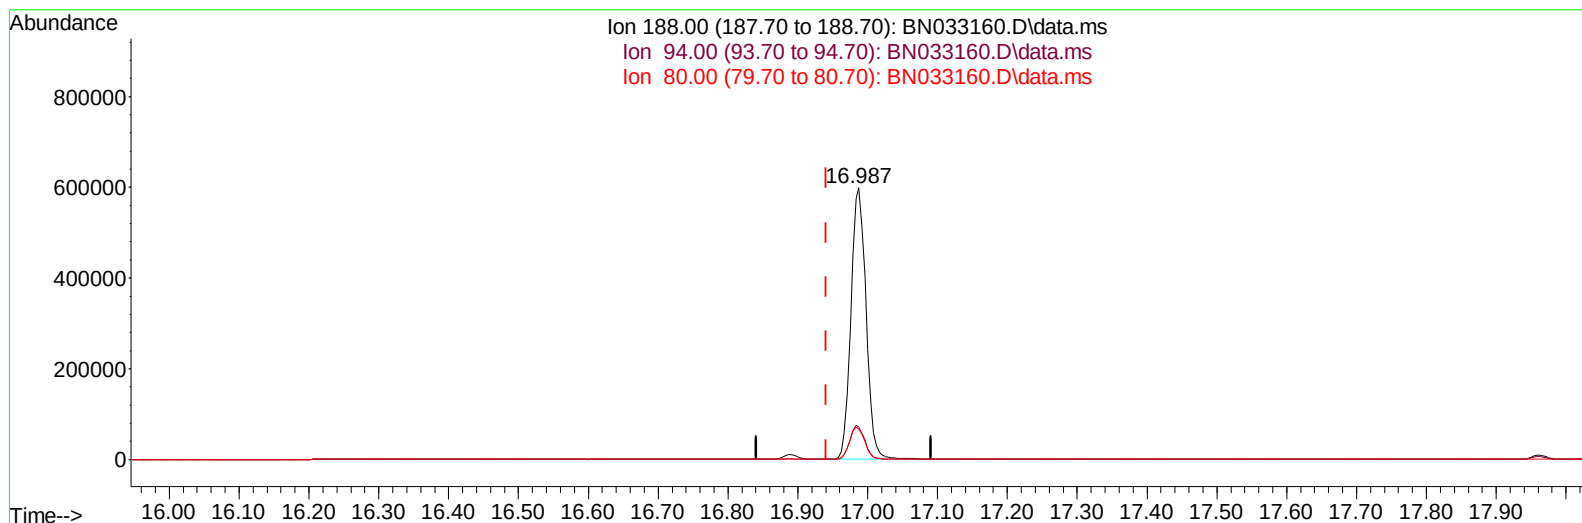

TIC: BN033160.D\data.ms

(13) Phenanthrene-d10 (I)

16.987min (+ 0.047) 0.40 ng/u1

response 893983

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.40	11.91
80.00	13.10	11.17
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080124\
Data File : BN033160.D
Acq On : 01 Aug 2024 09:31
Operator : MA/JU
Sample : P3378-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B10

Manual IntegrationsAPPROVED

Quant Time: Aug 01 10:54:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/01/2024
Supervised By :mohammad ahmed 08/13/2024

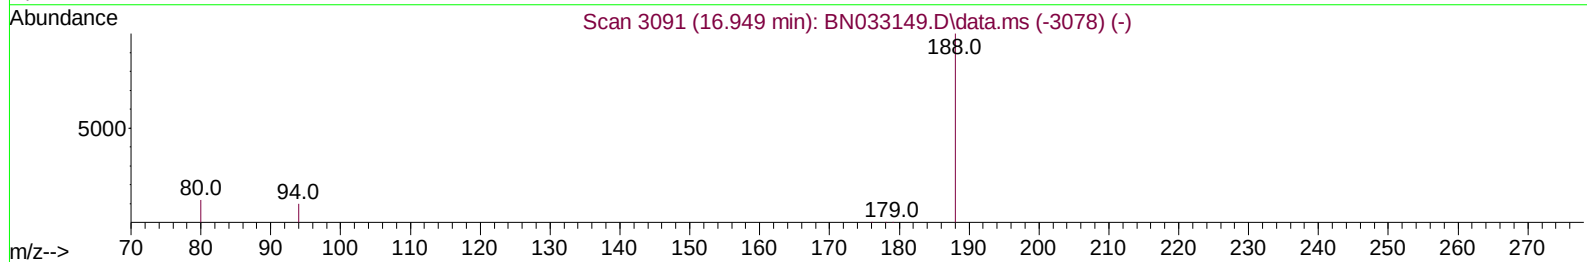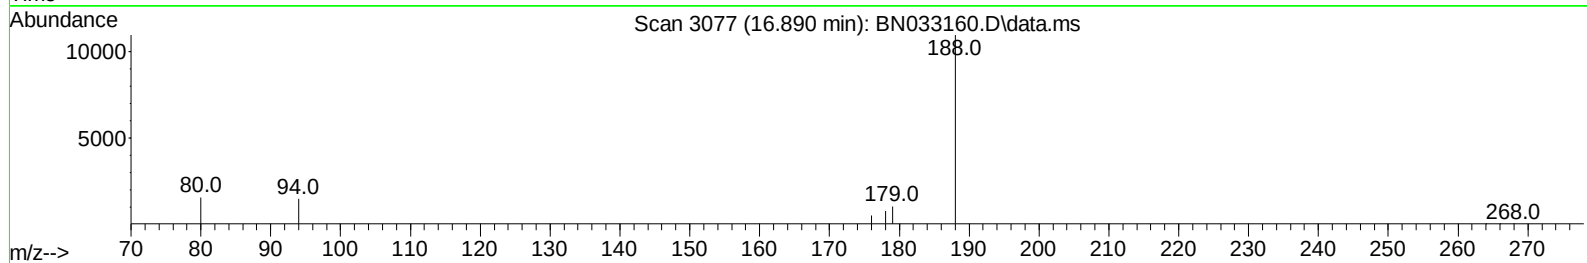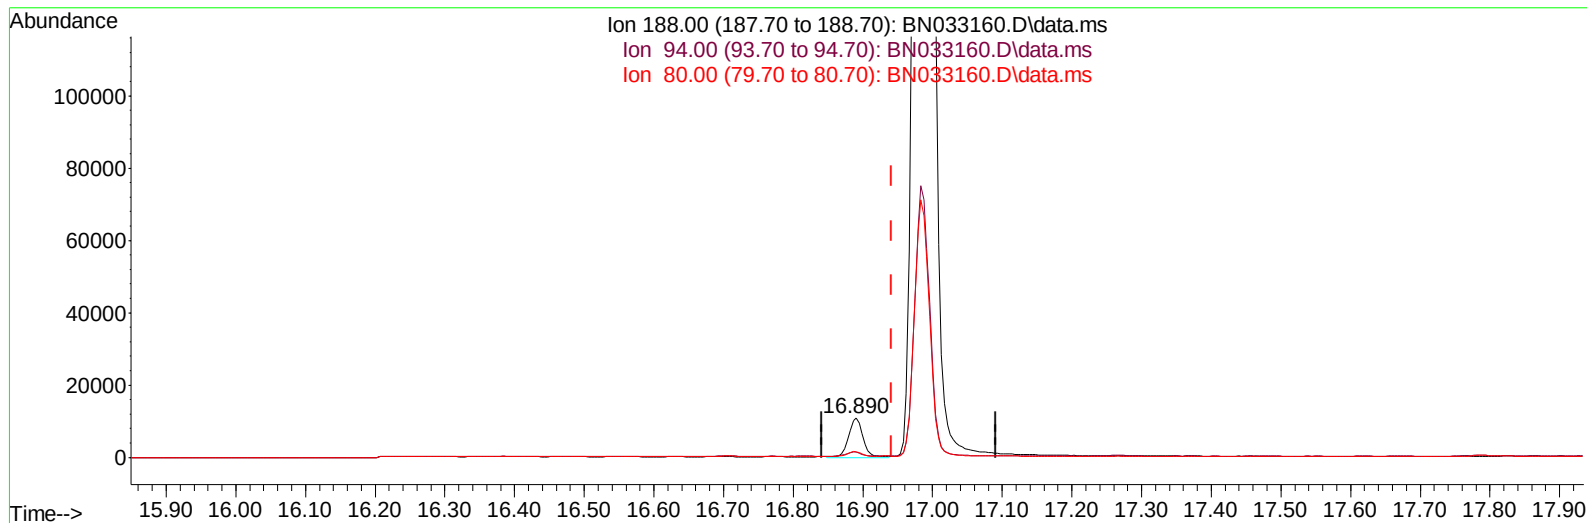

TIC: BN033160.D\data.ms

(13) Phenanthrene-d10 (I)

16.890min (-0.051) 0.40 ng/ul m

response 15903

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.40	13.61
80.00	13.10	14.40
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080124\
Data File : BN033160.D
Acq On : 01 Aug 2024 09:31
Operator : MA/JU
Sample : P3378-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B10

Manual IntegrationsAPPROVED

Quant Time: Aug 01 10:54:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/01/2024
Supervised By :mohammad ahmed 08/13/2024

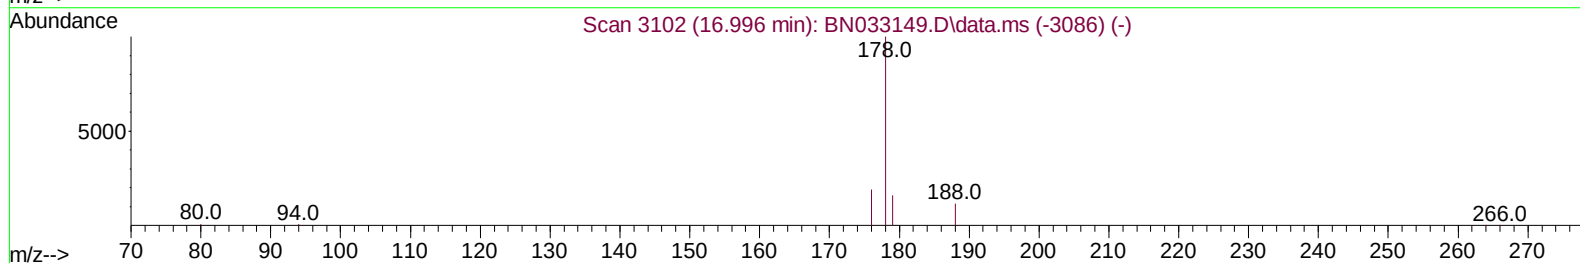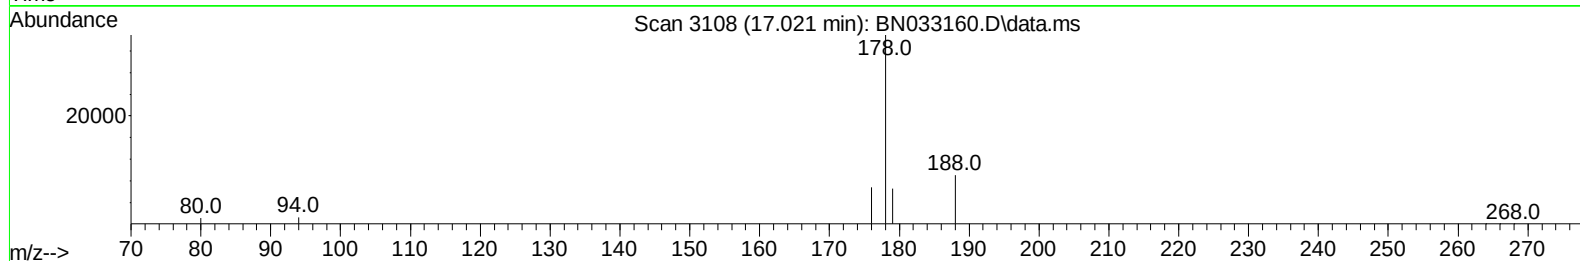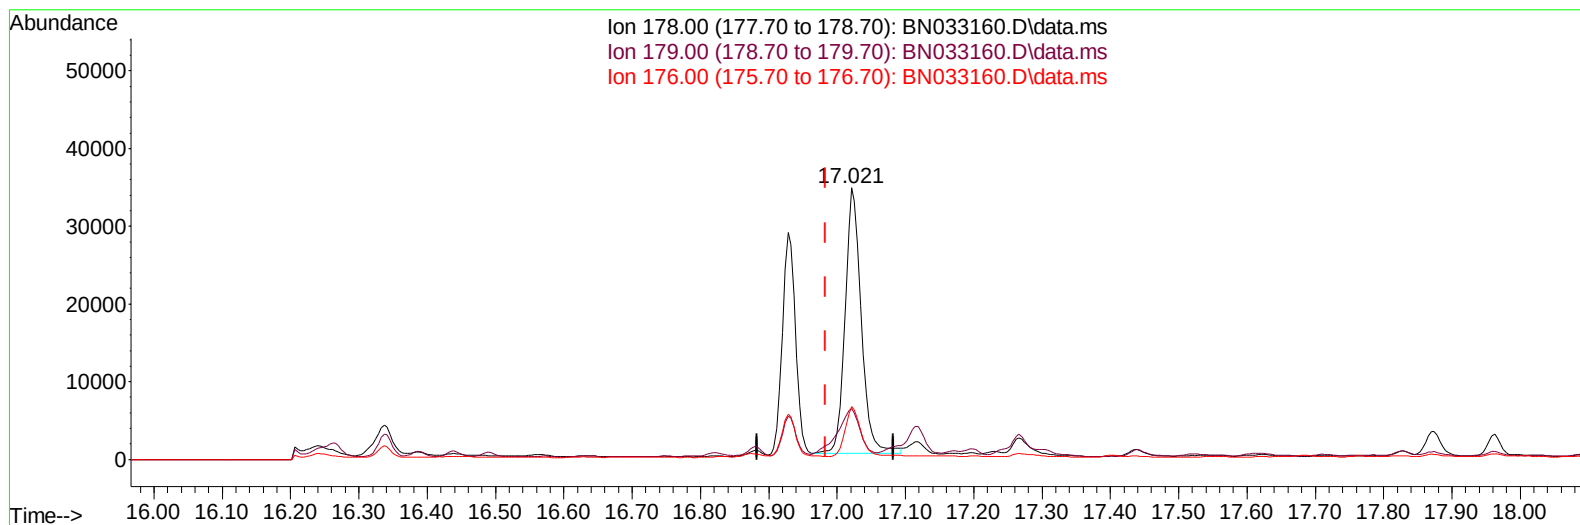

TIC: BN033160.D\data.ms

(15) Phenanthrene

17.021min (+ 0.038) 1.31 ng/ul

response 56016

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	17.10	18.69
176.00	19.90	19.37
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080124\
 Data File : BN033160.D
 Acq On : 01 Aug 2024 09:31
 Operator : MA/JU
 Sample : P3378-08
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0B10

Manual IntegrationsAPPROVED

Quant Time: Aug 01 10:54:42 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 30 14:49:49 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/01/2024
 Supervised By :mohammad ahmed 08/13/2024

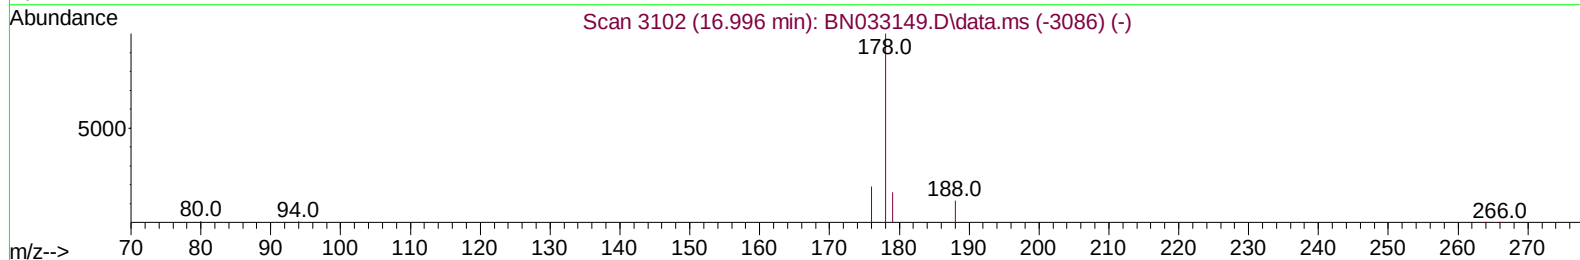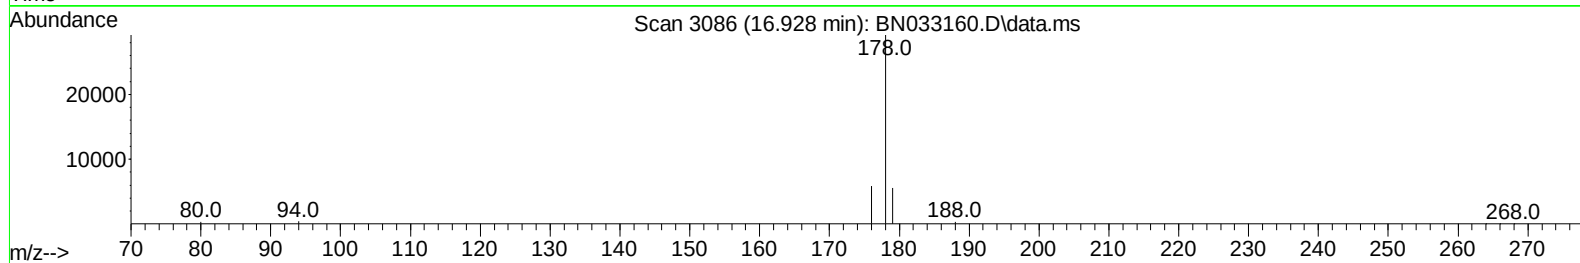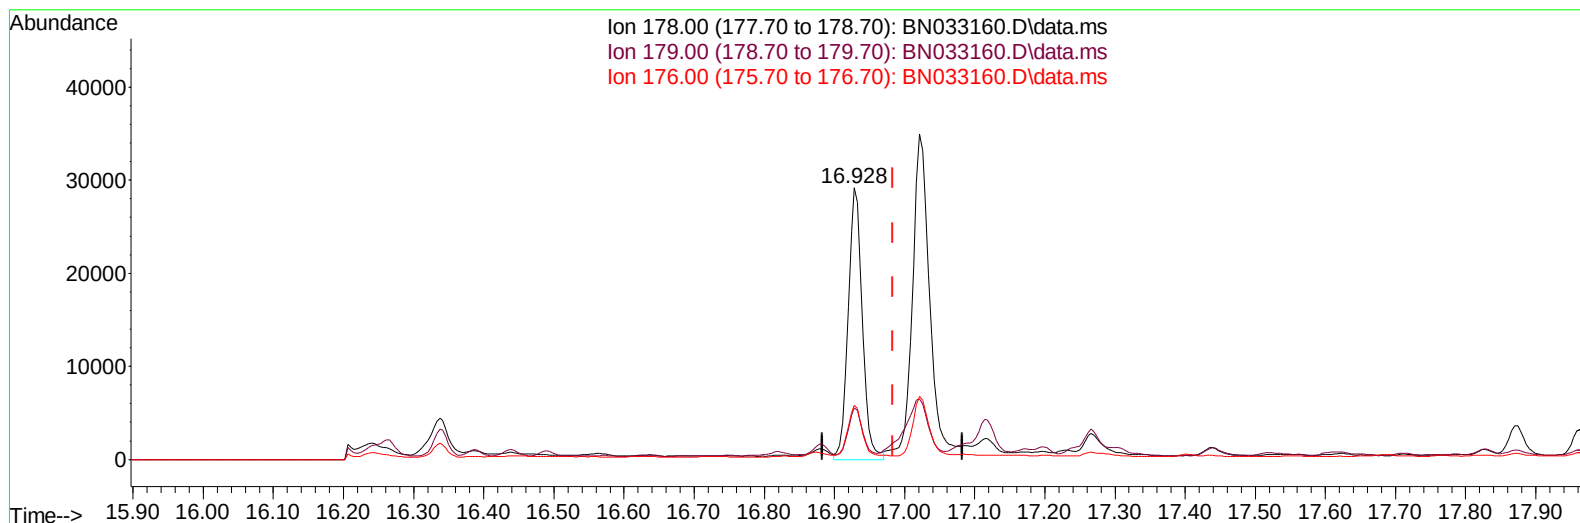

TIC: BN033160.D\data.ms

(15) Phenanthrene

16.928min (-0.055) 0.96 ng/ul m

response 41022

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	17.10	18.98
176.00	19.90	20.03
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080124\
 Data File : BN033160.D
 Acq On : 01 Aug 2024 09:31
 Operator : MA/JU
 Sample : P3378-08
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0B10

Manual IntegrationsAPPROVED

Quant Time: Aug 01 10:54:42 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 30 14:49:49 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/01/2024
 Supervised By :mohammad ahmed 08/13/2024

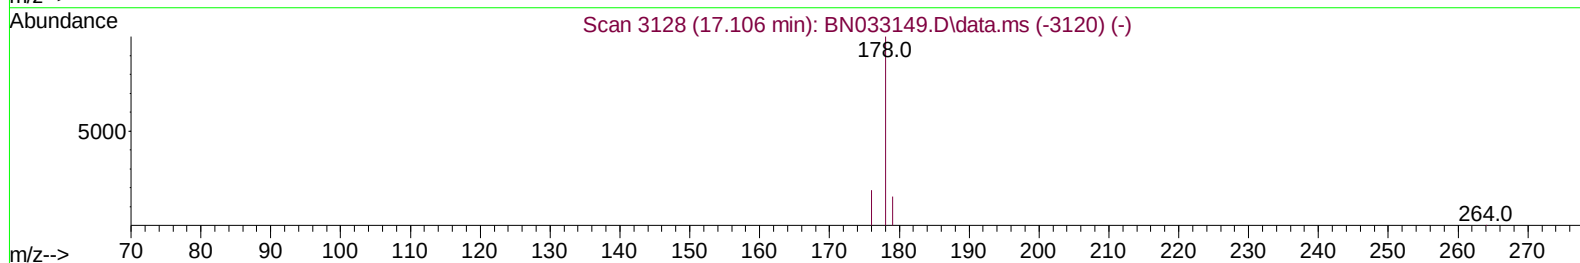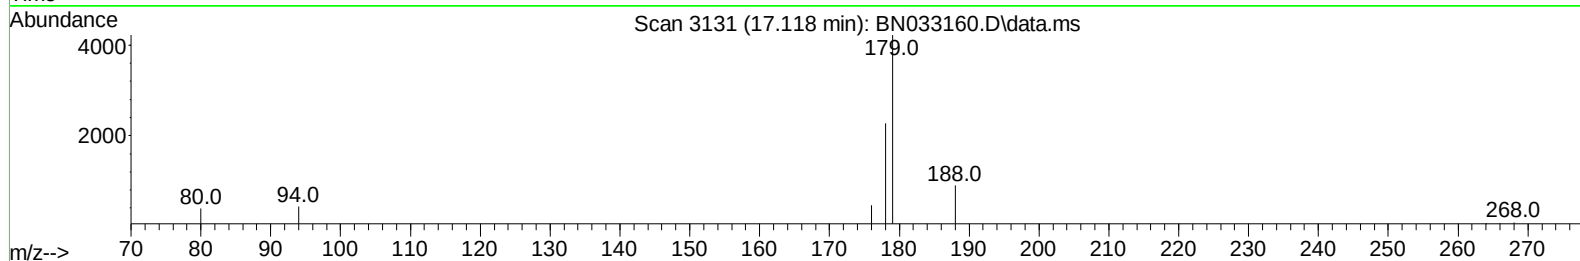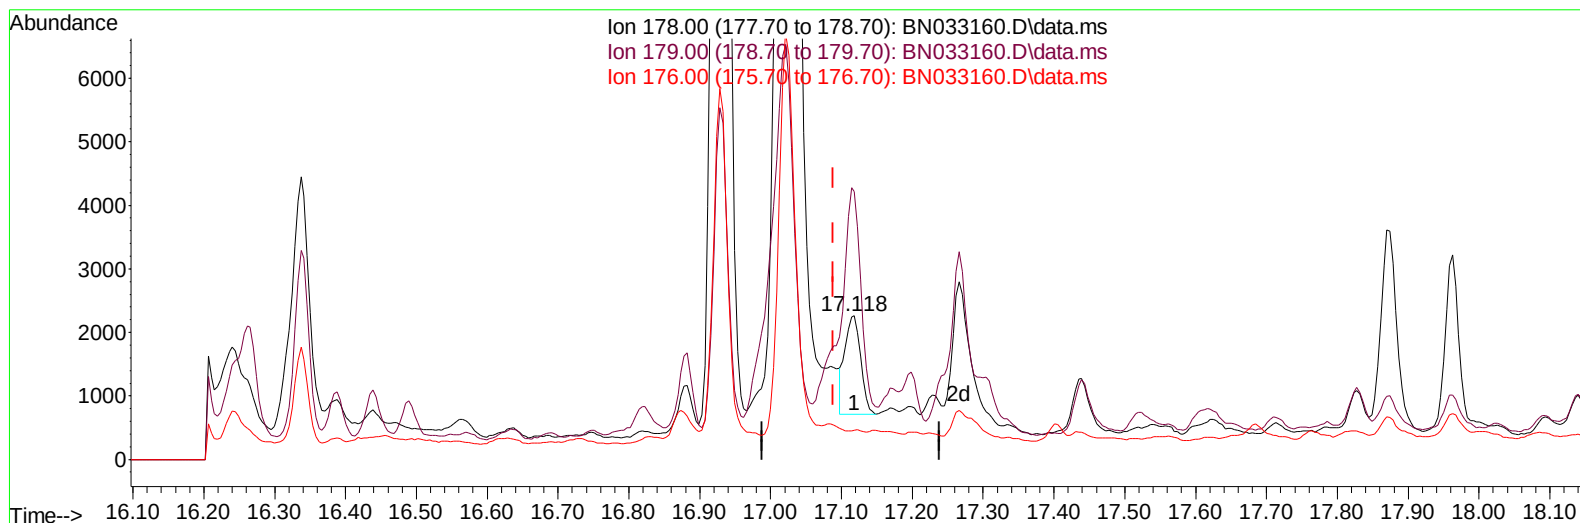

TIC: BN033160.D\data.ms

(16) Anthracene

17.118min (+ 0.030) 0.06 ng/u1

response 2396

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	17.90	186.11#
176.00	19.80	20.46
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080124\
Data File : BN033160.D
Acq On : 01 Aug 2024 09:31
Operator : MA/JU
Sample : P3378-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B10

Manual IntegrationsAPPROVED

Quant Time: Aug 01 10:54:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/01/2024
Supervised By :mohammad ahmed 08/13/2024

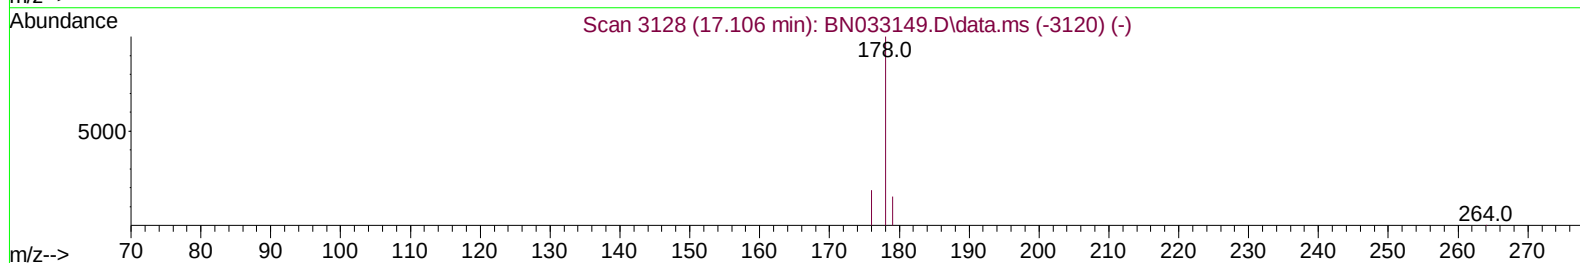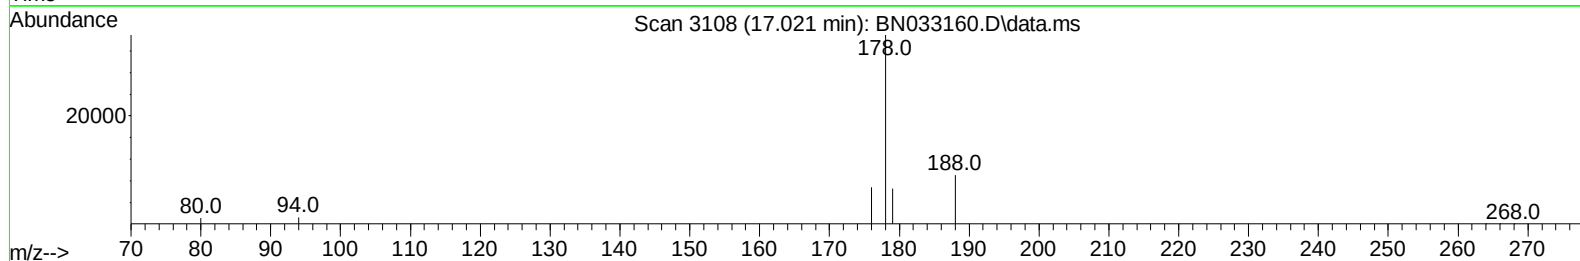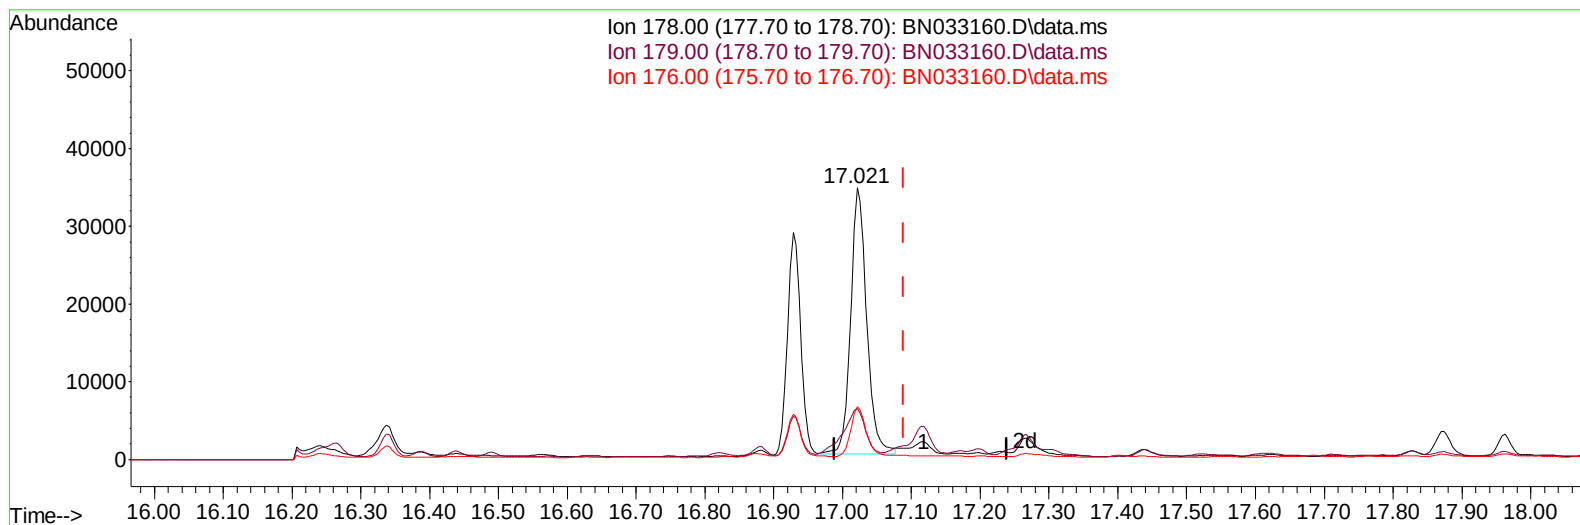

TIC: BN033160.D\data.ms

(16) Anthracene

17.021min (-0.067) 1.45 ng/ul m

response 55594

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	17.90	18.69
176.00	19.80	19.37
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080124\
Data File : BN033160.D
Acq On : 01 Aug 2024 09:31
Operator : MA/JU
Sample : P3378-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B10

Manual IntegrationsAPPROVED

Quant Time: Aug 01 10:54:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/01/2024
Supervised By :mohammad ahmed 08/13/2024

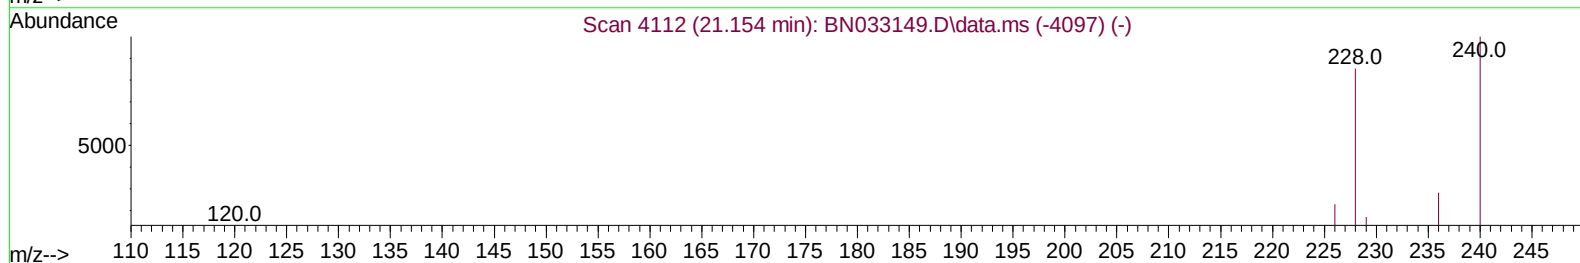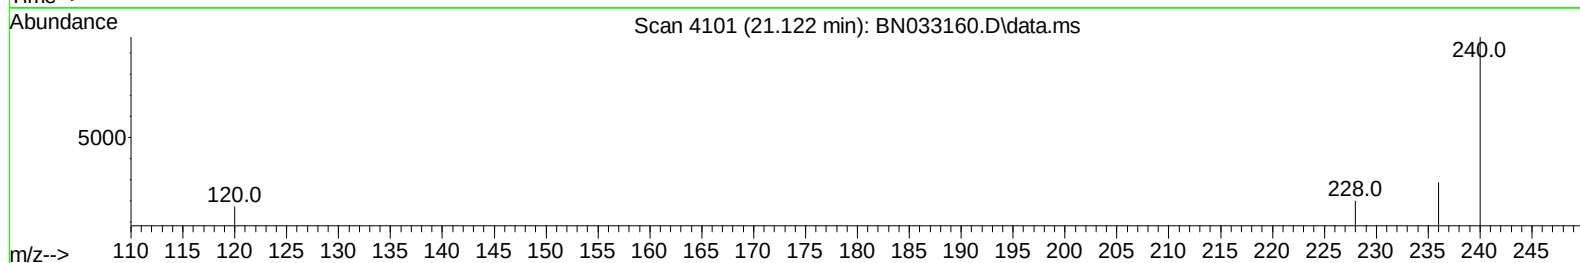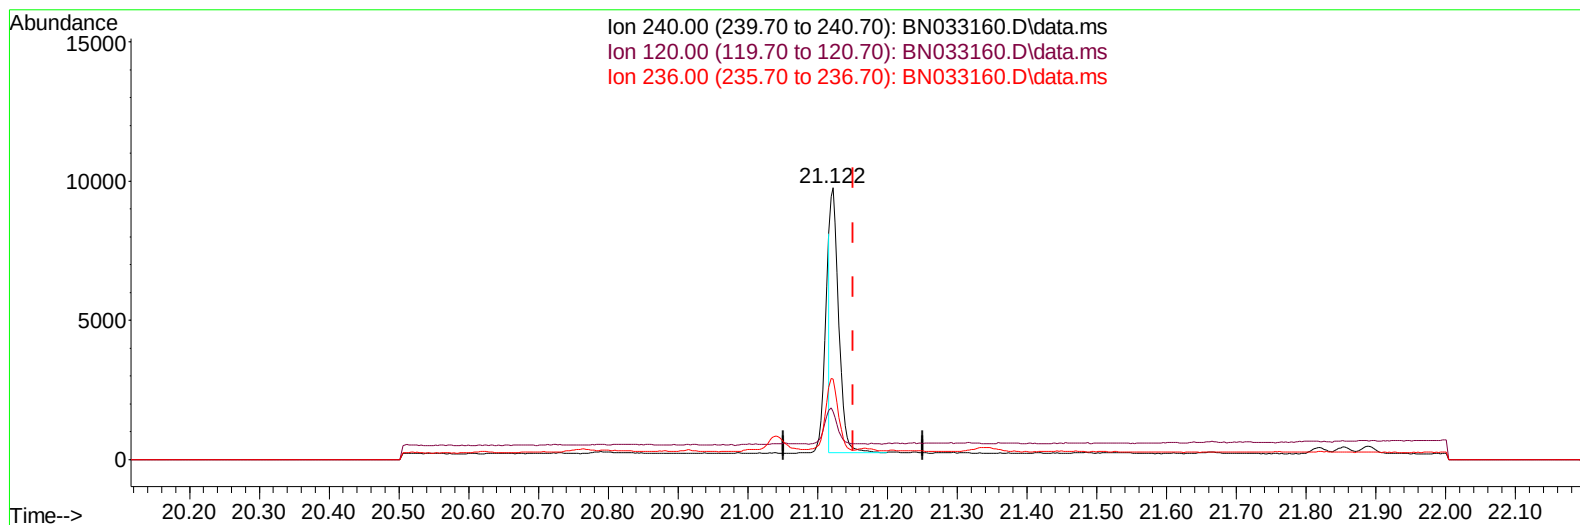

TIC: BN033160.D\data.ms

(17) Chrysene-d12

21.122min (-0.029) 0.40 ng/u1

response 7965

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	21.40	17.67
236.00	29.50	29.69
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080124\
Data File : BN033160.D
Acq On : 01 Aug 2024 09:31
Operator : MA/JU
Sample : P3378-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B10

Manual IntegrationsAPPROVED

Quant Time: Aug 01 10:54:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/01/2024
Supervised By :mohammad ahmed 08/13/2024

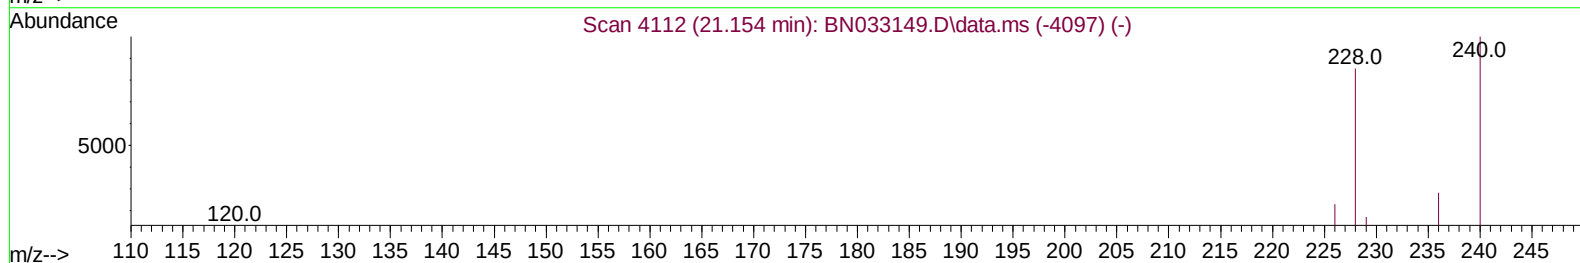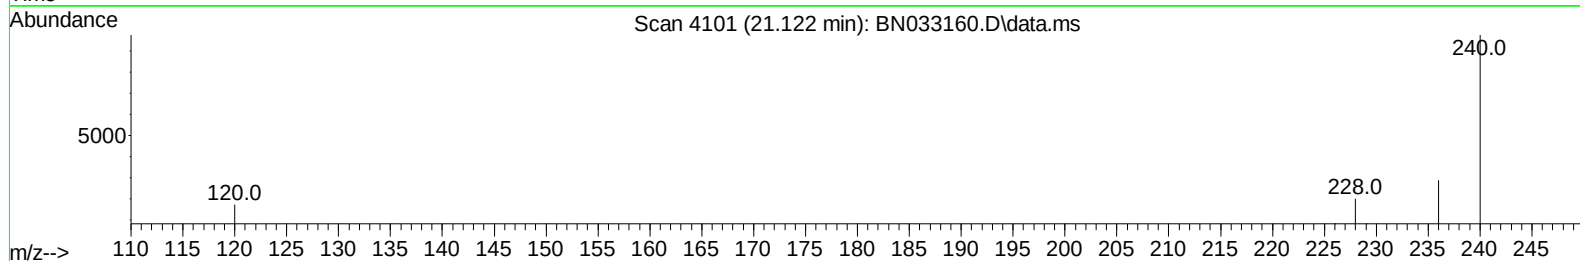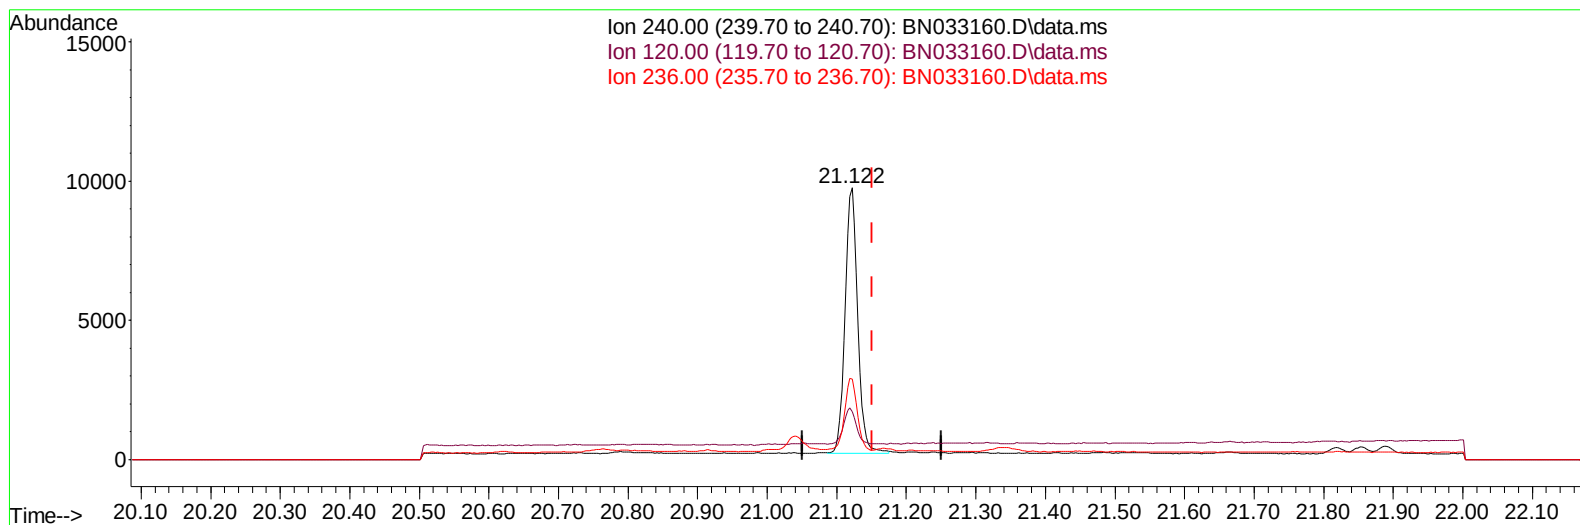

TIC: BN033160.D\data.ms

(17) Chrysene-d12

21.122min (-0.029) 0.40 ng/ul m

response 12015

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	21.40	17.67
236.00	29.50	29.69
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080124\
Data File : BN033160.D
Acq On : 01 Aug 2024 09:31
Operator : MA/JU
Sample : P3378-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B10

Manual IntegrationsAPPROVED

Quant Time: Aug 01 10:54:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/01/2024
Supervised By :mohammad ahmed 08/13/2024

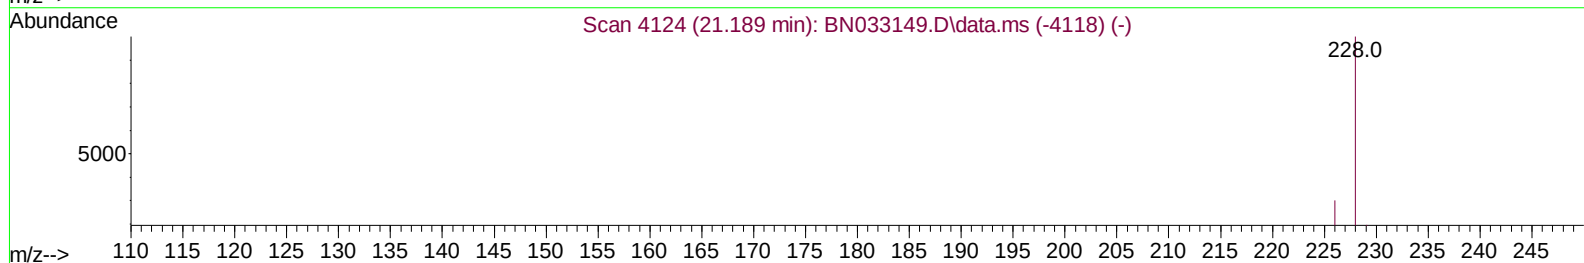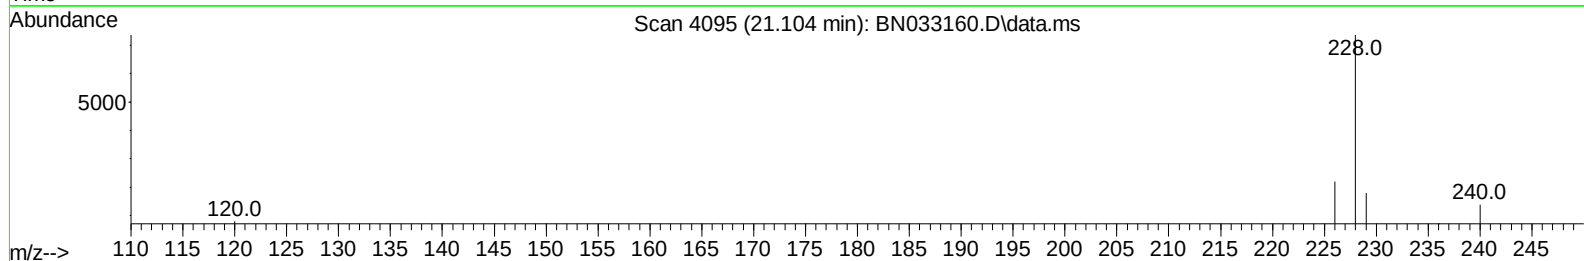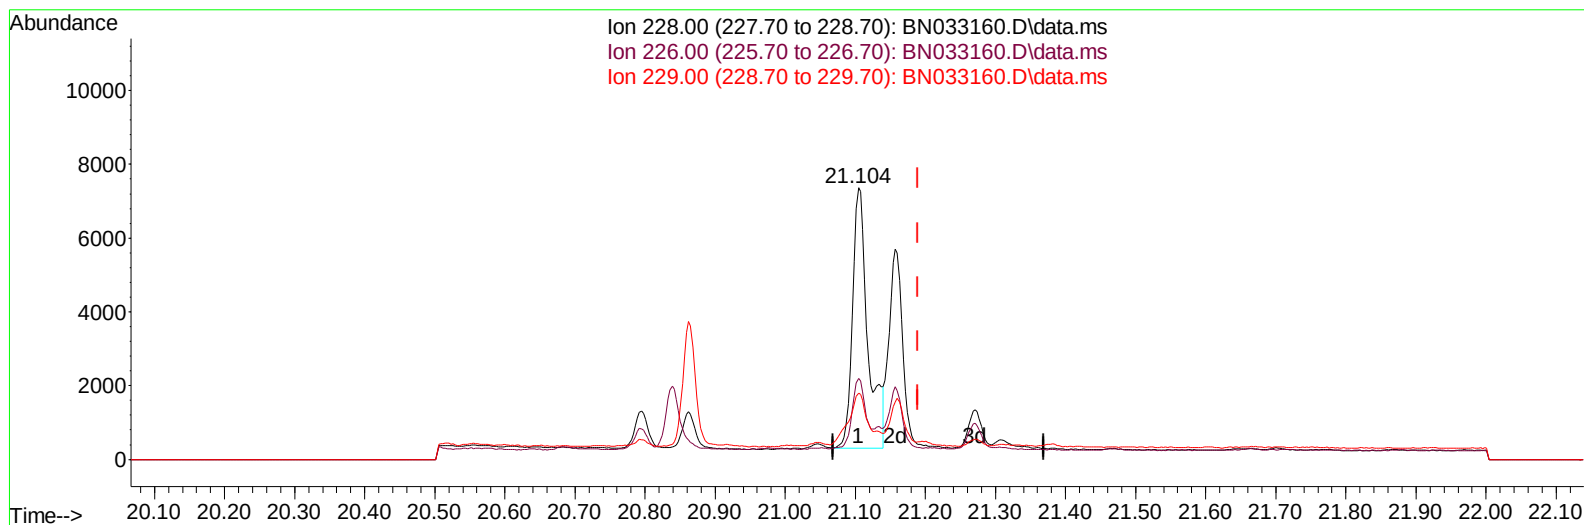

TIC: BN033160.D\data.ms

(22) Chrysene

21.104min (-0.085) 0.22 ng/u1

response 10754

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	30.90	29.88
229.00	21.30	24.34
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080124\
Data File : BN033160.D
Acq On : 01 Aug 2024 09:31
Operator : MA/JU
Sample : P3378-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B10

Manual IntegrationsAPPROVED

Quant Time: Aug 01 10:54:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/01/2024
Supervised By :mohammad ahmed 08/13/2024

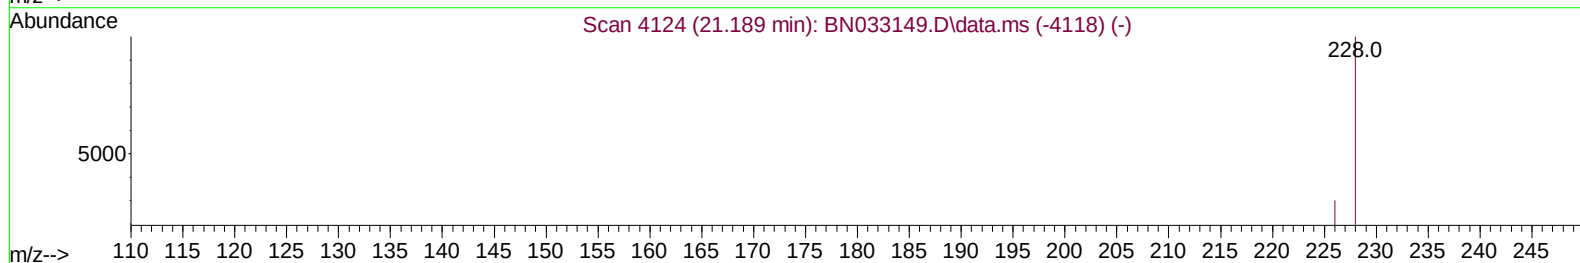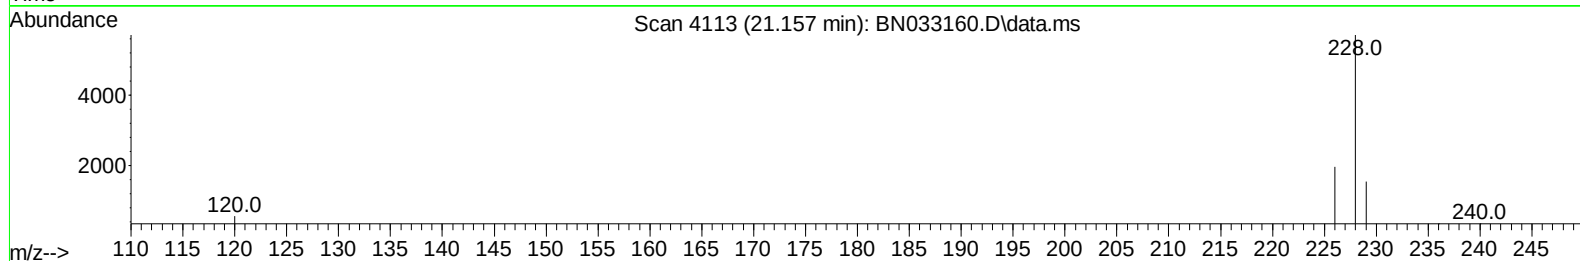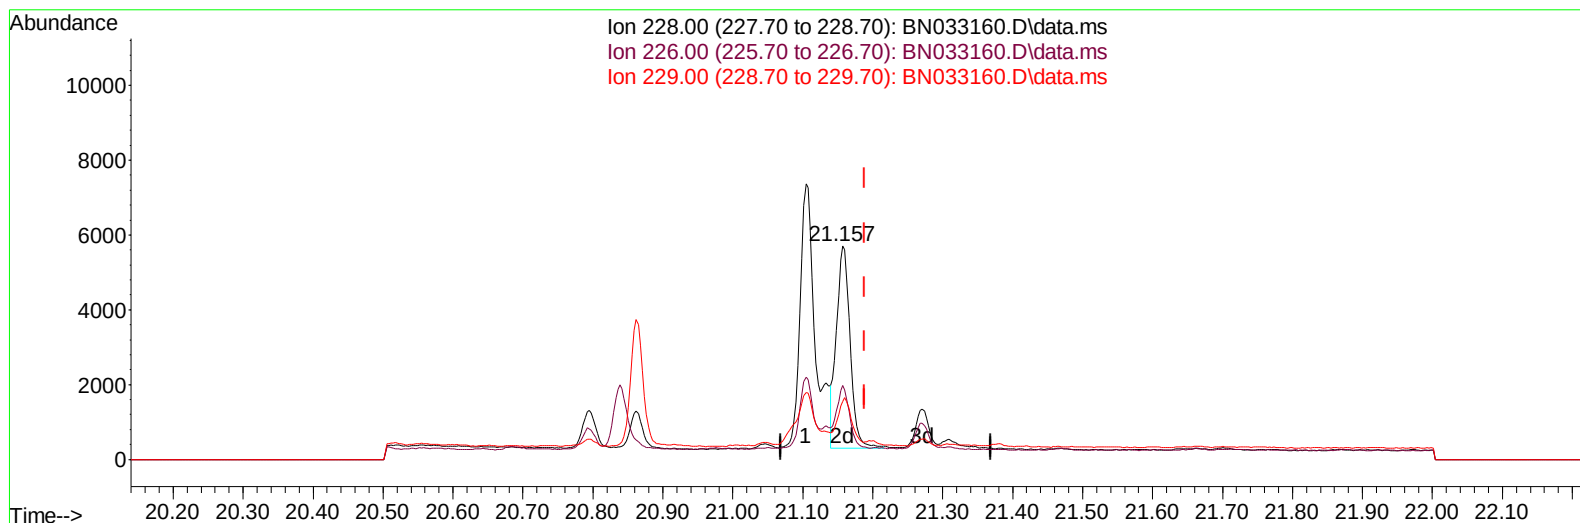

TIC: BN033160.D\data.ms

(22) Chrysene

21.157min (-0.032) 0.15 ng/ul m

response 7360

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	30.90	34.55
229.00	21.30	27.31#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080124\
Data File : BN033160.D
Acq On : 01 Aug 2024 09:31
Operator : MA/JU
Sample : P3378-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B10

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/01/2024
Supervised By :mohammad ahmed 08/13/2024

Quant Time: Aug 01 10:54:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

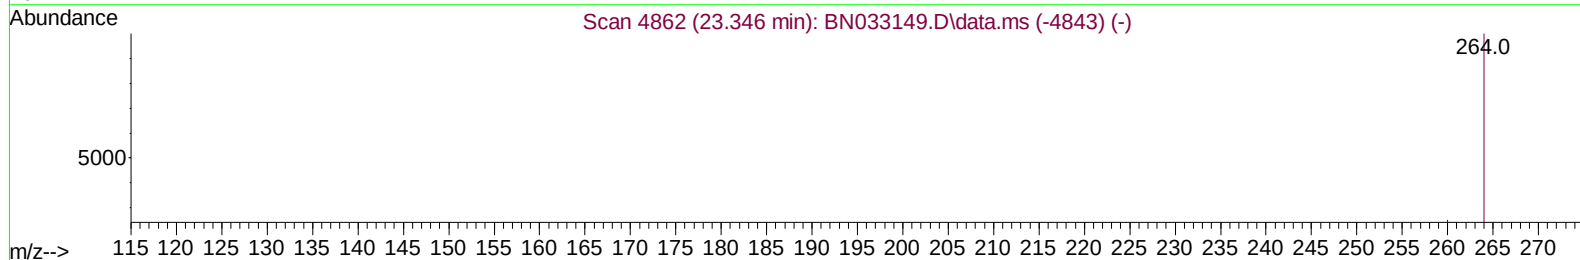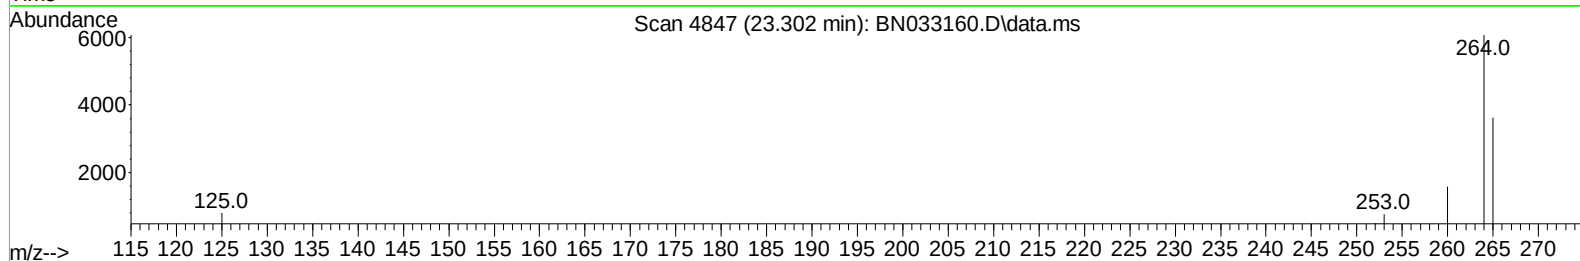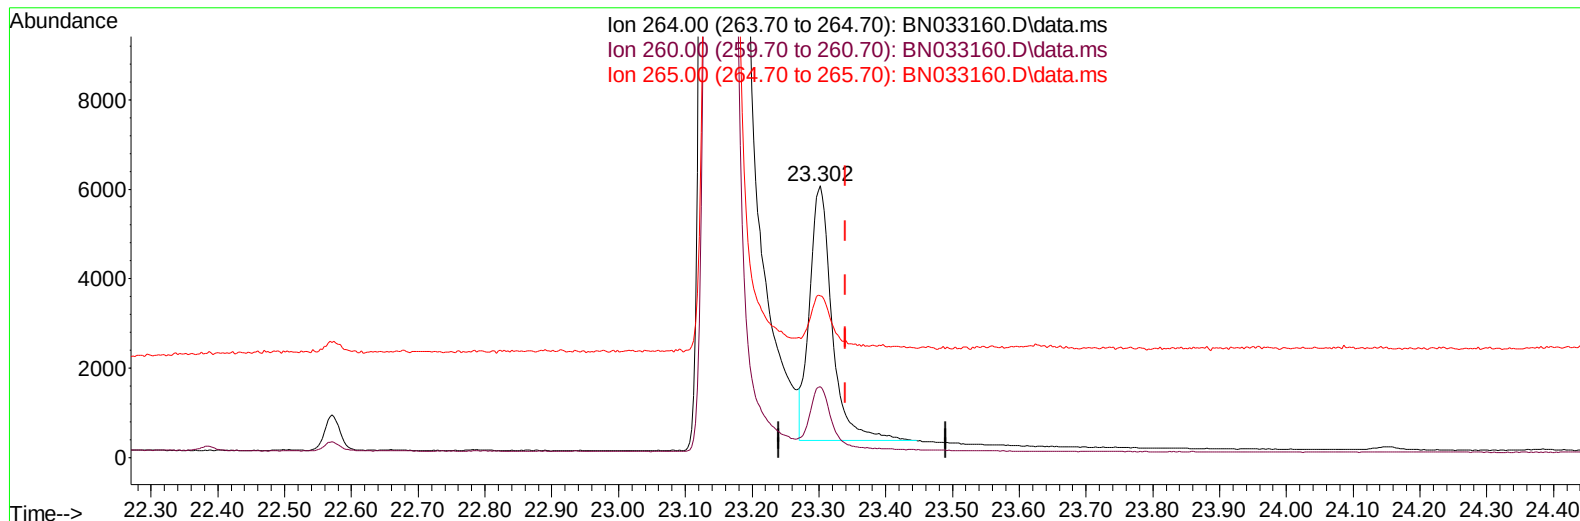

TIC: BN033160.D\data.ms

(23) Perylene-d12 (I)

23.302min (-0.038) 0.40 ng/u1

response 13567

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.50	26.18
265.00	80.60	59.65#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080124\
Data File : BN033160.D
Acq On : 01 Aug 2024 09:31
Operator : MA/JU
Sample : P3378-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B10

Manual IntegrationsAPPROVED

Quant Time: Aug 01 10:54:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/01/2024
Supervised By :mohammad ahmed 08/13/2024

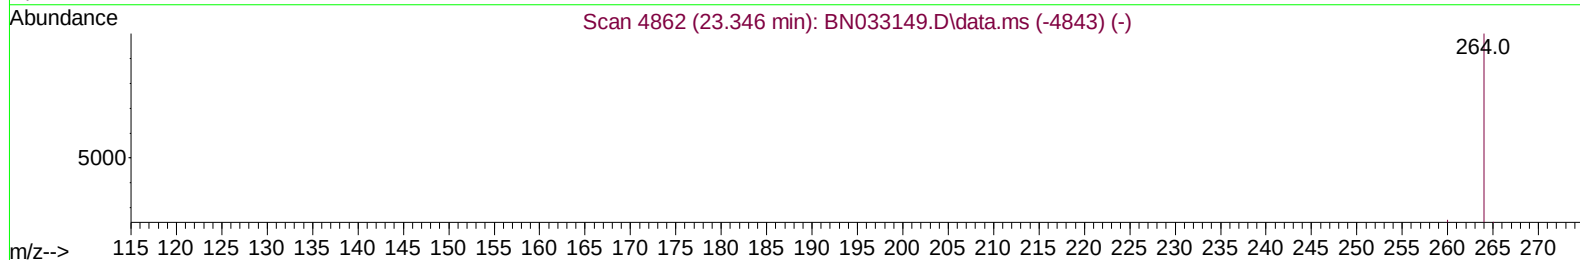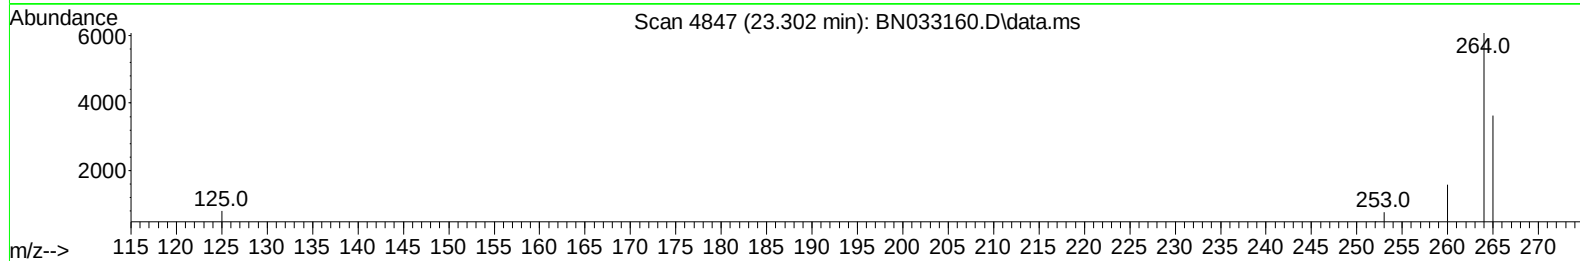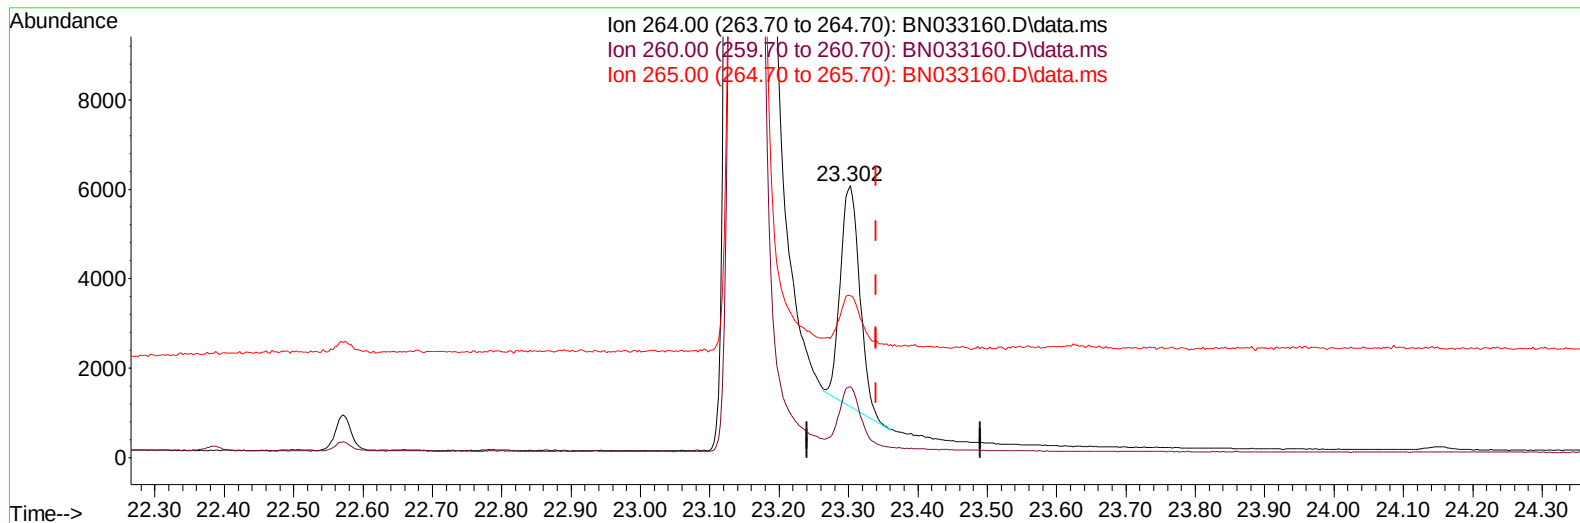

TIC: BN033160.D\data.ms

(23) Perylene-d12 (I)

23.302min (-0.038) 0.40 ng/ul m

response 9543

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.50	26.18
265.00	80.60	59.65#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080124\
Data File : BN033160.D
Acq On : 01 Aug 2024 09:31
Operator : MA/JU
Sample : P3378-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B10

Manual IntegrationsAPPROVED

Quant Time: Aug 01 10:54:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/01/2024
Supervised By :mohammad ahmed 08/13/2024

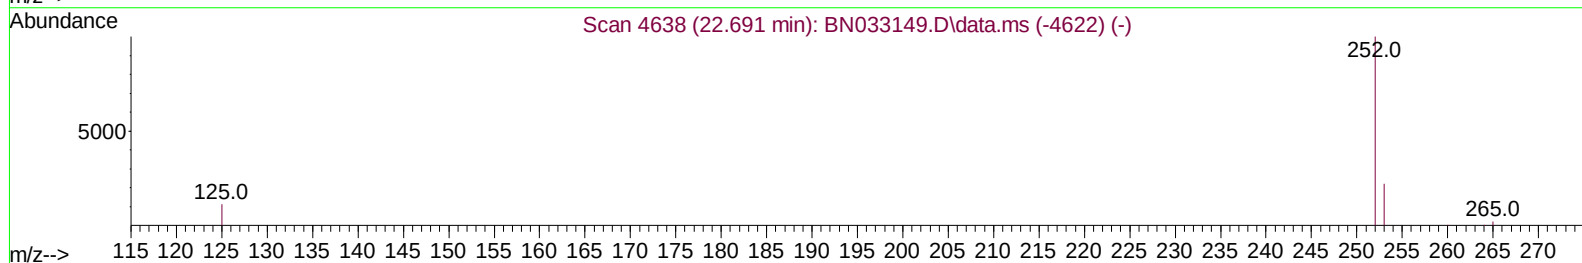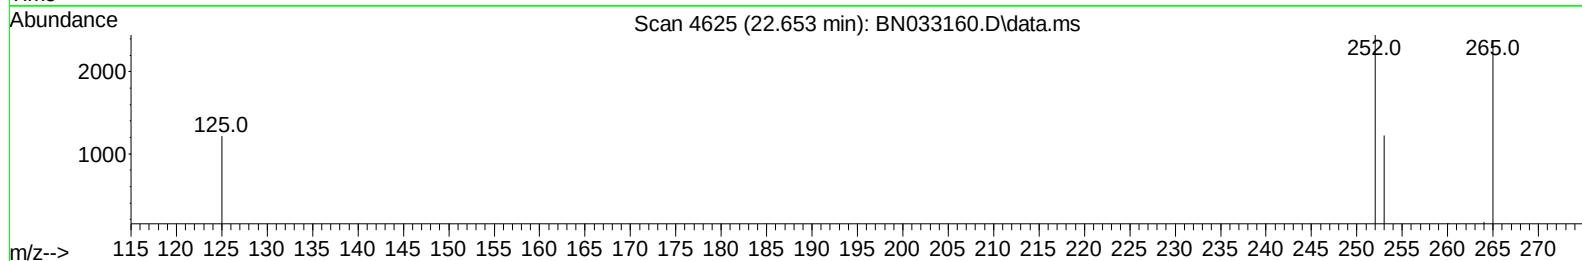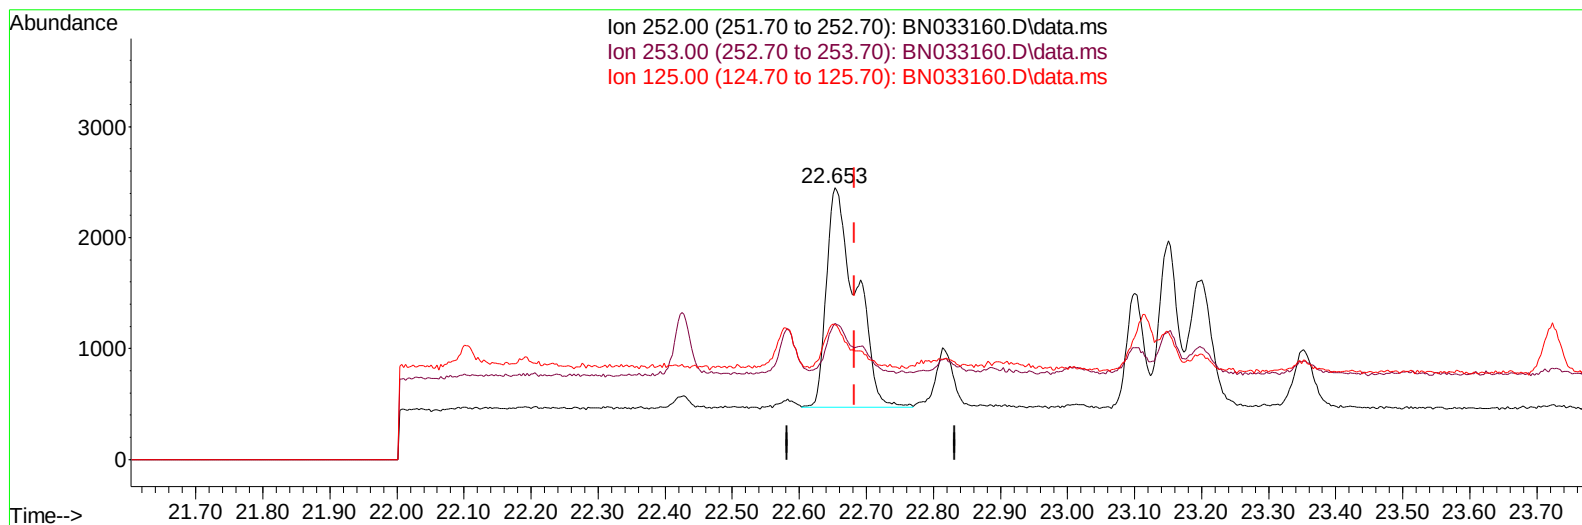

TIC: BN033160.D\data.ms

(24) Benzo(b)fluoranthene

22.653min (-0.029) 0.22 ng/u1

response 6055

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	30.30	50.04
125.00	25.50	49.67
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080124\
Data File : BN033160.D
Acq On : 01 Aug 2024 09:31
Operator : MA/JU
Sample : P3378-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B10

Manual IntegrationsAPPROVED

Quant Time: Aug 01 10:54:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/01/2024
Supervised By :mohammad ahmed 08/13/2024

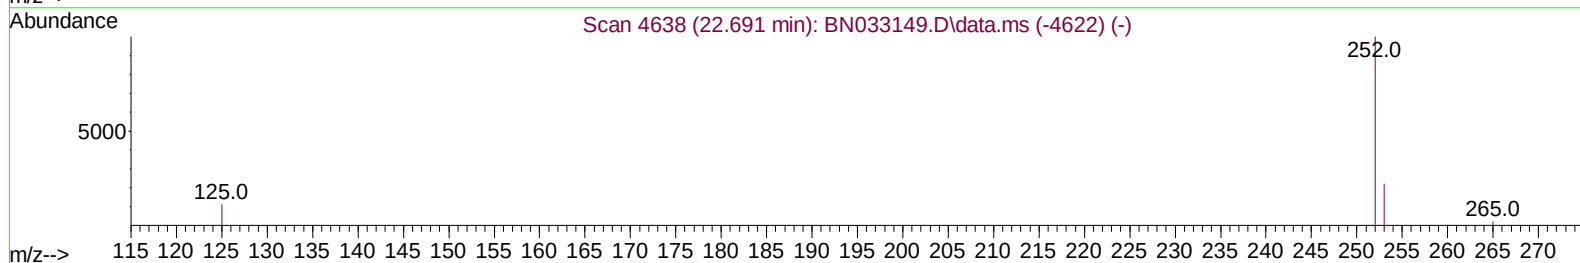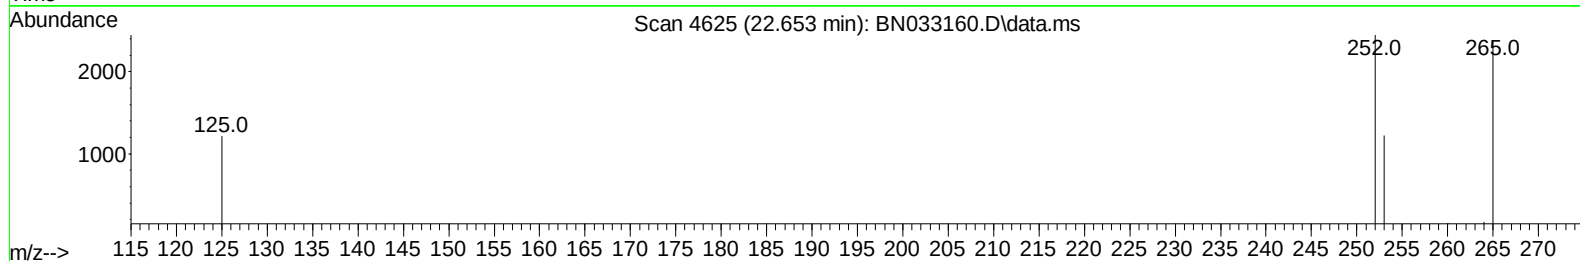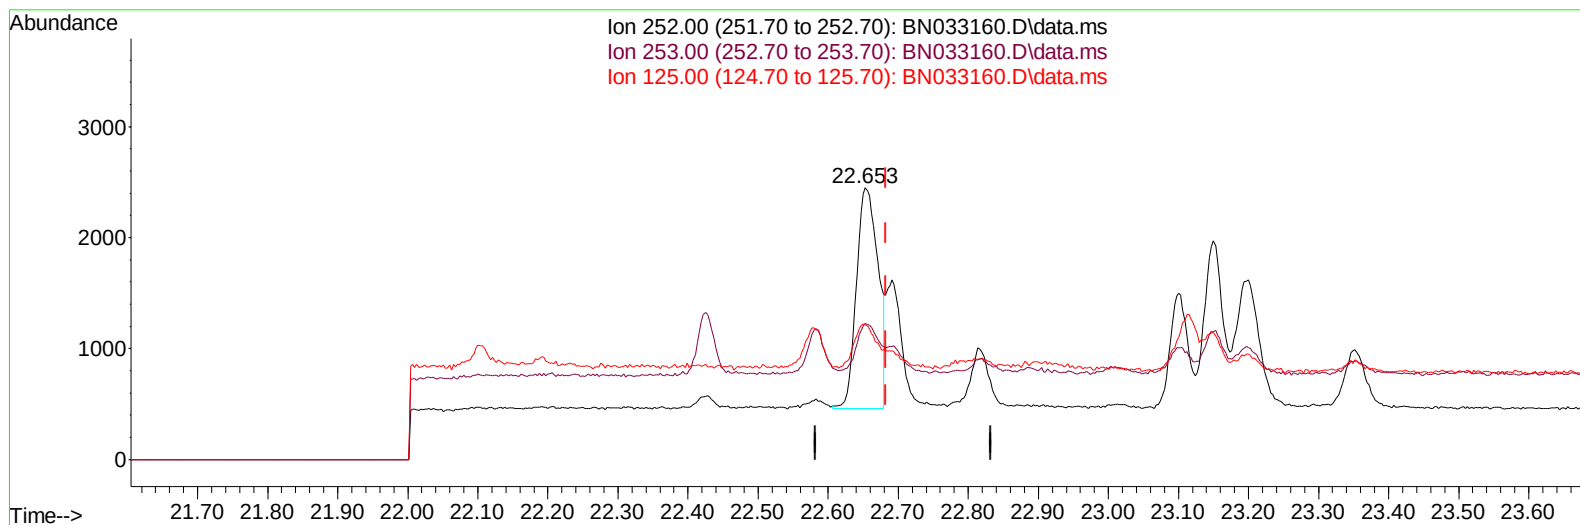

TIC: BN033160.D\data.ms

(24) Benzo(b)fluoranthene

22.653min (-0.029) 0.15 ng/ul m

response 4282

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	30.30	50.04
125.00	25.50	49.67
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080124\
Data File : BN033160.D
Acq On : 01 Aug 2024 09:31
Operator : MA/JU
Sample : P3378-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B10

Manual IntegrationsAPPROVED

Quant Time: Aug 01 10:54:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/01/2024
Supervised By :mohammad ahmed 08/13/2024

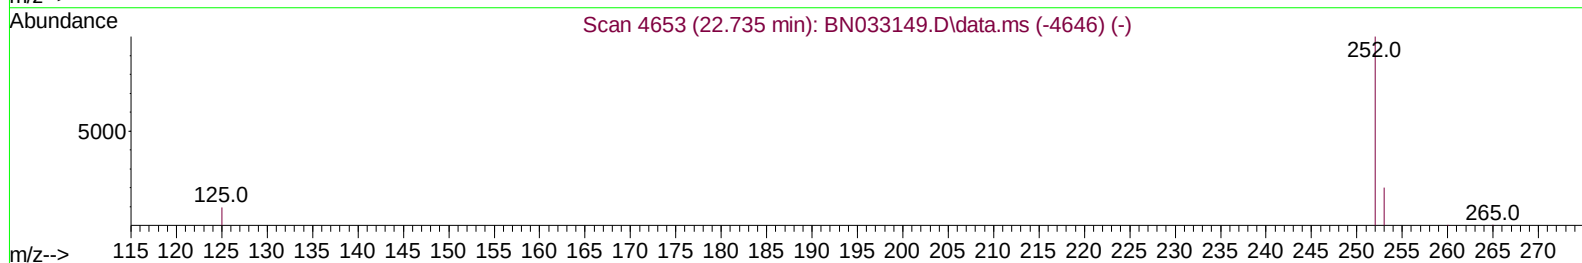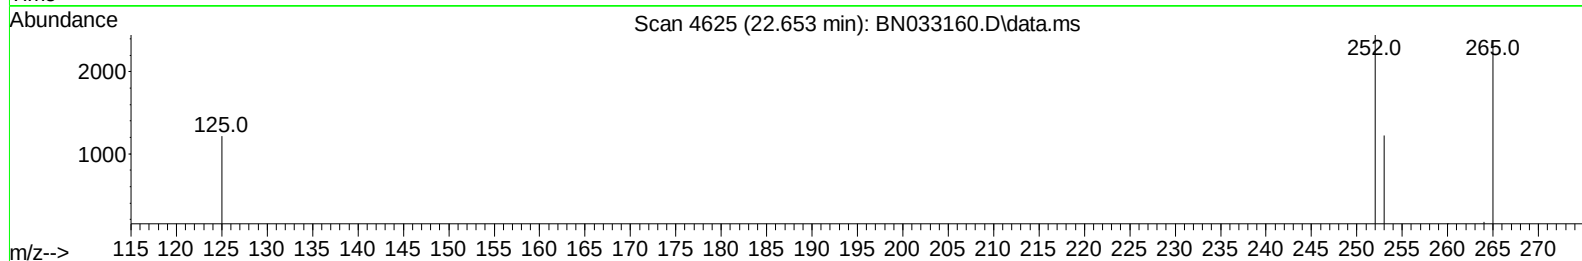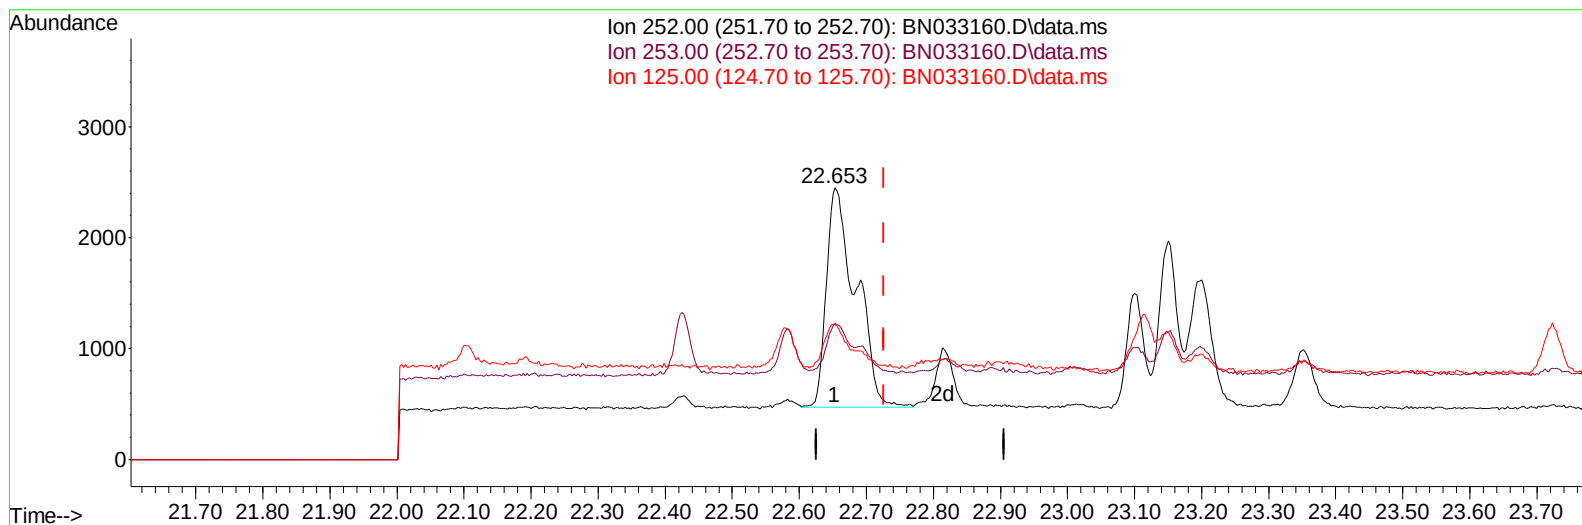

TIC: BN033160.D\data.ms

(25) Benzo(k)fluoranthene

22.653min (-0.073) 0.18 ng/u1

response 6035

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	31.10	50.04#
125.00	26.10	49.67#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080124\
Data File : BN033160.D
Acq On : 01 Aug 2024 09:31
Operator : MA/JU
Sample : P3378-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B10

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/01/2024
Supervised By :mohammad ahmed 08/13/2024

Quant Time: Aug 01 10:54:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

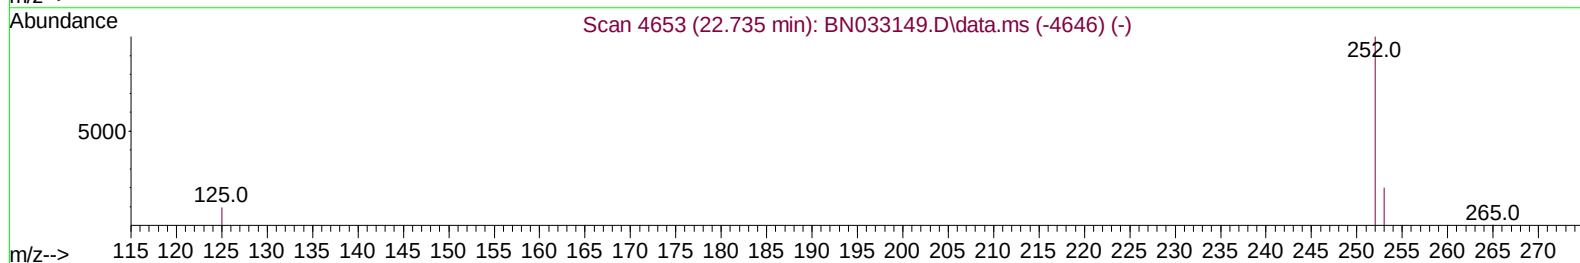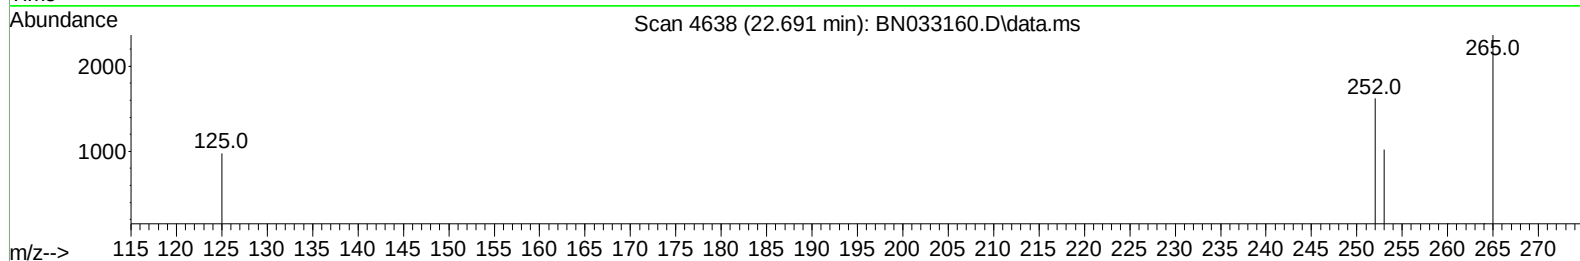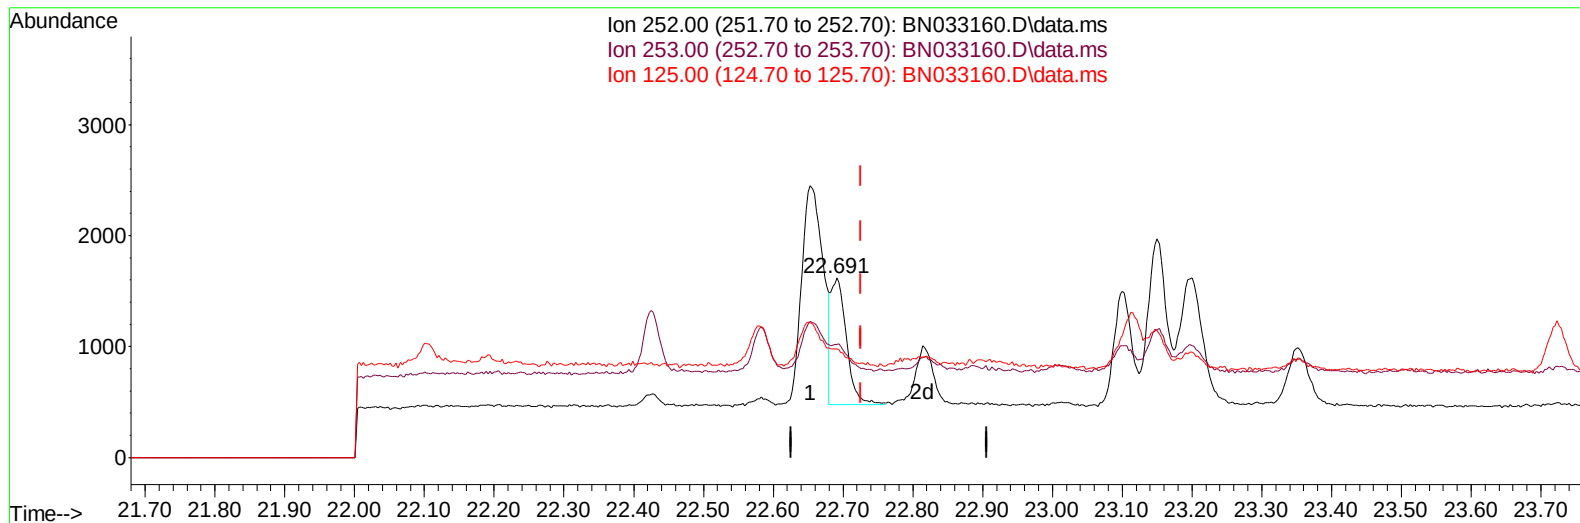

TIC: BN033160.D\data.ms

(25) Benzo(k)fluoranthene

22.691min (-0.035) 0.05 ng/ul m

response 1766

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	31.10	62.88#
125.00	26.10	60.47#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080124\
 Data File : BN033160.D
 Acq On : 01 Aug 2024 09:31
 Operator : MA/JU
 Sample : P3378-08
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0B10

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/01/2024
 Supervised By :mohammad ahmed 08/13/2024

Quant Time: Aug 01 10:54:42 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 30 14:49:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.478	152	3248m	0.400	ng/ul	-0.07
4) Naphthalene-d8	10.234	136	10417	0.400	ng/ul	#-0.08
9) Acenaphthene-d10	14.120	164	6623	0.400	ng/ul	-0.04
13) Phenanthrene-d10	16.890	188	15903m	0.400	ng/ul	-0.05
17) Chrysene-d12	21.122	240	12015m	0.400	ng/ul	-0.03
23) Perylene-d12	23.302	264	9543m	0.400	ng/ul	-0.04
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.052	96	16100	3.919	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.846	152	4288	0.252	ng/ul	-0.08
18) Fluoranthene-d10	18.935	212	12357	0.363	ng/ul	-0.04
Target Compounds						
					Qvalue	
5) Naphthalene	10.284	128	35201	1.316	ng/ul#	93
7) 2-Methylnaphthalene	11.923	142	1606	0.089	ng/ul	99
8) 1-Methylnaphthalene	12.132	142	80369	4.101	ng/ul	99
10) Acenaphthylene	13.838	152	22817	0.842	ng/ul#	96
11) Acenaphthene	14.180	153	992475	48.679	ng/ul	98
12) Fluorene	15.184	166	477973	20.114	ng/ul	98
15) Phenanthrene	16.928	178	41022m	0.962	ng/ul	
16) Anthracene	17.021	178	55594m	1.450	ng/ul	
19) Fluoranthene	18.967	202	272743	6.894	ng/ul	95
20) Pyrene	19.330	202	231236	5.451	ng/ul	98
21) Benzo(a)anthracene	21.104	228	10754	0.262	ng/ul	95
22) Chrysene	21.157	228	7360m	0.154	ng/ul	
24) Benzo(b)fluoranthene	22.653	252	4282m	0.154	ng/ul	
25) Benzo(k)fluoranthene	22.691	252	1766m	0.053	ng/ul	
26) Benzo(a)pyrene	23.200	252	2466	0.094	ng/ul#	54
27) Indeno(1,2,3-cd)pyrene	25.517	276	1258	0.032	ng/ul#	94
29) Benzo(g,h,i)perylene	26.188	276	1146	0.036	ng/ul#	42

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080124\
Data File : BN033160.D
Acq On : 01 Aug 2024 09:31
Operator : MA/JU
Sample : P3378-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B10

Manual IntegrationsAPPROVED

Quant Time: Aug 01 10:54:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/01/2024
Supervised By :mohammad ahmed 08/13/2024

