

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080124\
 Data File : BN033139.D
 Acq On : 31 Jul 2024 20:15
 Operator : MA/JU
 Sample : P3359-12
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1GD6

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 08/01/2024
 Supervised By :mohammad ahmed 08/13/2024

Quant Time: Jul 31 23:34:19 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 30 14:49:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.495	152	2453	0.400	ng/ul	-0.05
4) Naphthalene-d8	10.245	136	8550	0.400	ng/ul	-0.07
9) Acenaphthene-d10	14.134	164	5587	0.400	ng/ul	#-0.03
13) Phenanthrene-d10	16.903	188	11922m	0.400	ng/ul	-0.04
17) Chrysene-d12	21.157	240	10589	0.400	ng/ul	0.00
23) Perylene-d12	23.323	264	4696m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.052	96	13945	4.494	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.890	152	4032	0.289	ng/ul	-0.04
18) Fluoranthene-d10	18.953	212	10822	0.361	ng/ul	-0.02
Target Compounds						
5) Naphthalene	10.295	128	885	0.040	ng/ul#	Qvalue 74

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080124\
Data File : BN033139.D
Acq On : 31 Jul 2024 20:15
Operator : MA/JU
Sample : P3359-12
Misc :
ALS Vial : 16 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
E1GD6

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 08/01/2024
Supervised By :mohammad ahmed 08/13/2024


Quant Time: Jul 31 23:34:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

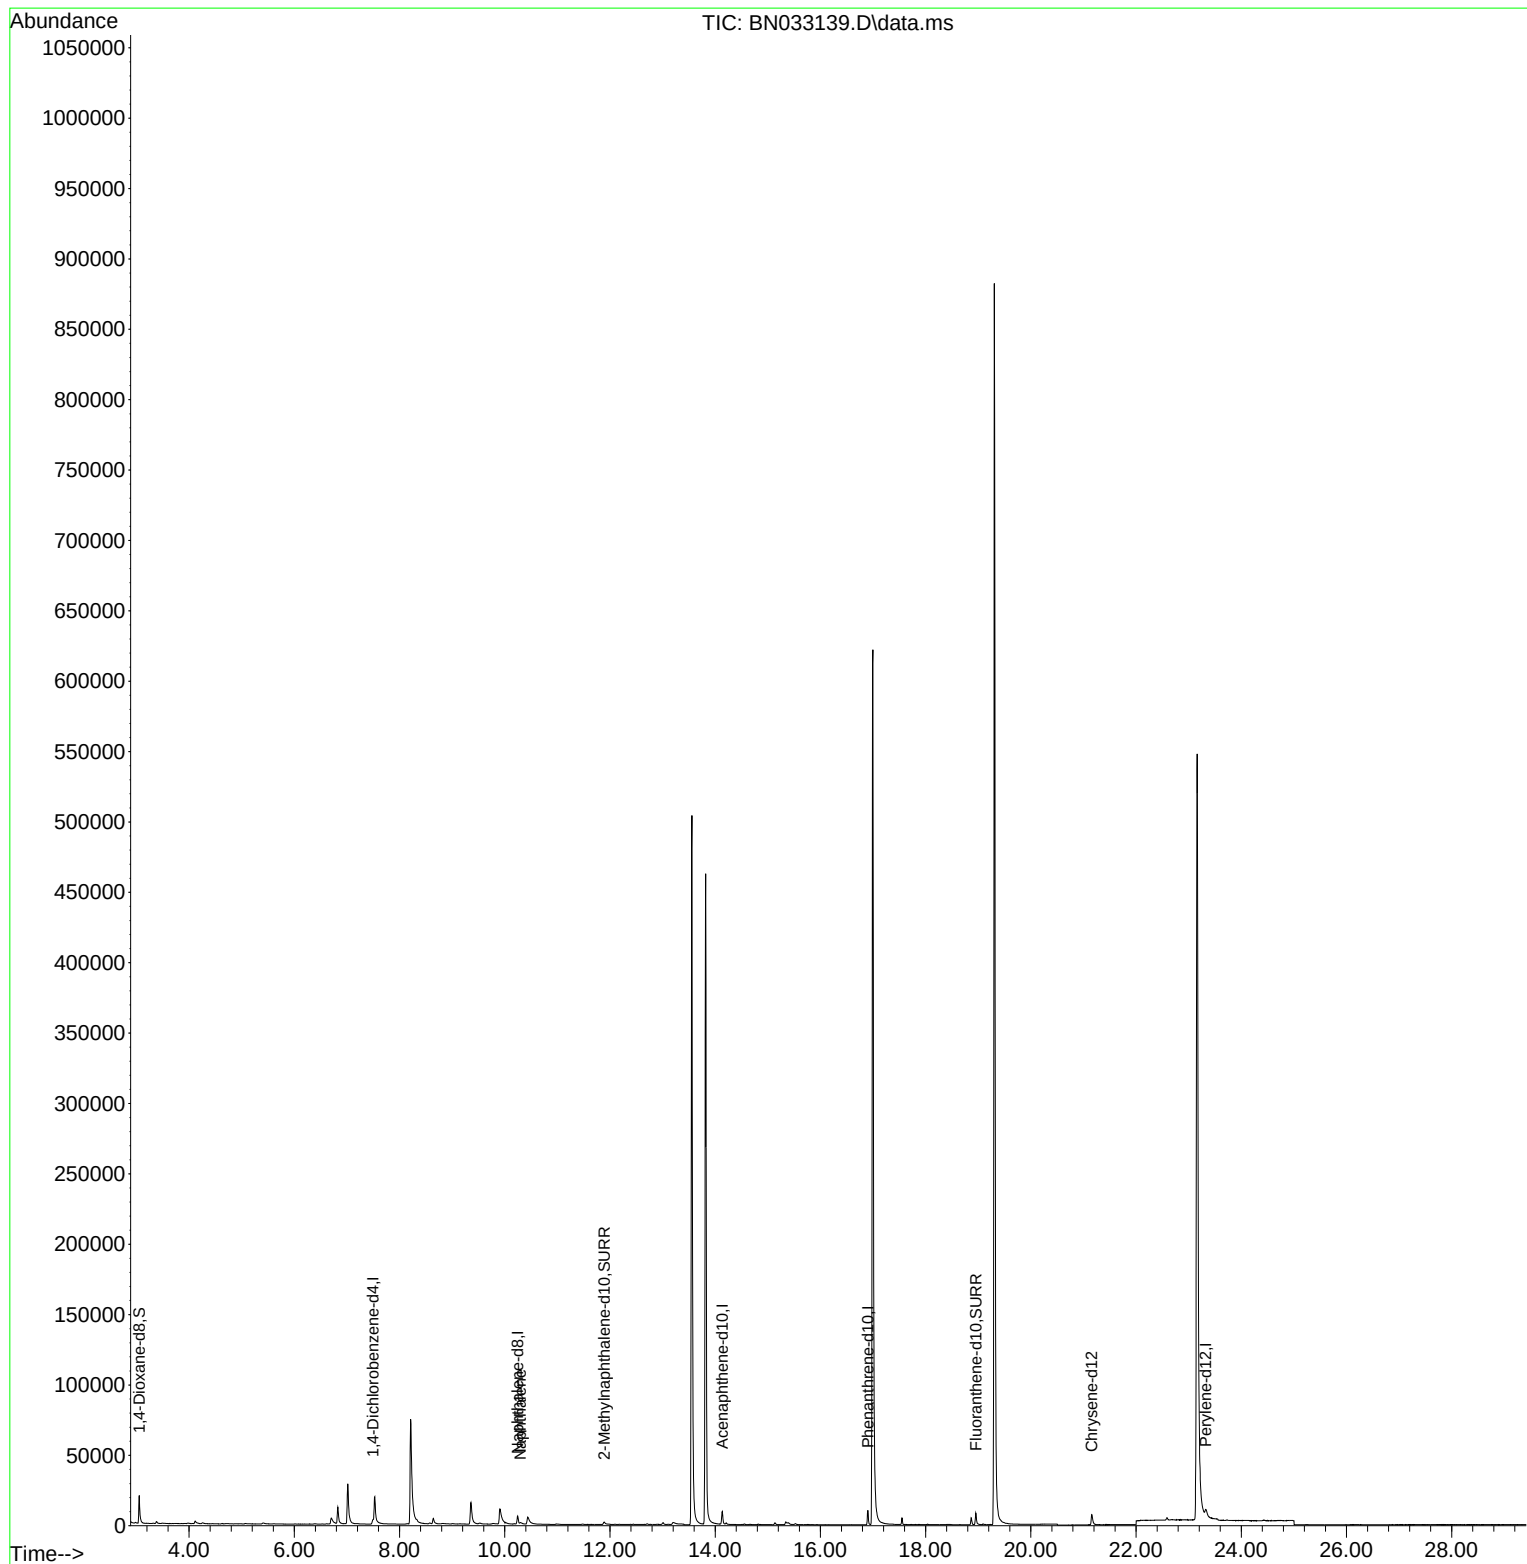

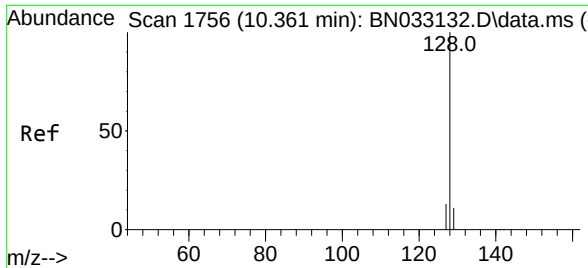

#5
 Naphthalene
 Concen: 0.040 ng/ul
 RT: 10.295 min Scan# 11
 Delta R.T. -0.082 min
 Lab File: BN033139.D
 Acq: 31 Jul 2024 20:15

Instrument :
 BNA_N
 ClientSampleId :
 E1GD6

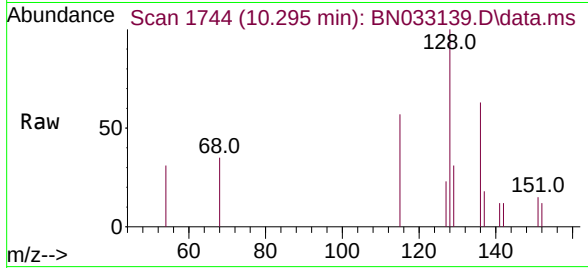

Tgt Ion:	128	Resp:	88
Ion	Ratio	Lower	Upper
128	100		
129	30.5	12.0	18.0
127	22.5	12.7	19.1

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 08/01/2024
 Supervised By :mohammad ahmed 08/13/2024

