

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080124\
 Data File : BN033146.D
 Acq On : 01 Aug 2024 00:29
 Operator : MA/JU
 Sample : P3378-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0B05

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 08/01/2024
 Supervised By :mohammad ahmed 08/13/2024

Quant Time: Aug 01 01:50:56 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 30 14:49:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.490	152	2821	0.400	ng/ul	-0.06
4) Naphthalene-d8	10.245	136	9497	0.400	ng/ul	#-0.07
9) Acenaphthene-d10	14.129	164	6156	0.400	ng/ul	-0.03
13) Phenanthrene-d10	16.899	188	13203m	0.400	ng/ul	-0.04
17) Chrysene-d12	21.154	240	11129	0.400	ng/ul	0.00
23) Perylene-d12	23.320	264	5678m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.052	96	14887	4.172	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.884	152	3537	0.228	ng/ul	-0.04
18) Fluoranthene-d10	18.949	212	11174	0.355	ng/ul	-0.02
Target Compounds						
5) Naphthalene	10.295	128	3191	0.131	ng/ul	Qvalue 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080124\
Data File : BN033146.D
Acq On : 01 Aug 2024 00:29
Operator : MA/JU
Sample : P3378-06
Misc :
ALS Vial : 23 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0B05

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 08/01/2024
Supervised By :mohammad ahmed 08/13/2024


Quant Time: Aug 01 01:50:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

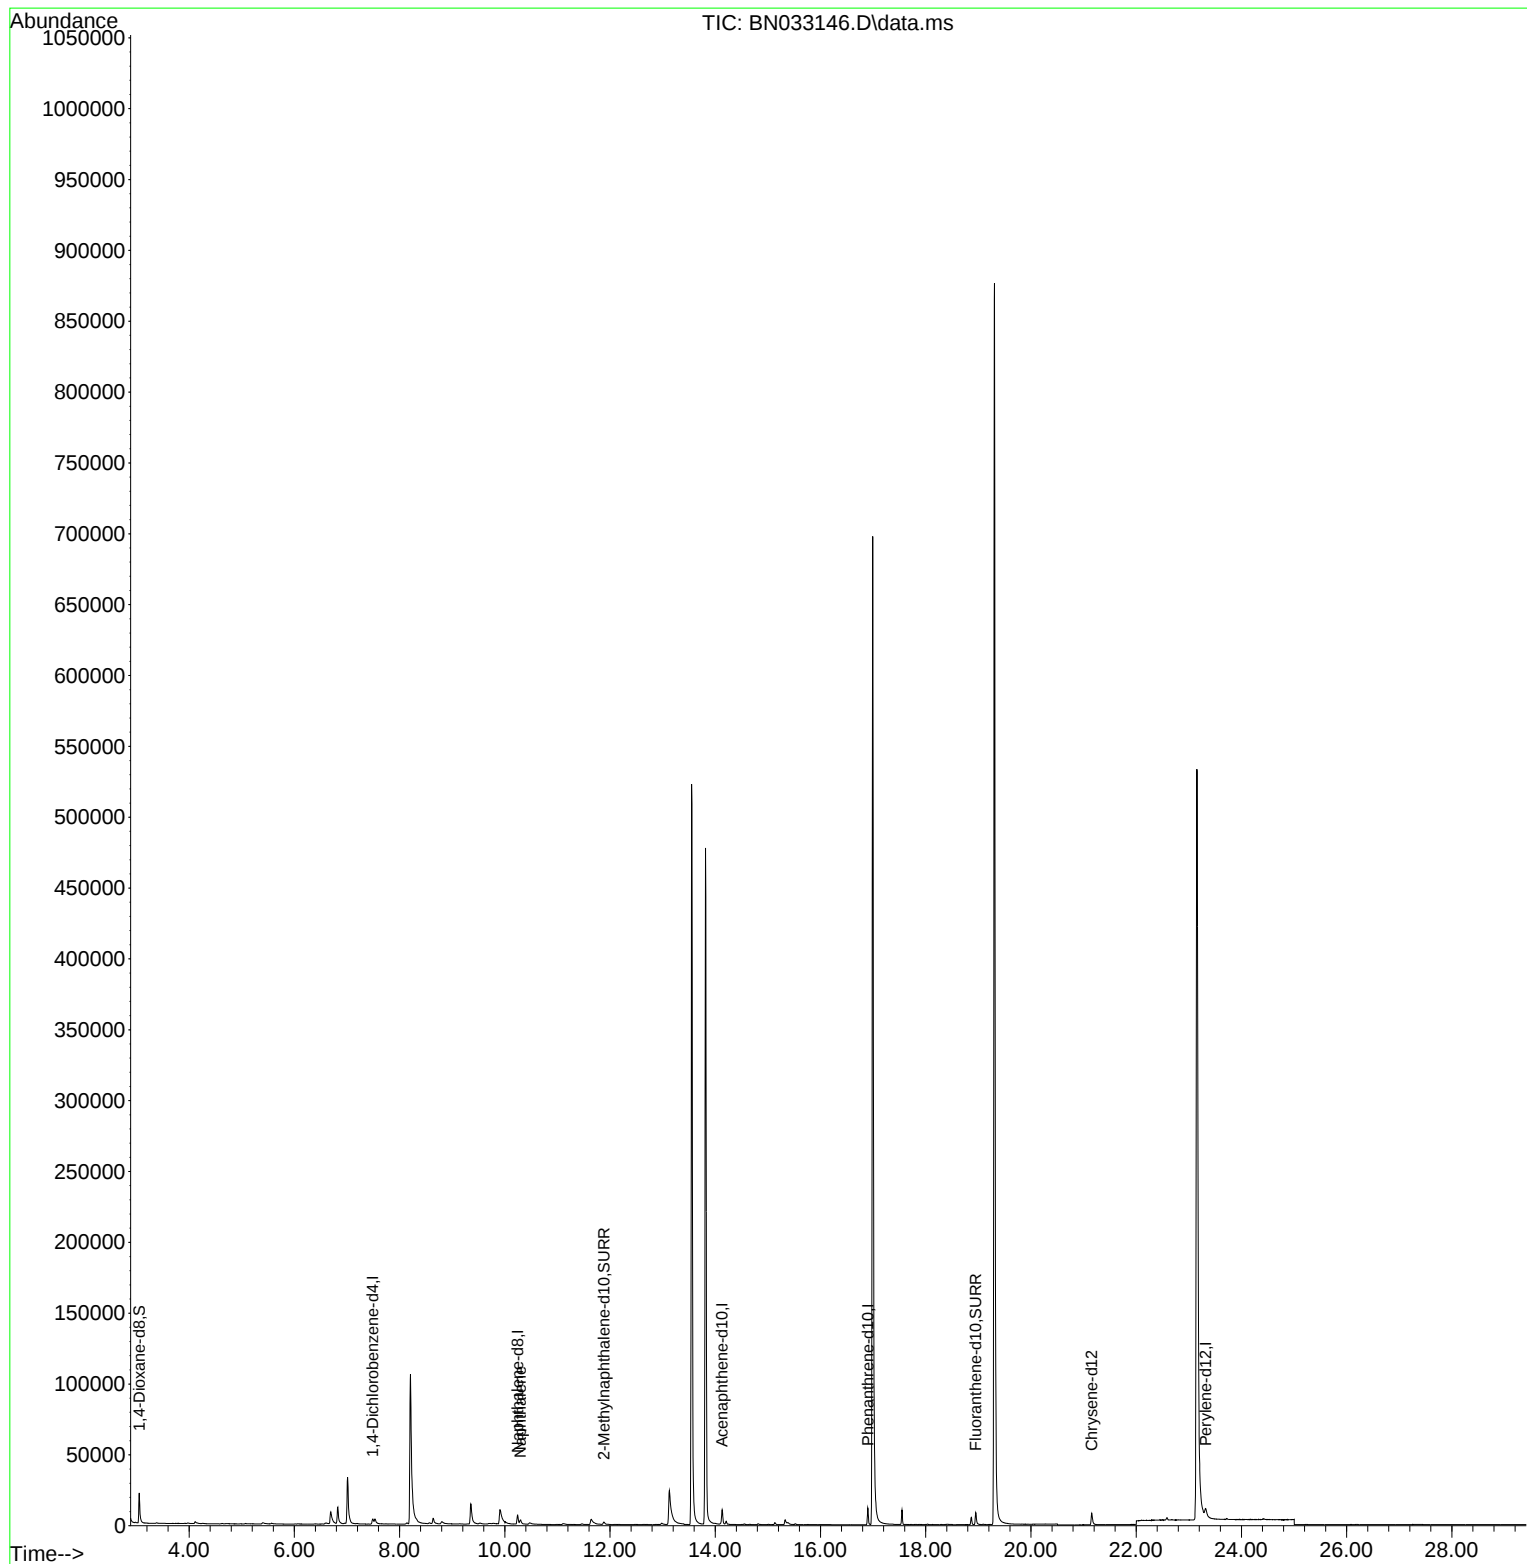

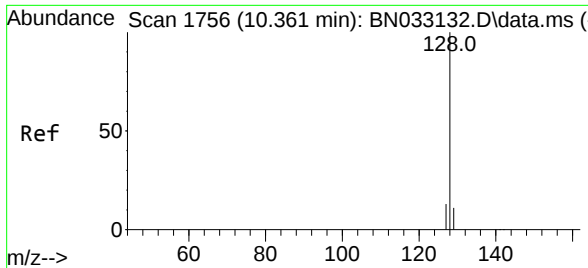

#5
Naphthalene
Concen: 0.131 ng/ul
RT: 10.295 min Scan# 1756
Delta R.T. -0.082 min
Lab File: BN033146.D
Acq: 01 Aug 2024 00:29

Instrument :
BNA_N
ClientSampleId :
C0B05

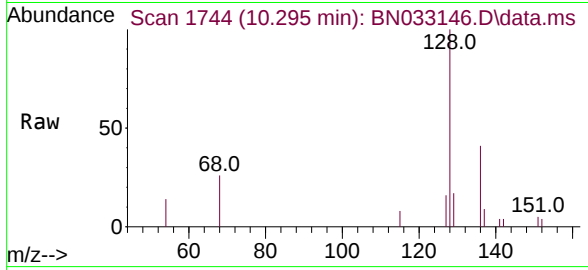

Tgt Ion:	128	Resp:	319
Ion Ratio	Lower	Upper	
128	100		
129	17.1	12.0	18.0
127	16.5	12.7	19.1

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 08/01/2024
Supervised By :mohammad ahmed 08/13/2024

