

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080822\
 Data File : BN021067.D
 Acq On : 08 Aug 2022 17:02
 Operator : CG/JU
 Sample : PB146821BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Aug 08 23:11:06 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 08 23:08:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.797	152	2945	0.400	ng/ul	0.00
4) Naphthalene-d8	10.589	136	9612	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.451	164	5536	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.200	188	10918	0.400	ng/ul	0.00
17) Chrysene-d12	21.424	240	7879	0.400	ng/ul	0.00
23) Perylene-d12	23.760	264	8211	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.202	96	17648	4.684	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.206	152	4419	0.314	ng/ul	0.02
18) Fluoranthene-d10	19.243	212	10644	0.437	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.605	202	1525	0.042	ng/ul#	1
26) Benzo(a)pyrene	23.602	252	2995	0.086	ng/ul#	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080822\
Data File : BN021067.D
Acq On : 08 Aug 2022 17:02
Operator : CG/JU
Sample : PB146821BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Aug 08 23:11:06 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 08 23:08:49 2022
Response via : Initial Calibration




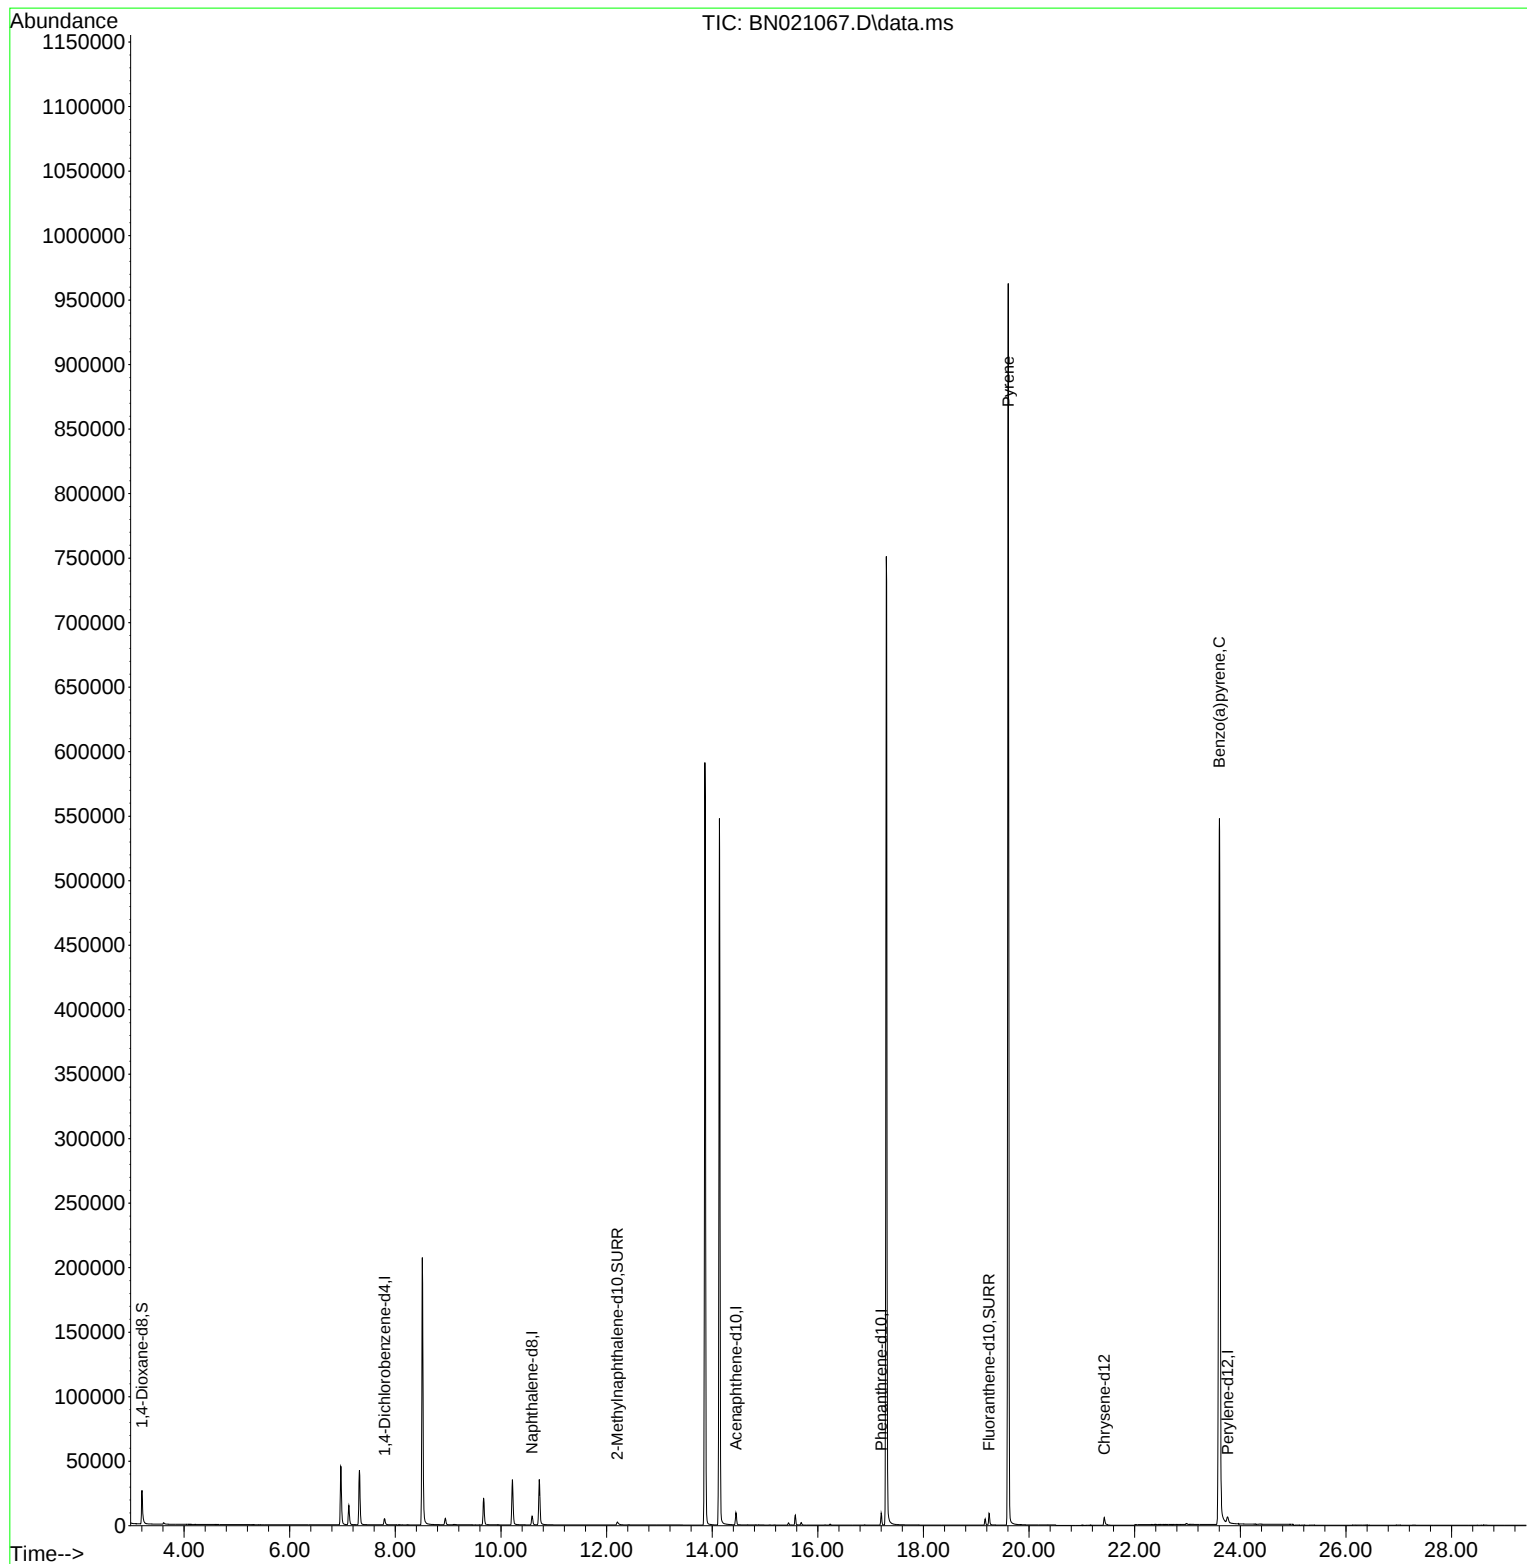


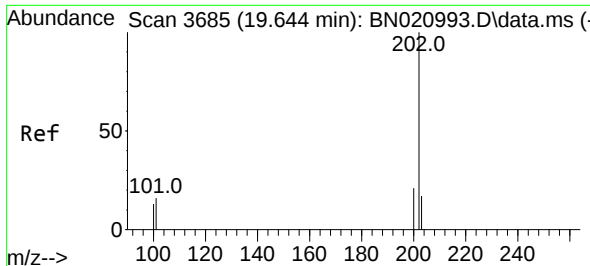

#20
Pyrene
Concen: 0.042 ng/ul
RT: 19.605 min Scan# 30
Delta R.T. -0.032 min
Lab File: BN021067.D
Acq: 08 Aug 2022 17:02

Instrument :
BNA_N
ClientSampleId :

Tgt Ion:202 Resp: 1525
Ion Ratio Lower Upper
202 100
101 181.1 11.3 16.9#
100 1325.6 9.0 13.4#

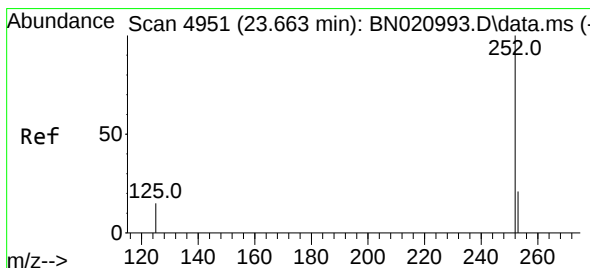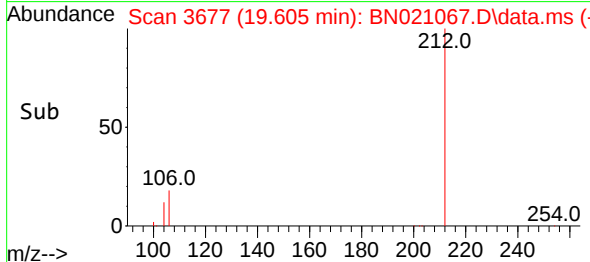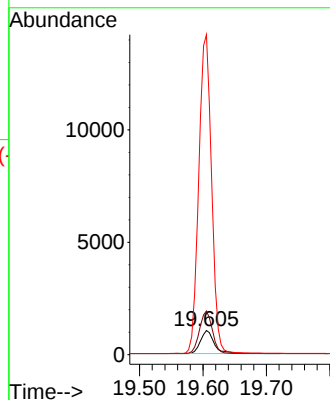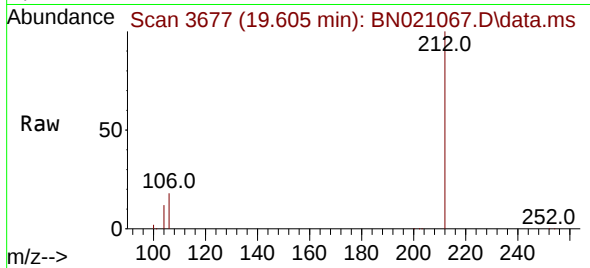

#26
Benzo(a)pyrene
Concen: 0.086 ng/ul
RT: 23.602 min Scan# 4930
Delta R.T. -0.064 min
Lab File: BN021067.D
Acq: 08 Aug 2022 17:02

Tgt Ion:252 Resp: 2995
Ion Ratio Lower Upper
252 100
253 42.8 22.1 33.1#
125 33.6 14.7 22.1#

