

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080822\
 Data File : BN021068.D
 Acq On : 08 Aug 2022 17:40
 Operator : CG/JU
 Sample : PB146835BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Aug 08 23:11:18 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 08 23:08:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.797	152	2798	0.400	ng/ul	0.00
4) Naphthalene-d8	10.591	136	9223	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.452	164	5306	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.201	188	10392	0.400	ng/ul	0.00
17) Chrysene-d12	21.430	240	7487	0.400	ng/ul	0.00
23) Perylene-d12	23.763	264	7868	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.207	96	16851	4.708	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.208	152	4243	0.314	ng/ul	0.02
18) Fluoranthene-d10	19.245	212	10307	0.446	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.607	202	1485	0.043	ng/ul#	1
26) Benzo(a)pyrene	23.605	252	2851	0.086	ng/ul#	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080822\
Data File : BN021068.D
Acq On : 08 Aug 2022 17:40
Operator : CG/JU
Sample : PB146835BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Aug 08 23:11:18 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 08 23:08:49 2022
Response via : Initial Calibration




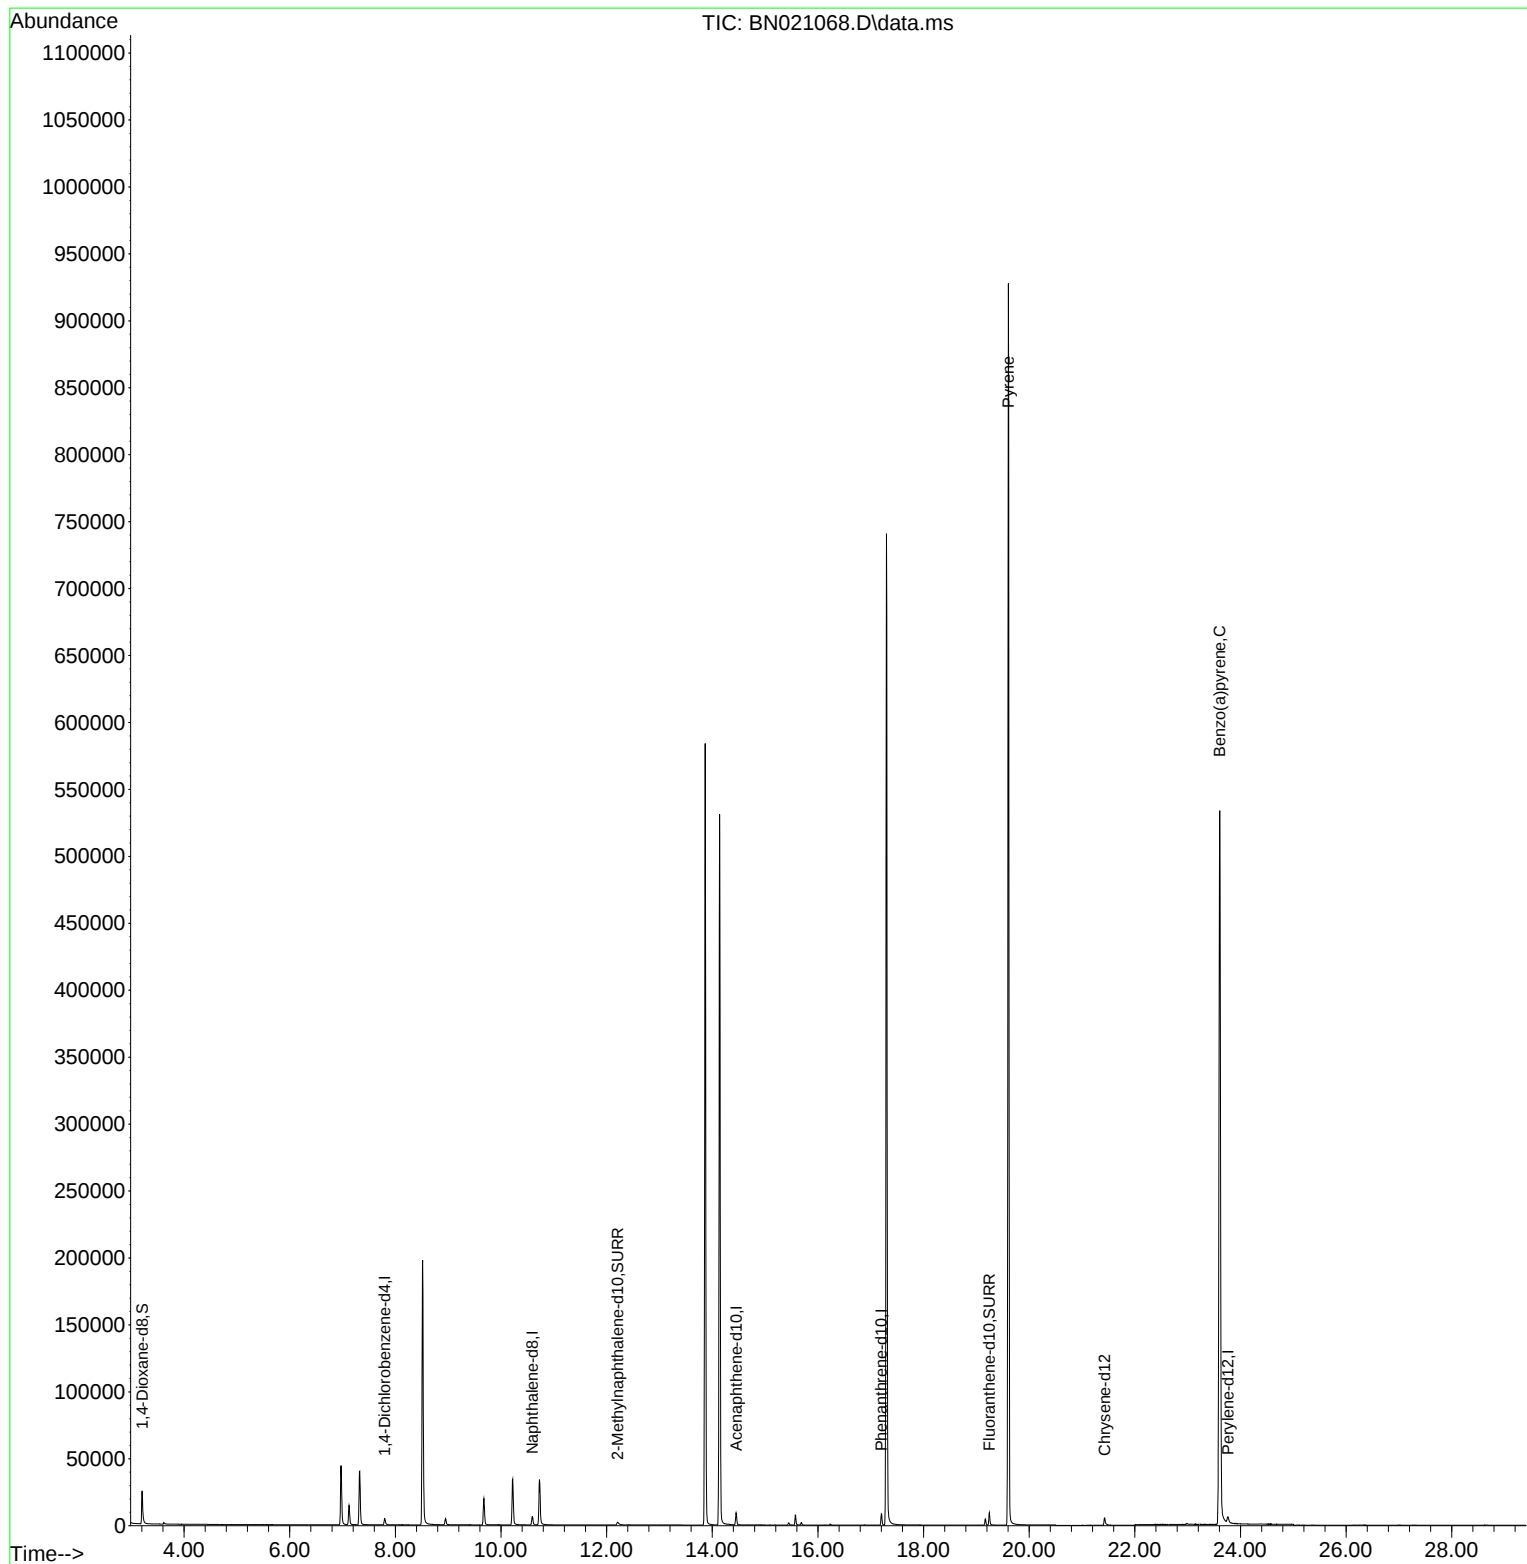


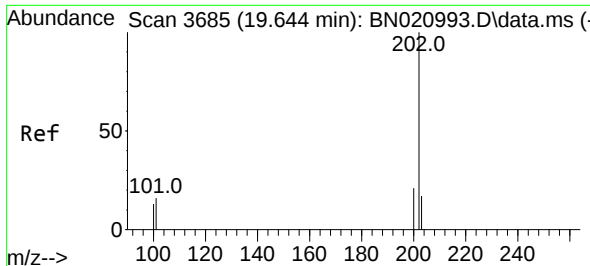

#20
Pyrene
Concen: 0.043 ng/ul
RT: 19.607 min Scan# 30
Delta R.T. -0.031 min
Lab File: BN021068.D
Acq: 08 Aug 2022 17:40

Instrument :
BNA_N
ClientSampleId :

Tgt Ion:202 Resp: 1485
Ion Ratio Lower Upper
202 100
101 182.2 11.3 16.9#
100 1331.4 9.0 13.4#

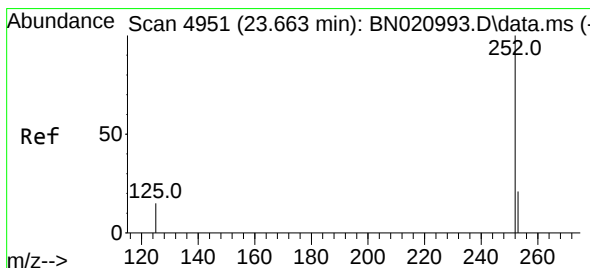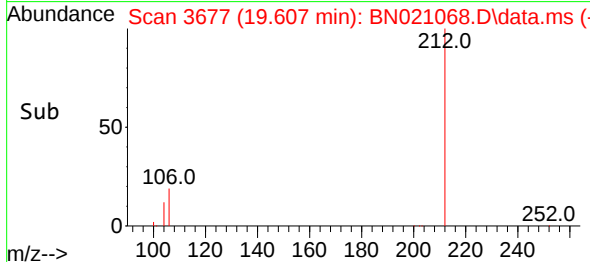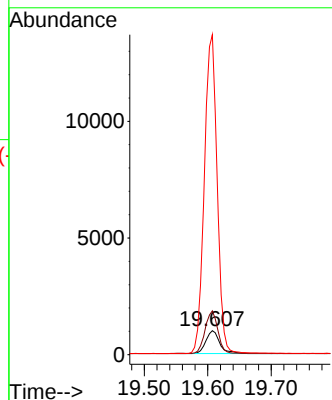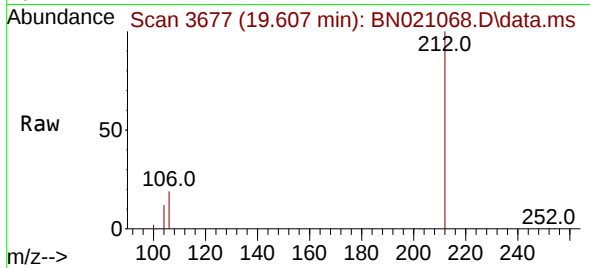

#26
Benzo(a)pyrene
Concen: 0.086 ng/ul
RT: 23.605 min Scan# 4931
Delta R.T. -0.061 min
Lab File: BN021068.D
Acq: 08 Aug 2022 17:40

Tgt Ion:252 Resp: 2851
Ion Ratio Lower Upper
252 100
253 43.2 22.1 33.1#
125 32.9 14.7 22.1#

