

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080822\
 Data File : BN021069.D
 Acq On : 08 Aug 2022 18:19
 Operator : CG/JU
 Sample : N4069-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Aug 08 23:11:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 08 23:08:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.801	152	2682	0.400	ng/ul	0.01
4) Naphthalene-d8	10.591	136	8614	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.452	164	5079	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.201	188	10149	0.400	ng/ul	0.00
17) Chrysene-d12	21.424	240	7482	0.400	ng/ul	0.00
23) Perylene-d12	23.757	264	7616	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.207	96	14440	4.208	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.202	152	4209	0.333	ng/ul	0.01
18) Fluoranthene-d10	19.245	212	9689	0.419	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.607	202	1517	0.044	ng/ul#	1
26) Benzo(a)pyrene	23.605	252	2596	0.081	ng/ul#	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080822\
Data File : BN021069.D
Acq On : 08 Aug 2022 18:19
Operator : CG/JU
Sample : N4069-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Aug 08 23:11:28 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 08 23:08:49 2022
Response via : Initial Calibration




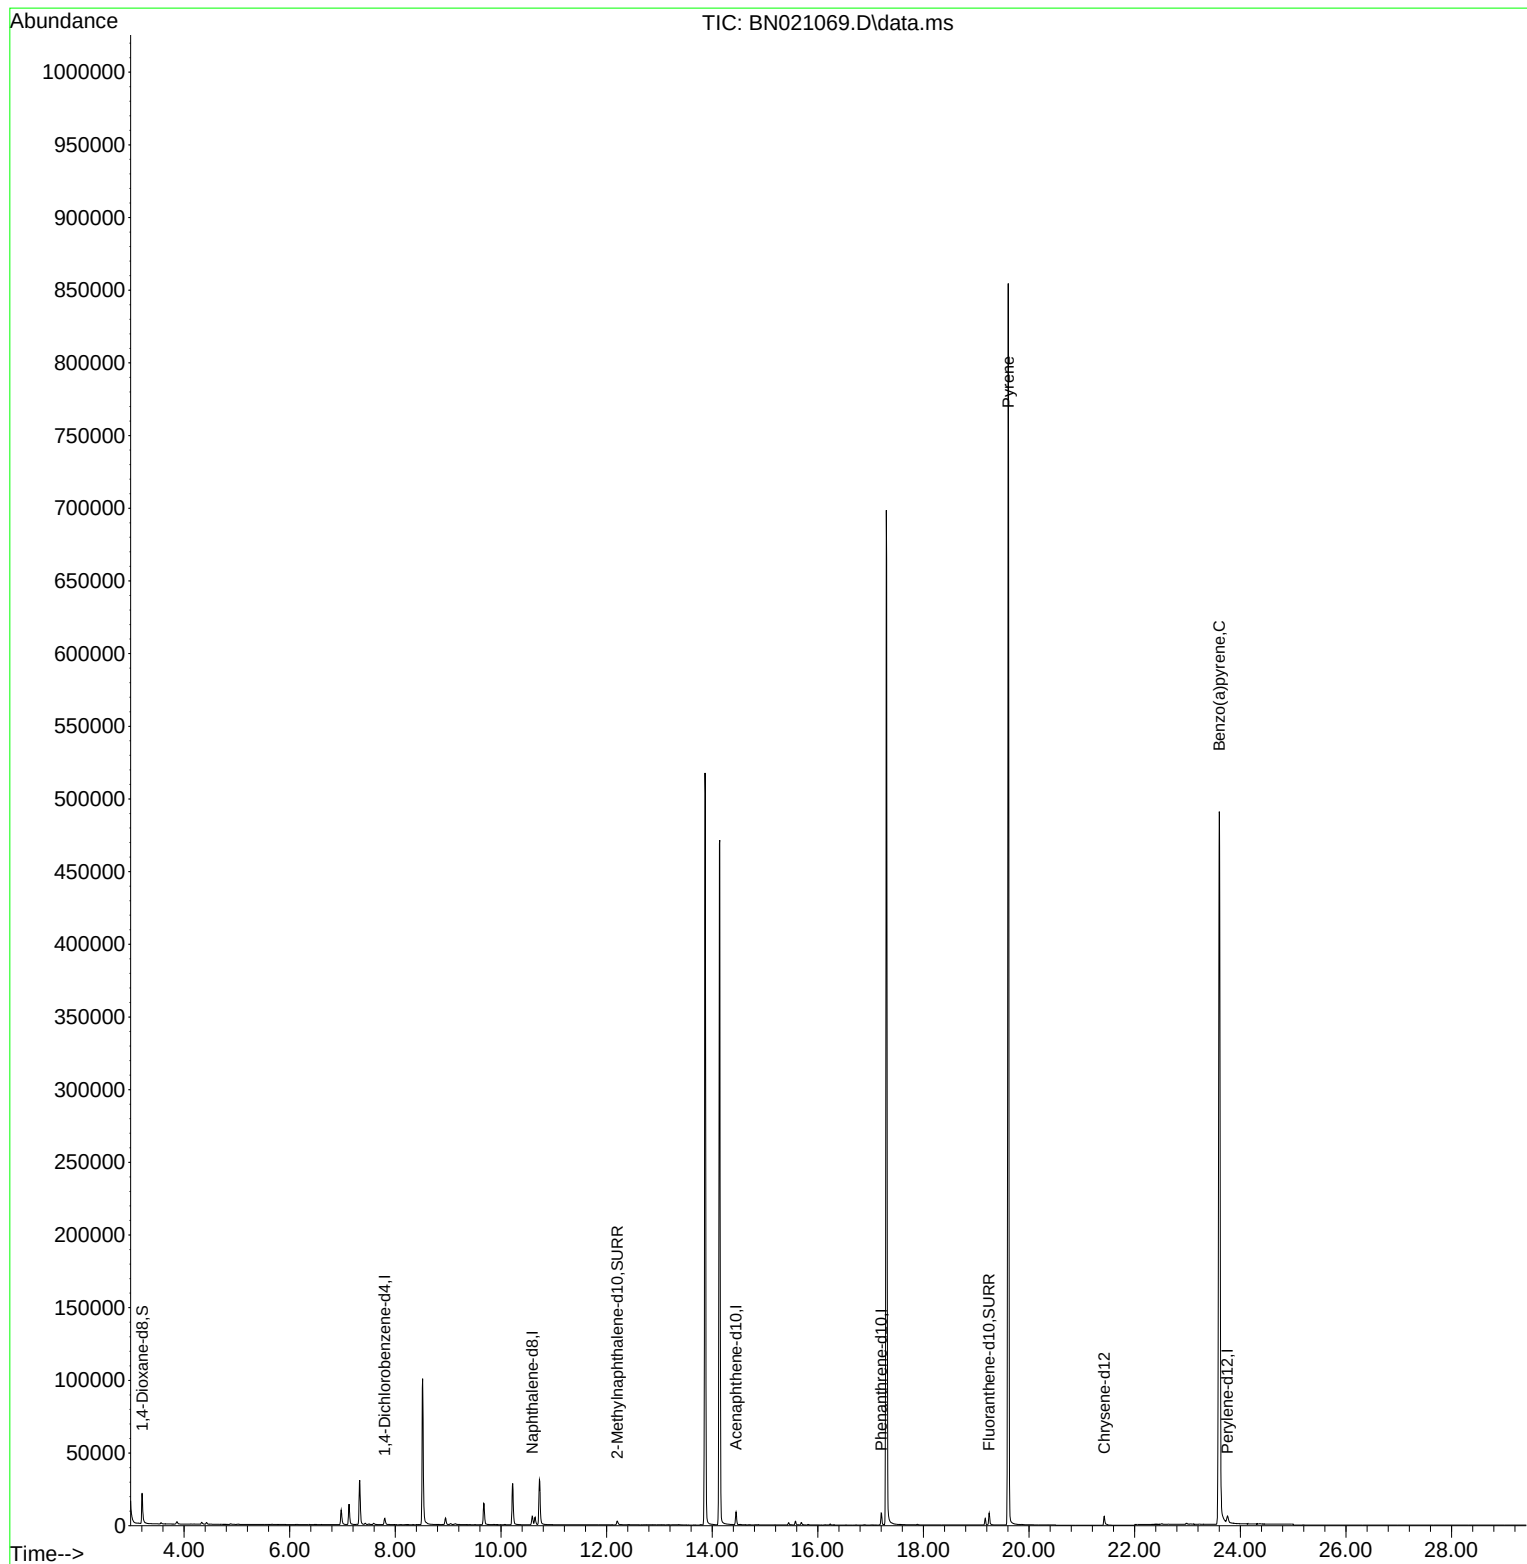


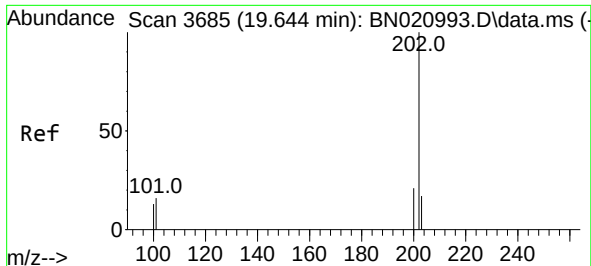

#20
Pyrene
Concen: 0.044 ng/ul
RT: 19.607 min Scan# 3677
Delta R.T. -0.031 min
Lab File: BN021069.D
Acq: 08 Aug 2022 18:19

Instrument :
BNA_N
ClientSampleId :

Tgt Ion:202 Resp: 1517
Ion Ratio Lower Upper
202 100
101 176.9 11.3 16.9#
100 1287.5 9.0 13.4#

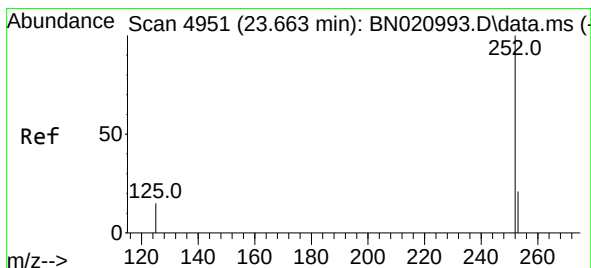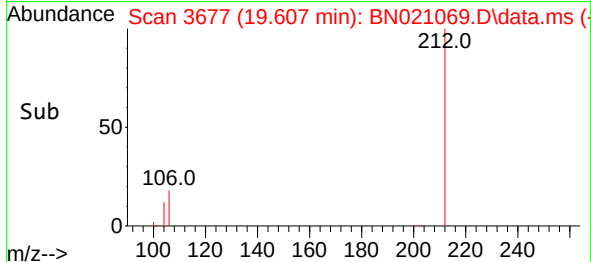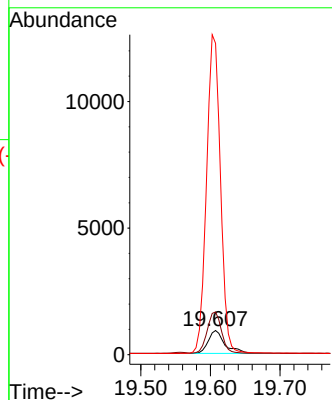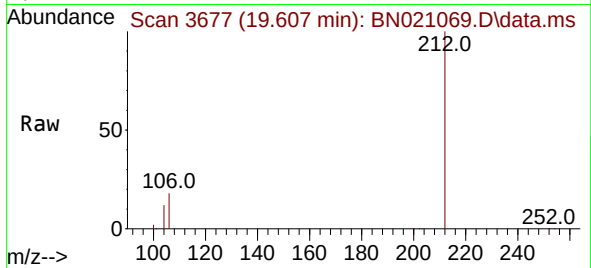

#26
Benzo(a)pyrene
Concen: 0.081 ng/ul
RT: 23.605 min Scan# 4931
Delta R.T. -0.061 min
Lab File: BN021069.D
Acq: 08 Aug 2022 18:19

Tgt Ion:252 Resp: 2596
Ion Ratio Lower Upper
252 100
253 46.2 22.1 33.1#
125 33.6 14.7 22.1#

