
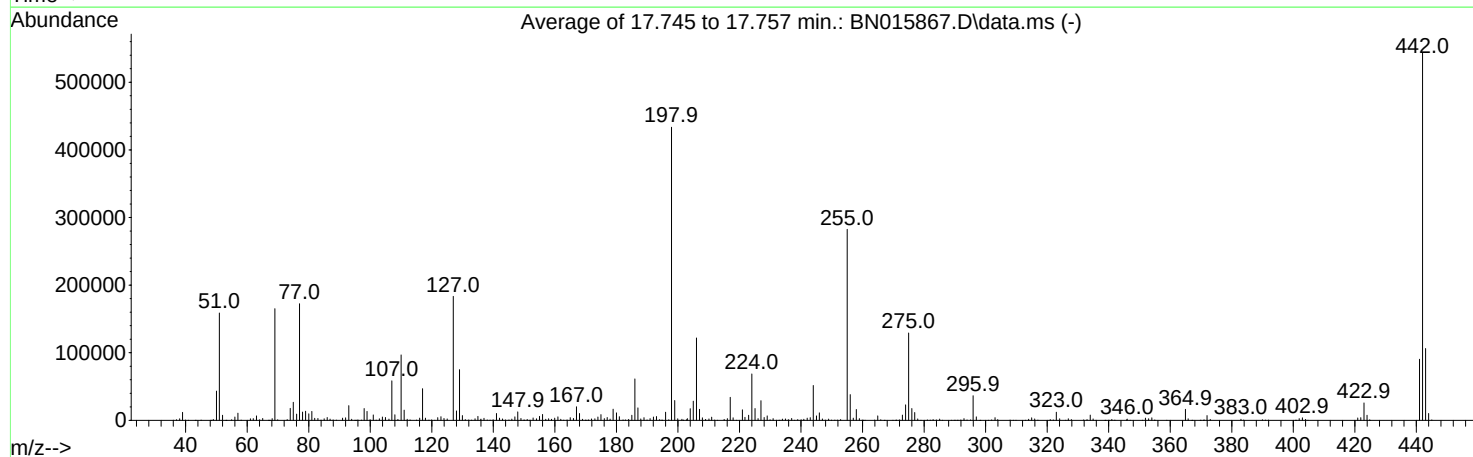


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081321\
 Data File : BN015867.D
 Acq On : 13 Aug 2021 07:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN081221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 13 18:43:52 2021

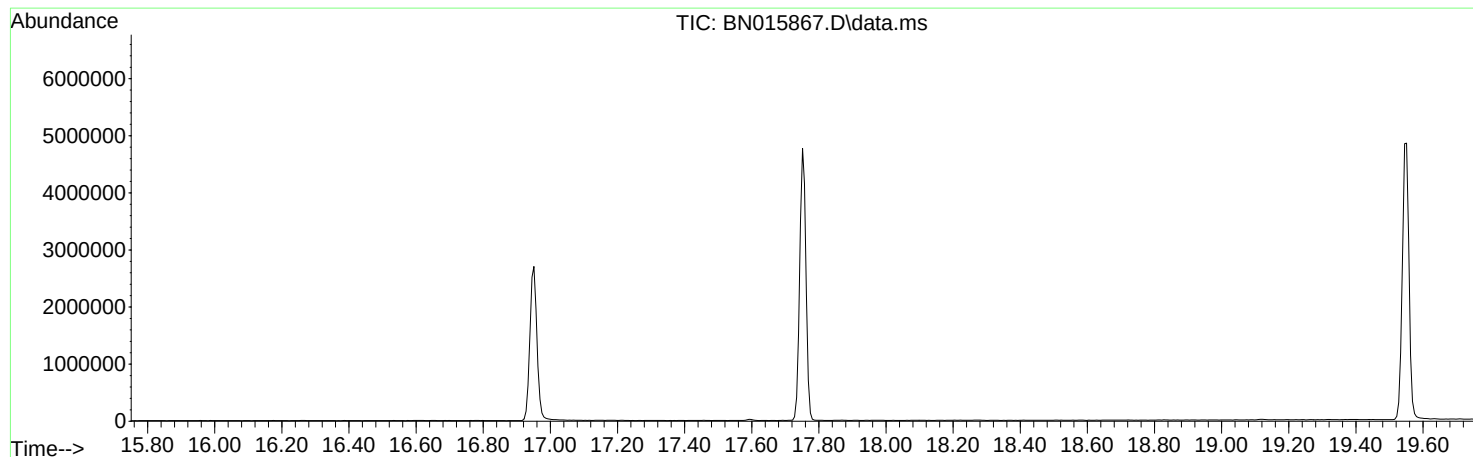

AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.7	158911	PASS
68	69	0.00	2	1.5	2542	PASS
69	198	0.00	100	38.1	165141	PASS
70	69	0.00	2	0.6	917	PASS
127	198	10	80	42.3	183339	PASS
197	198	0.00	2	0.2	920	PASS
198	198	100	100	100.0	433429	PASS
199	198	5	9	6.8	29323	PASS
275	198	10	60	29.8	129275	PASS
365	198	1	100	3.8	16312	PASS
441	198	0.01	100	20.8	90355	PASS
442	442	50	100	100.0	544021	PASS
443	442	15	24	19.5	106221	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/13/2021	BNA_N	<u>BN015867.D</u>
Compound Name	Response	Retention Time
DDT	1542976	20.792
DDD	17140	20.345
DDE	2672	19.839
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19812	1562788	1.27

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081321\
Data File : BN015867.D
Acq On : 13 Aug 2021 07:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 13 13:18:41 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 11 11:23:50 2021
Response via : Initial Calibration

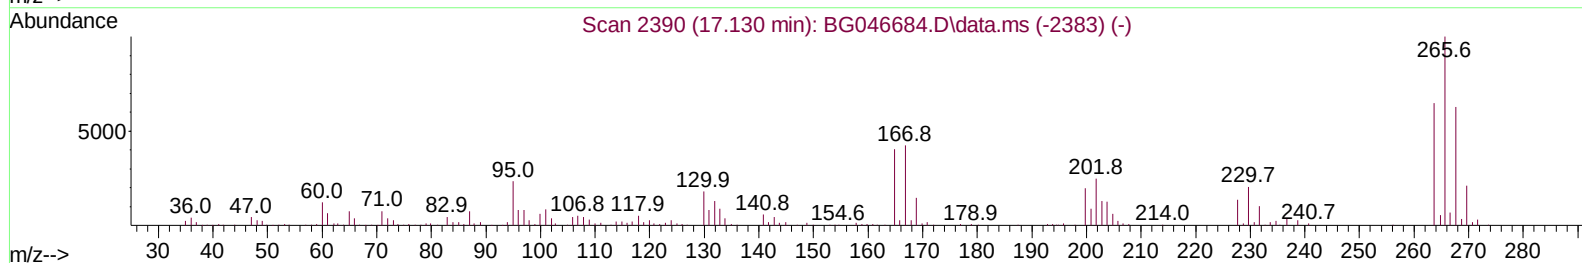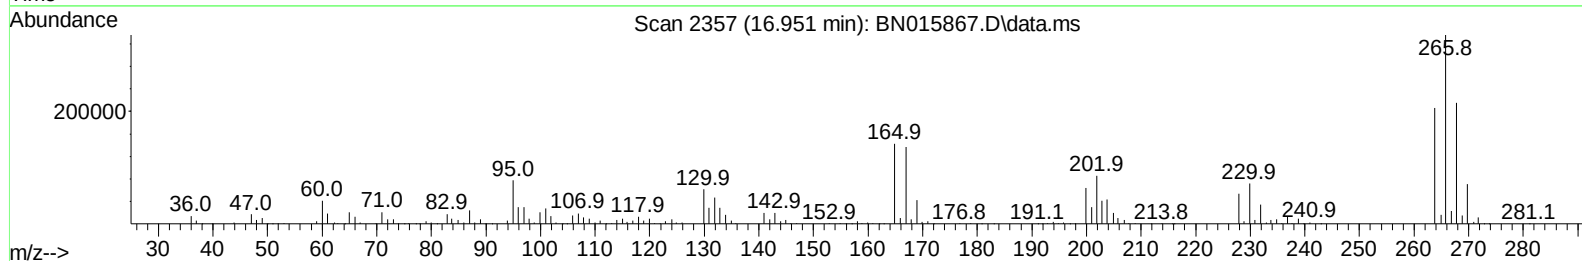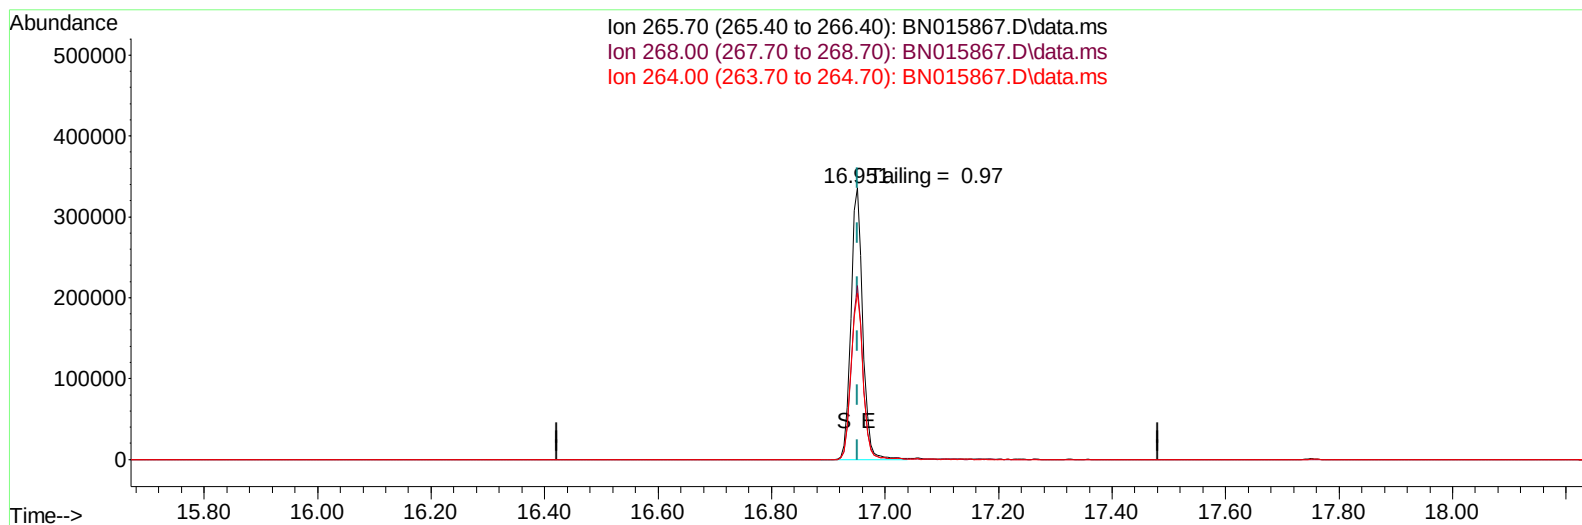

TIC: BN015867.D\data.ms

(70) Pentachlorophenol (C)

16.951min (-0.000) 19551.64 ng




response 489155

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.05
264.00	61.60	61.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081321\
Data File : BN015867.D
Acq On : 13 Aug 2021 07:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 13 13:18:41 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 11 11:23:50 2021
Response via : Initial Calibration

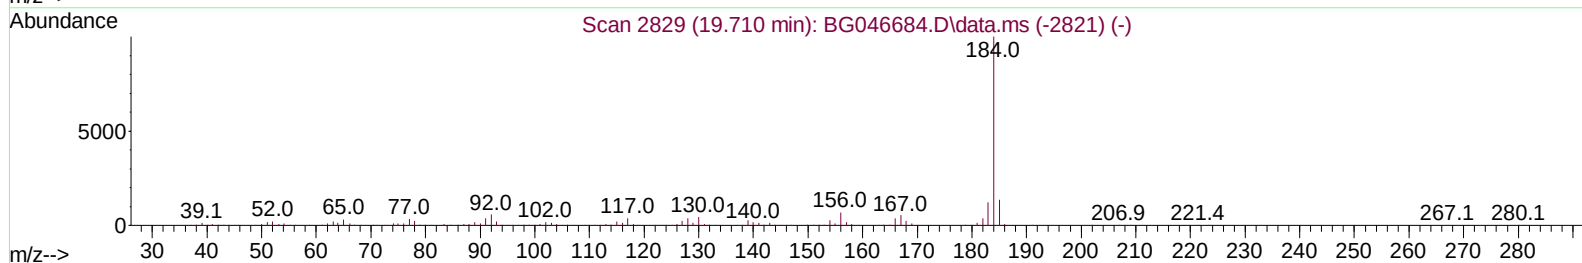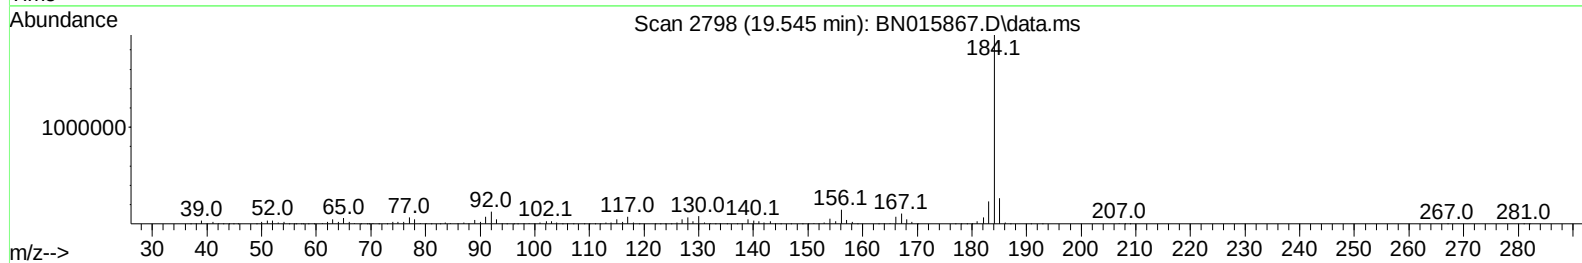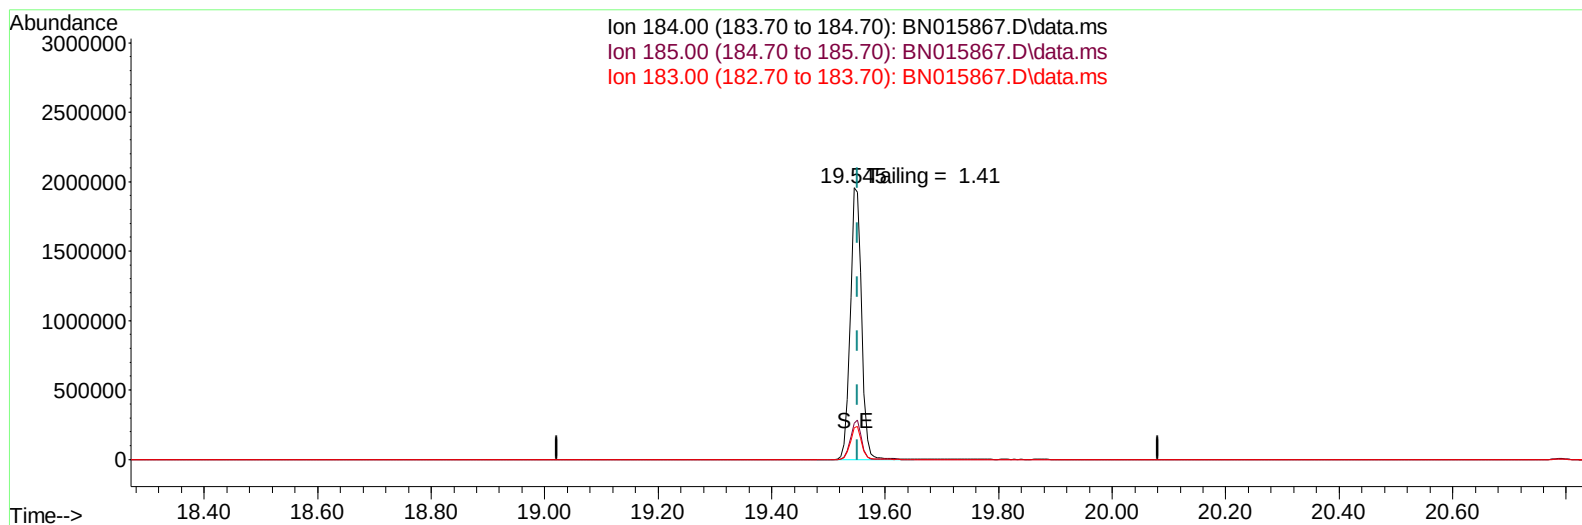

TIC: BN015867.D\data.ms

(77) Benzidine

19.545min (-0.006) 0.00 ng

response 2722937

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.42
183.00	13.20	11.81
0.00	0.00	0.00