
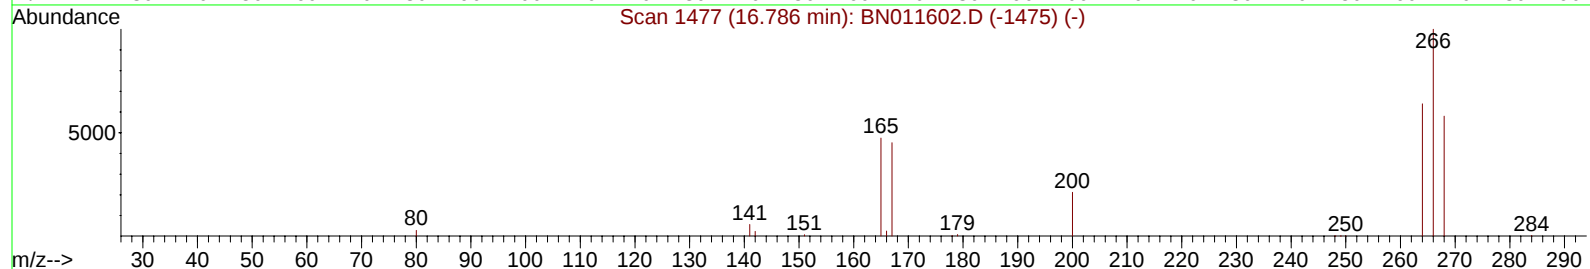
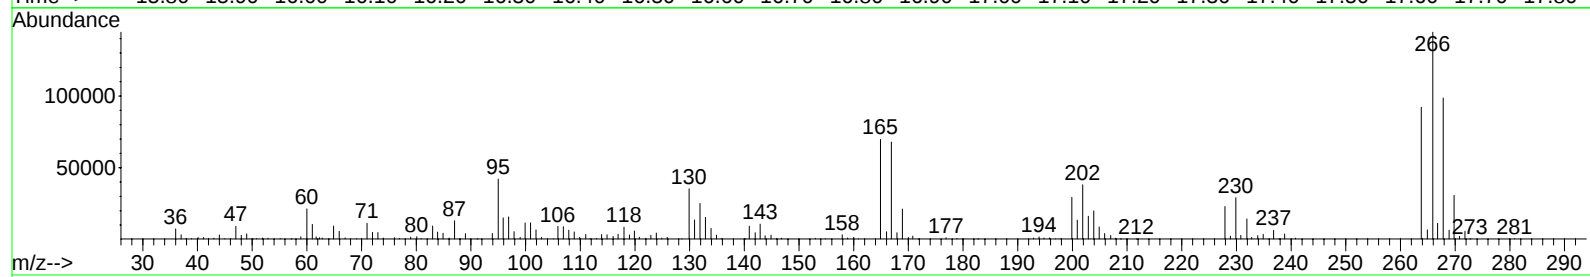


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082620\
 Data File : BN011643.D
 Acq On : 26 Aug 2020 13:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 26 18:32:00 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN082420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 25 03:31:11 2020
 Response via : Initial Calibration

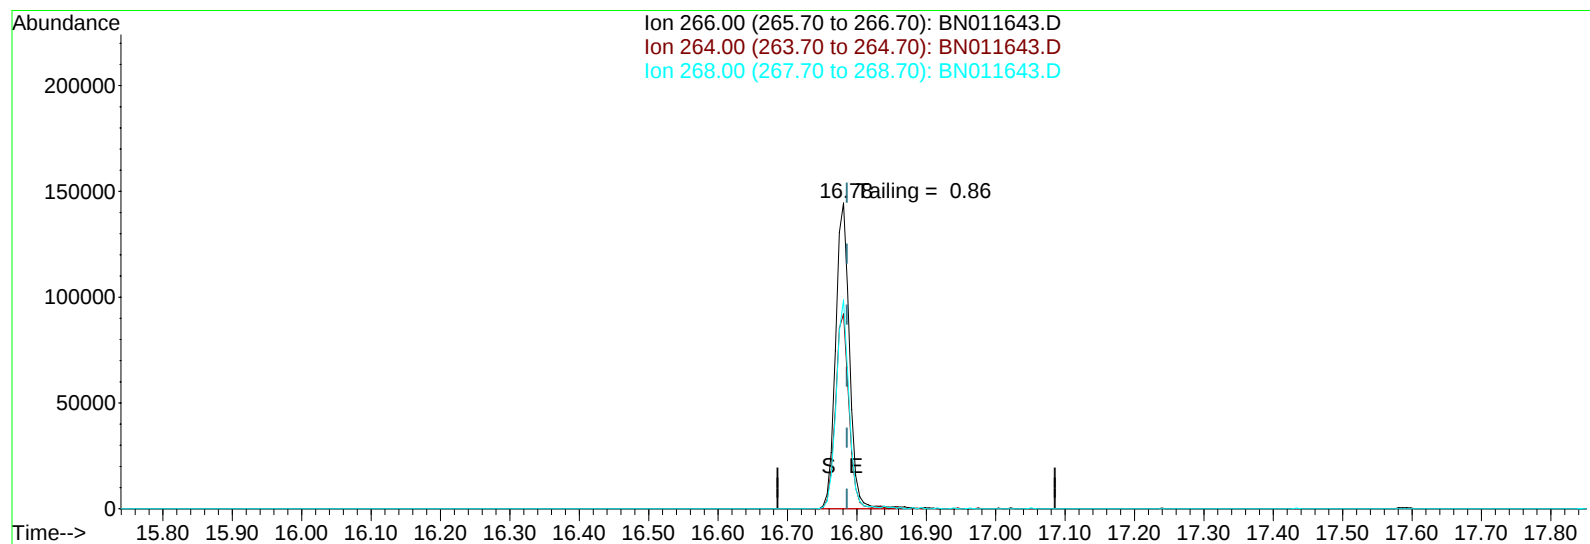

TIC: BN011643.D

(24) Pentachlorophenol

16.781min (-0.005) 0.00ng

response 200327

Ion	Exp%	Act%
266.00	100	100
264.00	60.10	61.79
268.00	60.50	63.20
0.00	0.00	0.00