

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082620\
 Data File : BN011652.D
 Acq On : 26 Aug 2020 19:21
 Operator : CG/JU
 Sample : L3783-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BP-VPB181-GW-518-520

Quant Time: Aug 27 00:25:41 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN082420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 25 03:31:11 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	2577	0.40	ng	-0.02
7) Naphthalene-d8	10.53	136	10471	0.40	ng	-0.01
13) Acenaphthene-d10	14.38	164	6275	0.40	ng	-0.01
19) Phenanthrene-d10	17.13	188	13739	0.40	ng	-0.01
29) Chrysene-d12	21.32	240	15463	0.40	ng	-0.01
36) Perylene-d12	23.58	264	16669	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.34	112	1115	0.14	ng	0.00
5) Phenol-d6	6.91	99	989	0.08	ng	0.00
8) Nitrobenzene-d5	8.88	82	2522	0.28	ng	-0.03
11) 2-Methylnaphthalene-d10	12.13	152	4512	0.23	ng	-0.01
14) 2,4,6-Tribromophenol	15.88	330	904	0.26	ng	0.00
15) 2-Fluorobiphenyl	13.01	172	6449	0.26	ng	-0.01
27) Fluoranthene-d10	19.17	212	14347	0.32	ng	0.00
31) Terphenyl-d14	19.77	244	12944	0.33	ng	-0.01
Target Compounds						Qvalue
34) Bis(2-ethylhexyl)phthalate	21.26	149	13685	0.354	ng	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082620\
Data File : BN011652.D
Acq On : 26 Aug 2020 19:21
Operator : CG/JU
Sample : L3783-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BP-VPB181-GW-518-520

Quant Time: Aug 27 00:25:41 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN082420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 25 03:31:11 2020
Response via : Initial Calibration

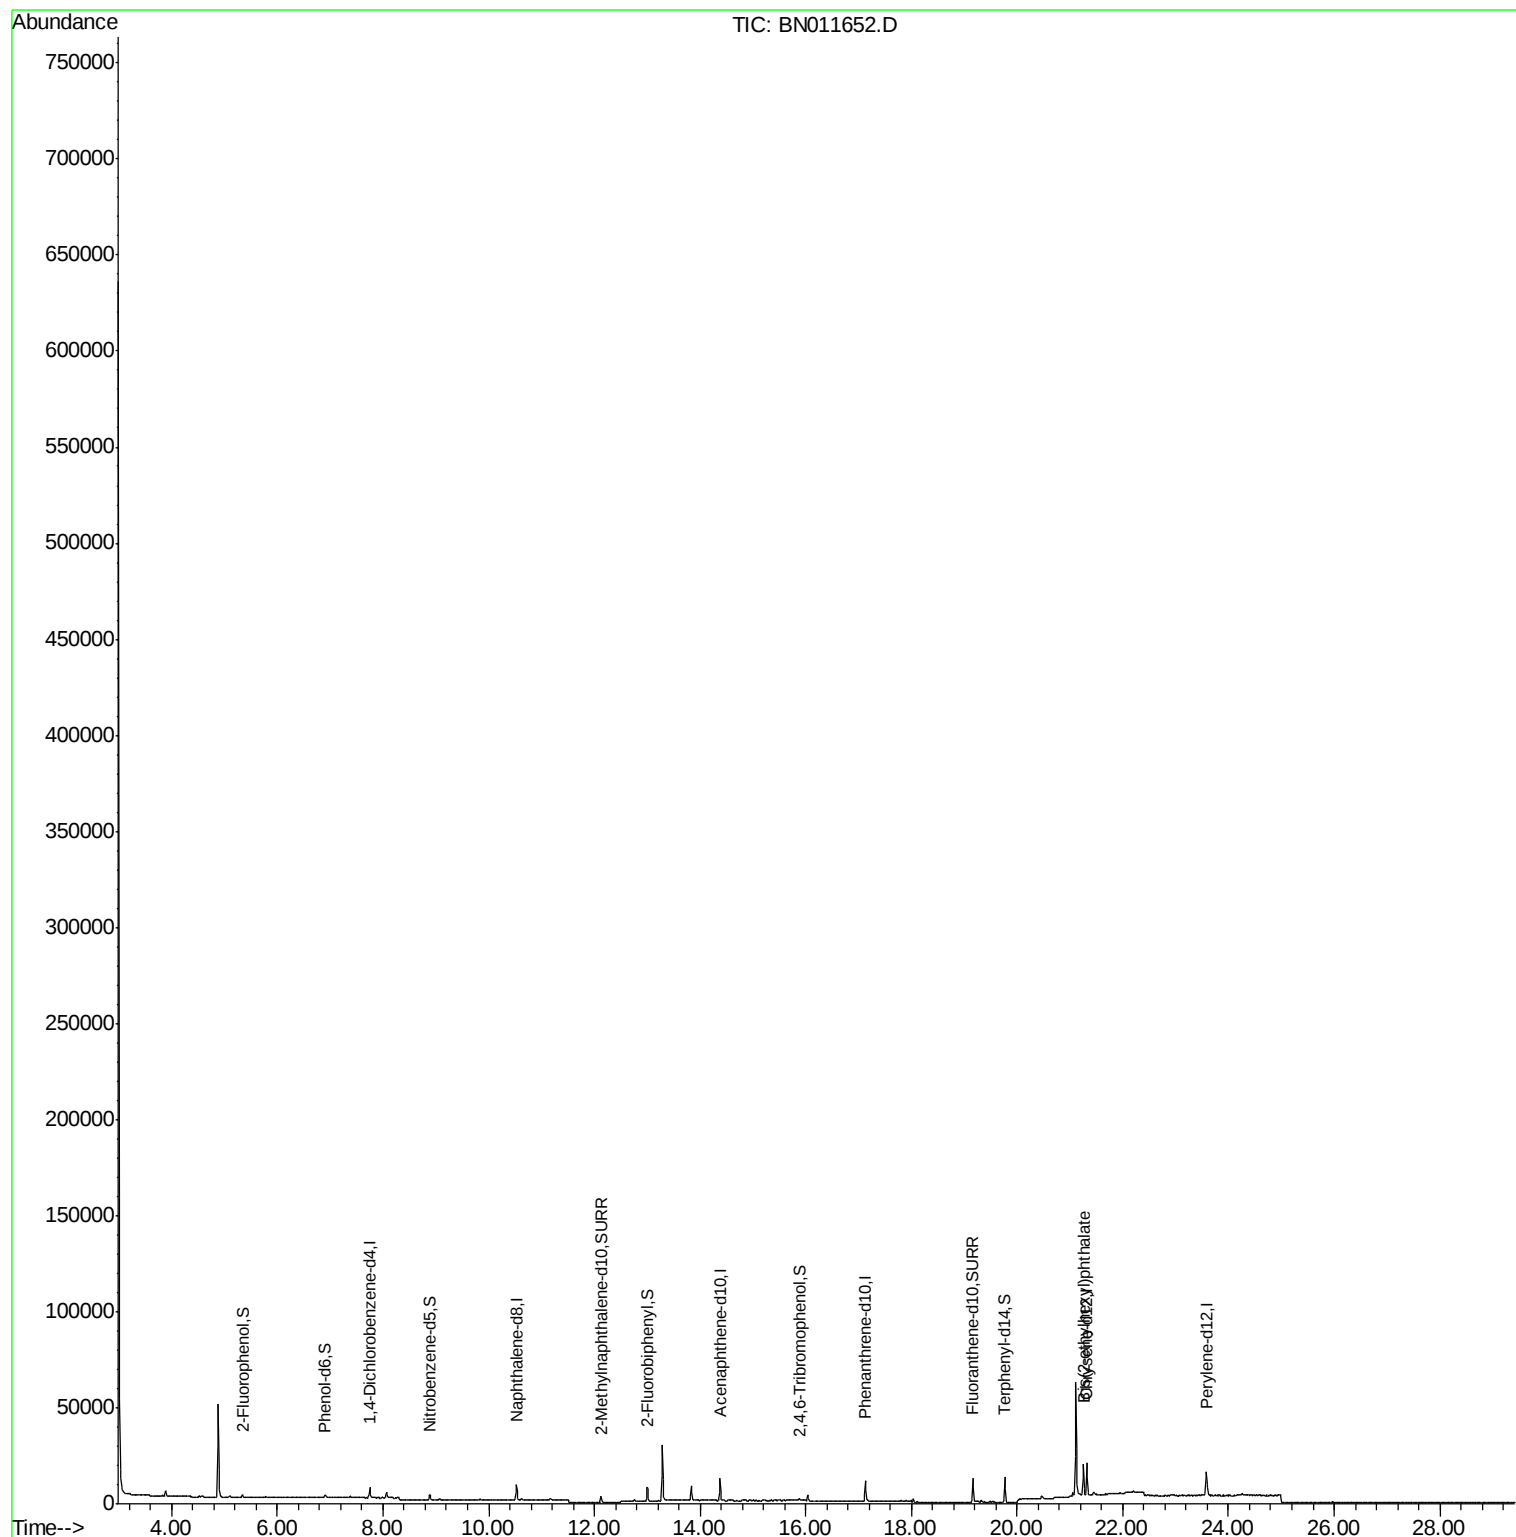

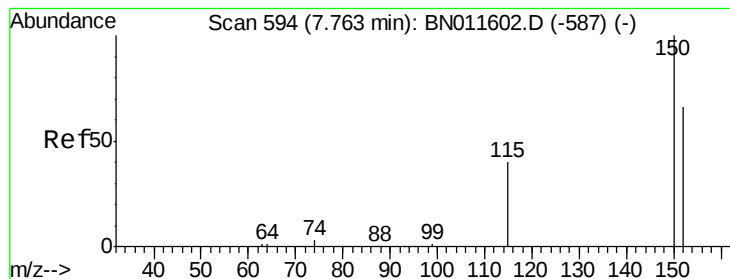


#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.75 min Scan# 592
Delta R.T. -0.02 min
Lab File: BN011652.D
Acq: 26 Aug 2020 19:21

Instrument :
BNA_N
ClientSampleId :
BP-VPB181-GW-518-520

Tot Ion:152 Resp: 2577
Ion Ratio Lower Upper
152 100
150 156.9 112.4 168.6
115 67.2 56.9 85.3

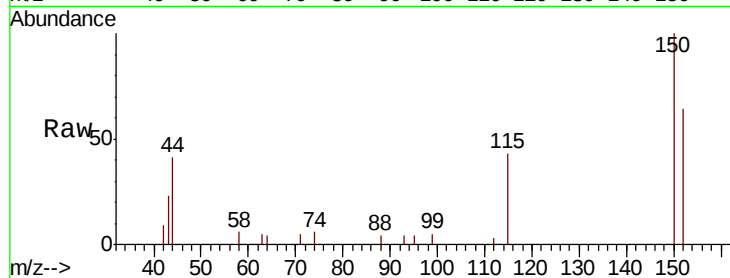


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

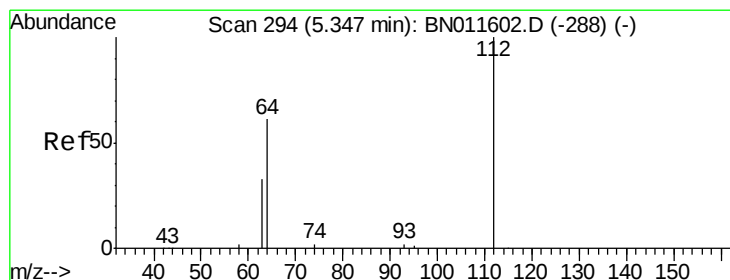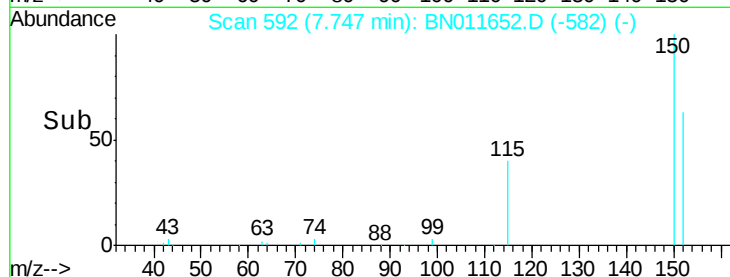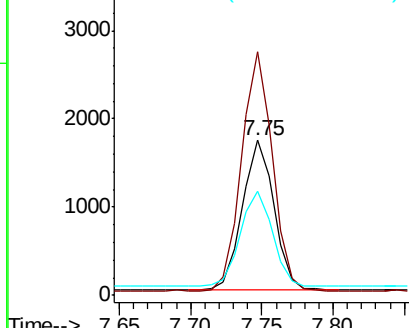



#4


2-Fluorophenol
Concen: 0.135 ng
RT: 5.34 min Scan# 293
Delta R.T. -0.01 min
Lab File: BN011652.D
Acq: 26 Aug 2020 19:21

Tgt Ion:112 Resp: 1115
Ion Ratio Lower Upper
112 100
64 61.9 49.6 74.4
63 32.8 26.4 39.6

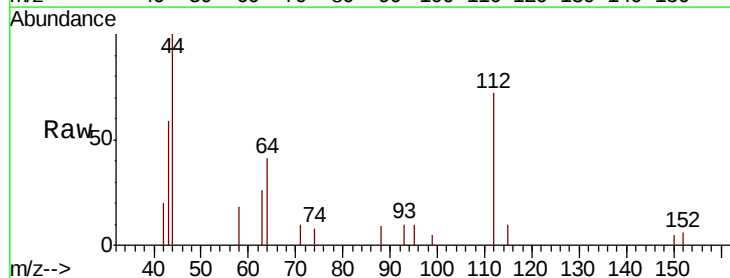

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BNC
Ion 63.00 (62.70 to 63.70): BNC

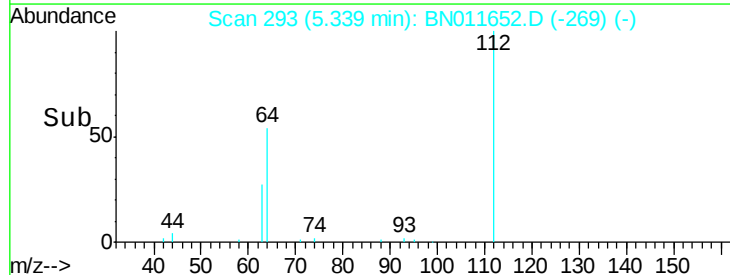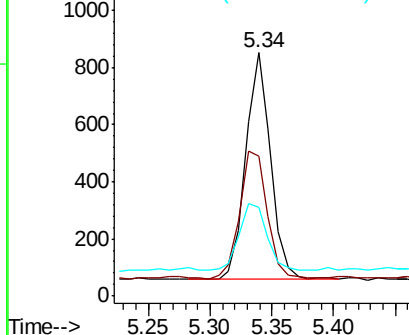

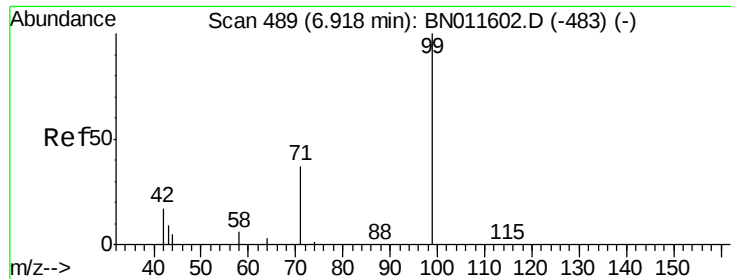

#5

Phenol-d6

Concen: 0.085 ng

RT: 6.91 min Scan# 488

Delta R.T. -0.01 min

Lab File: BN011652.D

Acq: 26 Aug 2020 19:21

Instrument :

BNA_N

ClientSampleId :

BP-VPB181-GW-518-520


Tot Ion: 99 Resp: 989

Ion Ratio Lower Upper

99 100

42 25.2 0.0 0.0#

71 43.2 0.0 0.0#



Abundance Ion 99.00 (98.70 to 99.70): BN011602.D (-483) (-)

Ion 42.00 (41.70 to 42.70): BN011602.D (-483) (-)

Ion 71.00 (70.70 to 71.70): BN011602.D (-483) (-)

6.91

800

600



400

200

0

6.80 6.85 6.90 6.95 7.00

Time-->



#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.53 min Scan# 837

Delta R.T. -0.01 min

Lab File: BN011652.D

Acq: 26 Aug 2020 19:21

Tgt Ion: 136 Resp: 10471


Ion Ratio Lower Upper

136 100

137 11.7 11.5 17.3

54 8.2 11.9 17.9#

68 6.6 12.3 18.5#



Abundance Ion 136.00 (135.70 to 136.70): BN011602.D (-832) (-)

Ion 137.00 (136.70 to 137.70): BN011602.D (-832) (-)

Ion 54.00 (53.70 to 54.70): BN011602.D (-832) (-)

Ion 68.00 (67.70 to 68.70): BN011602.D (-832) (-)

10.53

10000

8000

6000


4000


2000

0

10.40 10.50 10.60

Time-->









#8
 Nitrobenzene-d5
 Concen: 0.278 ng
 RT: 8.88 min Scan# 707
 Delta R.T. -0.03 min
 Lab File: BN011652.D
 Acq: 26 Aug 2020 19:21

Instrument :
 BNA_N
 ClientSampleId :
 BP-VPB181-GW-518-520

Tot Ion	Ratio	Lower	Upper
82	100		
128	34.1	31.1	46.7
54	60.2	37.1	55.7#

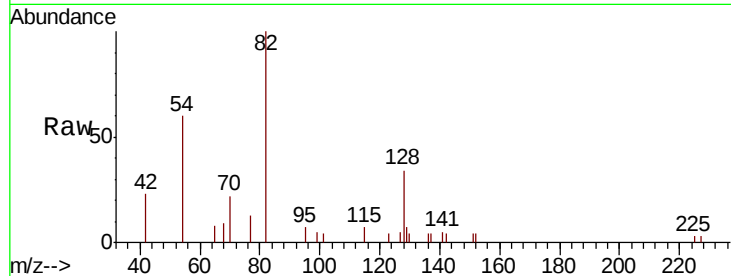


Abundance Ion 82.00 (81.70 to 82.70): BN0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BN0


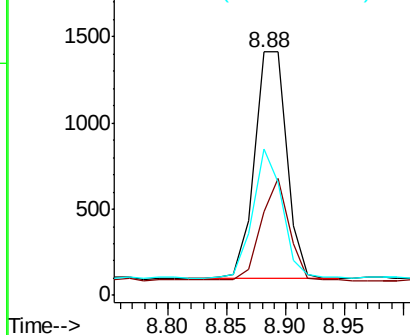



#11
 2-Methylnaphthalene-d10
 Concen: 0.228 ng
 RT: 12.13 min Scan# 1052
 Delta R.T. -0.01 min
 Lab File: BN011652.D
 Acq: 26 Aug 2020 19:21

Tgt Ion	Ratio	Lower	Upper
152	100		
151	20.7	16.4	24.6



Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 151.00 (150.70 to 151.70): E

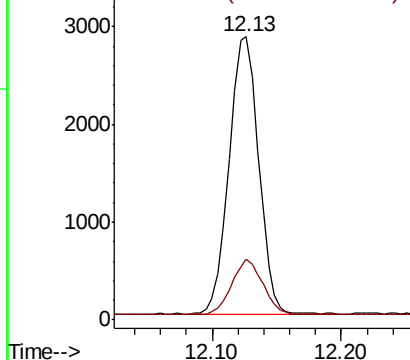



#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.38 min Scan# 1285

Delta R.T. -0.01 min

Lab File: BN011652.D

Acq: 26 Aug 2020 19:21

Instrument :

BNA_N

ClientSampleId :

BP-VPB181-GW-518-520


Tot Ion:164 Resp: 6275

Ion Ratio Lower Upper

164 100

162 103.2 80.8 121.2

160 46.6 35.6 53.4

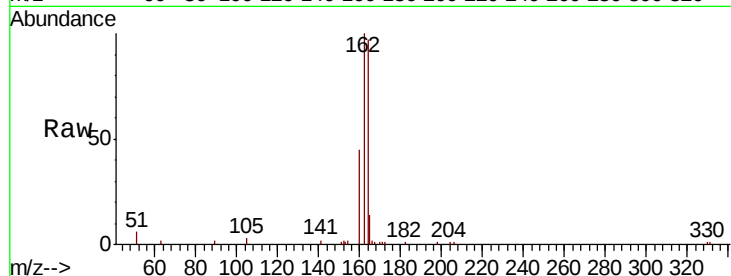



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

14.38

Time-->



#14

2,4,6-Tribromophenol

Concen: 0.262 ng

RT: 15.88 min Scan# 1403

Delta R.T. -0.00 min

Lab File: BN011652.D

Acq: 26 Aug 2020 19:21


Tgt Ion:330 Resp: 904

Ion Ratio Lower Upper

330 100

332 0.0 0.0 0.0

141 39.2 29.4 44.2




Abundance Ion 330.00 (329.70 to 330.70): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

15.88

Time-->









#15
 2-Fluorobiphenyl
 Concen: 0.264 ng
 RT: 13.01 min Scan# 1177
 Delta R.T. -0.01 min
 Lab File: BN011652.D
 Acq: 26 Aug 2020 19:21




Instrument :
 BNA_N
 ClientSampleId :
 BP-VPB181-GW-518-520


Tot Ion:172 Resp: 6449
 Ion Ratio Lower Upper
 172 100
 171 35.1 28.6 42.8
 170 22.0 18.2 27.2

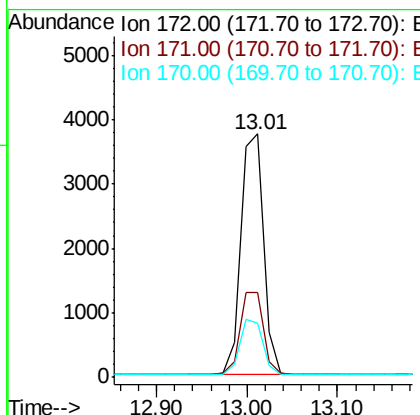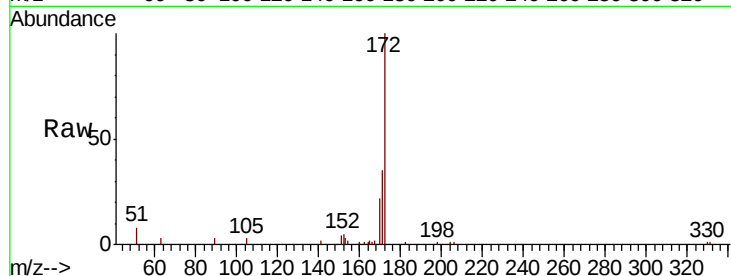

#19
 Phenanthrene-d10
 Concen: 0.400 ng
 RT: 17.13 min Scan# 1505
 Delta R.T. -0.01 min
 Lab File: BN011652.D
 Acq: 26 Aug 2020 19:21

Tgt Ion:188 Resp: 13739
 Ion Ratio Lower Upper
 188 100
 94 0.0 0.0 0.0
 80 9.4 9.2 13.8

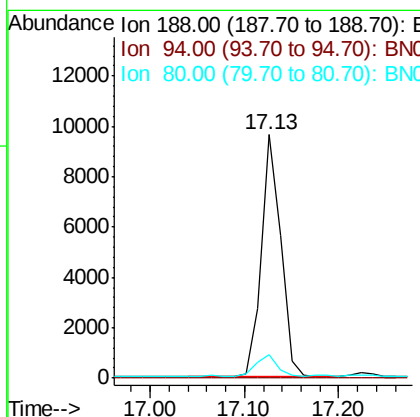

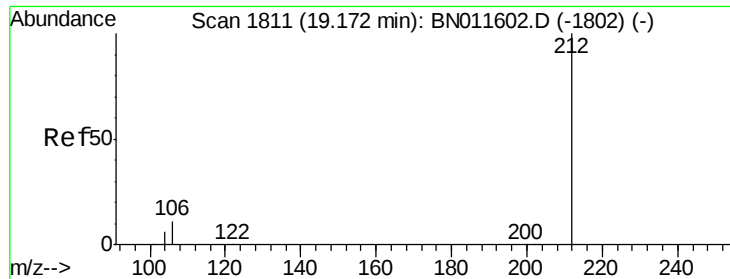

#27

Fluoranthene-d10

Concen: 0.320 ng

RT: 19.17 min Scan# 1810

Delta R.T. -0.01 min

Lab File: BN011652.D

Acq: 26 Aug 2020 19:21

Instrument :

BNA_N

ClientSampleId :

BP-VPB181-GW-518-520


Tot Ion:212 Resp: 14347

Ion Ratio Lower Upper

212 100

106 11.0 8.9 13.3




104 6.3 5.3 7.9

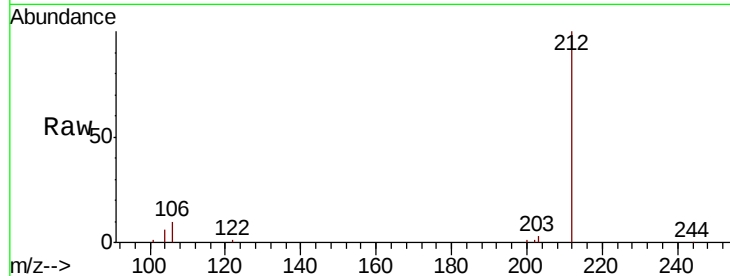

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

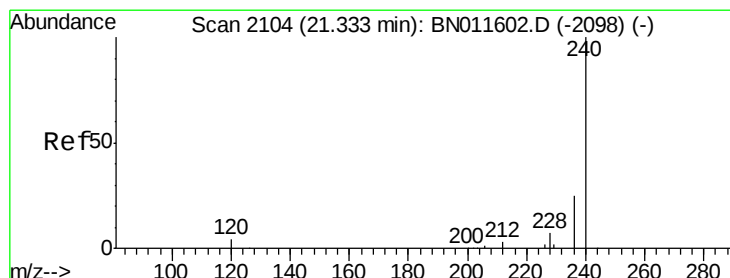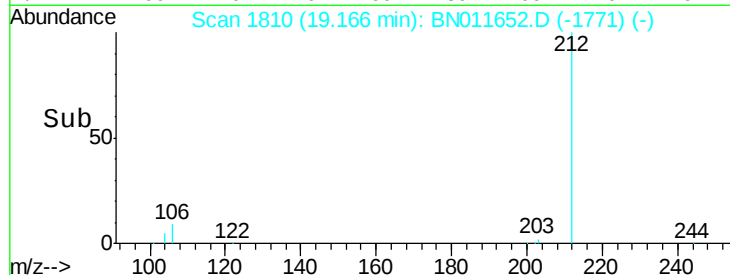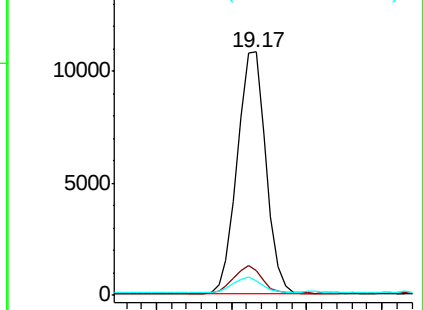

#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.32 min Scan# 2103

Delta R.T. -0.01 min

Lab File: BN011652.D

Acq: 26 Aug 2020 19:21


Tgt Ion:240 Resp: 15463

Ion Ratio Lower Upper

240 100

120 10.7 6.0 9.0#



236 27.1 20.8 31.2

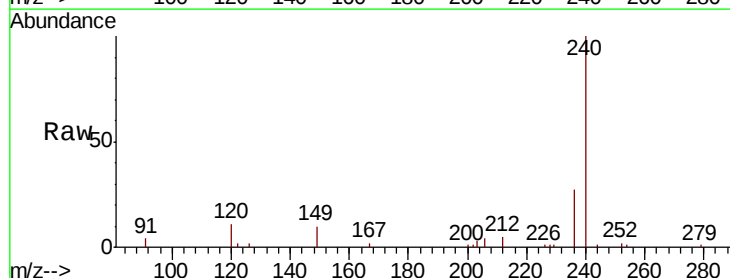


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

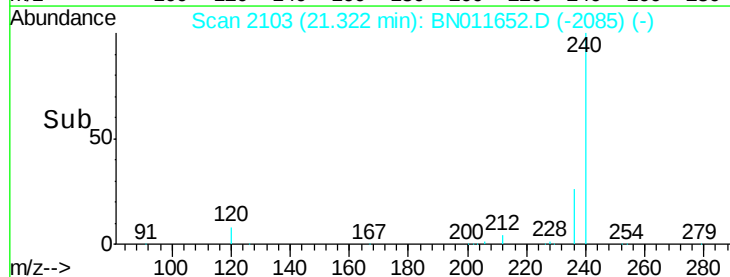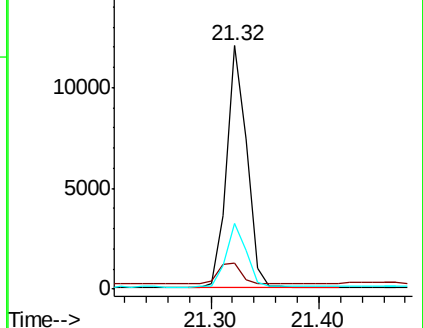

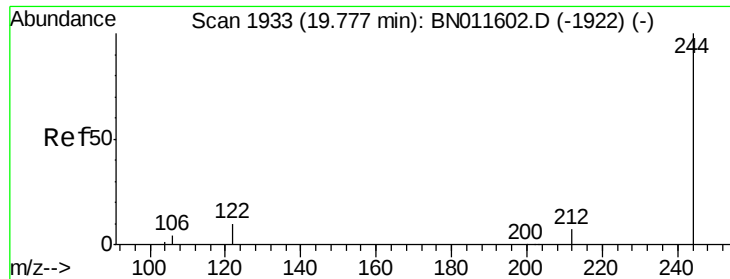

#31

Terphenyl-d14

Concen: 0.328 ng

RT: 19.77 min Scan# 1931

Delta R.T. -0.01 min

Lab File: BN011652.D

Acq: 26 Aug 2020 19:21

Instrument :

BNA_N

ClientSampleId :

BP-VPB181-GW-518-520


Tot Ion:244 Resp: 12944

Ion Ratio Lower Upper

244 100

212 8.5 6.5 9.7




122 11.5 9.5 14.3

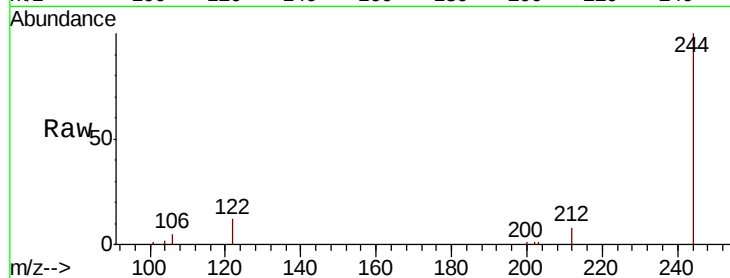

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

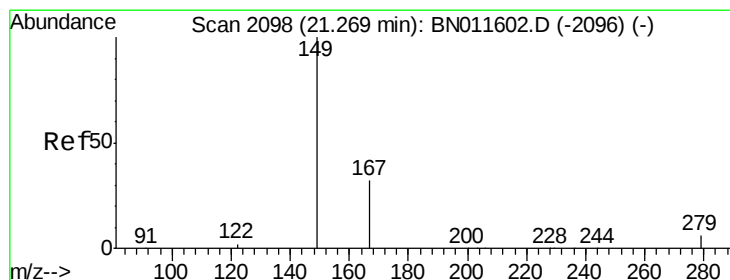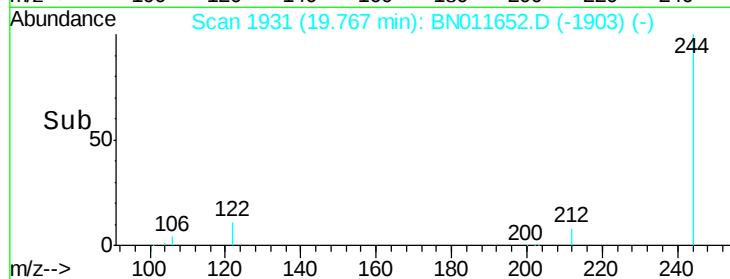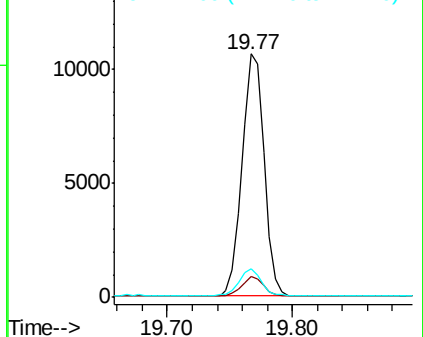

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.354 ng

RT: 21.26 min Scan# 2097

Delta R.T. -0.01 min

Lab File: BN011652.D

Acq: 26 Aug 2020 19:21


Tgt Ion:149 Resp: 13685

Ion Ratio Lower Upper

149 100

167 28.3 20.6 31.0



279 5.1 3.8 5.8



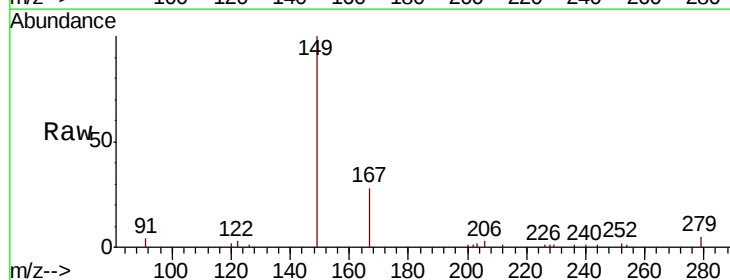


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

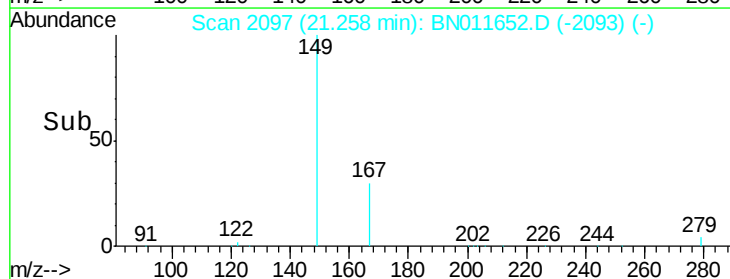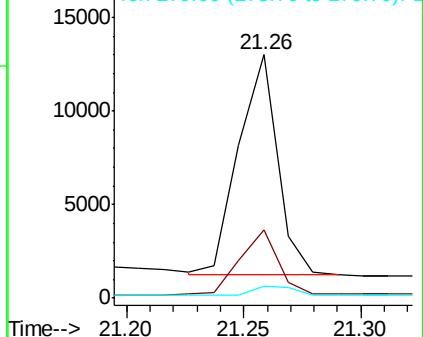

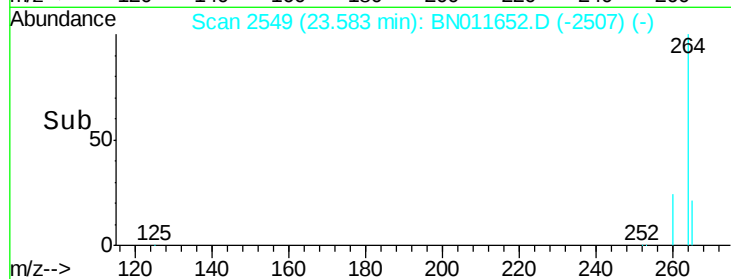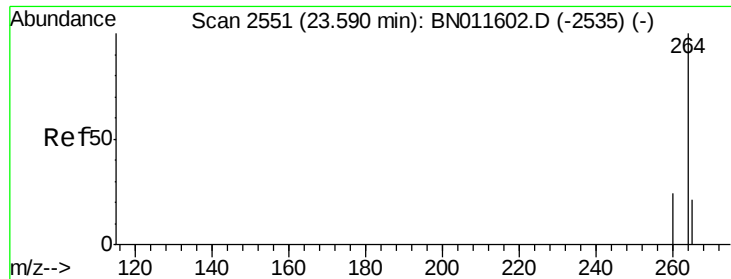

#36

Pervlene-d12

Concen: 0.400 ng

RT: 23.58 min Scan# 2549

Delta R.T. -0.01 min

Lab File: BN011652.D

Acq: 26 Aug 2020 19:21

Instrument :

BNA_N

ClientSampleId :

BP-VPB181-GW-518-520

Tot Ion: 264 Resp: 16669

Ion Ratio Lower Upper

264 100

260 24.7 19.6 29.4

265 50.8 40.7 61.1

