


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082620\
 Data File : BN011643.D
 Acq On : 26 Aug 2020 13:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 25 03:31:11 2020

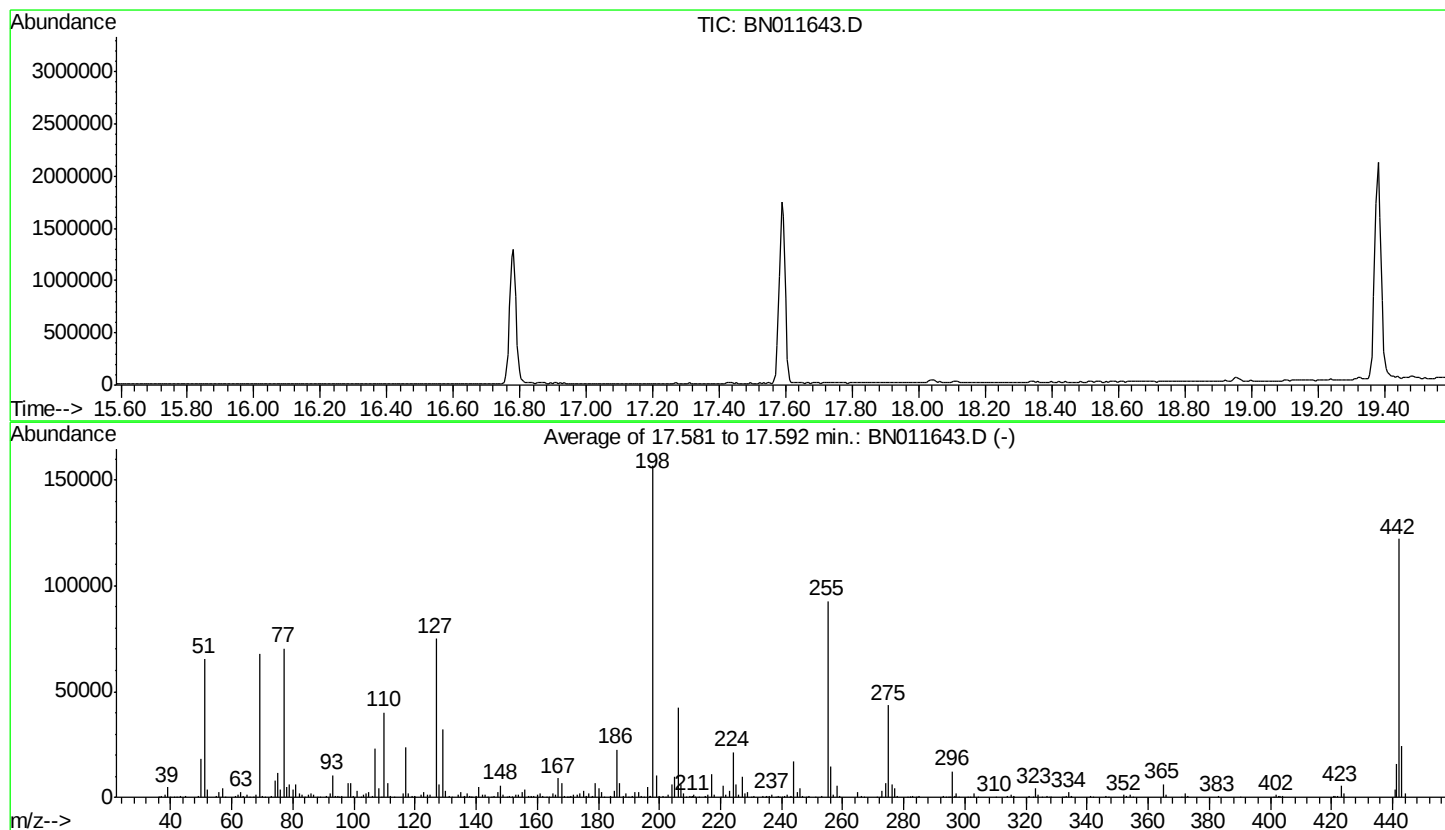

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.7	65504	PASS
68	69	0.00	2	2.0	1387	PASS
69	198	0.00	100	43.4	68050	PASS
70	69	0.00	2	0.7	499	PASS
127	198	10	80	47.8	75064	PASS
197	198	0.00	2	0.4	569	PASS
198	198	100	100	100.0	156949	PASS
199	198	5	9	6.6	10422	PASS
275	198	10	60	27.6	43368	PASS
365	198	1	100	4.0	6273	PASS
441	198	0.01	100	10.2	16077	PASS
442	198	50	100	77.9	122285	PASS
443	442	15	24	19.6	23977	PASS