

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082919\
 Data File : BN007495.D
 Acq On : 29 Aug 2019 09:57
 Operator : HP/JU
 Sample : PB122591BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB122591BL

Quant Time: Aug 29 12:26:41 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Aug 24 00:38:17 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.40	152	4844	0.40	ng	0.00
7) Naphthalene-d8	10.15	136	21246	0.40	ng	-0.01
13) Acenaphthene-d10	14.05	164	13711	0.40	ng	0.00
19) Phenanthrene-d10	16.80	188	36295	0.40	ng	0.00
27) Chrysene-d12	21.02	240	36346	0.40	ng	0.00
34) Perylene-d12	23.13	264	33776	0.40	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Fluorophenol	5.03	112	5020	0.29	ng	0.00
5) Phenol-d6	6.60	99	6609	0.30	ng	0.00
8) Nitrobenzene-d5	8.53	82	4342	0.23	ng	0.00
11) 2-Methylnaphthalene-d10	11.76	152	11252	0.32	ng	0.00
14) 2,4,6-Tribromophenol	15.57	330	1831	0.26	ng	0.01
15) 2-Fluorobiphenyl	12.66	172	13444	0.24	ng	0.00
25) Fluoranthene-d10	18.84	212	37398	0.32	ng	0.00
29) Terphenyl-d14	19.46	244	28118	0.30	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
32) Bis(2-ethylhexyl)phthalate	20.96	149	803	Below Cal	#	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082919\
Data File : BN007495.D
Acq On : 29 Aug 2019 09:57
Operator : HP/JU
Sample : PB122591BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB122591BL

Quant Time: Aug 29 12:26:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 24 00:38:17 2019
Response via : Initial Calibration

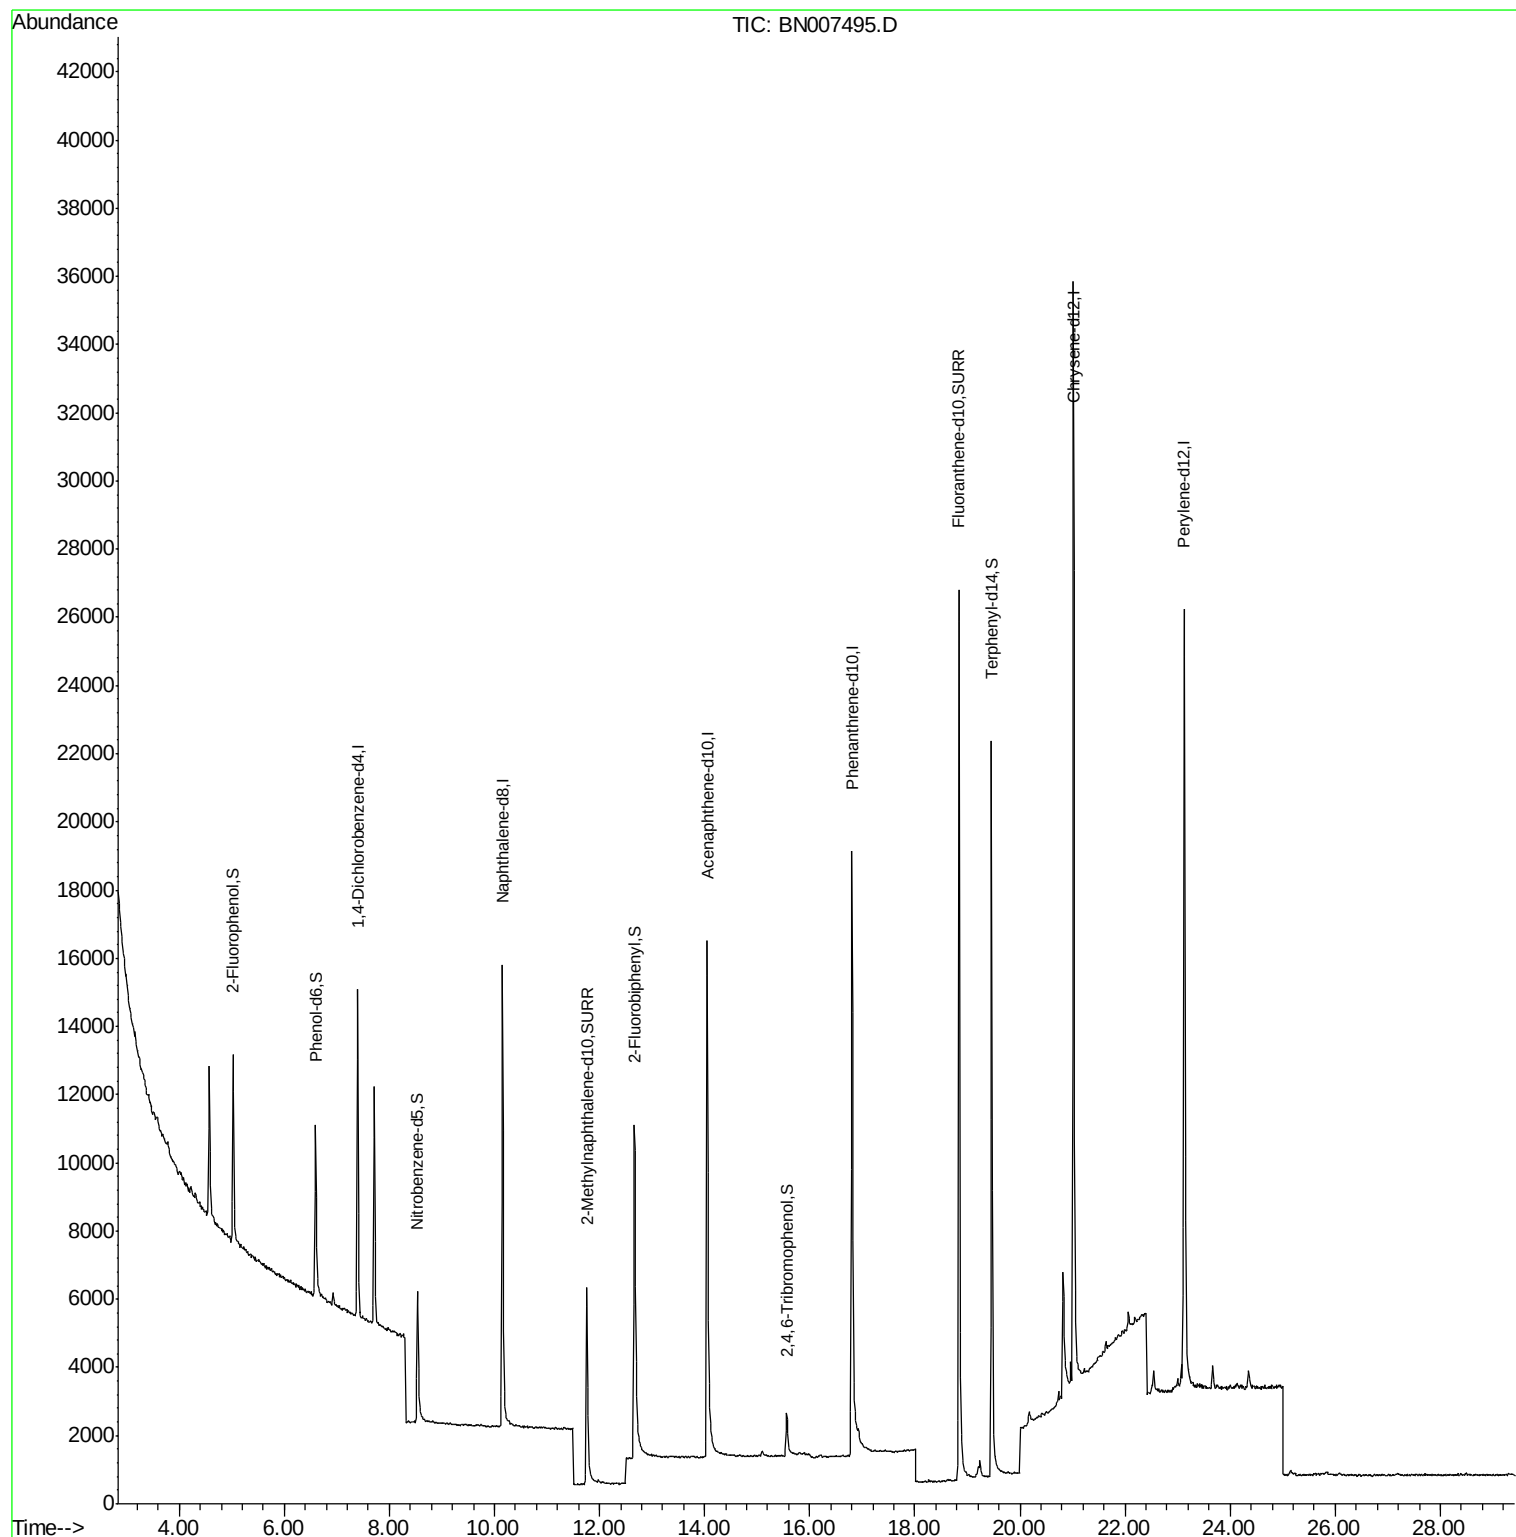

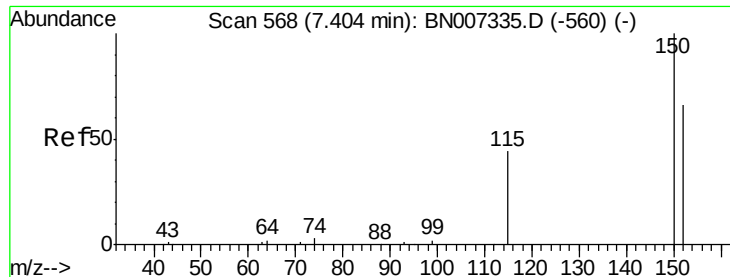


#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.40 min Scan# 567
Delta R.T. -0.01 min
Lab File: BN007495.D
Acq: 29 Aug 2019 09:57

Instrument :
BNA_N
ClientSampleId :
PB122591BL

Tgt Ion:152 Resp: 4844
Ion Ratio Lower Upper
152 100
150 153.7 109.1 163.7
115 69.1 59.6 89.4

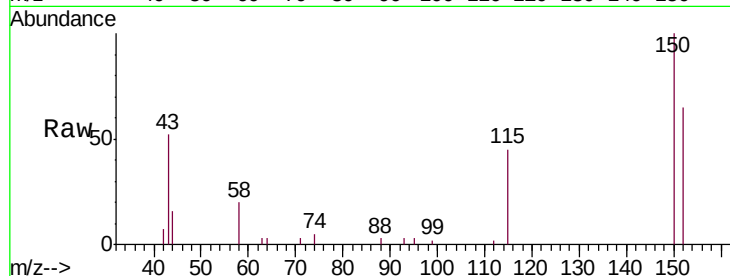


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

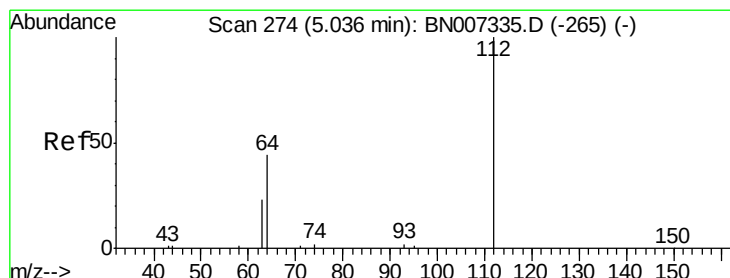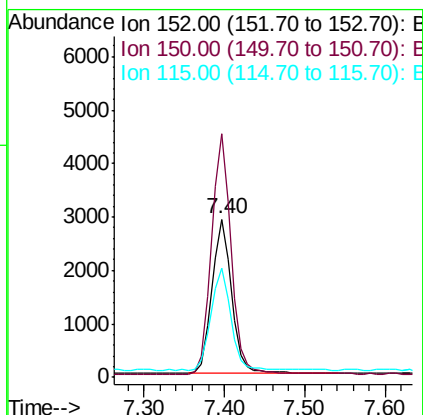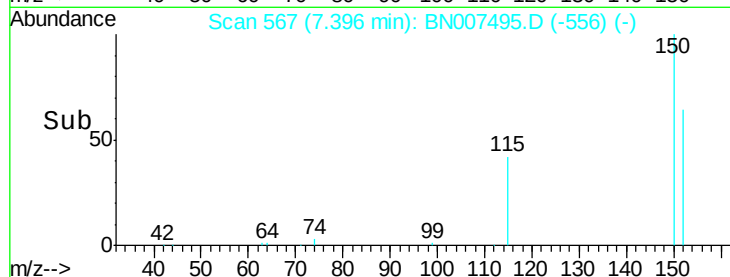



#4


2-Fluorophenol
Concen: 0.291 ng
RT: 5.03 min Scan# 273
Delta R.T. -0.01 min
Lab File: BN007495.D
Acq: 29 Aug 2019 09:57

Tgt Ion:112 Resp: 5020
Ion Ratio Lower Upper
112 100
64 53.6 42.3 63.5
63 26.7 23.6 35.4

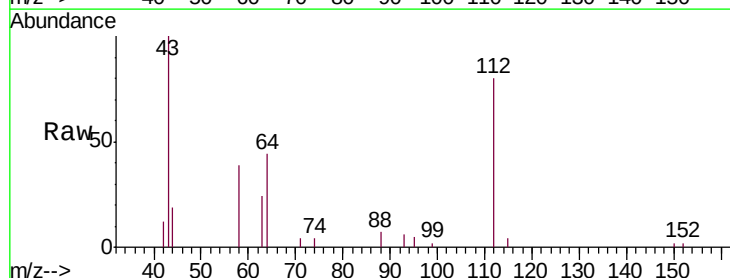

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BNC
Ion 63.00 (62.70 to 63.70): BNC

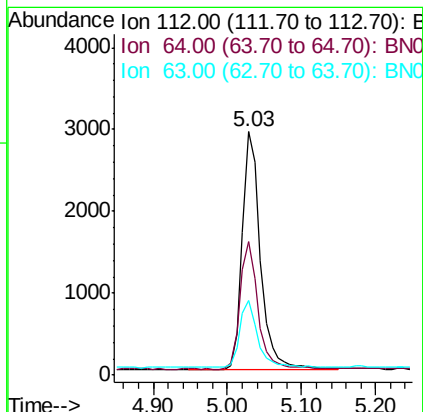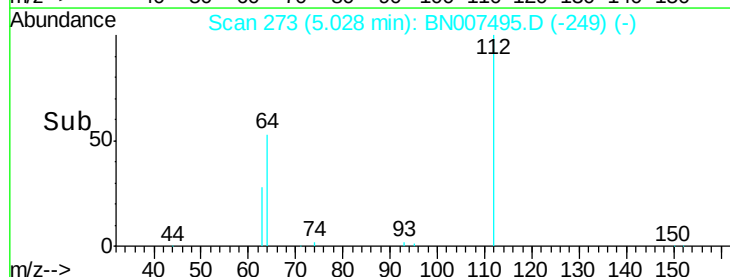

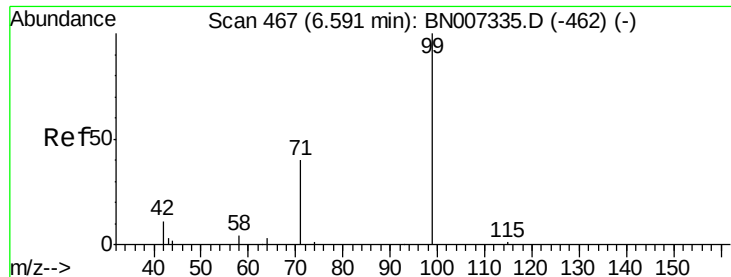

#5

Phenol-d6

Concen: 0.302 ng

RT: 6.60 min Scan# 468

Delta R.T. 0.01 min

Lab File: BN007495.D

Acq: 29 Aug 2019 09:57

Instrument :

BNA_N

ClientSampleId :

PB122591BL


Tgt Ion: 99 Resp: 6609

Ion Ratio Lower Upper

99 100

42 12.5 11.2 16.8




71 34.0 31.8 47.8

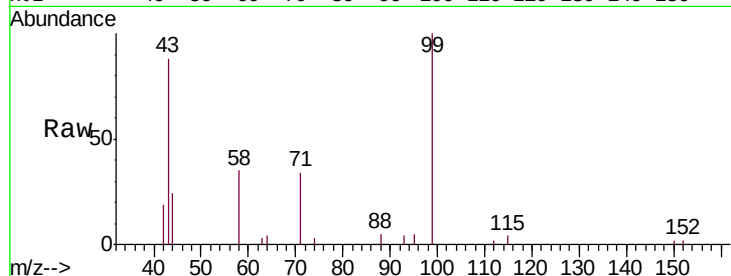

Abundance Ion 99.00 (98.70 to 99.70): BN007335.D (-462) (-)

Ion 42.00 (41.70 to 42.70): BN007335.D (-462) (-)

Ion 71.00 (70.70 to 71.70): BN007335.D (-462) (-)

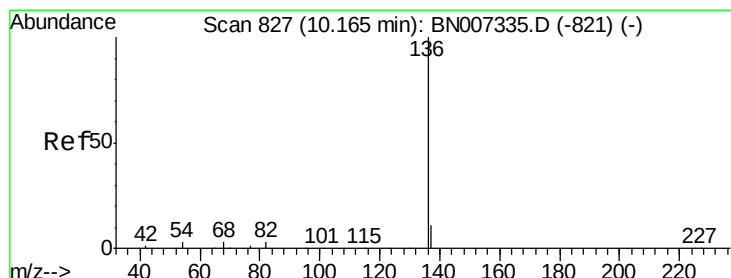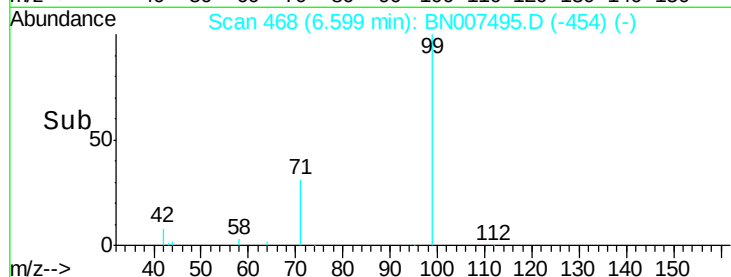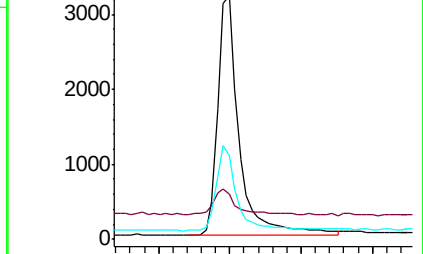

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.15 min Scan# 826

Delta R.T. -0.01 min

Lab File: BN007495.D

Acq: 29 Aug 2019 09:57

Tgt Ion: 136 Resp: 21246


Ion Ratio Lower Upper

136 100

137 11.2 12.9 19.3#

54 4.9 8.6 12.8#

68 6.5 17.0 25.4#


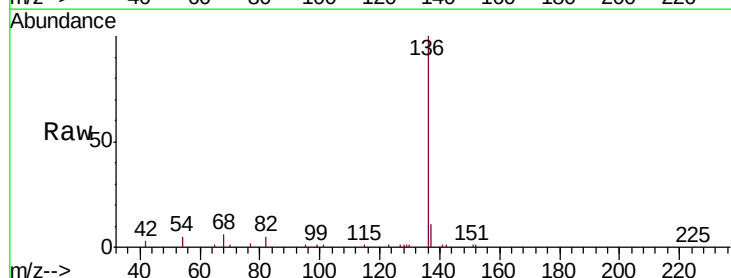



Abundance Ion 136.00 (135.70 to 136.70): BN007335.D (-821) (-)

Ion 137.00 (136.70 to 137.70): BN007335.D (-821) (-)

Ion 54.00 (53.70 to 54.70): BN007335.D (-821) (-)

Ion 68.00 (67.70 to 68.70): BN007335.D (-821) (-)

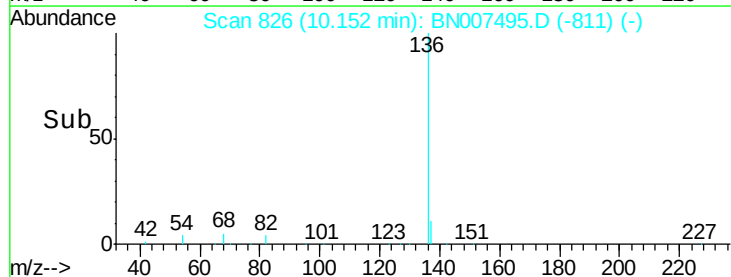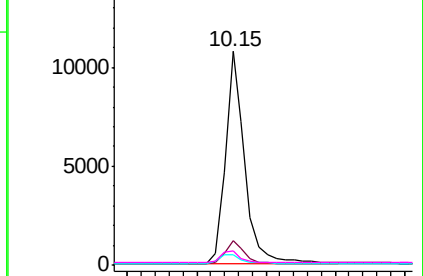

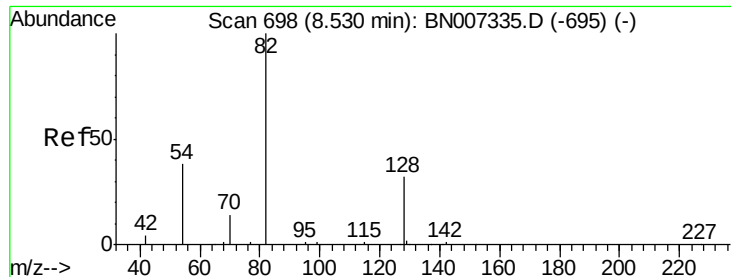

#8

Nitrobenzene-d5

Concen: 0.235 ng

RT: 8.53 min Scan# 698

Delta R.T. -0.00 min

Lab File: BN007495.D

Acq: 29 Aug 2019 09:57

Instrument :

BNA_N

ClientSampleId :

PB122591BL


Tgt Ion: 82 Resp: 4342

Ion Ratio Lower Upper

82 100

128 35.6 19.7 29.5#




54 37.9 25.8 38.6

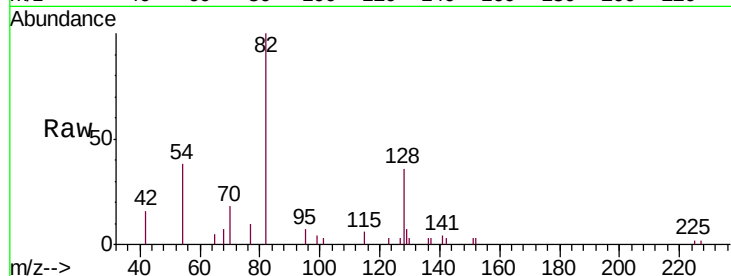

Abundance Ion 82.00 (81.70 to 82.70): BN007495.D (-690) (-)

Ion 128.00 (127.70 to 128.70): BN007495.D (-690) (-)

Ion 54.00 (53.70 to 54.70): BN007495.D (-690) (-)

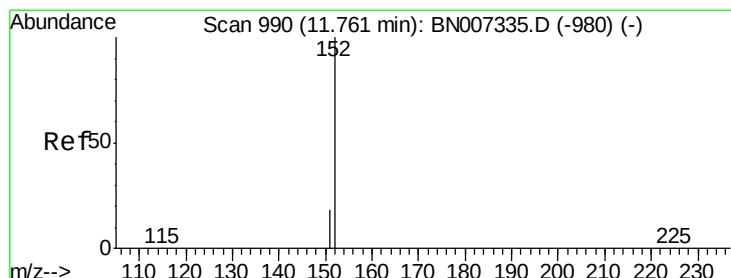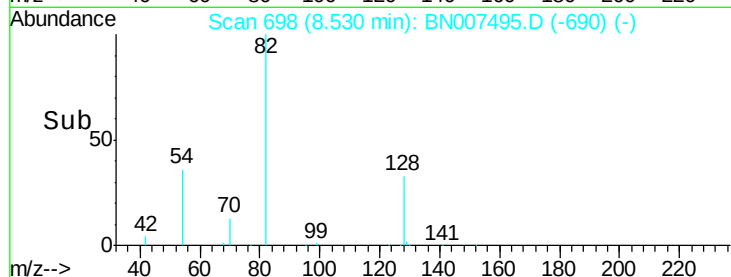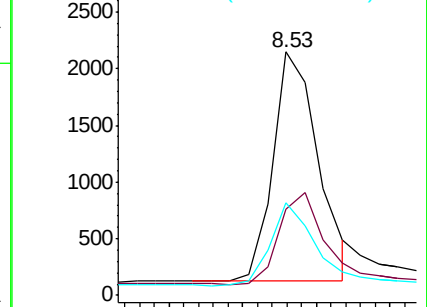

#11

2-Methylnaphthalene-d10

Concen: 0.319 ng

RT: 11.76 min Scan# 989

Delta R.T. -0.00 min

Lab File: BN007495.D


Acq: 29 Aug 2019 09:57

Tgt Ion: 152 Resp: 11252

Ion Ratio Lower Upper



152 100


151 17.9 16.2 24.2

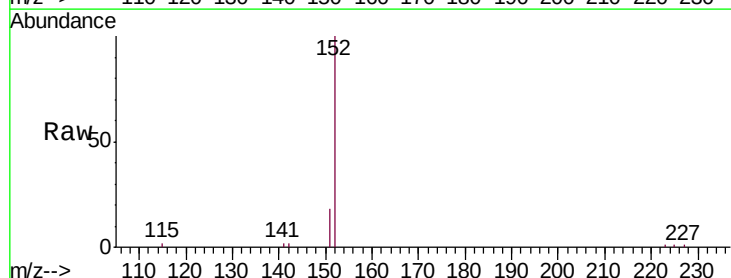

Abundance Ion 152.00 (151.70 to 152.70): BN007495.D (-945) (-)

Ion 151.00 (150.70 to 151.70): BN007495.D (-945) (-)

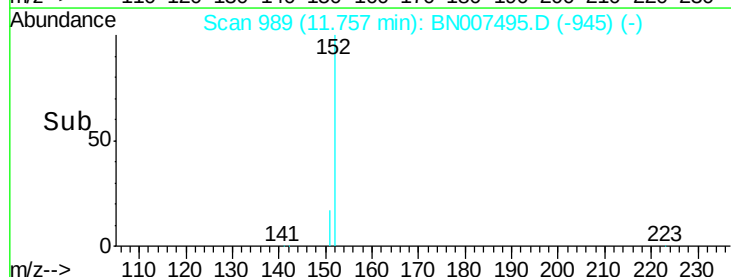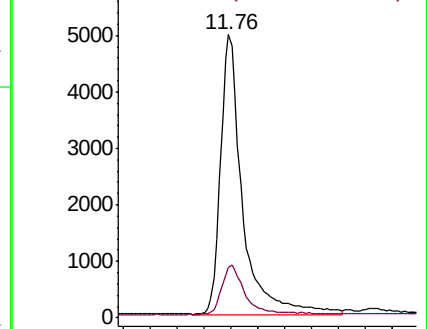

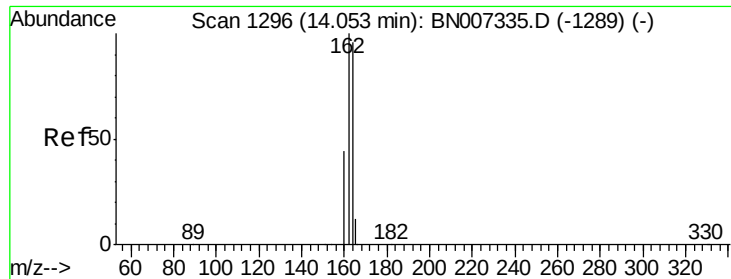

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.05 min Scan# 1296

Delta R.T. -0.00 min

Lab File: BN007495.D

Acq: 29 Aug 2019 09:57

Instrument :

BNA_N

ClientSampleId :

PB122591BL


Tgt Ion:164 Resp: 13711

Ion Ratio Lower Upper

164 100

162 103.0 83.5 125.3




160 47.1 38.2 57.4

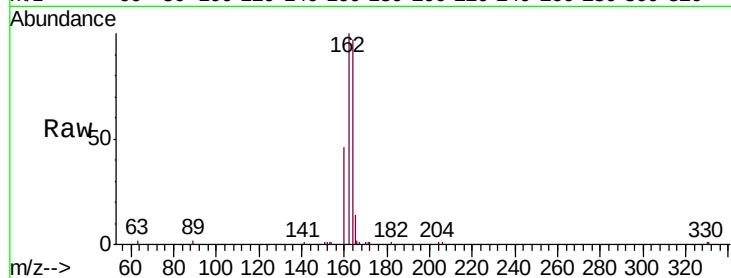

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

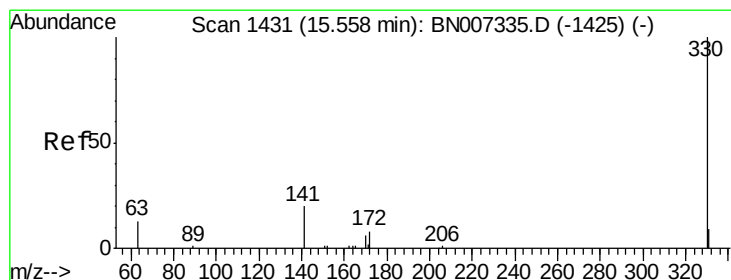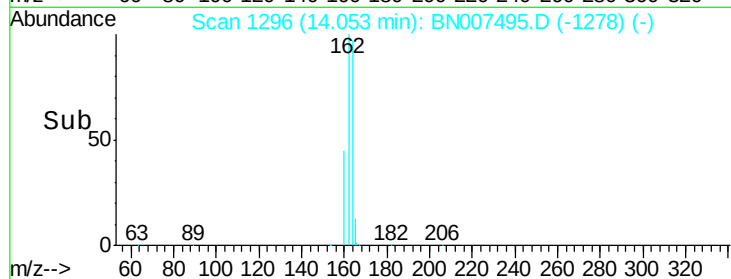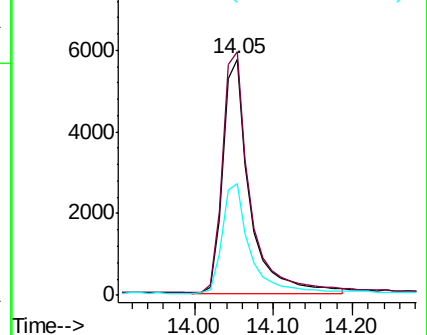

#14

2,4,6-Tribromophenol

Concen: 0.255 ng

RT: 15.57 min Scan# 1432

Delta R.T. 0.01 min

Lab File: BN007495.D

Acq: 29 Aug 2019 09:57


Tgt Ion:330 Resp: 1831

Ion Ratio Lower Upper

330 100

332 0.0 0.0 0.0



141 36.5 26.9 40.3

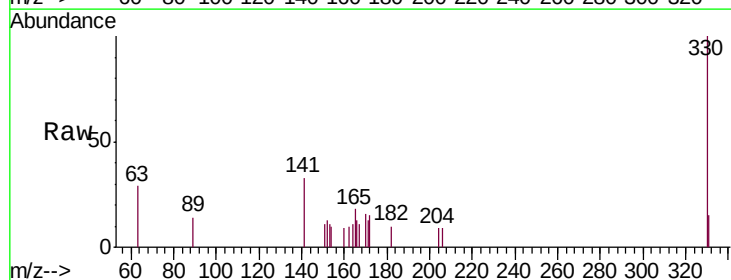


Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



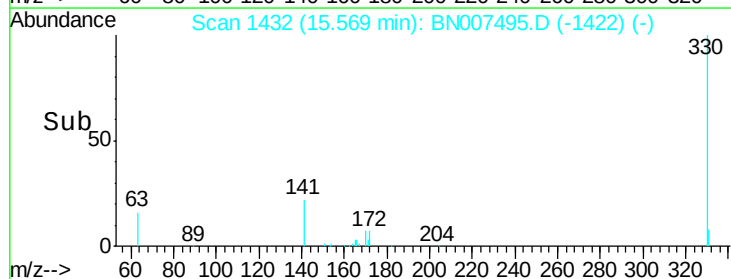
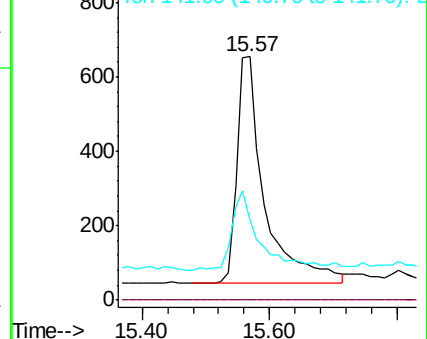


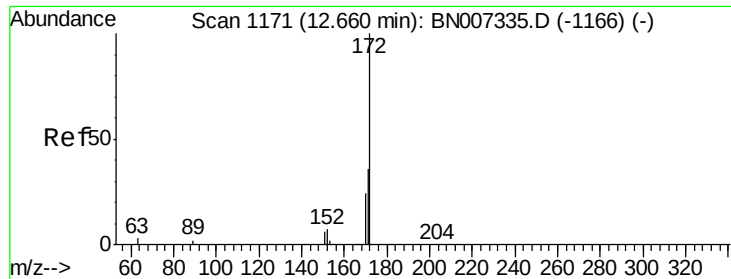

#15
2-Fluorobiphenyl
Concen: 0.243 ng
RT: 12.66 min Scan# 1171
Delta R.T. -0.00 min
Lab File: BN007495.D
Acq: 29 Aug 2019 09:57




Instrument :
BNA_N
ClientSampleId :
PB122591BL


Tgt Ion:172 Resp: 13444
Ion Ratio Lower Upper
172 100
171 37.1 30.3 45.5
170 24.4 20.7 31.1

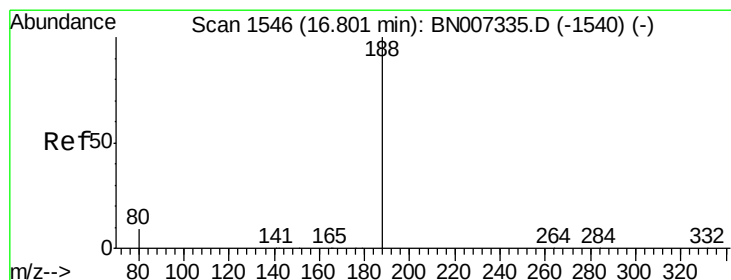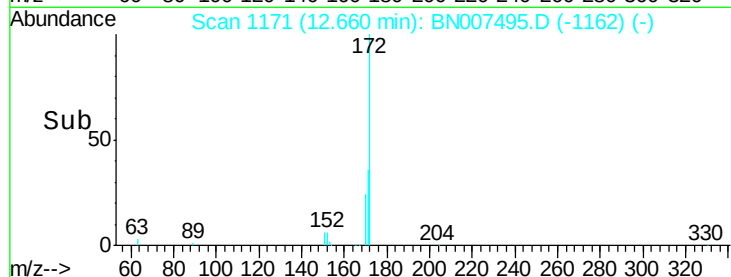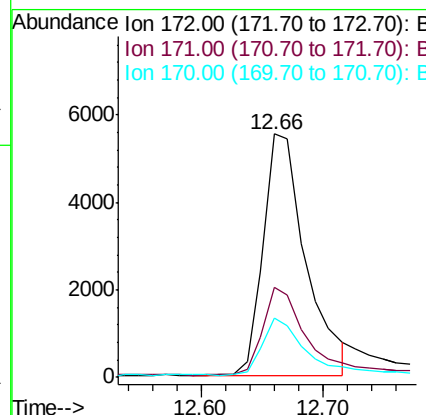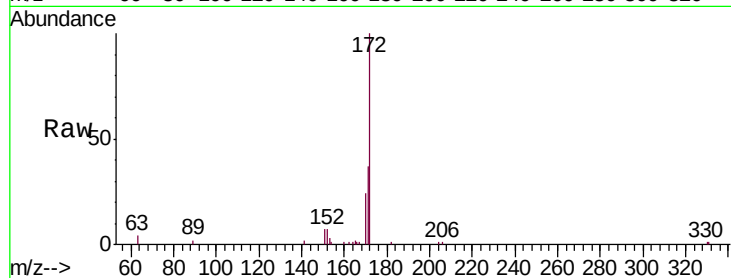

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 16.80 min Scan# 1546
Delta R.T. -0.00 min
Lab File: BN007495.D
Acq: 29 Aug 2019 09:57

Tgt Ion:188 Resp: 36295
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 11.0 11.8 17.8#

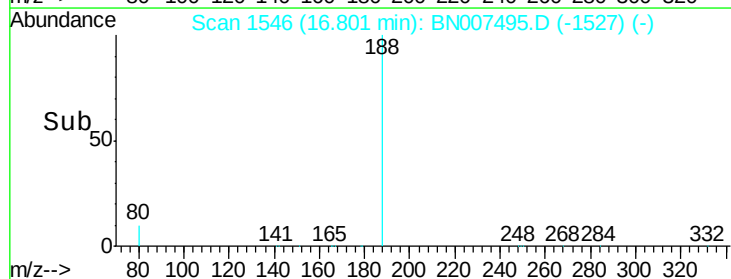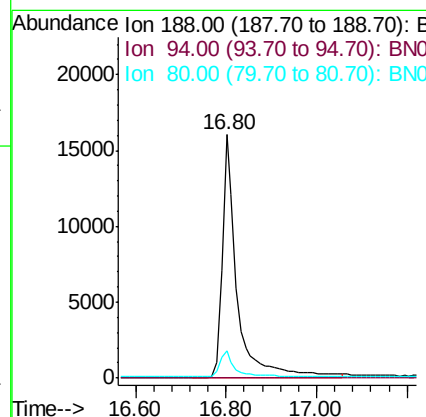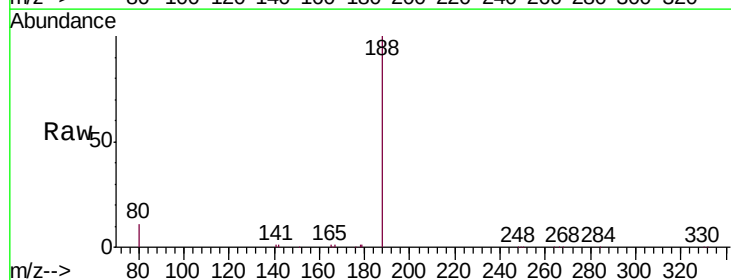

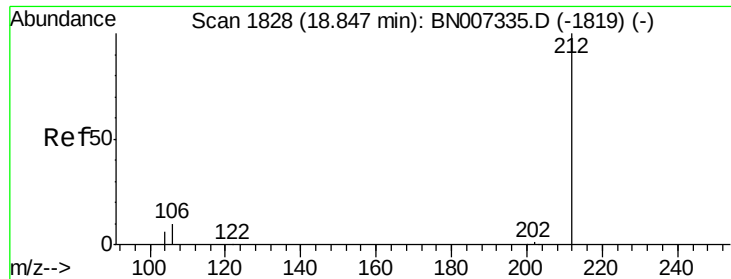

#25

Fluoranthene-d10

Concen: 0.320 ng

RT: 18.84 min Scan# 1827

Delta R.T. -0.01 min

Lab File: BN007495.D

Acq: 29 Aug 2019 09:57

Instrument :

BNA_N

ClientSampleId :

PB122591BL


Tgt Ion:212 Resp: 37398

Ion Ratio Lower Upper

212 100

106 12.3 9.0 13.4




104 7.0 5.4 8.2

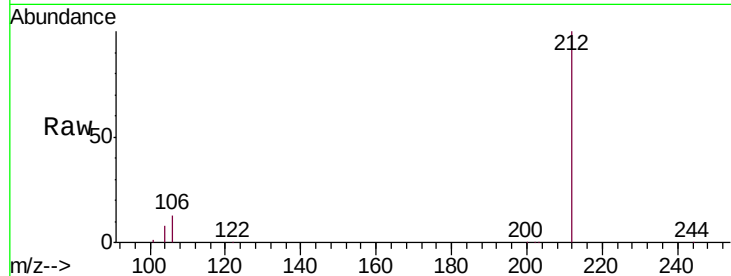

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

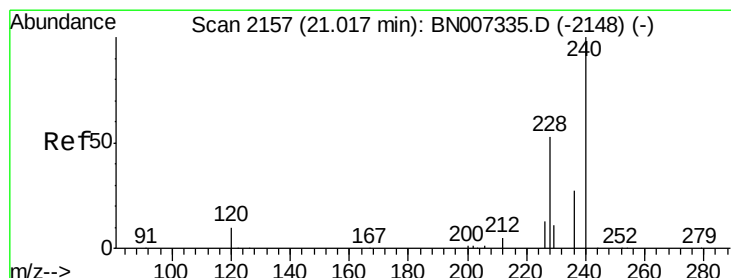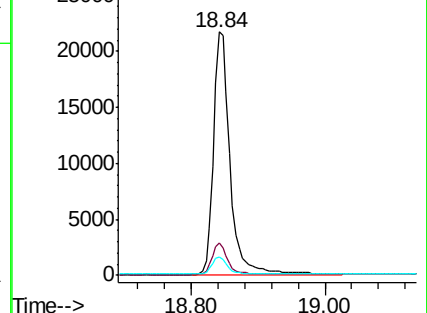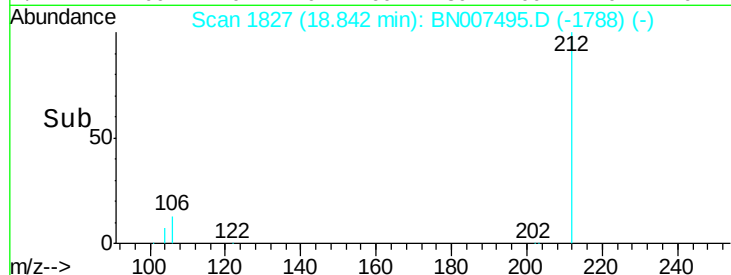

#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.02 min Scan# 2157

Delta R.T. -0.00 min

Lab File: BN007495.D

Acq: 29 Aug 2019 09:57


Tgt Ion:240 Resp: 36346

Ion Ratio Lower Upper

240 100

120 11.5 9.6 14.4



236 27.6 22.2 33.2

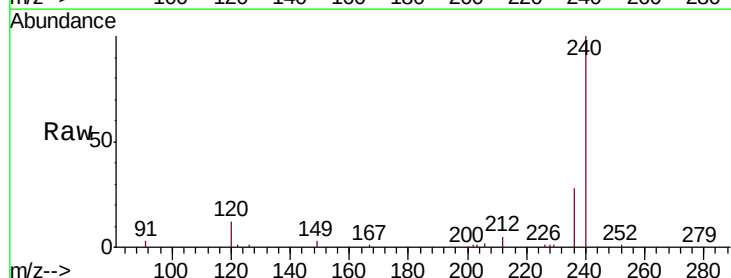


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

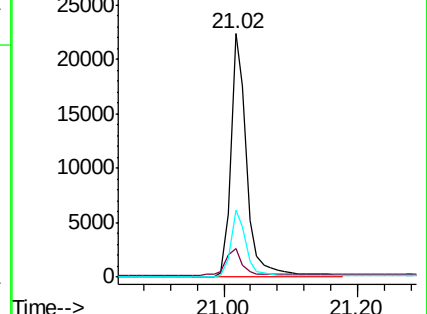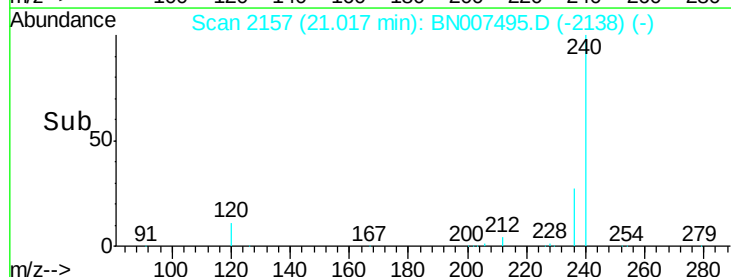

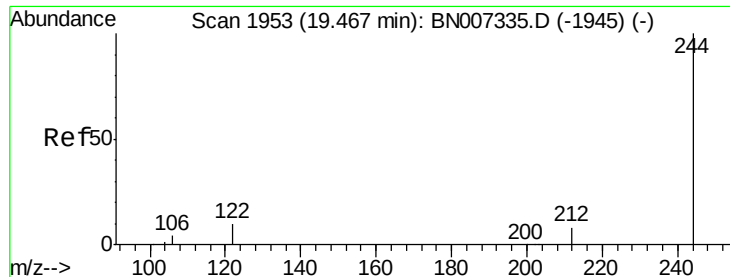

#29

Terphenyl-d14

Concen: 0.296 ng

RT: 19.46 min Scan# 1952

Delta R.T. -0.00 min

Lab File: BN007495.D

Acq: 29 Aug 2019 09:57

Instrument :

BNA_N

ClientSampleId :

PB122591BL


Tgt Ion:244 Resp: 28118

Ion Ratio Lower Upper

244 100

212 7.9 7.0 10.6




122 11.5 9.6 14.4

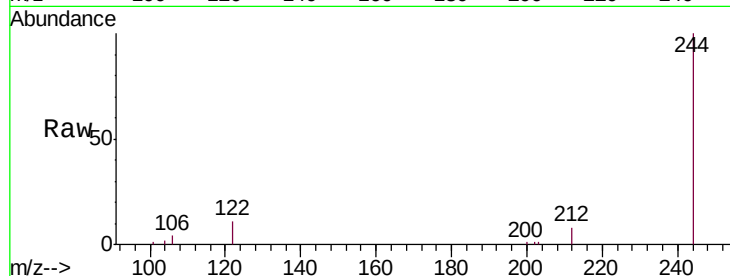

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

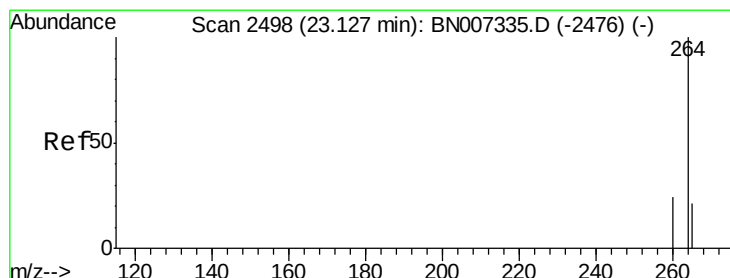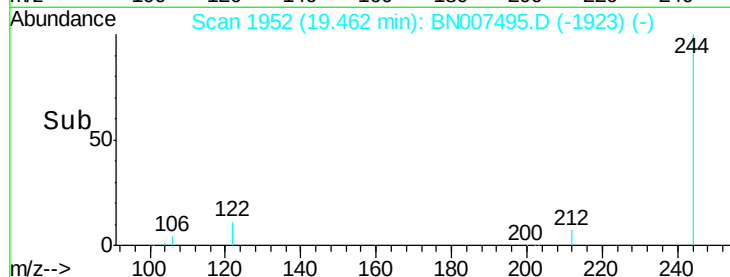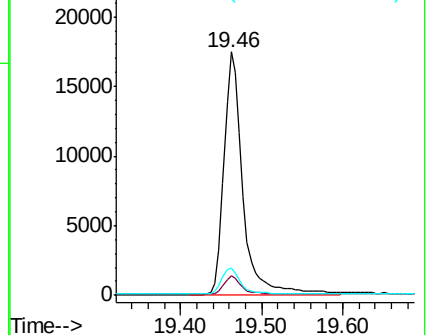

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.13 min Scan# 2498

Delta R.T. -0.00 min

Lab File: BN007495.D

Acq: 29 Aug 2019 09:57


Tgt Ion:264 Resp: 33776

Ion Ratio Lower Upper

264 100

260 24.7 19.7 29.5

265 32.9 29.9 44.9

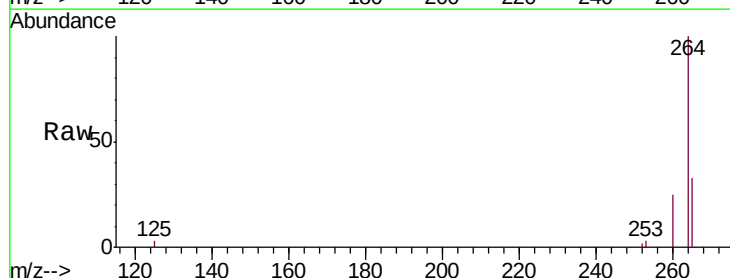

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

