


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082919\
 Data File : BN007493.D
 Acq On : 29 Aug 2019 08:10
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 29 12:18:45 2019

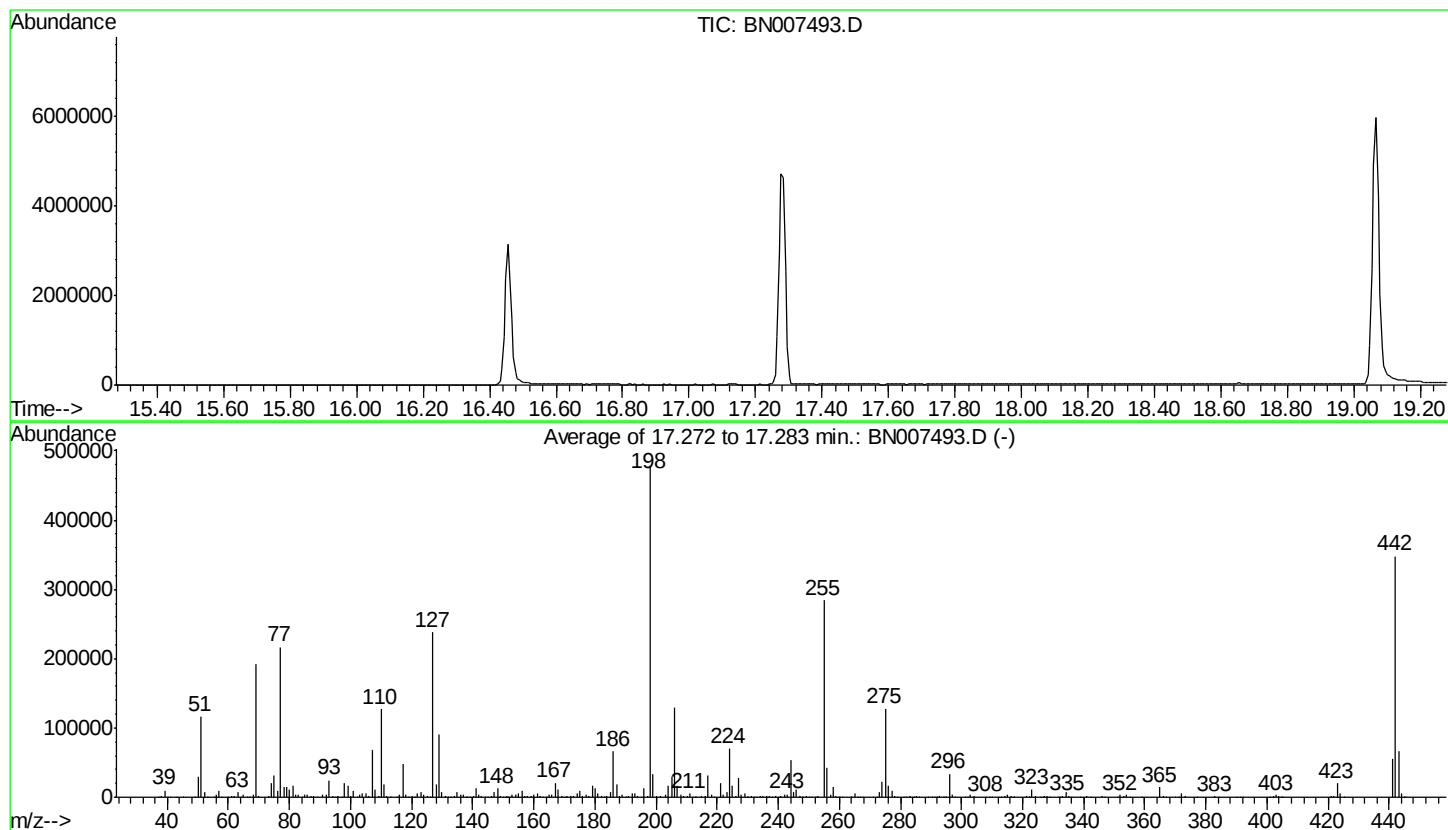

AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.2	115828	PASS
68	69	0.00	2	1.9	3565	PASS
69	198	0.00	100	40.0	191473	PASS
70	69	0.00	2	0.6	1055	PASS
127	198	10	80	49.6	237632	PASS
197	198	0.00	2	0.4	1888	PASS
198	198	100	100	100.0	478677	PASS
199	198	5	9	6.8	32621	PASS
275	198	10	60	26.7	127778	PASS
365	198	1	100	3.1	14686	PASS
441	198	0.01	100	11.5	54882	PASS
442	198	50	100	72.7	347818	PASS
443	442	15	24	19.4	67416	PASS